

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123021\
 Data File : PS017880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2021 22:34
 Operator : AJ\MA
 Sample : M5257-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:16:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.126	6.715	643.2E6	276.5E6	411.542	463.888
Target Compounds							
1) T	Dalapon	2.932f	2.447	114.0E6	204.0E6	44.472	263.532 #
2) T	3,5-DICHL...	0.000	5.942	0	47507702	N.D.	52.399
3) T	4-Nitroph...	6.959	0.000	11482560	0	16.980	N.D. #
5) T	DICAMBA	7.296	0.000	18531237	0	2.931	N.D. #
6) T	MCPD	7.475	0.000	6771842	0	1.437	N.D. #
7) T	MCPA	7.620	0.000	5401188	0	<MDL	N.D. #
8) T	DICHLORPROP	7.946f	0.000	3963590	0	2.537	N.D. #
9) T	2,4-D	8.201	0.000	8869651	0	5.017	N.D. #
10) T	Pentachlo...	8.534	0.000	8863718	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.086	0.000	7088369	0	<MDL	N.D. #
12) T	2,4,5-T	9.385	0.000	6426918	0	<MDL	N.D. #
13) T	2,4-DB	9.879f	0.000	36830061	0	24.941	N.D. #
14) T	DINOSEB	11.037	9.805	55241938	57740136	8.079	22.349 #
15) T	Picloram	10.873	0.000	45613630	0	4.204	N.D. #
16) T	DCPA	11.333	0.000	8216692	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123021\
Data File : PS017880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2021 22:34
Operator : AJ\MA
Sample : M5257-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

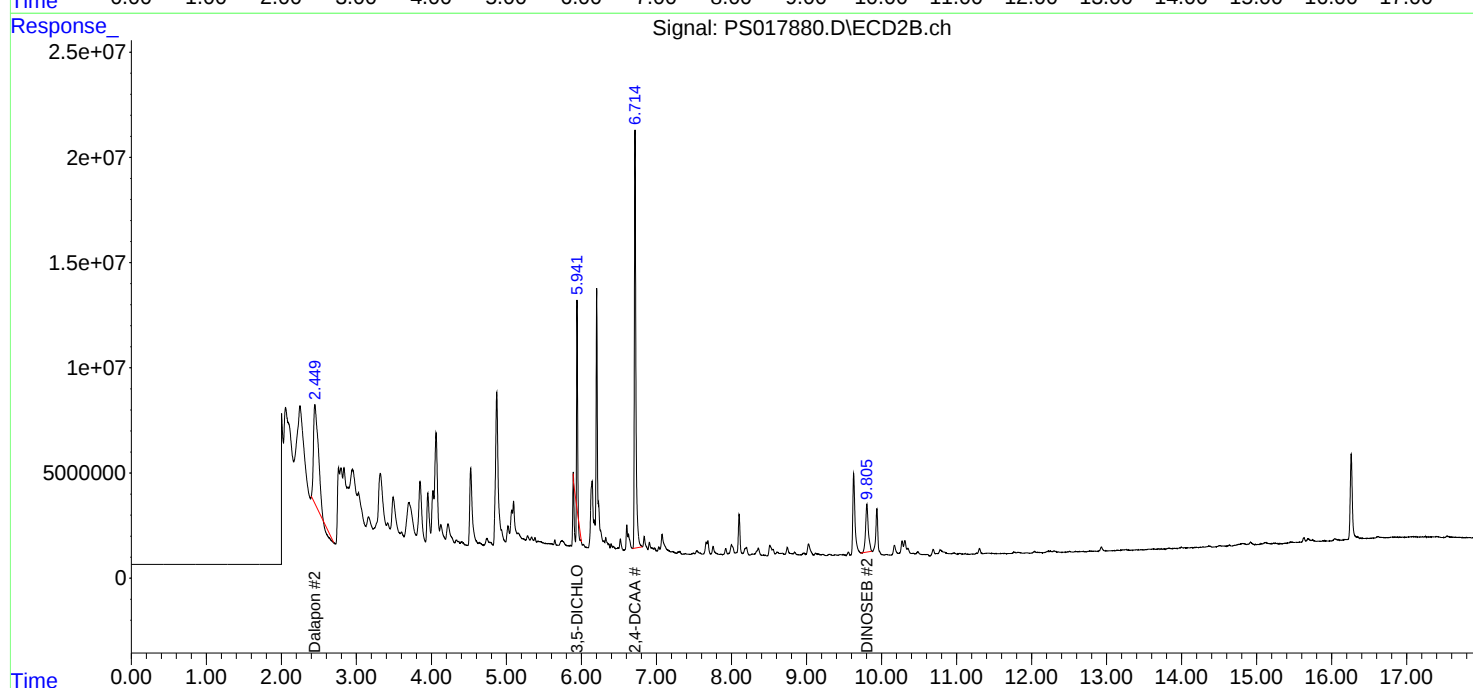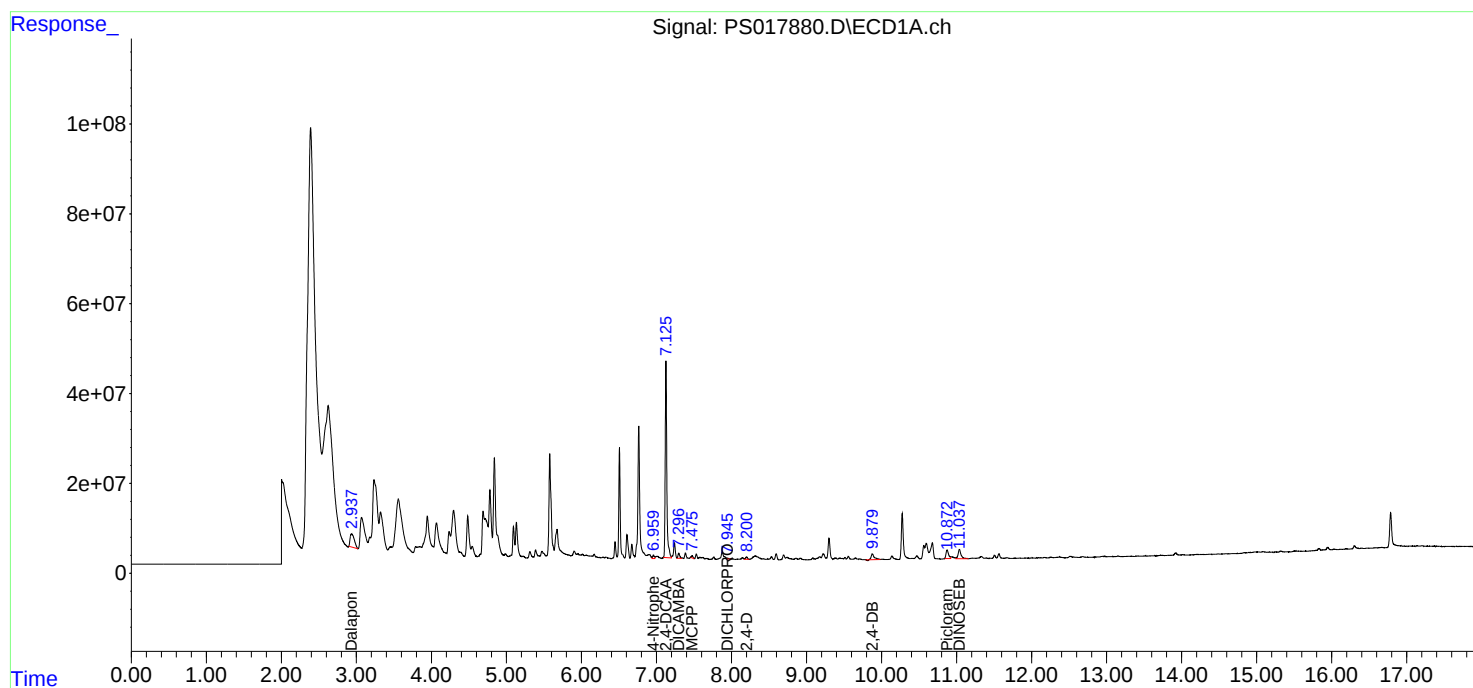


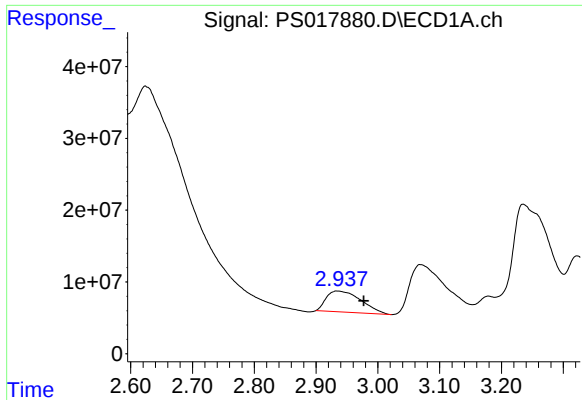

#1 Dalapon


R.T.: 2.932 min
Delta R.T.: -0.045 min
Response: 113963593
Conc: 44.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

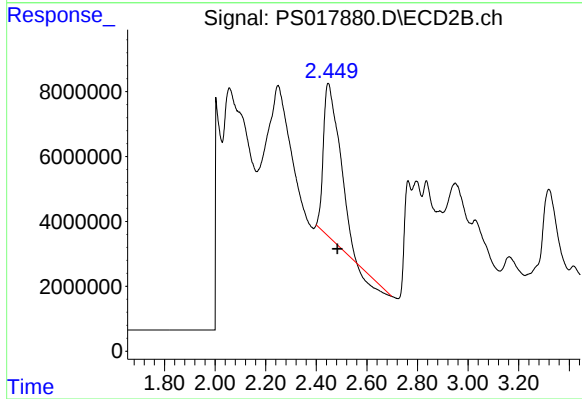


#1 Dalapon

R.T.: 2.447 min
Delta R.T.: -0.037 min
Response: 203999817
Conc: 263.53 ng/ml

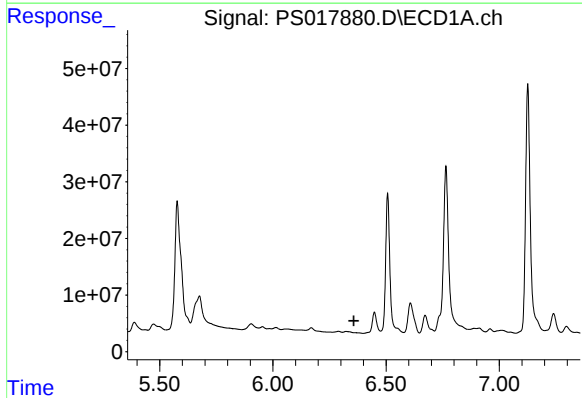


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

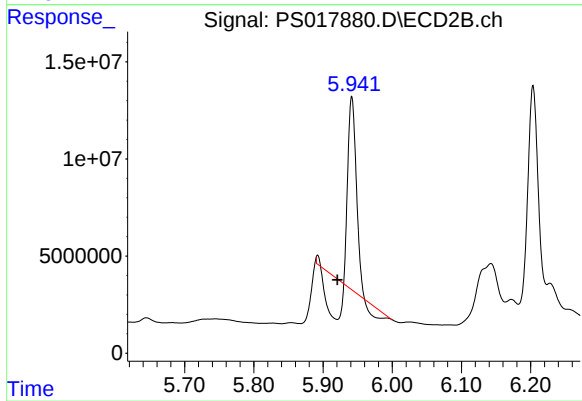

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.942 min
Delta R.T.: 0.021 min
Response: 47507702
Conc: 52.40 ng/ml

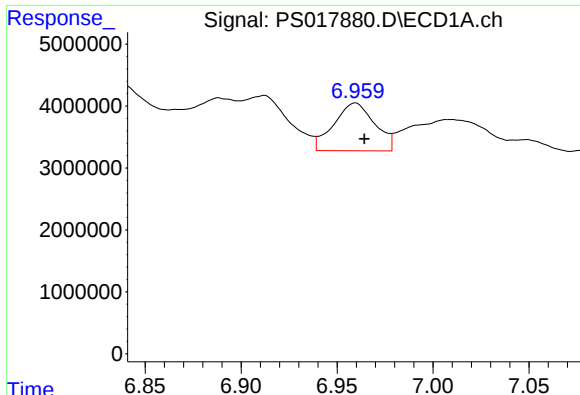

#3 4-Nitrophenol


R.T.: 6.959 min
Delta R.T.: -0.005 min
Response: 11482560
Conc: 16.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

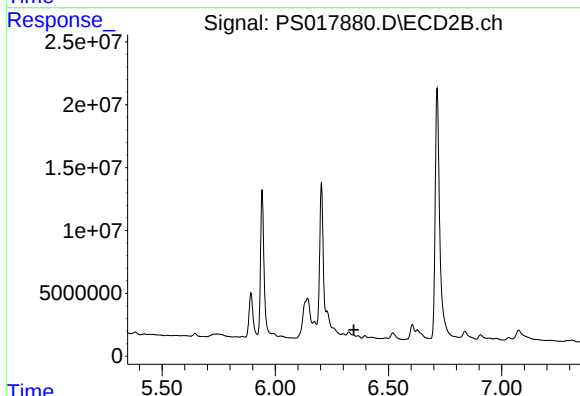


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.347 min
Response: 0
Conc: N.D.

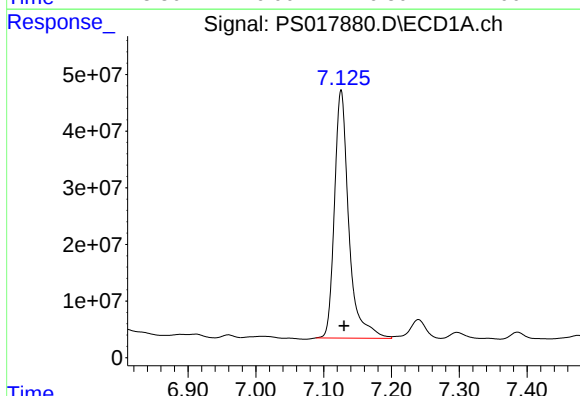


#4 2,4-DCAA

R.T.: 7.126 min
Delta R.T.: -0.004 min
Response: 643217422
Conc: 411.54 ng/ml

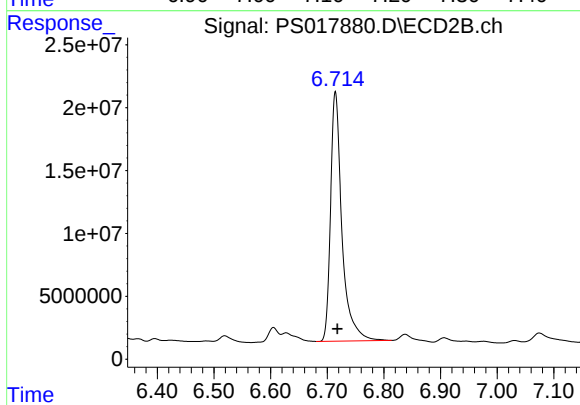

#4 2,4-DCAA


R.T.: 6.715 min
Delta R.T.: -0.003 min
Response: 276524505
Conc: 463.89 ng/ml

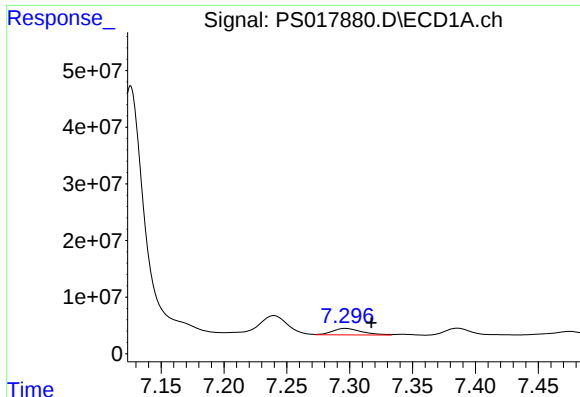

#5 DICAMBA


R.T.: 7.296 min
Delta R.T.: -0.021 min
Response: 18531237
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

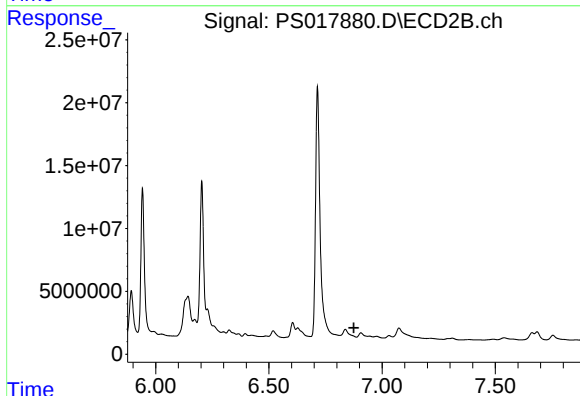


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

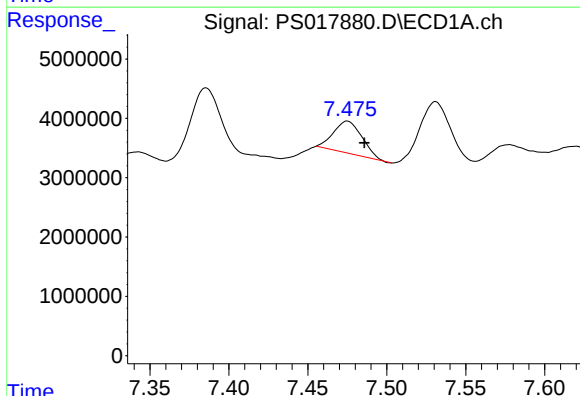


#6 MCP

R.T.: 7.475 min
Delta R.T.: -0.011 min
Response: 6771842
Conc: 1.44 ug/ml

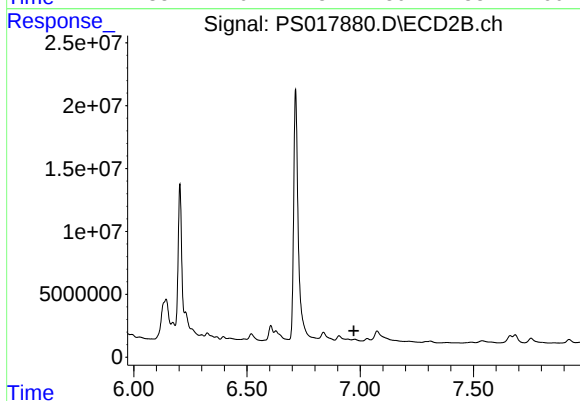

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.972 min
Response: 0
Conc: N.D.

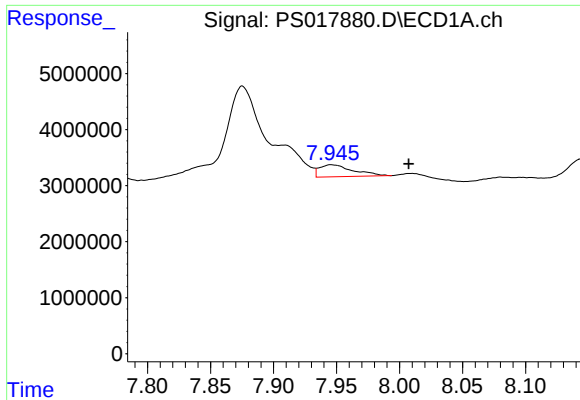

#8 DICHLORPROP


R.T.: 7.946 min
Delta R.T.: -0.062 min
Response: 3963590
Conc: 2.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

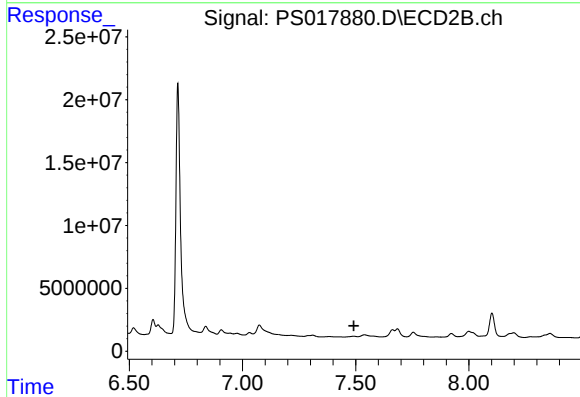


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.492 min
Response: 0
Conc: N.D.

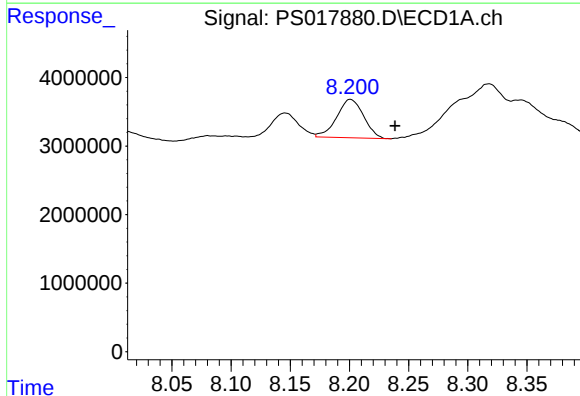


#9 2,4-D

R.T.: 8.201 min
Delta R.T.: -0.038 min
Response: 8869651
Conc: 5.02 ng/ml

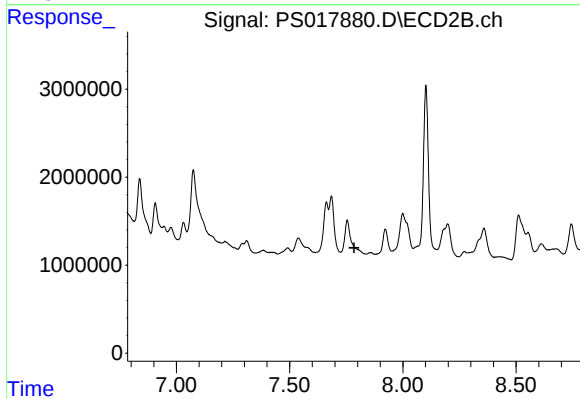

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

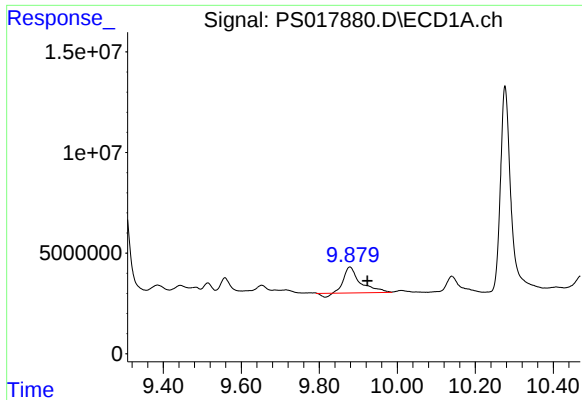

#13 2,4-DB


R.T.: 9.879 min
Delta R.T.: -0.045 min
Response: 36830061
Conc: 24.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

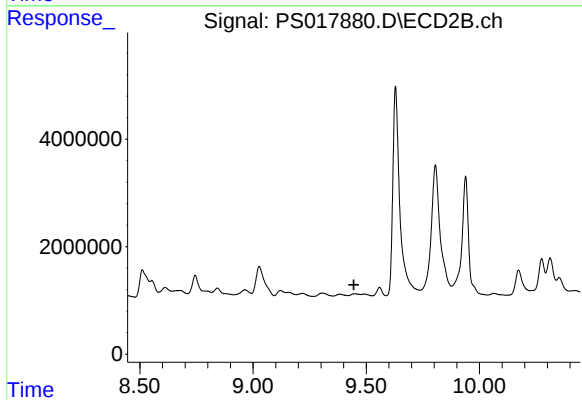


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.445 min
Response: 0
Conc: N.D.

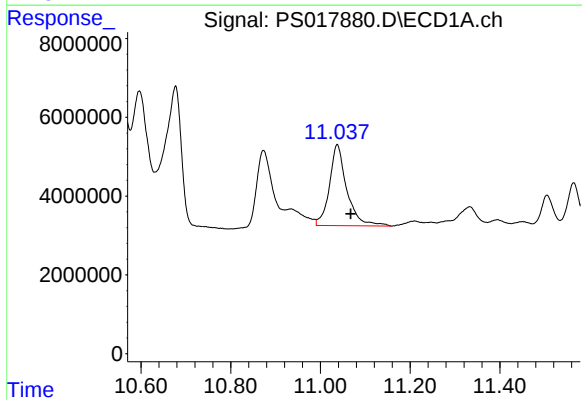


#14 DINOSEB

R.T.: 11.037 min
Delta R.T.: -0.030 min
Response: 55241938
Conc: 8.08 ng/ml

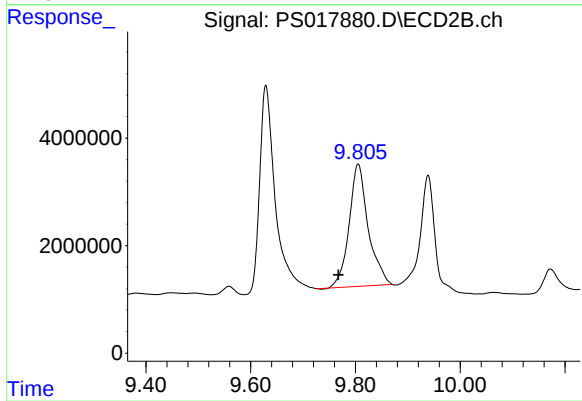

#14 DINOSEB


R.T.: 9.805 min
Delta R.T.: 0.038 min
Response: 57740136
Conc: 22.35 ng/ml

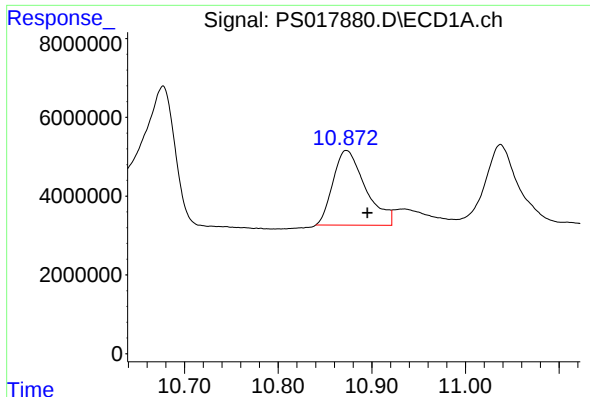

#15 Picloram

R.T.: 10.873 min
Delta R.T.: -0.022 min
Response: 45613630
Conc: 4.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

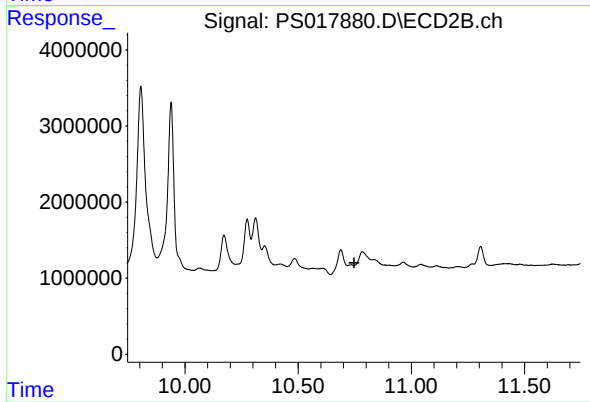

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.747 min
Response: 0
Conc: N.D.