

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123024\
 Data File : PS028847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2024 08:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 01:36:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251f	0.000	5719833	0	2.529	N.D. #
Target Compounds							
1) T	Dalapon	2.654f	2.705f	2758917	5883273	<MDL	2.989 #
2) T	3,5-DICHL...	6.374	0.000	2354217	0	<MDL	N.D. #
3) T	4-Nitroph...	6.995	0.000	4493131	0	2.991	N.D. #
5) T	DICAMBA	7.370f	0.000	945909	0	<MDL	N.D. #
6) T	MCP	7.531f	0.000	55286	0	<MDL	N.D. #
7) T	MCPA	7.695f	0.000	296389	0	<MDL	N.D. #
8) T	DICHLORPROP	8.131f	8.644f	976229	1617023	<MDL	1.172 #
9) T	2,4-D	8.372f	0.000	12048099	0	4.228	N.D. #
10) T	Pentachlo...	8.657f	9.447	1526396	3461551	<MDL	<MDL #
11) T	2,4,5-TP ...	9.190	0.000	4693384	0	<MDL	N.D. #
12) T	2,4,5-T	9.451f	10.254	3433191	1947441	<MDL	<MDL #
13) T	2,4-DB	10.058	0.000	3925389	0	1.257	N.D. #
14) T	DINOSEB	11.241f	0.000	3018669	0	<MDL	N.D. #
15) T	Picloram	11.089	12.279	41712621	18512163	1.556	1.442
16) T	DCPA	11.570	12.279f	404173	18512163	<MDL	1.723 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123024\
Data File : PS028847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2024 08:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 01:36:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

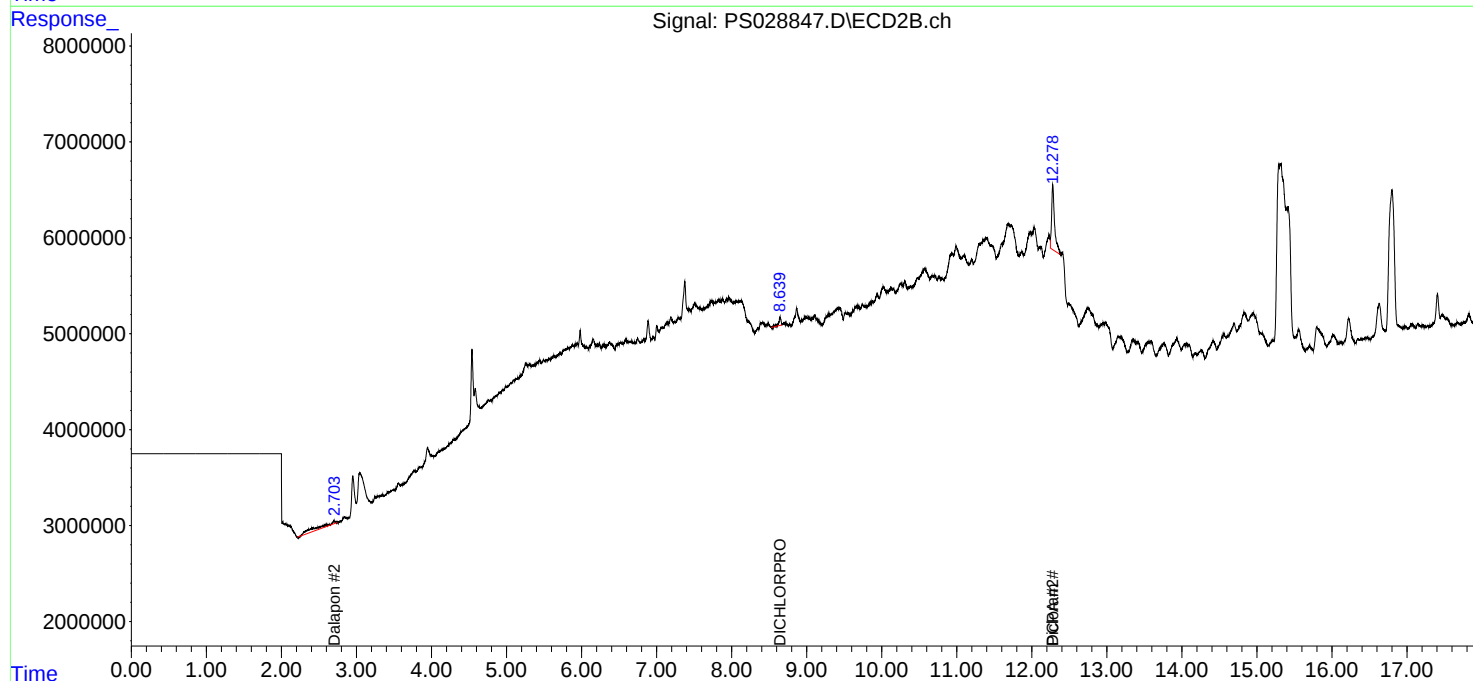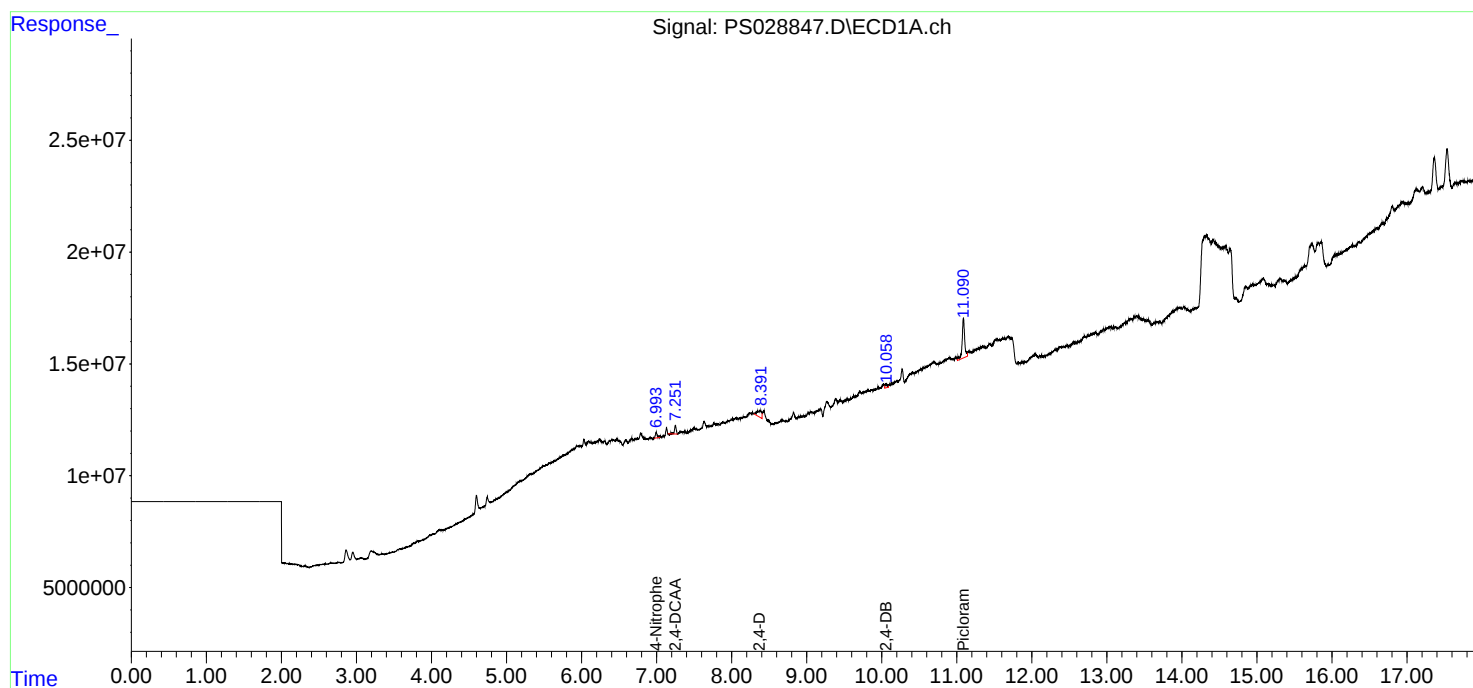


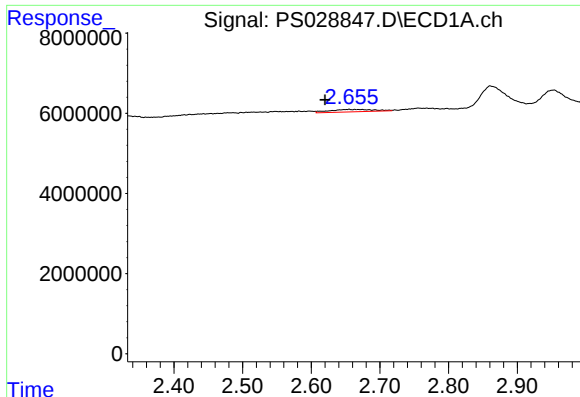

#1 Dalapon


R.T.: 2.654 min
Delta R.T.: 0.034 min
Response: 2758917
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

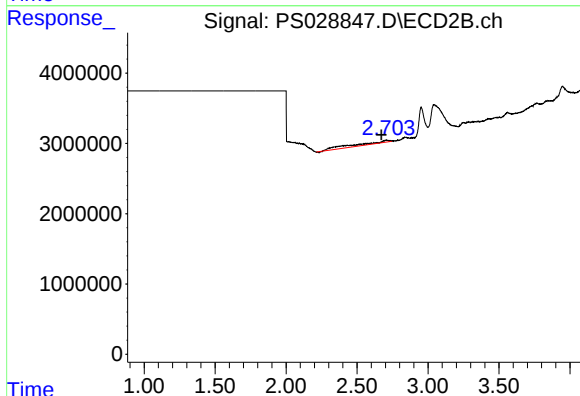


#1 Dalapon

R.T.: 2.705 min
Delta R.T.: 0.032 min
Response: 5883273
Conc: 2.99 ng/ml

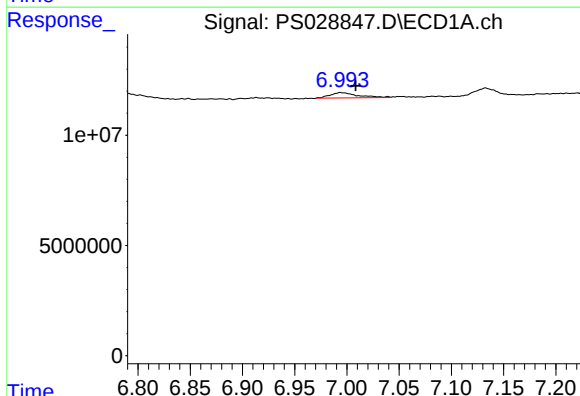


#3 4-Nitrophenol

R.T.: 6.995 min
Delta R.T.: -0.014 min
Response: 4493131
Conc: 2.99 ng/ml

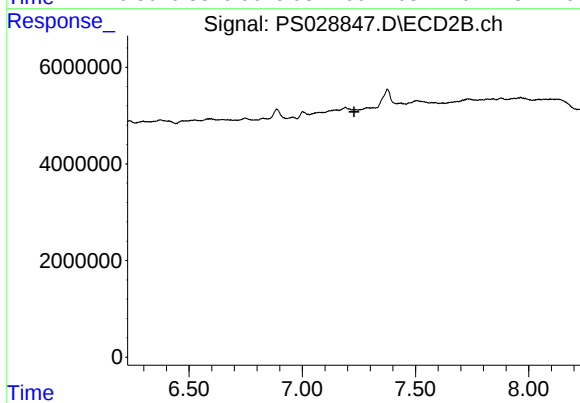

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

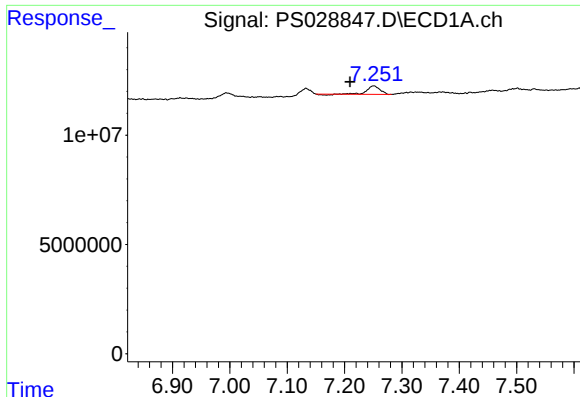

#4 2,4-DCAA


R.T.: 7.251 min
Delta R.T.: 0.041 min
Response: 5719833
Conc: 2.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

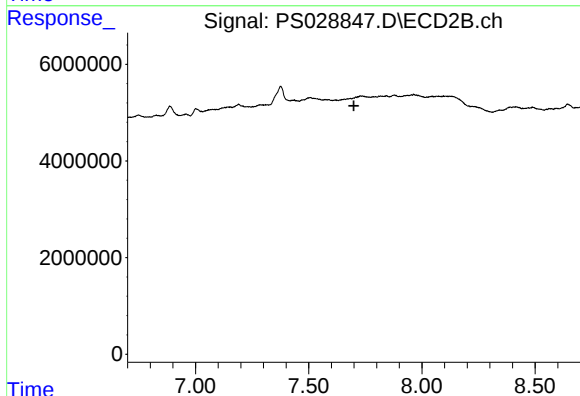


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.699 min
Response: 0
Conc: N.D.

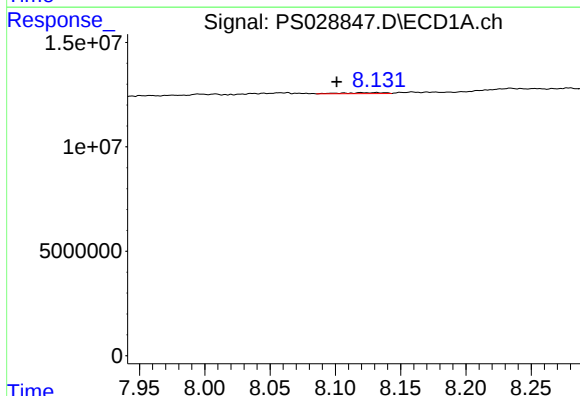


#8 DICHLORPROP

R.T.: 8.131 min
Delta R.T.: 0.030 min
Response: 976229
Conc: N.D.

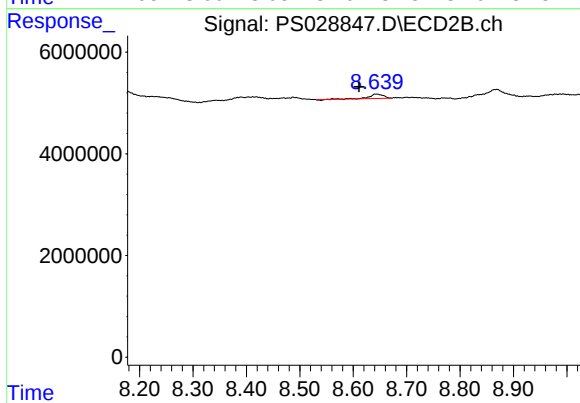

#8 DICHLORPROP


R.T.: 8.644 min
Delta R.T.: 0.033 min
Response: 1617023
Conc: 1.17 ng/ml

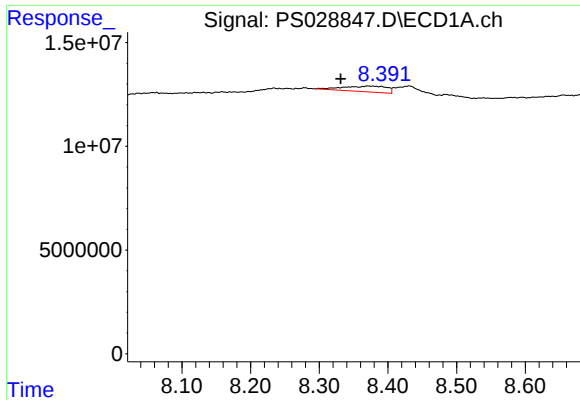

#9 2,4-D


R.T.: 8.372 min
Delta R.T.: 0.041 min
Response: 12048099
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

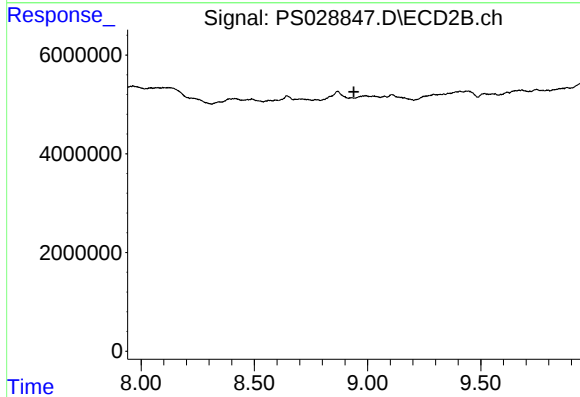


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.939 min
Response: 0
Conc: N.D.

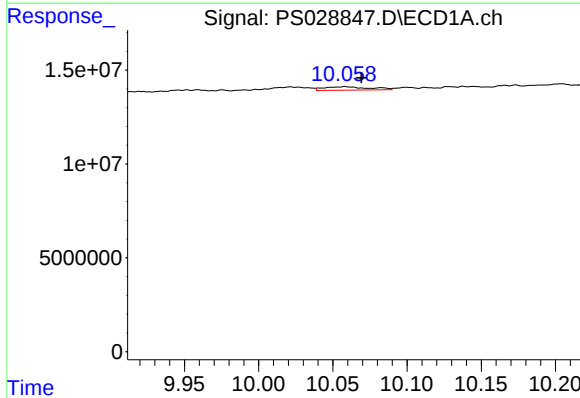


#13 2,4-DB

R.T.: 10.058 min
Delta R.T.: -0.011 min
Response: 3925389
Conc: 1.26 ng/ml

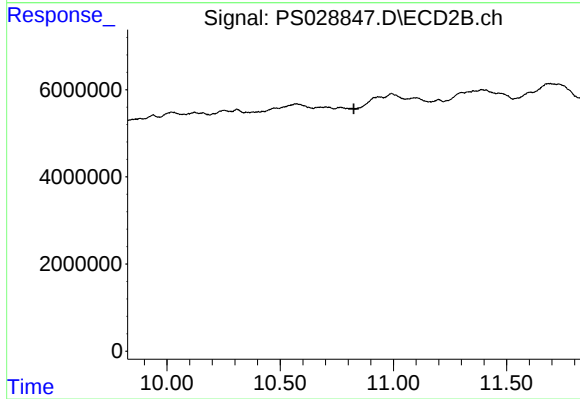

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.826 min
Response: 0
Conc: N.D.

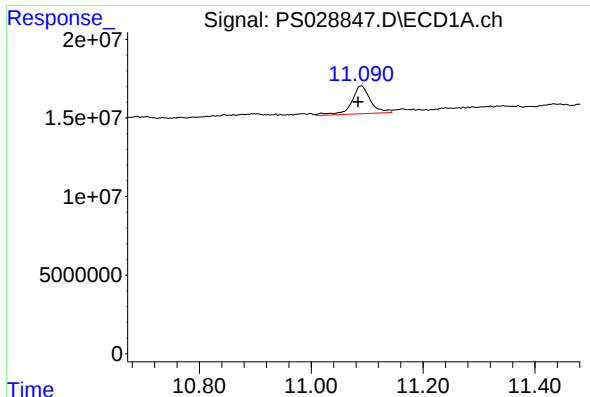

#15 Picloram


R.T.: 11.089 min
Delta R.T.: 0.005 min
Response: 41712621
Conc: 1.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

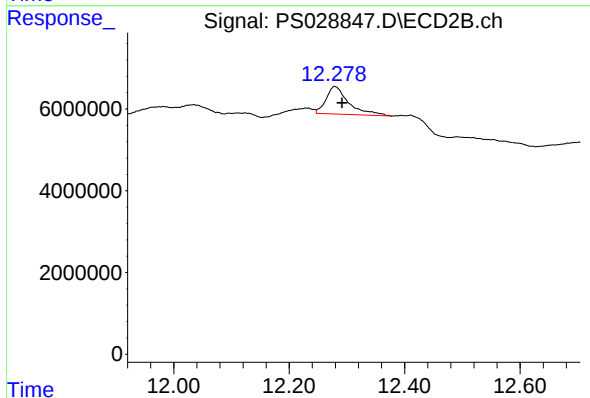


#15 Picloram

R.T.: 12.279 min
Delta R.T.: -0.013 min
Response: 18512163
Conc: 1.44 ng/ml

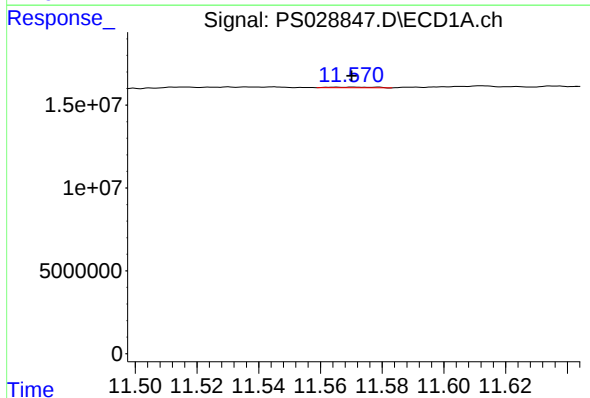

#16 DCPA

R.T.: 11.570 min
Delta R.T.: 0.000 min
Response: 404173
Conc: N.D.

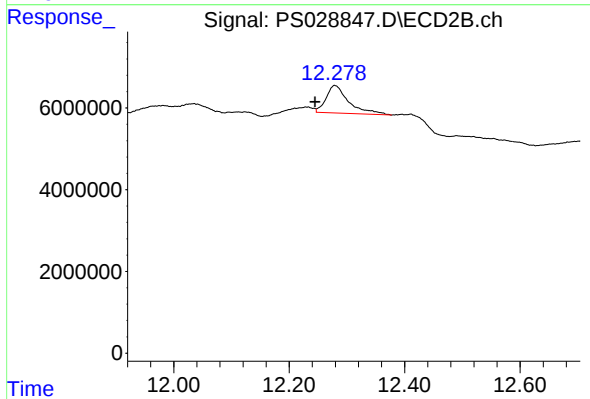

#16 DCPA

R.T.: 12.279 min
Delta R.T.: 0.034 min
Response: 18512163
Conc: 1.72 ng/ml