

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123119\
 Data File : PS008252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2019 09:13
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 11:38:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) T	2,4,5-T	7.324	7.144	84670664	62519303	7.046 14.958 #
14) T	DINOSEB	9.012	0.000	25082413	0	2.588 N.D. #
15) T	Picloram	8.867	8.826	404.2E6	213.9E6	163.983 32.767 #
16) T	DCPA	9.286	8.777	17725697	6597358	1.306 <MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123119\
Data File : PS008252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2019 09:13
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 11:38:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

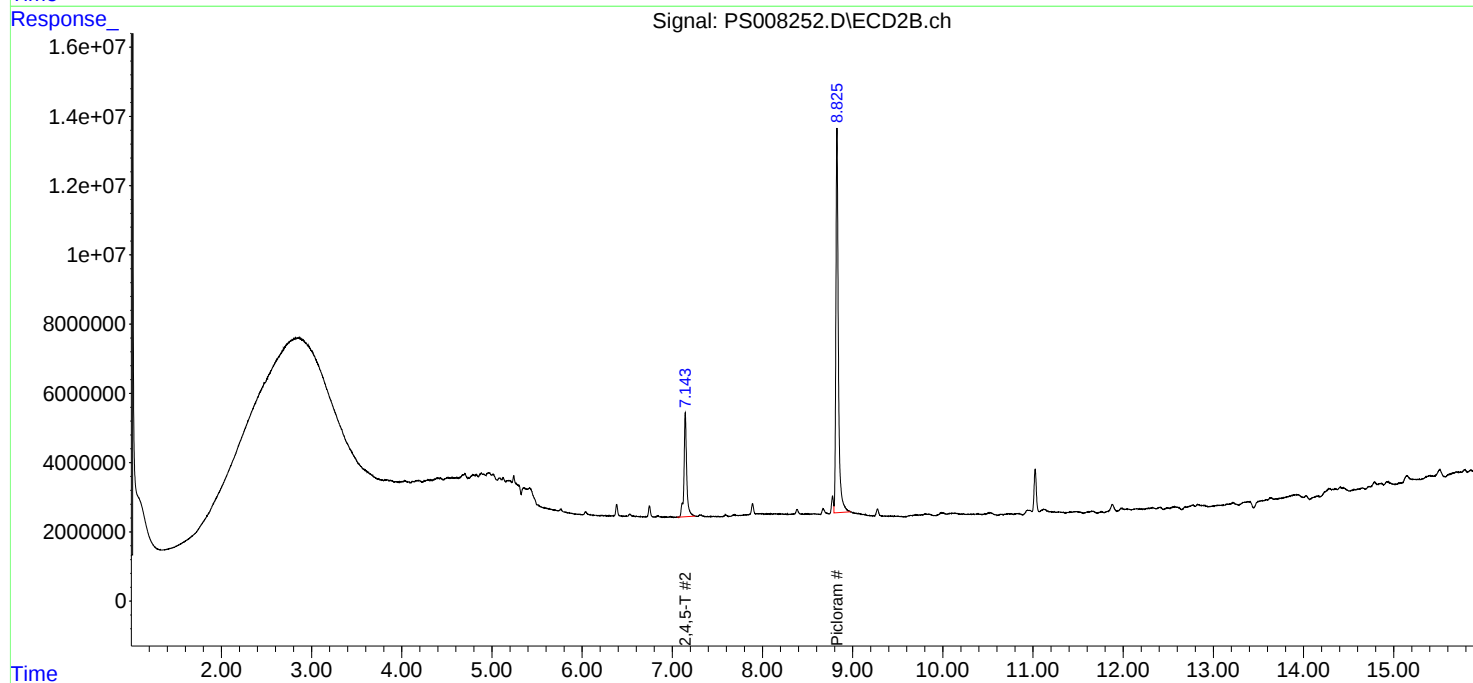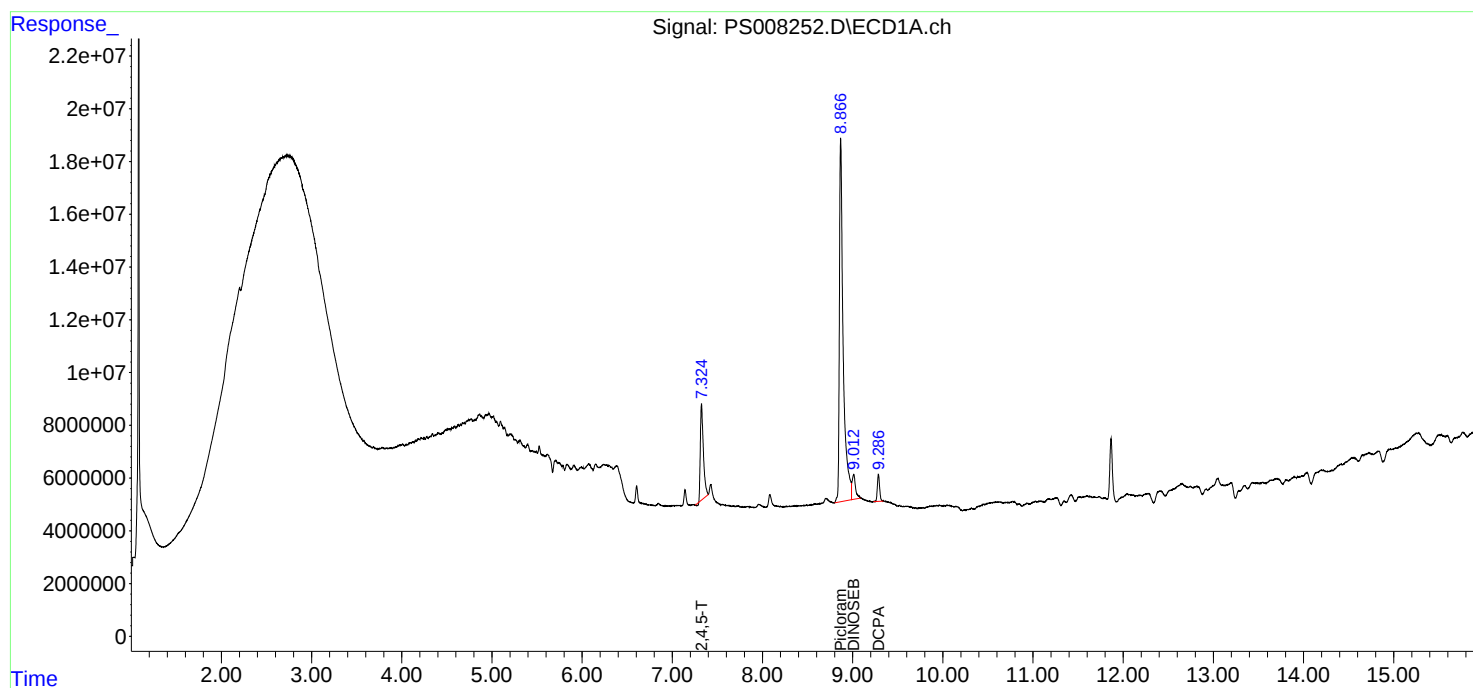


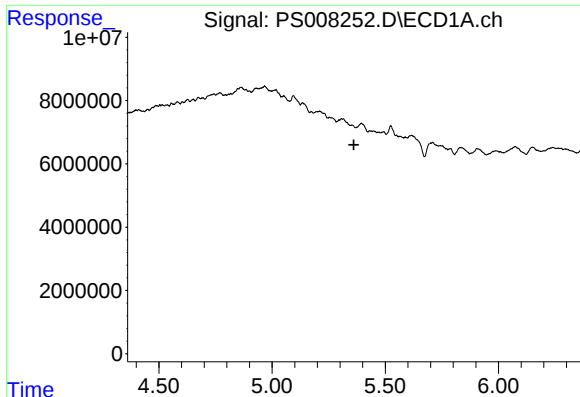

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

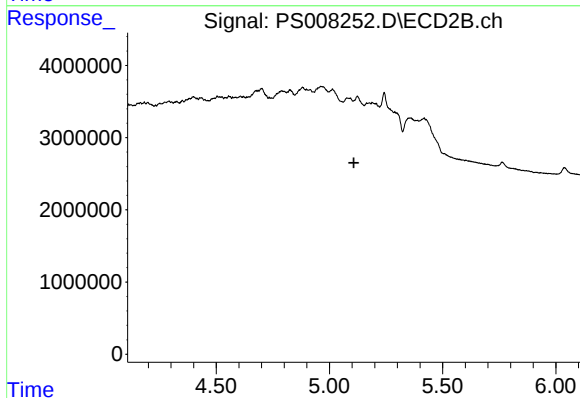


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

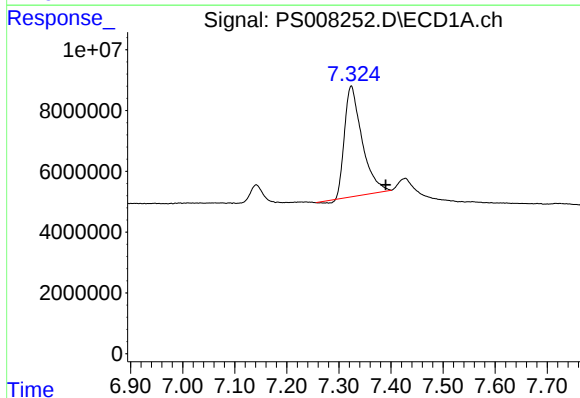


#12 2,4,5-T

R.T.: 7.324 min
Delta R.T.: -0.066 min
Response: 84670664
Conc: 7.05 ng/ml

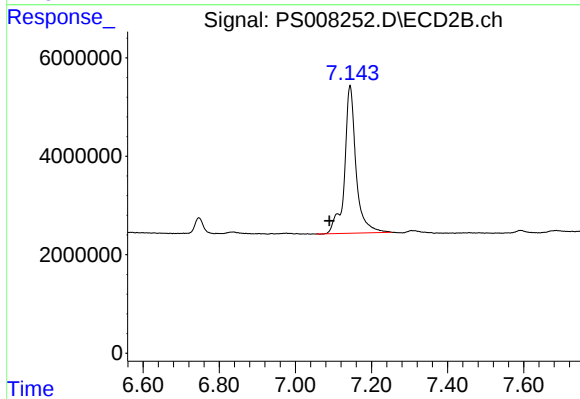

#12 2,4,5-T


R.T.: 7.144 min
Delta R.T.: 0.054 min
Response: 62519303
Conc: 14.96 ng/ml

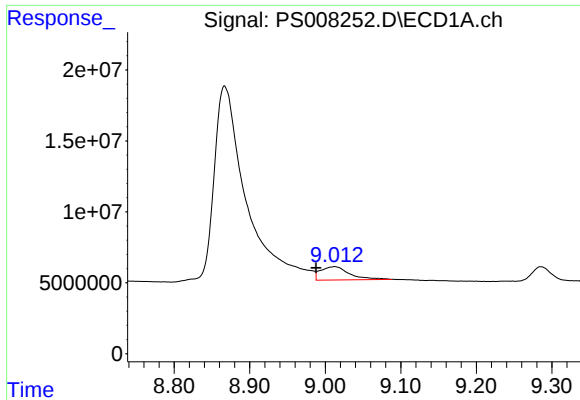

#14 DINOSEB


R.T.: 9.012 min
Delta R.T.: 0.024 min
Response: 25082413
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

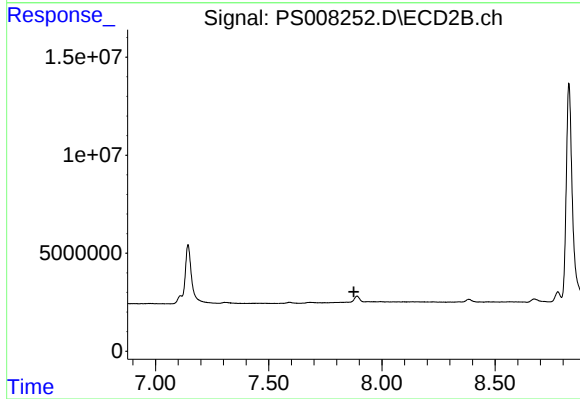


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 7.876 min
Response: 0
Conc: N.D.

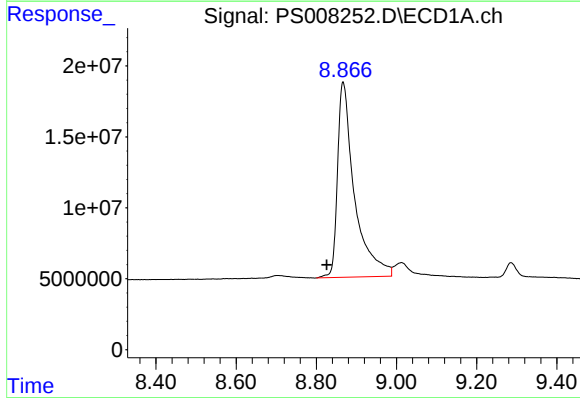


#15 Picloram

R.T.: 8.867 min
Delta R.T.: 0.041 min
Response: 404163412
Conc: 163.98 ng/ml

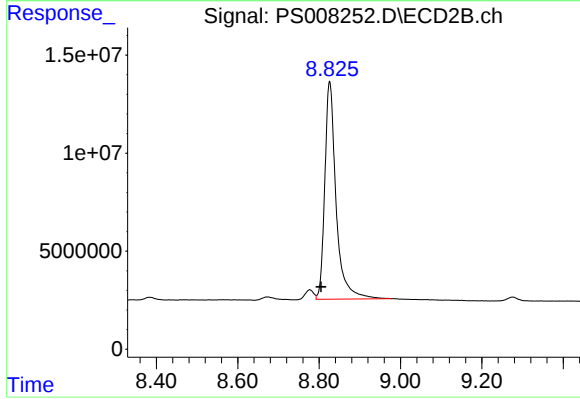

#15 Picloram


R.T.: 8.826 min
Delta R.T.: 0.021 min
Response: 213859894
Conc: 32.77 ng/ml

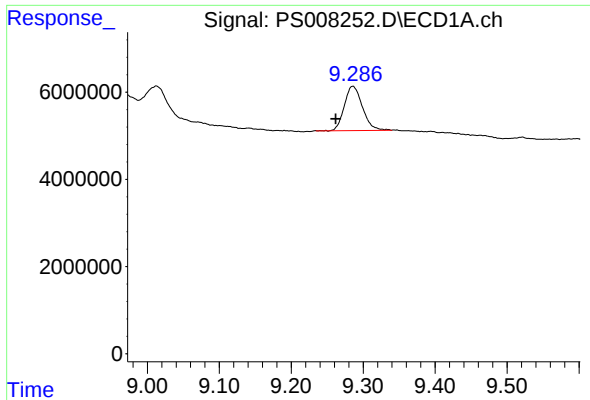

#16 DCPA

R.T.: 9.286 min
Delta R.T.: 0.024 min
Response: 17725697
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

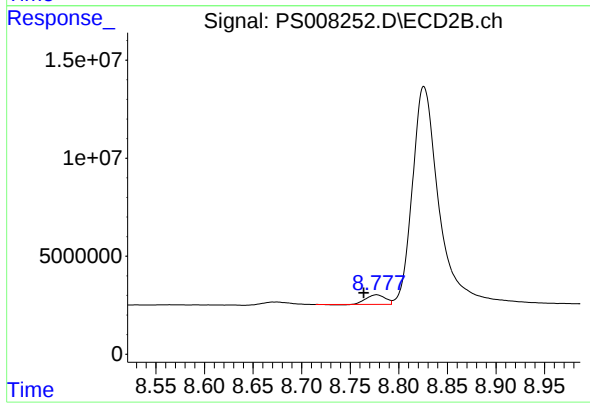

#16 DCPA

R.T.: 8.777 min
Delta R.T.: 0.013 min
Response: 6597358
Conc: N.D.