

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS123119\  
 Data File : PS008253.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 31 Dec 2019 09:35  
 Operator : SM\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 31 11:38:26 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS122619.M  
 Quant Title : 8080.M  
 QLast Update : Fri Dec 27 02:43:58 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2  | Resp#1     | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|-------|------------|---------|---------|---------|
| -----                       |          |       |       |            |         |         |         |
| System Monitoring Compounds |          |       |       |            |         |         |         |
| 4) S                        | 2,4-DCAA | 5.377 | 5.124 | 785.1E6    | 377.3E6 | 388.596 | 421.366 |
| Target Compounds            |          |       |       |            |         |         |         |
| 7) T                        | MCPA     | 0.000 | 5.440 | 0 29275681 |         | N.D.    | 7.695   |
| 15) T                       | Picloram | 0.000 | 8.848 | 0 125.8E6  |         | N.D.    | 19.275  |
| -----                       |          |       |       |            |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS123119\  
Data File : PS008253.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 31 Dec 2019 09:35  
Operator : SM\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 31 11:38:26 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS122619.M  
Quant Title : 8080.M  
QLast Update : Fri Dec 27 02:43:58 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

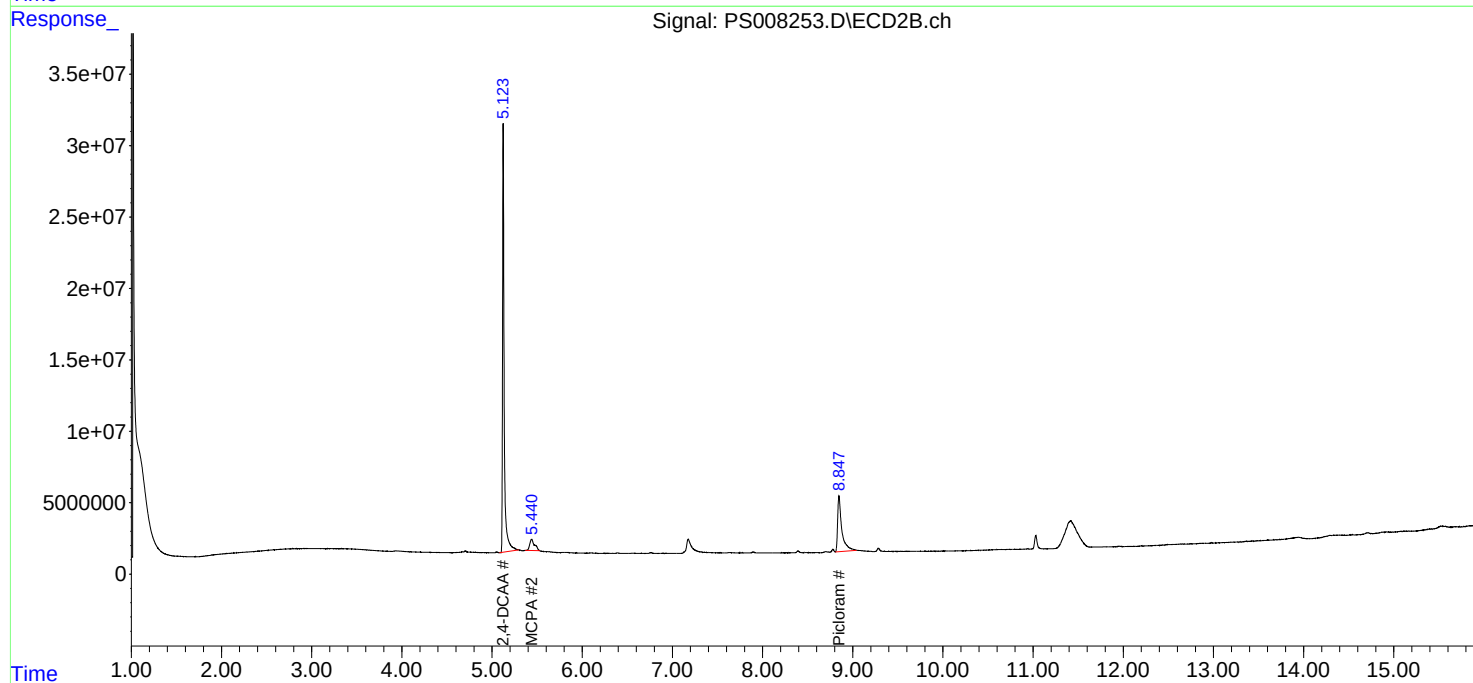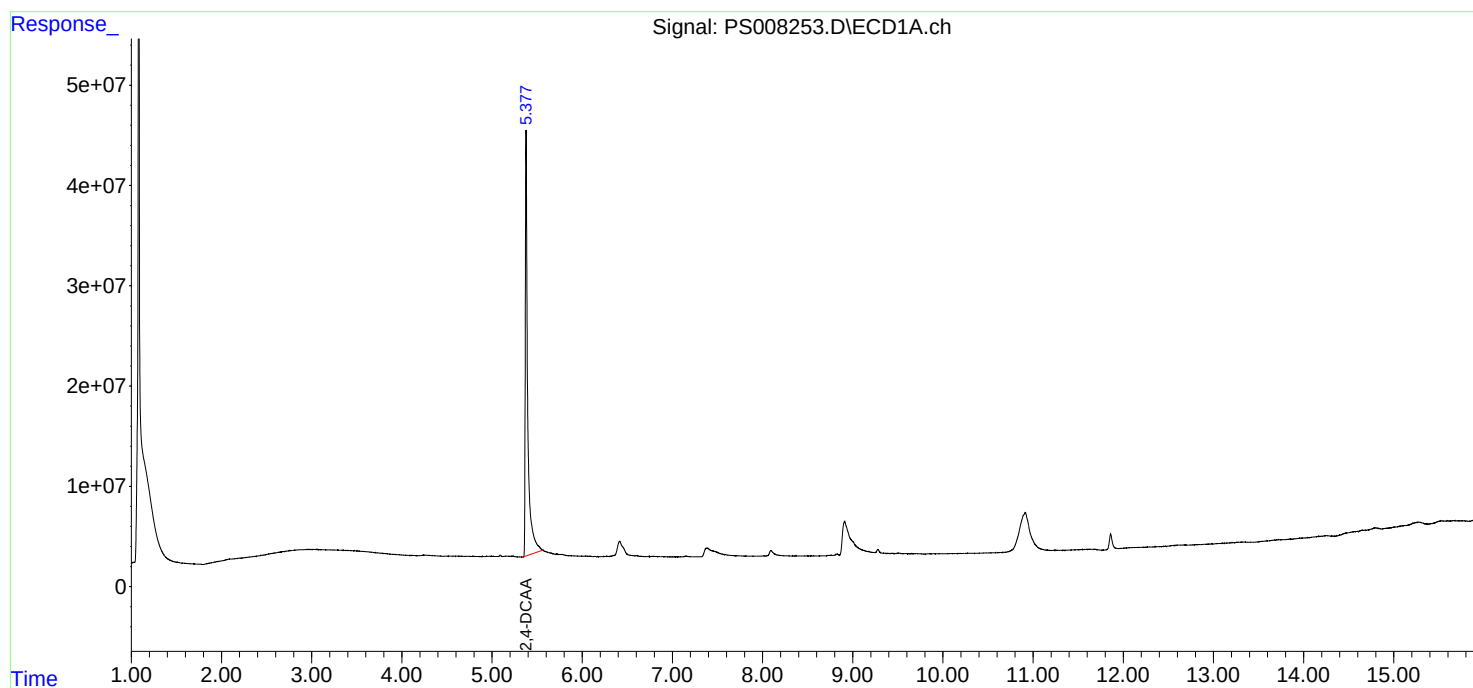


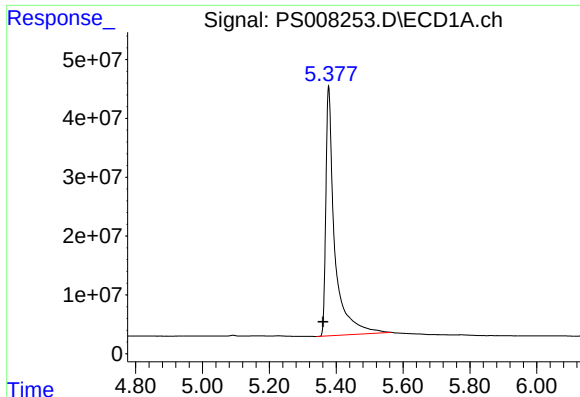

#4 2,4-DCAA


R.T.: 5.377 min  
Delta R.T.: 0.016 min  
Response: 785097502  
Conc: 388.60 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

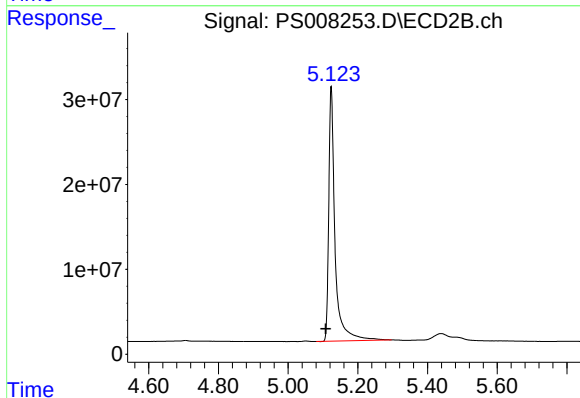


#4 2,4-DCAA

R.T.: 5.124 min  
Delta R.T.: 0.015 min  
Response: 377283940  
Conc: 421.37 ng/ml

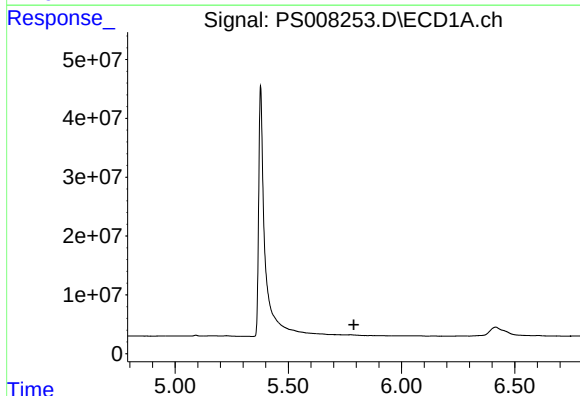


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 5.789 min  
Response: 0  
Conc: N.D.

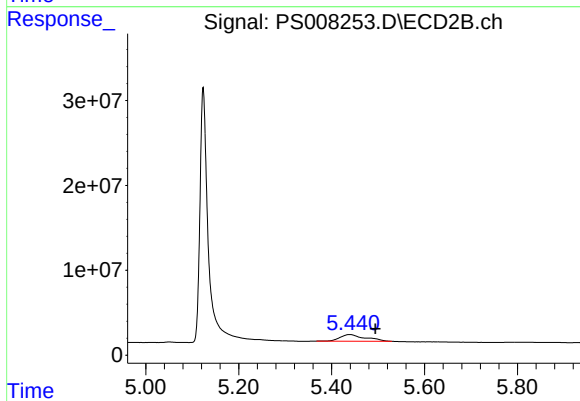

#7 MCPA


R.T.: 5.440 min  
Delta R.T.: -0.054 min  
Response: 29275681  
Conc: 7.70 ug/ml

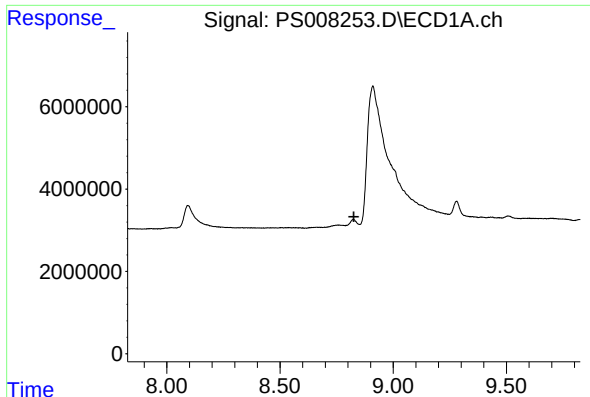

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 8.826 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

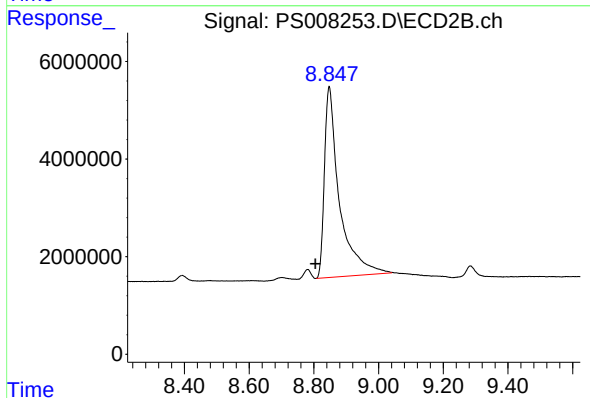

#15 Picloram

R.T.: 8.848 min  
Delta R.T.: 0.043 min  
Response: 125803197  
Conc: 19.28 ng/ml