

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123119\
 Data File : PS008265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2019 15:21
 Operator : SM\AJ
 Sample : PB125823BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125823BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 16:36:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.362	5.110	795.2E6	400.9E6	393.614	447.749
Target Compounds							
1) T	Dalapon	1.941	1.659	43146590	19287930	17.973	18.907
2) T	3,5-DICHL...	0.000	4.448	0	52453726	N.D.	45.048
5) T	DICAMBA	5.449	5.209	117.7E6	9680443	16.193	2.841 #
7) T	MCPA	5.817	5.474	38308324	31154120	5.009	8.189 #
9) T	2,4-D	6.393	0.000	91700462	0	55.881	N.D. #
10) T	Pentachlo...	0.000	6.306	0	52266082	N.D.	4.107
11) T	2,4,5-TP ...	0.000	6.695	0	27811814	N.D.	5.566
14) T	DINOSEB	0.000	7.874	0	6363865	N.D.	1.699
15) T	Picloram	0.000	8.838	0	10497961	N.D.	1.608



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123119\
Data File : PS008265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2019 15:21
Operator : SM\AJ
Sample : PB125823BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125823BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 16:36:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

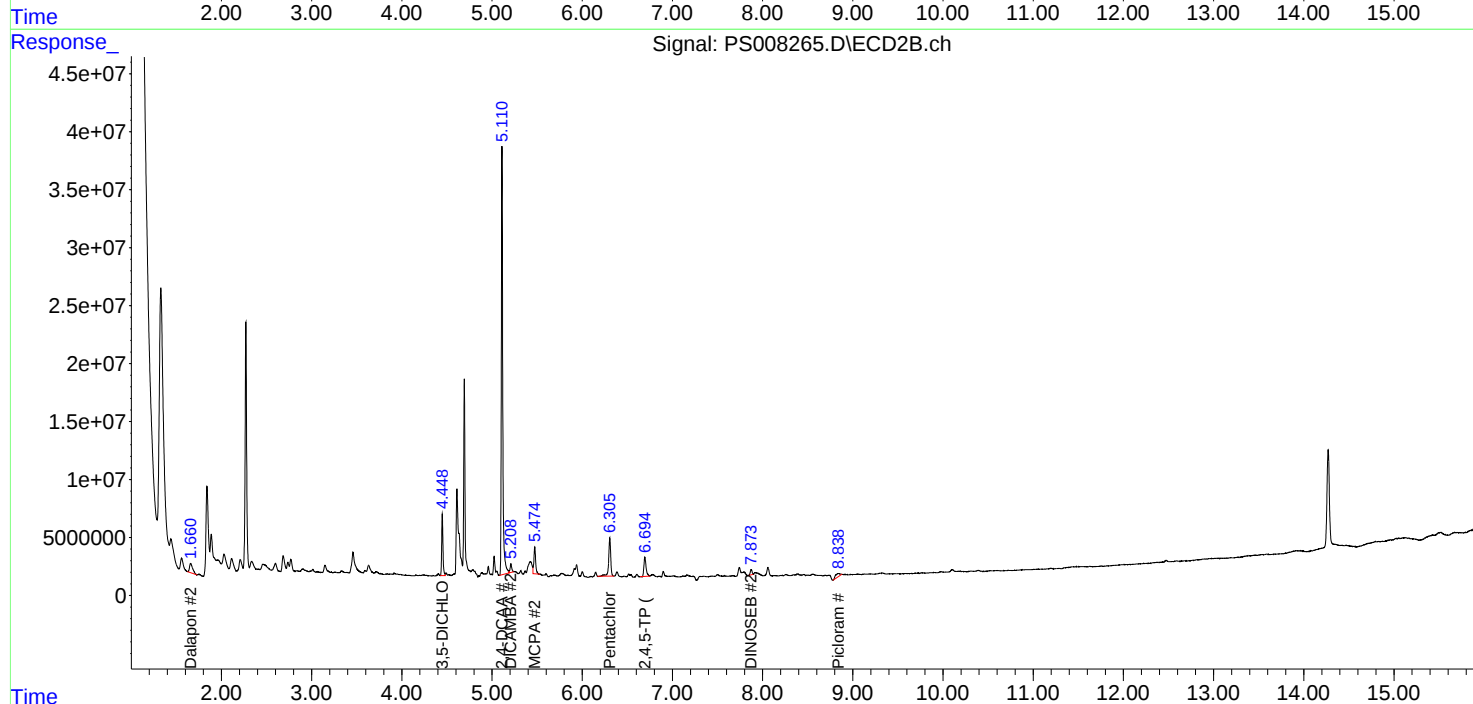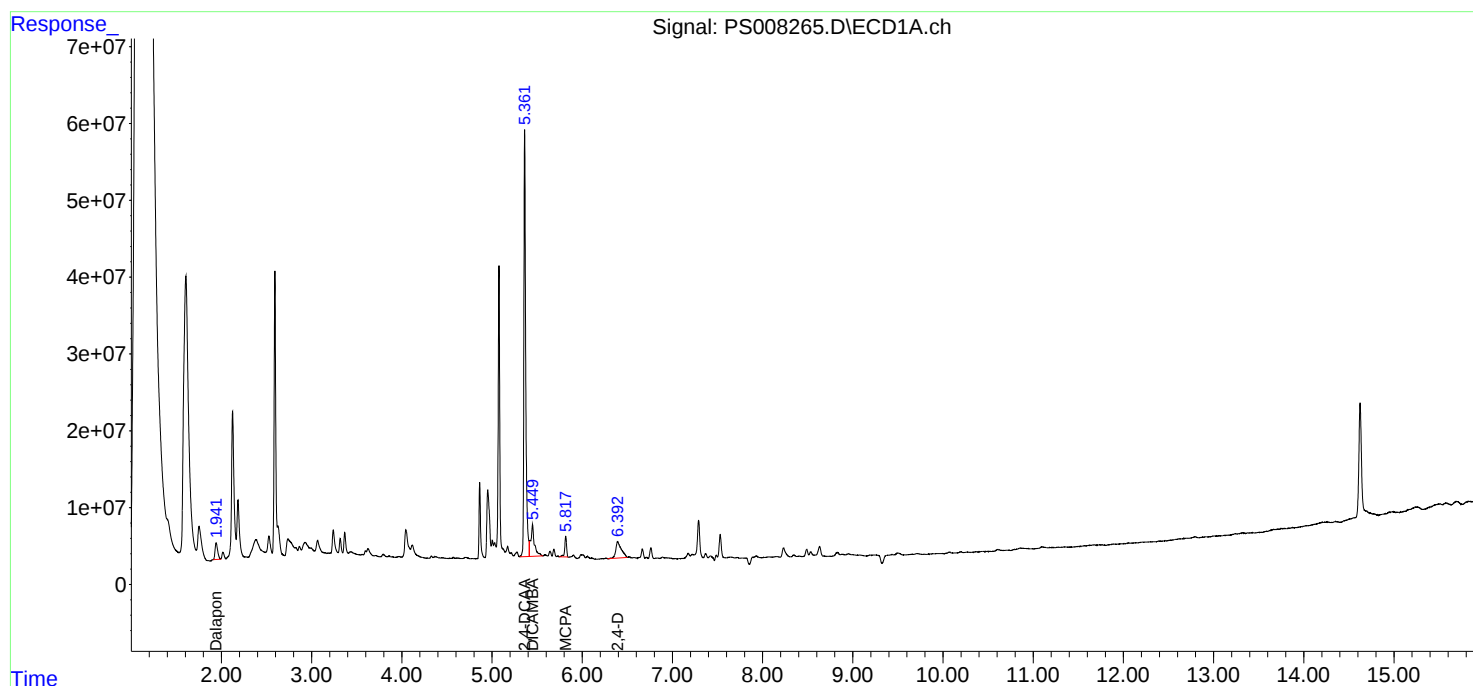


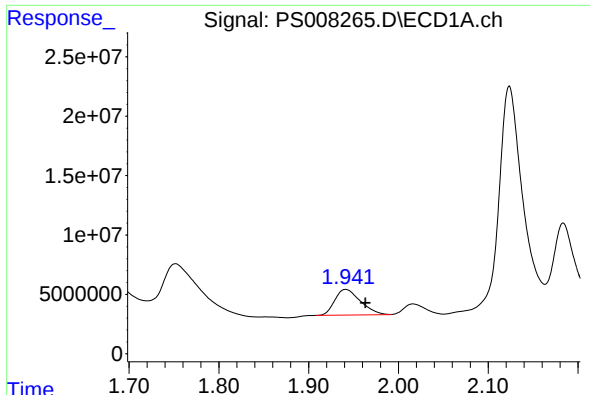

#1 Dalapon


R.T.: 1.941 min
Delta R.T.: -0.022 min
Response: 43146590
Conc: 17.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125823BL

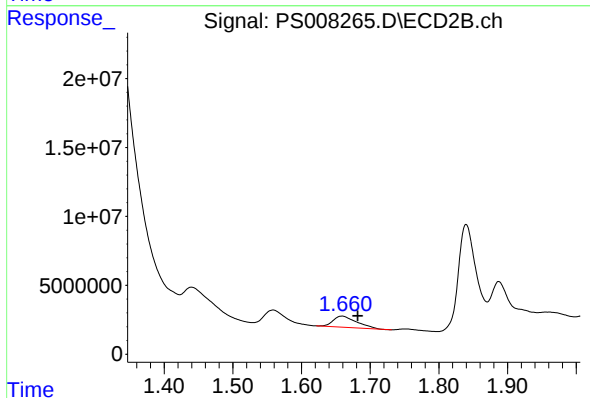


#1 Dalapon

R.T.: 1.659 min
Delta R.T.: -0.023 min
Response: 19287930
Conc: 18.91 ng/ml

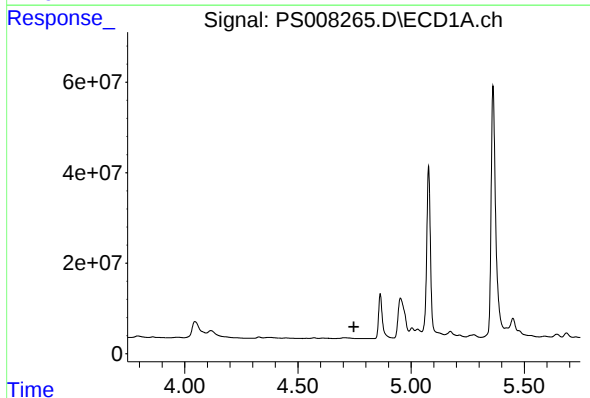


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

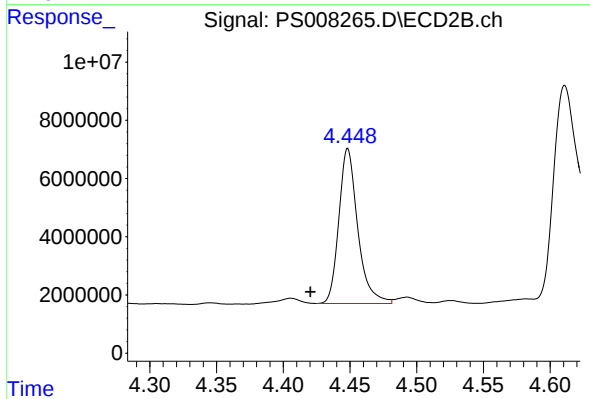

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: 0.028 min
Response: 52453726
Conc: 45.05 ng/ml

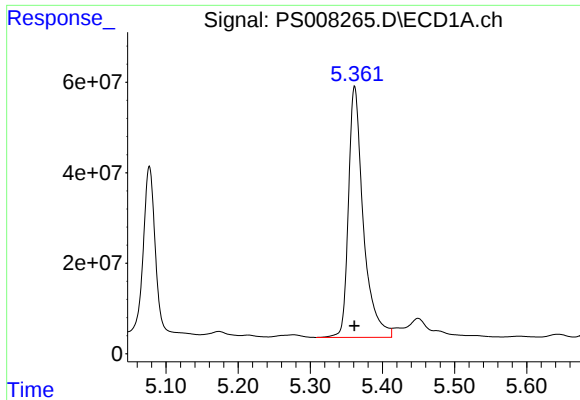

#4 2,4-DCAA


R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 795234263
Conc: 393.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125823BL

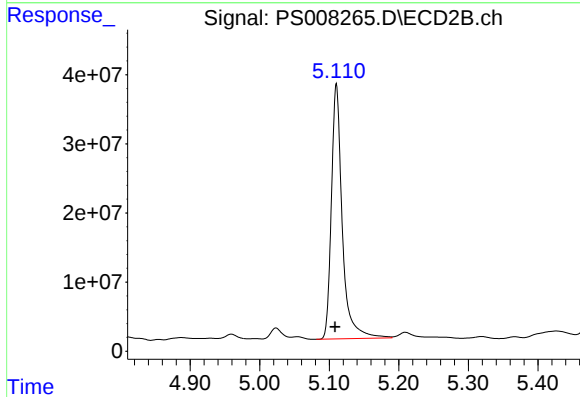


#4 2,4-DCAA

R.T.: 5.110 min
Delta R.T.: 0.002 min
Response: 400906468
Conc: 447.75 ng/ml

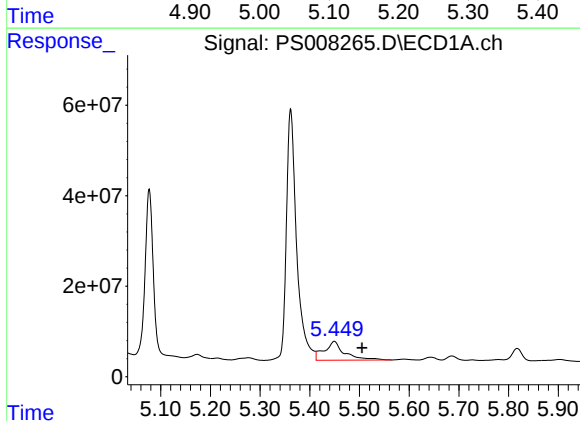


#5 DICAMBA

R.T.: 5.449 min
Delta R.T.: -0.056 min
Response: 117747612
Conc: 16.19 ng/ml

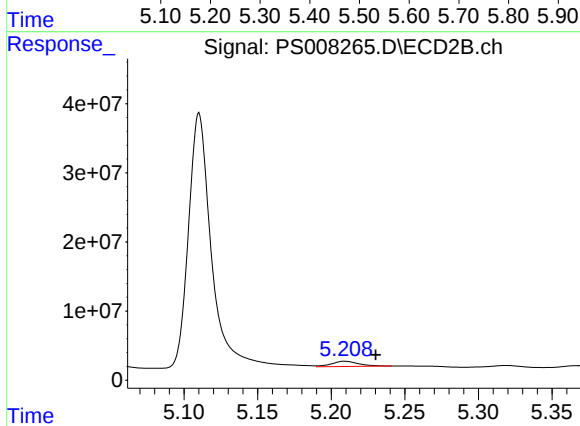

#5 DICAMBA


R.T.: 5.209 min
Delta R.T.: -0.021 min
Response: 9680443
Conc: 2.84 ng/ml

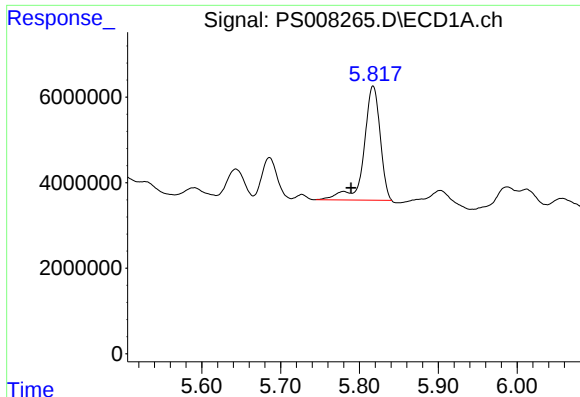

#7 MCPA


R.T.: 5.817 min
Delta R.T.: 0.028 min
Response: 38308324
Conc: 5.01 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125823BL

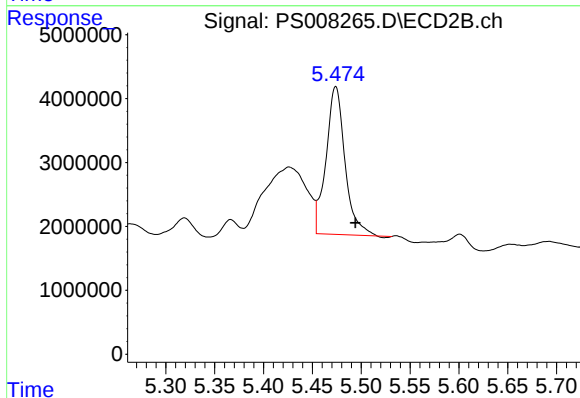


#7 MCPA

R.T.: 5.474 min
Delta R.T.: -0.020 min
Response: 31154120
Conc: 8.19 ug/ml

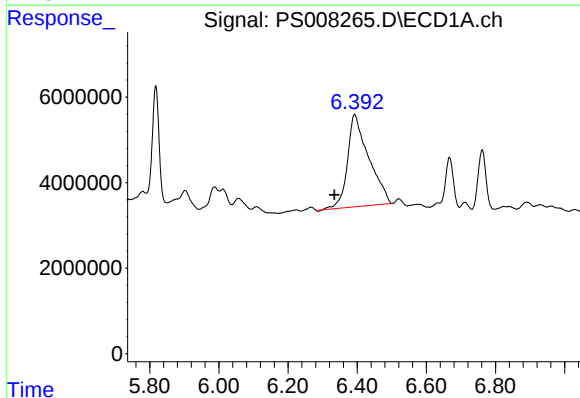


#9 2,4-D

R.T.: 6.393 min
Delta R.T.: 0.058 min
Response: 91700462
Conc: 55.88 ng/ml

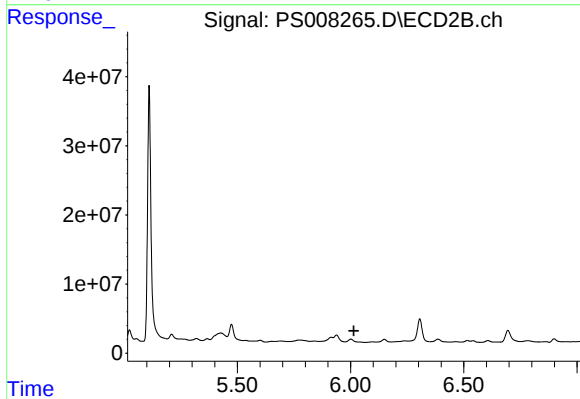

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

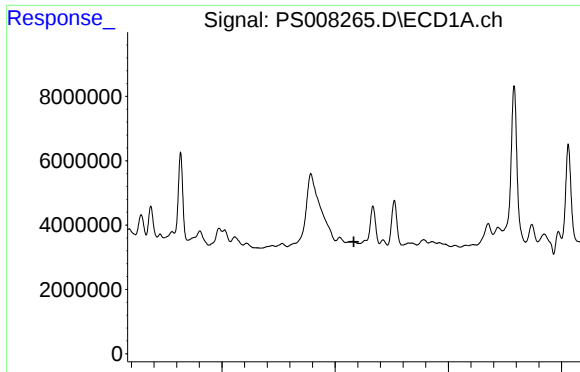

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125823BL

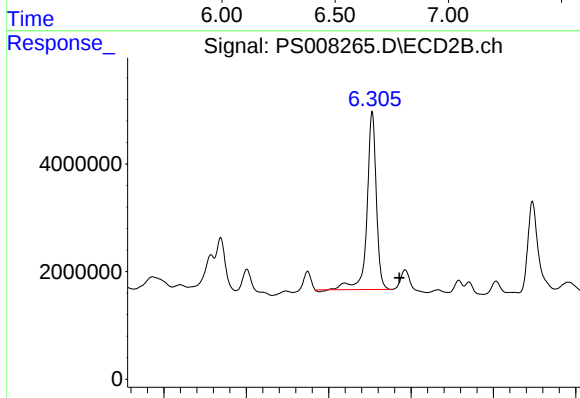


#10 Pentachlorophenol

R.T.: 6.306 min
Delta R.T.: -0.066 min
Response: 52266082
Conc: 4.11 ng/ml

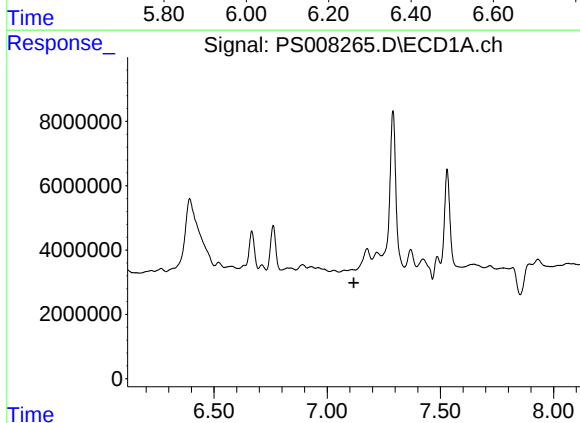


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

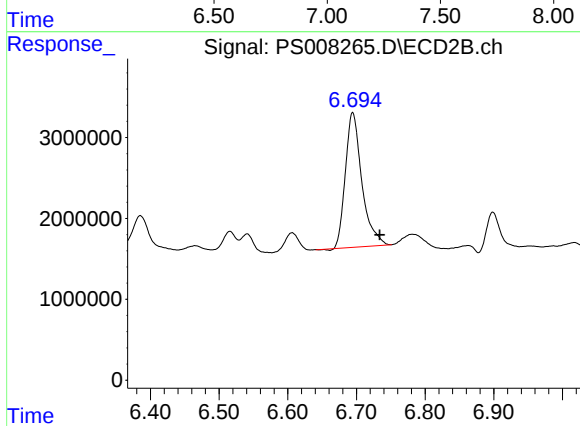

#11 2,4,5-TP (SILVEX)


R.T.: 6.695 min
Delta R.T.: -0.039 min
Response: 27811814
Conc: 5.57 ng/ml

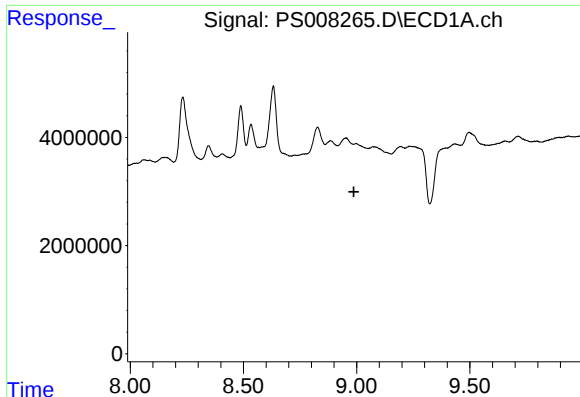

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125823BL

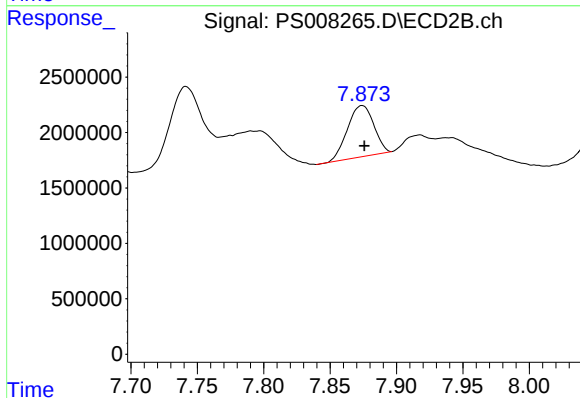


#14 DINOSEB

R.T.: 7.874 min
Delta R.T.: -0.002 min
Response: 6363865
Conc: 1.70 ng/ml

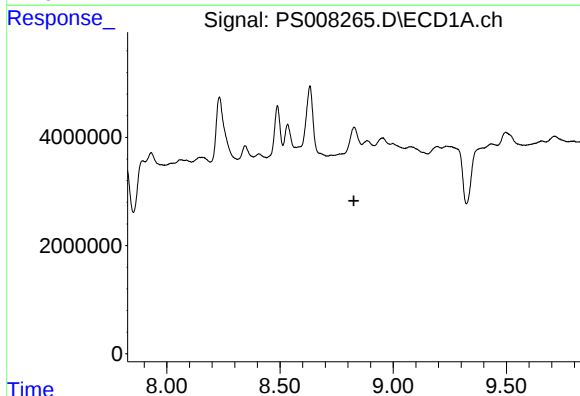

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

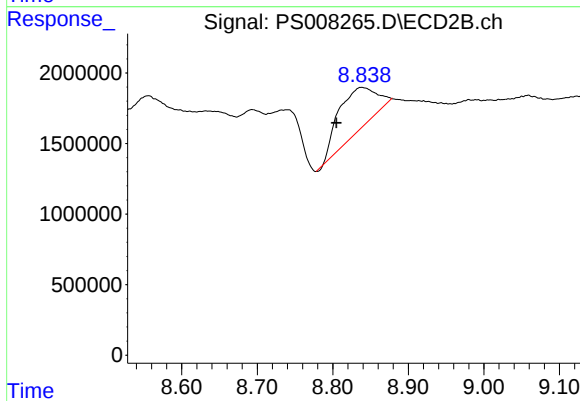

#15 Picloram

R.T.: 8.838 min
Delta R.T.: 0.033 min
Response: 10497961
Conc: 1.61 ng/ml