

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123120\
 Data File : PS013626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 10:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 14:46:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.915	401.4E6	207.5E6	431.118	527.470
Target Compounds							
5) T	DICAMBA	0.000	7.083	0	4476320	N.D.	2.663
10) T	Pentachlo...	8.642	8.438	11486277	5926387	<MDL	1.051 #
12) T	2,4,5-T	9.483	0.000	9386180	0	1.698	N.D. #
14) T	DINOSEB	11.181	0.000	27858590	0	6.574	N.D. #
15) T	Picloram	0.000	10.942f	0	6145280	N.D.	1.765
16) T	DCPA	11.449	10.942	10925525	6145280	1.611	2.021 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123120\
Data File : PS013626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 10:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 14:46:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

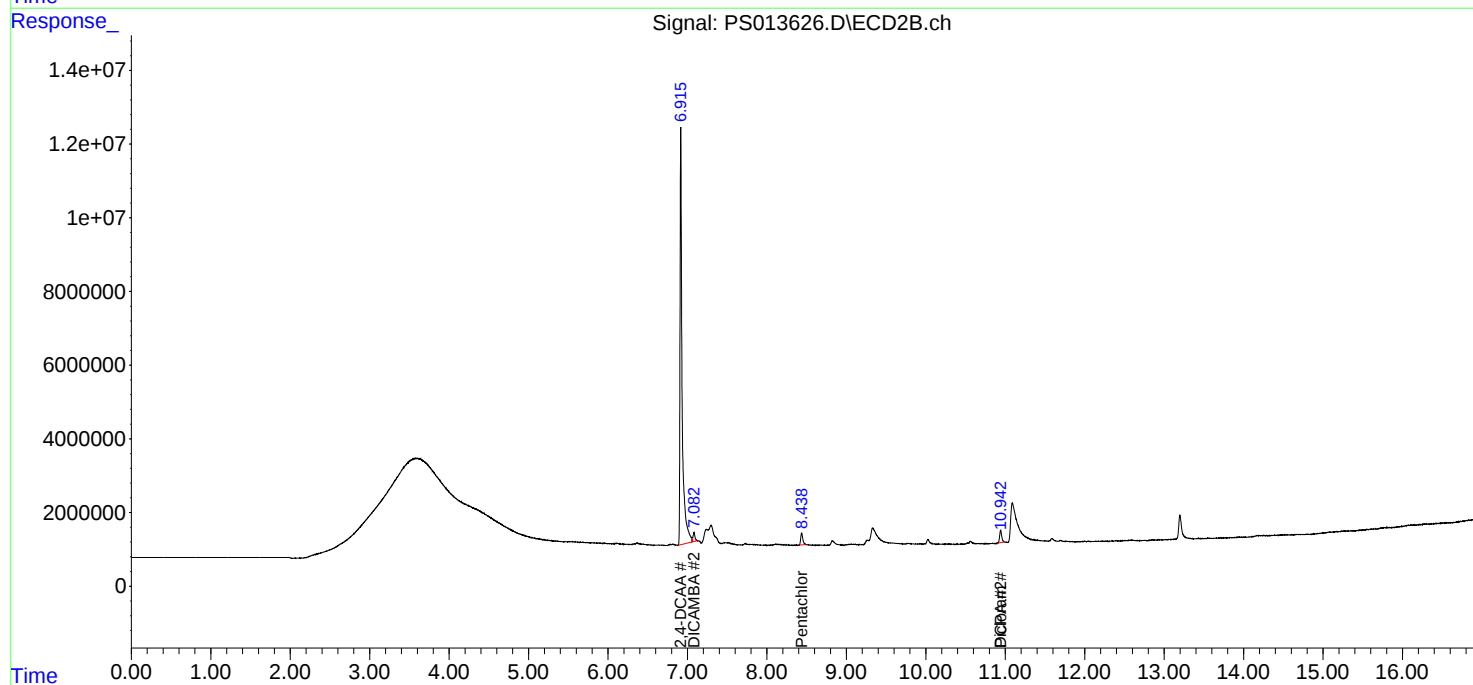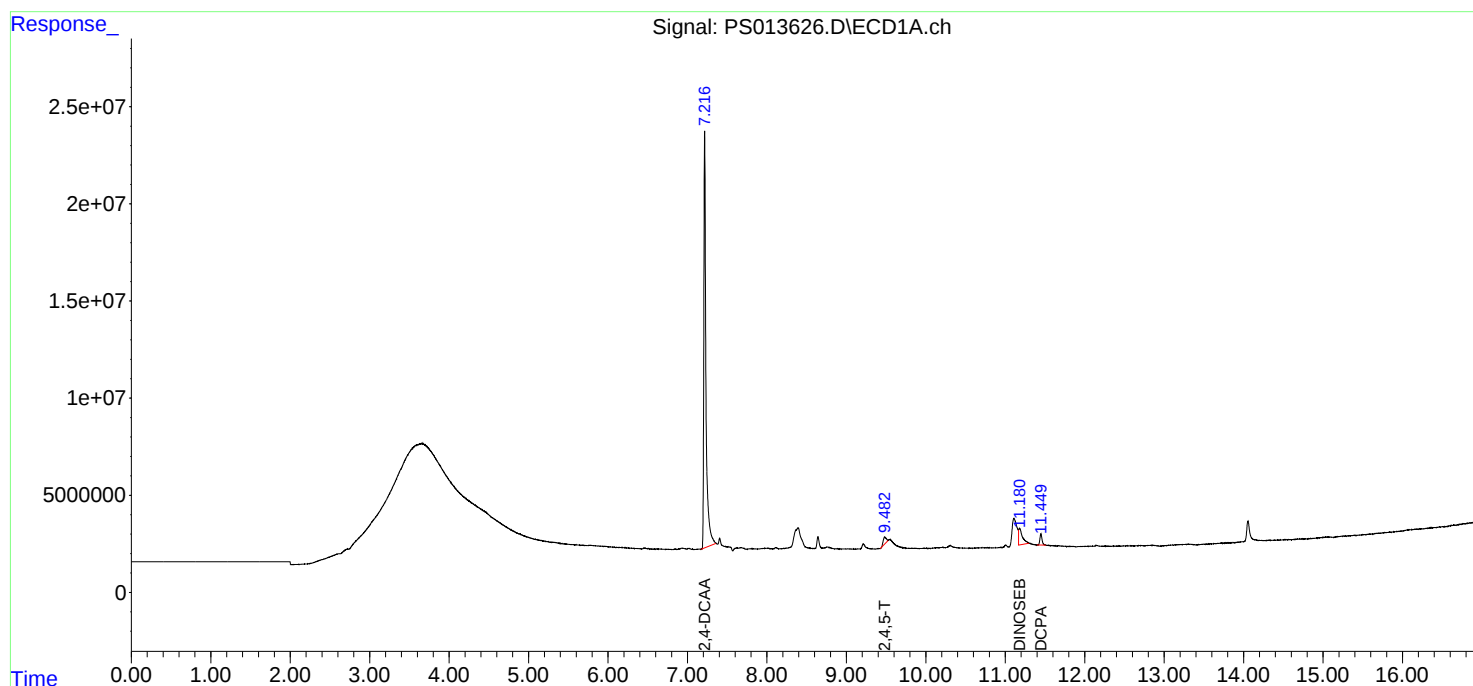


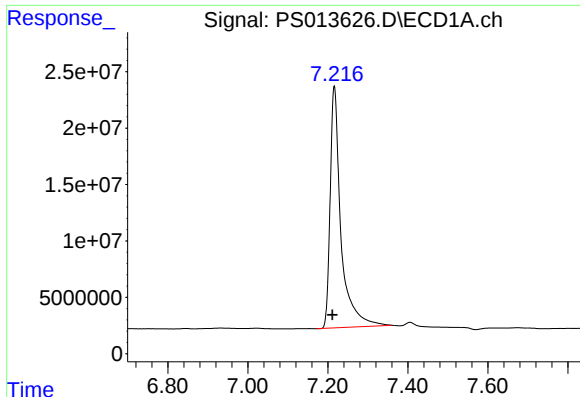

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.005 min
Response: 401396596
Conc: 431.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

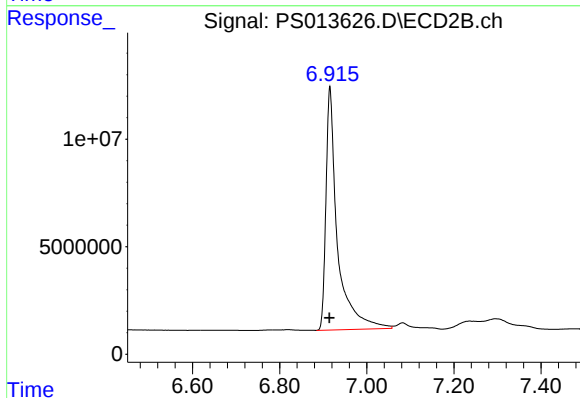


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.001 min
Response: 207486447
Conc: 527.47 ng/ml

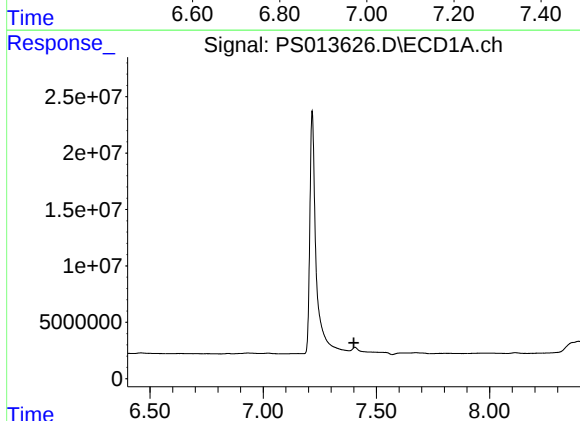


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

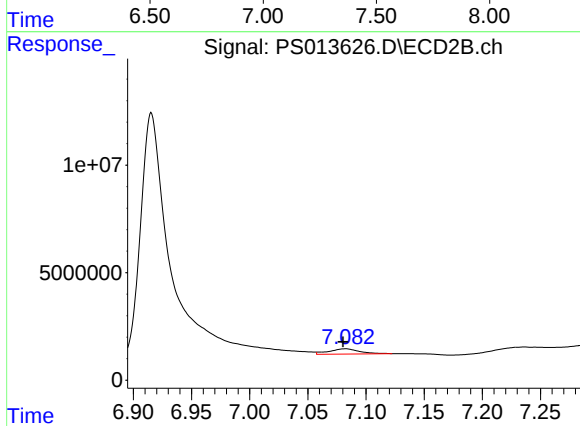

#5 DICAMBA


R.T.: 7.083 min
Delta R.T.: 0.003 min
Response: 4476320
Conc: 2.66 ng/ml

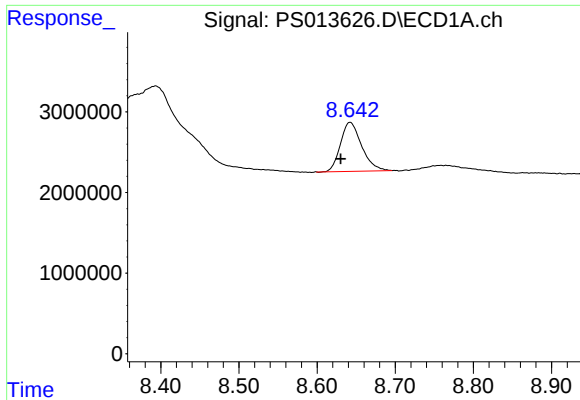

#10 Pentachlorophenol


R.T.: 8.642 min
Delta R.T.: 0.012 min
Response: 11486277
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

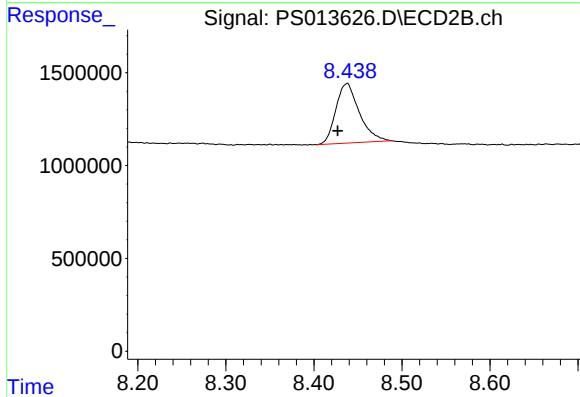


#10 Pentachlorophenol

R.T.: 8.438 min
Delta R.T.: 0.011 min
Response: 5926387
Conc: 1.05 ng/ml

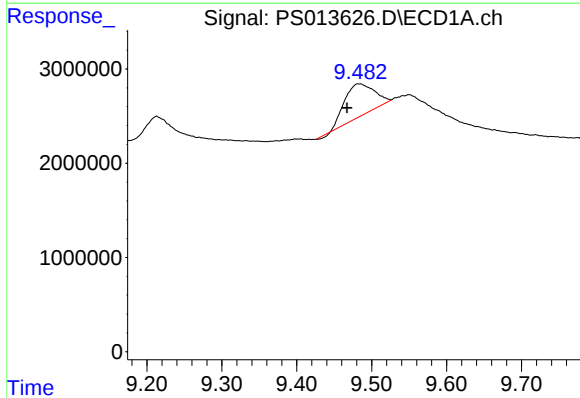


#12 2,4,5-T

R.T.: 9.483 min
Delta R.T.: 0.016 min
Response: 9386180
Conc: 1.70 ng/ml

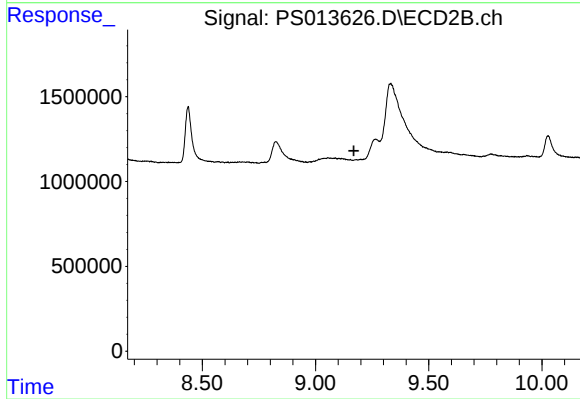

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

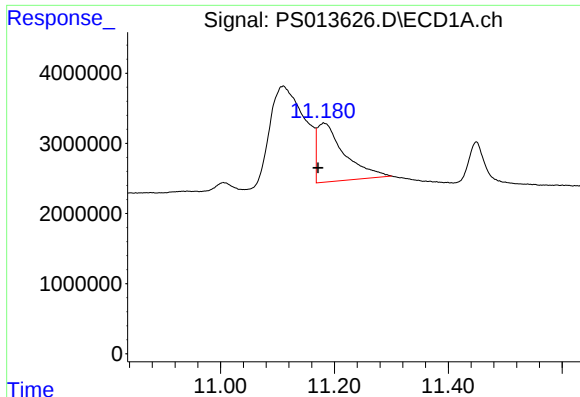

#14 DINOSEB


R.T.: 11.181 min
Delta R.T.: 0.010 min
Response: 27858590
Conc: 6.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

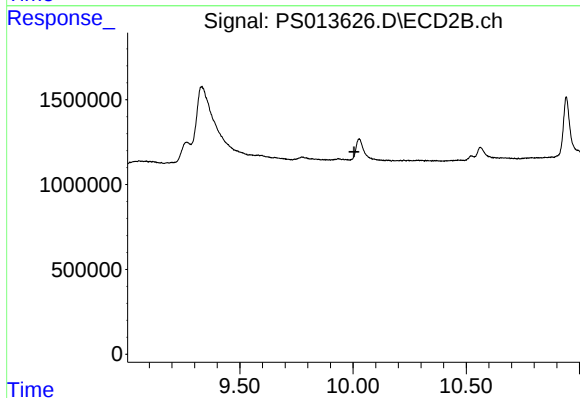


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.004 min
Response: 0
Conc: N.D.

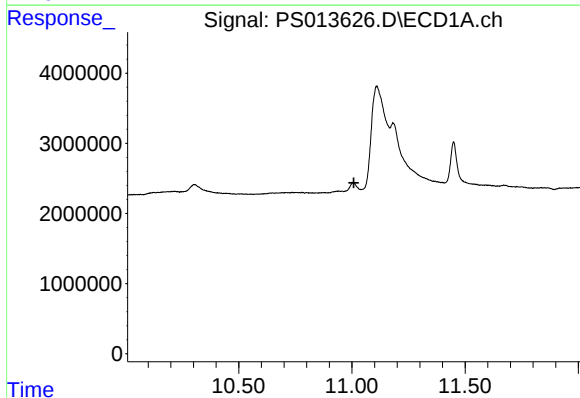


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

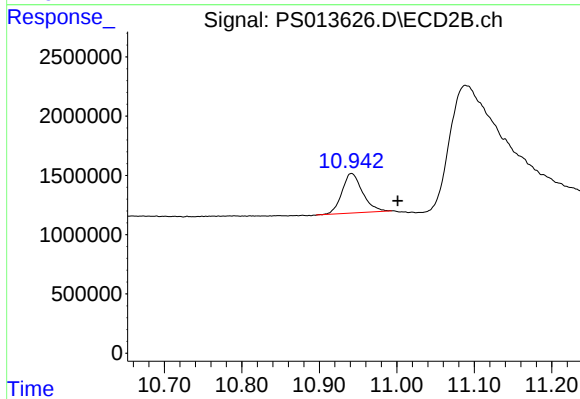

#15 Picloram


R.T.: 10.942 min
Delta R.T.: -0.059 min
Response: 6145280
Conc: 1.76 ng/ml

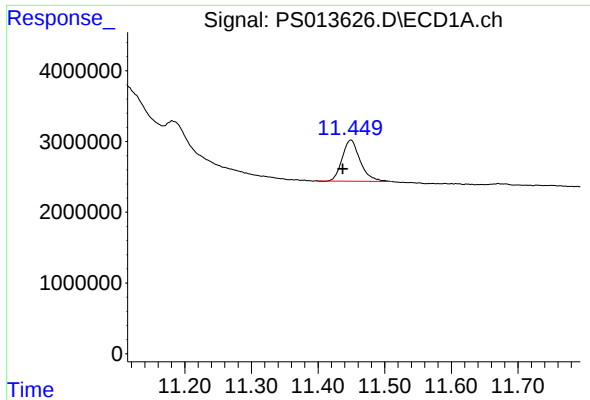

#16 DCPA

R.T.: 11.449 min
Delta R.T.: 0.012 min
Response: 10925525
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

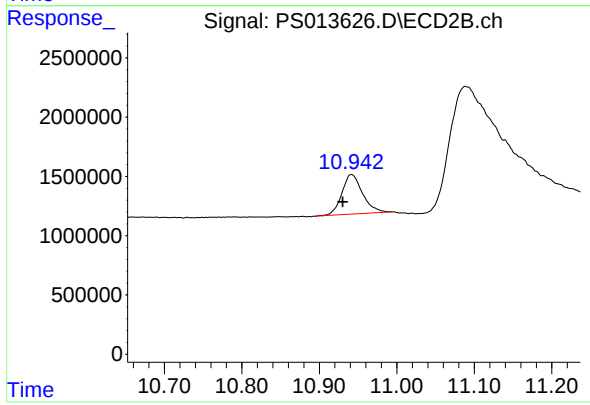

#16 DCPA

R.T.: 10.942 min
Delta R.T.: 0.012 min
Response: 6145280
Conc: 2.02 ng/ml