

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123120\
 Data File : PS013635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 13:27
 Operator : DD\AJ
 Sample : L5242-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-1(494+26)

Manual Integrations
 APPROVED

Ankita
 1/4/2021 2:26:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 14:49:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.208	6.911	189.9E6	100.7E6	204.000m	256.019 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123120\
Data File : PS013635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 13:27
Operator : DD\AJ
Sample : L5242-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SAMPLE-1(494+26)


Manual Integrations
APPROVED

Ankita
1/4/2021 2:26:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 14:49:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

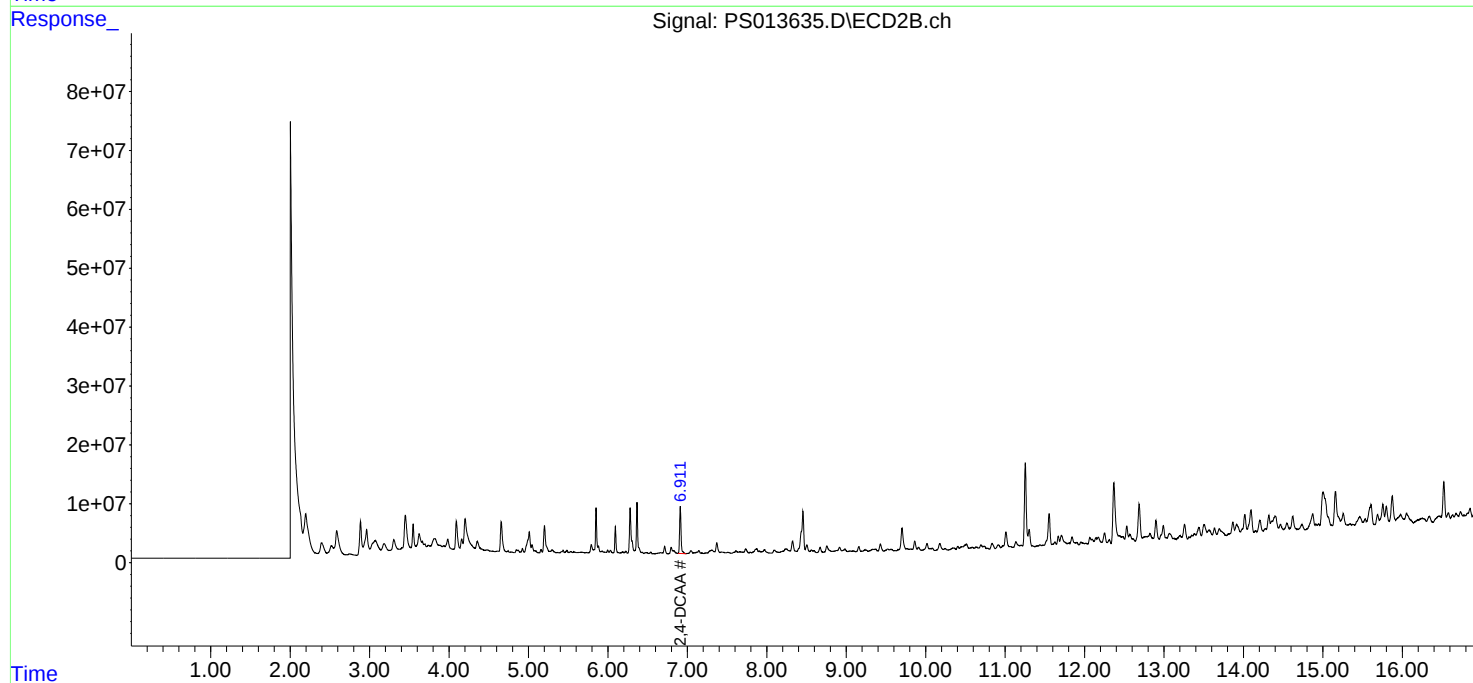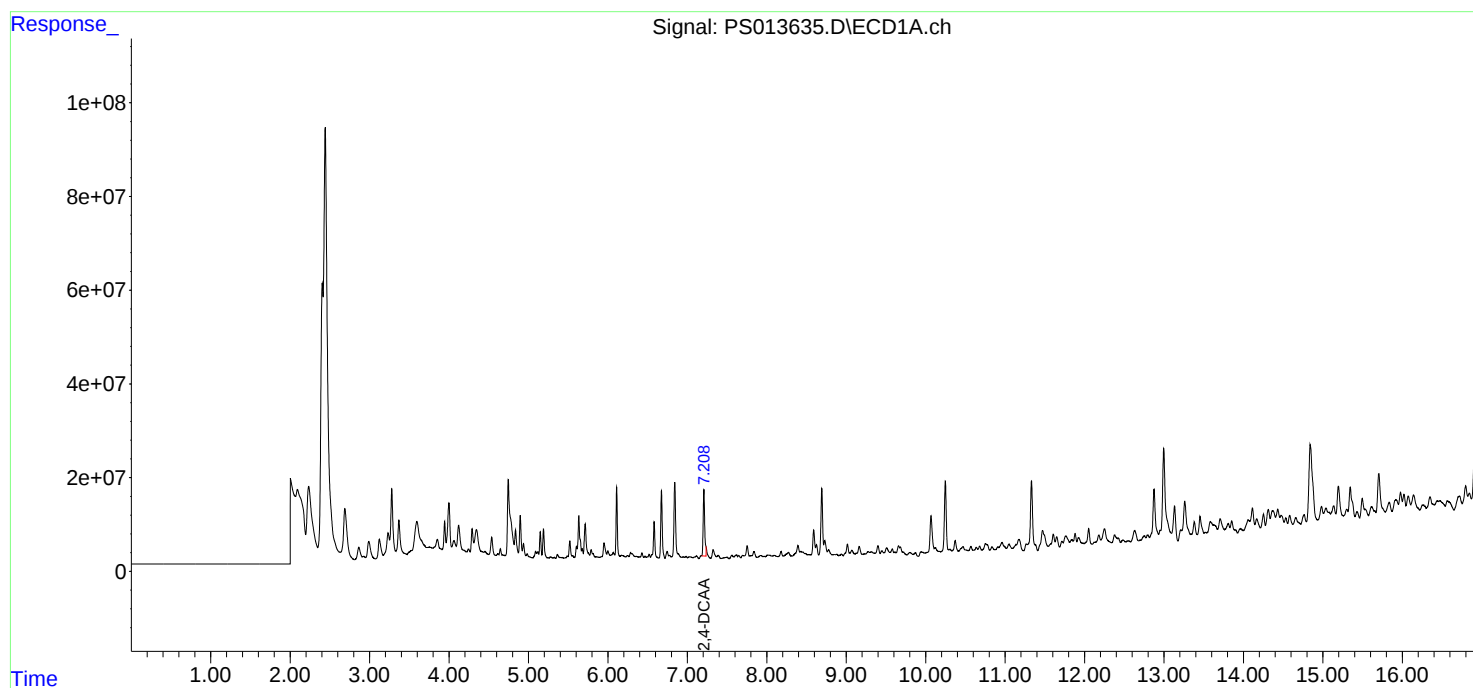

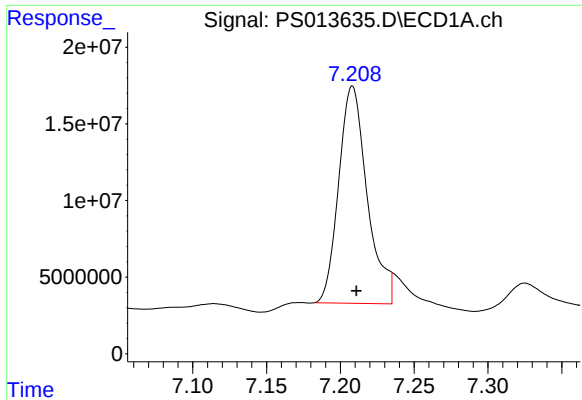


#4 2,4-DCAA

R.T.: 7.208 min
Delta R.T.: -0.003 min
Response: 189935701
Conc: 204.00 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SAMPLE-1(494+26)

Manual Integrations
APPROVED

Ankita
1/4/2021 2:26:48 PM

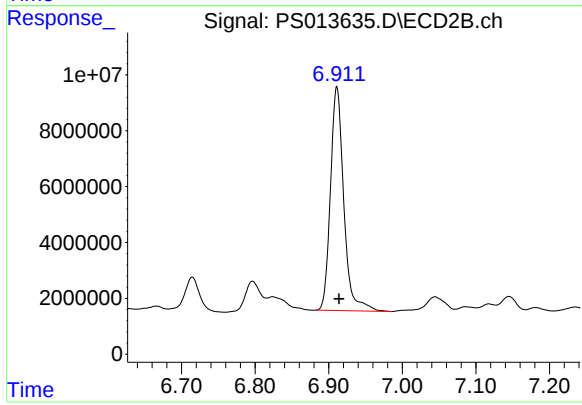

#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: -0.003 min
Response: 100707944
Conc: 256.02 ng/ml