

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123124\
 Data File : PS028860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2024 08:11
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:24:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	0.000	81668	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.663f	2.707f	5628080	5571113	1.998	2.830 #
2) T	3,5-DICHL...	6.370	0.000	1856462	0	<MDL	N.D. #
3) T	4-Nitroph...	6.992	0.000	3184476	0	2.120	N.D. #
5) T	DICAMBA	7.416	0.000	209911	0	<MDL	N.D. #
6) T	MCP	7.586	0.000	177921	0	<MDL	N.D. #
7) T	MCPA	0.000	8.217	0	5023711	N.D.	1.084
8) T	DICHLORPROP	8.078	8.651f	1905186	8513021	<MDL	6.170 #
10) T	Pentachlo...	8.669f	0.000	909684	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.180f	0.000	2423027	0	<MDL	N.D. #
12) T	2,4,5-T	9.512	0.000	972727	0	<MDL	N.D. #
13) T	2,4-DB	10.077	0.000	907549	0	<MDL	N.D. #
14) T	DINOSEB	11.265	0.000	470448	0	<MDL	N.D. #
15) T	Picloram	11.100	12.286	22995475	17733571	<MDL	1.381 #
16) T	DCPA	11.556	12.286f	776387	17733571	<MDL	1.650 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123124\
Data File : PS028860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2024 08:11
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:24:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

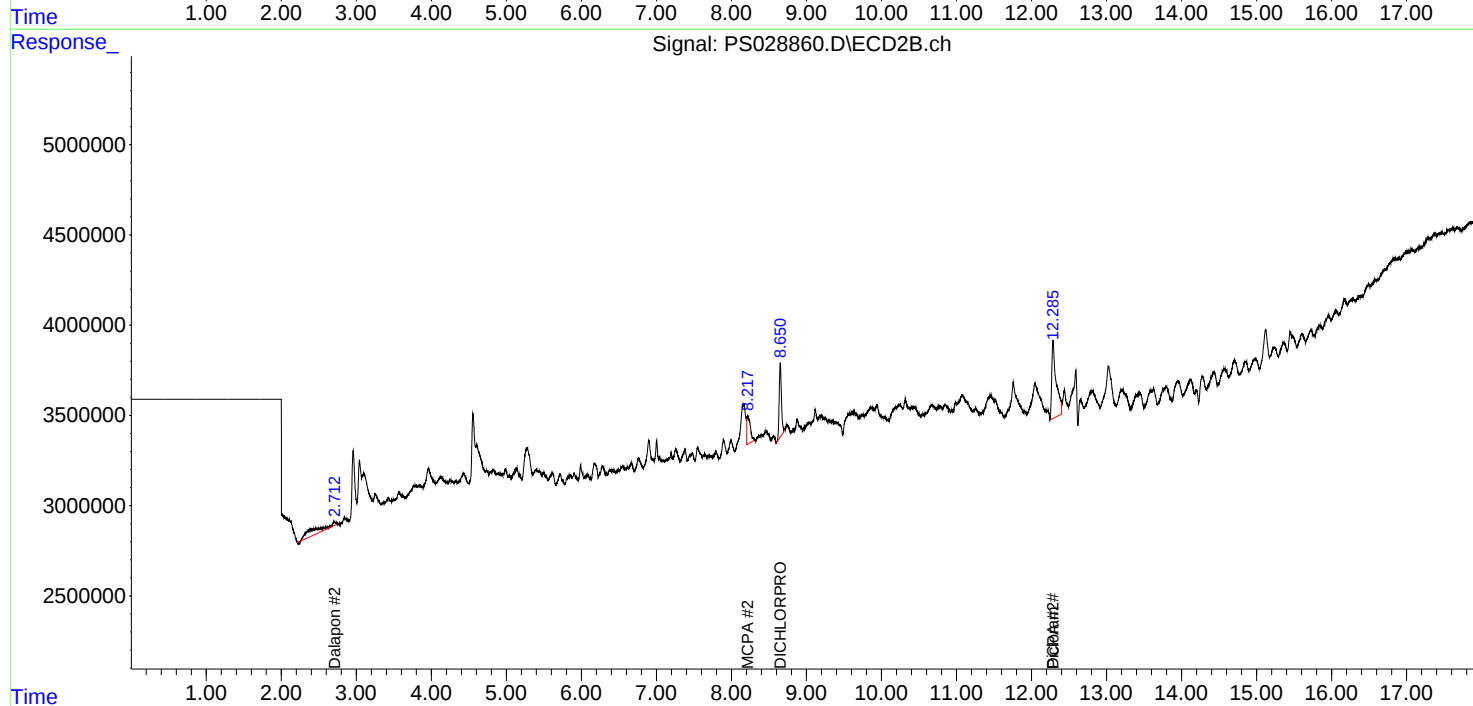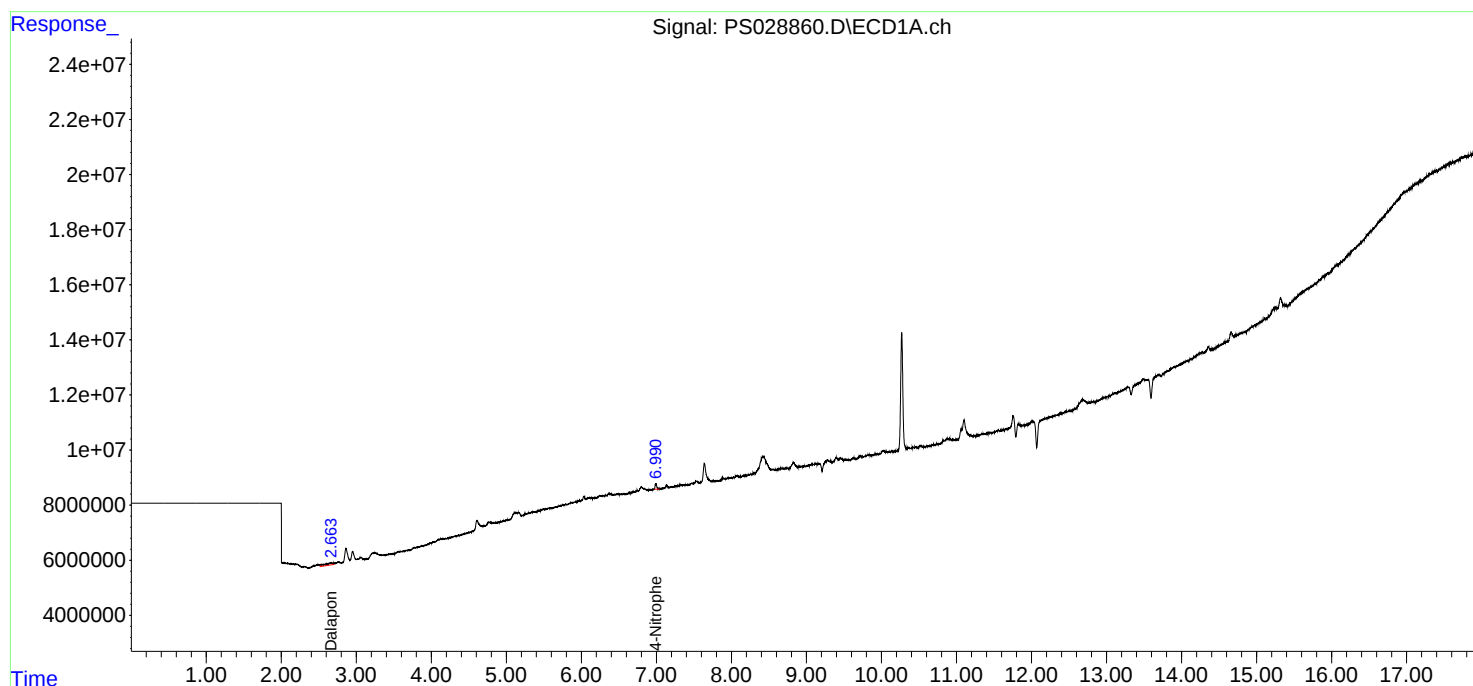


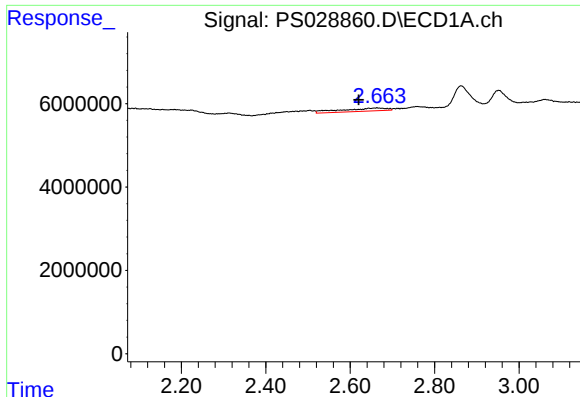

#1 Dalapon


R.T.: 2.663 min
Delta R.T.: 0.043 min
Response: 5628080
Conc: 2.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

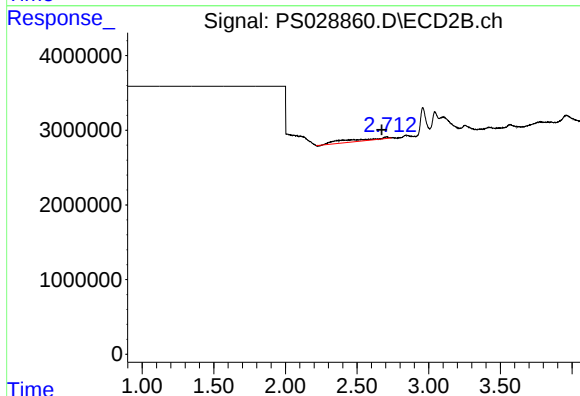


#1 Dalapon

R.T.: 2.707 min
Delta R.T.: 0.034 min
Response: 5571113
Conc: 2.83 ng/ml

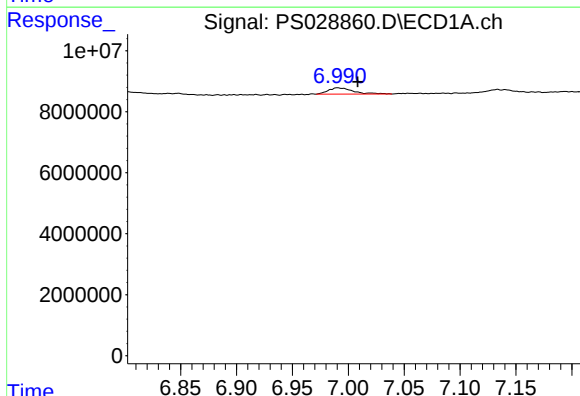


#3 4-Nitrophenol

R.T.: 6.992 min
Delta R.T.: -0.017 min
Response: 3184476
Conc: 2.12 ng/ml

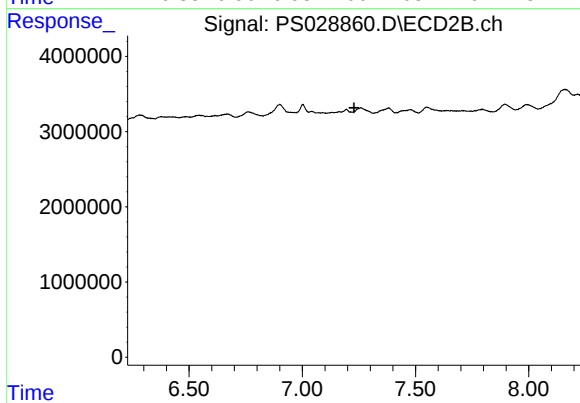

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

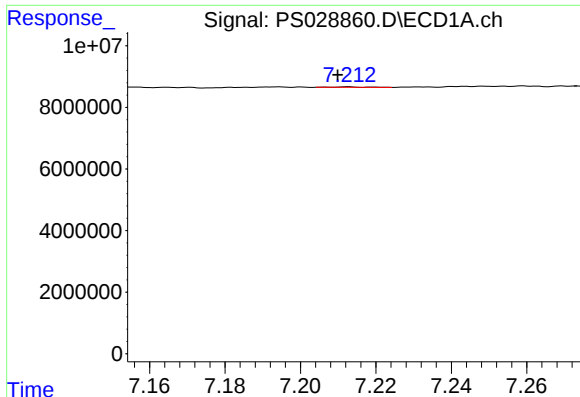

#4 2,4-DCAA


R.T.: 7.212 min
Delta R.T.: 0.002 min
Response: 81668
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

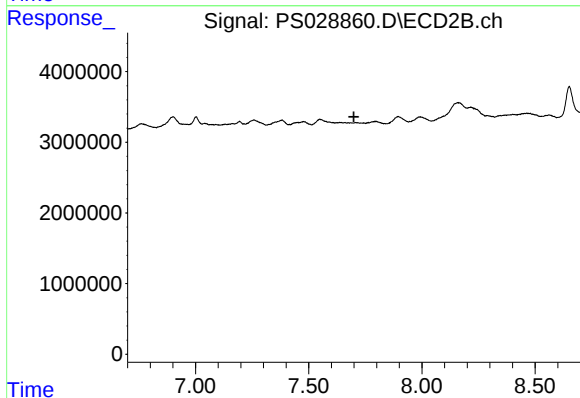


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.699 min
Response: 0
Conc: N.D.

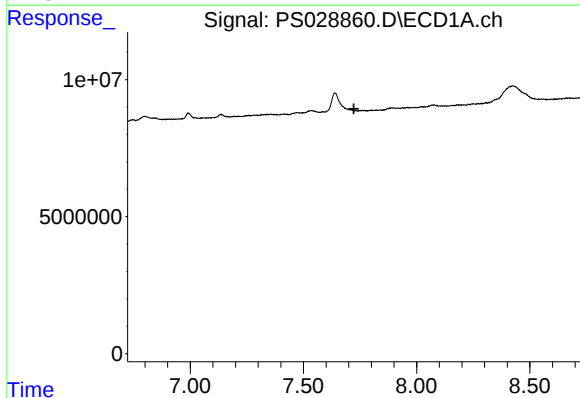


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.723 min
Response: 0
Conc: N.D.

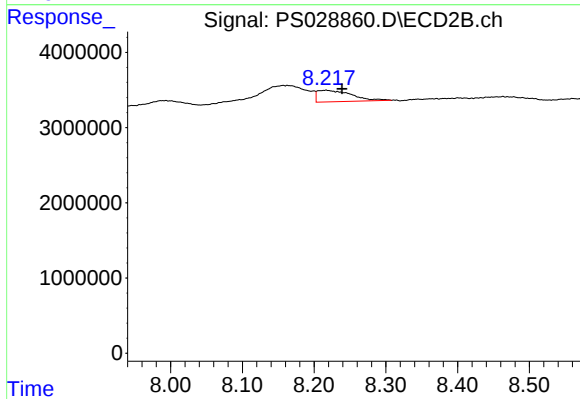

#7 MCPA


R.T.: 8.217 min
Delta R.T.: -0.023 min
Response: 5023711
Conc: 1.08 ug/ml

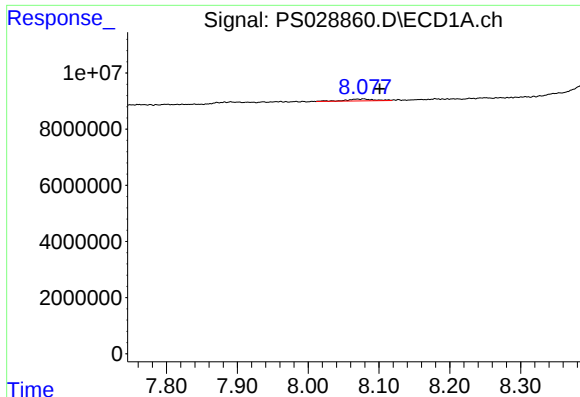

#8 DICHLORPROP


R.T.: 8.078 min
Delta R.T.: -0.023 min
Response: 1905186
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

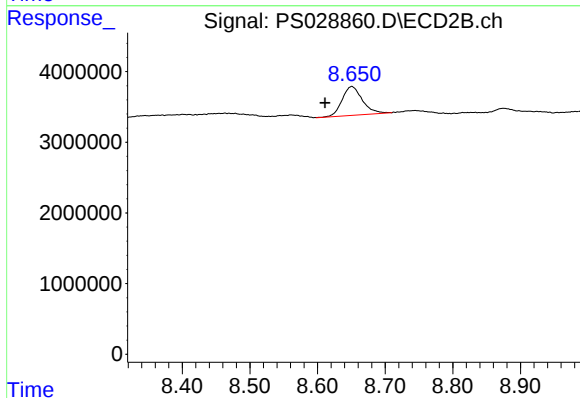


#8 DICHLORPROP

R.T.: 8.651 min
Delta R.T.: 0.040 min
Response: 8513021
Conc: 6.17 ng/ml

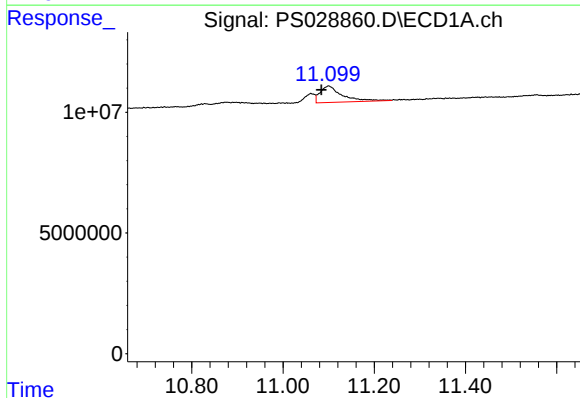


#15 Picloram

R.T.: 11.100 min
Delta R.T.: 0.016 min
Response: 22995475
Conc: N.D.

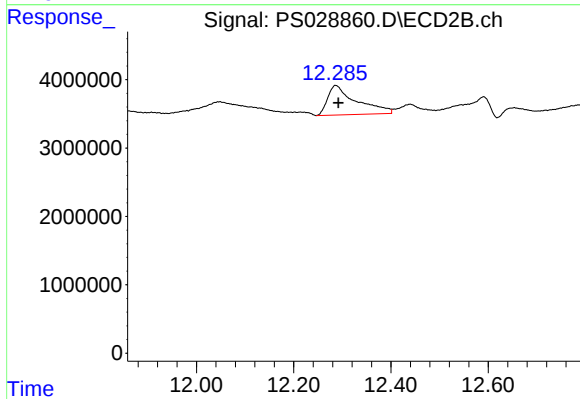

#15 Picloram


R.T.: 12.286 min
Delta R.T.: -0.006 min
Response: 17733571
Conc: 1.38 ng/ml

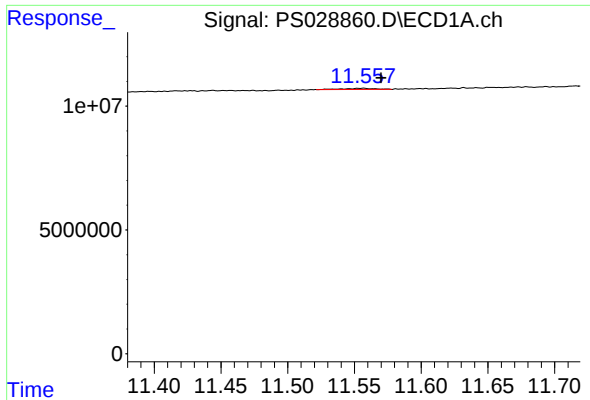

#16 DCPA

R.T.: 11.556 min
Delta R.T.: -0.014 min
Response: 776387
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

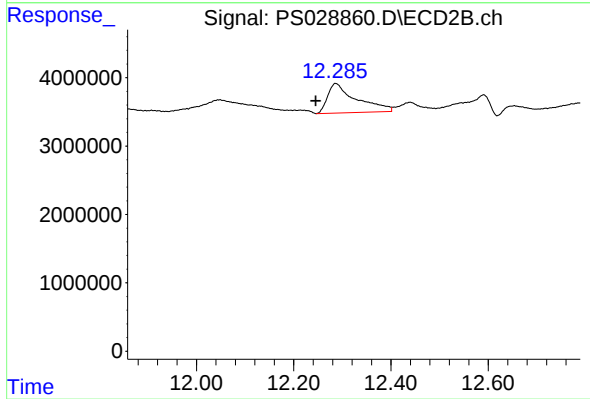

#16 DCPA

R.T.: 12.286 min
Delta R.T.: 0.041 min
Response: 17733571
Conc: 1.65 ng/ml