

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081325\
 Data File : PS031433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2025 17:36
 Operator : AR\AJ
 Sample : Q2808-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:08:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.750	13429256	8282732	4.231	9.798 #
Target Compounds							
1) T	Dalapon	0.000	2.674	0	755.1E6	N.D.	283.767
2) T	3,5-DICHL...	6.445	0.000	28424067	0	6.024	N.D. #
5) T	DICAMBA	7.486	7.967	81935	37473857	<MDL	6.594 #
6) T	MCP	7.682	8.049	8164182	106.7E6	1.015	60.384 #
7) T	MCPA	7.817	8.265f	31391051	68205871	3.151	24.311 #
8) T	DICHLORPROP	8.157f	8.642	3082274	21780705	<MDL	16.315 #
10) T	Pentachlo...	8.719	9.565f	13587114	112.8E6	<MDL	3.238 #
11) T	2,4,5-TP ...	9.298	9.887	38807404	27669496	2.165	2.110
12) T	2,4,5-T	9.604	10.336	33499878	93922218	2.286	7.933 #
13) T	2,4-DB	10.161	10.914	51716426	80432848	26.912	83.363 #
14) T	DINOSEB	11.382	11.291	13297271	431.6E6	1.049	45.635 #
15) T	Picloram	11.173	12.407	3175272	121.1E6	<MDL	6.907 #
16) T	DCPA	11.666	12.319	13629170	300.8E6	<MDL	15.266 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081325\
Data File : PS031433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2025 17:36
Operator : AR\AJ
Sample : Q2808-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:08:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

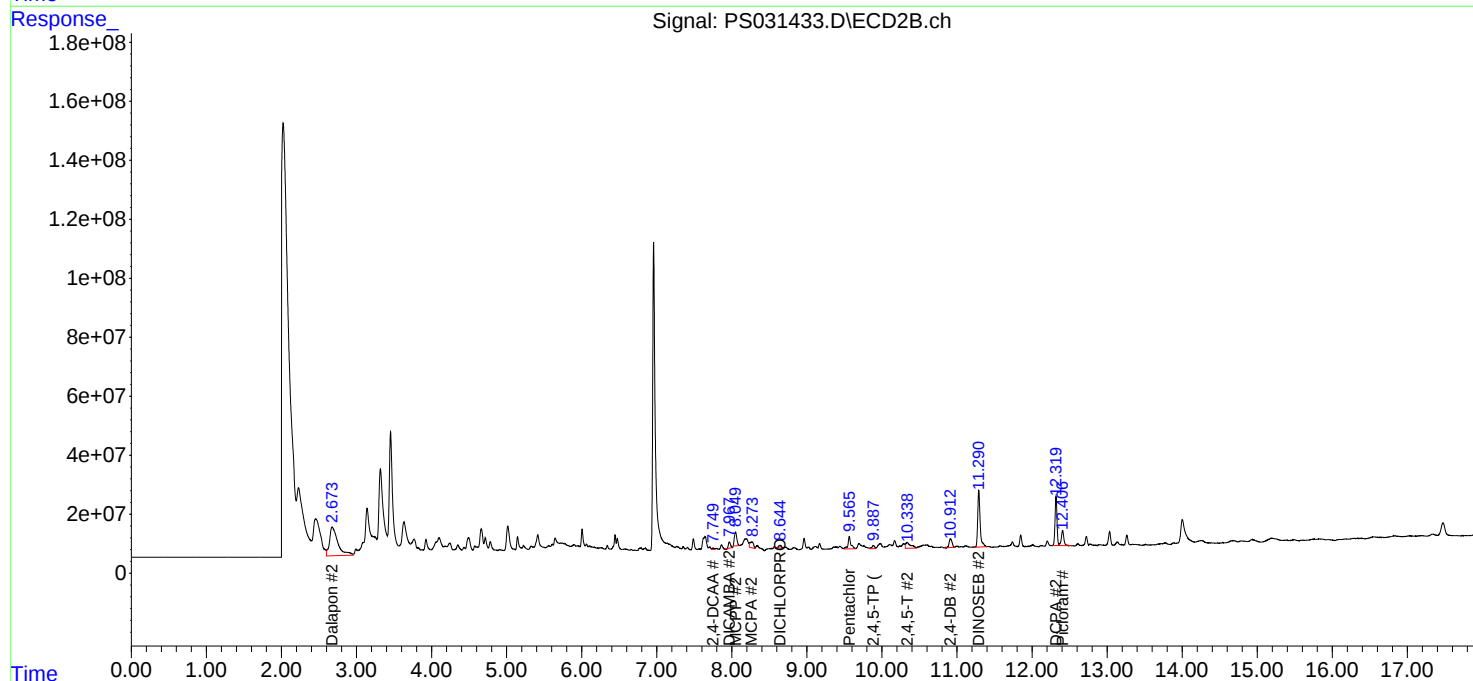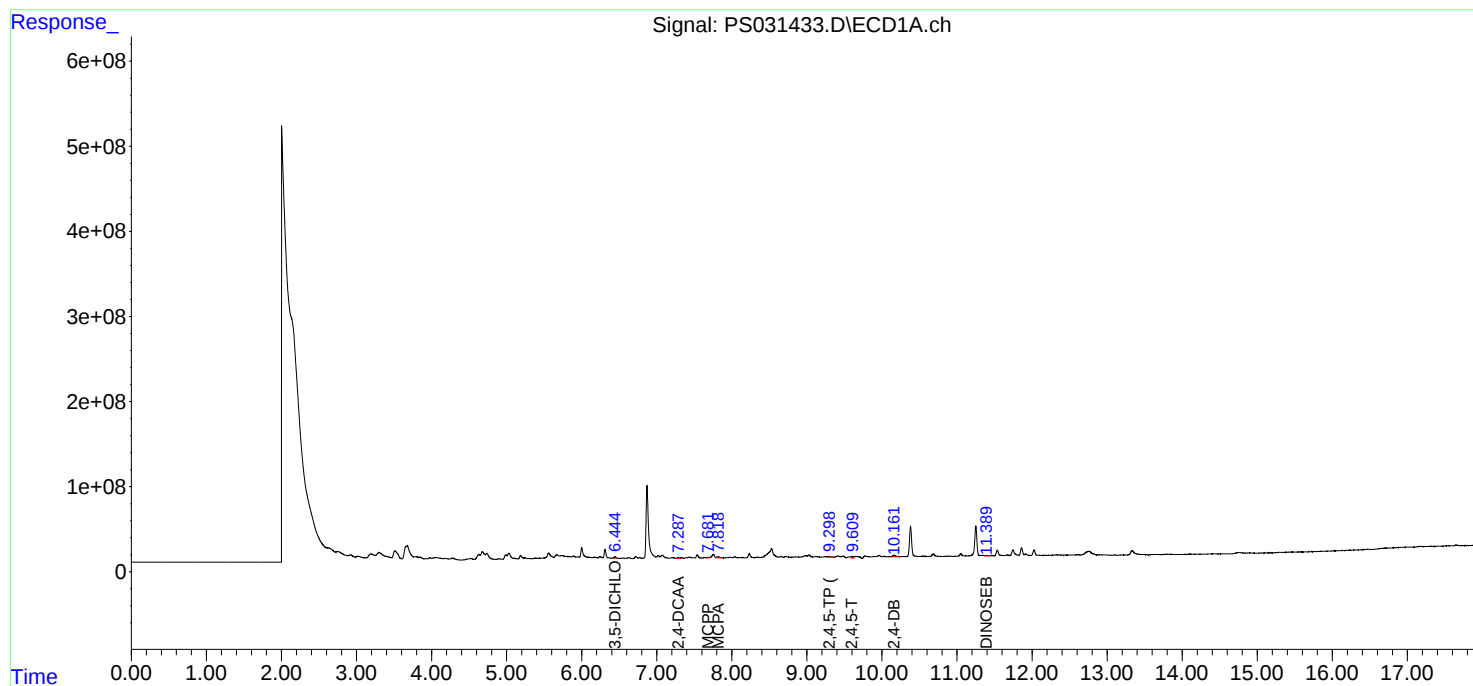


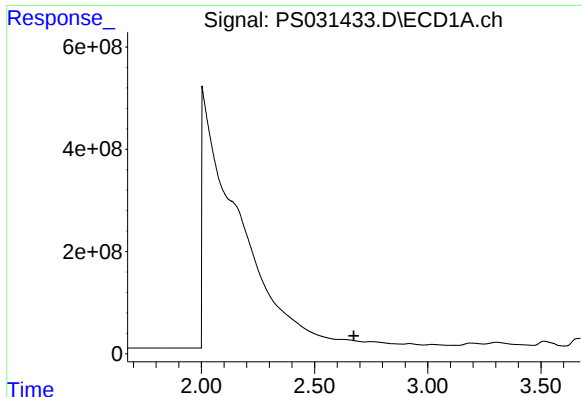

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

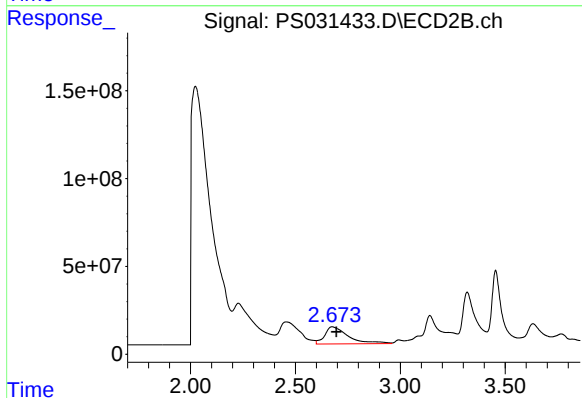


#1 Dalapon

R.T.: 2.674 min
Delta R.T.: -0.020 min
Response: 755108400
Conc: 283.77 ng/ml

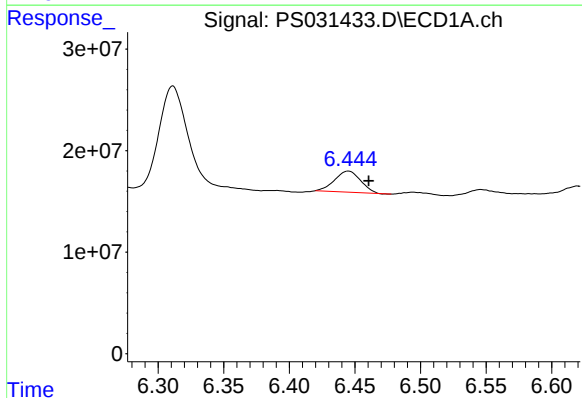


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.445 min
Delta R.T.: -0.016 min
Response: 28424067
Conc: 6.02 ng/ml

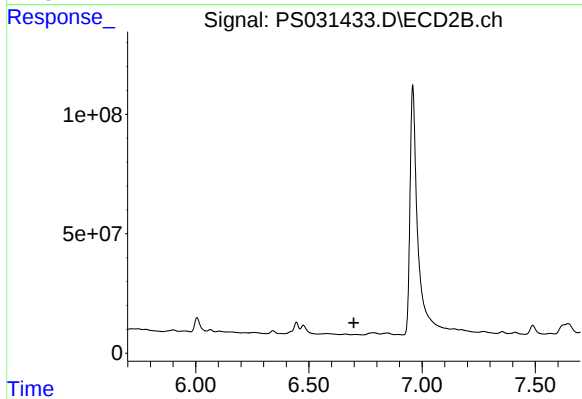

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

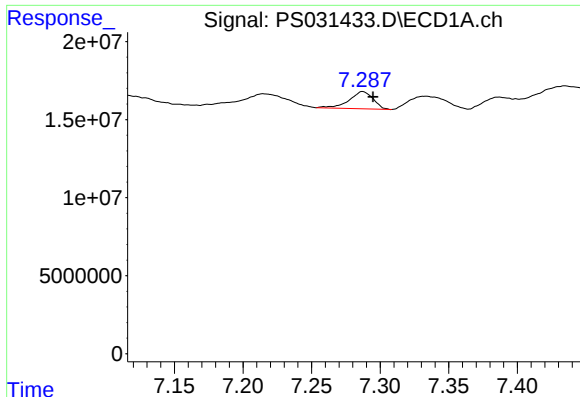

#4 2,4-DCAA


R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 13429256
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

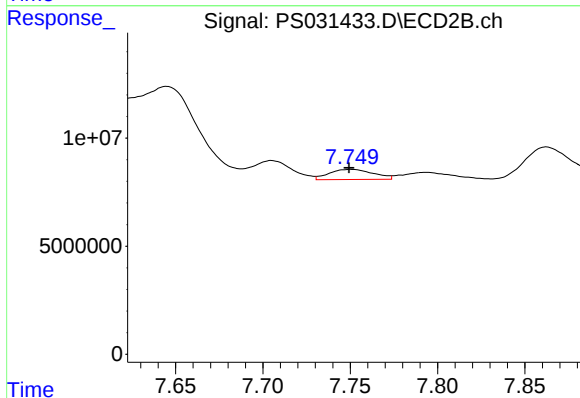


#4 2,4-DCAA

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 8282732
Conc: 9.80 ng/ml

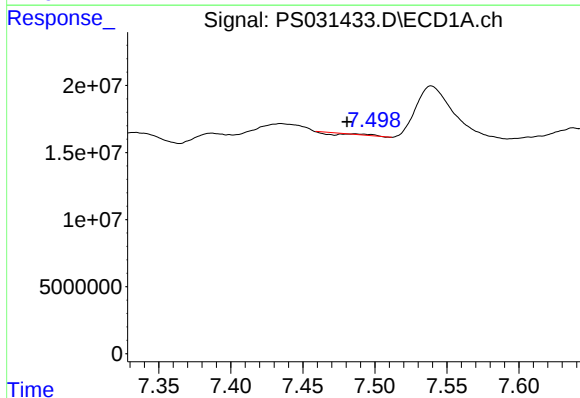


#5 DICAMBA

R.T.: 7.486 min
Delta R.T.: 0.005 min
Response: 81935
Conc: N.D.

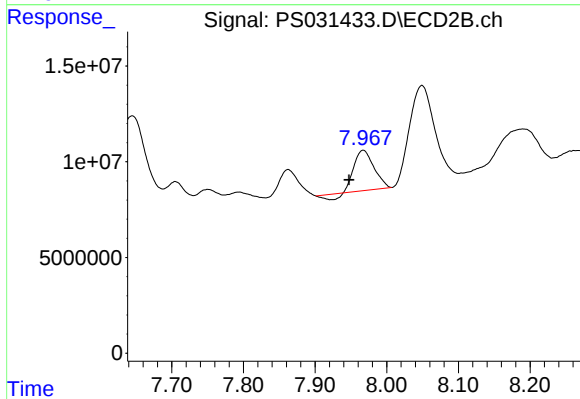

#5 DICAMBA


R.T.: 7.967 min
Delta R.T.: 0.020 min
Response: 37473857
Conc: 6.59 ng/ml

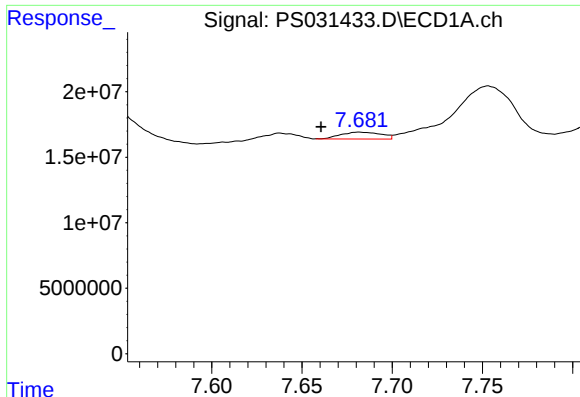

#6 MCP


R.T.: 7.682 min
Delta R.T.: 0.021 min
Response: 8164182
Conc: 1.01 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

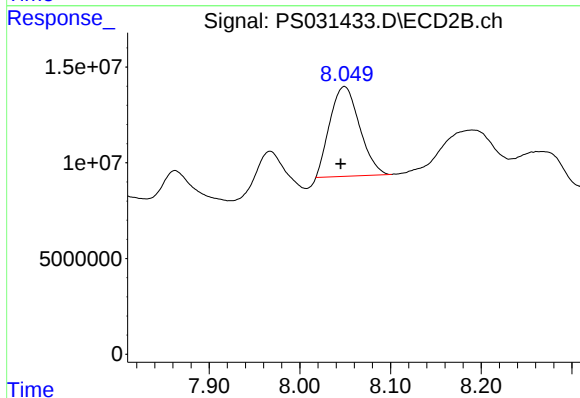


#6 MCP

R.T.: 8.049 min
Delta R.T.: 0.004 min
Response: 106749532
Conc: 60.38 ug/ml

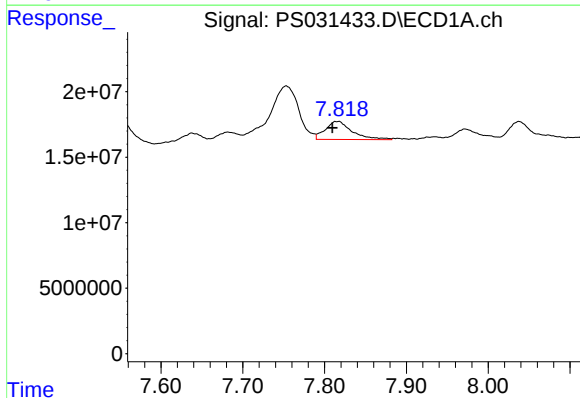


#7 MCPA

R.T.: 7.817 min
Delta R.T.: 0.008 min
Response: 31391051
Conc: 3.15 ug/ml

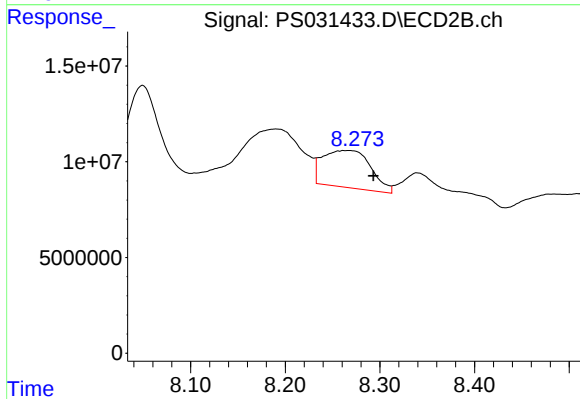

#7 MCPA


R.T.: 8.265 min
Delta R.T.: -0.028 min
Response: 68205871
Conc: 24.31 ug/ml

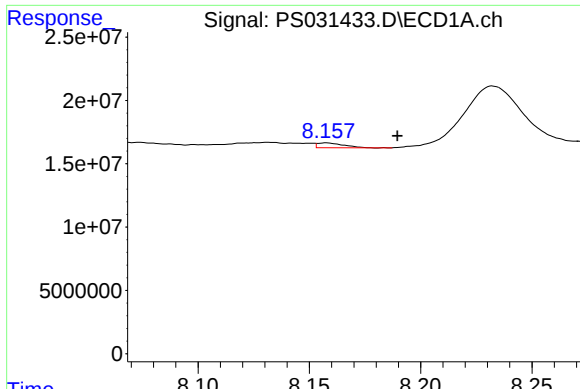

#8 DICHLORPROP


R.T.: 8.157 min
Delta R.T.: -0.032 min
Response: 3082274
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

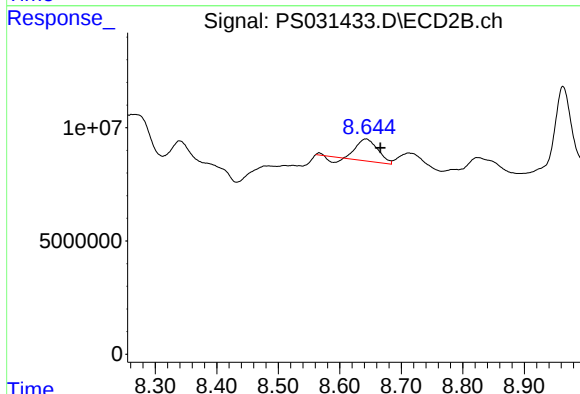


#8 DICHLORPROP

R.T.: 8.642 min
Delta R.T.: -0.024 min
Response: 21780705
Conc: 16.31 ng/ml

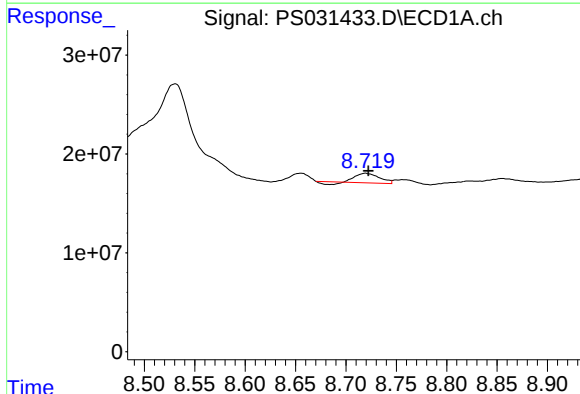


#10 Pentachlorophenol

R.T.: 8.719 min
Delta R.T.: -0.003 min
Response: 13587114
Conc: N.D.

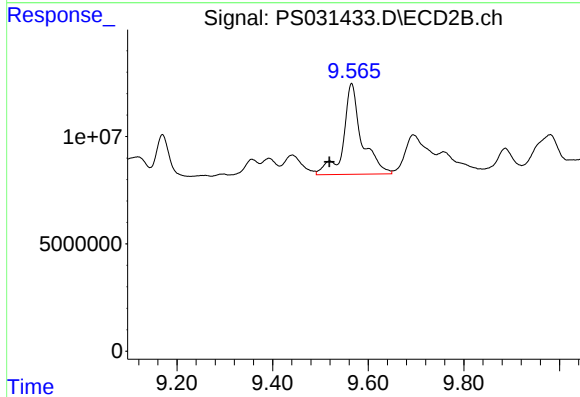

#10 Pentachlorophenol


R.T.: 9.565 min
Delta R.T.: 0.047 min
Response: 112772014
Conc: 3.24 ng/ml

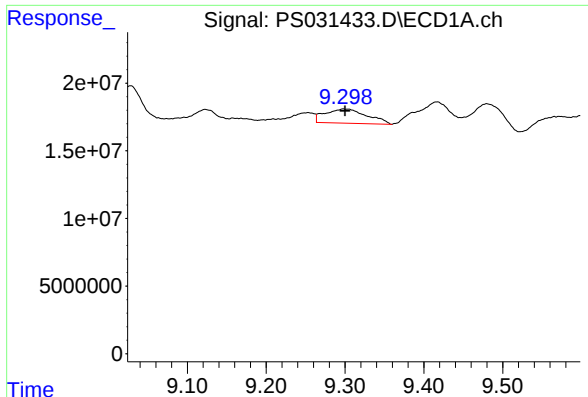

#11 2,4,5-TP (SILVEX)


R.T.: 9.298 min
Delta R.T.: -0.002 min
Response: 38807404
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

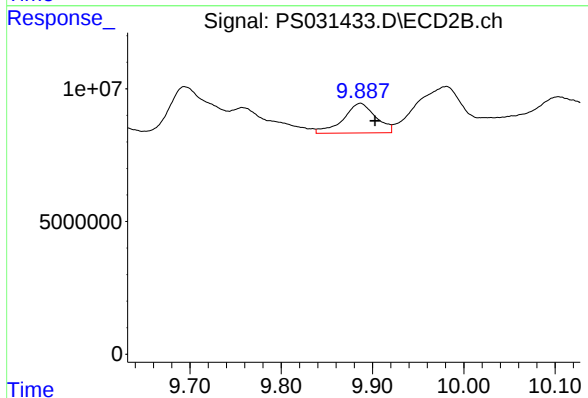


#11 2,4,5-TP (SILVEX)

R.T.: 9.887 min
Delta R.T.: -0.016 min
Response: 27669496
Conc: 2.11 ng/ml

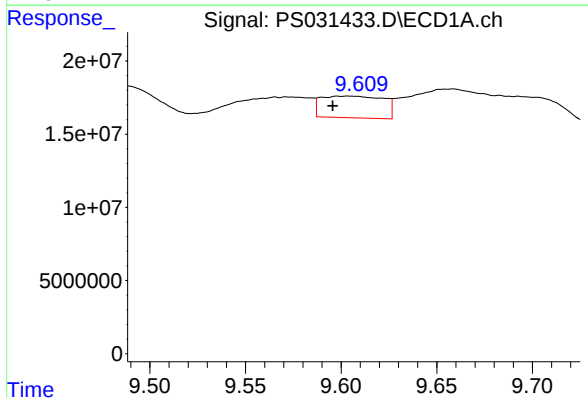


#12 2,4,5-T

R.T.: 9.604 min
Delta R.T.: 0.008 min
Response: 33499878
Conc: 2.29 ng/ml

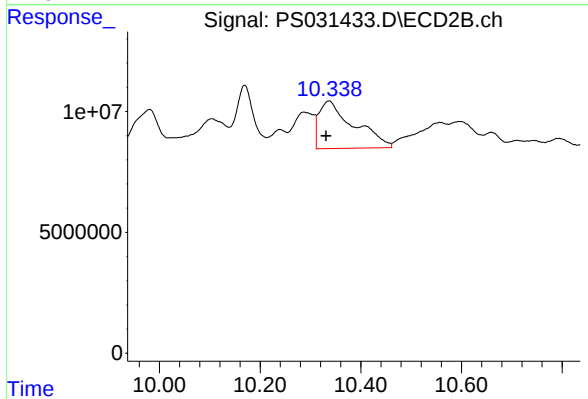

#12 2,4,5-T


R.T.: 10.336 min
Delta R.T.: 0.005 min
Response: 93922218
Conc: 7.93 ng/ml

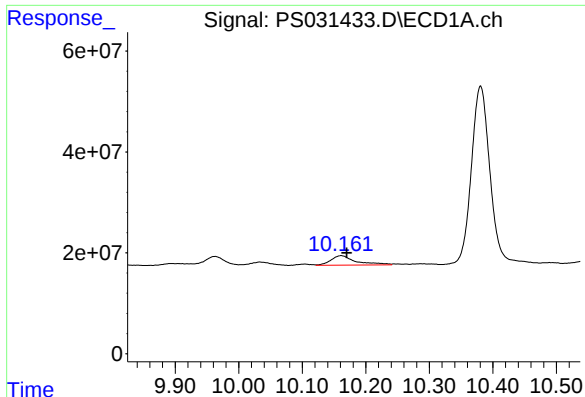

#13 2,4-DB


R.T.: 10.161 min
Delta R.T.: -0.009 min
Response: 51716426
Conc: 26.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

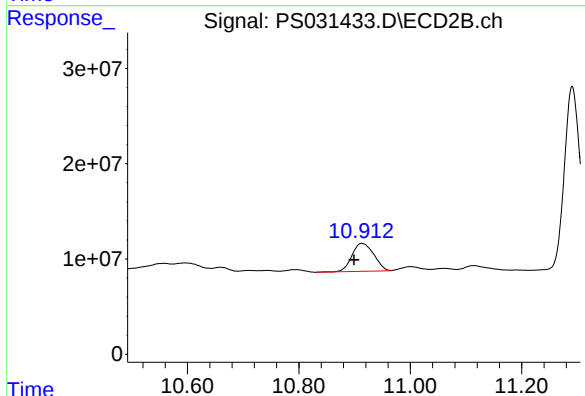


#13 2,4-DB

R.T.: 10.914 min
Delta R.T.: 0.015 min
Response: 80432848
Conc: 83.36 ng/ml

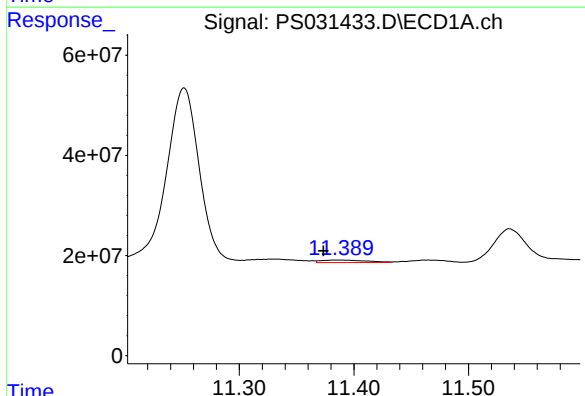


#14 DINOSEB

R.T.: 11.382 min
Delta R.T.: 0.009 min
Response: 13297271
Conc: 1.05 ng/ml

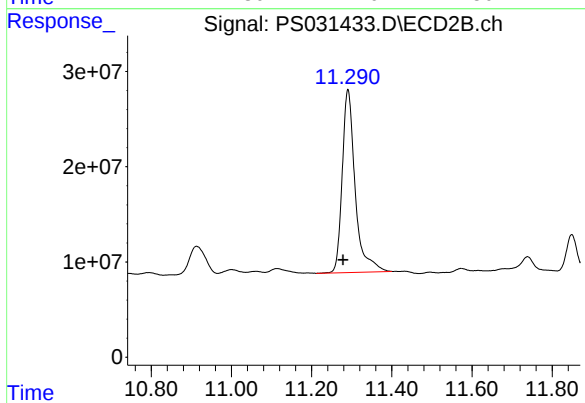

#14 DINOSEB


R.T.: 11.291 min
Delta R.T.: 0.012 min
Response: 431566809
Conc: 45.63 ng/ml

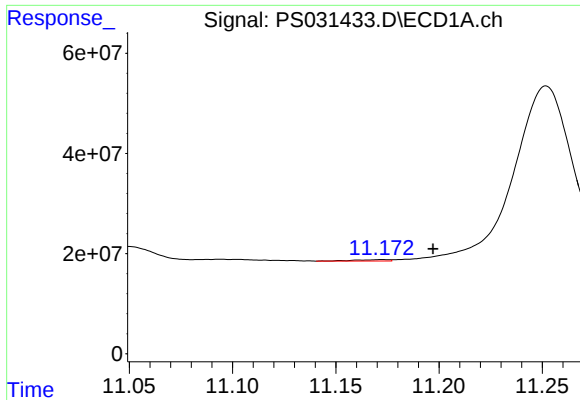

#15 Picloram


R.T.: 11.173 min
Delta R.T.: -0.024 min
Response: 3175272
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

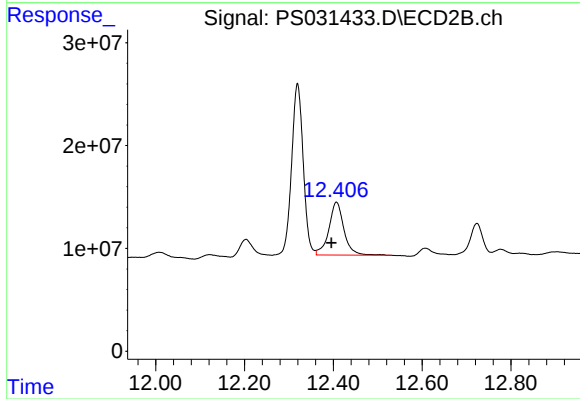


#15 Picloram

R.T.: 12.407 min
Delta R.T.: 0.012 min
Response: 121074004
Conc: 6.91 ng/ml

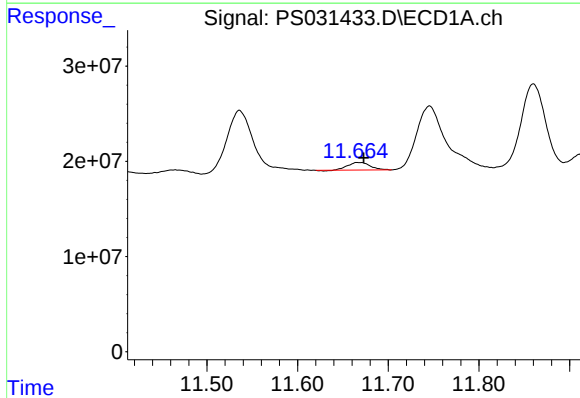

#16 DCPA

R.T.: 11.666 min
Delta R.T.: -0.007 min
Response: 13629170
Conc: N.D.

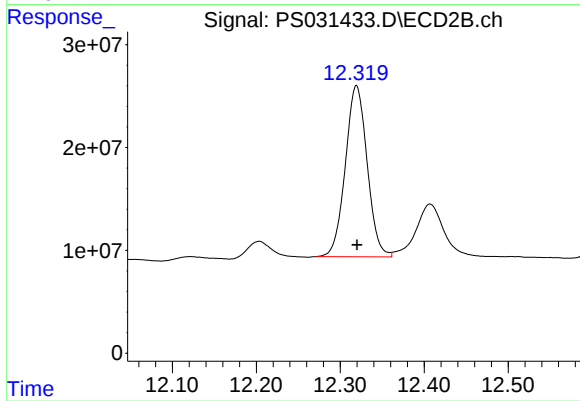

#16 DCPA

R.T.: 12.319 min
Delta R.T.: 0.000 min
Response: 300755022
Conc: 15.27 ng/ml