

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 10:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:04:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.272	7.611	1666.9E6	1595.4E6	367.869	437.626
Target Compounds							
1) T	Dalapon	2.652	0.000	5987831	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.445	0.000	744338	0	<MDL	N.D. #
3) T	4-Nitroph...	7.131f	0.000	123773	0	<MDL	N.D. #
7) T	MCPA	0.000	8.102f	0	1755903	N.D.	<MDL
8) T	DICHLORPROP	8.163	0.000	757817	0	<MDL	N.D. #
9) T	2,4-D	0.000	8.821f	0	10066650	N.D.	1.919
10) T	Pentachlo...	8.711	9.324f	1188337	4805965	<MDL	<MDL #
11) T	2,4,5-TP ...	9.261	0.000	4879778	0	<MDL	N.D. #
12) T	2,4,5-T	9.583	10.194	1754575	43332294	<MDL	1.827 #
13) T	2,4-DB	10.165	0.000	947437	0	<MDL	N.D. #
15) T	Picloram	0.000	12.249f	0	89959546	N.D.	2.419
16) T	DCPA	11.679f	0.000	5165501	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 10:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:04:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

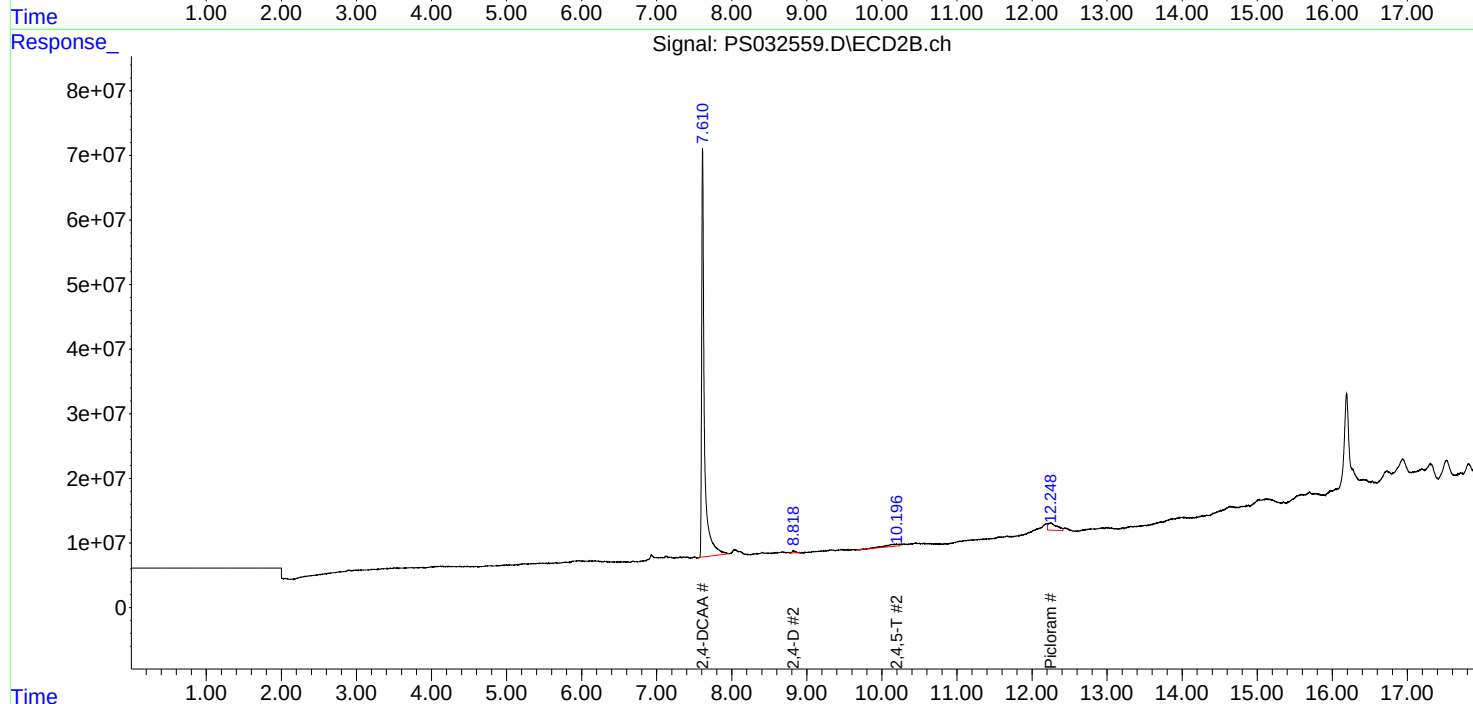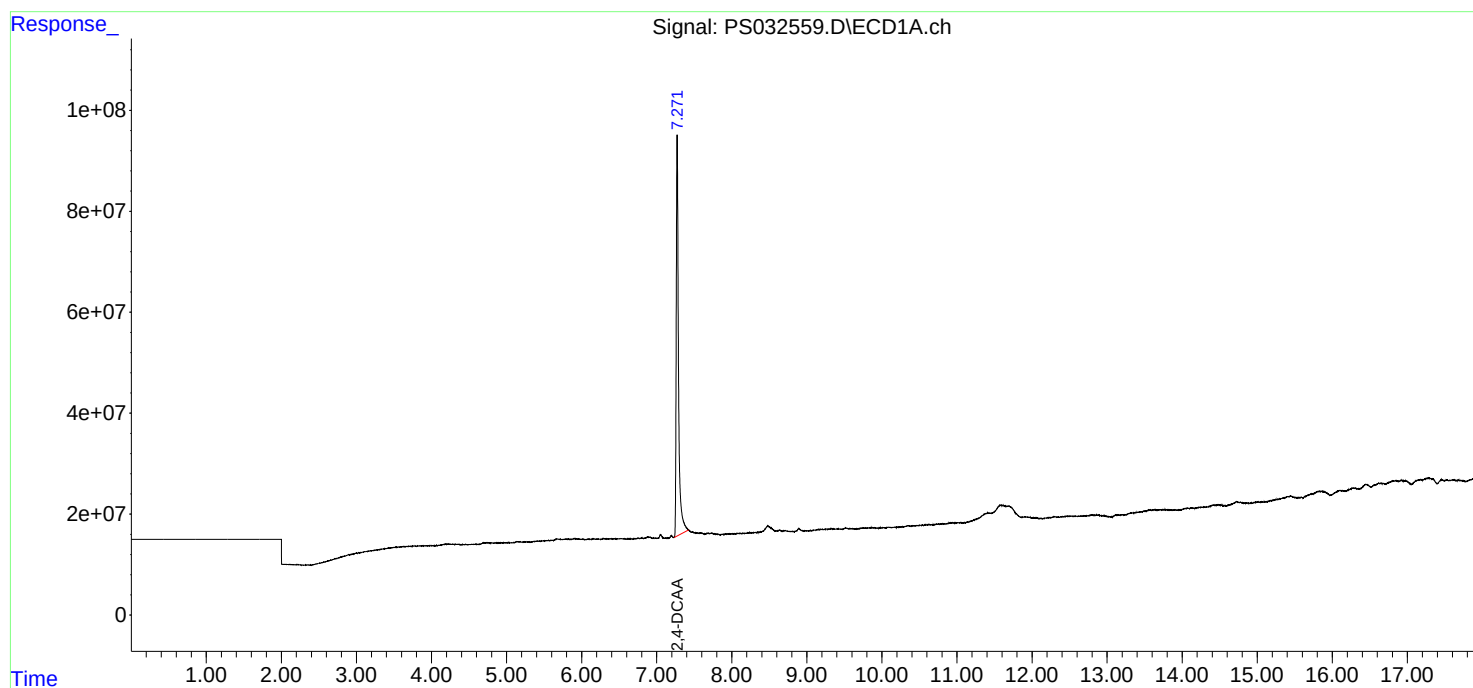


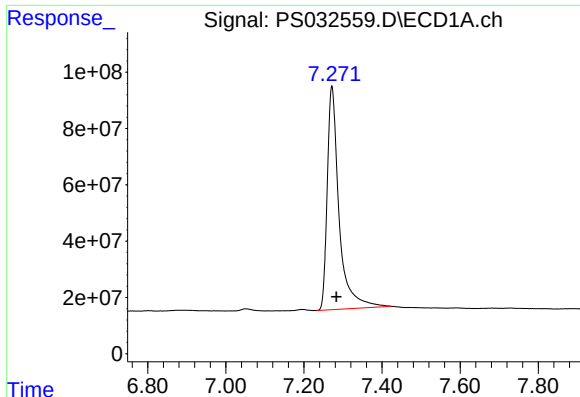

#4 2,4-DCAA


R.T.: 7.272 min
Delta R.T.: -0.012 min
Response: 1666914256
Conc: 367.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

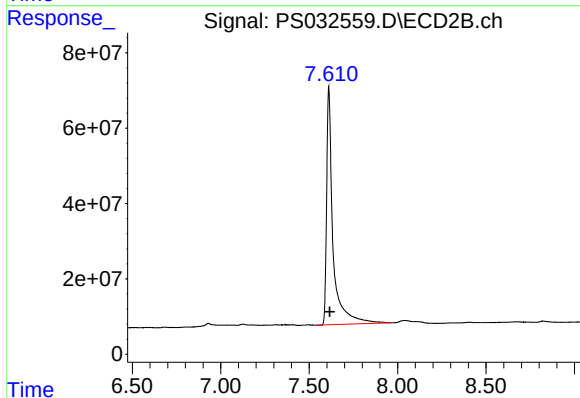


#4 2,4-DCAA

R.T.: 7.611 min
Delta R.T.: -0.006 min
Response: 1595363109
Conc: 437.63 ng/ml

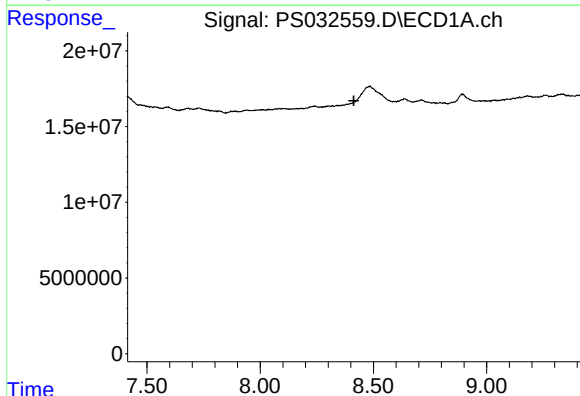


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.414 min
Response: 0
Conc: N.D.

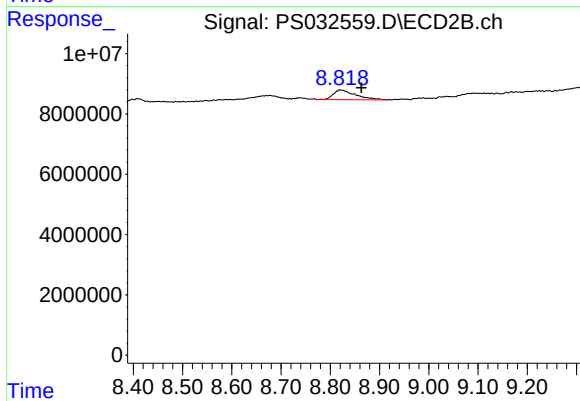

#9 2,4-D


R.T.: 8.821 min
Delta R.T.: -0.043 min
Response: 10066650
Conc: 1.92 ng/ml

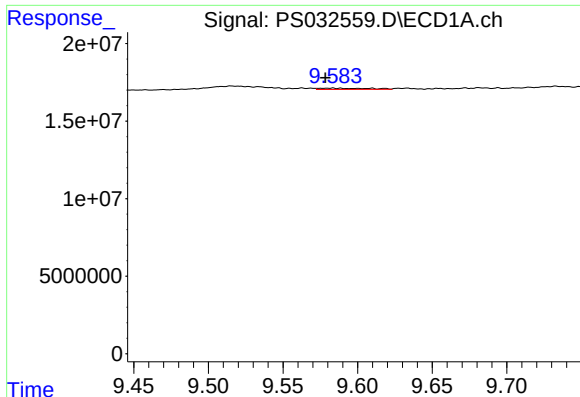

#12 2,4,5-T


R.T.: 9.583 min
Delta R.T.: 0.005 min
Response: 1754575
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

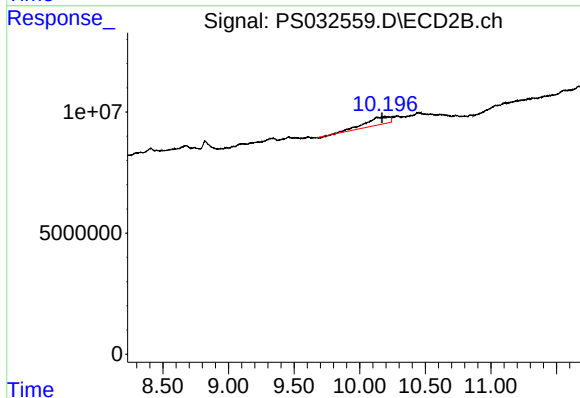


#12 2,4,5-T

R.T.: 10.194 min
Delta R.T.: 0.022 min
Response: 43332294
Conc: 1.83 ng/ml

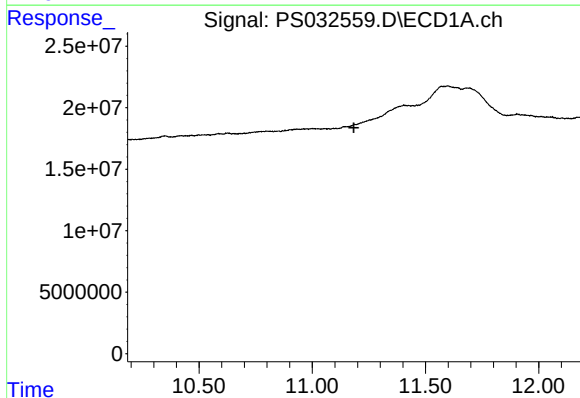

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.184 min
Response: 0
Conc: N.D.

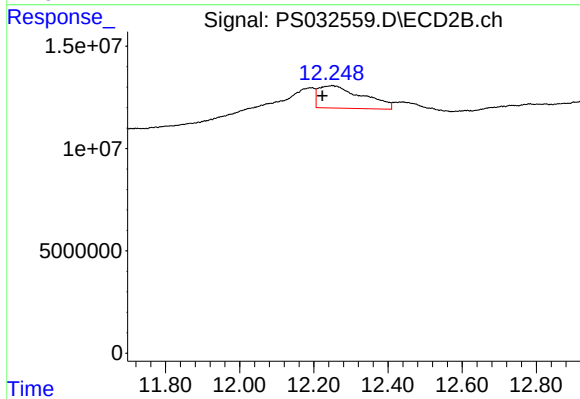

#15 Picloram

R.T.: 12.249 min
Delta R.T.: 0.026 min
Response: 89959546
Conc: 2.42 ng/ml