

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 14:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:05:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.273	7.614	1657.3E6	1685.1E6	365.739	462.230 #
Target Compounds							
2) T	3,5-DICHL...	6.447	0.000	686060	0	<MDL	N.D. #
7) T	MCPA	7.800	0.000	781985	0	<MDL	N.D. #
8) T	DICHLORPROP	8.170	0.000	564532	0	<MDL	N.D. #
9) T	2,4-D	8.380f	8.846	110878	2618056	<MDL	<MDL #
10) T	Pentachlo...	8.695	9.348	4027492	2414088	<MDL	<MDL #
11) T	2,4,5-TP ...	9.269	0.000	3309166	0	<MDL	N.D. #
12) T	2,4,5-T	9.599	10.133f	8683925	9599590	<MDL	<MDL #
13) T	2,4-DB	10.159	0.000	589541	0	<MDL	N.D. #
14) T	DINOSEB	11.330	11.101	3494321	2229013	<MDL	<MDL #
15) T	Picloram	11.146f	0.000	1759694	0	<MDL	N.D. #
16) T	DCPA	11.627	0.000	2375809	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 14:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:05:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

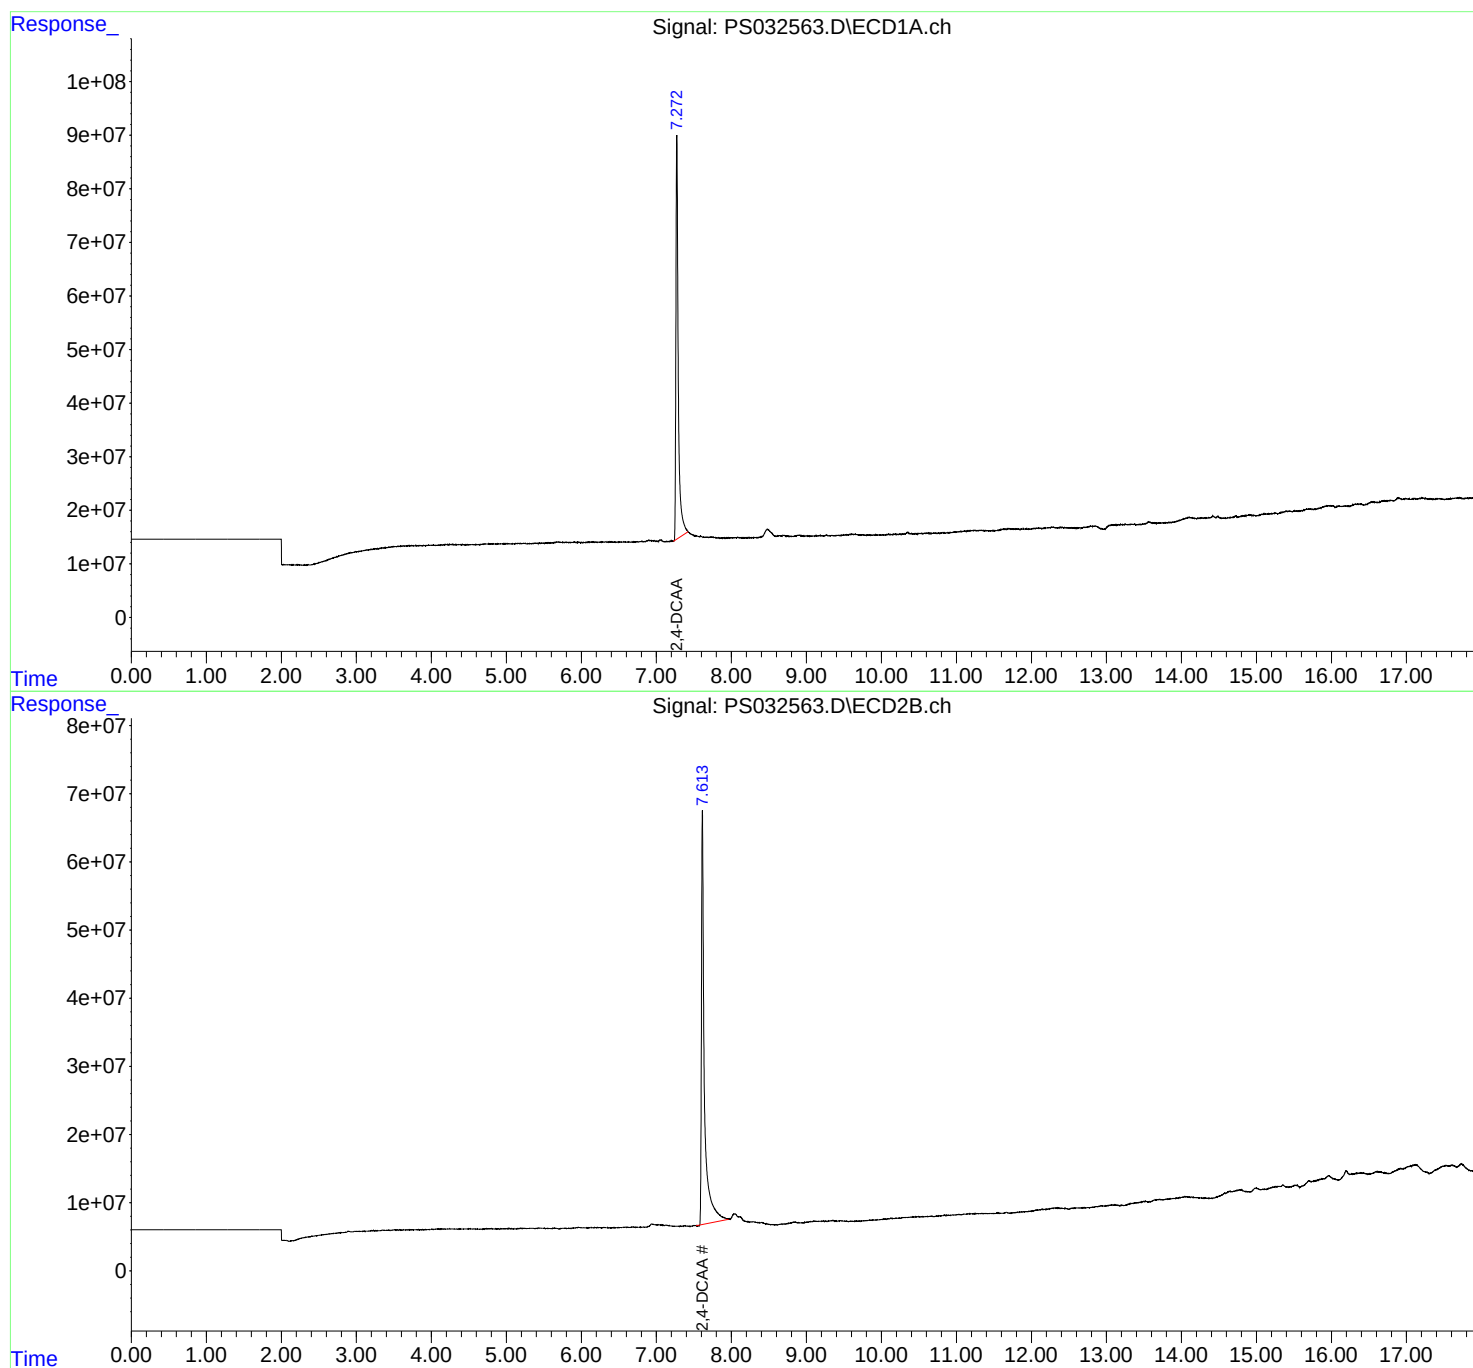


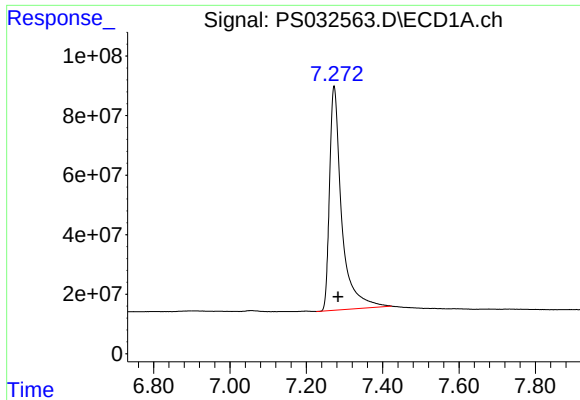

#4 2,4-DCAA

R.T.: 7.273 min
Delta R.T.: -0.011 min
Response: 1657264694
Conc: 365.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

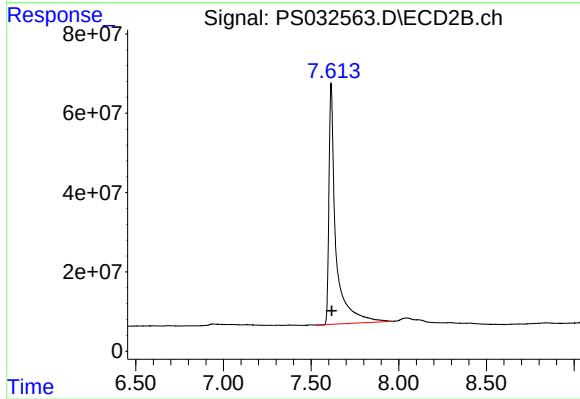

#4 2,4-DCAA

R.T.: 7.614 min
Delta R.T.: -0.003 min
Response: 1685059348
Conc: 462.23 ng/ml