

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 17:33
 Operator : AR\AJ
 Sample : Q3732-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:05:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.273	7.615	560.6E6	523.0E6	123.723	143.470
Target Compounds							
1) T	Dalapon	0.000	2.565f	0	2711.2E6	N.D.	389.878
3) T	4-Nitroph...	0.000	7.175	0	26696912	N.D.	11.761
5) T	DICAMBA	7.452	7.765f	13600029	2700271	<MDL	<MDL #
6) T	MCP	7.658	7.930	-524393	31203719	N.D.	2.346
7) T	MCPA	7.801	8.184f	48383431	-2764914	3.604	N.D. #
8) T	DICHLORPROP	8.142f	8.480f	9230533	29008461	2.075	6.083 #
9) T	2,4-D	0.000	8.882	0	11554256	N.D.	2.203
10) T	Pentachlo...	8.727	9.351	5915001	26791277	<MDL	<MDL #
11) T	2,4,5-TP ...	9.309f	9.720	181.8E6	632.4E6	6.988	23.550 #
12) T	2,4,5-T	9.617f	10.177	399.5E6	229.5E6	16.757	9.675 #
13) T	2,4-DB	10.162	10.756	281.9E6	67994758	106.976	18.029 #
14) T	DINOSEB	0.000	11.113	0	159.5E6	N.D.	9.015
15) T	Picloram	11.180	12.234	261.1E6	385.6E6	12.300	10.371
16) T	DCPA	11.618f	12.136	64983974	-5683414	1.937	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 17:33
Operator : AR\AJ
Sample : Q3732-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:05:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

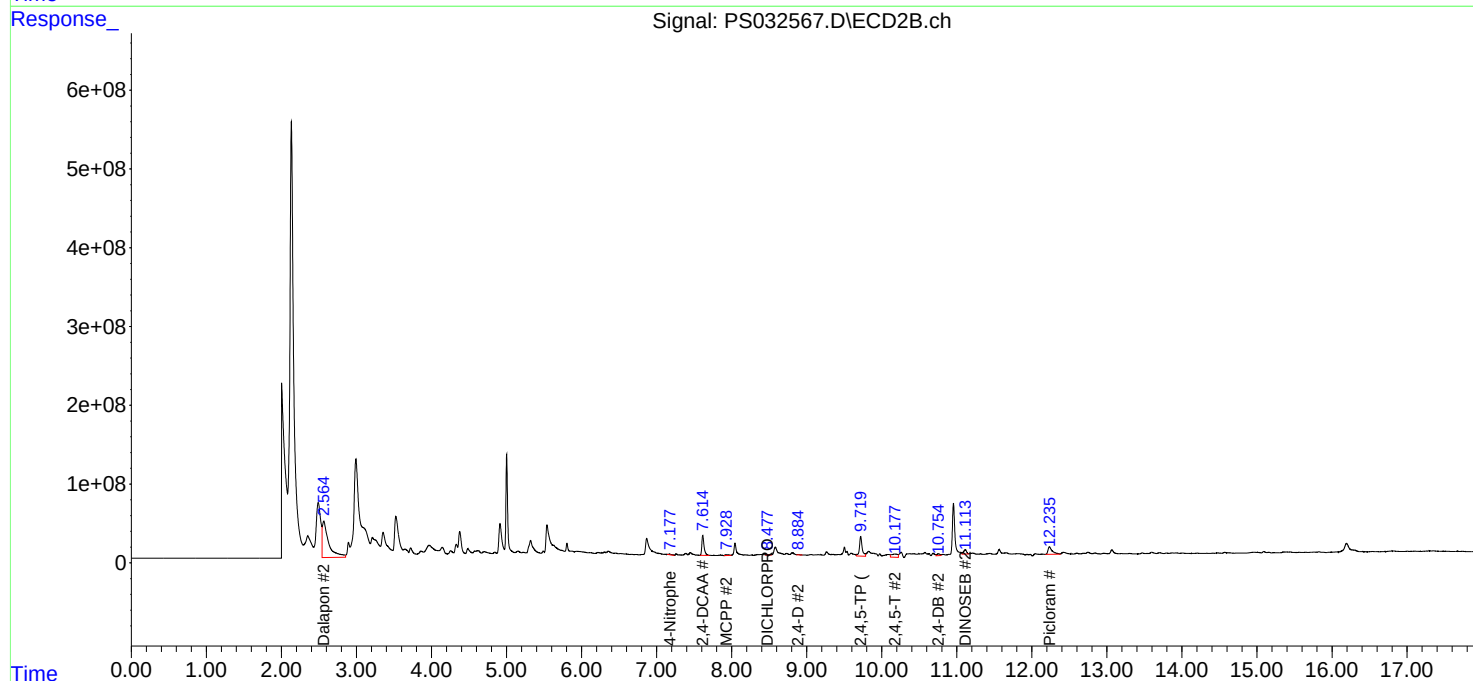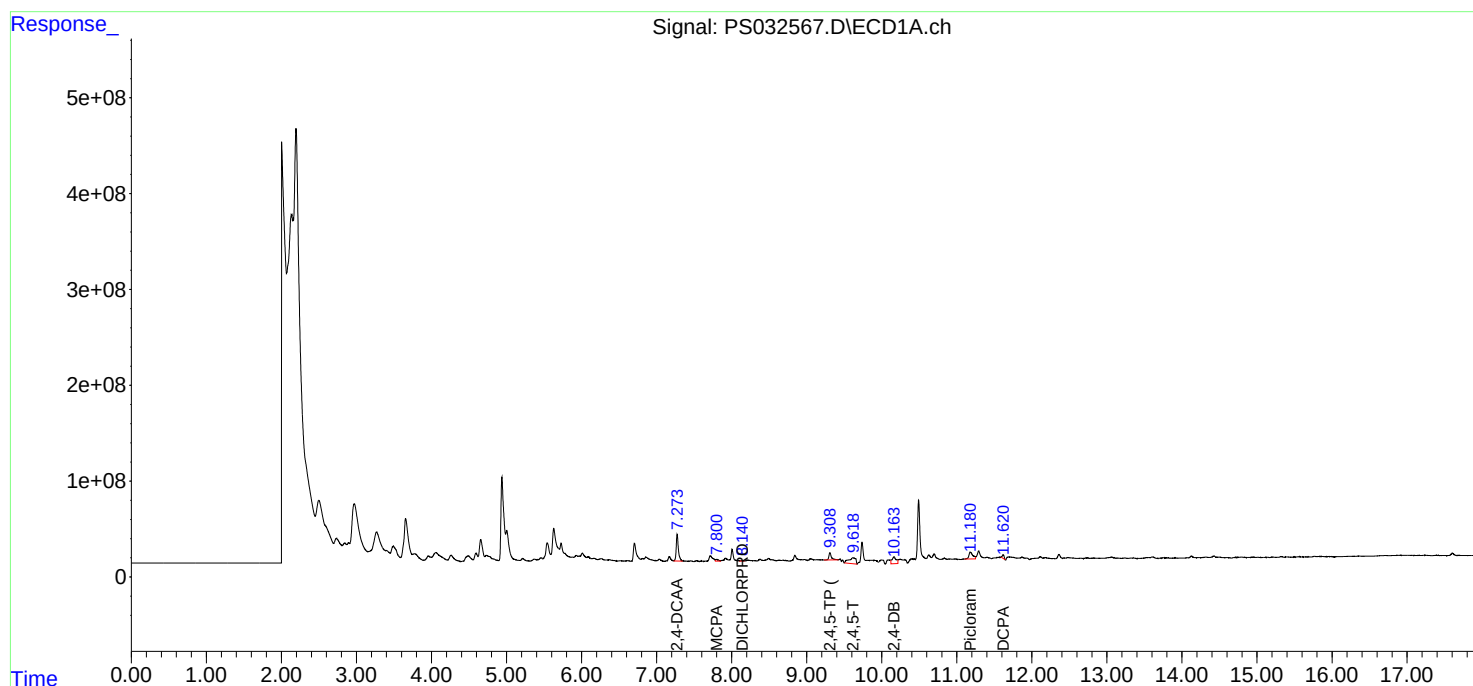


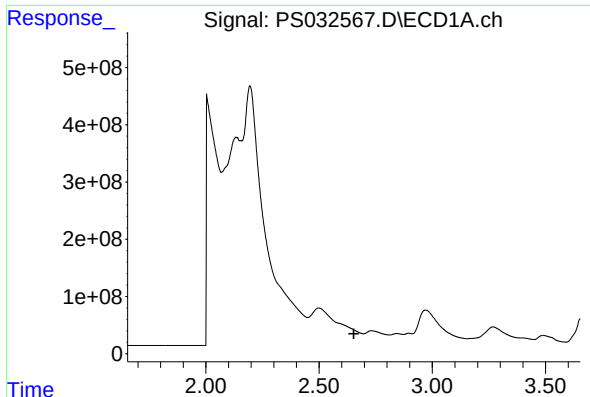

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

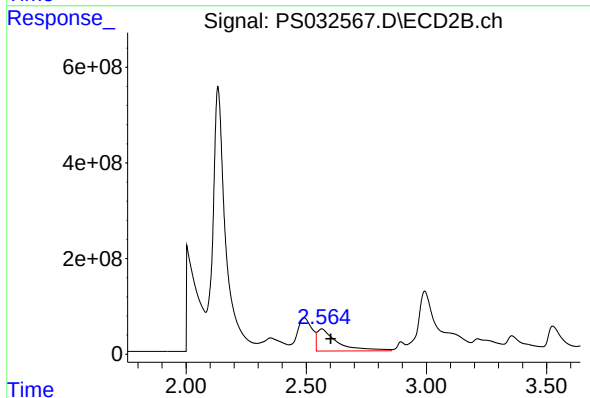


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: -0.038 min
Response: 2711212673
Conc: 389.88 ng/ml

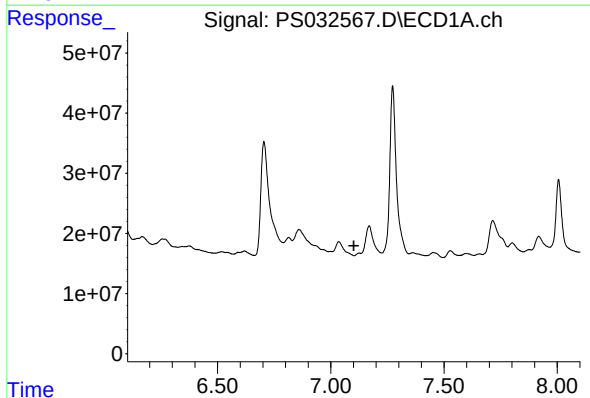


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.102 min
Response: 0
Conc: N.D.

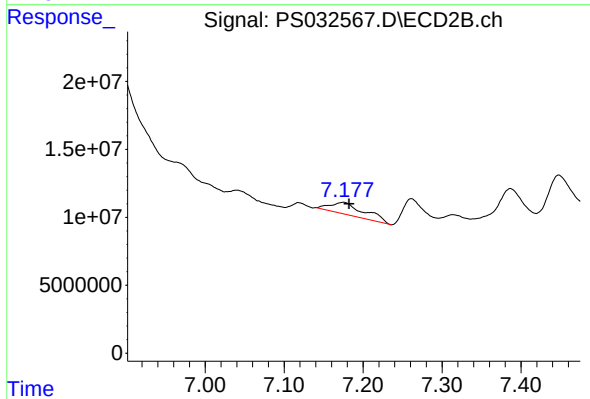

#3 4-Nitrophenol


R.T.: 7.175 min
Delta R.T.: -0.007 min
Response: 26696912
Conc: 11.76 ng/ml

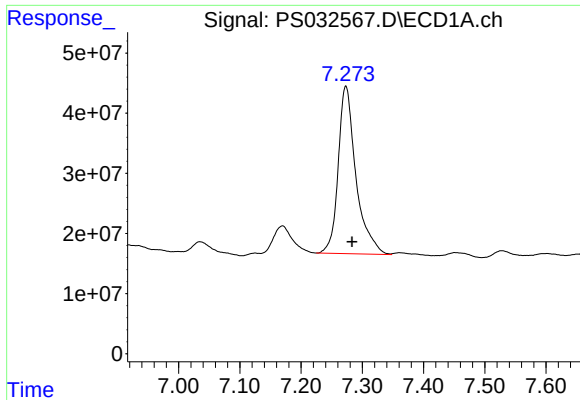

#4 2,4-DCAA


R.T.: 7.273 min
Delta R.T.: -0.010 min
Response: 560624827
Conc: 123.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

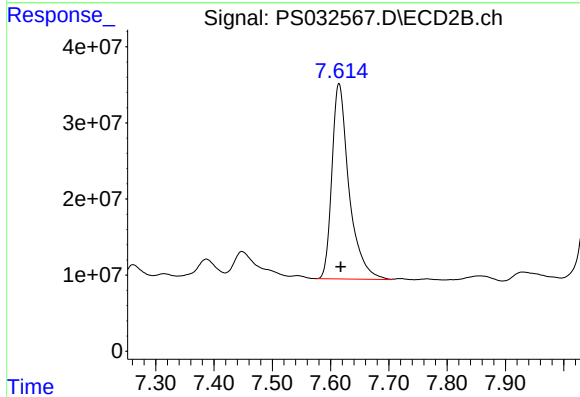


#4 2,4-DCAA

R.T.: 7.615 min
Delta R.T.: -0.003 min
Response: 523018169
Conc: 143.47 ng/ml

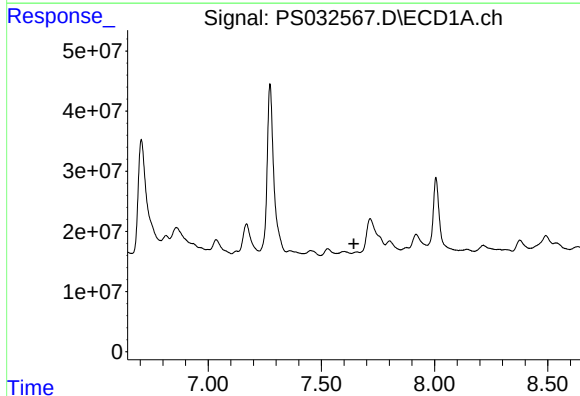


#6 MCP

R.T.: 7.658 min
Delta R.T.: 0.014 min
Response: -524393
Conc: N.D.

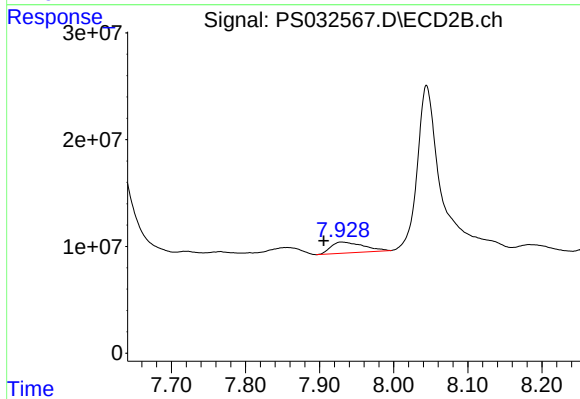

#6 MCP


R.T.: 7.930 min
Delta R.T.: 0.025 min
Response: 31203719
Conc: 2.35 ug/ml

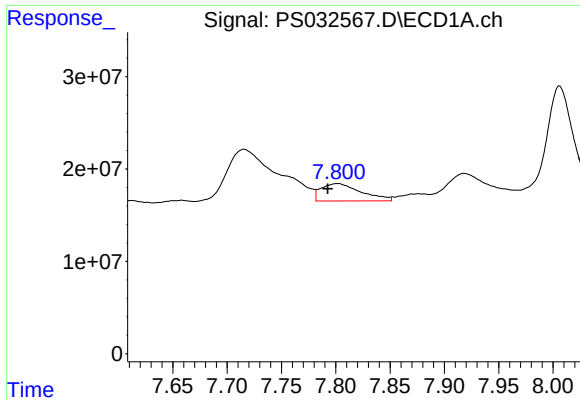

#7 MCPA


R.T.: 7.801 min
Delta R.T.: 0.009 min
Response: 48383431
Conc: 3.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

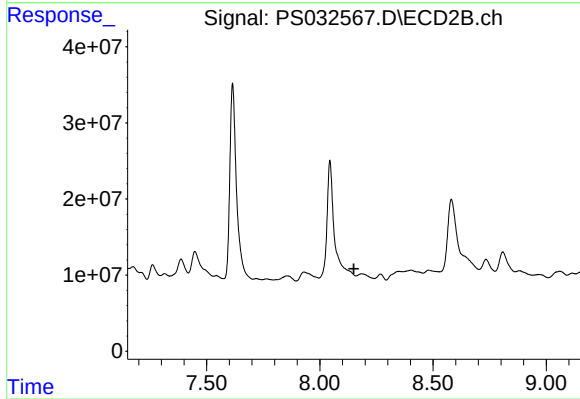


#7 MCPA

R.T.: 8.184 min
Delta R.T.: 0.033 min
Response: -2764914
Conc: N.D.

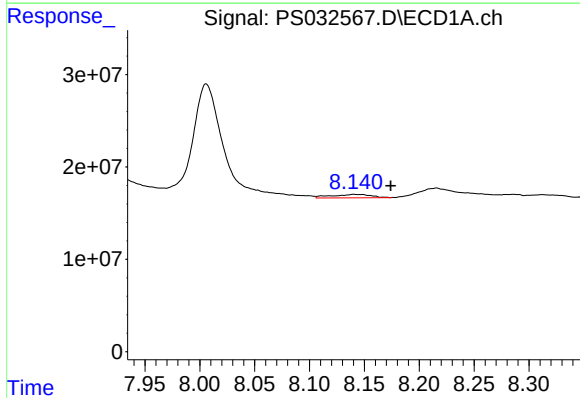


#8 DICHLORPROP

R.T.: 8.142 min
Delta R.T.: -0.032 min
Response: 9230533
Conc: 2.07 ng/ml

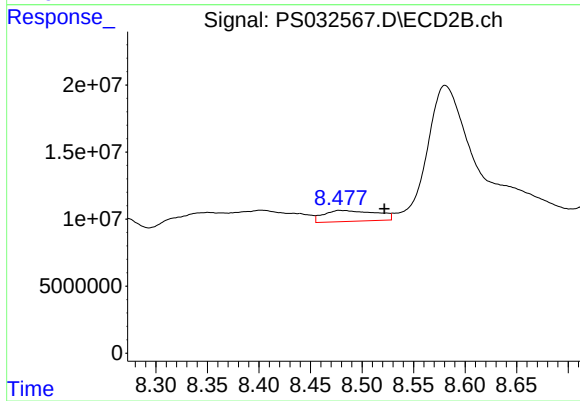

#8 DICHLORPROP


R.T.: 8.480 min
Delta R.T.: -0.042 min
Response: 29008461
Conc: 6.08 ng/ml

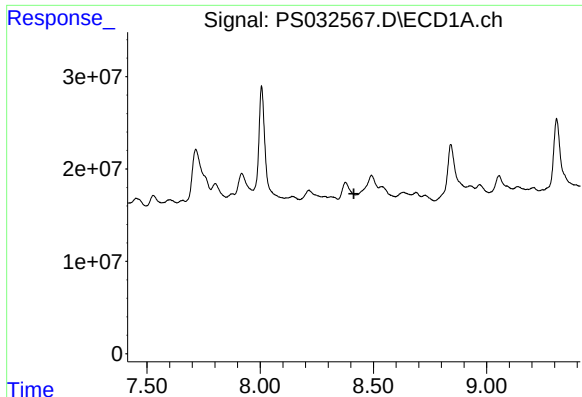

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

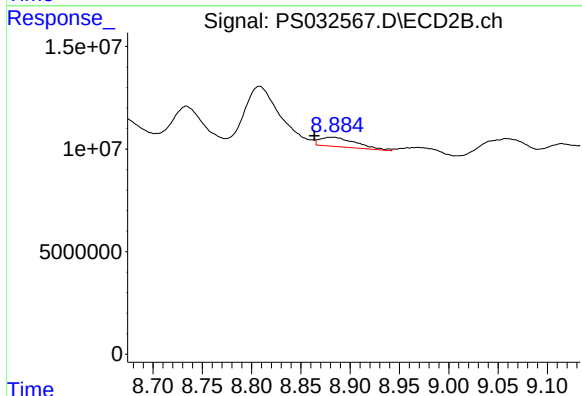


#9 2,4-D

R.T.: 8.882 min
Delta R.T.: 0.018 min
Response: 11554256
Conc: 2.20 ng/ml

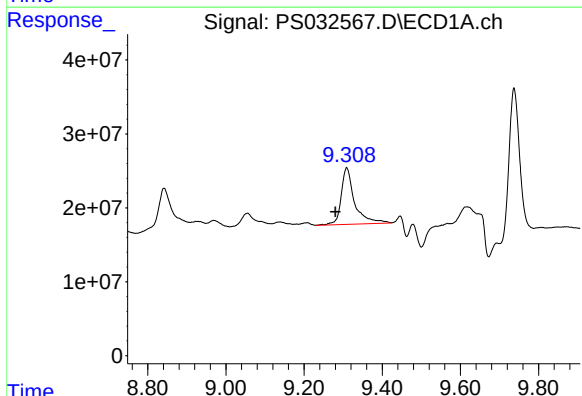


#11 2,4,5-TP (SILVEX)

R.T.: 9.309 min
Delta R.T.: 0.029 min
Response: 181766805
Conc: 6.99 ng/ml

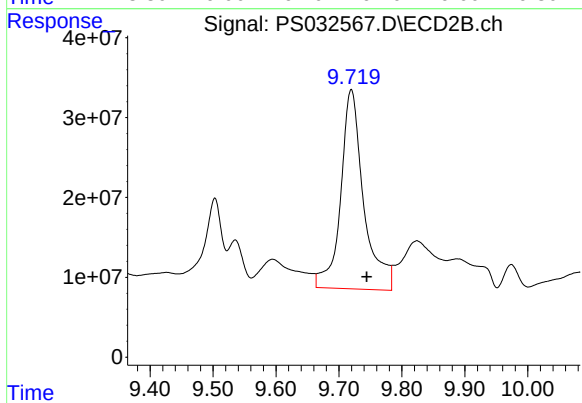

#11 2,4,5-TP (SILVEX)


R.T.: 9.720 min
Delta R.T.: -0.024 min
Response: 632398462
Conc: 23.55 ng/ml

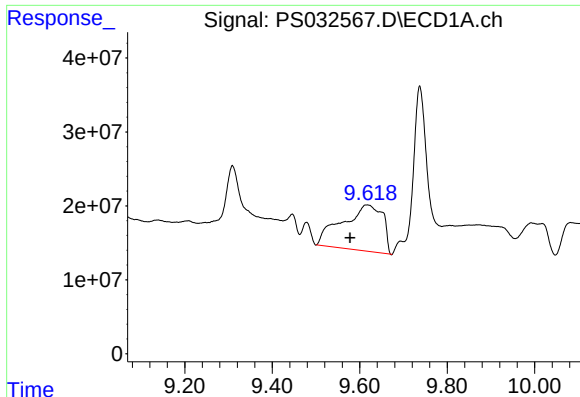

#12 2,4,5-T


R.T.: 9.617 min
Delta R.T.: 0.038 min
Response: 399464433
Conc: 16.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

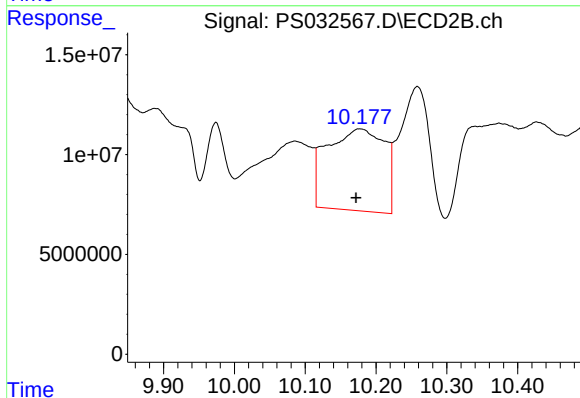


#12 2,4,5-T

R.T.: 10.177 min
Delta R.T.: 0.006 min
Response: 229482990
Conc: 9.68 ng/ml

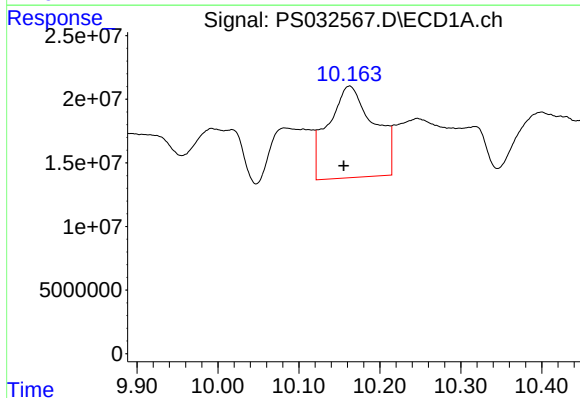


#13 2,4-DB

R.T.: 10.162 min
Delta R.T.: 0.007 min
Response: 281894253
Conc: 106.98 ng/ml

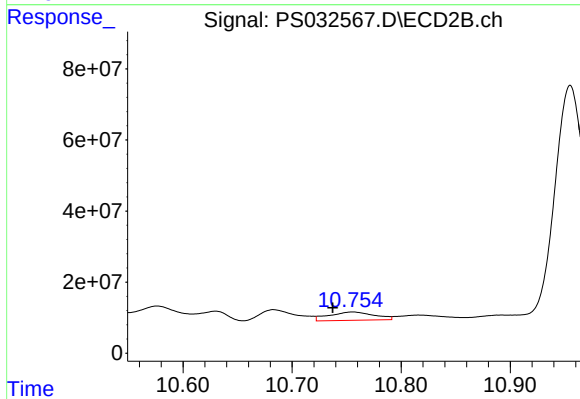

#13 2,4-DB


R.T.: 10.756 min
Delta R.T.: 0.018 min
Response: 67994758
Conc: 18.03 ng/ml

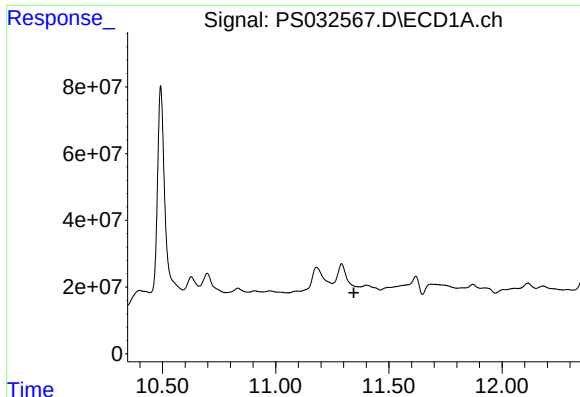

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

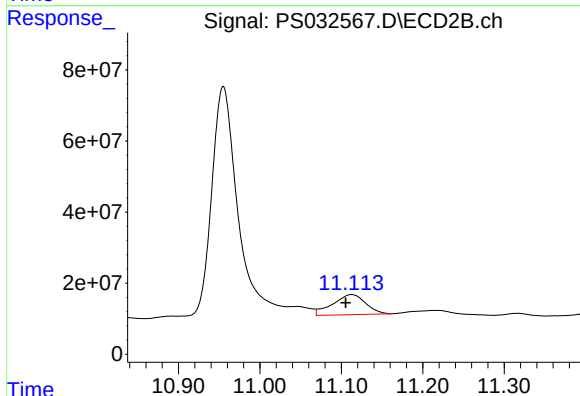


#14 DINOSEB

R.T.: 11.113 min
Delta R.T.: 0.007 min
Response: 159457524
Conc: 9.02 ng/ml

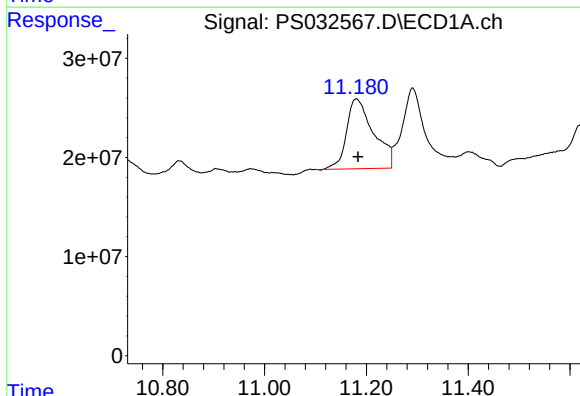


#15 Picloram

R.T.: 11.180 min
Delta R.T.: -0.004 min
Response: 261067221
Conc: 12.30 ng/ml

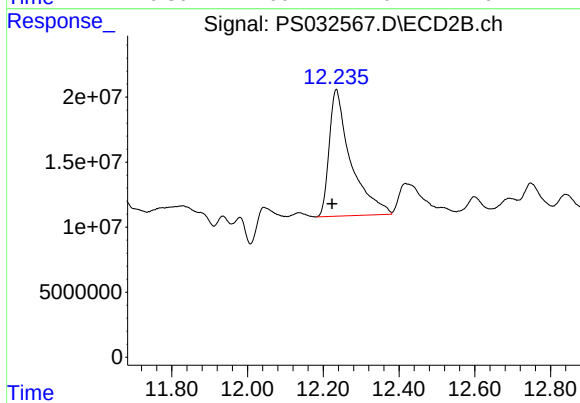

#15 Picloram


R.T.: 12.234 min
Delta R.T.: 0.011 min
Response: 385613843
Conc: 10.37 ng/ml

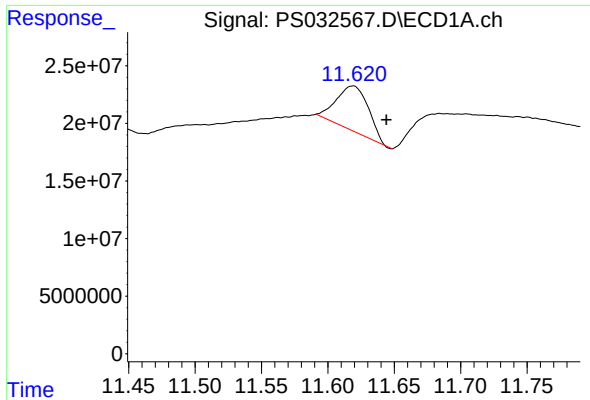

#16 DCPA

R.T.: 11.618 min
Delta R.T.: -0.026 min
Response: 64983974
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

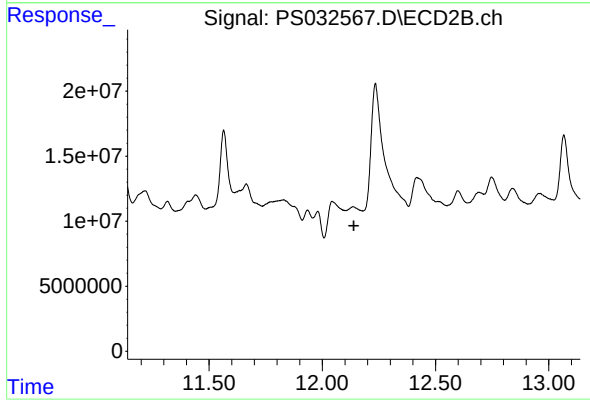

#16 DCPA

R.T.: 12.136 min
Delta R.T.: -0.003 min
Response: -5683414
Conc: N.D.