

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 18:21
 Operator : AR\AJ
 Sample : Q3732-01MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:06:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.290	0.000	416.4E6	0	91.890	N.D. #
Target Compounds							
1) T	Dalapon	2.616f	2.631f	2249.4E6	2884.2E6	313.342	414.749 #
3) T	4-Nitroph...	0.000	7.169	0	1657.3E6	N.D.	730.094
5) T	DICAMBA	7.485	0.000	11840.4E6	0	627.601	N.D. #
6) T	MCP	0.000	7.884	0	39788.5E6	N.D.	2991.405
7) T	MCPA	7.827f	0.000	15820.3E6	0	1178.350	N.D. #
8) T	DICHLORPROP	8.202f	8.552f	18347.5E6	380.5E6	4124.180	79.780 #
9) T	2,4-D	0.000	8.882	0	216.9E6	N.D.	41.352
11) T	2,4,5-TP ...	9.266	0.000	15289.3E6	0	587.788	N.D. #
12) T	2,4,5-T	9.562	0.000	1921.4E6	0	80.601	N.D. #
13) T	2,4-DB	10.187f	0.000	16058.7E6	0	6094.127	N.D. #
14) T	DINOSEB	11.327	0.000	403.1E6	0	19.373	N.D. #
16) T	DCPA	11.657	0.000	1394.9E6	0	41.576	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 18:21
Operator : AR\AJ
Sample : Q3732-01MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:06:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

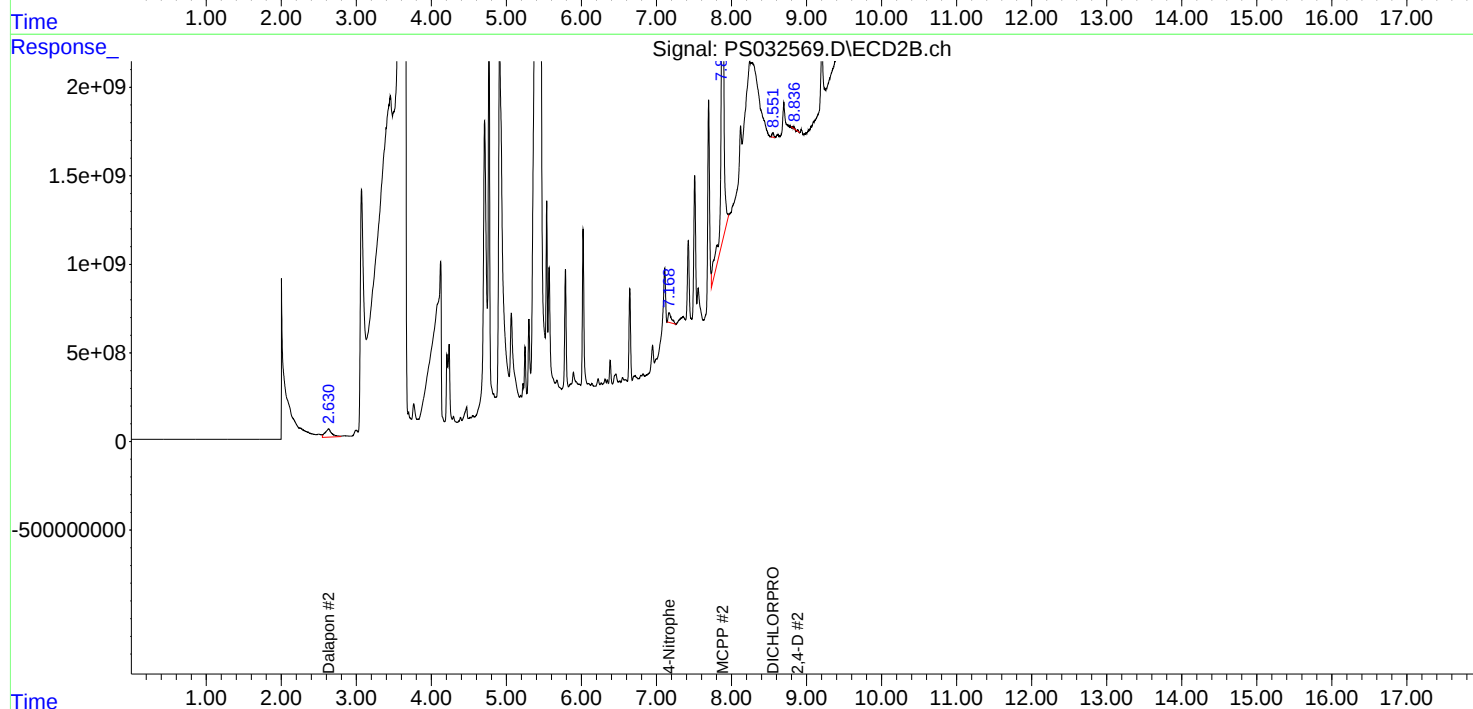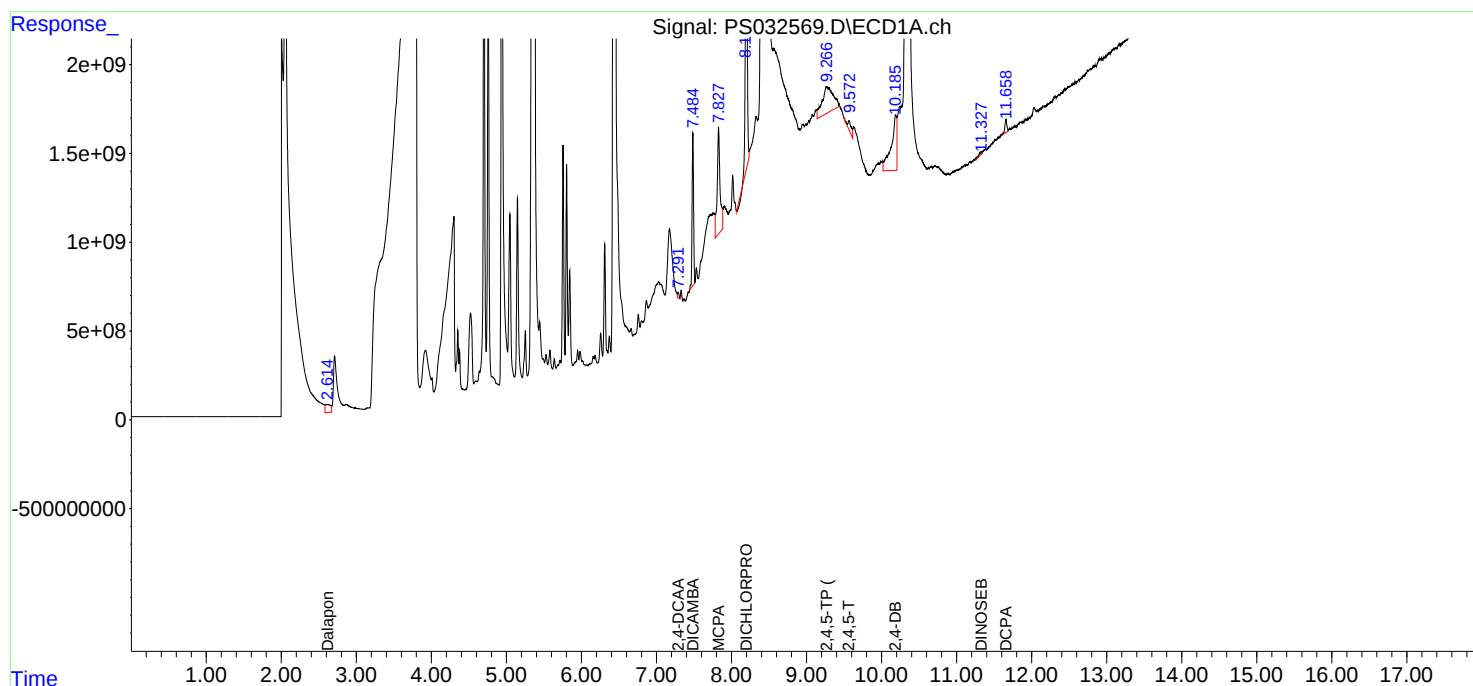


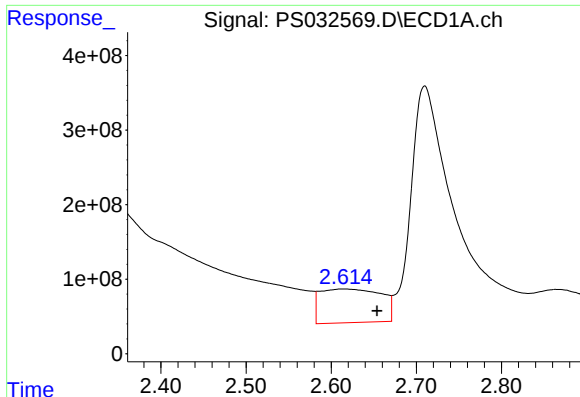

#1 Dalapon


R.T.: 2.616 min
Delta R.T.: -0.038 min
Response: 2249407986
Conc: 313.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

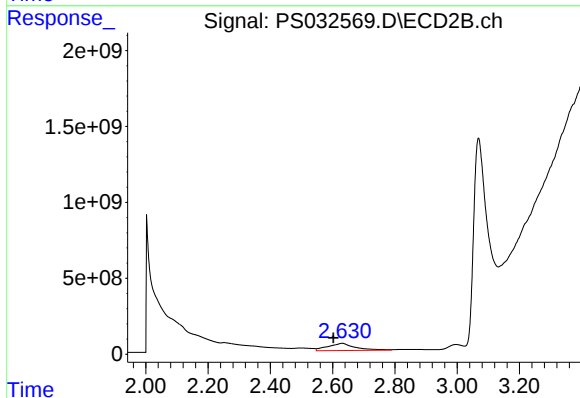


#1 Dalapon

R.T.: 2.631 min
Delta R.T.: 0.028 min
Response: 2884162695
Conc: 414.75 ng/ml

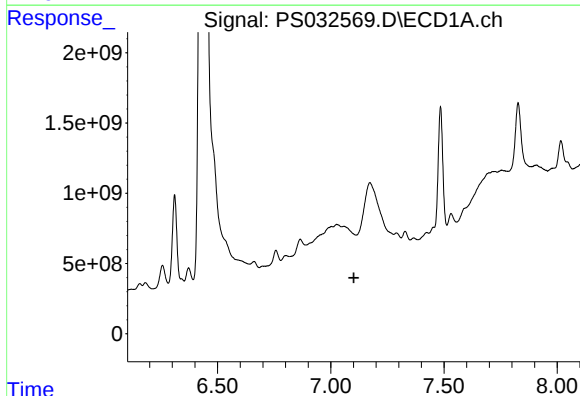


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.102 min
Response: 0
Conc: N.D.

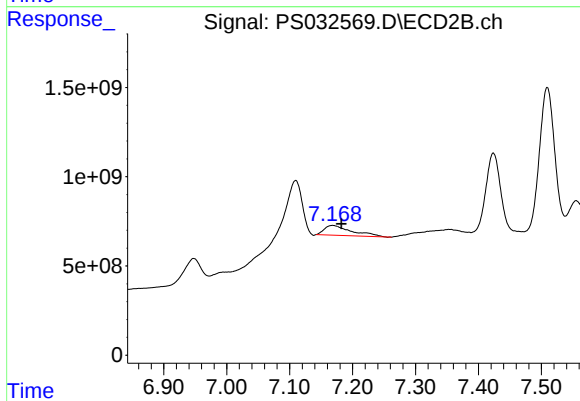

#3 4-Nitrophenol


R.T.: 7.169 min
Delta R.T.: -0.013 min
Response: 1657256125
Conc: 730.09 ng/ml

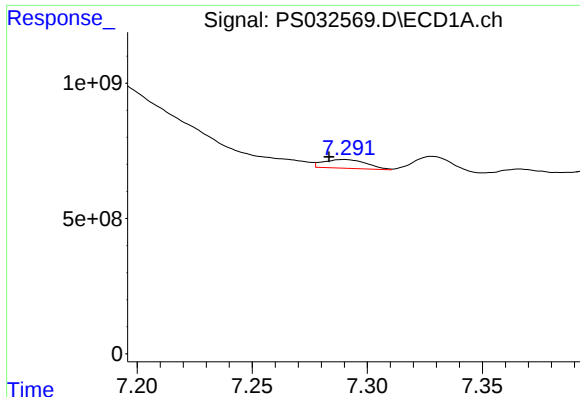

#4 2,4-DCAA


R.T.: 7.290 min
Delta R.T.: 0.006 min
Response: 416380459
Conc: 91.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

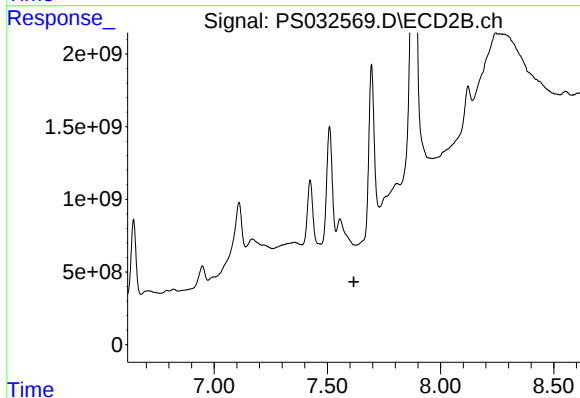


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

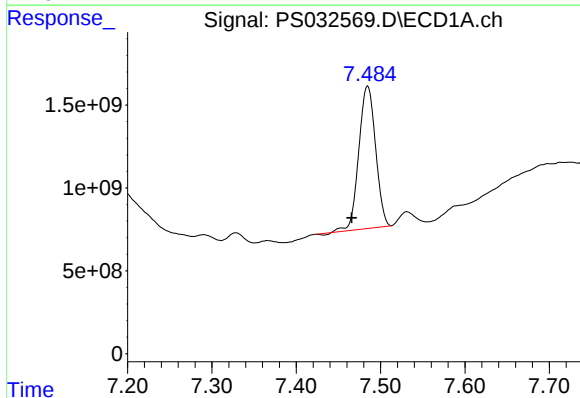


#5 DICAMBA

R.T.: 7.485 min
Delta R.T.: 0.019 min
Response: 11840419521
Conc: 627.60 ng/ml

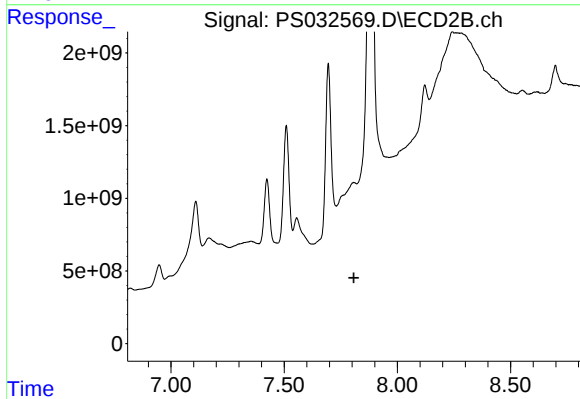

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.808 min
Response: 0
Conc: N.D.

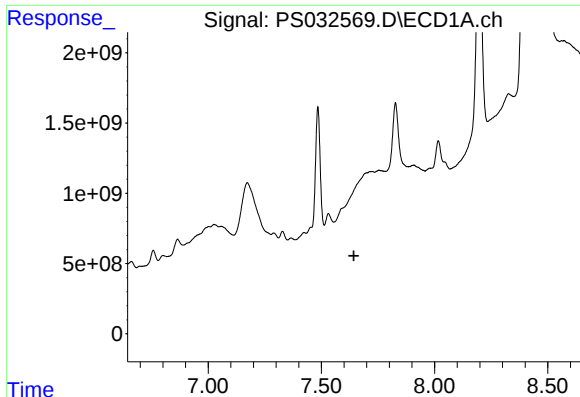

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

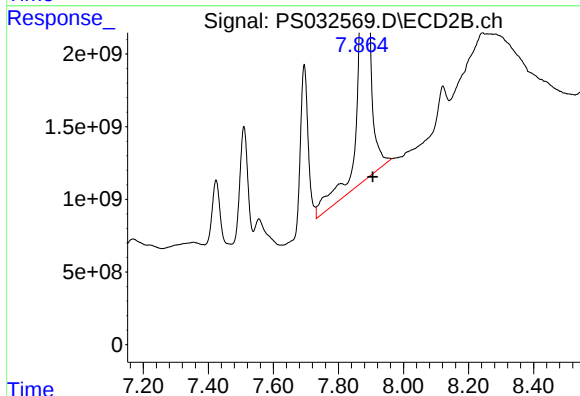


#6 MCP

R.T.: 7.884 min
Delta R.T.: -0.022 min
Response: 39788528532
Conc: 2991.40 ug/ml

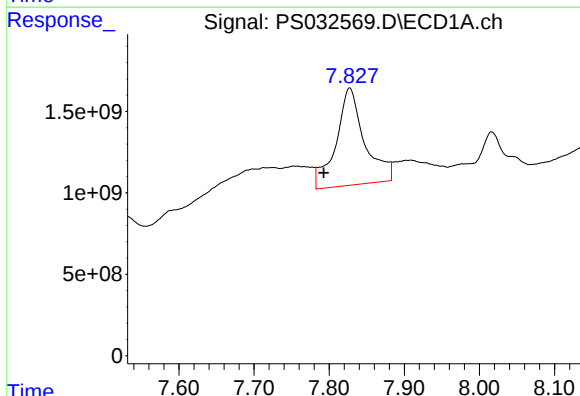


#7 MCP

R.T.: 7.827 min
Delta R.T.: 0.035 min
Response: 15820252811
Conc: 1178.35 ug/ml

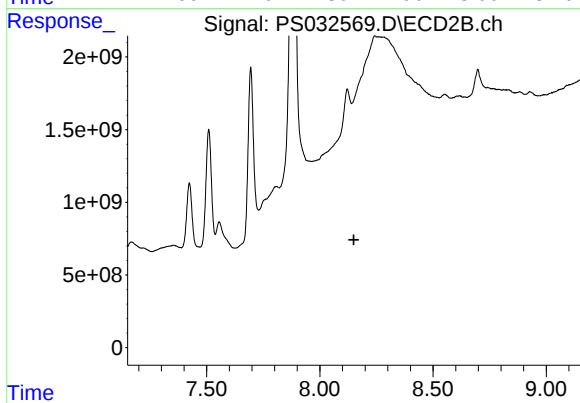

#7 MCP


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

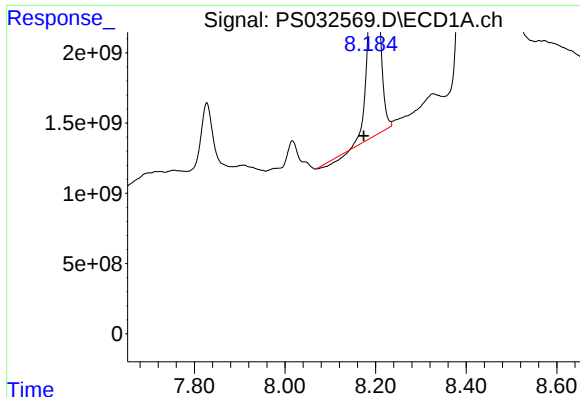

#8 DICHLORPROP


R.T.: 8.202 min
Delta R.T.: 0.028 min
Response: 18347476291
Conc: 4124.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

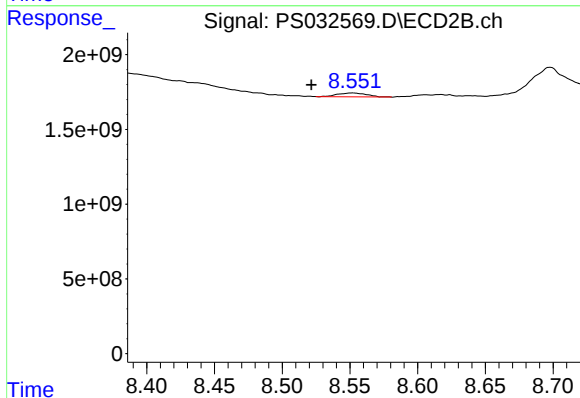


#8 DICHLORPROP

R.T.: 8.552 min
Delta R.T.: 0.030 min
Response: 380480743
Conc: 79.78 ng/ml

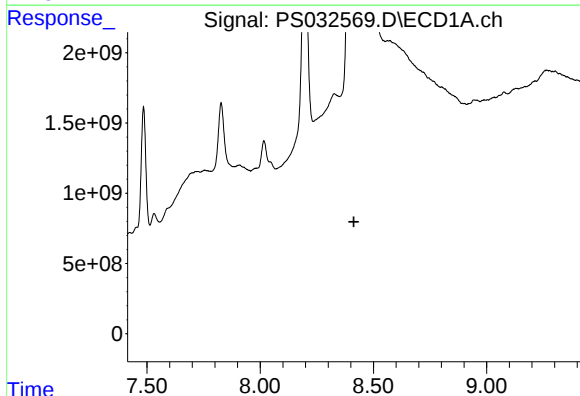


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.414 min
Response: 0
Conc: N.D.

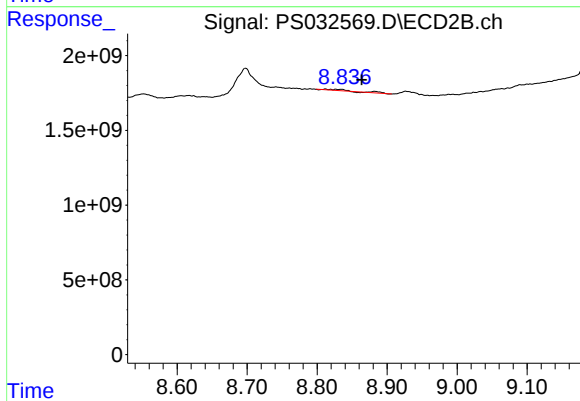

#9 2,4-D


R.T.: 8.882 min
Delta R.T.: 0.018 min
Response: 216918674
Conc: 41.35 ng/ml

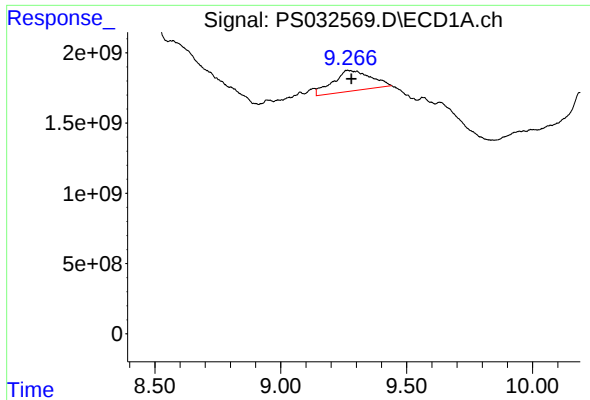

#11 2,4,5-TP (SILVEX)


R.T.: 9.266 min
Delta R.T.: -0.015 min
Response: 15289288673
Conc: 587.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

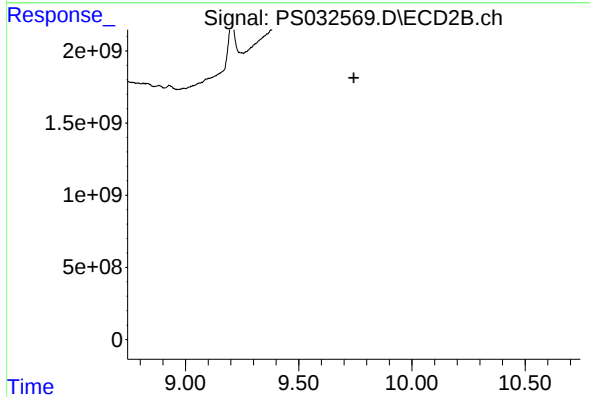


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.744 min
Response: 0
Conc: N.D.

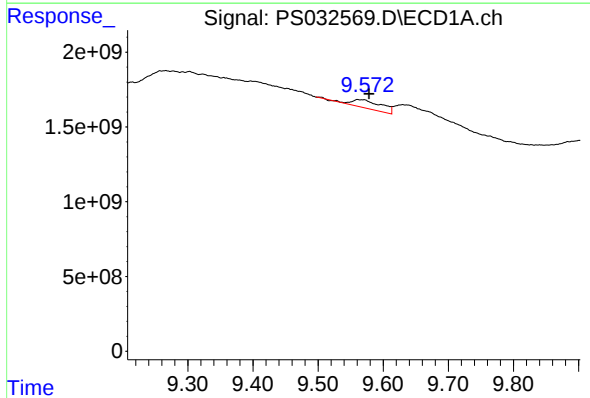


#12 2,4,5-T

R.T.: 9.562 min
Delta R.T.: -0.016 min
Response: 1921385560
Conc: 80.60 ng/ml

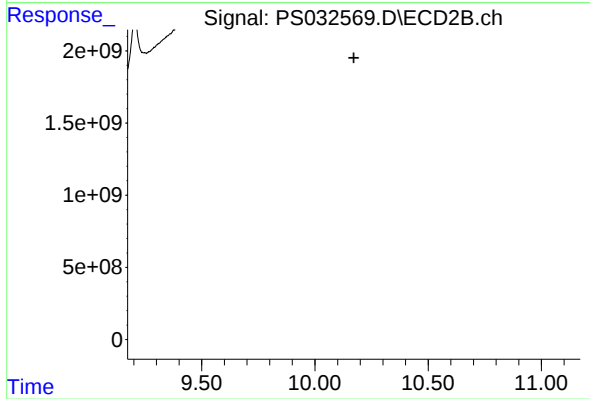

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 10.172 min
Response: 0
Conc: N.D.

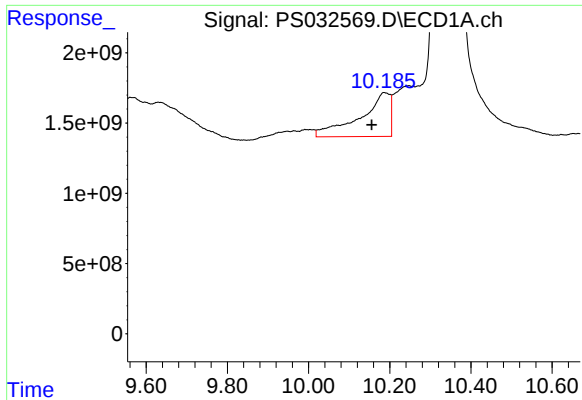

#13 2,4-DB


R.T.: 10.187 min
Delta R.T.: 0.031 min
Response: 16058730266
Conc: 6094.13 ng/m

Instrument :
ECD_S
ClientSampleId :

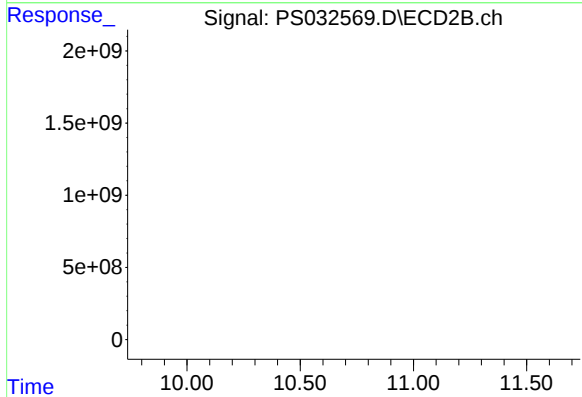


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

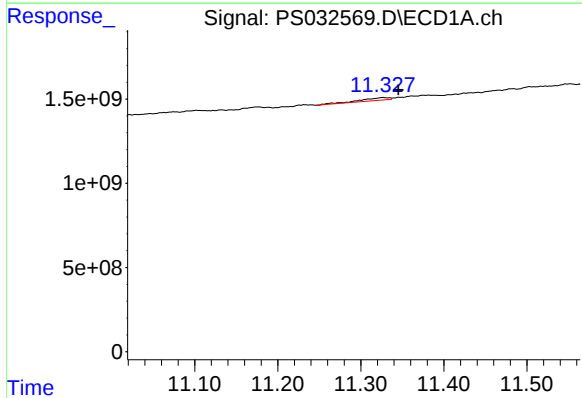


#14 DINOSEB

R.T.: 11.327 min
Delta R.T.: -0.018 min
Response: 403101808
Conc: 19.37 ng/ml

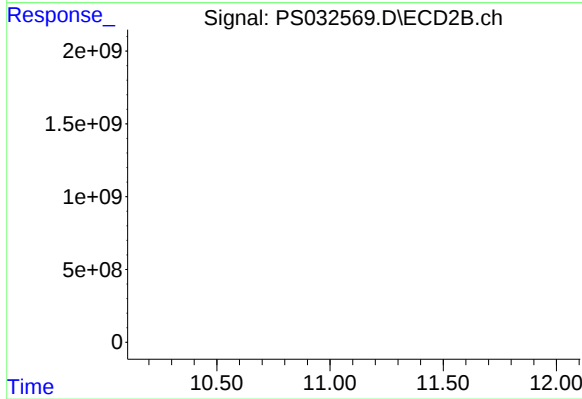

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.105 min
Response: 0
Conc: N.D.

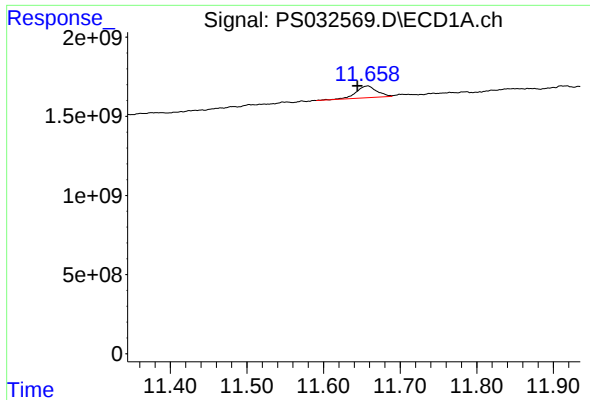

#16 DCPA

R.T.: 11.657 min
Delta R.T.: 0.013 min
Response: 1394946549
Conc: 41.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

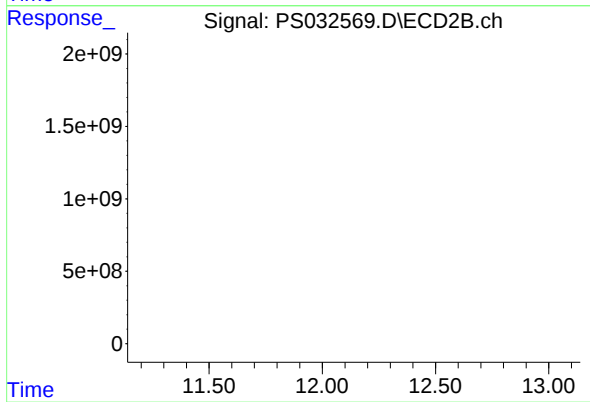

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.140 min
Response: 0
Conc: N.D.