

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 18:45
 Operator : AR\AJ
 Sample : Q3733-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:06:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	0.000	26585341	0	5.867	N.D. #
Target Compounds							
1) T	Dalapon	2.635	0.000	305.6E6	0	42.568	N.D. #
2) T	3,5-DICHL...	6.440	6.582	24465949	28537012	3.784	4.749 #
3) T	4-Nitroph...	7.111	0.000	14049358	0	10.465	N.D. #
5) T	DICAMBA	7.473	7.798	18050839	508.7E6	<MDL	29.453 #
6) T	MCPD	7.637	0.000	20944565	0	1.923	N.D. #
7) T	MCPA	7.801	0.000	154.8E6	0	11.528	N.D. #
8) T	DICHLORPROP	8.169	0.000	91524252	0	20.573	N.D. #
9) T	2,4-D	8.403	0.000	23617922	0	5.235	N.D. #
10) T	Pentachlo...	8.706	0.000	20159068	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.291	0.000	8753667	0	<MDL	N.D. #
12) T	2,4,5-T	9.578	0.000	51585864	0	2.164	N.D. #
13) T	2,4-DB	10.199f	0.000	243.0E6	0	92.209	N.D. #
14) T	DINOSEB	11.342	0.000	161.7E6	0	7.773	N.D. #
15) T	Picloram	11.202	0.000	60457439	0	2.848	N.D. #
16) T	DCPA	11.664	0.000	97075186	0	2.893	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 18:45
Operator : AR\AJ
Sample : Q3733-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:06:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

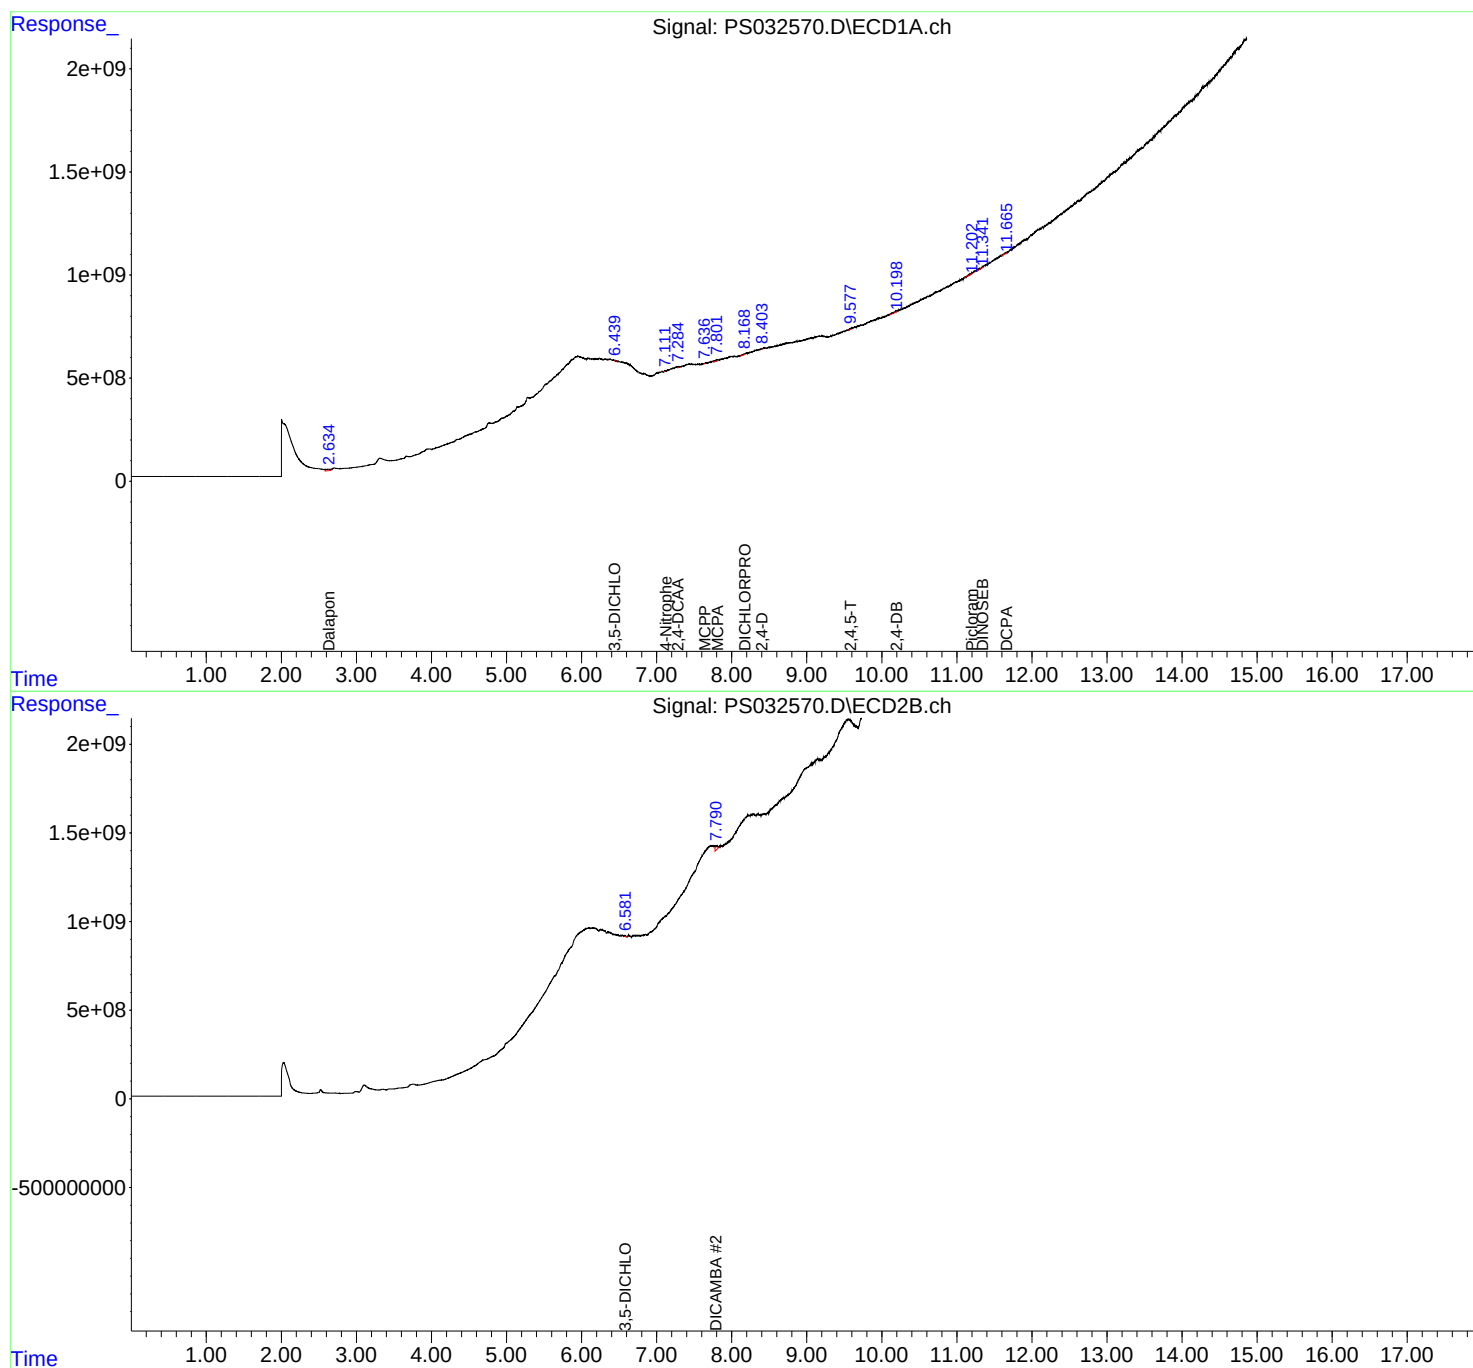


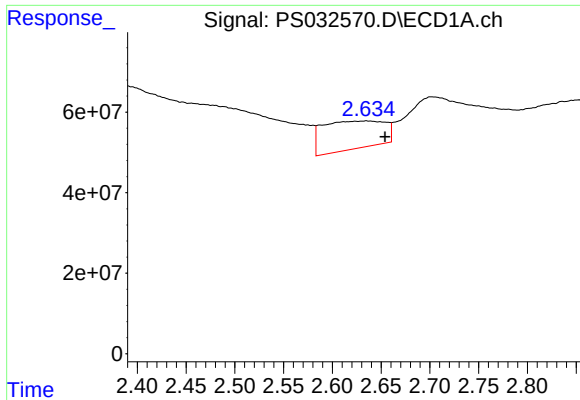

#1 Dalapon


R.T.: 2.635 min
Delta R.T.: -0.019 min
Response: 305586082
Conc: 42.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

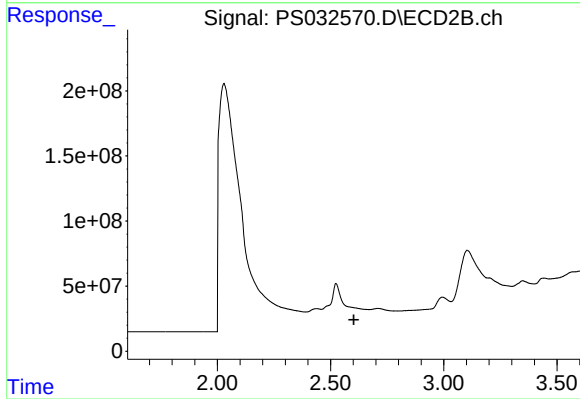


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.603 min
Response: 0
Conc: N.D.

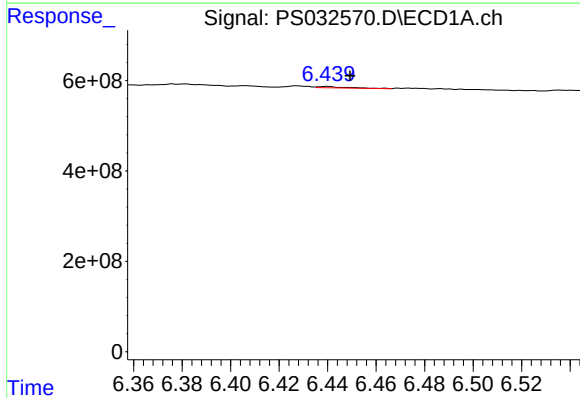


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.440 min
Delta R.T.: -0.010 min
Response: 24465949
Conc: 3.78 ng/ml

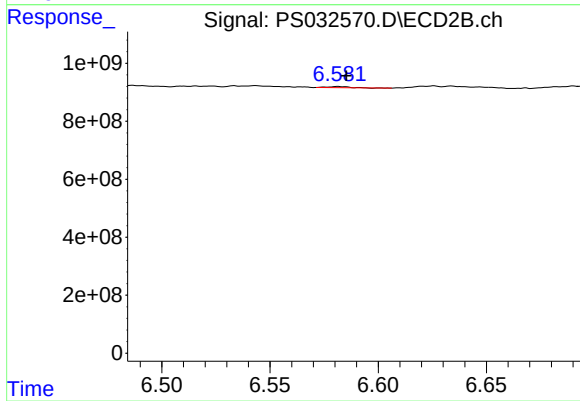

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.582 min
Delta R.T.: -0.004 min
Response: 28537012
Conc: 4.75 ng/ml

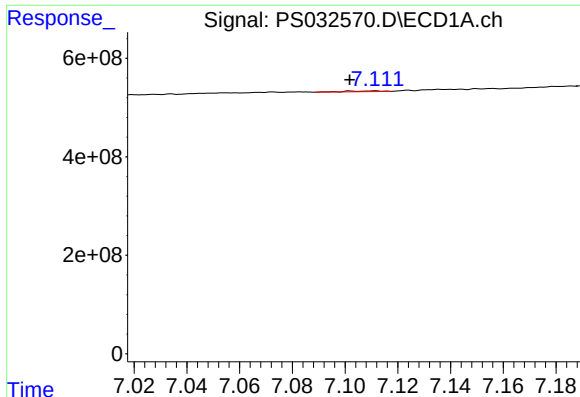

#3 4-Nitrophenol


R.T.: 7.111 min
Delta R.T.: 0.010 min
Response: 14049358
Conc: 10.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

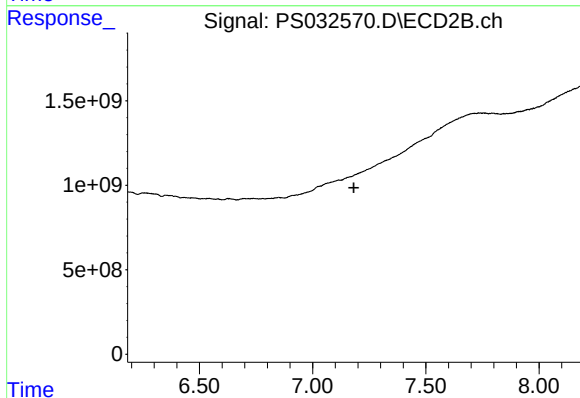


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

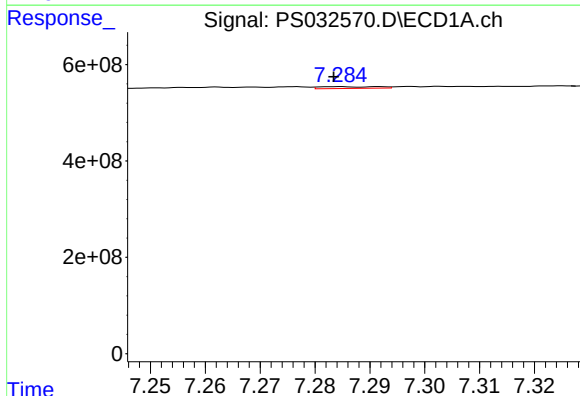


#4 2,4-DCAA

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 26585341
Conc: 5.87 ng/ml

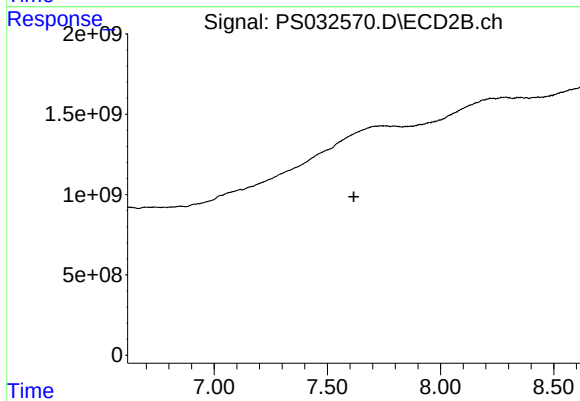

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

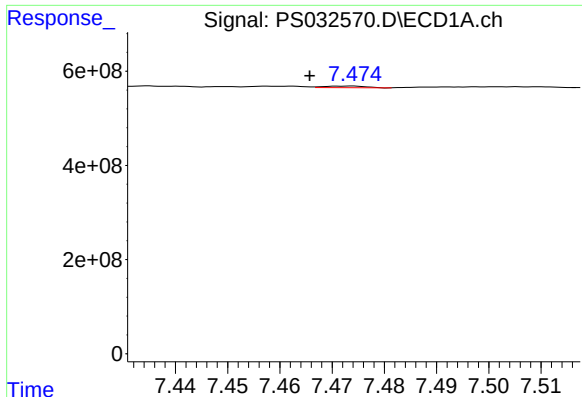

#5 DICAMBA


R.T.: 7.473 min
Delta R.T.: 0.008 min
Response: 18050839
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

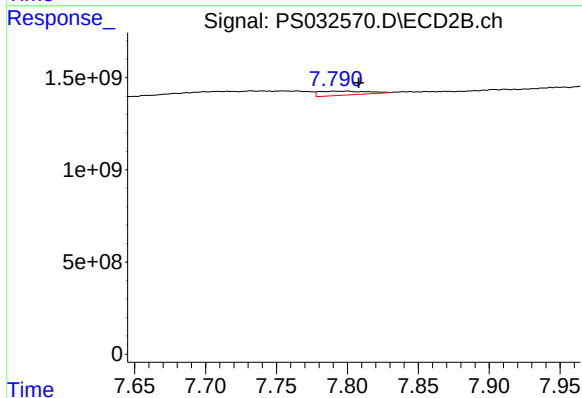


#5 DICAMBA

R.T.: 7.798 min
Delta R.T.: -0.010 min
Response: 508732951
Conc: 29.45 ng/ml

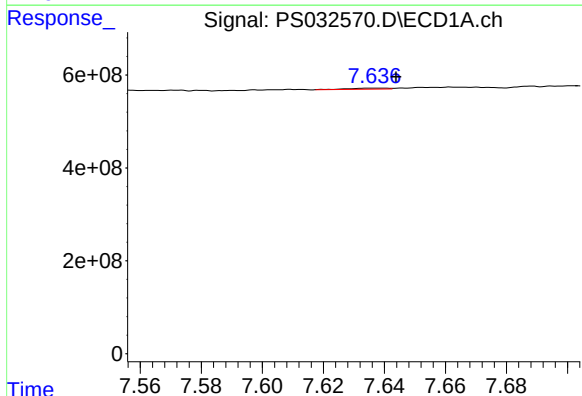


#6 MCP

R.T.: 7.637 min
Delta R.T.: -0.007 min
Response: 20944565
Conc: 1.92 ug/ml

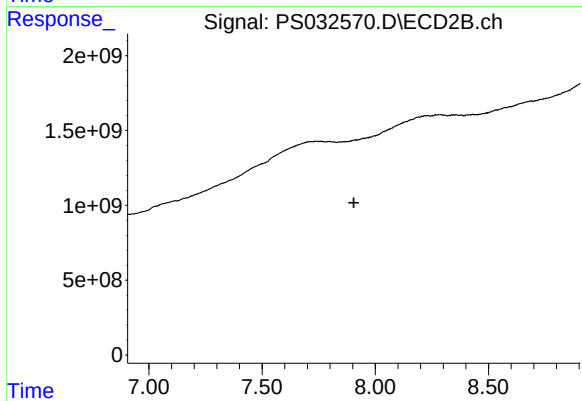

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.906 min
Response: 0
Conc: N.D.

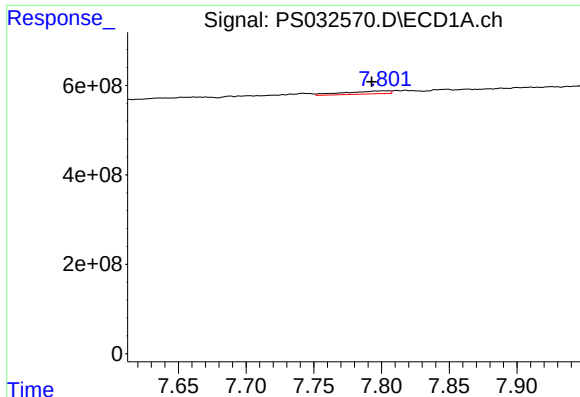

#7 MCPA


R.T.: 7.801 min
Delta R.T.: 0.009 min
Response: 154774964
Conc: 11.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

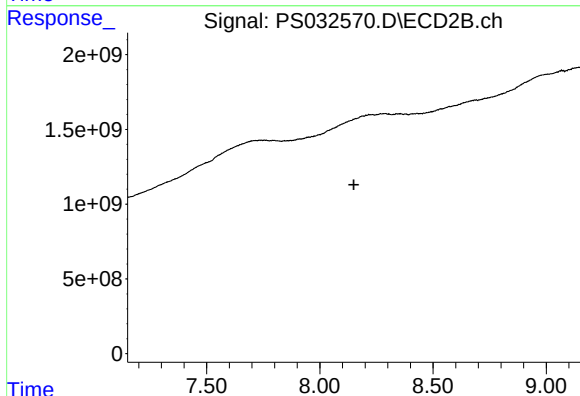


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

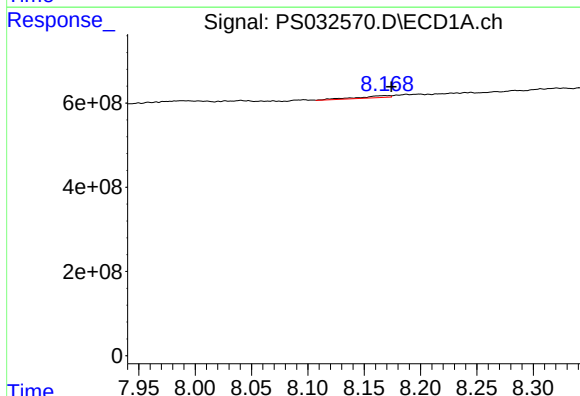


#8 DICHLORPROP

R.T.: 8.169 min
Delta R.T.: -0.005 min
Response: 91524252
Conc: 20.57 ng/ml

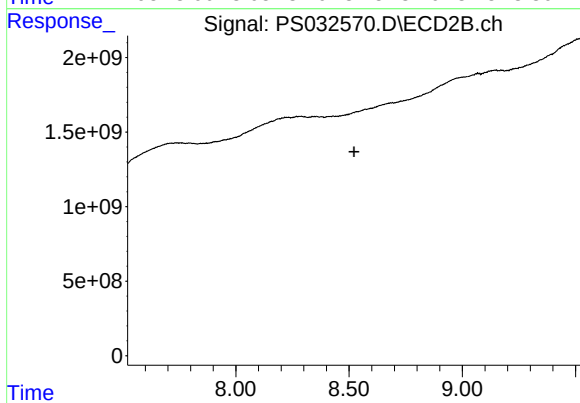

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.522 min
Response: 0
Conc: N.D.

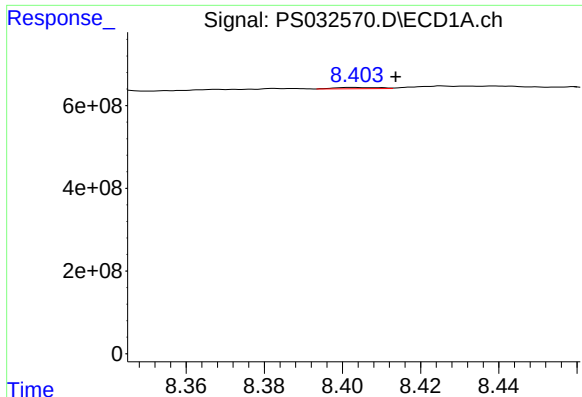

#9 2,4-D


R.T.: 8.403 min
Delta R.T.: -0.011 min
Response: 23617922
Conc: 5.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

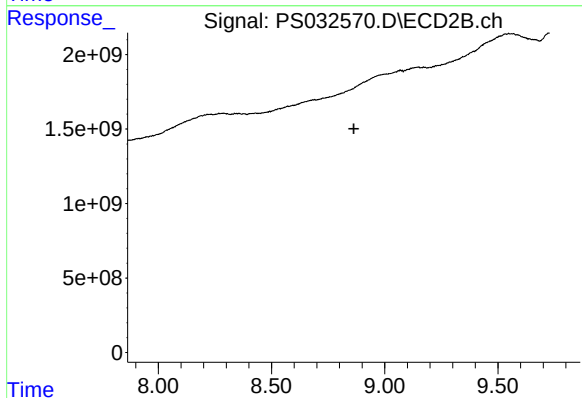


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.

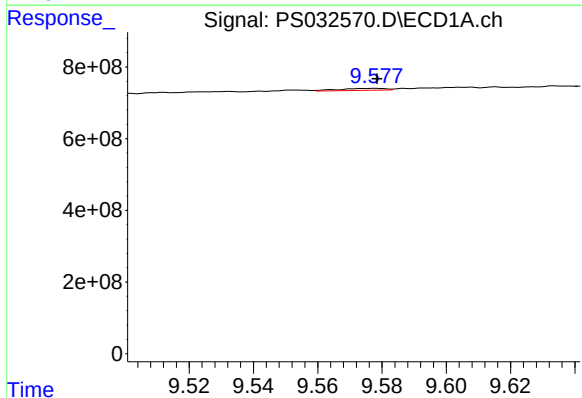


#12 2,4,5-T

R.T.: 9.578 min
Delta R.T.: 0.000 min
Response: 51585864
Conc: 2.16 ng/ml

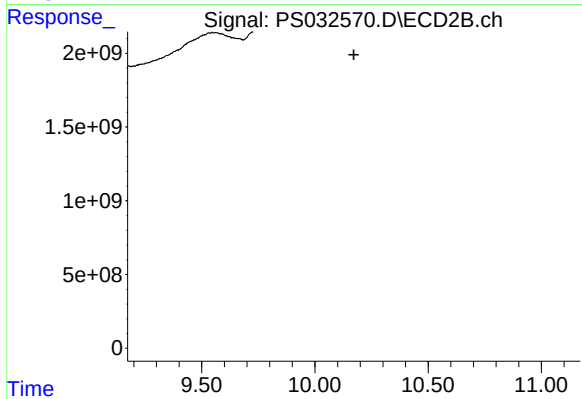

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 10.172 min
Response: 0
Conc: N.D.

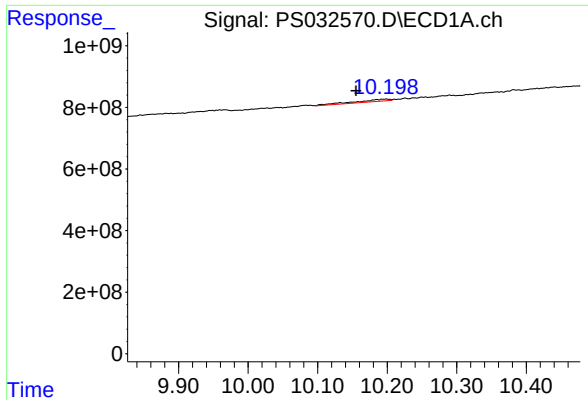

#13 2,4-DB


R.T.: 10.199 min
Delta R.T.: 0.044 min
Response: 242980849
Conc: 92.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

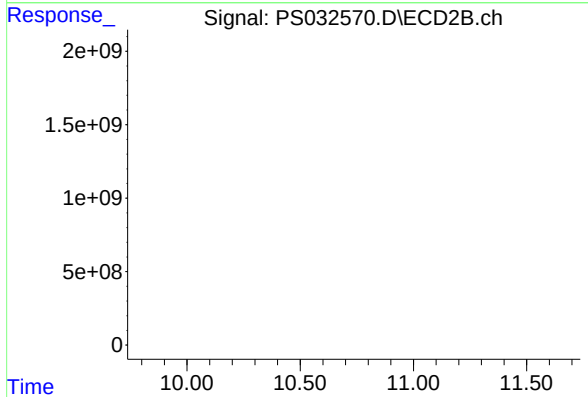


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

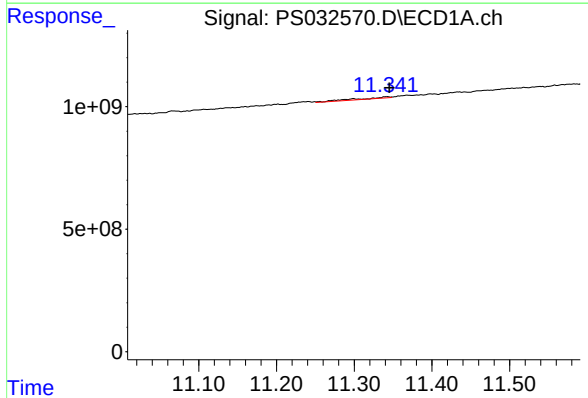


#14 DINOSEB

R.T.: 11.342 min
Delta R.T.: -0.003 min
Response: 161737134
Conc: 7.77 ng/ml

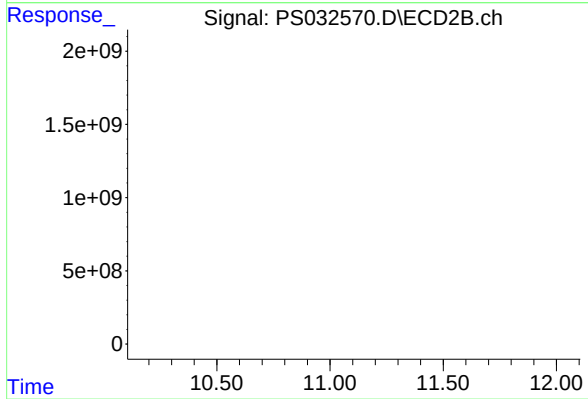

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.105 min
Response: 0
Conc: N.D.

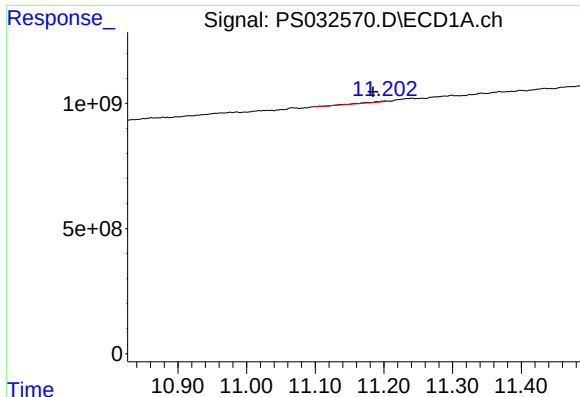

#15 Picloram


R.T.: 11.202 min
Delta R.T.: 0.018 min
Response: 60457439
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

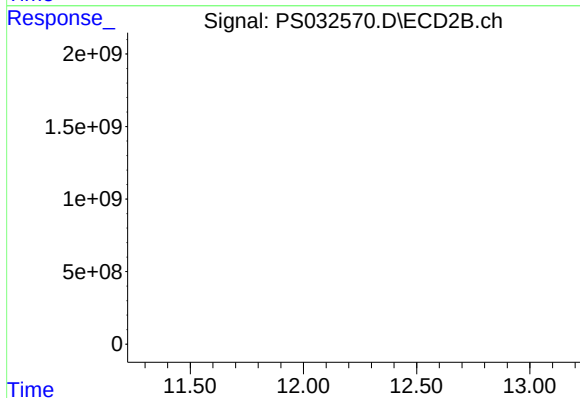


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.223 min
Response: 0
Conc: N.D.

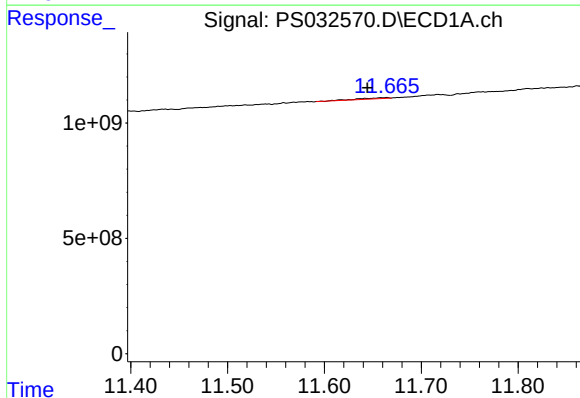

#16 DCPA

R.T.: 11.664 min
Delta R.T.: 0.020 min
Response: 97075186
Conc: 2.89 ng/ml

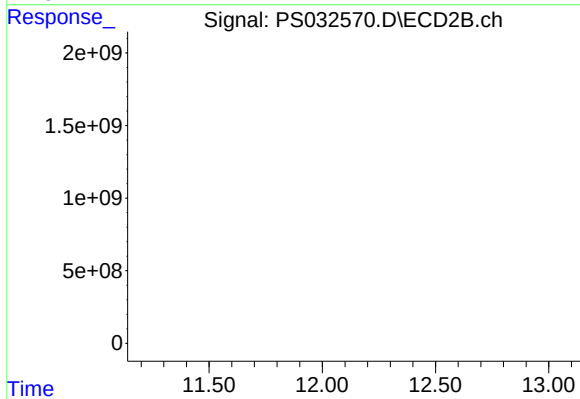

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.140 min
Response: 0
Conc: N.D.