

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 19:09
 Operator : AR\AJ
 Sample : Q3735-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:06:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.322f	0.000	350.0E6	0	77.235	N.D.	#
Target Compounds								
1) T	Dalapon	2.647	0.000	31755982	0	4.424	N.D.	#
2) T	3,5-DICHL...	6.445	6.588	13828849	32826872	2.139	5.463	#
3) T	4-Nitroph...	7.074f	0.000	9577895	0	7.135	N.D.	#
5) T	DICAMBA	7.465	7.770f	15632111	2007.5E6	<MDL	116.227	#
6) T	MCPD	7.681f	0.000	49853522	0	4.578	N.D.	#
7) T	MCPA	7.793	0.000	24941041	0	1.858	N.D.	#
8) T	DICHLORPROP	8.182	0.000	96763001	0	21.751	N.D.	#
10) T	Pentachlo...	8.719	0.000	27819300	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.258	0.000	15567608	0	<MDL	N.D.	#
12) T	2,4,5-T	9.597	0.000	37852168	0	1.588	N.D.	#
13) T	2,4-DB	10.168	0.000	39441082	0	14.967	N.D.	#
14) T	DINOSEB	11.317f	0.000	45616205	0	2.192	N.D.	#
15) T	Picloram	11.199	0.000	85431834	0	4.025	N.D.	#
16) T	DCPA	11.664	0.000	63516901	0	1.893	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 19:09
Operator : AR\AJ
Sample : Q3735-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:06:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

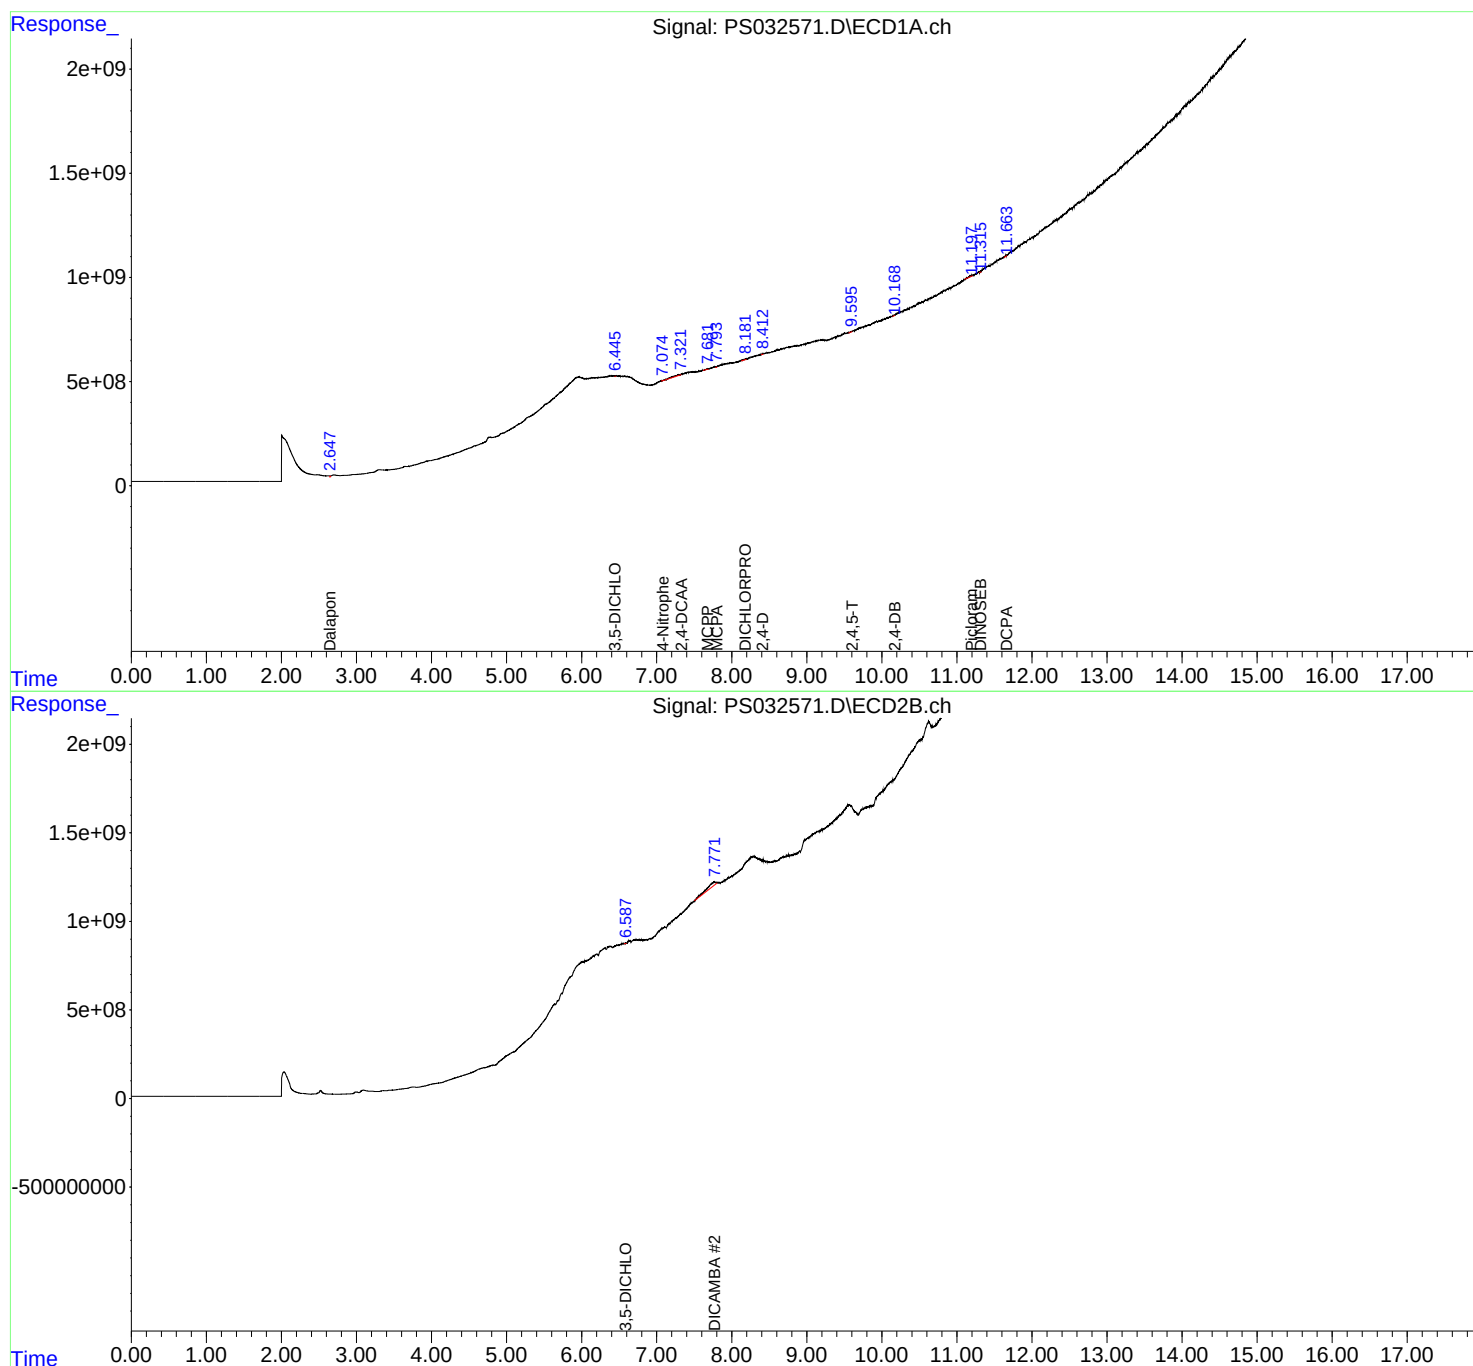


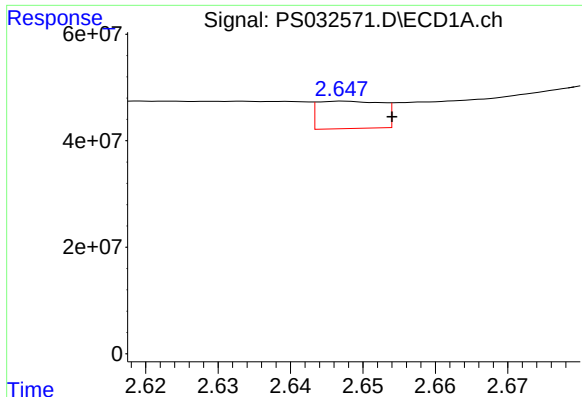

#1 Dalapon


R.T.: 2.647 min
Delta R.T.: -0.007 min
Response: 31755982
Conc: 4.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

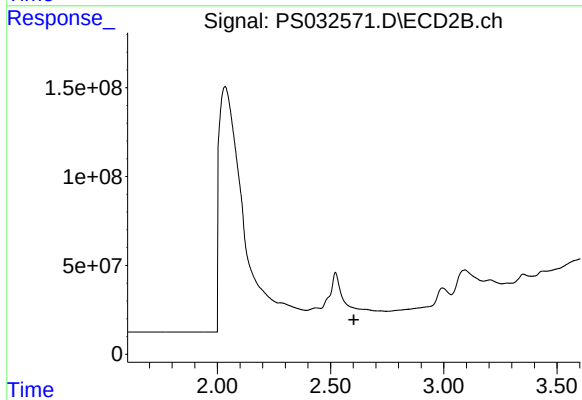


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.603 min
Response: 0
Conc: N.D.

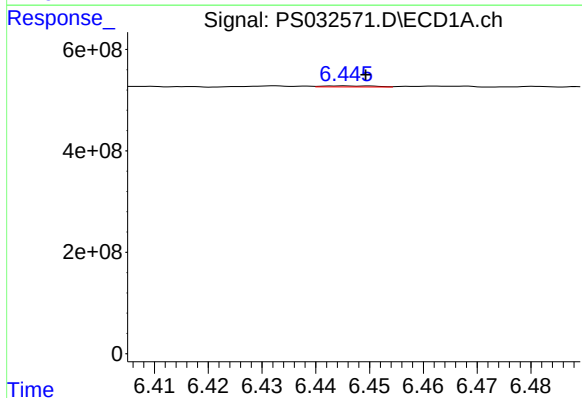


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.445 min
Delta R.T.: -0.004 min
Response: 13828849
Conc: 2.14 ng/ml

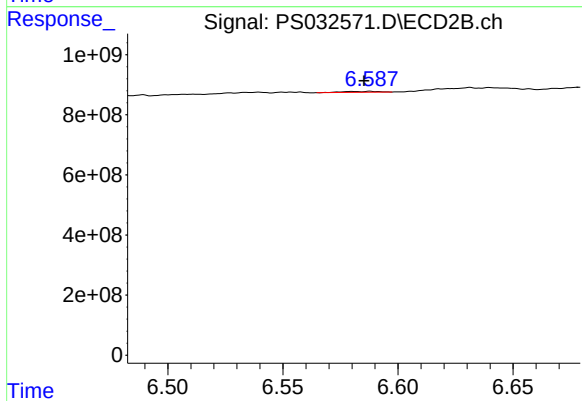

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.588 min
Delta R.T.: 0.002 min
Response: 32826872
Conc: 5.46 ng/ml

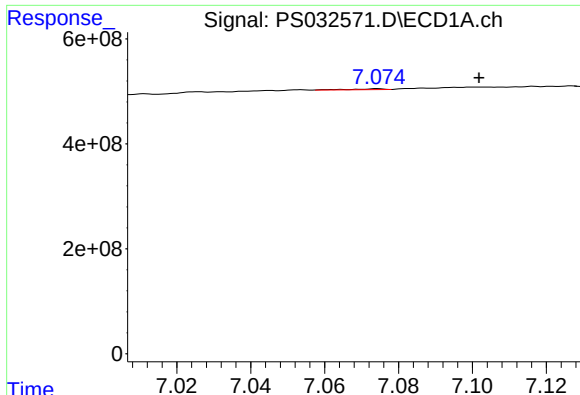

#3 4-Nitrophenol


R.T.: 7.074 min
Delta R.T.: -0.028 min
Response: 9577895
Conc: 7.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

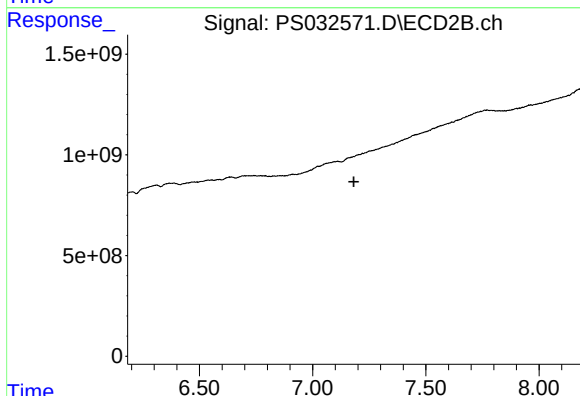


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

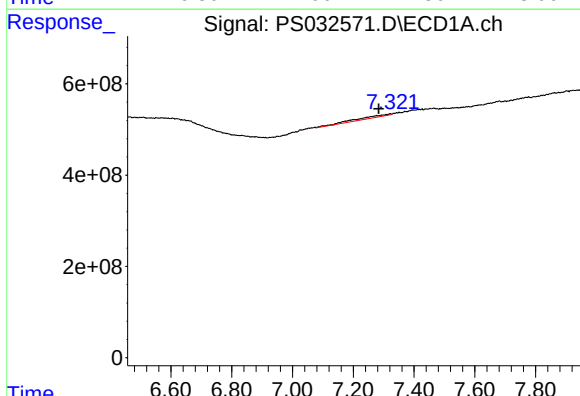


#4 2,4-DCAA

R.T.: 7.322 min
Delta R.T.: 0.038 min
Response: 349973975
Conc: 77.24 ng/ml

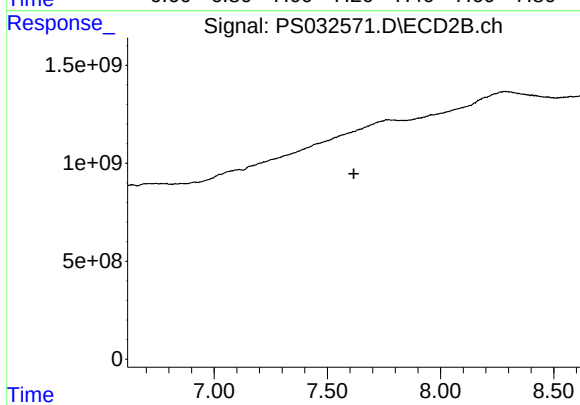

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

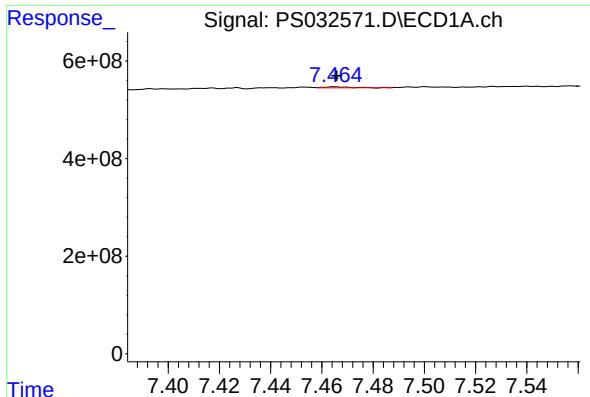

#5 DICAMBA


R.T.: 7.465 min
Delta R.T.: 0.000 min
Response: 15632111
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

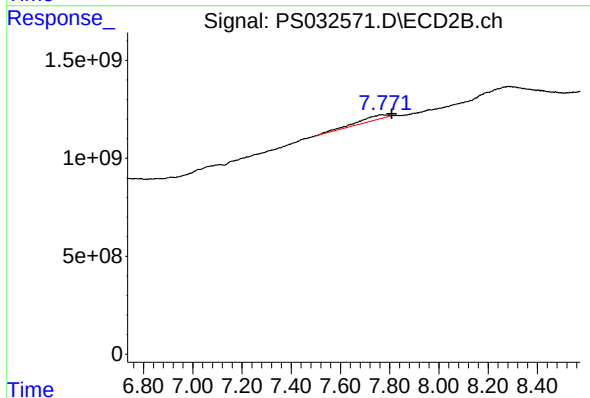


#5 DICAMBA

R.T.: 7.770 min
Delta R.T.: -0.038 min
Response: 2007532485
Conc: 116.23 ng/ml

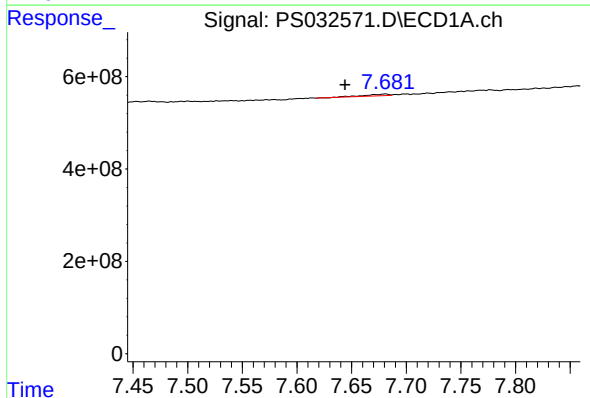


#6 MCP

R.T.: 7.681 min
Delta R.T.: 0.037 min
Response: 49853522
Conc: 4.58 ug/ml

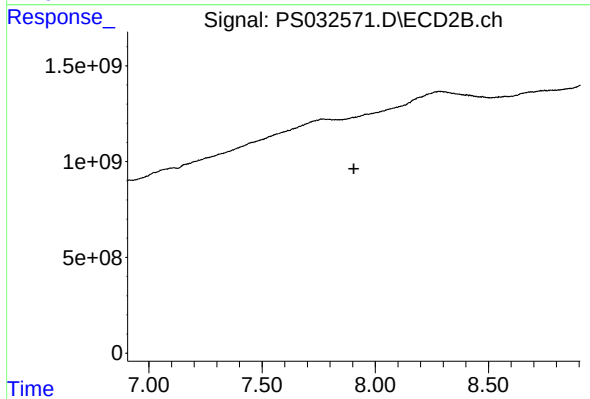

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.906 min
Response: 0
Conc: N.D.

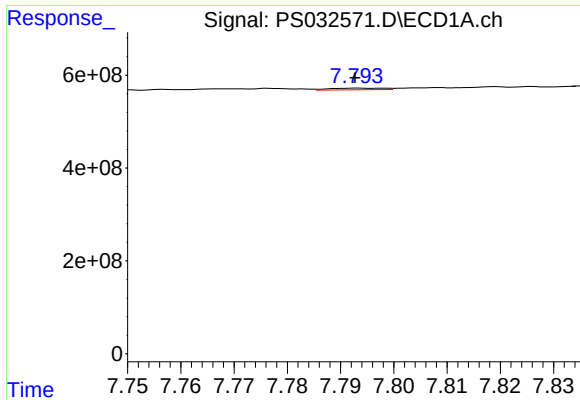

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 24941041
Conc: 1.86 ug/ml

Instrument :
ECD_S
ClientSampleId :

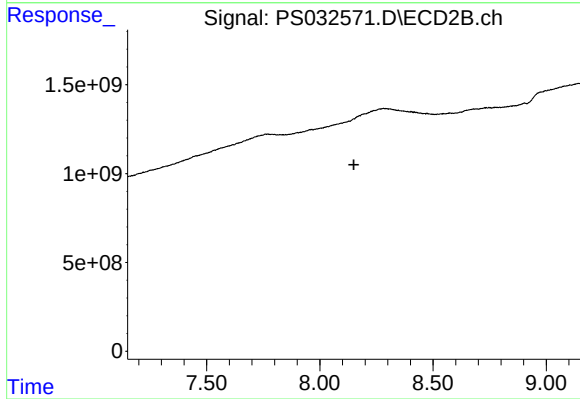


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

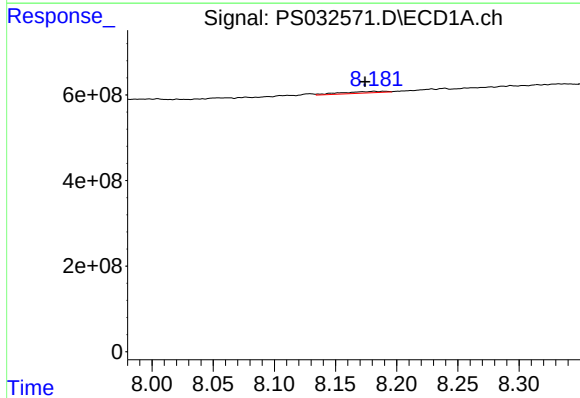


#8 DICHLORPROP

R.T.: 8.182 min
Delta R.T.: 0.008 min
Response: 96763001
Conc: 21.75 ng/ml

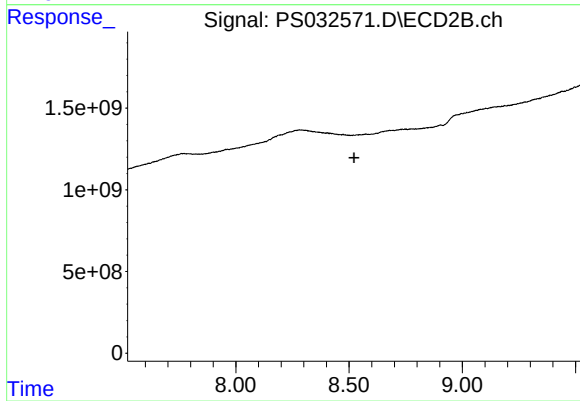

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.522 min
Response: 0
Conc: N.D.

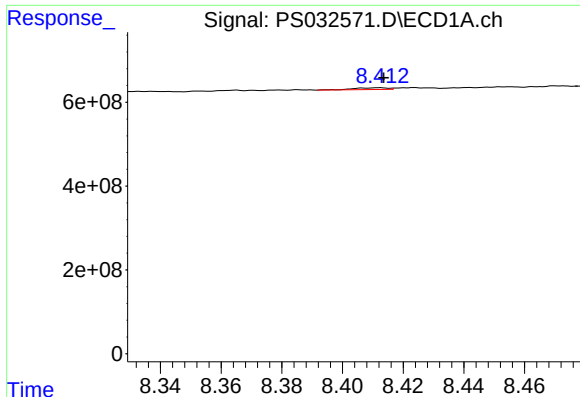

#9 2,4-D


R.T.: 8.412 min
Delta R.T.: -0.002 min
Response: 31408241
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

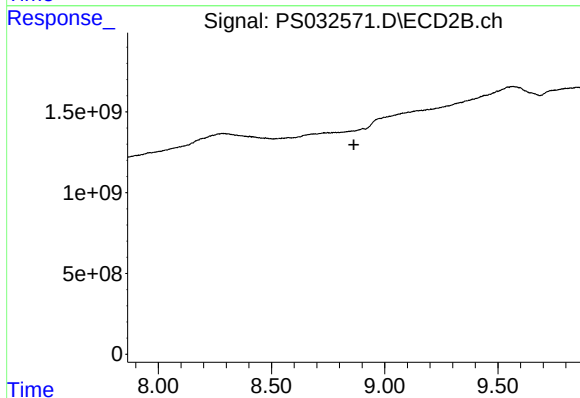


#9 2,4-D

R.T.: 8.904 min
Delta R.T.: 0.040 min
Response: -193993463
Conc: N.D.

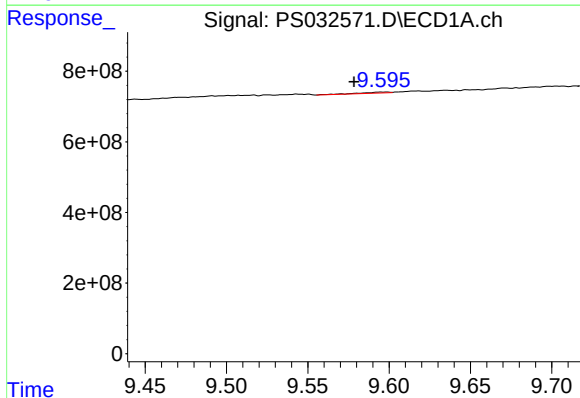


#12 2,4,5-T

R.T.: 9.597 min
Delta R.T.: 0.019 min
Response: 37852168
Conc: 1.59 ng/ml

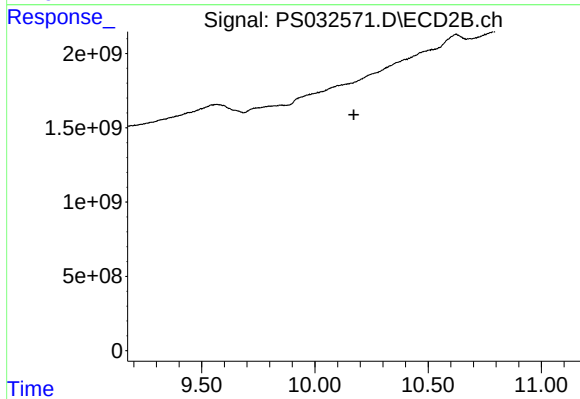

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 10.172 min
Response: 0
Conc: N.D.

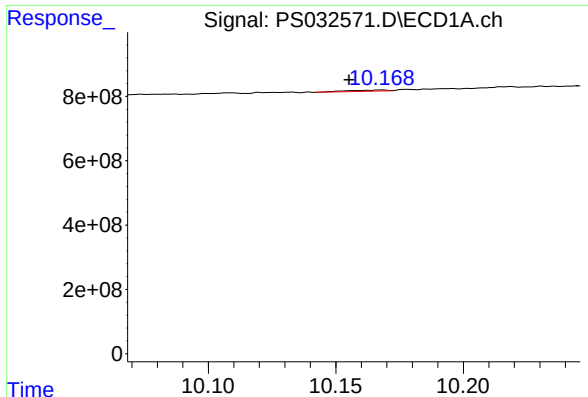

#13 2,4-DB


R.T.: 10.168 min
Delta R.T.: 0.013 min
Response: 39441082
Conc: 14.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

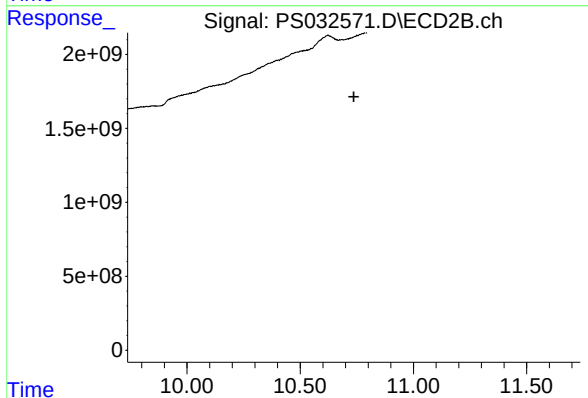


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

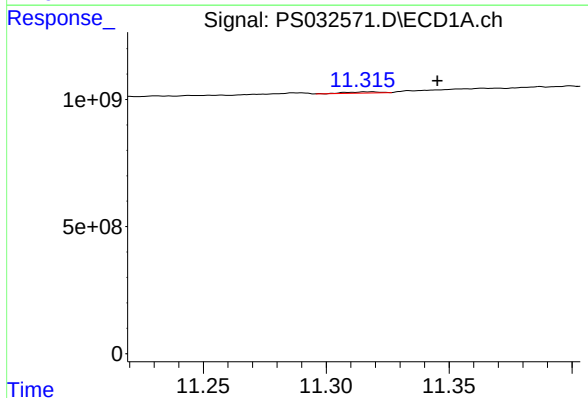


#14 DINOSEB

R.T.: 11.317 min
Delta R.T.: -0.028 min
Response: 45616205
Conc: 2.19 ng/ml

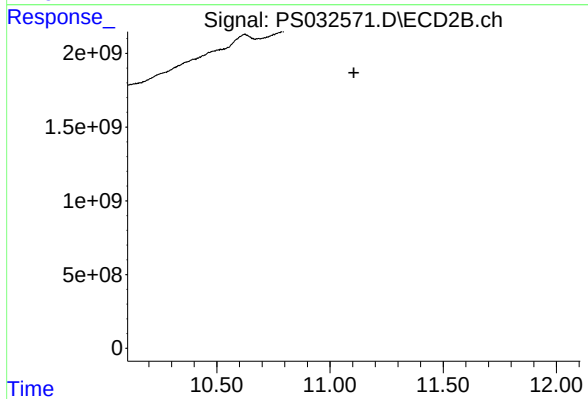

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.105 min
Response: 0
Conc: N.D.

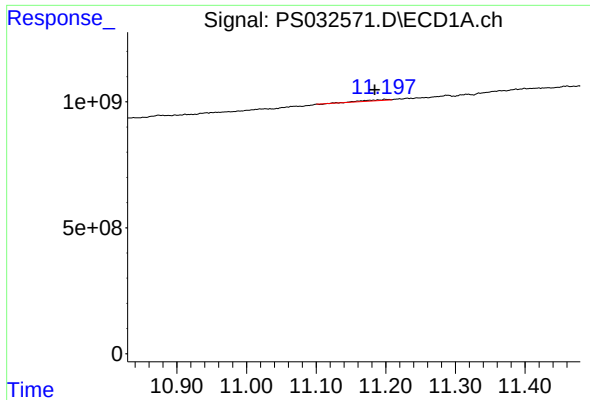

#15 Picloram


R.T.: 11.199 min
Delta R.T.: 0.015 min
Response: 85431834
Conc: 4.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

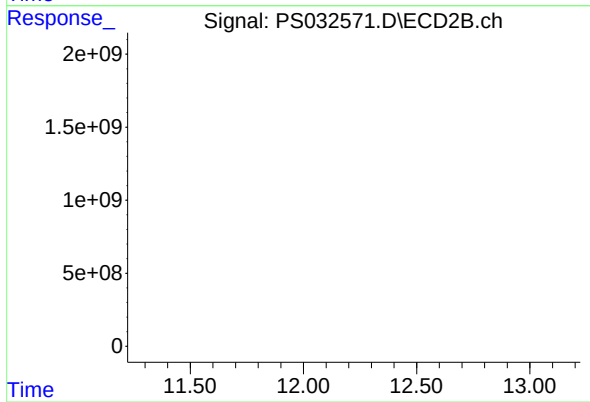


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.223 min
Response: 0
Conc: N.D.

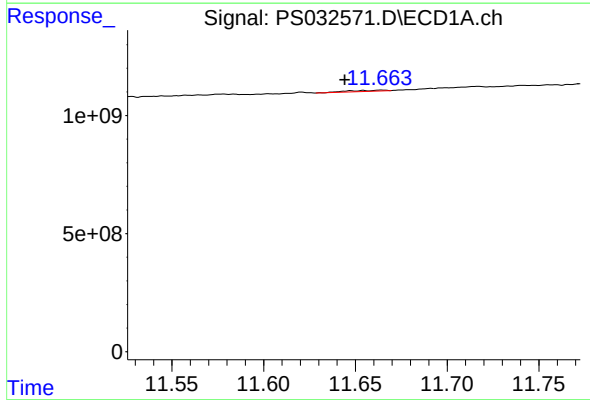

#16 DCPA

R.T.: 11.664 min
Delta R.T.: 0.020 min
Response: 63516901
Conc: 1.89 ng/ml

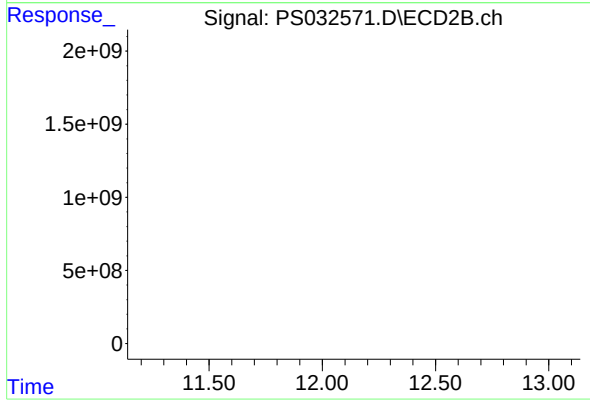

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.140 min
Response: 0
Conc: N.D.