

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 19:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:06:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	0.000	40121472	0	8.854	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.449	0.000	7363885	0	1.139	N.D. #
3) T	4-Nitroph...	7.082	7.226f	18170765	48385345	13.535	21.316 #
5) T	DICAMBA	7.458	0.000	16051603	0	<MDL	N.D. #
6) T	MCP	7.644	7.898	21765088	19297505	1.999	1.451 #
7) T	MCPA	7.784	0.000	75869964	0	5.651	N.D. #
8) T	DICHLORPROP	8.165	8.520	37425867	1202.3E6	8.413	252.103 #
10) T	Pentachlo...	8.711	9.371	36677511	380.2E6	<MDL	6.477 #
11) T	2,4,5-TP ...	9.274	0.000	78296412	0	3.010	N.D. #
12) T	2,4,5-T	9.581	0.000	8436891	0	<MDL	N.D. #
13) T	2,4-DB	10.163	0.000	33872181	0	12.854	N.D. #
14) T	DINOSEB	11.336	0.000	37918273	0	1.822	N.D. #
15) T	Picloram	11.191	0.000	140.2E6	0	6.603	N.D. #
16) T	DCPA	11.621	0.000	26222029	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 19:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:06:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

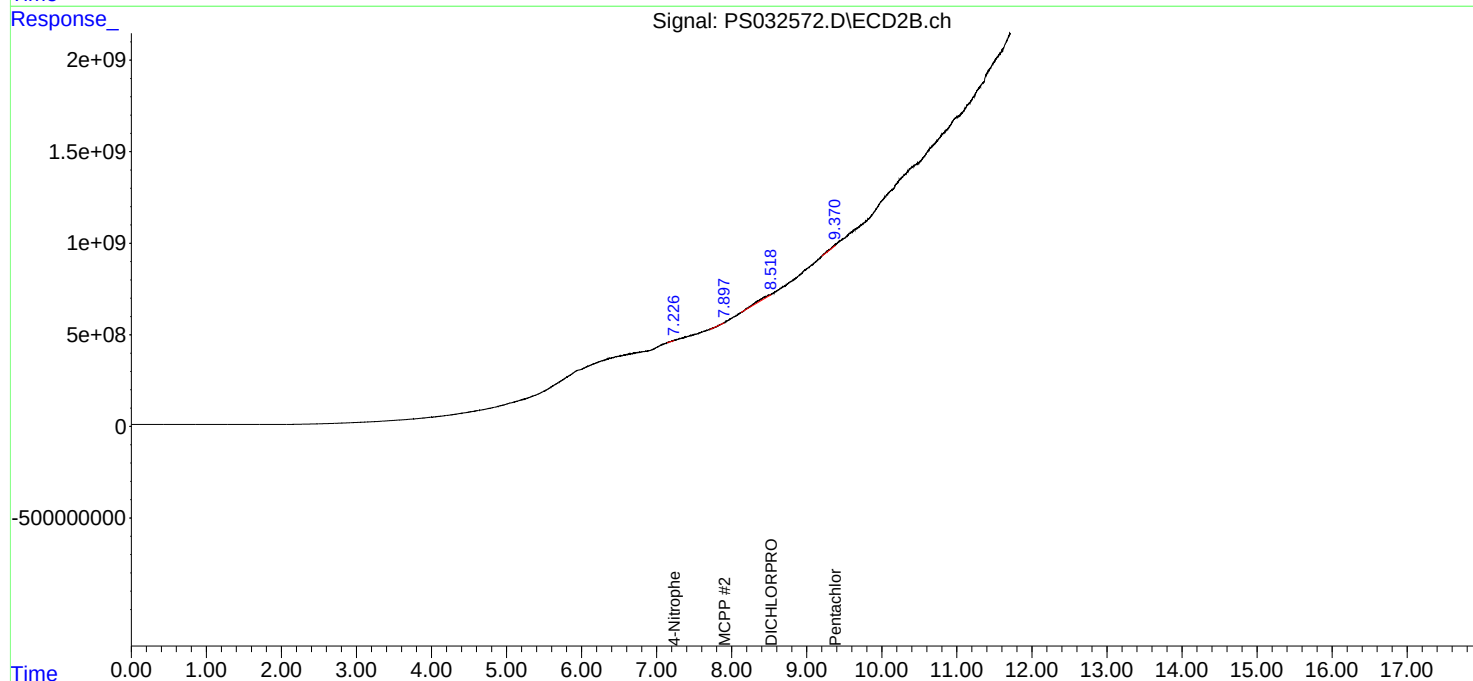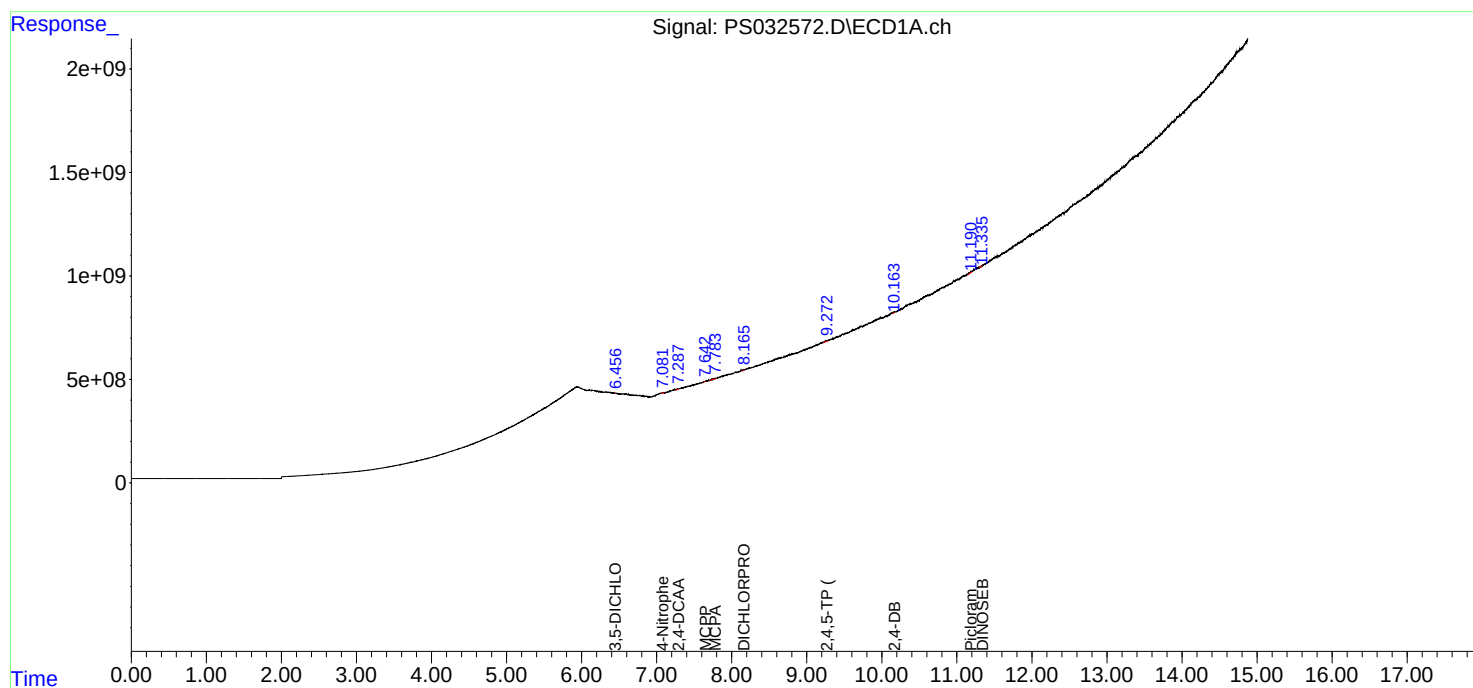


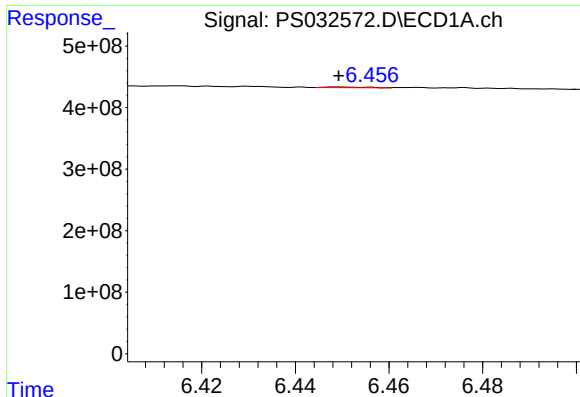

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.449 min
Delta R.T.: 0.000 min
Response: 7363885
Conc: 1.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

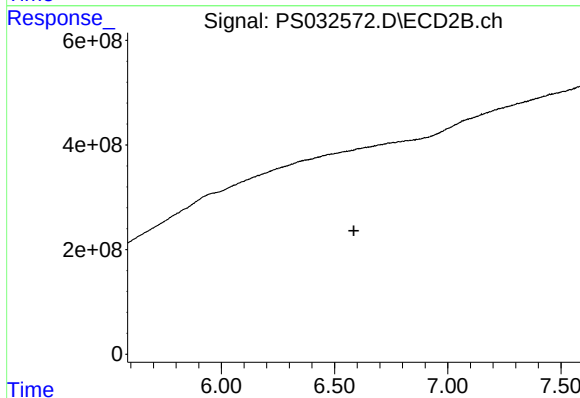


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

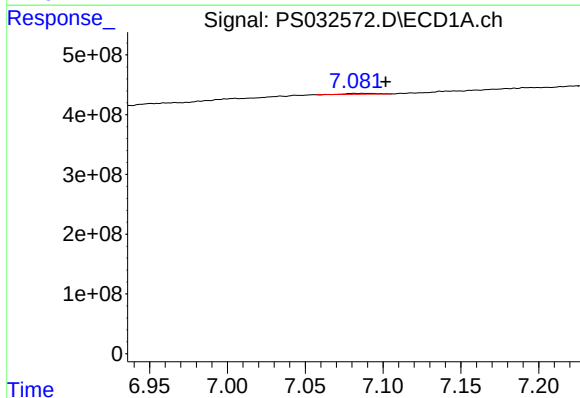


#3 4-Nitrophenol

R.T.: 7.082 min
Delta R.T.: -0.020 min
Response: 18170765
Conc: 13.54 ng/ml

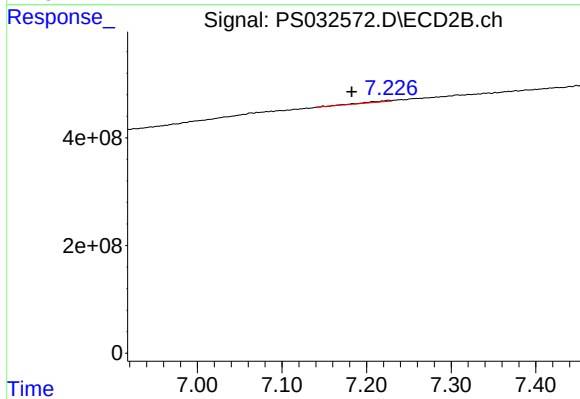

#3 4-Nitrophenol


R.T.: 7.226 min
Delta R.T.: 0.044 min
Response: 48385345
Conc: 21.32 ng/ml

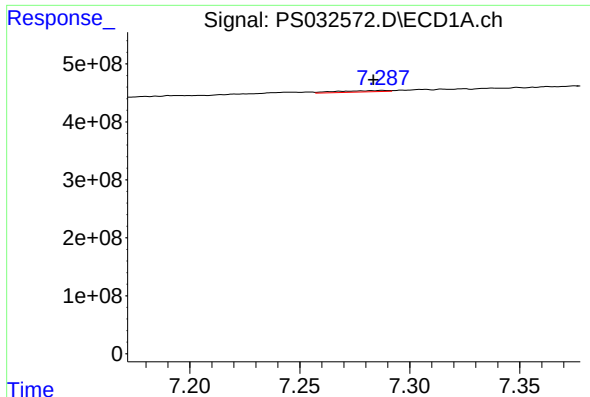

#4 2,4-DCAA


R.T.: 7.288 min
Delta R.T.: 0.004 min
Response: 40121472
Conc: 8.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

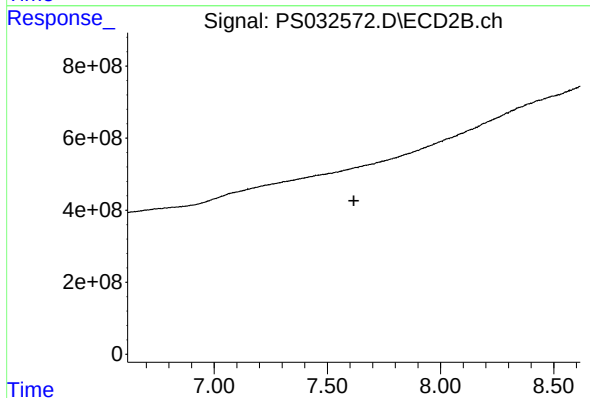


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

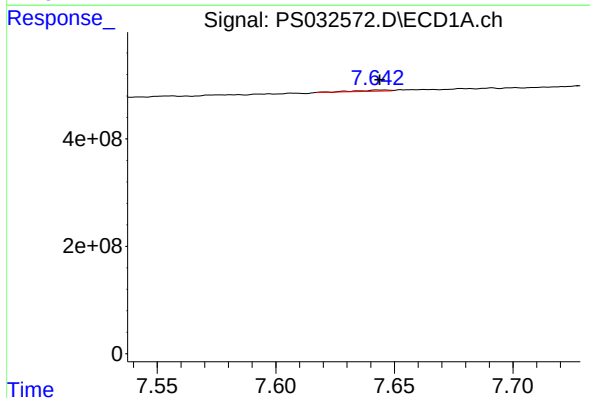


#6 MCP

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 21765088
Conc: 2.00 ug/ml

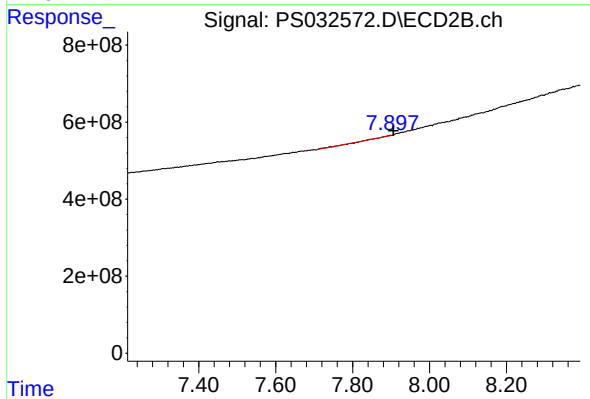

#6 MCP


R.T.: 7.898 min
Delta R.T.: -0.008 min
Response: 19297505
Conc: 1.45 ug/ml

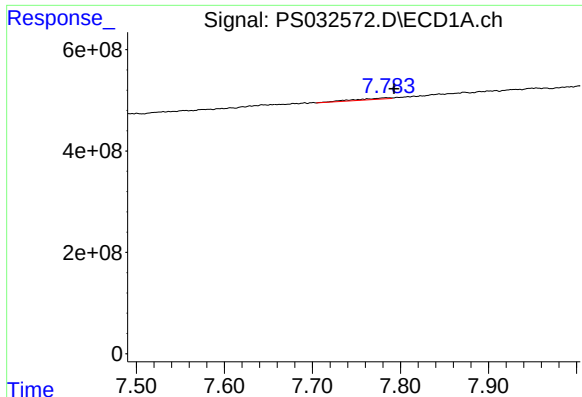

#7 MCPA


R.T.: 7.784 min
Delta R.T.: -0.009 min
Response: 75869964
Conc: 5.65 ug/ml

Instrument :
ECD_S
ClientSampleId :

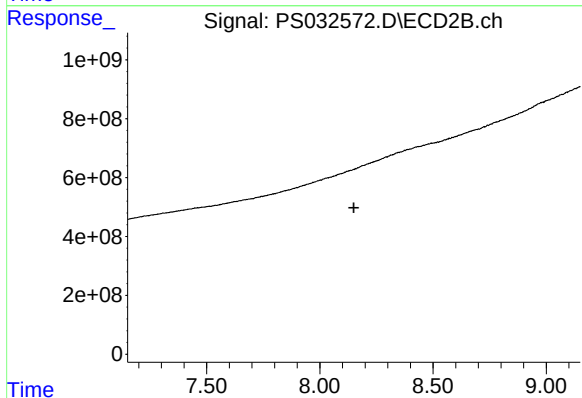


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

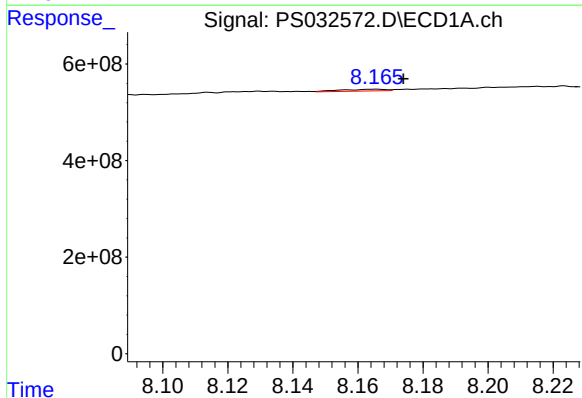


#8 DICHLORPROP

R.T.: 8.165 min
Delta R.T.: -0.009 min
Response: 37425867
Conc: 8.41 ng/ml

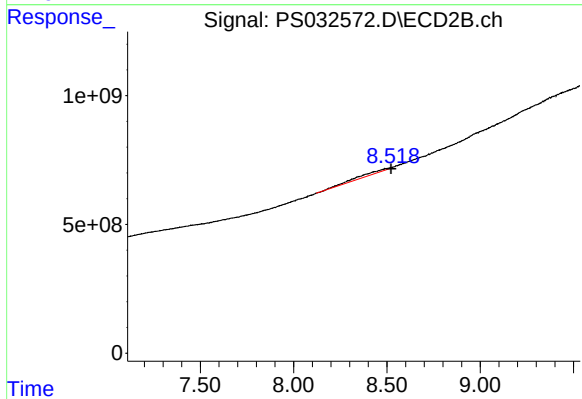

#8 DICHLORPROP


R.T.: 8.520 min
Delta R.T.: -0.001 min
Response: 1202315842
Conc: 252.10 ng/ml

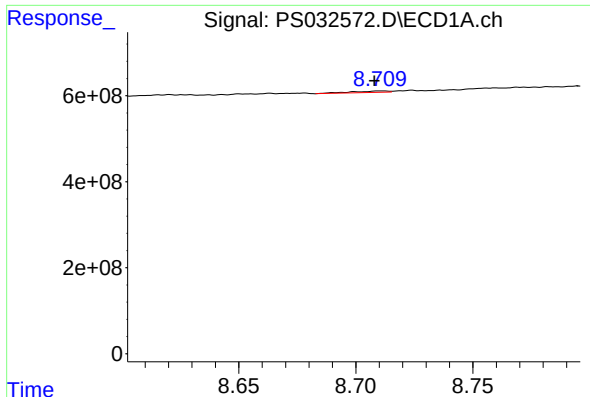

#10 Pentachlorophenol


R.T.: 8.711 min
Delta R.T.: 0.003 min
Response: 36677511
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

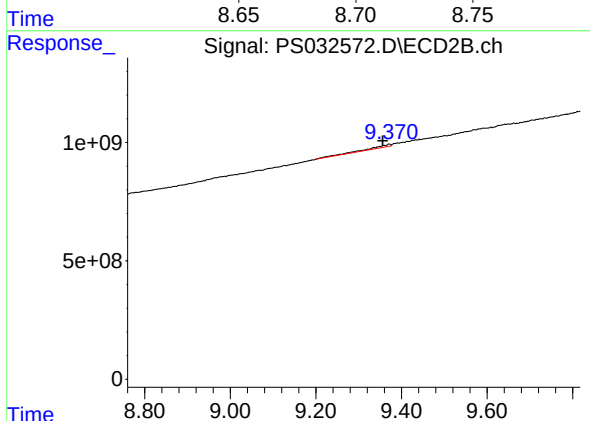


#10 Pentachlorophenol

R.T.: 9.371 min
Delta R.T.: 0.015 min
Response: 380208256
Conc: 6.48 ng/ml

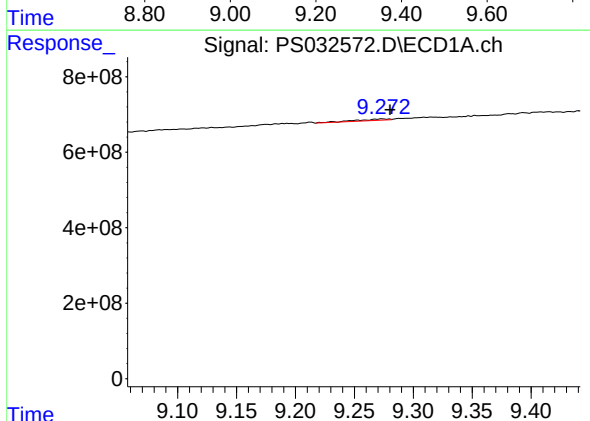


#11 2,4,5-TP (SILVEX)

R.T.: 9.274 min
Delta R.T.: -0.007 min
Response: 78296412
Conc: 3.01 ng/ml

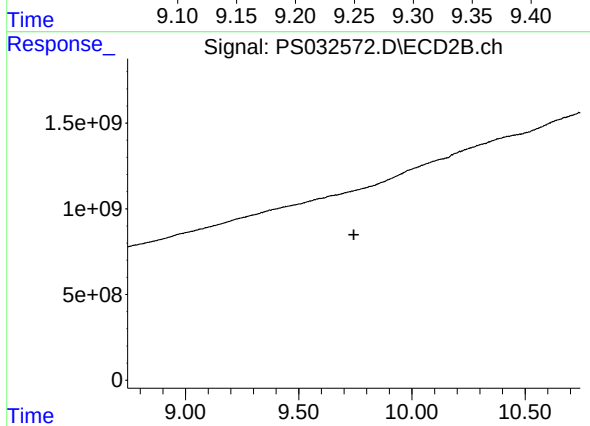

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.744 min
Response: 0
Conc: N.D.

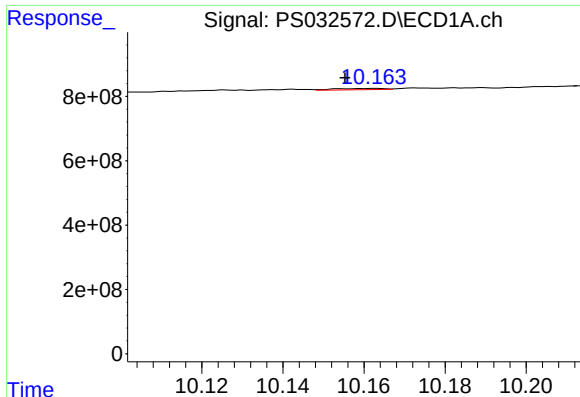

#13 2,4-DB


R.T.: 10.163 min
Delta R.T.: 0.007 min
Response: 33872181
Conc: 12.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

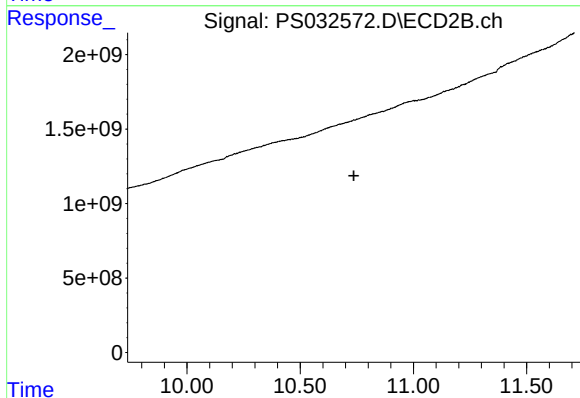


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

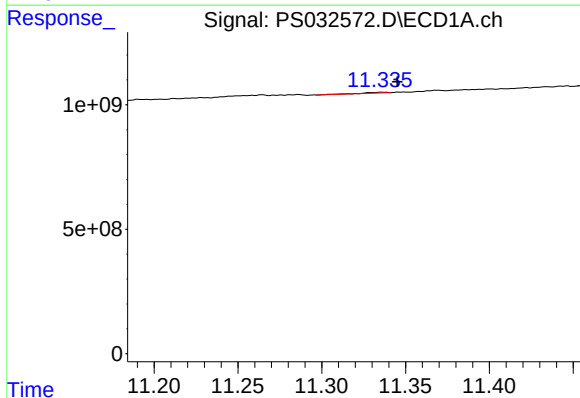


#14 DINOSEB

R.T.: 11.336 min
Delta R.T.: -0.009 min
Response: 37918273
Conc: 1.82 ng/ml

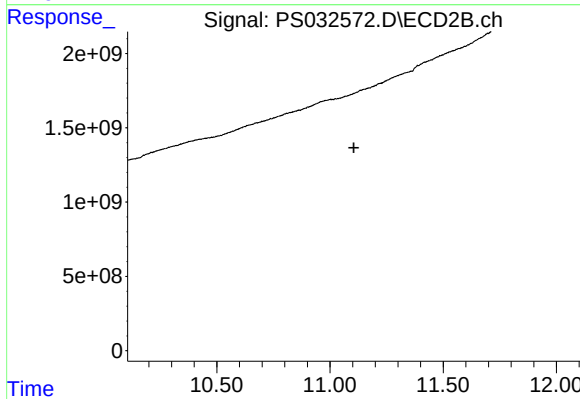

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.105 min
Response: 0
Conc: N.D.

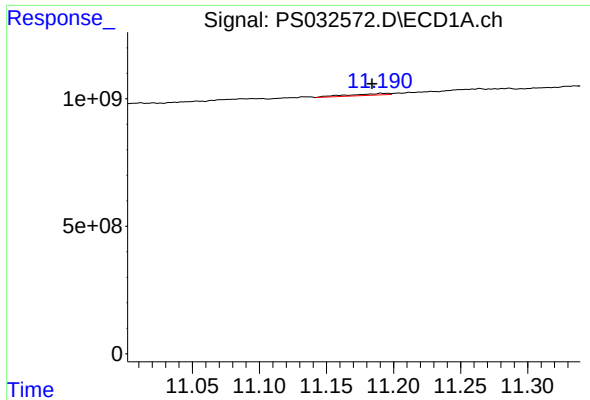

#15 Picloram

R.T.: 11.191 min
Delta R.T.: 0.007 min
Response: 140153109
Conc: 6.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

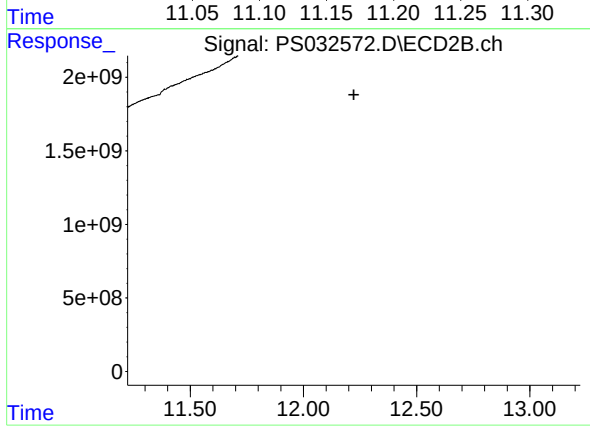

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.223 min
Response: 0
Conc: N.D.