

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
 Data File : PS032573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 19:57
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:06:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.254f	0.000	123.2E6	0	27.195	N.D. #
Target Compounds							
1) T	Dalapon	2.638	2.609	1671.9E6	2711.6E6	232.902	389.935 #
2) T	3,5-DICHL...	6.439	0.000	12786531	0	1.977	N.D. #
3) T	4-Nitroph...	7.089	7.205	8615049	52438565	6.417	23.101 #
5) T	DICAMBA	7.460	0.000	3780699	0	<MDL	N.D. #
6) T	MCPD	7.626	0.000	3129970	0	<MDL	N.D. #
7) T	MCPA	7.788	0.000	48382502	0	3.604	N.D. #
8) T	DICHLORPROP	8.199	0.000	53814801	0	12.097	N.D. #
9) T	2,4-D	8.410	0.000	30386098	0	6.735	N.D. #
11) T	2,4,5-TP ...	9.300	0.000	322.8E6	0	12.408	N.D. #
13) T	2,4-DB	10.149	0.000	125.6E6	0	47.652	N.D. #
14) T	DINOSEB	11.331	0.000	10555203	0	<MDL	N.D. #
16) T	DCPA	11.649	0.000	107.0E6	0	3.188	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120125\
Data File : PS032573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 19:57
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:06:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

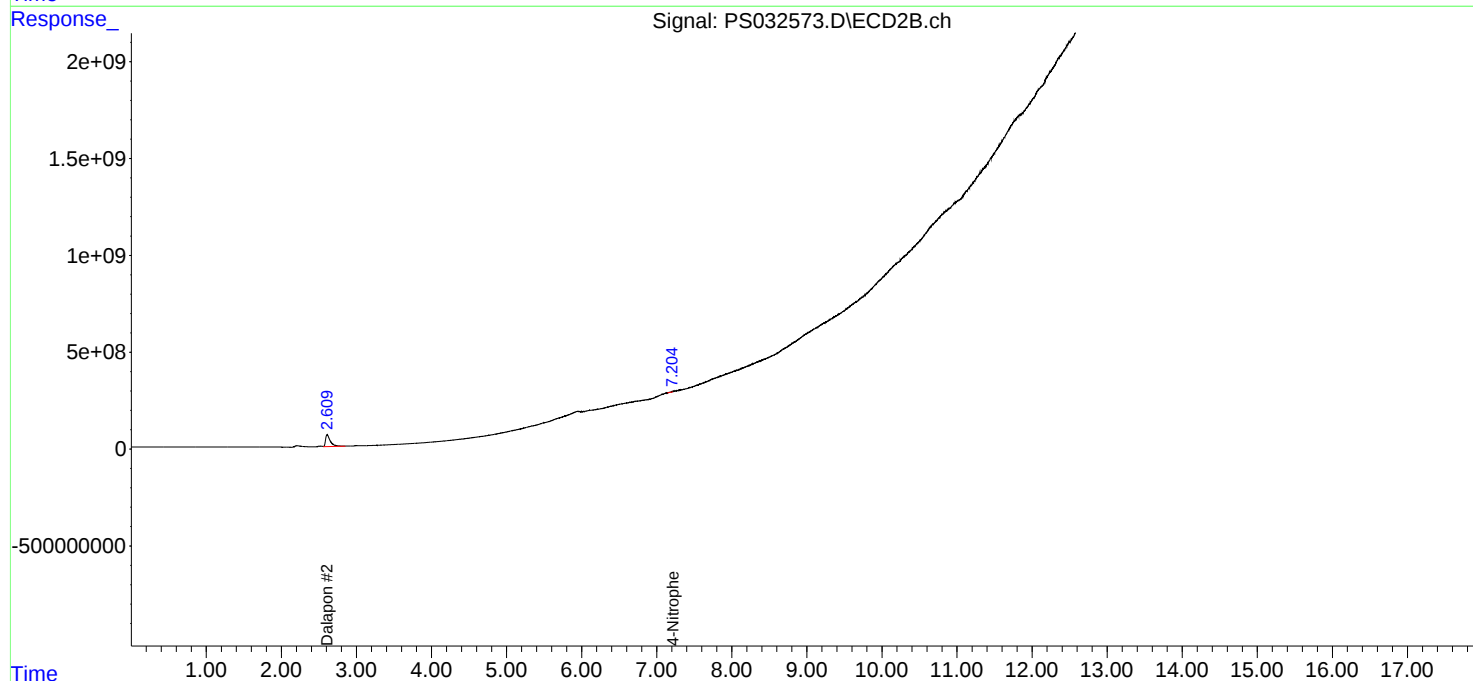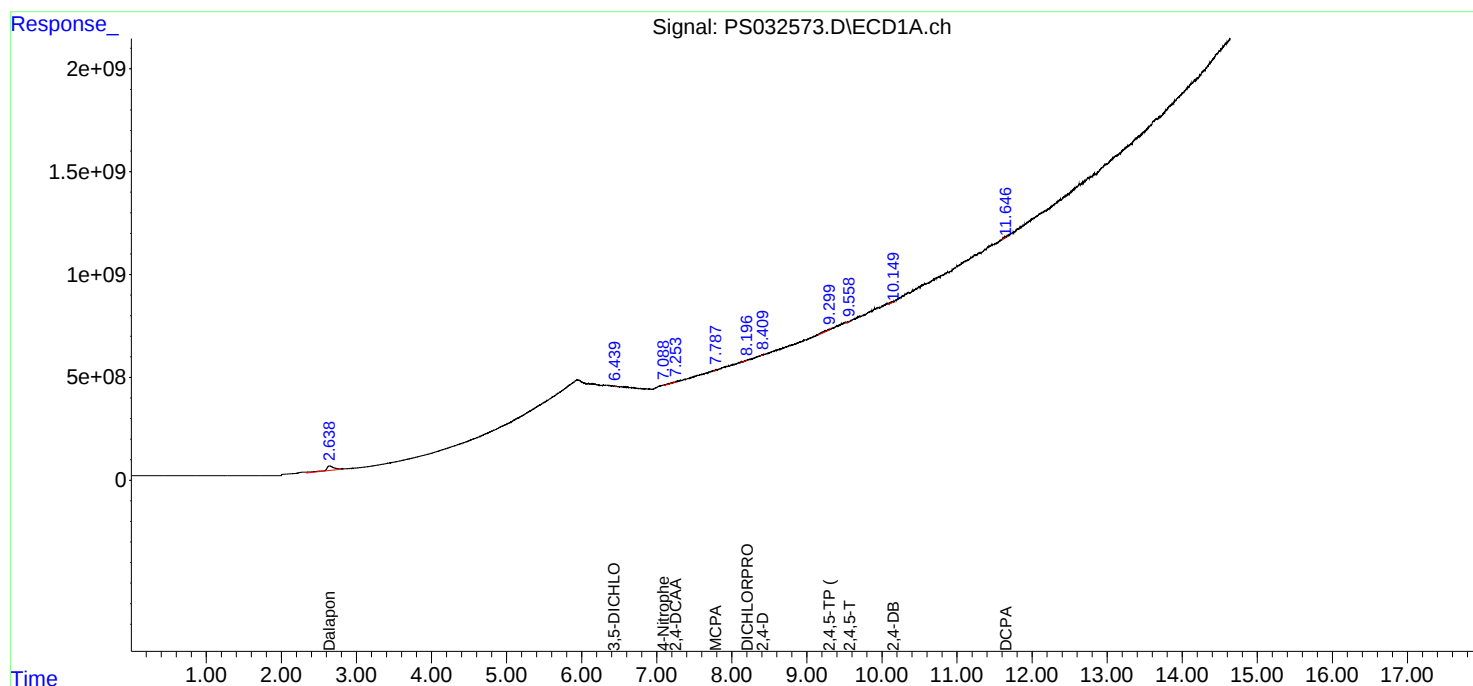


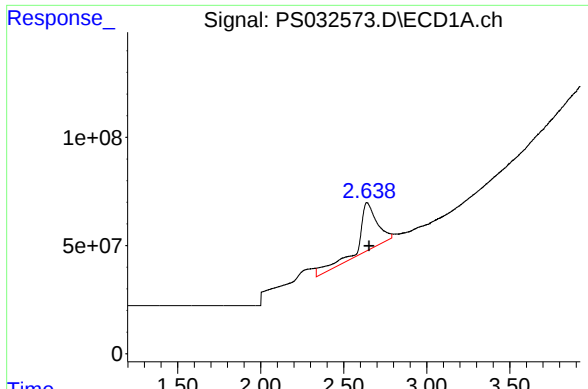

#1 Dalapon


R.T.: 2.638 min
Delta R.T.: -0.016 min
Response: 1671948066
Conc: 232.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

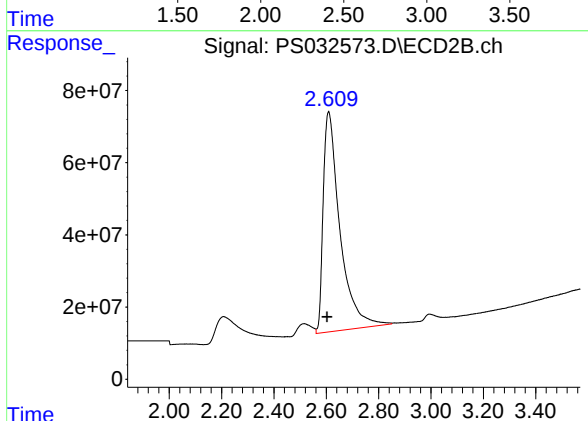


#1 Dalapon

R.T.: 2.609 min
Delta R.T.: 0.006 min
Response: 2711609407
Conc: 389.94 ng/ml

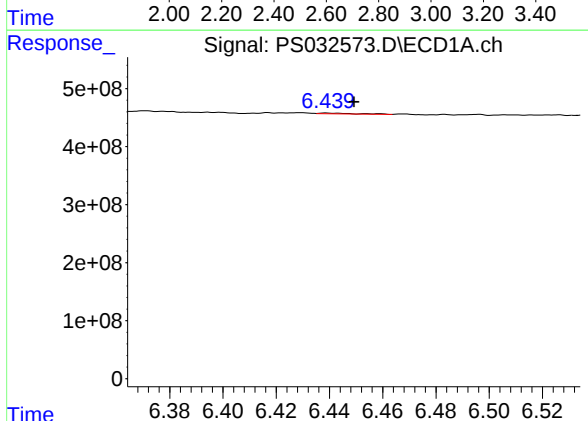


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.439 min
Delta R.T.: -0.010 min
Response: 12786531
Conc: 1.98 ng/ml

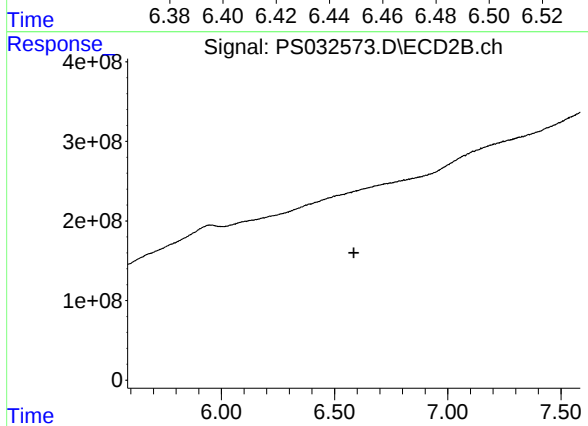

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

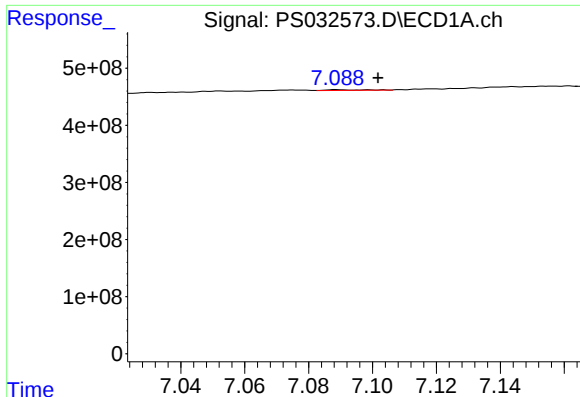

#3 4-Nitrophenol


R.T.: 7.089 min
Delta R.T.: -0.013 min
Response: 8615049
Conc: 6.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

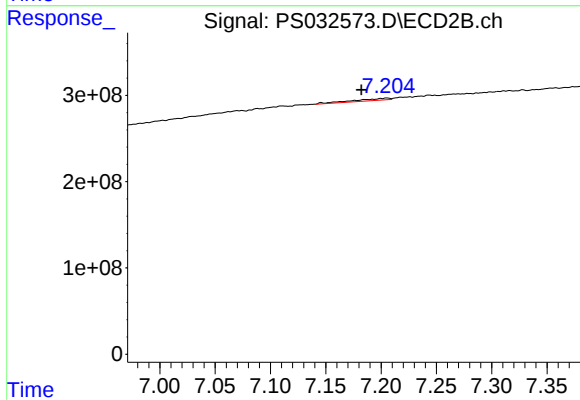


#3 4-Nitrophenol

R.T.: 7.205 min
Delta R.T.: 0.023 min
Response: 52438565
Conc: 23.10 ng/ml

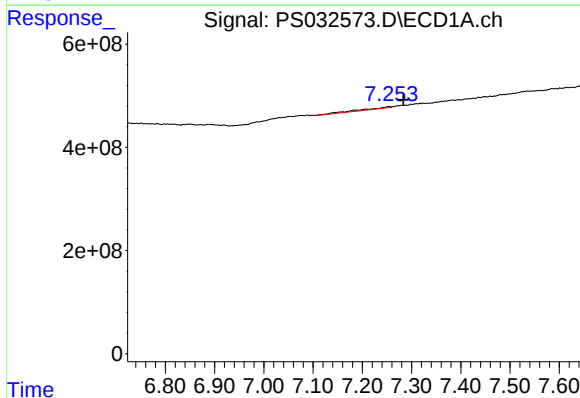


#4 2,4-DCAA

R.T.: 7.254 min
Delta R.T.: -0.030 min
Response: 123227296
Conc: 27.19 ng/ml

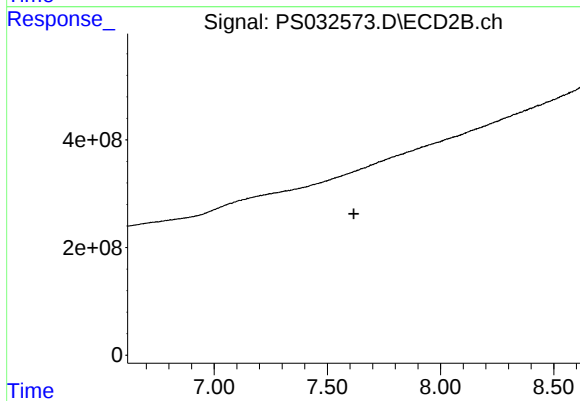

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

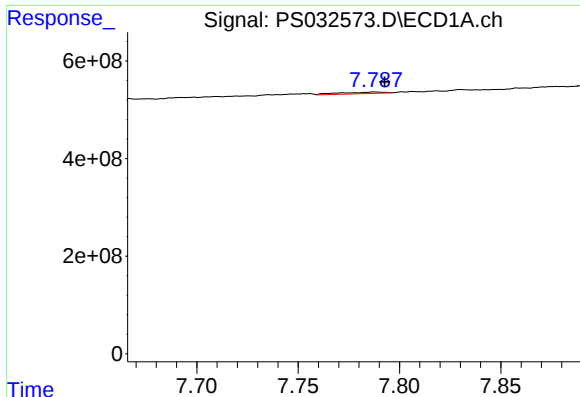

#7 MCPA


R.T.: 7.788 min
Delta R.T.: -0.005 min
Response: 48382502
Conc: 3.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

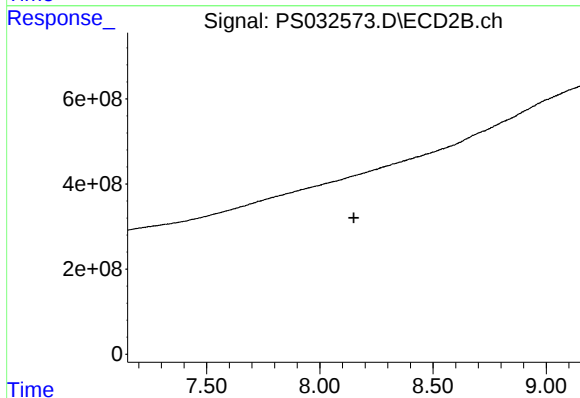


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

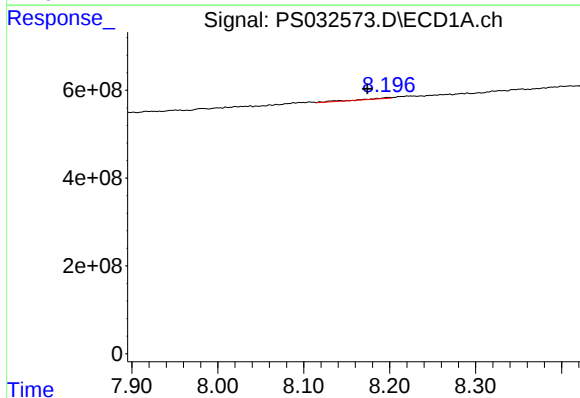


#8 DICHLORPROP

R.T.: 8.199 min
Delta R.T.: 0.025 min
Response: 53814801
Conc: 12.10 ng/ml

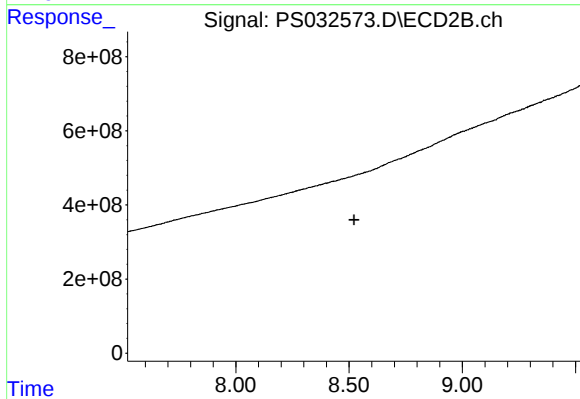

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.522 min
Response: 0
Conc: N.D.

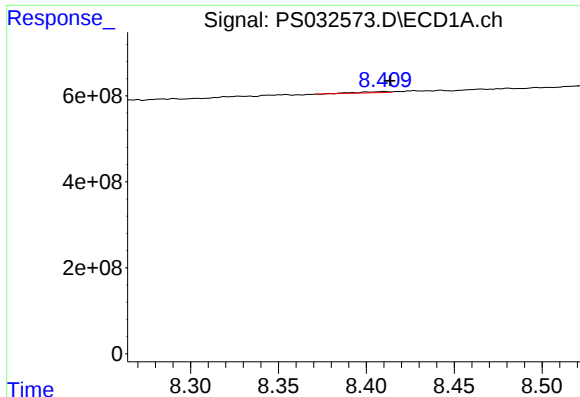

#9 2,4-D


R.T.: 8.410 min
Delta R.T.: -0.004 min
Response: 30386098
Conc: 6.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

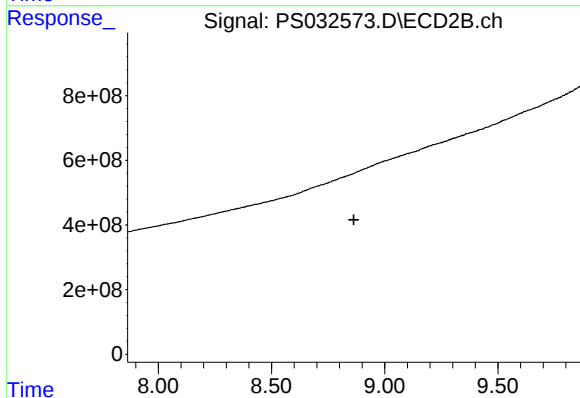


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.

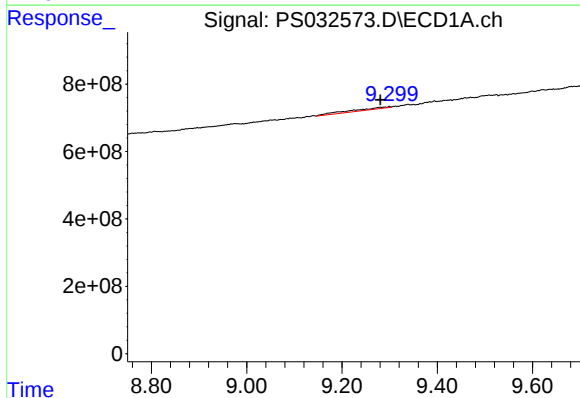


#11 2,4,5-TP (SILVEX)

R.T.: 9.300 min
Delta R.T.: 0.019 min
Response: 322762151
Conc: 12.41 ng/ml

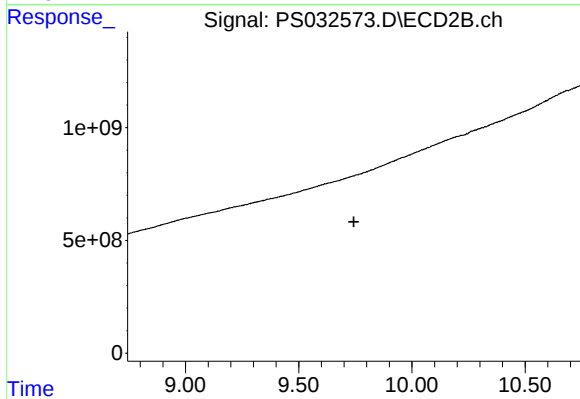

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.744 min
Response: 0
Conc: N.D.

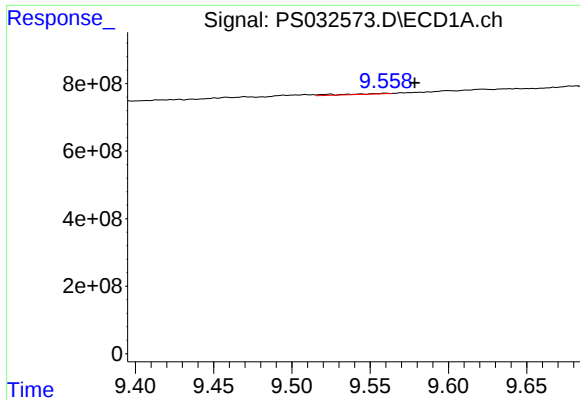

#12 2,4,5-T


R.T.: 9.560 min
Delta R.T.: -0.019 min
Response: 33701280
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

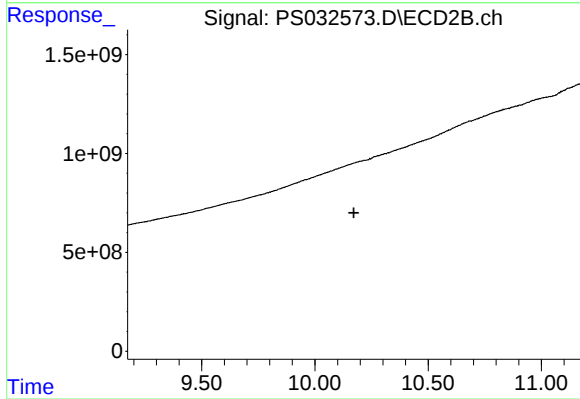


#12 2,4,5-T

R.T.: 10.217 min
Delta R.T.: 0.045 min
Response: -10181923424
Conc: N.D.

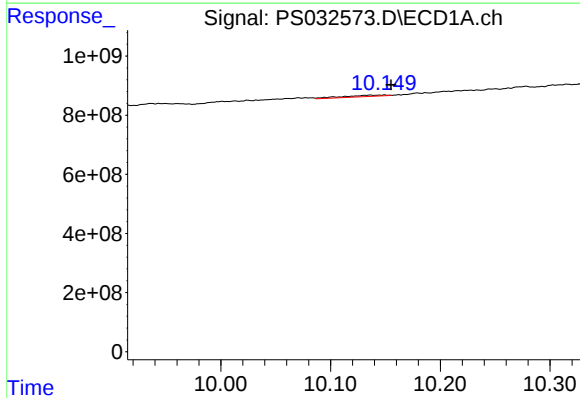


#13 2,4-DB

R.T.: 10.149 min
Delta R.T.: -0.006 min
Response: 125568334
Conc: 47.65 ng/ml

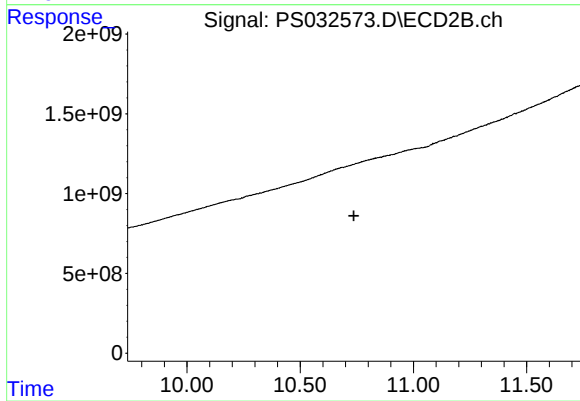

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.737 min
Response: 0
Conc: N.D.

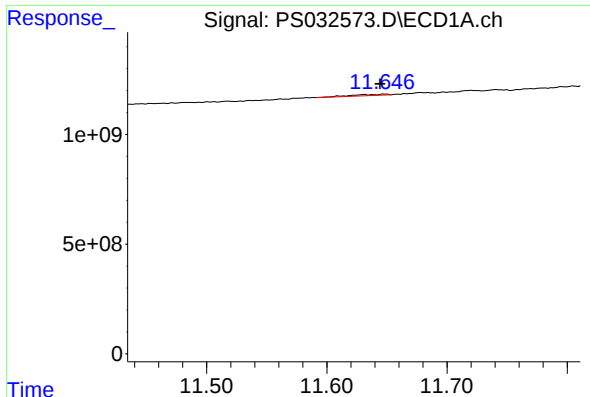

#16 DCPA

R.T.: 11.649 min
Delta R.T.: 0.004 min
Response: 106961310
Conc: 3.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

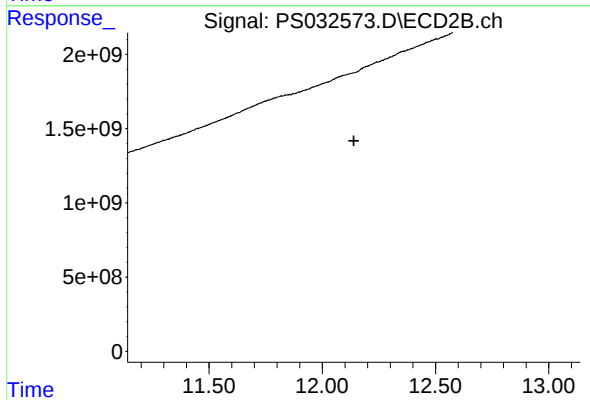

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.140 min
Response: 0
Conc: N.D.