

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
 Data File : PS018079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 08:29
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:17:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.316	0.000	26583323	0	12.357	N.D.	#
5) T	DICAMBA	0.000	6.849f	0	13837226	N.D.	5.263	
6) T	MCP	0.000	6.849	0	13837226	N.D.	6.433	
7) T	MCPA	7.485f	0.000	3273788	0	<MDL	N.D.	#
9) T	2,4-D	8.200f	0.000	101.5E6	0	55.745	N.D.	#
11) T	2,4,5-TP ...	9.000	8.434f	2729047	28568295	<MDL	8.014	#
12) T	2,4,5-T	9.284	0.000	6906494	0	<MDL	N.D.	#
13) T	2,4-DB	9.827	0.000	6354779	0	3.844	N.D.	#
15) T	Picloram	10.806	10.664	123.2E6	46085087	10.322	9.855	
16) T	DCPA	11.243	10.664f	7842163	46085087	<MDL	10.437	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
Data File : PS018079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 08:29
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:17:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

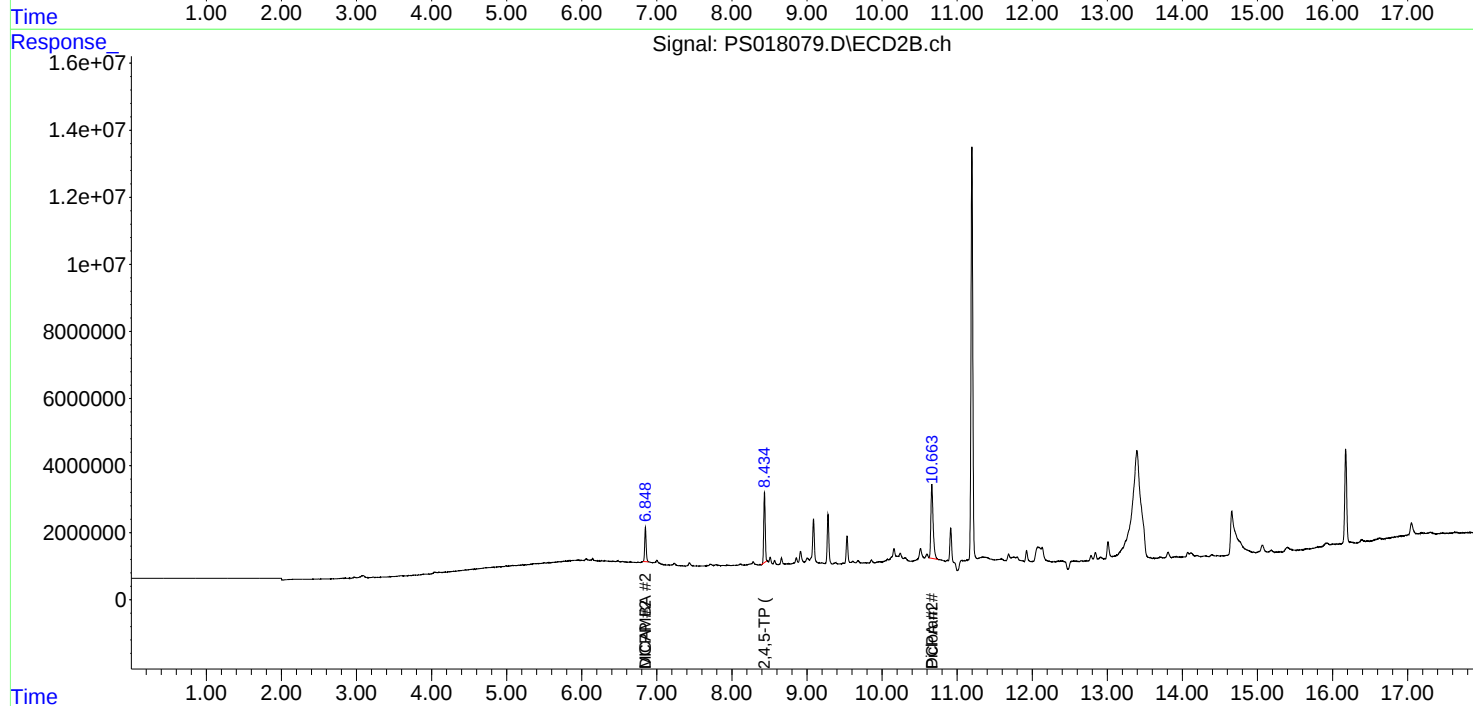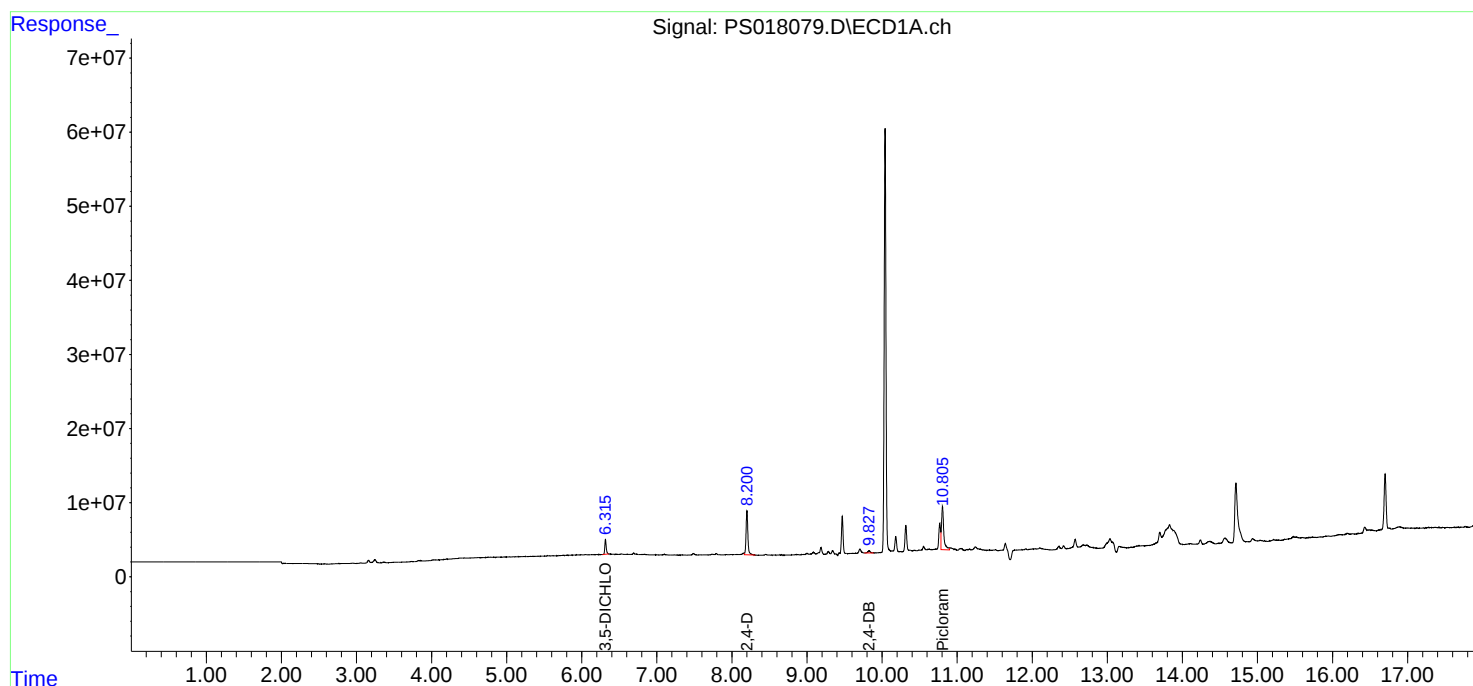


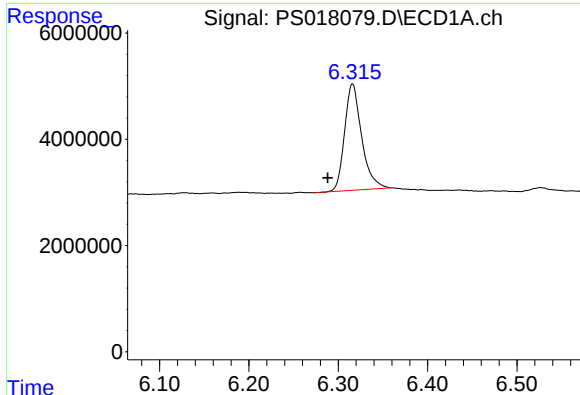

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.316 min
Delta R.T.: 0.028 min
Response: 26583323
Conc: 12.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

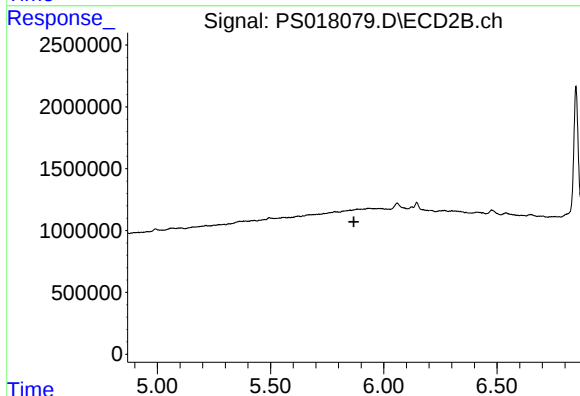


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.868 min
Response: 0
Conc: N.D.

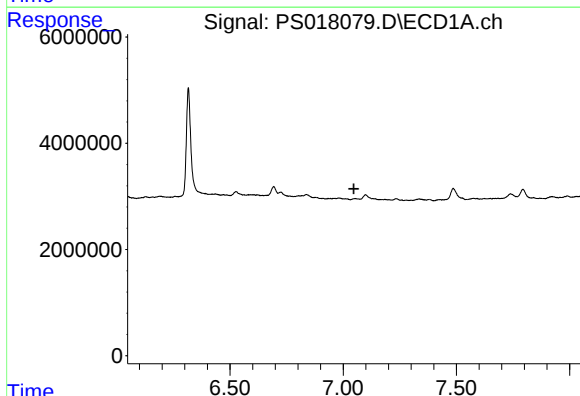


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.047 min
Response: 0
Conc: N.D.

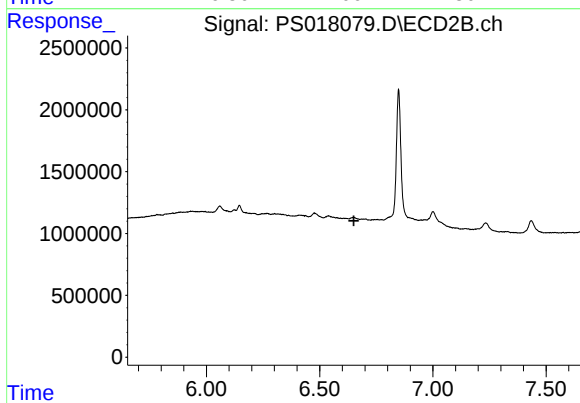

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

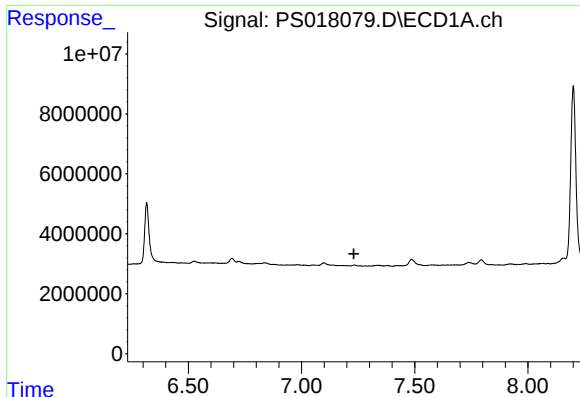

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

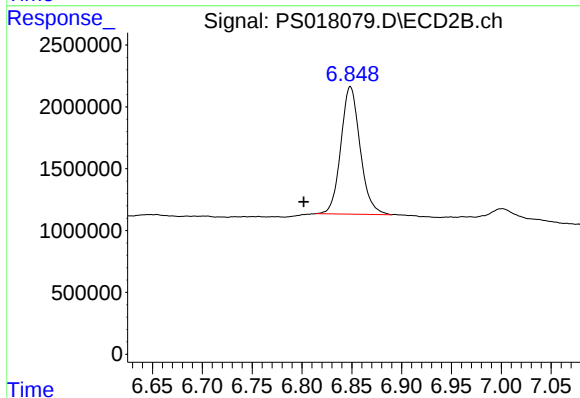


#5 DICAMBA

R.T.: 6.849 min
Delta R.T.: 0.047 min
Response: 13837226
Conc: 5.26 ng/ml

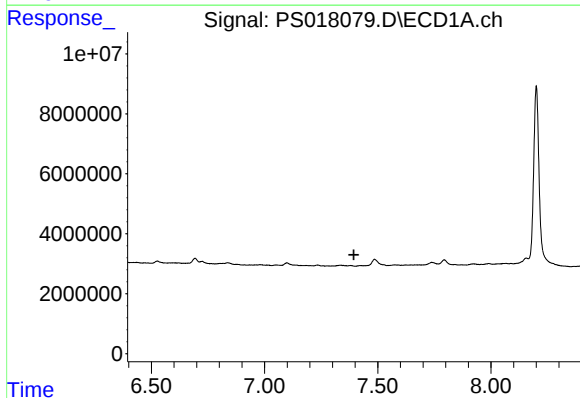


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

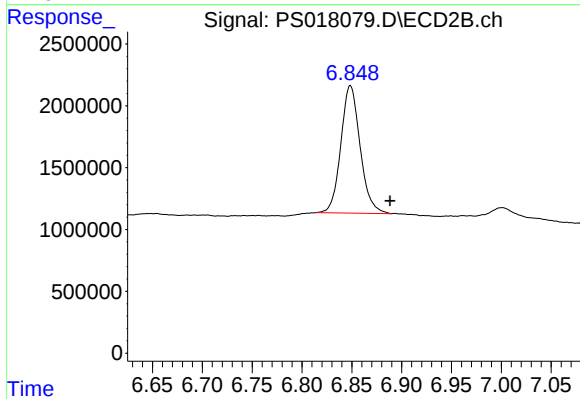

#6 MCP


R.T.: 6.849 min
Delta R.T.: -0.040 min
Response: 13837226
Conc: 6.43 ug/ml

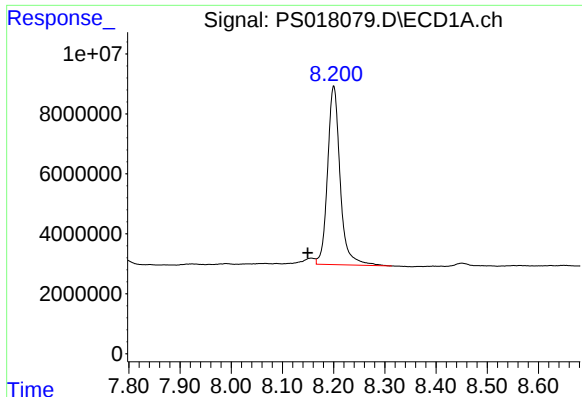

#9 2,4-D


R.T.: 8.200 min
Delta R.T.: 0.051 min
Response: 101508864
Conc: 55.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

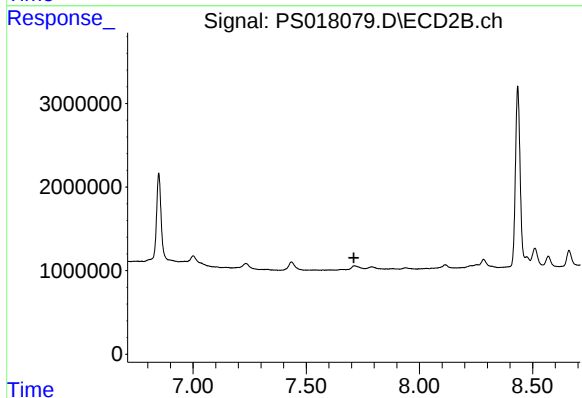


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

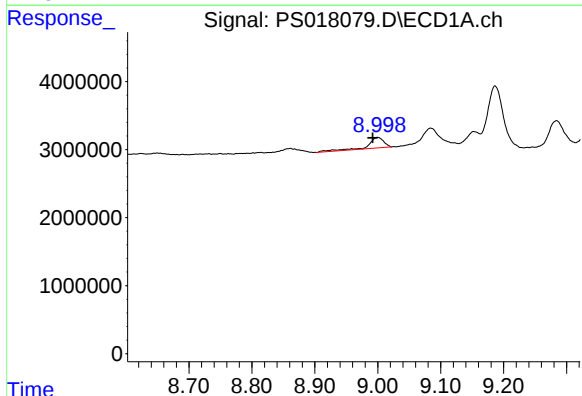


#11 2,4,5-TP (SILVEX)

R.T.: 9.000 min
Delta R.T.: 0.008 min
Response: 2729047
Conc: N.D.

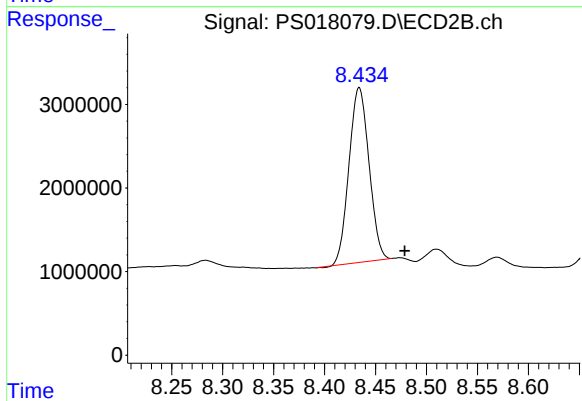

#11 2,4,5-TP (SILVEX)


R.T.: 8.434 min
Delta R.T.: -0.045 min
Response: 28568295
Conc: 8.01 ng/ml

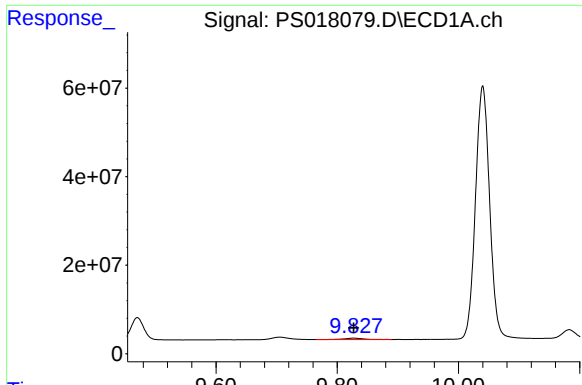

#13 2,4-DB


R.T.: 9.827 min
Delta R.T.: 0.000 min
Response: 6354779
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

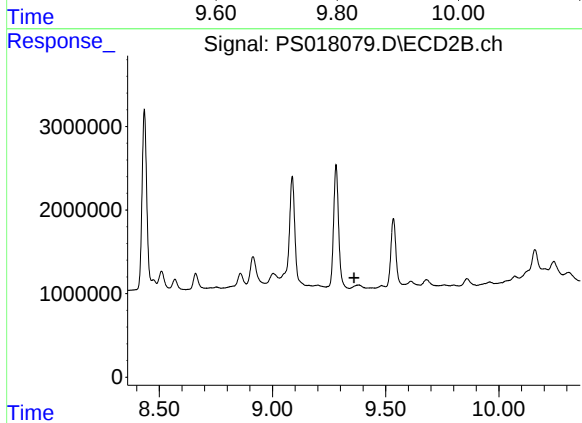


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

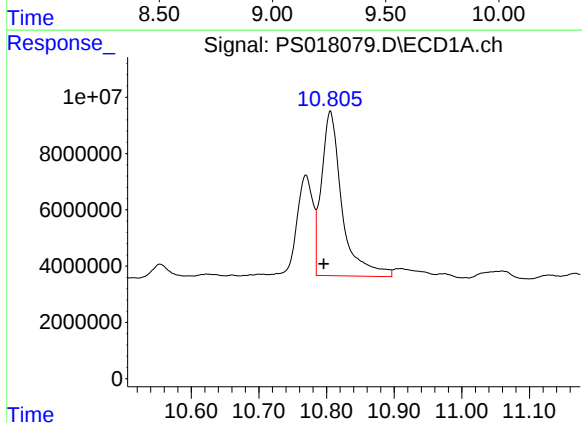


#15 Picloram

R.T.: 10.806 min
Delta R.T.: 0.010 min
Response: 123198963
Conc: 10.32 ng/ml

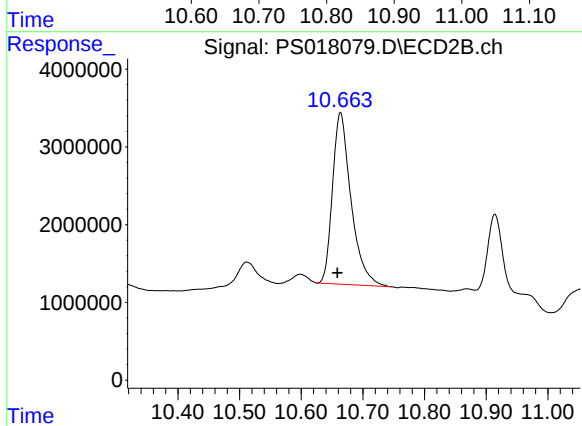

#15 Picloram


R.T.: 10.664 min
Delta R.T.: 0.005 min
Response: 46085087
Conc: 9.86 ng/ml

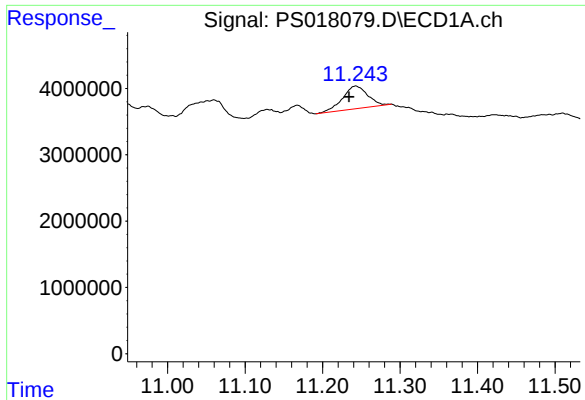

#16 DCPA

R.T.: 11.243 min
Delta R.T.: 0.008 min
Response: 7842163
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

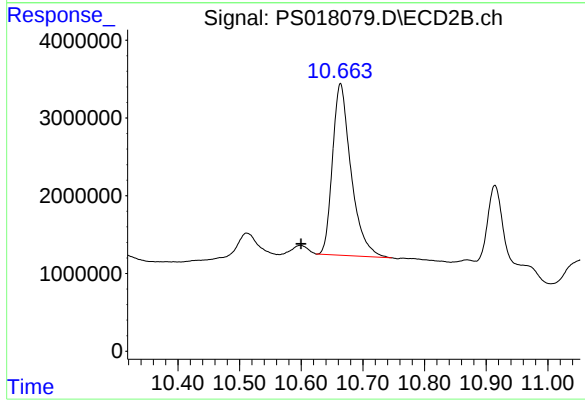

#16 DCPA

R.T.: 10.664 min
Delta R.T.: 0.064 min
Response: 46085087
Conc: 10.44 ng/ml