

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
 Data File : PS018086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 12:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc : FOR ABDUL RAUF
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:20:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.049	6.646	648.6E6	313.0E6	448.693	539.470
Target Compounds							
9) T	2,4-D	8.179	0.000	38433494	0	21.106	N.D. #
11) T	2,4,5-TP ...	0.000	8.444	0	13938319	N.D.	3.910
15) T	Picloram	10.784	10.685	7834693	40992011	<MDL	8.766 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
Data File : PS018086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 12:25
Operator : AJ\MA
Sample : I.BLK
Misc : FOR ABDUL RAUF
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:20:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

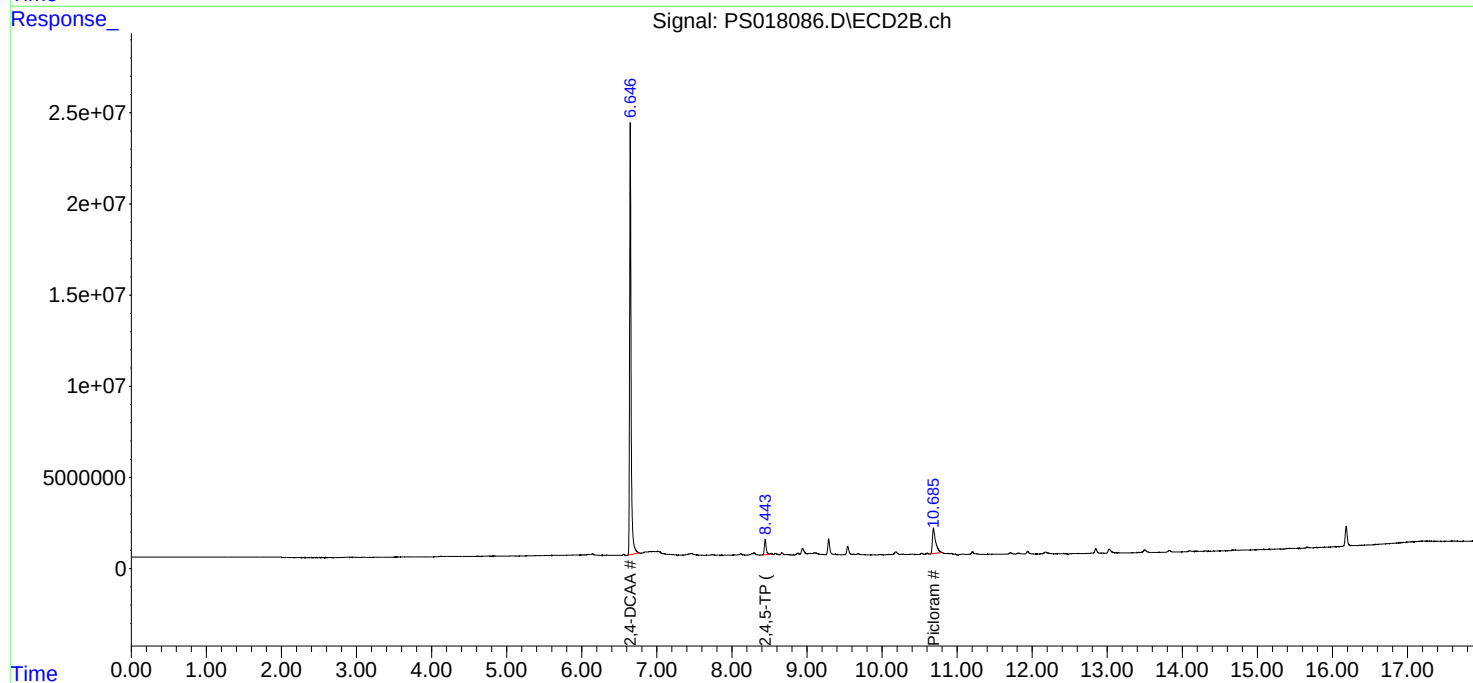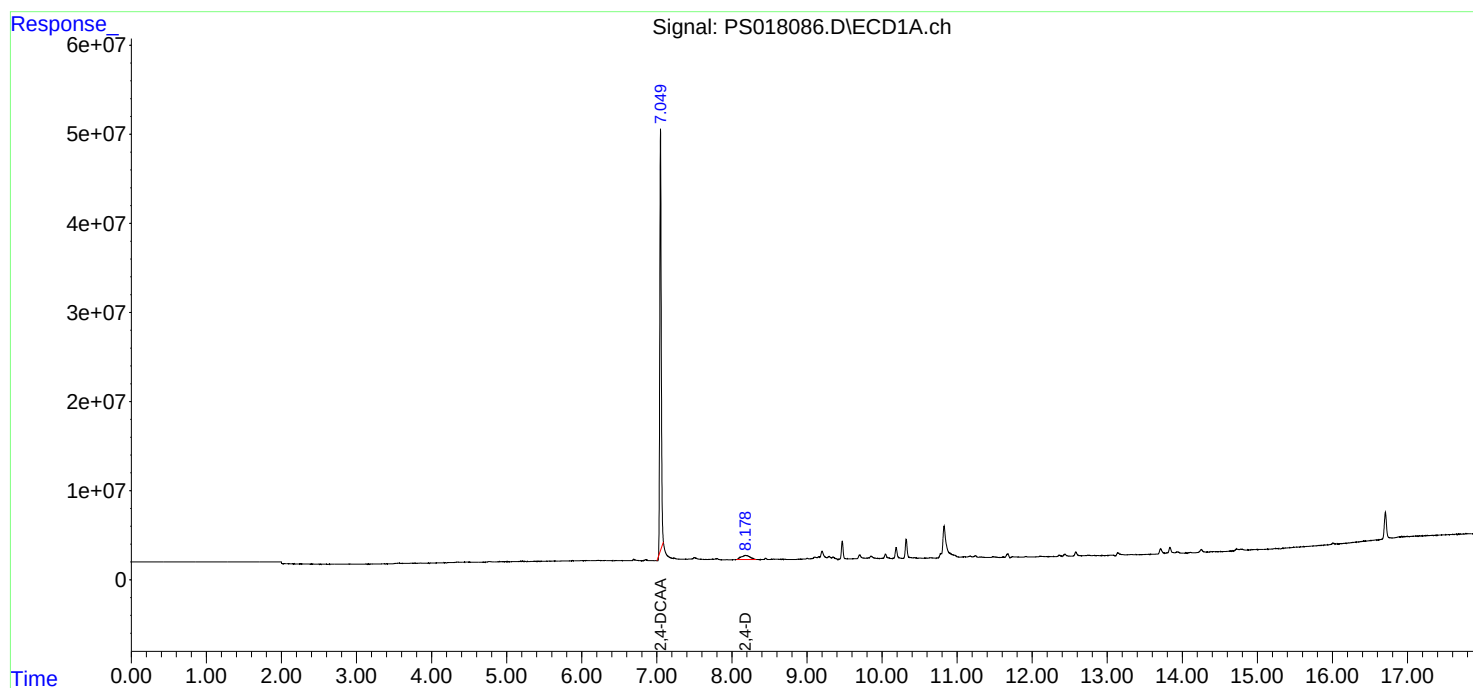


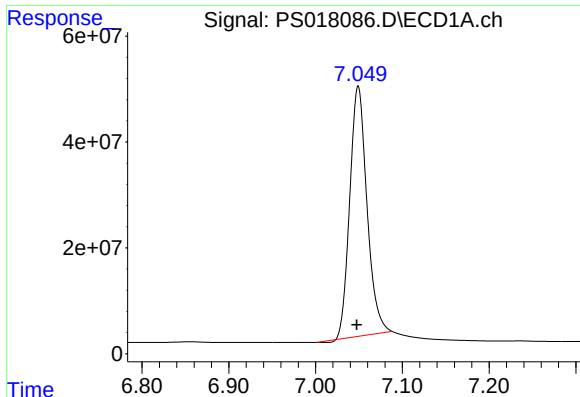

#4 2,4-DCAA


R.T.: 7.049 min
Delta R.T.: 0.002 min
Response: 648579805
Conc: 448.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

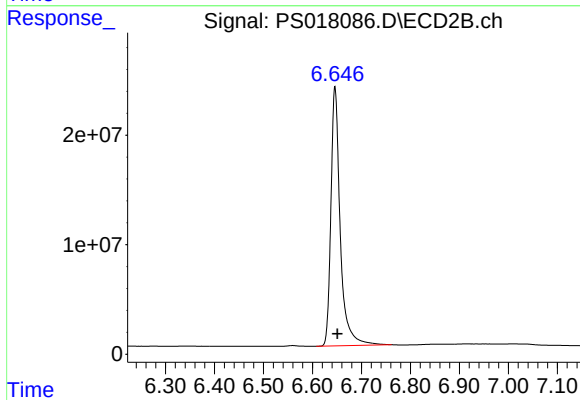


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 313026762
Conc: 539.47 ng/ml

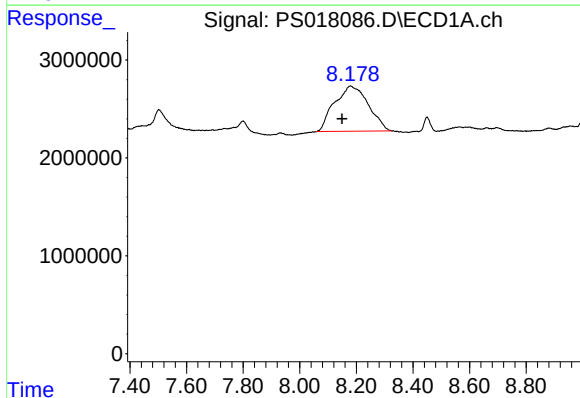


#9 2,4-D

R.T.: 8.179 min
Delta R.T.: 0.030 min
Response: 38433494
Conc: 21.11 ng/ml

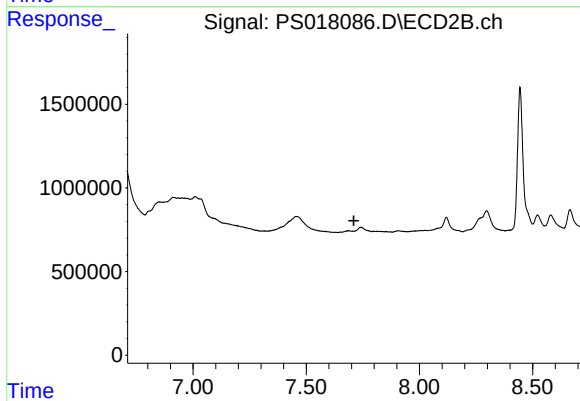

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

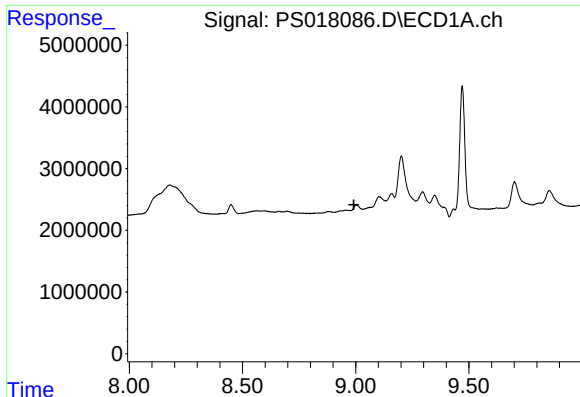

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

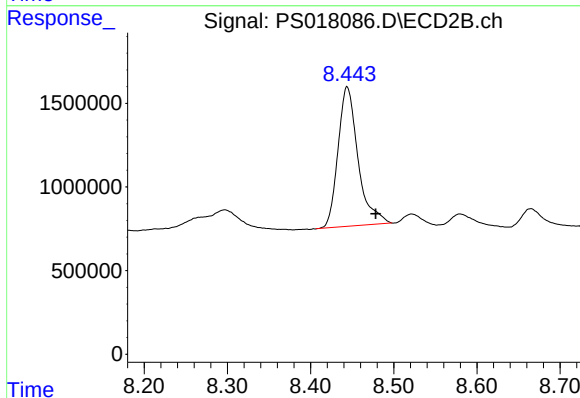


#11 2,4,5-TP (SILVEX)

R.T.: 8.444 min
Delta R.T.: -0.035 min
Response: 13938319
Conc: 3.91 ng/ml

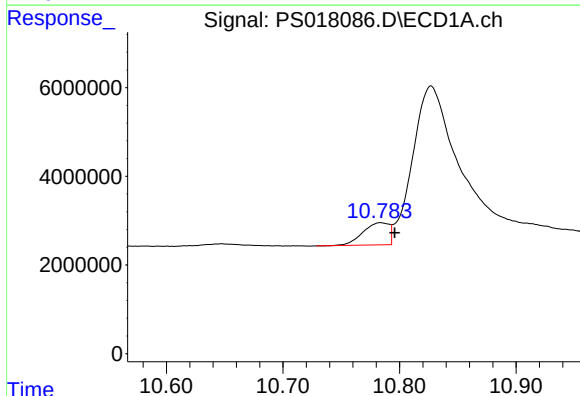

#15 Picloram

R.T.: 10.784 min
Delta R.T.: -0.012 min
Response: 7834693
Conc: N.D.

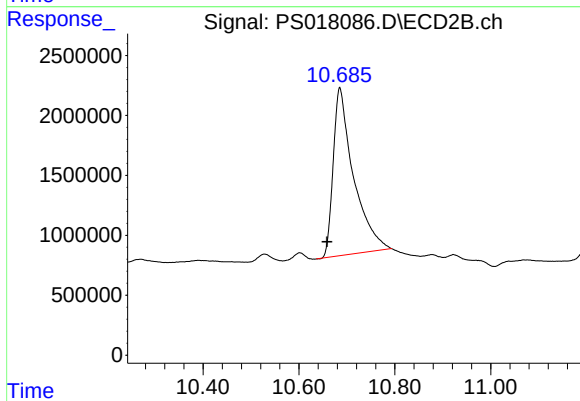

#15 Picloram

R.T.: 10.685 min
Delta R.T.: 0.026 min
Response: 40992011
Conc: 8.77 ng/ml