

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
 Data File : PS018087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 12:52
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc : FOR ABDUL RAUF
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:21:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.047	6.646	1028.0E6	410.7E6	711.188	707.801
Target Compounds							
1) T	Dalapon	2.908	2.419	1496.6E6	458.1E6	610.072	599.026
2) T	3,5-DICHL...	6.287	5.862	1382.7E6	586.4E6	642.727	662.840
3) T	4-Nitroph...	6.875	6.282	583.4E6	224.4E6	722.357	732.164
5) T	DICAMBA	7.233	6.800	4034.9E6	1713.7E6	646.161	651.846
6) T	MCPD	7.402	6.894	303.1E6	136.7E6	64.921	63.555
7) T	MCPA	7.550	7.104	426.6E6	191.6E6	63.945	64.200
8) T	DICHLORPROP	7.920	7.411	1004.4E6	430.7E6	638.510	645.325
9) T	2,4-D	8.147	7.701	1205.3E6	509.1E6	661.940	691.813
10) T	Pentachlo...	8.446	8.113	13863.3E6	5524.0E6	656.216	655.871
11) T	2,4,5-TP ...	8.995	8.475	5543.5E6	2364.6E6	655.098	663.338
12) T	2,4,5-T	9.278	8.851	5851.5E6	2268.3E6	660.131	693.443
13) T	2,4-DB	9.826	9.354	1170.4E6	298.1E6	708.038	673.756
14) T	DINOSEB	10.972	9.675	4192.6E6	1613.6E6	638.442	646.746
15) T	Picloram	10.798	10.654	7930.8E6	3113.2E6	664.446	665.751
16) T	DCPA	11.240	10.601	7123.5E6	2907.4E6	659.296	658.450


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012022\
Data File : PS018087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 12:52
Operator : AJ\MA
Sample : HSTDCCC750
Misc : FOR ABDUL RAUF
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:21:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

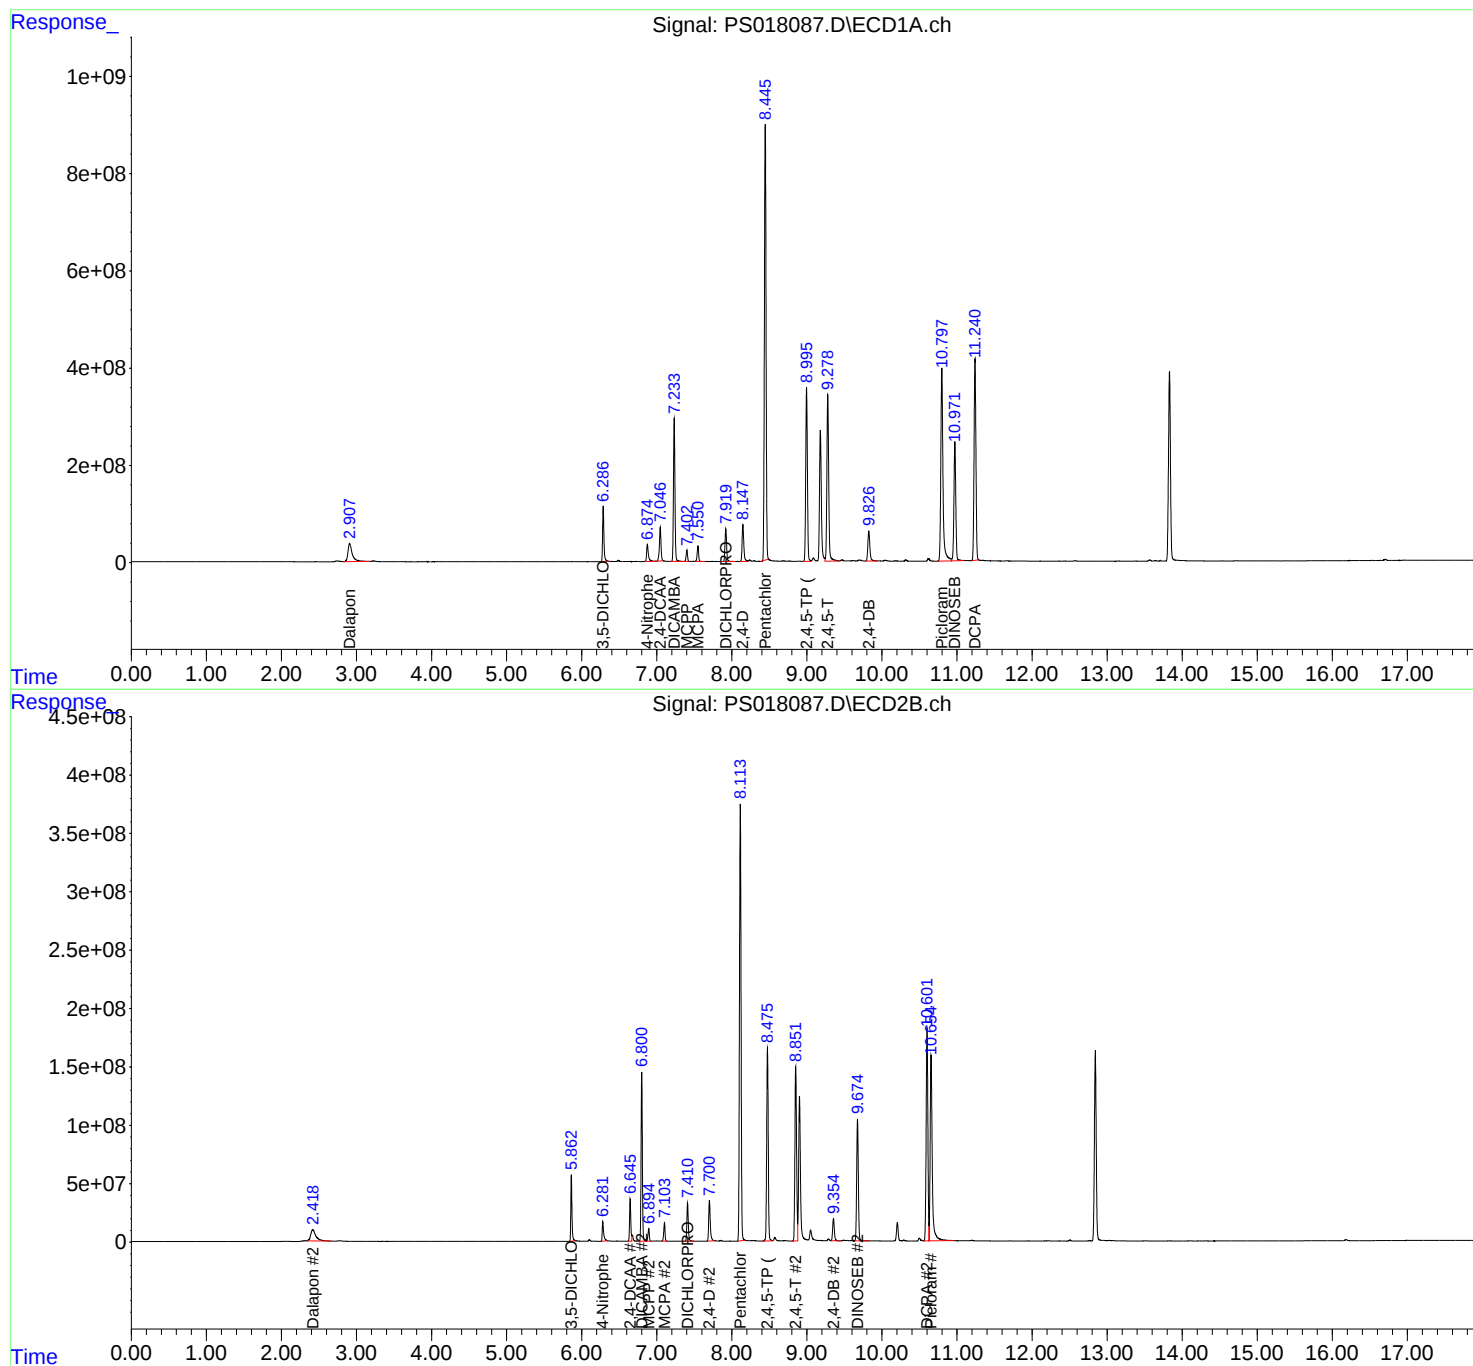


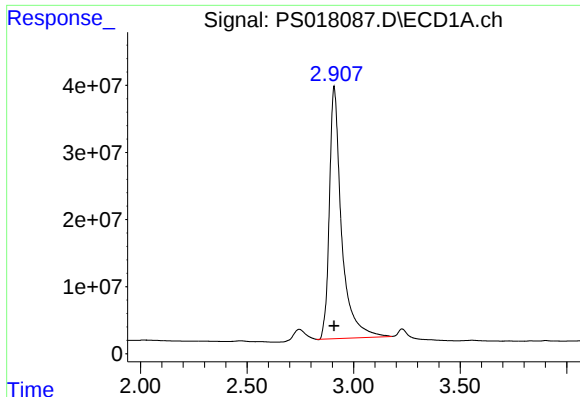

#1 Dalapon


R.T.: 2.908 min
Delta R.T.: -0.001 min
Response: 1496644010
Conc: 610.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

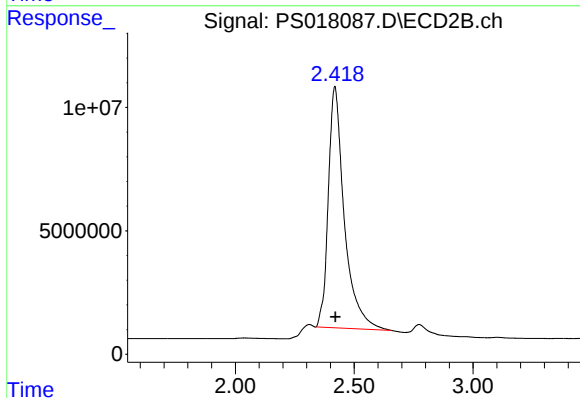


#1 Dalapon

R.T.: 2.419 min
Delta R.T.: -0.002 min
Response: 458068495
Conc: 599.03 ng/ml

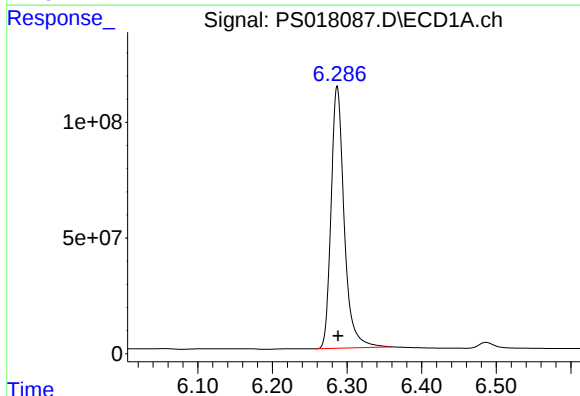


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.287 min
Delta R.T.: -0.001 min
Response: 1382661453
Conc: 642.73 ng/ml

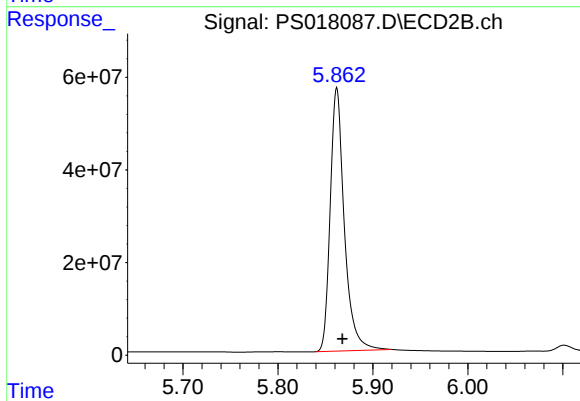

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 586368043
Conc: 662.84 ng/ml

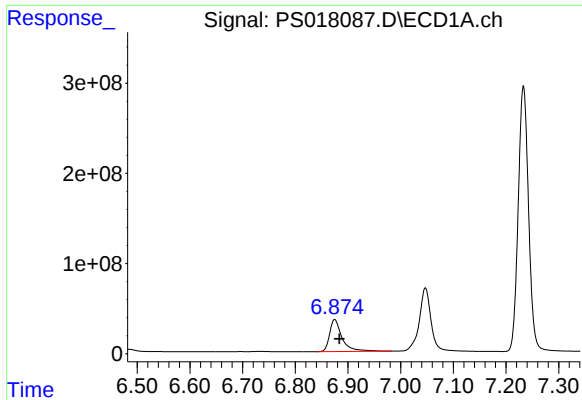

#3 4-Nitrophenol


R.T.: 6.875 min
Delta R.T.: -0.009 min
Response: 583436050
Conc: 722.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

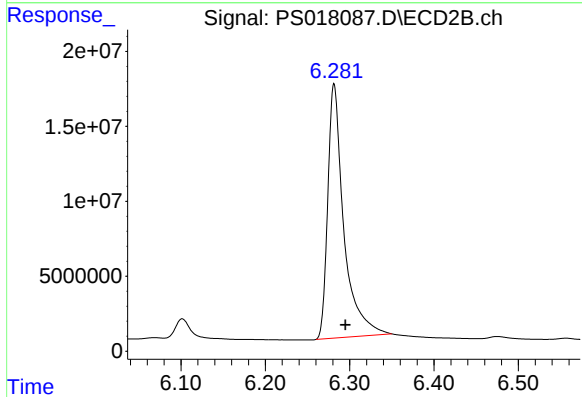


#3 4-Nitrophenol

R.T.: 6.282 min
Delta R.T.: -0.013 min
Response: 224424465
Conc: 732.16 ng/ml

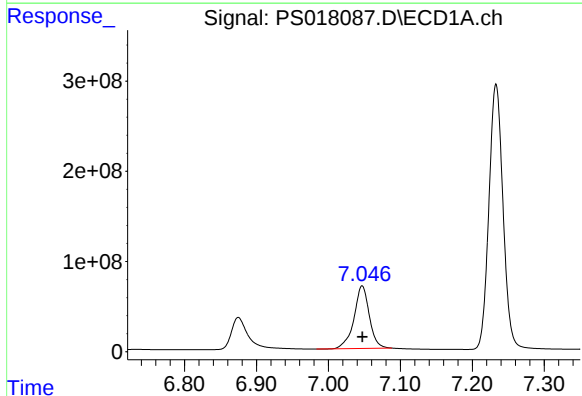


#4 2,4-DCAA

R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 1028014119
Conc: 711.19 ng/ml

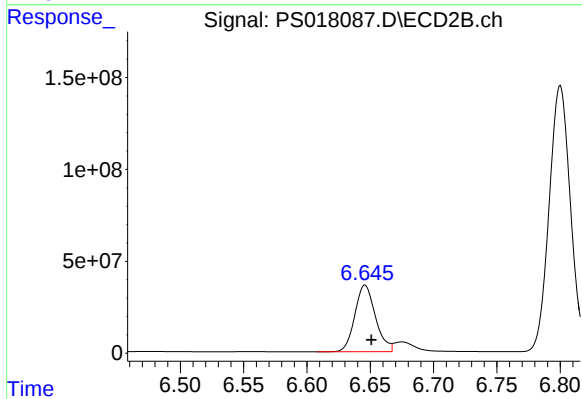

#4 2,4-DCAA


R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 410700816
Conc: 707.80 ng/ml

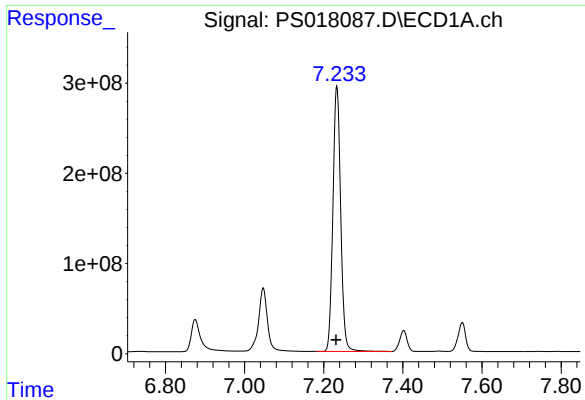

#5 DICAMBA


R.T.: 7.233 min
Delta R.T.: 0.002 min
Response: 4034899431
Conc: 646.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

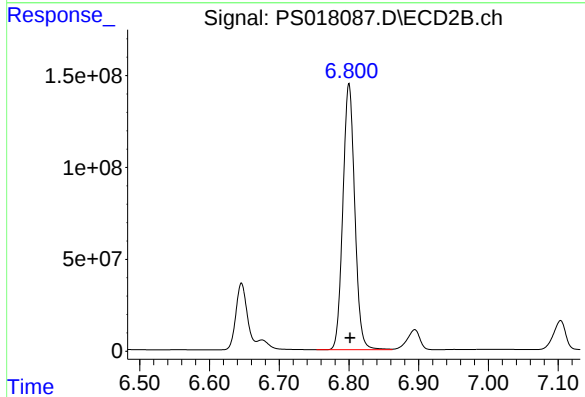


#5 DICAMBA

R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 1713738313
Conc: 651.85 ng/ml

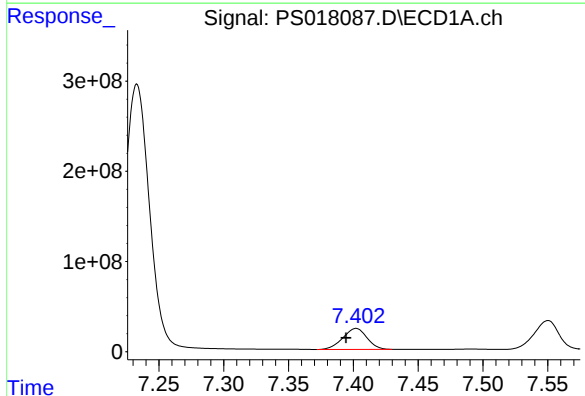


#6 MCP

R.T.: 7.402 min
Delta R.T.: 0.008 min
Response: 303111589
Conc: 64.92 ug/ml

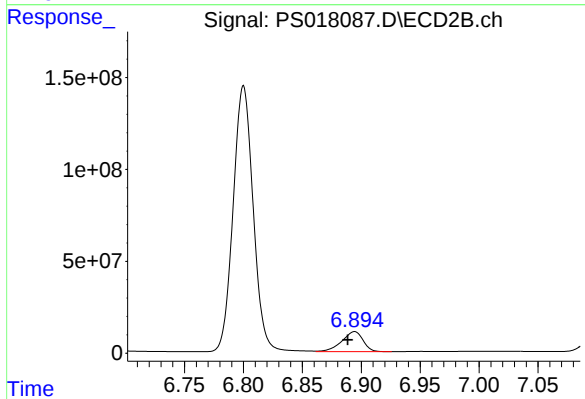

#6 MCP


R.T.: 6.894 min
Delta R.T.: 0.006 min
Response: 136701719
Conc: 63.55 ug/ml

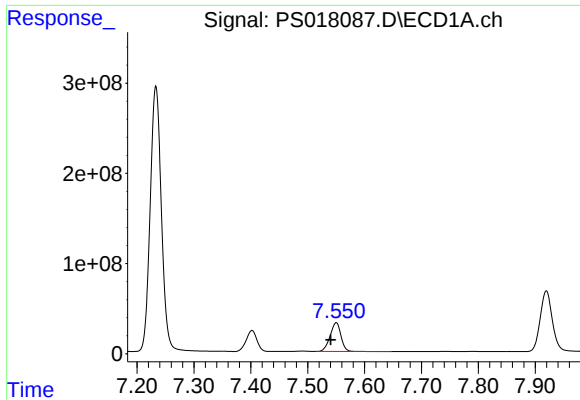

#7 MCPA


R.T.: 7.550 min
Delta R.T.: 0.010 min
Response: 426624981
Conc: 63.95 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

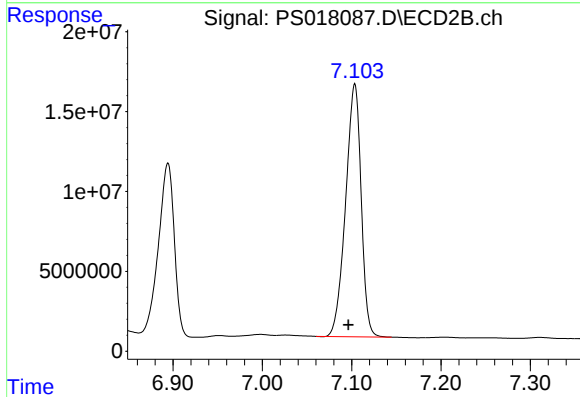


#7 MCPA

R.T.: 7.104 min
Delta R.T.: 0.007 min
Response: 191569127
Conc: 64.20 ug/ml

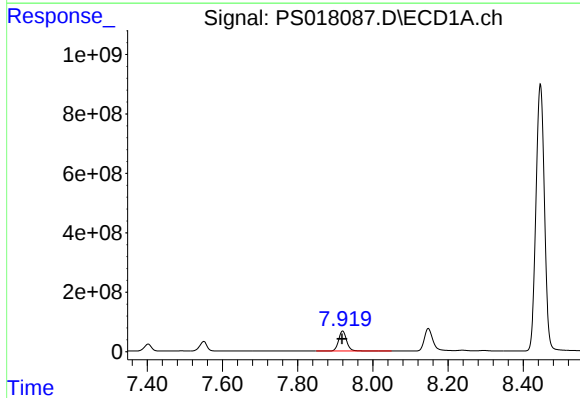


#8 DICHLORPROP

R.T.: 7.920 min
Delta R.T.: 0.002 min
Response: 1004405927
Conc: 638.51 ng/ml

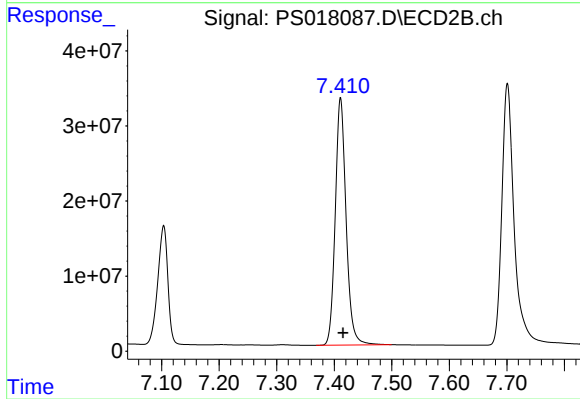

#8 DICHLORPROP


R.T.: 7.411 min
Delta R.T.: -0.004 min
Response: 430705151
Conc: 645.32 ng/ml

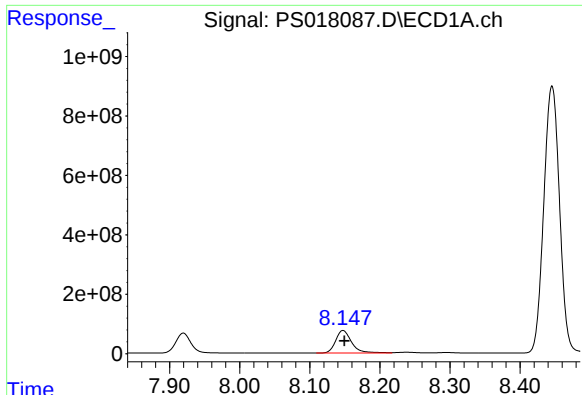

#9 2,4-D


R.T.: 8.147 min
Delta R.T.: -0.002 min
Response: 1205349446
Conc: 661.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

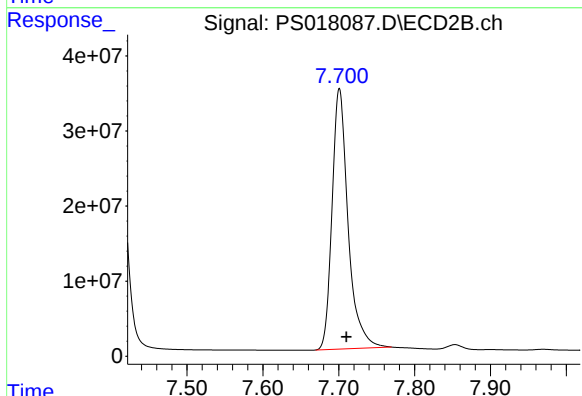


#9 2,4-D

R.T.: 7.701 min
Delta R.T.: -0.009 min
Response: 509137088
Conc: 691.81 ng/ml

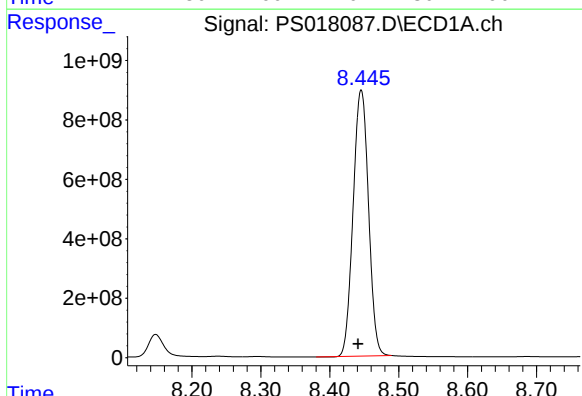


#10 Pentachlorophenol

R.T.: 8.446 min
Delta R.T.: 0.004 min
Response: 13863265724
Conc: 656.22 ng/ml

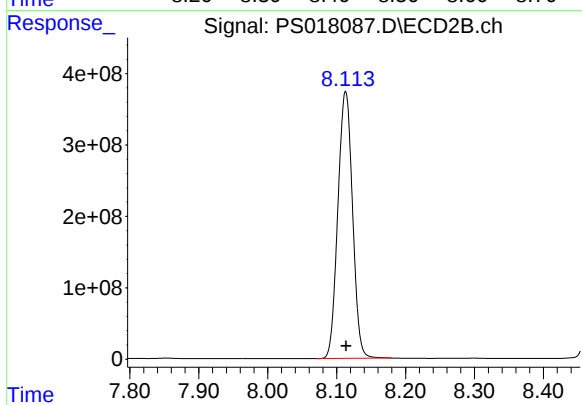

#10 Pentachlorophenol


R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 5523985087
Conc: 655.87 ng/ml

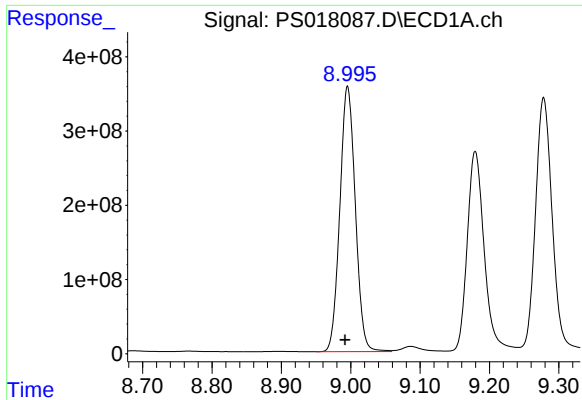

#11 2,4,5-TP (SILVEX)


R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 5543531369
Conc: 655.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

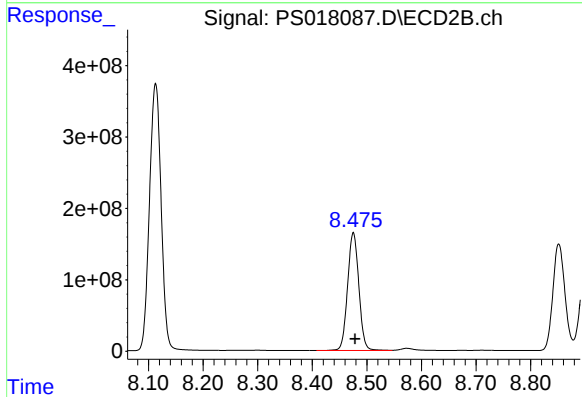


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 2364595250
Conc: 663.34 ng/ml

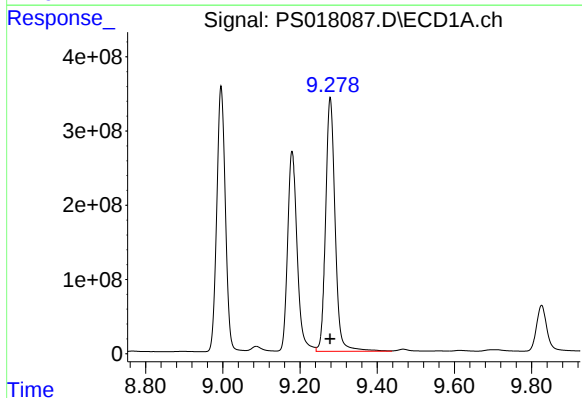


#12 2,4,5-T

R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 5851489977
Conc: 660.13 ng/ml

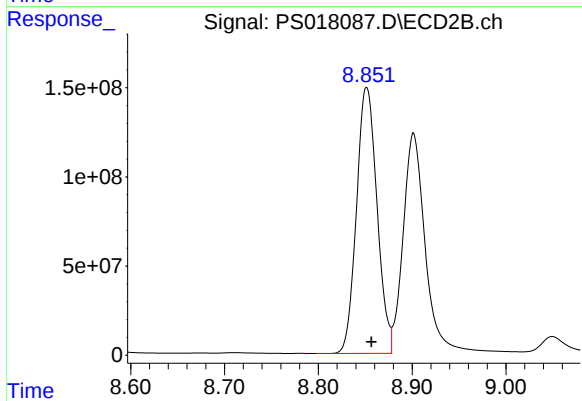

#12 2,4,5-T


R.T.: 8.851 min
Delta R.T.: -0.005 min
Response: 2268264962
Conc: 693.44 ng/ml

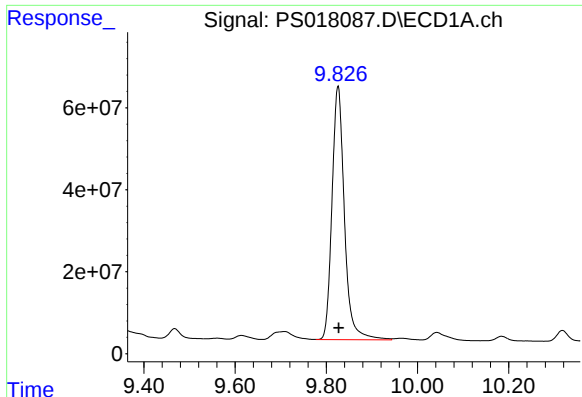

#13 2,4-DB


R.T.: 9.826 min
Delta R.T.: -0.002 min
Response: 1170411135
Conc: 708.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

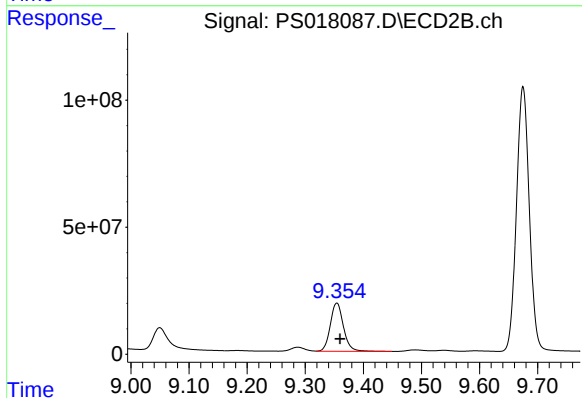


#13 2,4-DB

R.T.: 9.354 min
Delta R.T.: -0.005 min
Response: 298108142
Conc: 673.76 ng/ml

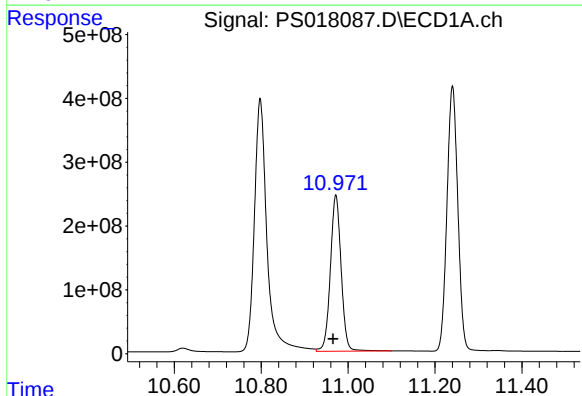


#14 DINOSEB

R.T.: 10.972 min
Delta R.T.: 0.006 min
Response: 4192614217
Conc: 638.44 ng/ml

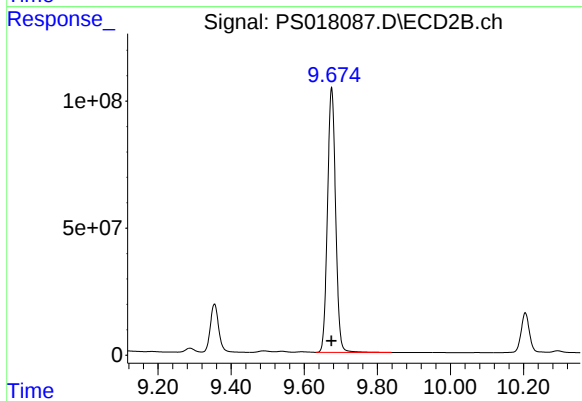

#14 DINOSEB


R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 1613641814
Conc: 646.75 ng/ml

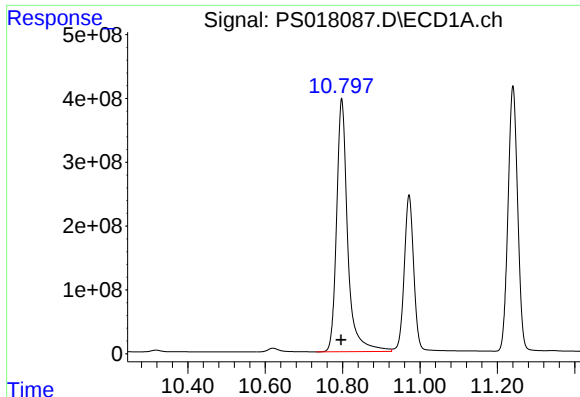

#15 Picloram


R.T.: 10.798 min
Delta R.T.: 0.002 min
Response: 7930768457
Conc: 664.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

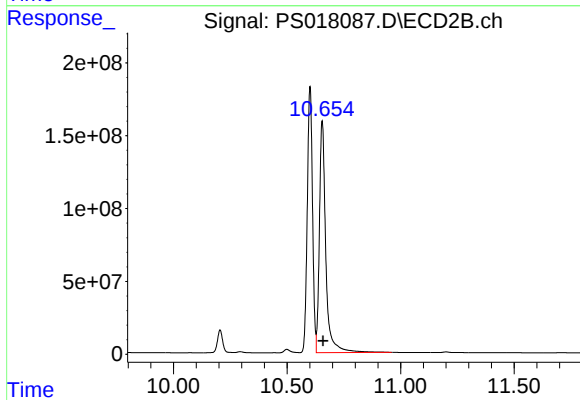


#15 Picloram

R.T.: 10.654 min
Delta R.T.: -0.005 min
Response: 3113150784
Conc: 665.75 ng/ml

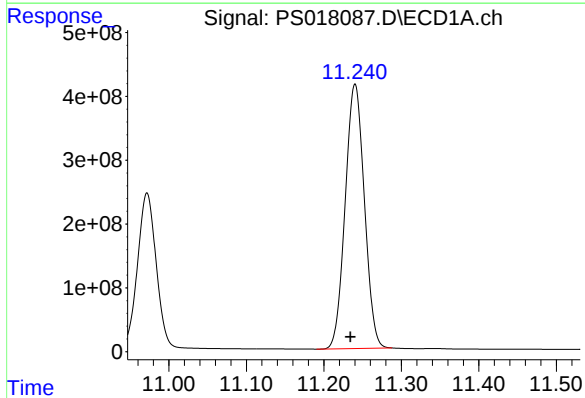

#16 DCPA

R.T.: 11.240 min
Delta R.T.: 0.006 min
Response: 7123547732
Conc: 659.30 ng/ml

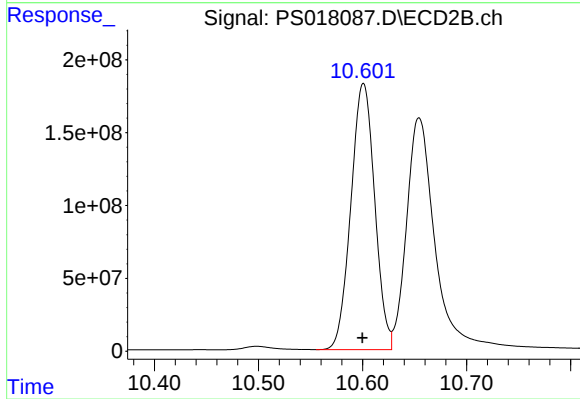

#16 DCPA

R.T.: 10.601 min
Delta R.T.: 0.001 min
Response: 2907377539
Conc: 658.45 ng/ml