

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012723\
 Data File : PS021892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2023 08:33
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:16:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.362	6.844	11652400	1991324	4.186	1.108 #
Target Compounds							
1) T	Dalapon	2.506	0.000	1844988	0	<MDL	N.D. #
3) T	4-Nitroph...	6.213	6.428	12355086	1093994	8.476	<MDL #
5) T	DICAMBA	6.523	7.024f	485275	4147.3E6	<MDL	487.757 #
6) T	MCP	6.697	7.024f	208738	4147.3E6	<MDL	625.383 #
7) T	MCPA	6.804	0.000	7888320	0	<MDL	N.D. #
9) T	2,4-D	7.284	7.880	7803.8E6	879977	2009.311	<MDL #
10) T	Pentachlo...	7.543	8.318	6891059	3793586	<MDL	<MDL #
11) T	2,4,5-TP ...	8.099	8.690	27506348	6545168	1.493	<MDL #
12) T	2,4,5-T	8.289f	0.000	13745170	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.615f	0	21294618	N.D.	14.213
14) T	DINOSEB	0.000	9.906	0	2087386	N.D.	<MDL
15) T	Picloram	9.714	10.893	1666.9E6	5478582	58.760	<MDL #
16) T	DCPA	10.154	10.830	7172864	94569295	<MDL	6.784 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012723\
Data File : PS021892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2023 08:33
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:16:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

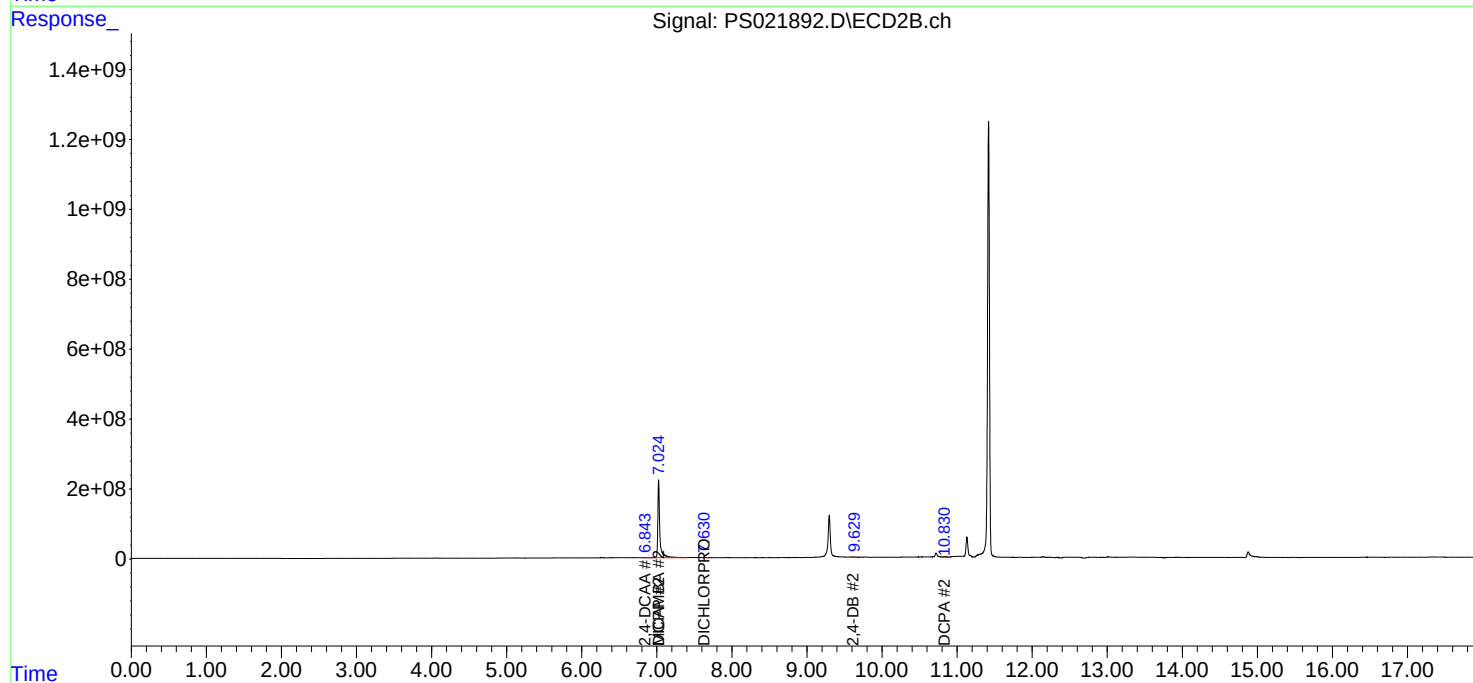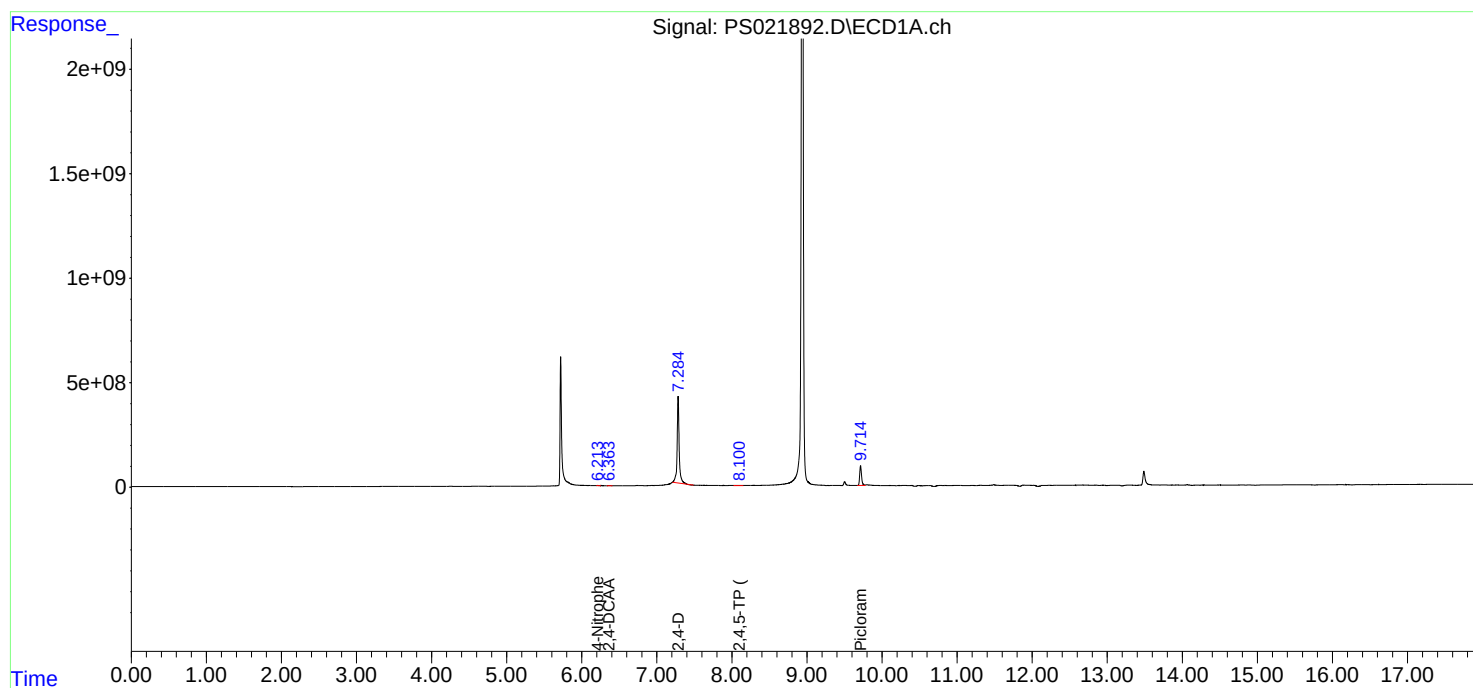


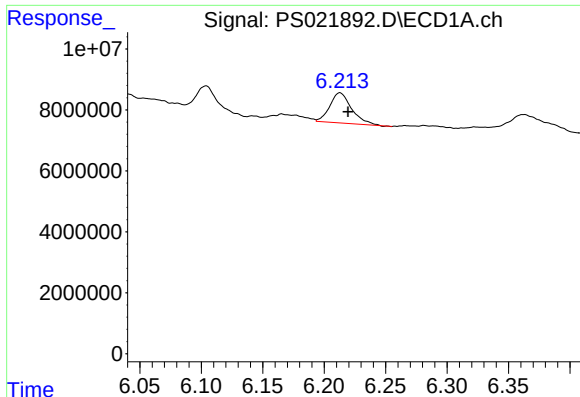

#3 4-Nitrophenol


R.T.: 6.213 min
Delta R.T.: -0.006 min
Response: 12355086
Conc: 8.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

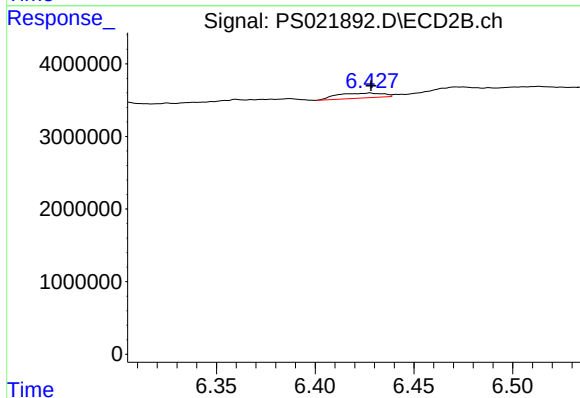


#3 4-Nitrophenol

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 1093994
Conc: N.D.

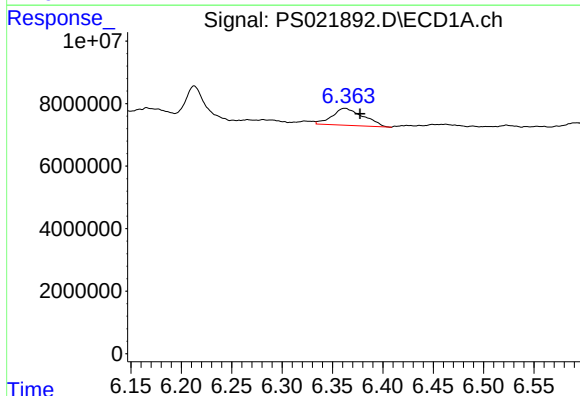


#4 2,4-DCAA

R.T.: 6.362 min
Delta R.T.: -0.015 min
Response: 11652400
Conc: 4.19 ng/ml

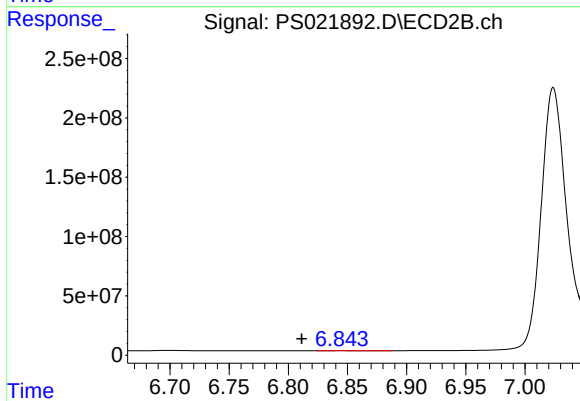

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: 0.033 min
Response: 1991324
Conc: 1.11 ng/ml

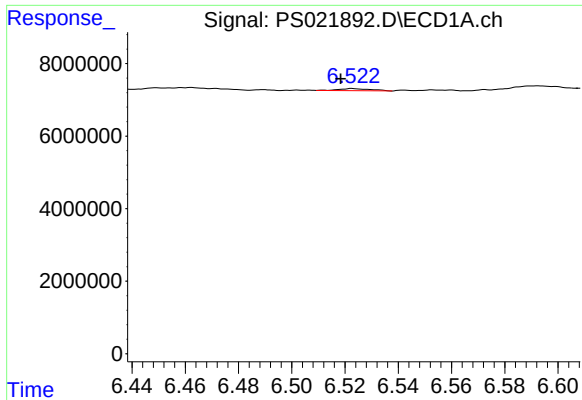

#5 DICAMBA


R.T.: 6.523 min
Delta R.T.: 0.004 min
Response: 485275
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

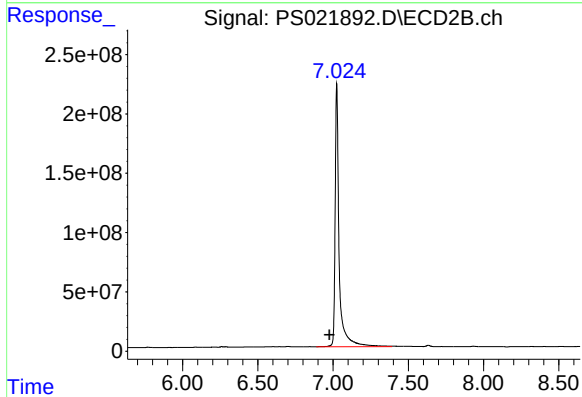


#5 DICAMBA

R.T.: 7.024 min
Delta R.T.: 0.049 min
Response: 4147279415
Conc: 487.76 ng/ml

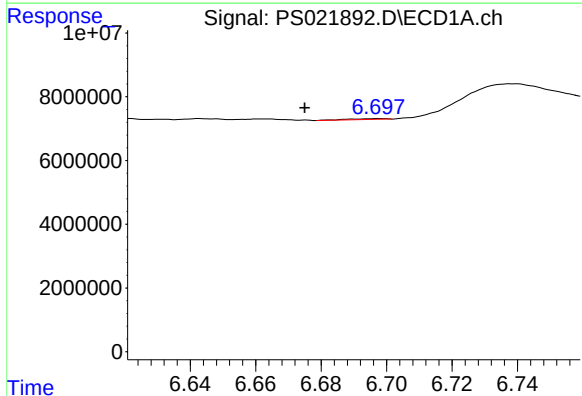


#6 MCPP

R.T.: 6.697 min
Delta R.T.: 0.023 min
Response: 208738
Conc: N.D.

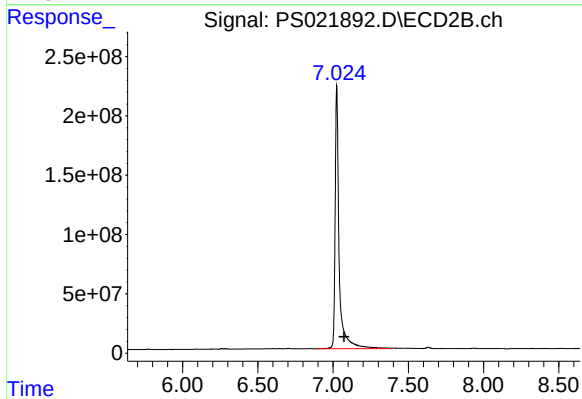

#6 MCPP


R.T.: 7.024 min
Delta R.T.: -0.050 min
Response: 4147279415
Conc: 625.38 ug/ml

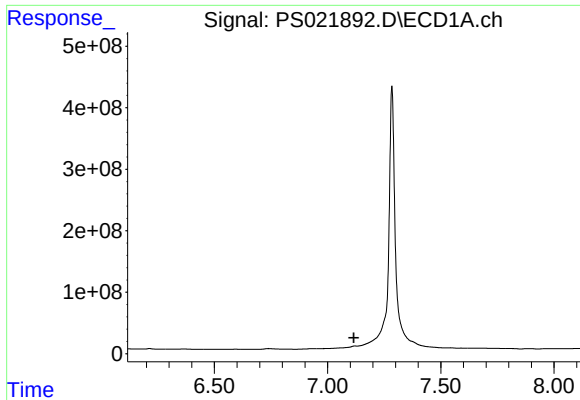

#8 DICHLORPROP


R.T.: 7.122 min
Delta R.T.: 0.005 min
Response: -55620978
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

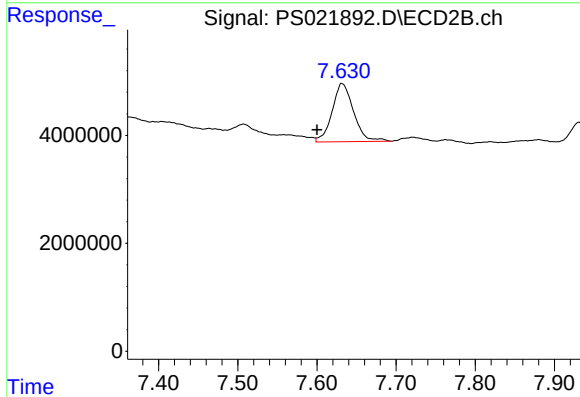


#8 DICHLORPROP

R.T.: 7.632 min
Delta R.T.: 0.031 min
Response: 20349149
Conc: 9.54 ng/ml

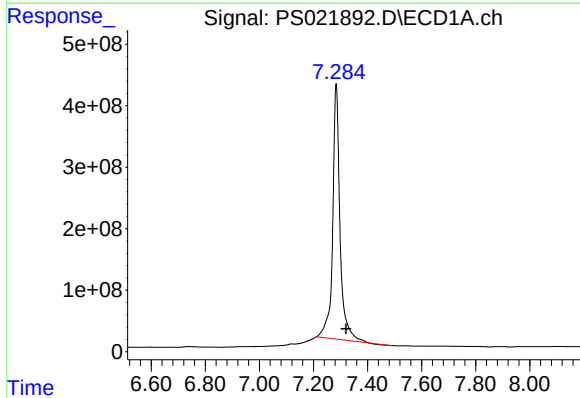


#9 2,4-D

R.T.: 7.284 min
Delta R.T.: -0.037 min
Response: 7803766404
Conc: 2009.31 ng/ml

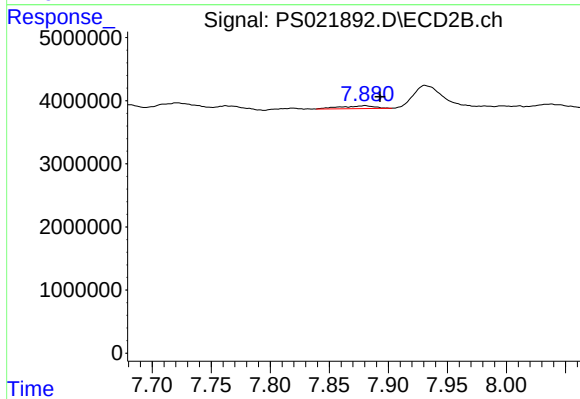

#9 2,4-D


R.T.: 7.880 min
Delta R.T.: -0.013 min
Response: 879977
Conc: N.D.

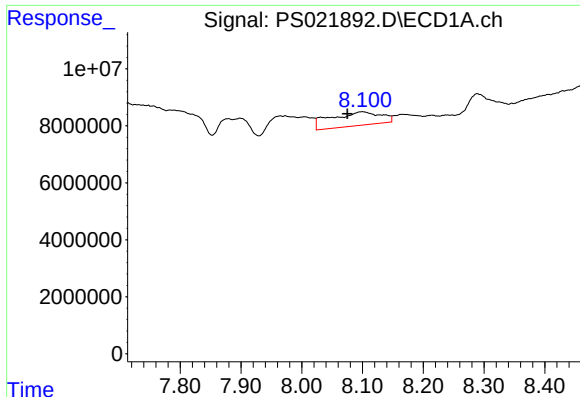

#11 2,4,5-TP (SILVEX)


R.T.: 8.099 min
Delta R.T.: 0.024 min
Response: 27506348
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

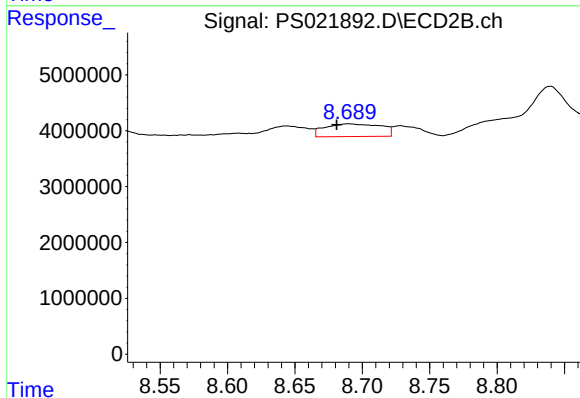


#11 2,4,5-TP (SILVEX)

R.T.: 8.690 min
Delta R.T.: 0.009 min
Response: 6545168
Conc: N.D.

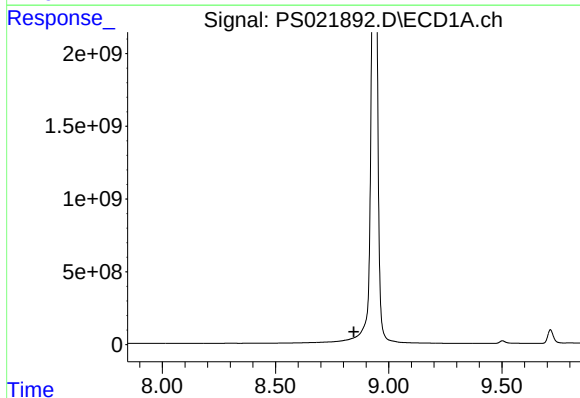


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.846 min
Response: 0
Conc: N.D.

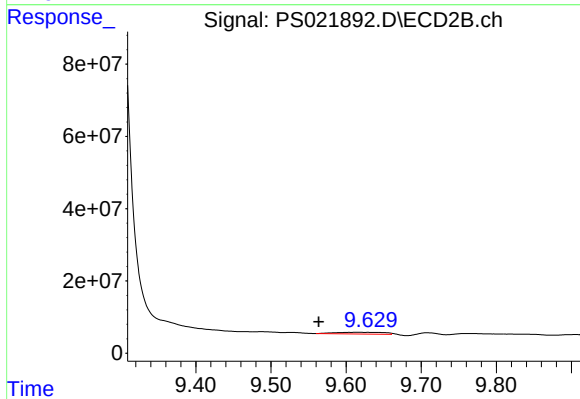

#13 2,4-DB


R.T.: 9.615 min
Delta R.T.: 0.051 min
Response: 21294618
Conc: 14.21 ng/ml

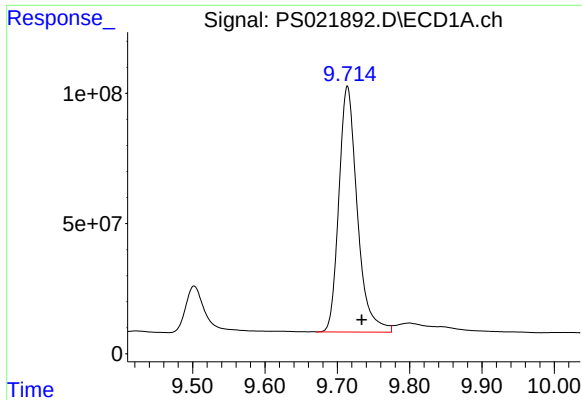

#15 Picloram


R.T.: 9.714 min
Delta R.T.: -0.020 min
Response: 1666870281
Conc: 58.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

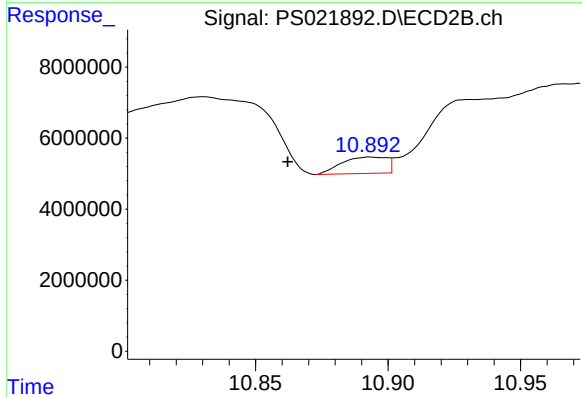


#15 Picloram

R.T.: 10.893 min
Delta R.T.: 0.031 min
Response: 5478582
Conc: N.D.

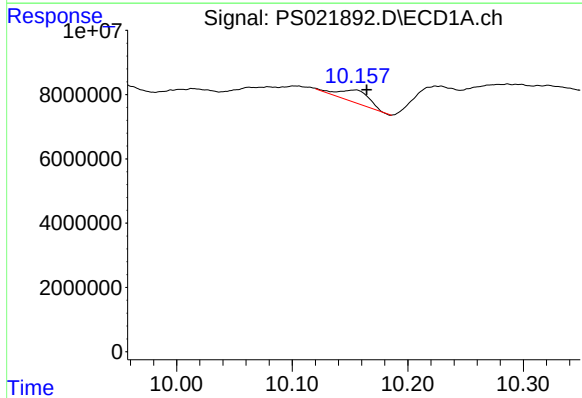

#16 DCPA

R.T.: 10.154 min
Delta R.T.: -0.011 min
Response: 7172864
Conc: N.D.

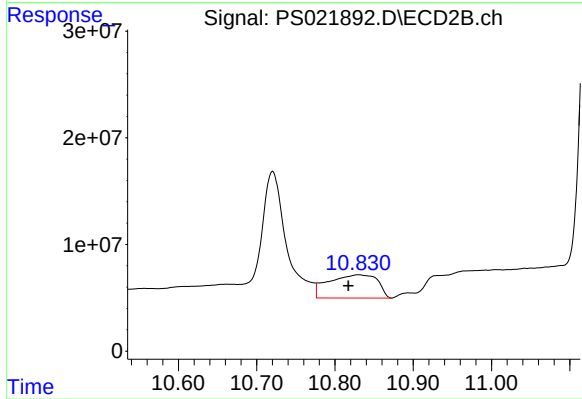

#16 DCPA

R.T.: 10.830 min
Delta R.T.: 0.013 min
Response: 94569295
Conc: 6.78 ng/ml