

Data Path : P:\HPCHEM1\ECD_S\Data\PS020118\
 Data File : PS000006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2018 14:34
 Operator : UA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 09:12:39 2018
 Quant Method : P:\HPCHEM1\ECD_S\Method\PS020118.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 03 09:12:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.836	11.212	235.0E6	216.1E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.175	2.552	288.7E6	230.4E6	682.500	682.500
2) T	3,5-DICHL...	10.249	9.354	314.8E6	286.1E6	697.500	697.500
3) T	4-Nitroph...	11.433	10.357	140.6E6	118.0E6	682.500	682.500
5) T	DICAMBA	12.156	11.503	870.1E6	827.4E6	705.000	705.000
6) T	MCPD	12.497	11.728	82262336	67522252	70.500	70.500
7) T	MCPA	12.749	12.107	145.3E6	113.4E6	69.750	69.750
8) T	DICHLORPROP	13.349	12.627	207.4E6	195.1E6	705.000	705.000
9) T	2,4-D	13.706	13.099	262.8E6	236.6E6	705.000	705.000
10) T	Pentachlo...	14.105	13.664	3970.6E6	3546.7E6	712.500	712.500
11) T	2,4,5-TP ...	14.972	14.272	1209.0E6	1142.6E6	712.500	712.500
12) T	2,4,5-T	15.370	14.804	1114.4E6	1007.4E6	712.500	712.500
13) T	2,4-DB	16.125	15.492	144.9E6	128.9E6	712.500	712.500
14) T	DINOSEB	17.639	15.925	727.2E6	667.9E6	705.000	705.000
15) T	Picloram	17.393	17.173	1360.7E6	1279.2E6	712.500	712.500
16) T	DCPA	17.980	17.115	1718.1E6	1571.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_S\Data\PS020118\
Data File : PS000006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2018 14:34
Operator : UA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 09:12:39 2018
Quant Method : P:\HPCHEM1\ECD_S\Method\PS020118.M
Quant Title : 8080.M
QLast Update : Sat Feb 03 09:12:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

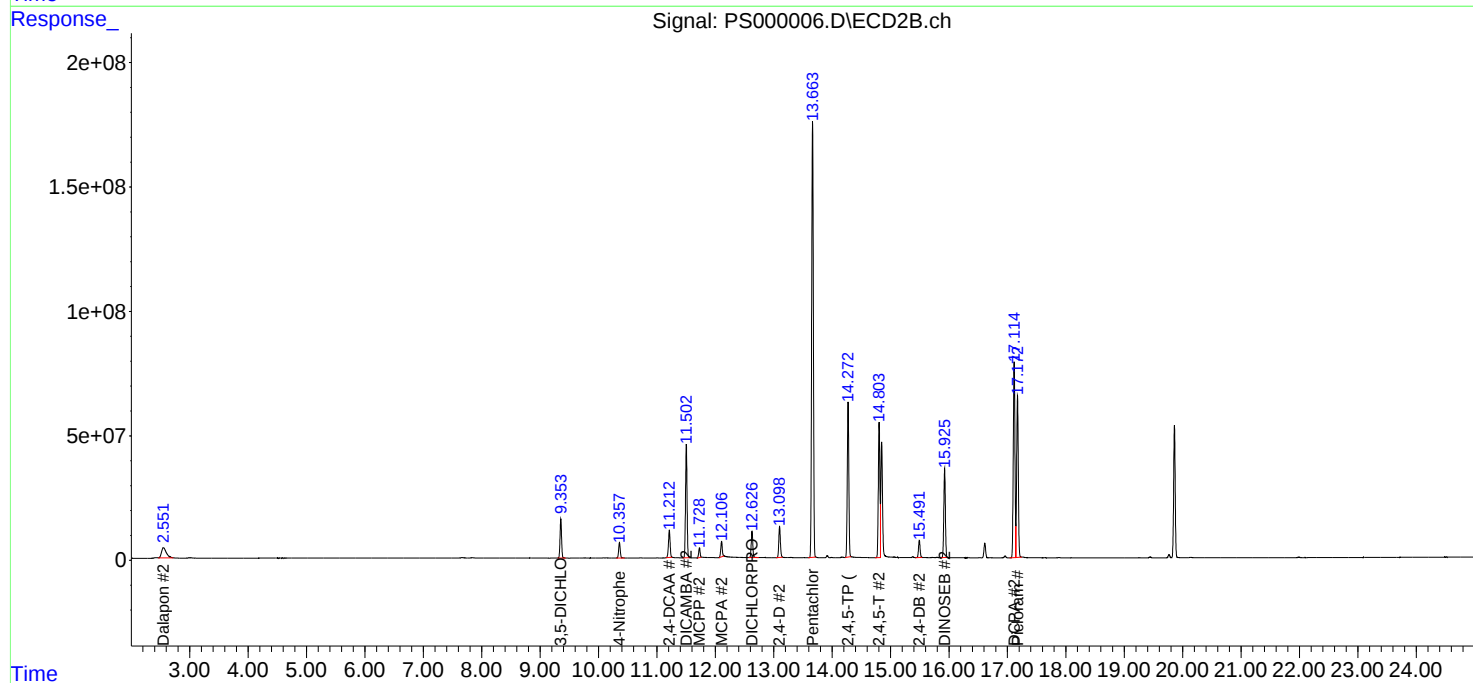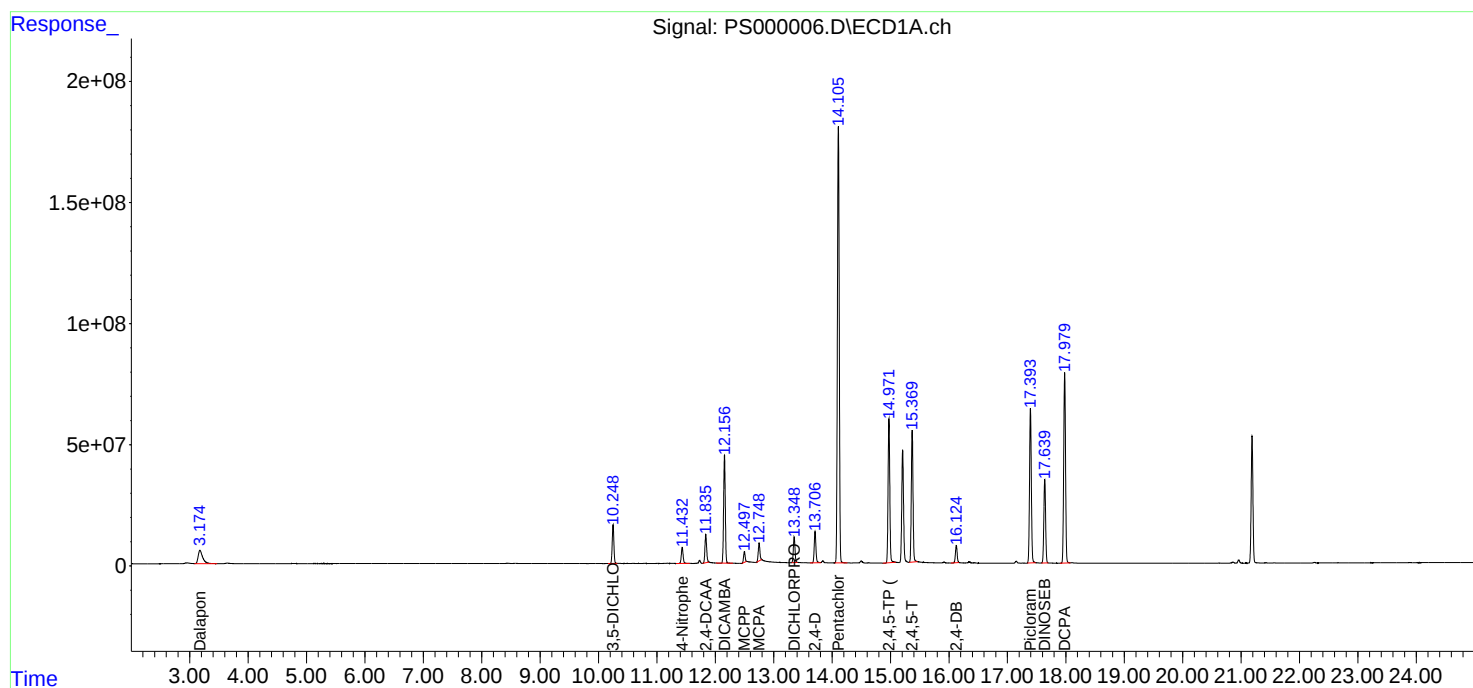


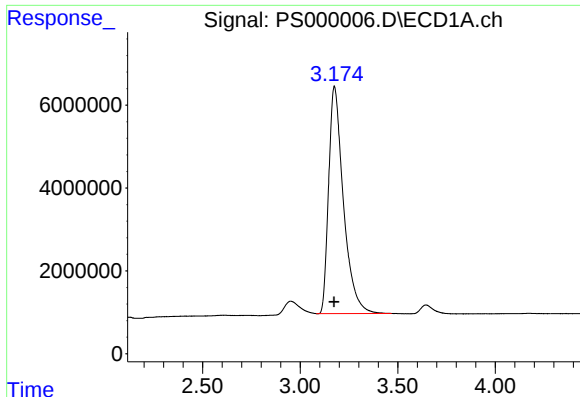

#1 Dalapon


R.T.: 3.175 min
Delta R.T.: 0.000 min
Response: 288662598
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

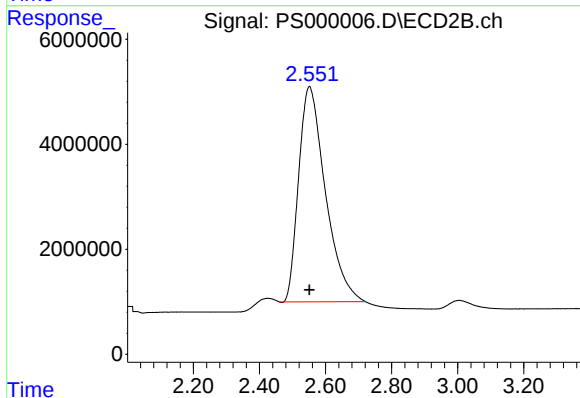


#1 Dalapon

R.T.: 2.552 min
Delta R.T.: 0.000 min
Response: 230432162
Conc: 682.50 ng/ml

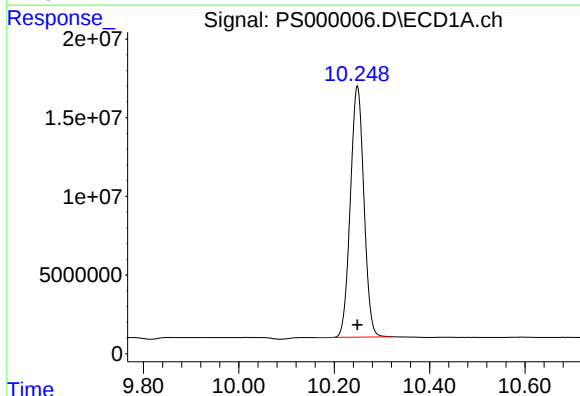


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.249 min
Delta R.T.: 0.000 min
Response: 314774964
Conc: 697.50 ng/ml

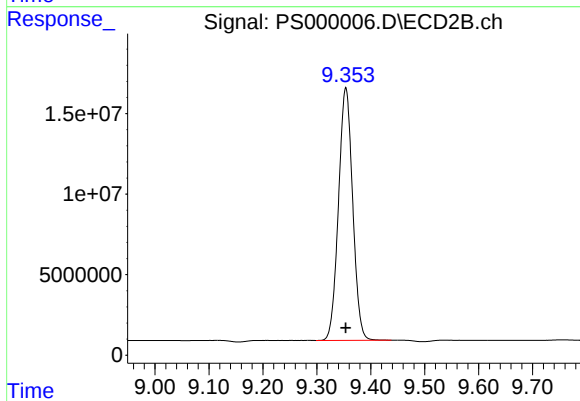

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.354 min
Delta R.T.: 0.000 min
Response: 286084762
Conc: 697.50 ng/ml

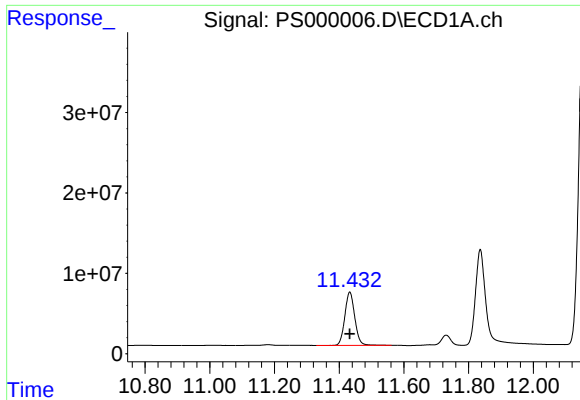

#3 4-Nitrophenol


R.T.: 11.433 min
Delta R.T.: 0.000 min
Response: 140563888
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

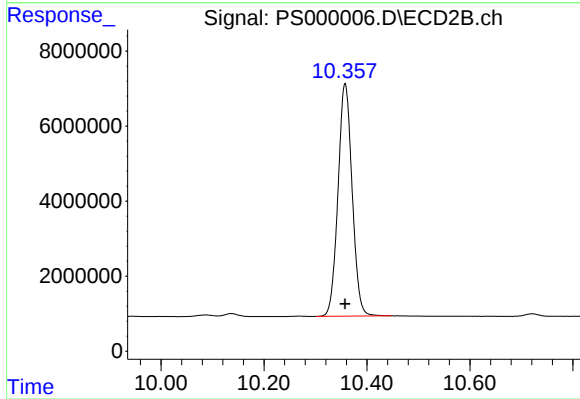


#3 4-Nitrophenol

R.T.: 10.357 min
Delta R.T.: 0.000 min
Response: 118034829
Conc: 682.50 ng/ml

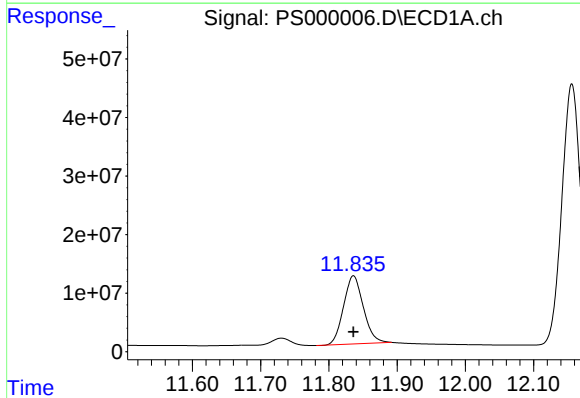


#4 2,4-DCAA

R.T.: 11.836 min
Delta R.T.: 0.000 min
Response: 234972224
Conc: 750.00 ng/ml

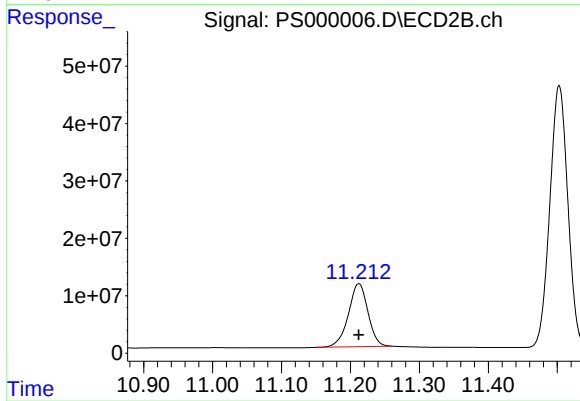

#4 2,4-DCAA


R.T.: 11.212 min
Delta R.T.: 0.000 min
Response: 216142946
Conc: 750.00 ng/ml

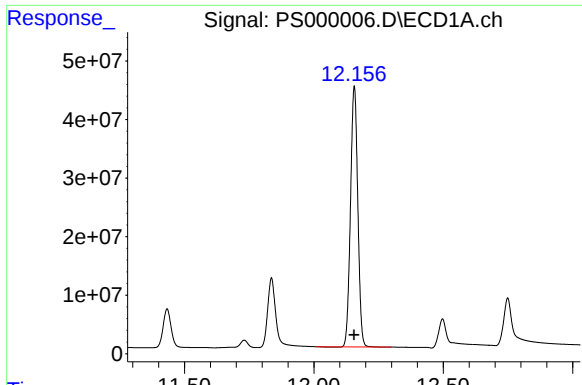

#5 DICAMBA


R.T.: 12.156 min
Delta R.T.: 0.000 min
Response: 870069350
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

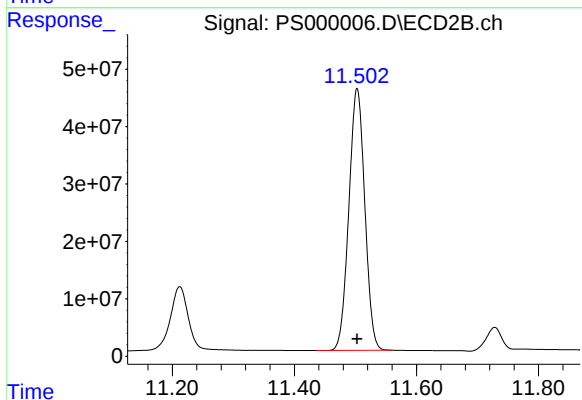


#5 DICAMBA

R.T.: 11.503 min
Delta R.T.: 0.000 min
Response: 827439462
Conc: 705.00 ng/ml

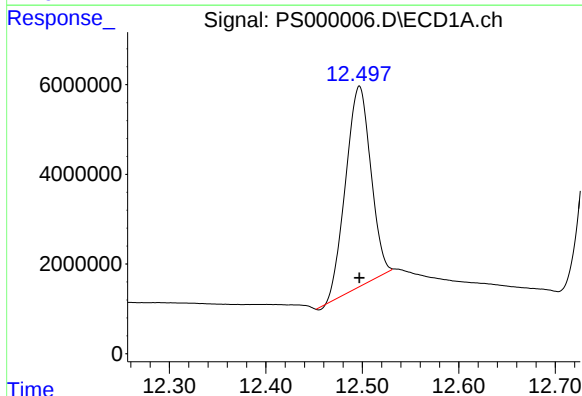


#6 MCP

R.T.: 12.497 min
Delta R.T.: 0.000 min
Response: 82262336
Conc: 70.50 ug/ml

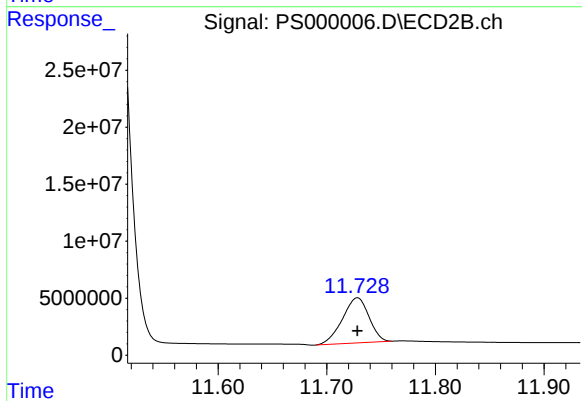

#6 MCP


R.T.: 11.728 min
Delta R.T.: 0.000 min
Response: 67522252
Conc: 70.50 ug/ml

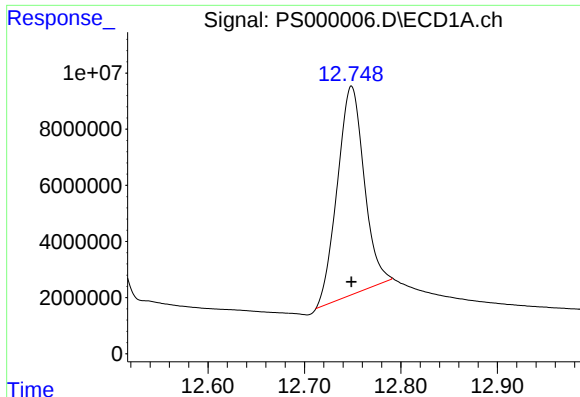

#7 MCPA


R.T.: 12.749 min
Delta R.T.: 0.000 min
Response: 145283507
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

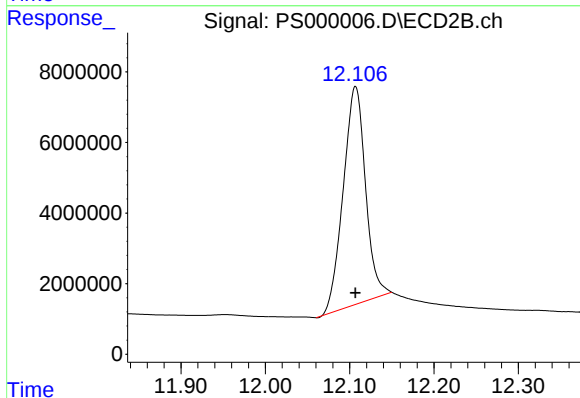


#7 MCPA

R.T.: 12.107 min
Delta R.T.: 0.000 min
Response: 113418193
Conc: 69.75 ug/ml

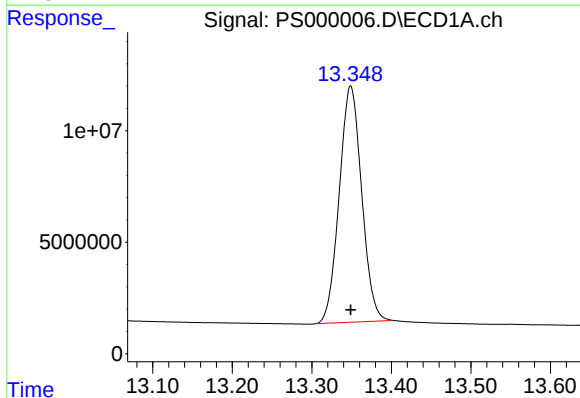


#8 DICHLORPROP

R.T.: 13.349 min
Delta R.T.: 0.000 min
Response: 207391405
Conc: 705.00 ng/ml

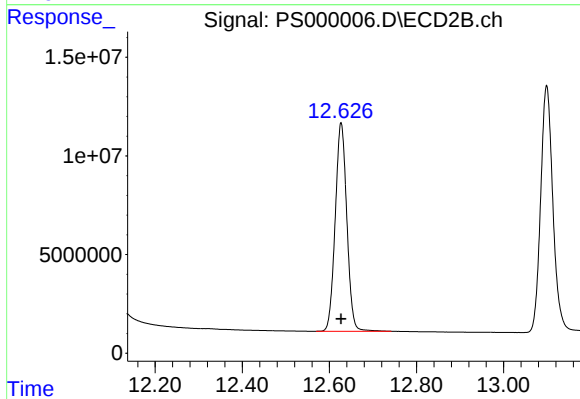

#8 DICHLORPROP


R.T.: 12.627 min
Delta R.T.: 0.000 min
Response: 195096785
Conc: 705.00 ng/ml

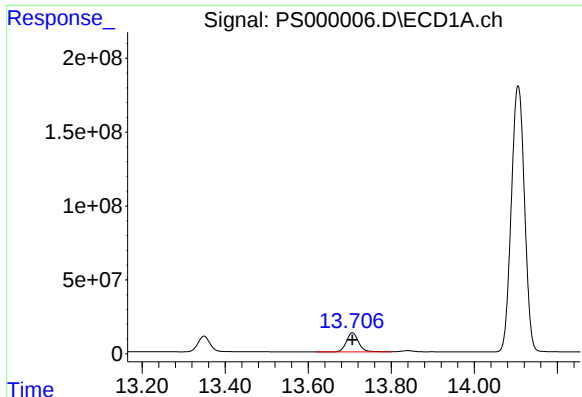

#9 2,4-D


R.T.: 13.706 min
Delta R.T.: 0.000 min
Response: 262847849
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

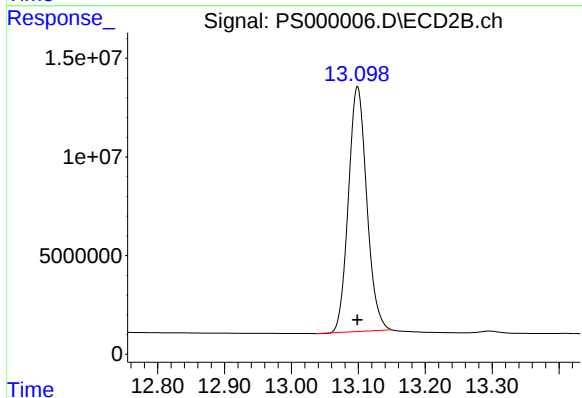


#9 2,4-D

R.T.: 13.099 min
Delta R.T.: 0.000 min
Response: 236638708
Conc: 705.00 ng/ml

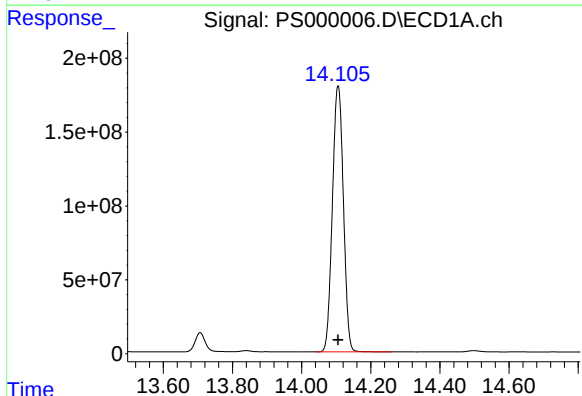


#10 Pentachlorophenol

R.T.: 14.105 min
Delta R.T.: 0.000 min
Response: 3970571277
Conc: 712.50 ng/ml

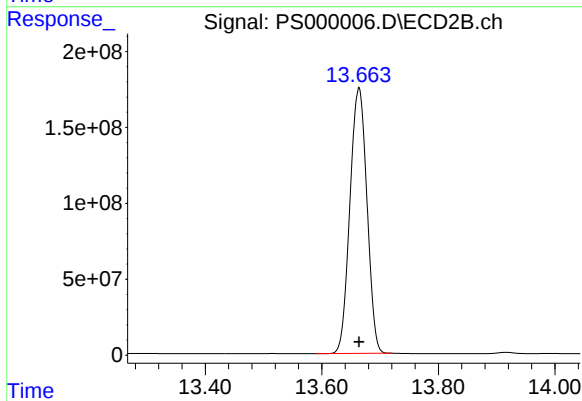

#10 Pentachlorophenol


R.T.: 13.664 min
Delta R.T.: 0.000 min
Response: 3546652219
Conc: 712.50 ng/ml

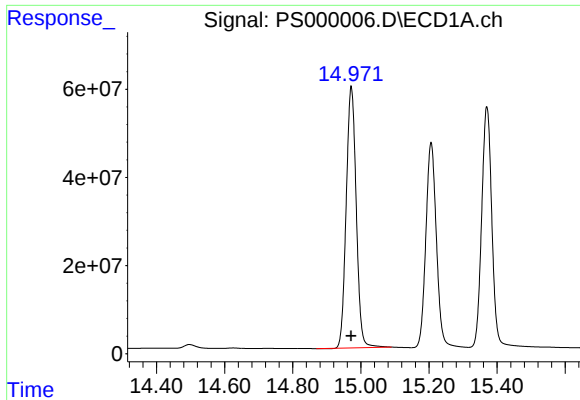

#11 2,4,5-TP (SILVEX)


R.T.: 14.972 min
Delta R.T.: 0.000 min
Response: 1209004035
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

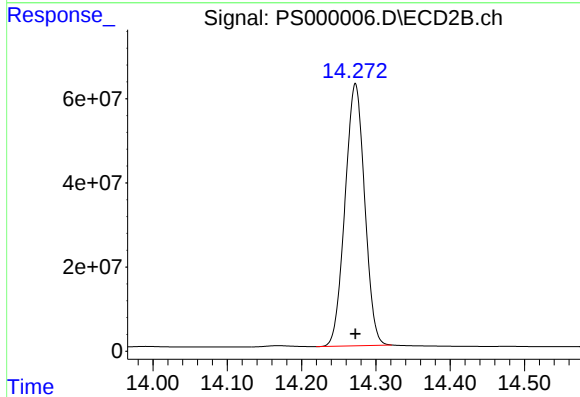


#11 2,4,5-TP (SILVEX)

R.T.: 14.272 min
Delta R.T.: 0.000 min
Response: 1142568052
Conc: 712.50 ng/ml

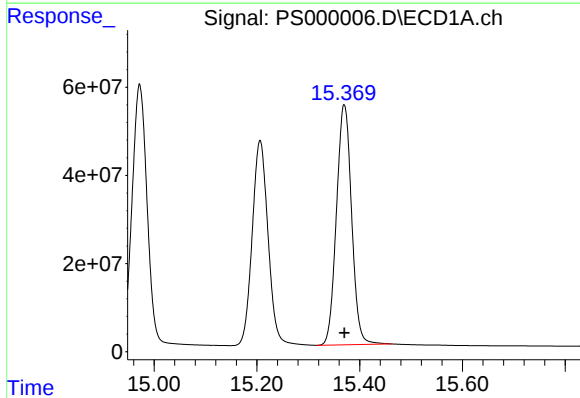


#12 2,4,5-T

R.T.: 15.370 min
Delta R.T.: 0.000 min
Response: 1114351087
Conc: 712.50 ng/ml

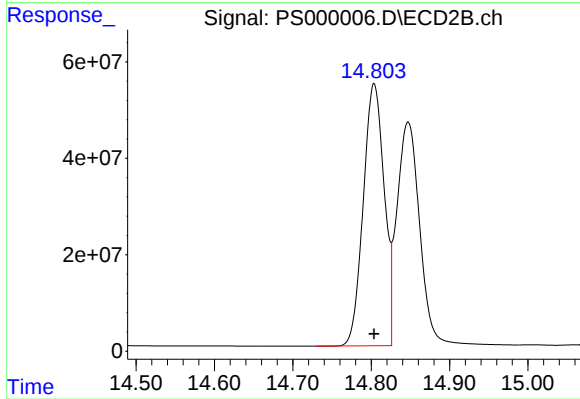

#12 2,4,5-T


R.T.: 14.804 min
Delta R.T.: 0.000 min
Response: 1007363691
Conc: 712.50 ng/ml

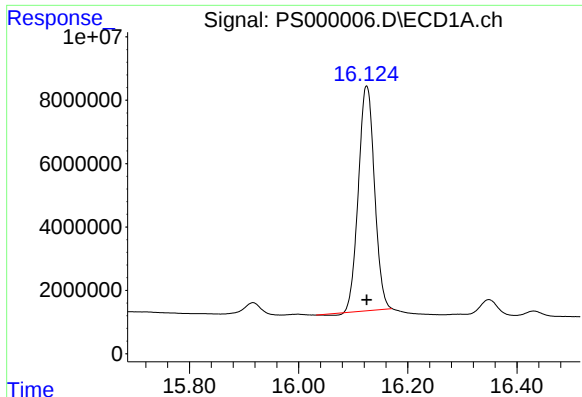

#13 2,4-DB


R.T.: 16.125 min
Delta R.T.: 0.000 min
Response: 144904857
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

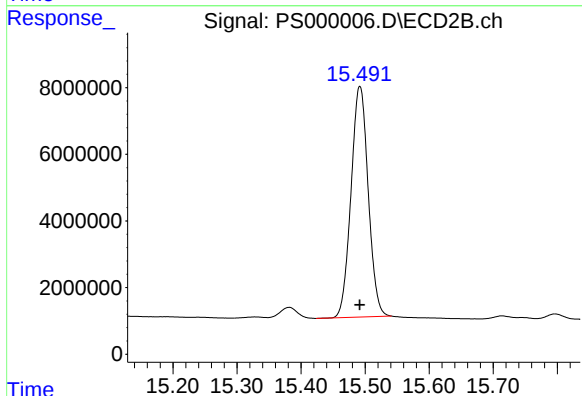


#13 2,4-DB

R.T.: 15.492 min
Delta R.T.: 0.000 min
Response: 128892737
Conc: 712.50 ng/ml

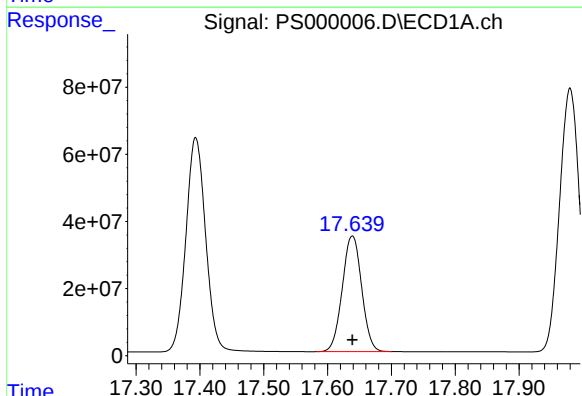


#14 DINOSEB

R.T.: 17.639 min
Delta R.T.: 0.000 min
Response: 727220104
Conc: 705.00 ng/ml

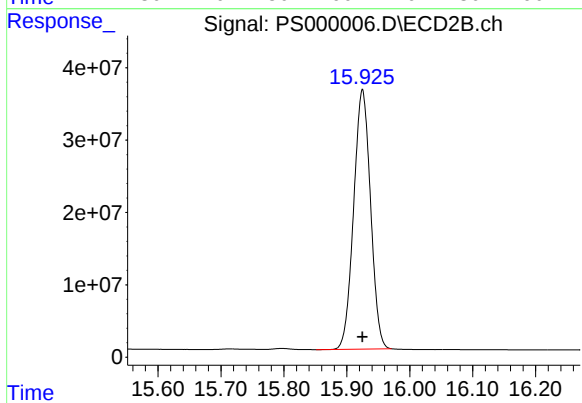

#14 DINOSEB


R.T.: 15.925 min
Delta R.T.: 0.000 min
Response: 667924640
Conc: 705.00 ng/ml

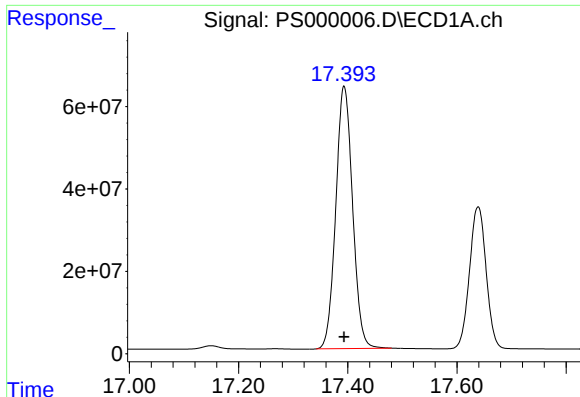

#15 Picloram


R.T.: 17.393 min
Delta R.T.: 0.000 min
Response: 1360658393
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

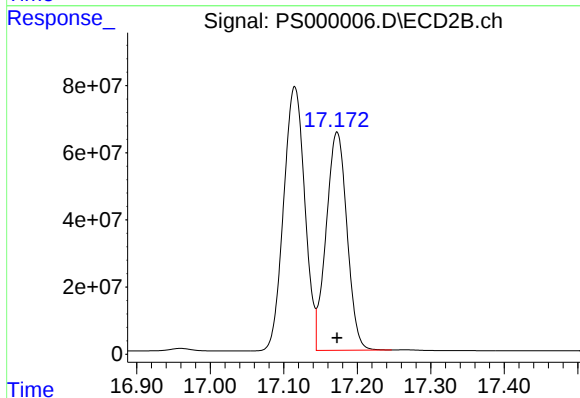


#15 Picloram

R.T.: 17.173 min
Delta R.T.: 0.000 min
Response: 1279153212
Conc: 712.50 ng/ml

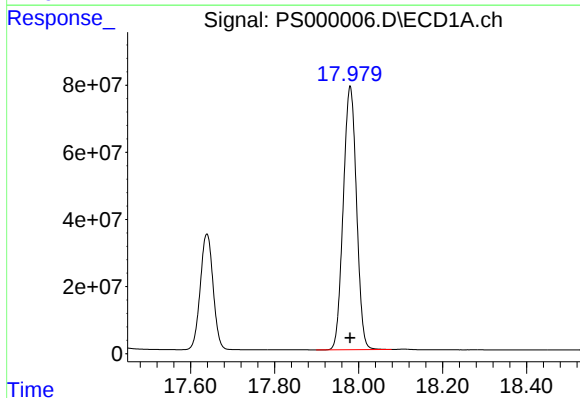

#16 DCPA

R.T.: 17.980 min
Delta R.T.: 0.000 min
Response: 1718059966
Conc: 720.00 ng/ml

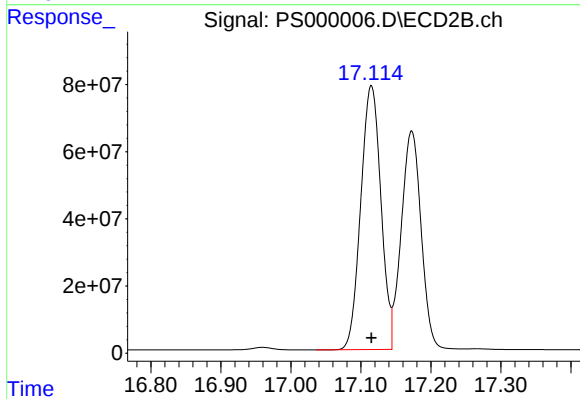

#16 DCPA

R.T.: 17.115 min
Delta R.T.: 0.000 min
Response: 1571880719
Conc: 720.00 ng/ml