

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020322\
 Data File : PS018218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 11:57
 Operator : AJ\MA
 Sample : N1335-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 22:21:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.041	6.649	678.8E6	278.4E6	469.585	479.738
Target Compounds							
1) T	Dalapon	2.856f	2.409	86395087	68701582	35.217	89.843 #
2) T	3,5-DICHL...	6.321	5.888	-3350202	107.1E6	N.D.	121.031
3) T	4-Nitroph...	6.857	6.330	56118882	18475691	69.481	60.275
5) T	DICAMBA	7.241	6.770	18265946	115.2E6	2.925	43.799 #
6) T	MCPD	7.365	6.924	69338090	66897520	14.851	31.102 #
7) T	MCPA	7.498f	7.126	266.4E6	10113266	39.931	3.389 #
8) T	DICHLORPROP	7.942	7.433	143.7E6	97756097	91.340	146.468 #
9) T	2,4-D	8.150	7.729	124.7E6	14313774	68.456	19.449 #
10) T	Pentachlo...	8.459	8.116	452.7E6	16479905	21.429	1.957 #
11) T	2,4,5-TP ...	9.045f	8.511	3181.0E6	737.8E6	375.907	206.985 #
12) T	2,4,5-T	9.335f	8.878	1249.5E6	444.4E6	140.963	135.852
13) T	2,4-DB	9.801	9.371	1839.8E6	590.2E6	1112.983	1333.835
14) T	DINOSEB	10.931	9.673	2370.0E6	648.8E6	360.899	260.040 #
15) T	Picloram	10.762	10.674	42238.0E6	5300.2E6	3538.728	1133.465 #
16) T	DCPA	11.218	0.000	726.7E6	0	67.261	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020322\
Data File : PS018218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 11:57
Operator : AJ\MA
Sample : N1335-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 22:21:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

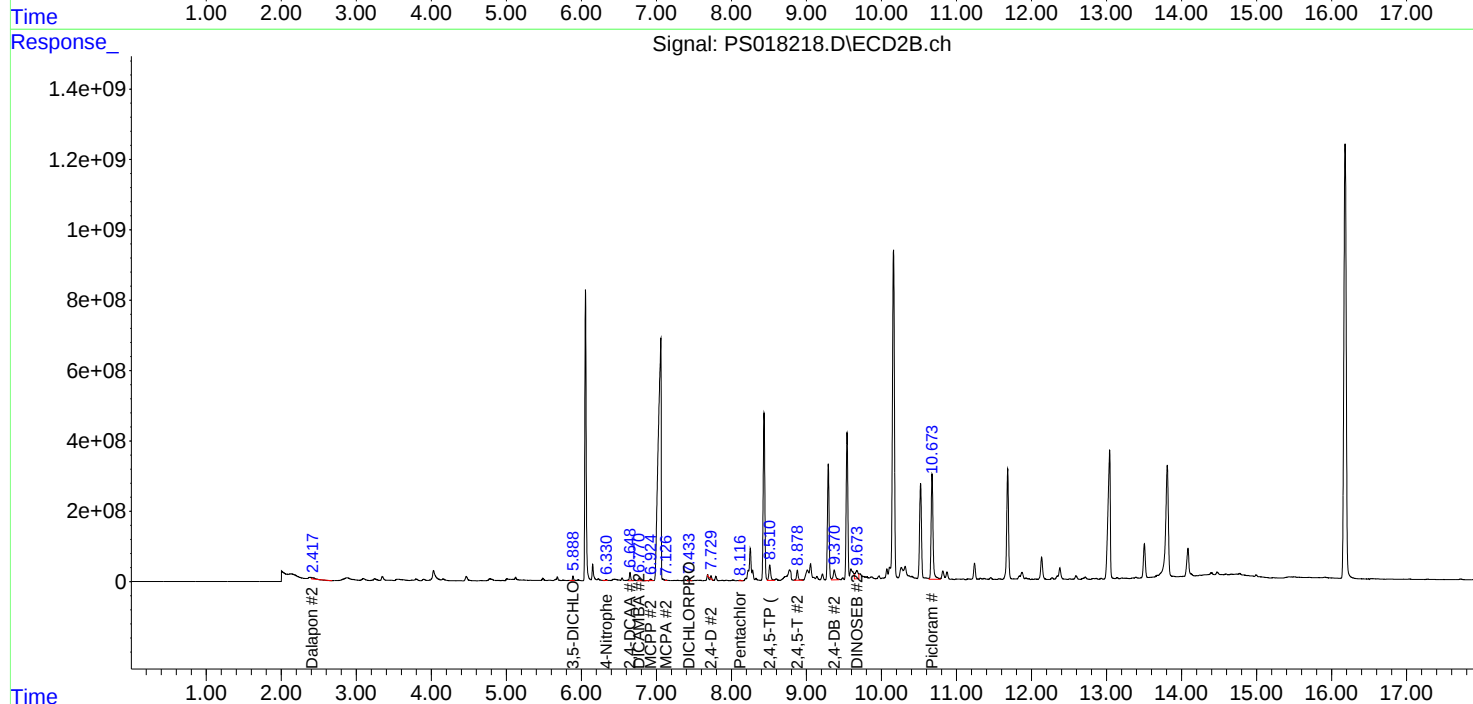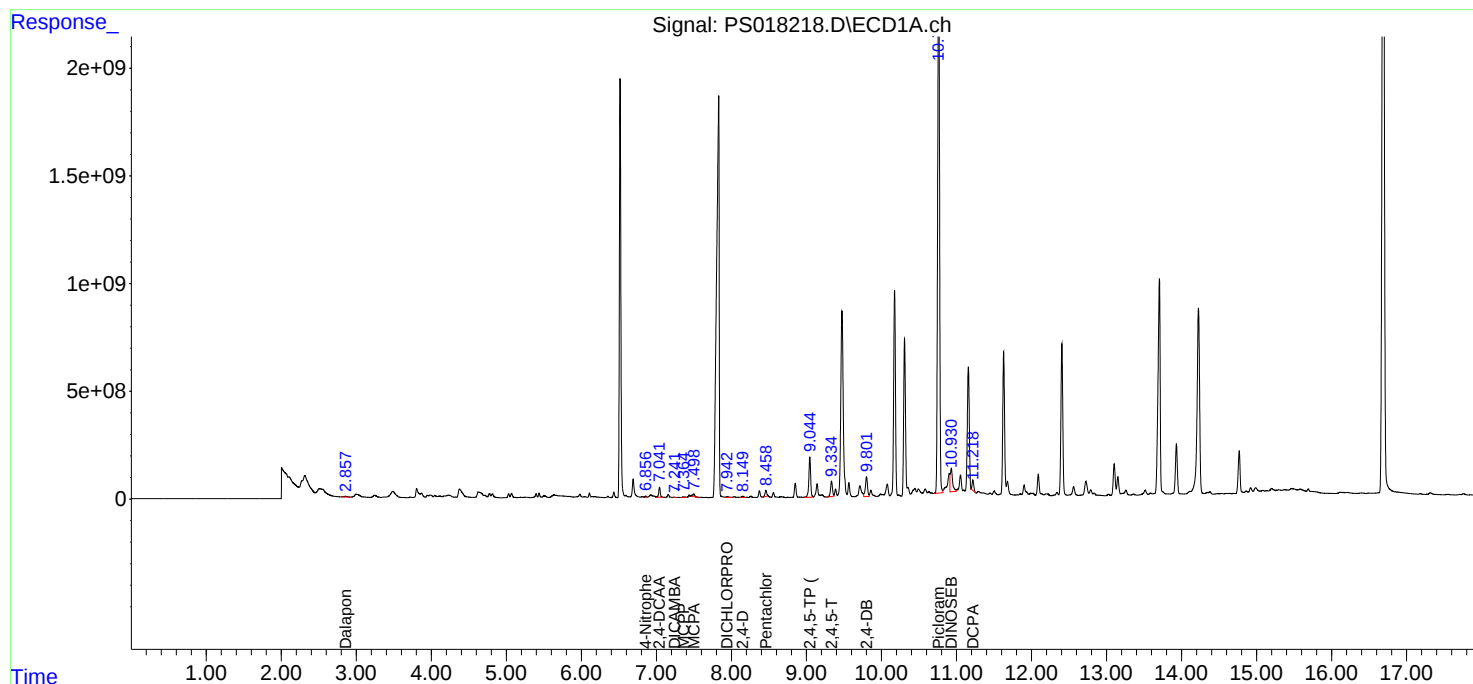


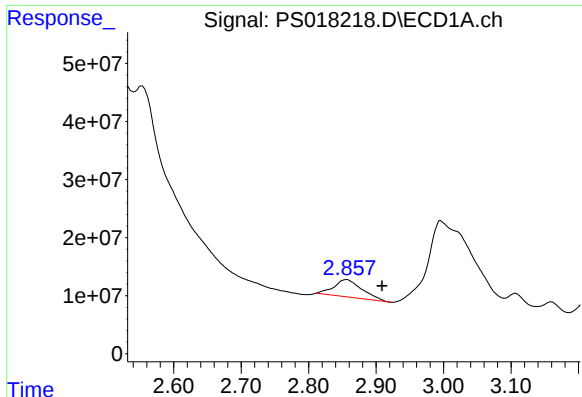

#1 Dalapon


R.T.: 2.856 min
Delta R.T.: -0.053 min
Response: 86395087
Conc: 35.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

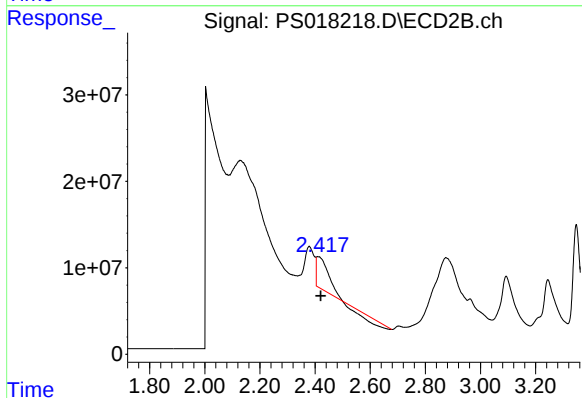


#1 Dalapon

R.T.: 2.409 min
Delta R.T.: -0.012 min
Response: 68701582
Conc: 89.84 ng/ml

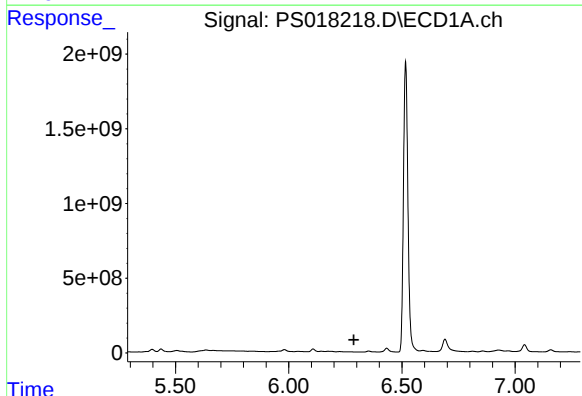


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.321 min
Delta R.T.: 0.033 min
Response: -3350202
Conc: N.D.

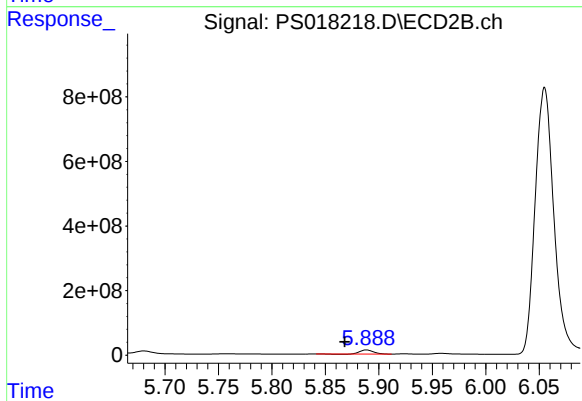

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.888 min
Delta R.T.: 0.021 min
Response: 107067704
Conc: 121.03 ng/ml

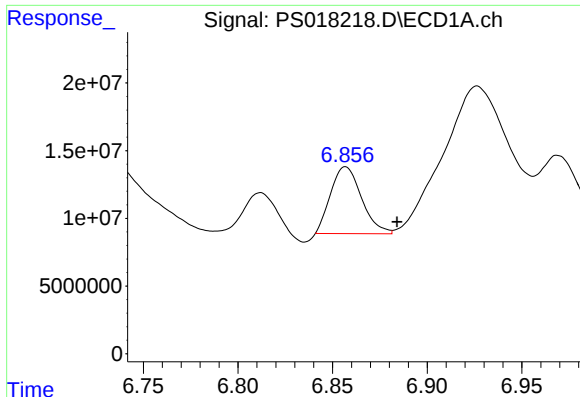

#3 4-Nitrophenol


R.T.: 6.857 min
Delta R.T.: -0.027 min
Response: 56118882
Conc: 69.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

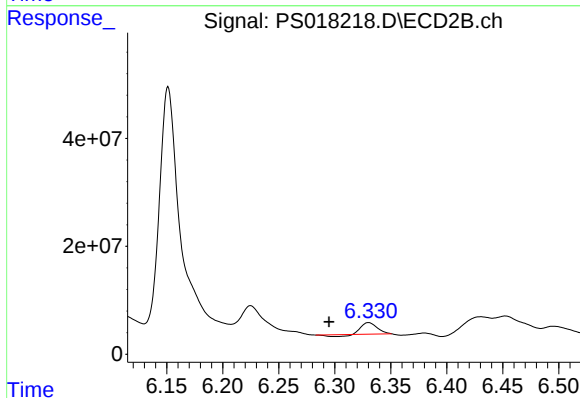


#3 4-Nitrophenol

R.T.: 6.330 min
Delta R.T.: 0.036 min
Response: 18475691
Conc: 60.28 ng/ml

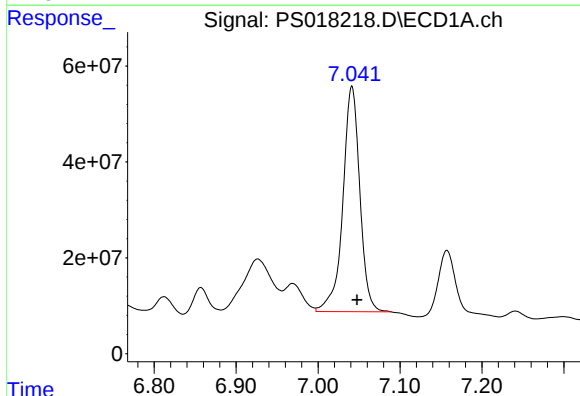


#4 2,4-DCAA

R.T.: 7.041 min
Delta R.T.: -0.006 min
Response: 678779323
Conc: 469.58 ng/ml

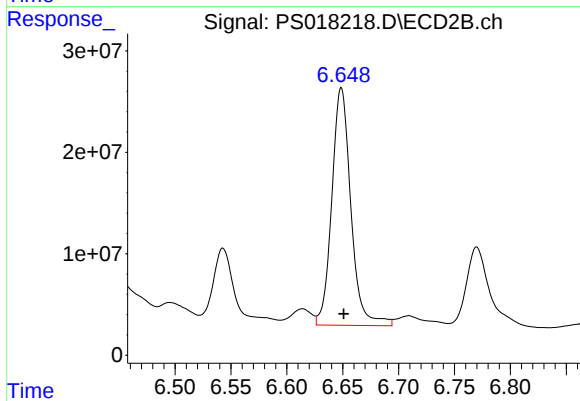

#4 2,4-DCAA


R.T.: 6.649 min
Delta R.T.: -0.002 min
Response: 278367321
Conc: 479.74 ng/ml

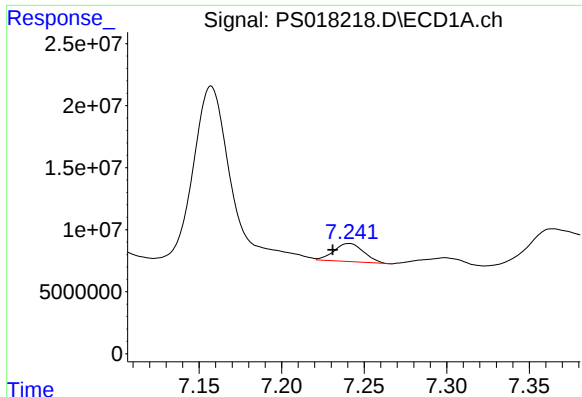

#5 DICAMBA


R.T.: 7.241 min
Delta R.T.: 0.010 min
Response: 18265946
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

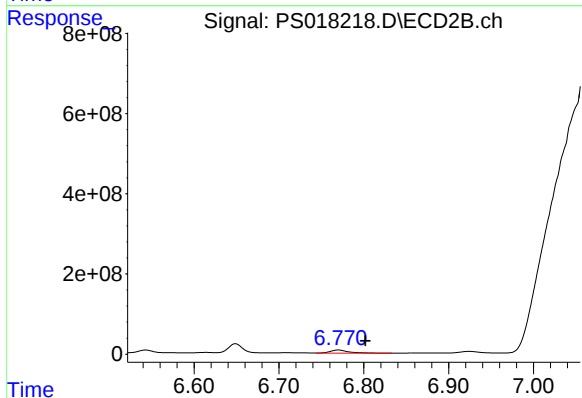


#5 DICAMBA

R.T.: 6.770 min
Delta R.T.: -0.032 min
Response: 115151048
Conc: 43.80 ng/ml

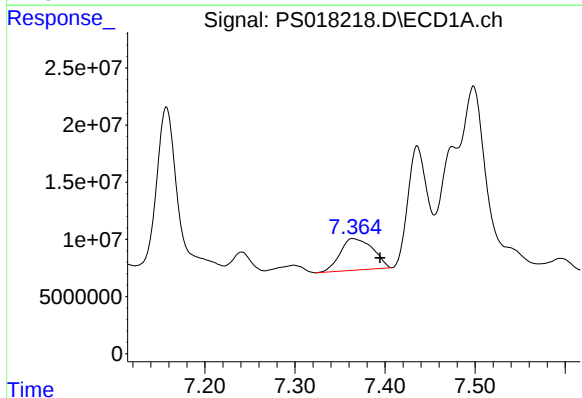


#6 MCP

R.T.: 7.365 min
Delta R.T.: -0.030 min
Response: 69338090
Conc: 14.85 ug/ml

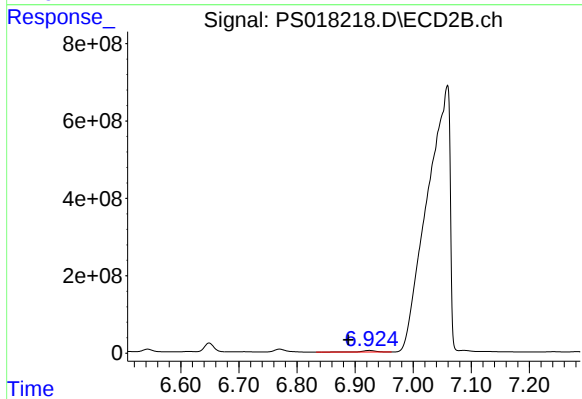

#6 MCP


R.T.: 6.924 min
Delta R.T.: 0.036 min
Response: 66897520
Conc: 31.10 ug/ml

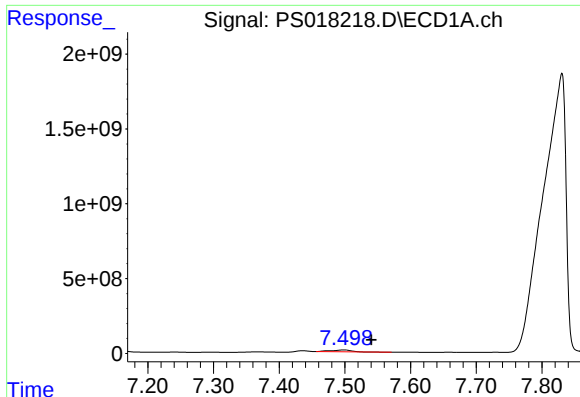

#7 MCPA


R.T.: 7.498 min
Delta R.T.: -0.042 min
Response: 266411053
Conc: 39.93 ug/ml

Instrument :
ECD_S
ClientSampleId :

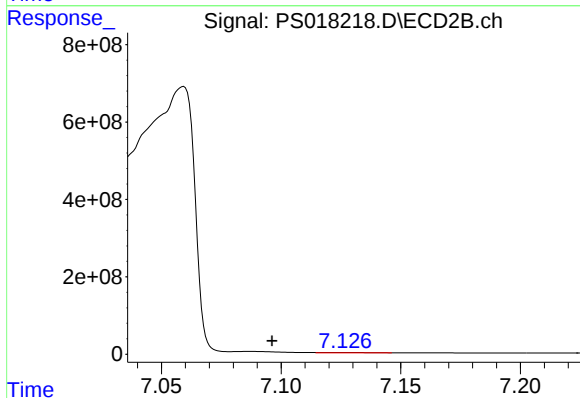


#7 MCPA

R.T.: 7.126 min
Delta R.T.: 0.030 min
Response: 10113266
Conc: 3.39 ug/ml

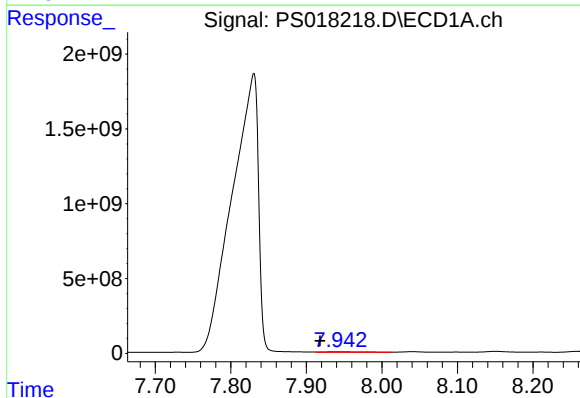


#8 DICHLORPROP

R.T.: 7.942 min
Delta R.T.: 0.024 min
Response: 143682023
Conc: 91.34 ng/ml

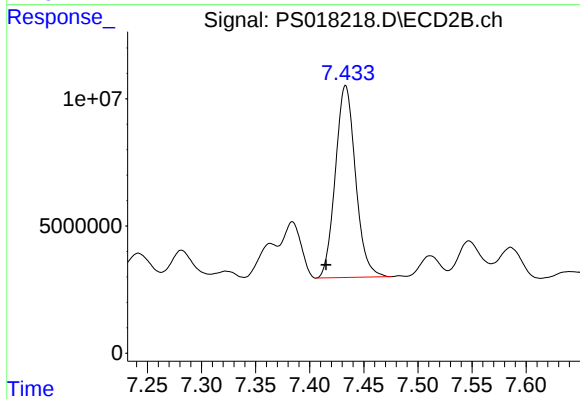

#8 DICHLORPROP


R.T.: 7.433 min
Delta R.T.: 0.018 min
Response: 97756097
Conc: 146.47 ng/ml

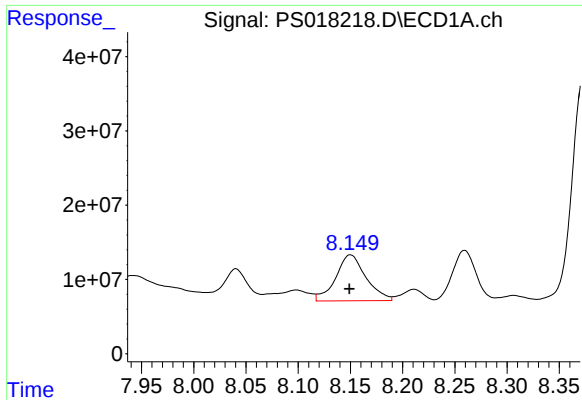

#9 2,4-D


R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 124653256
Conc: 68.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

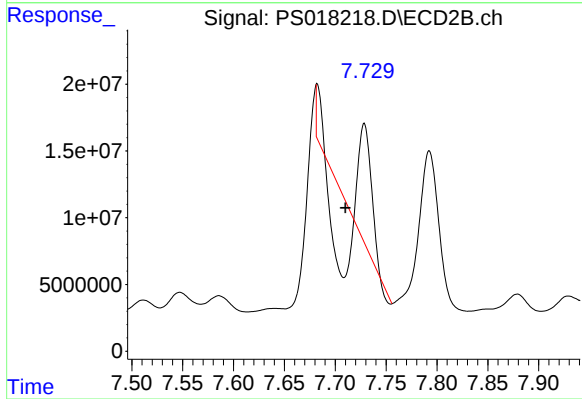


#9 2,4-D

R.T.: 7.729 min
Delta R.T.: 0.018 min
Response: 14313774
Conc: 19.45 ng/ml

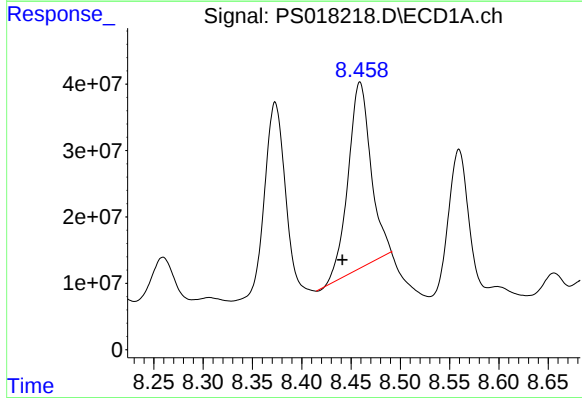


#10 Pentachlorophenol

R.T.: 8.459 min
Delta R.T.: 0.018 min
Response: 452711228
Conc: 21.43 ng/ml

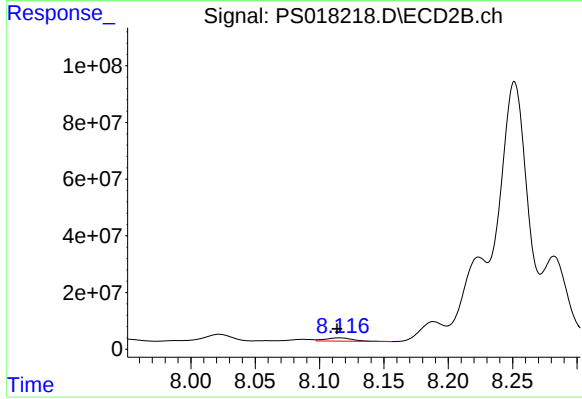

#10 Pentachlorophenol


R.T.: 8.116 min
Delta R.T.: 0.002 min
Response: 16479905
Conc: 1.96 ng/ml

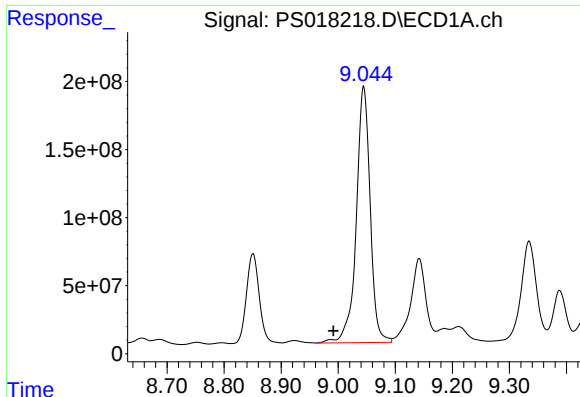

#11 2,4,5-TP (SILVEX)


R.T.: 9.045 min
Delta R.T.: 0.053 min
Response: 3180975300
Conc: 375.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

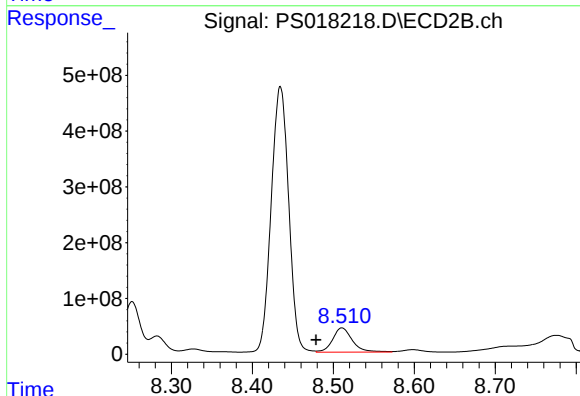


#11 2,4,5-TP (SILVEX)

R.T.: 8.511 min
Delta R.T.: 0.032 min
Response: 737838497
Conc: 206.99 ng/ml

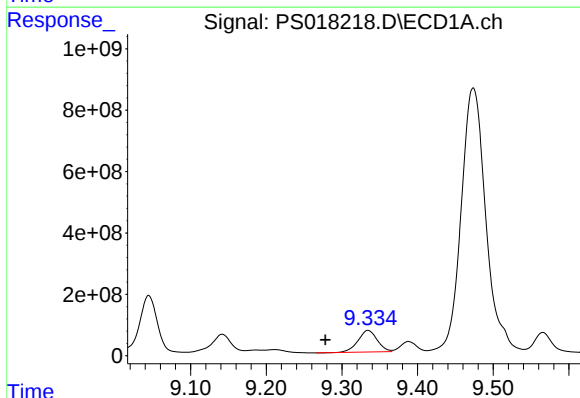


#12 2,4,5-T

R.T.: 9.335 min
Delta R.T.: 0.057 min
Response: 1249512474
Conc: 140.96 ng/ml

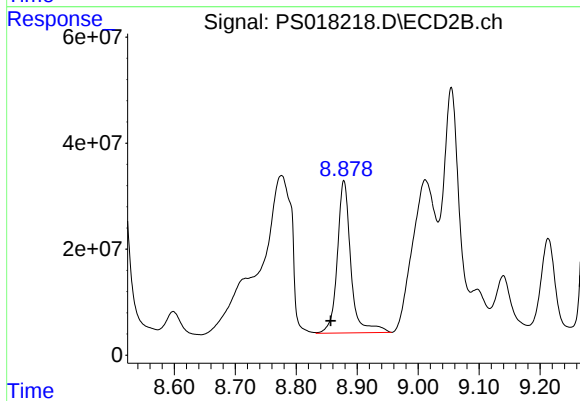

#12 2,4,5-T


R.T.: 8.878 min
Delta R.T.: 0.022 min
Response: 444373336
Conc: 135.85 ng/ml

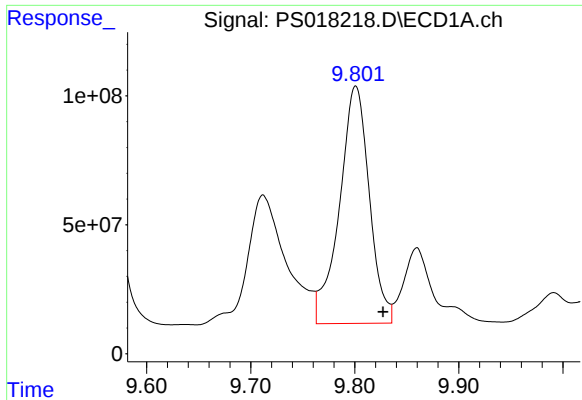

#13 2,4-DB


R.T.: 9.801 min
Delta R.T.: -0.026 min
Response: 1839798841
Conc: 1112.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

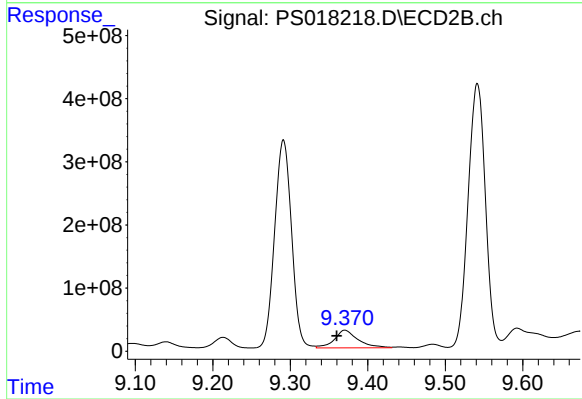


#13 2,4-DB

R.T.: 9.371 min
Delta R.T.: 0.011 min
Response: 590164720
Conc: 1333.83 ng/ml

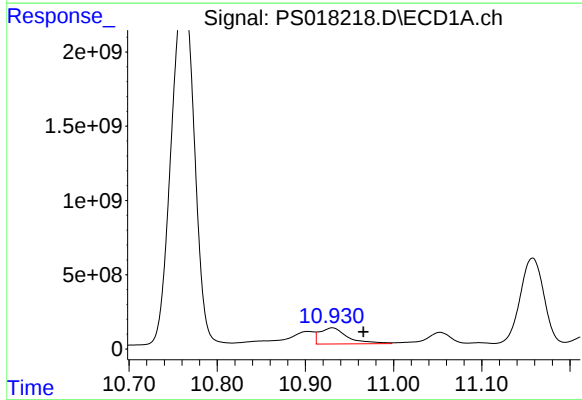


#14 DINOSEB

R.T.: 10.931 min
Delta R.T.: -0.035 min
Response: 2370005253
Conc: 360.90 ng/ml

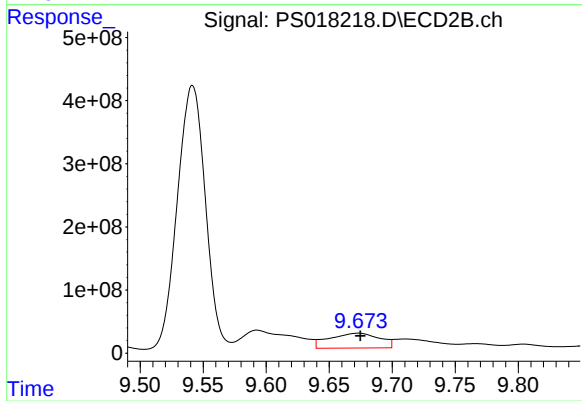

#14 DINOSEB


R.T.: 9.673 min
Delta R.T.: -0.002 min
Response: 648804818
Conc: 260.04 ng/ml

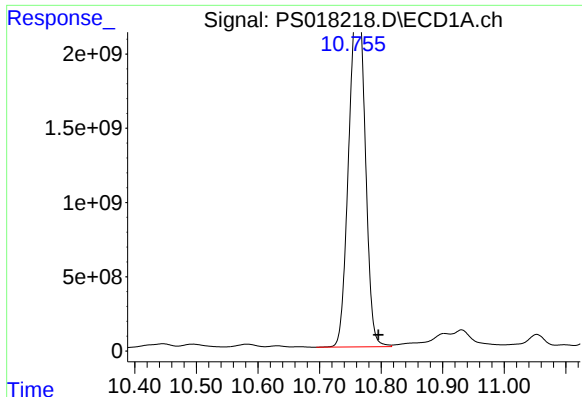

#15 Picloram


R.T.: 10.762 min
Delta R.T.: -0.034 min
Response: 42237951422
Conc: 3538.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

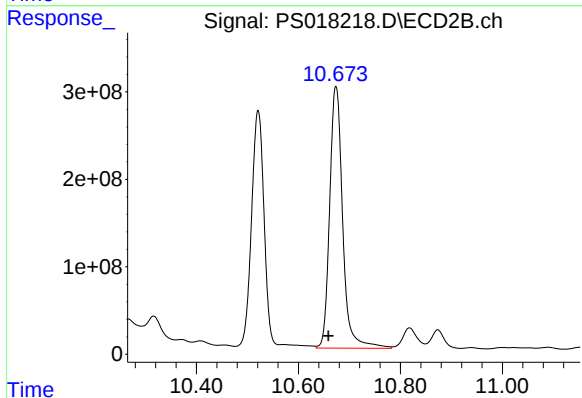


#15 Picloram

R.T.: 10.674 min
Delta R.T.: 0.015 min
Response: 5300248256
Conc: 1133.46 ng/ml

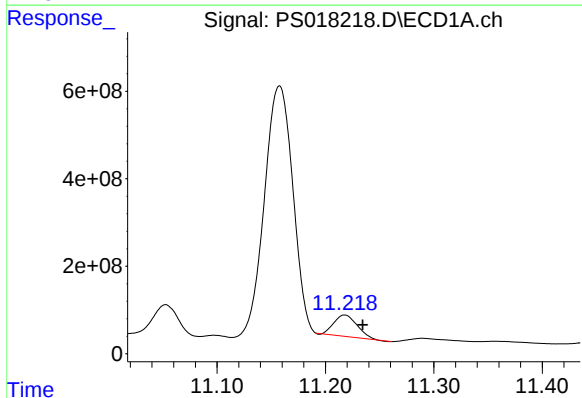

#16 DCPA

R.T.: 11.218 min
Delta R.T.: -0.017 min
Response: 726736464
Conc: 67.26 ng/ml

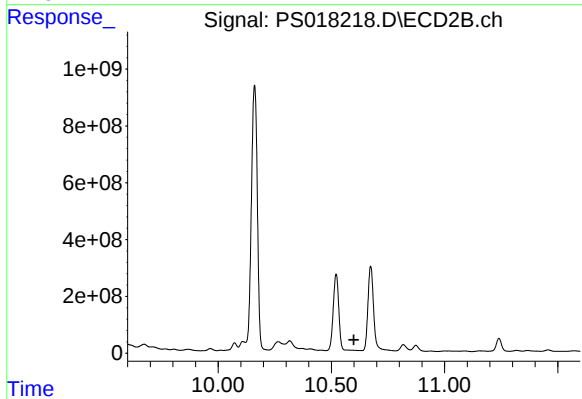

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.