

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020322\
 Data File : PS018219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 12:24
 Operator : AJ\MA
 Sample : N1335-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 22:22:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.041	6.648	888.4E6	364.0E6	614.609	627.392
Target Compounds							
1) T	Dalapon	2.857f	2.415	84820904	73972816	34.575	96.736 #
2) T	3,5-DICHL...	6.320	5.888	582439	107.5E6	<MDL	121.471 #
3) T	4-Nitroph...	6.858	6.329	19553767	17782380	24.210	58.013 #
5) T	DICAMBA	7.242	6.769	28074035	109.0E6	4.496	41.478 #
6) T	MCPD	7.359	6.866	58799390	7143740	12.594	3.321 #
7) T	MCPA	7.496f	7.060	155.3E6	19719.1E6	23.285	6608.424 #
8) T	DICHLORPROP	7.941	7.433	68086887	57253451	43.283	85.783 #
9) T	2,4-D	8.151	7.729	101.1E6	99983815	55.520	135.858 #
10) T	Pentachlo...	8.460	8.116	420.0E6	15777250	19.881	1.873 #
11) T	2,4,5-TP ...	8.988	8.511	27865375	861.2E6	3.293	241.594 #
12) T	2,4,5-T	9.336f	8.878	1716.4E6	396.7E6	193.631	121.289 #
13) T	2,4-DB	9.801	9.371	1760.5E6	588.4E6	1064.997	1329.834
14) T	DINOSEB	10.931	9.673	2613.0E6	593.4E6	397.901	237.846 #
15) T	Picloram	10.762	10.674	42484.7E6	4722.4E6	3559.402	1009.894 #
16) T	DCPA	11.219	0.000	777.7E6	0	71.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020322\
Data File : PS018219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 12:24
Operator : AJ\MA
Sample : N1335-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 22:22:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

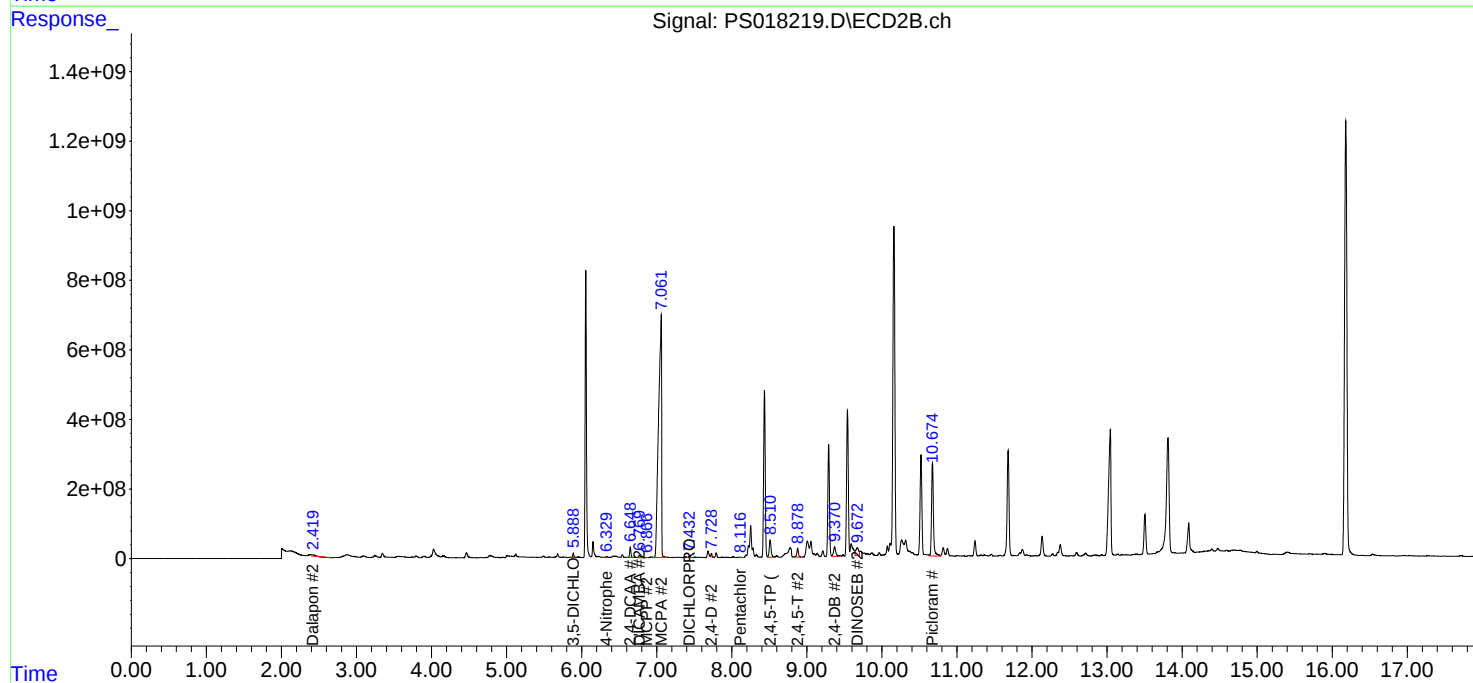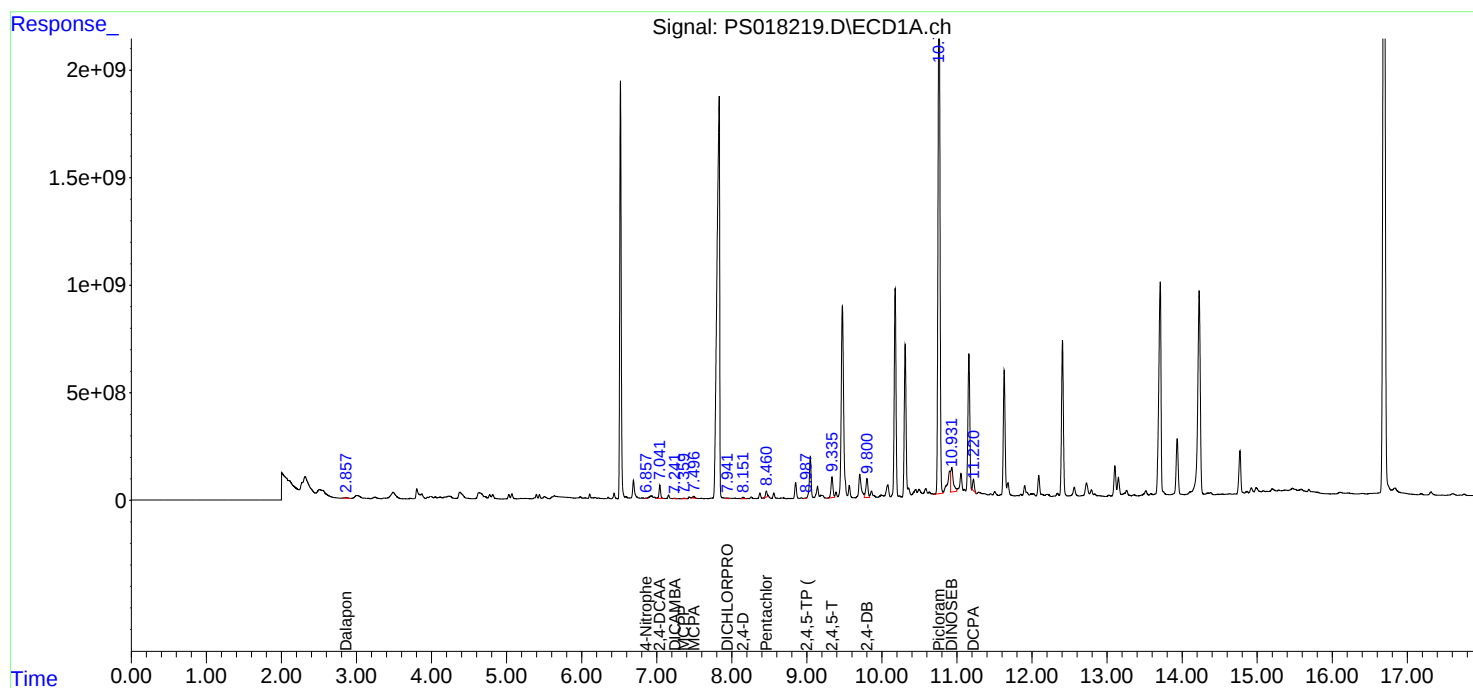


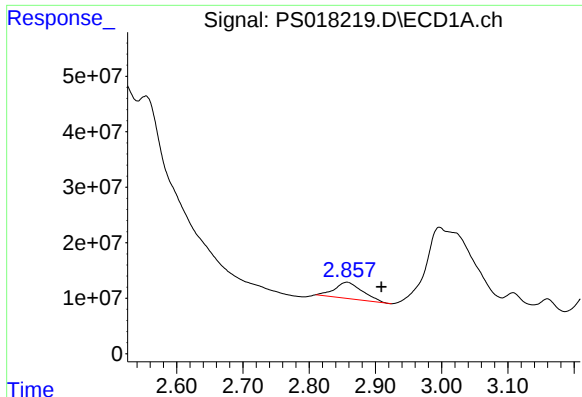

#1 Dalapon


R.T.: 2.857 min
Delta R.T.: -0.052 min
Response: 84820904
Conc: 34.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

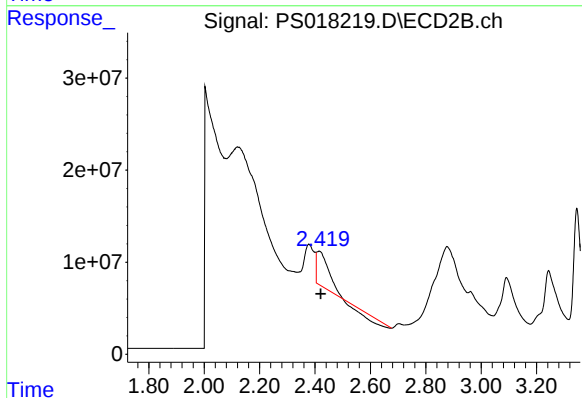


#1 Dalapon

R.T.: 2.415 min
Delta R.T.: -0.006 min
Response: 73972816
Conc: 96.74 ng/ml

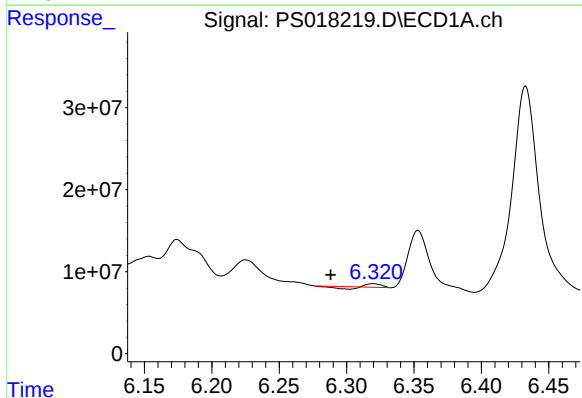


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.320 min
Delta R.T.: 0.032 min
Response: 582439
Conc: N.D.

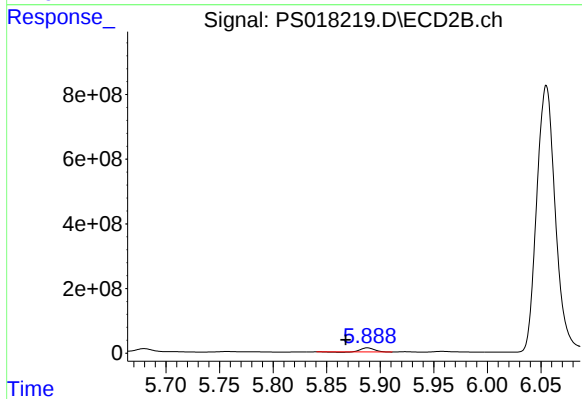

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.888 min
Delta R.T.: 0.020 min
Response: 107457179
Conc: 121.47 ng/ml

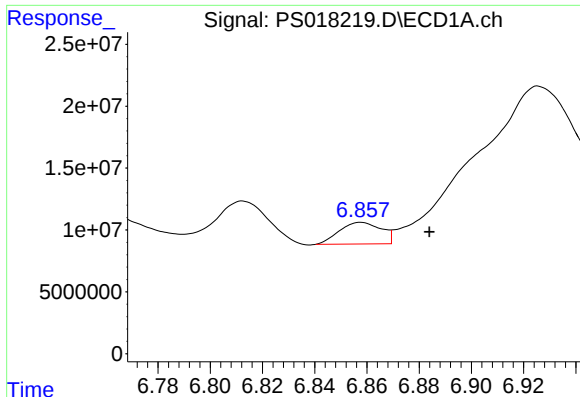

#3 4-Nitrophenol


R.T.: 6.858 min
Delta R.T.: -0.026 min
Response: 19553767
Conc: 24.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

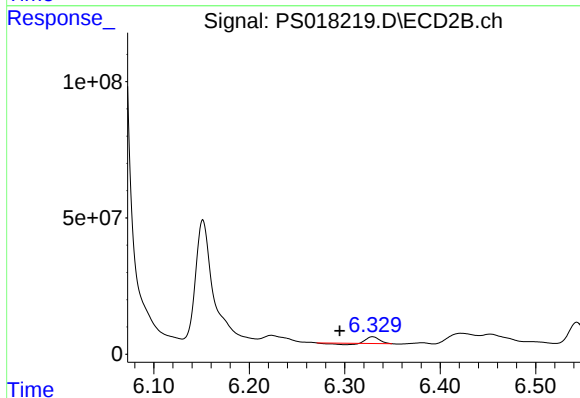


#3 4-Nitrophenol

R.T.: 6.329 min
Delta R.T.: 0.035 min
Response: 17782380
Conc: 58.01 ng/ml

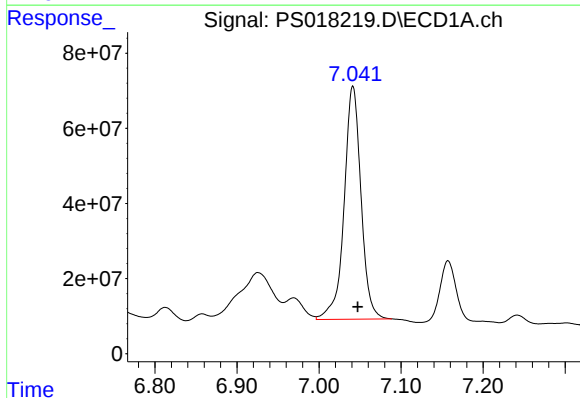


#4 2,4-DCAA

R.T.: 7.041 min
Delta R.T.: -0.006 min
Response: 888409228
Conc: 614.61 ng/ml

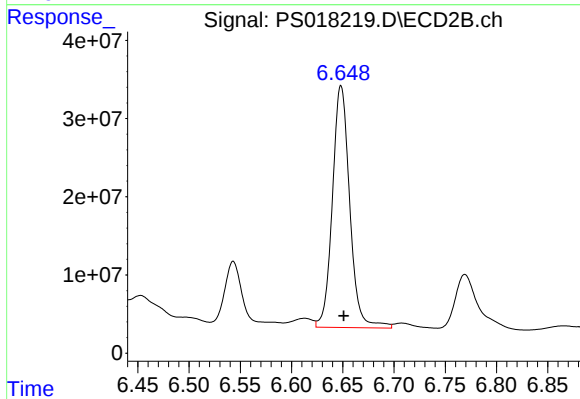

#4 2,4-DCAA


R.T.: 6.648 min
Delta R.T.: -0.003 min
Response: 364043746
Conc: 627.39 ng/ml

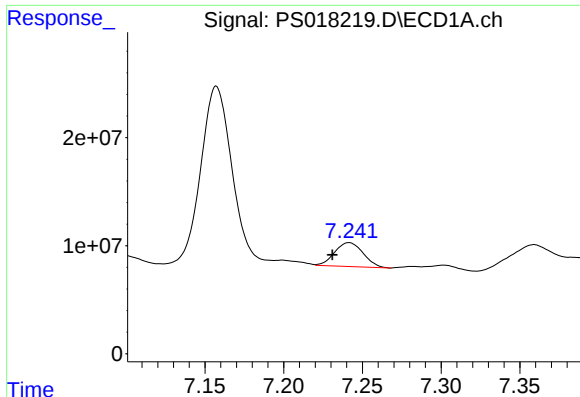

#5 DICAMBA


R.T.: 7.242 min
Delta R.T.: 0.011 min
Response: 28074035
Conc: 4.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

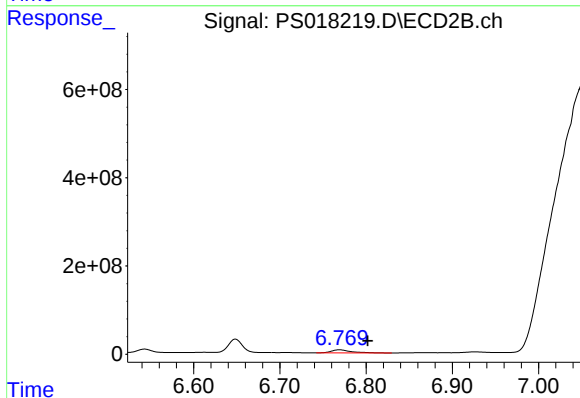


#5 DICAMBA

R.T.: 6.769 min
Delta R.T.: -0.033 min
Response: 109047212
Conc: 41.48 ng/ml

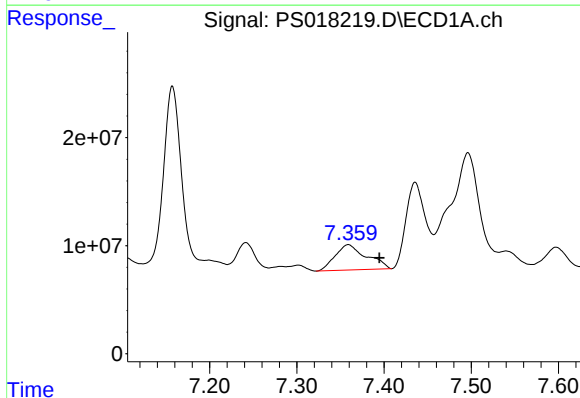


#6 MCP

R.T.: 7.359 min
Delta R.T.: -0.035 min
Response: 58799390
Conc: 12.59 ug/ml

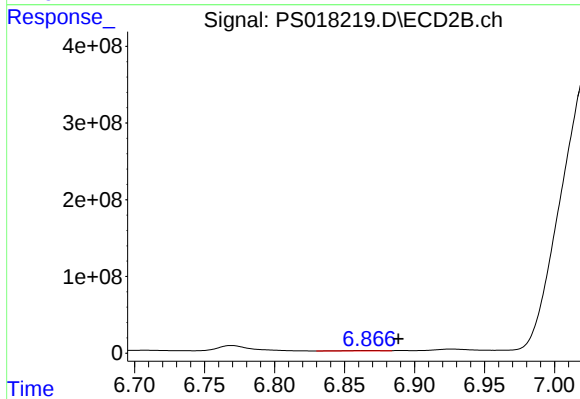

#6 MCP


R.T.: 6.866 min
Delta R.T.: -0.022 min
Response: 7143740
Conc: 3.32 ug/ml

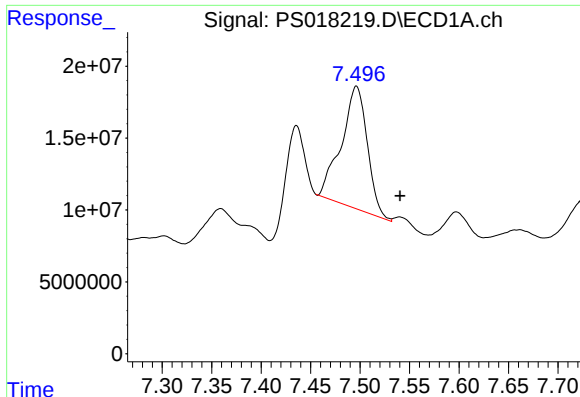

#7 MCPA


R.T.: 7.496 min
Delta R.T.: -0.044 min
Response: 155348950
Conc: 23.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

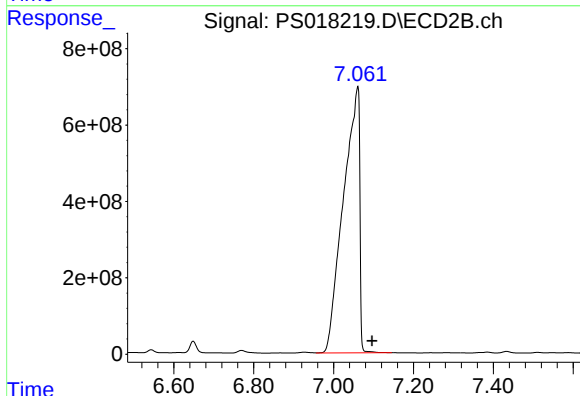


#7 MCPA

R.T.: 7.060 min
Delta R.T.: -0.036 min
Response: 19719079032
Conc: 6608.42 ug/ml

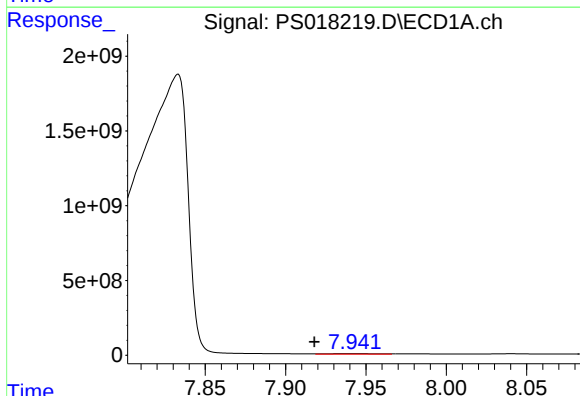


#8 DICHLORPROP

R.T.: 7.941 min
Delta R.T.: 0.023 min
Response: 68086887
Conc: 43.28 ng/ml

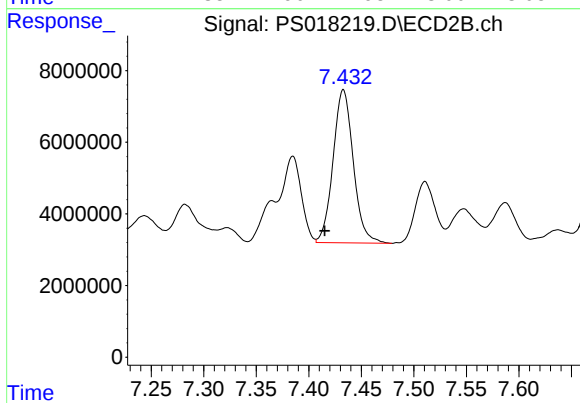

#8 DICHLORPROP


R.T.: 7.433 min
Delta R.T.: 0.018 min
Response: 57253451
Conc: 85.78 ng/ml

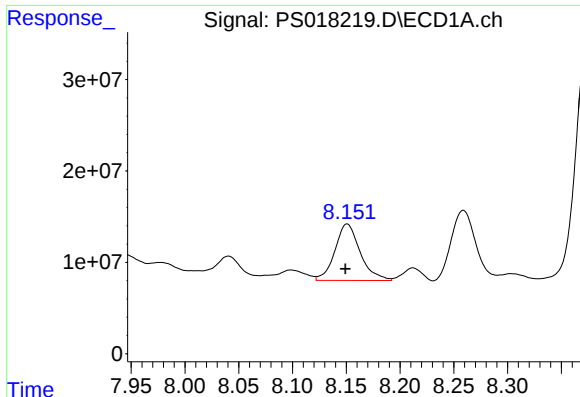

#9 2,4-D


R.T.: 8.151 min
Delta R.T.: 0.002 min
Response: 101098186
Conc: 55.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

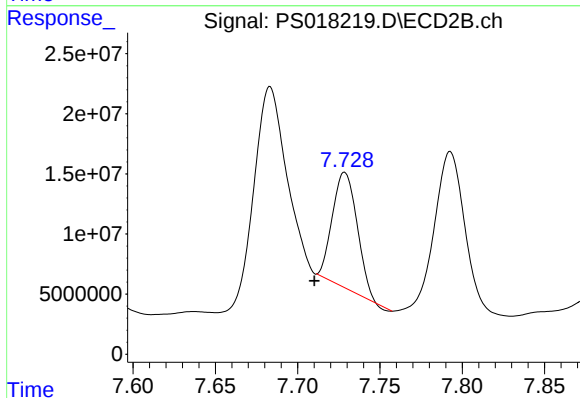


#9 2,4-D

R.T.: 7.729 min
Delta R.T.: 0.018 min
Response: 99983815
Conc: 135.86 ng/ml

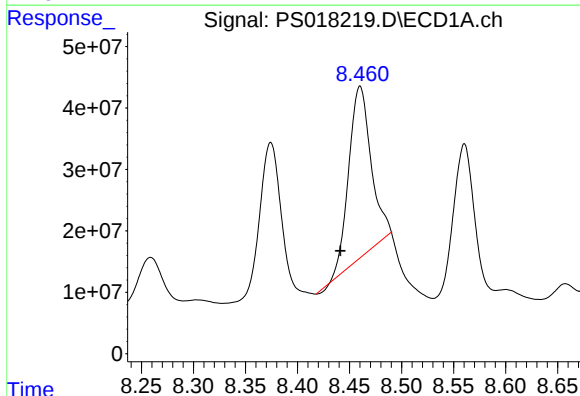


#10 Pentachlorophenol

R.T.: 8.460 min
Delta R.T.: 0.019 min
Response: 420004877
Conc: 19.88 ng/ml

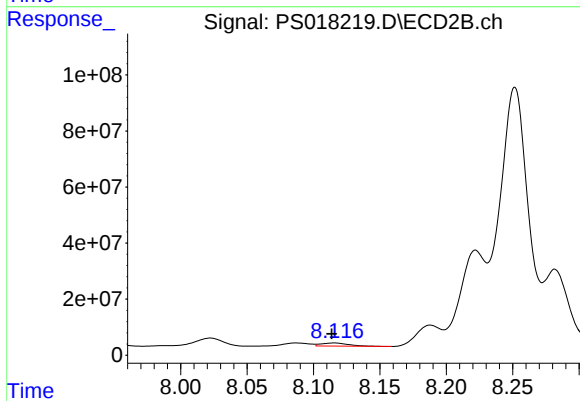

#10 Pentachlorophenol


R.T.: 8.116 min
Delta R.T.: 0.002 min
Response: 15777250
Conc: 1.87 ng/ml

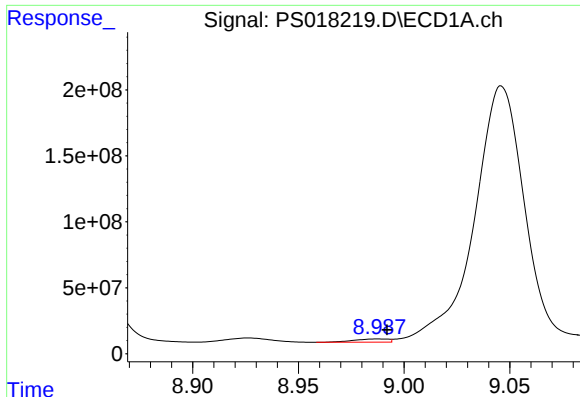

#11 2,4,5-TP (SILVEX)


R.T.: 8.988 min
Delta R.T.: -0.004 min
Response: 27865375
Conc: 3.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

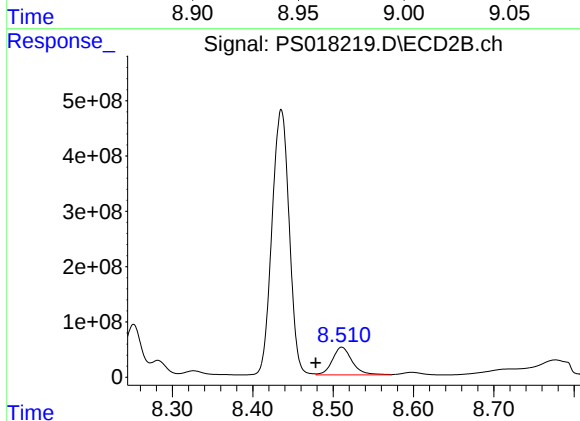


#11 2,4,5-TP (SILVEX)

R.T.: 8.511 min
Delta R.T.: 0.032 min
Response: 861206690
Conc: 241.59 ng/ml

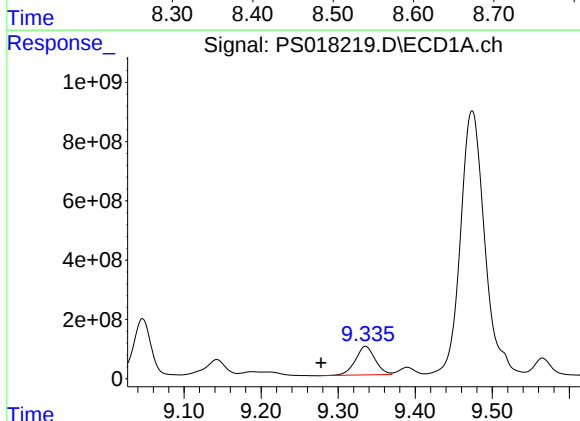


#12 2,4,5-T

R.T.: 9.336 min
Delta R.T.: 0.058 min
Response: 1716370223
Conc: 193.63 ng/ml

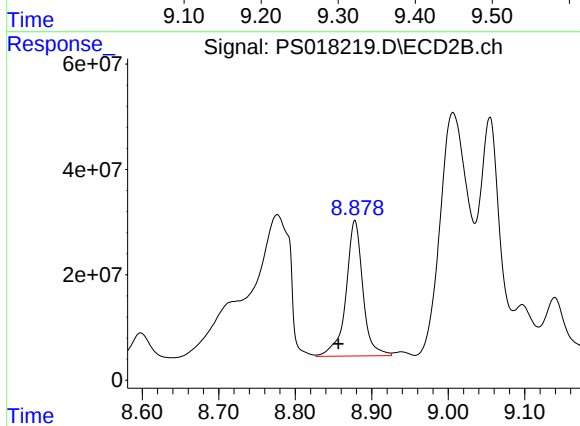

#12 2,4,5-T


R.T.: 8.878 min
Delta R.T.: 0.021 min
Response: 396739410
Conc: 121.29 ng/ml

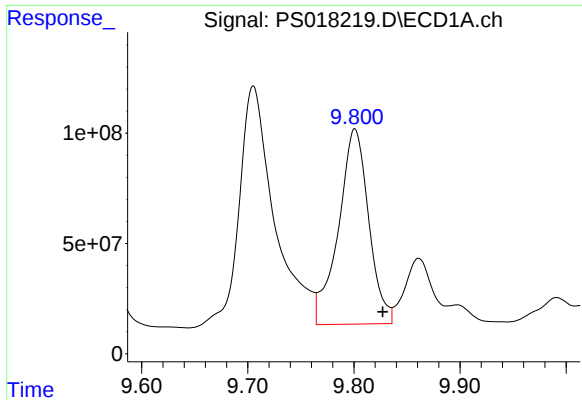

#13 2,4-DB


R.T.: 9.801 min
Delta R.T.: -0.026 min
Response: 1760476727
Conc: 1065.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

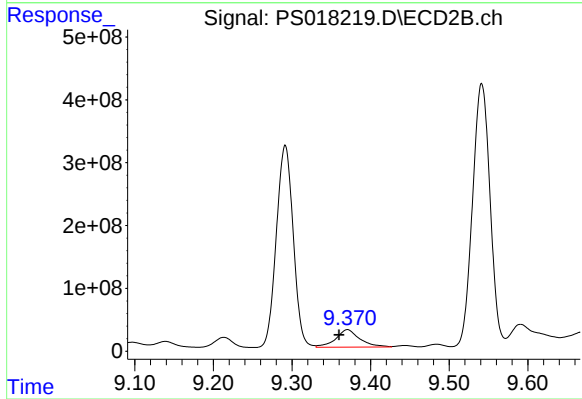


#13 2,4-DB

R.T.: 9.371 min
Delta R.T.: 0.011 min
Response: 588394746
Conc: 1329.83 ng/ml

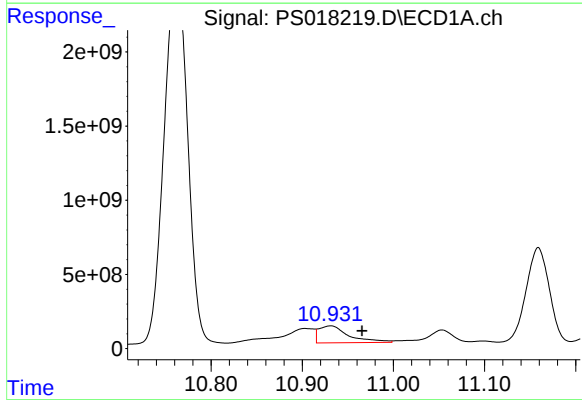


#14 DINOSEB

R.T.: 10.931 min
Delta R.T.: -0.035 min
Response: 2612995825
Conc: 397.90 ng/ml

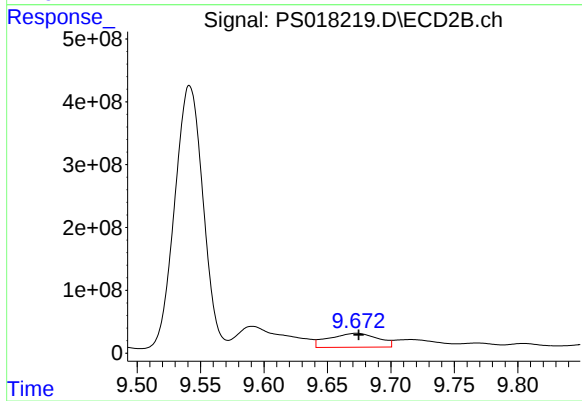

#14 DINOSEB


R.T.: 9.673 min
Delta R.T.: -0.002 min
Response: 593429640
Conc: 237.85 ng/ml

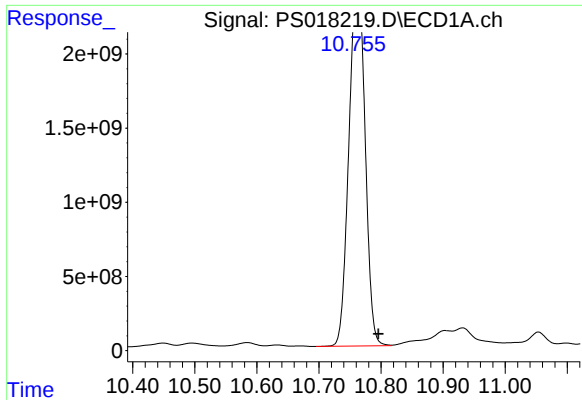

#15 Picloram


R.T.: 10.762 min
Delta R.T.: -0.034 min
Response: 42484715789
Conc: 3559.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

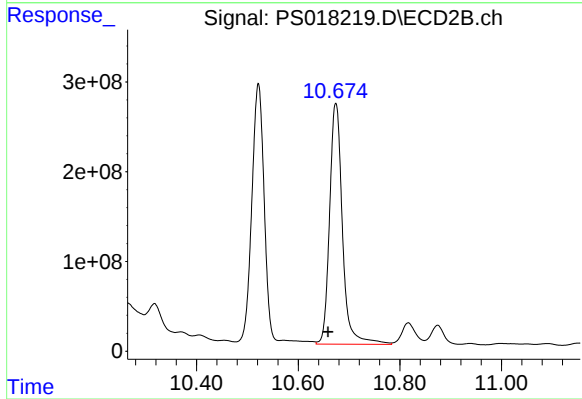


#15 Picloram

R.T.: 10.674 min
Delta R.T.: 0.015 min
Response: 4722414241
Conc: 1009.89 ng/ml

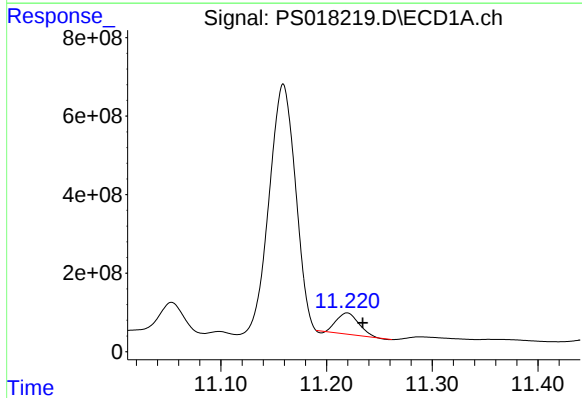

#16 DCPA

R.T.: 11.219 min
Delta R.T.: -0.015 min
Response: 777726149
Conc: 71.98 ng/ml

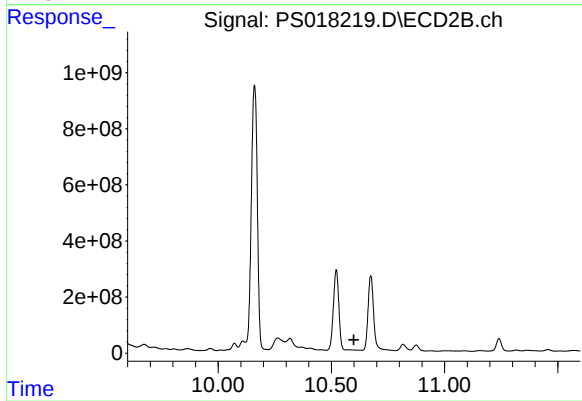

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.