

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
 Data File : PS018416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 09:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:19:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.032	6.643	582.2E6	354.9E6	349.888	532.601 #
Target Compounds							
5) T	DICAMBA	0.000	6.800	0	9061595	N.D.	3.227
9) T	2,4-D	0.000	7.761f	0	3440759	N.D.	3.676
10) T	Pentachlo...	8.429	8.112	4967987	2888907	<MDL	<MDL #
11) T	2,4,5-TP ...	8.981	8.443	8438319	24035624	<MDL	5.822 #
12) T	2,4,5-T	9.222	8.893f	100.4E6	8608837	9.985	2.187 #
13) T	2,4-DB	0.000	9.291f	0	13058199	N.D.	24.170
14) T	DINOSEB	10.938	9.672	98233688	5498315	12.644	1.891 #
15) T	Picloram	10.763	10.689f	2358363	246.5E6	<MDL	42.620 #
16) T	DCPA	11.209	10.591	15168347	9725065	1.261	1.959 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
Data File : PS018416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 09:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:19:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

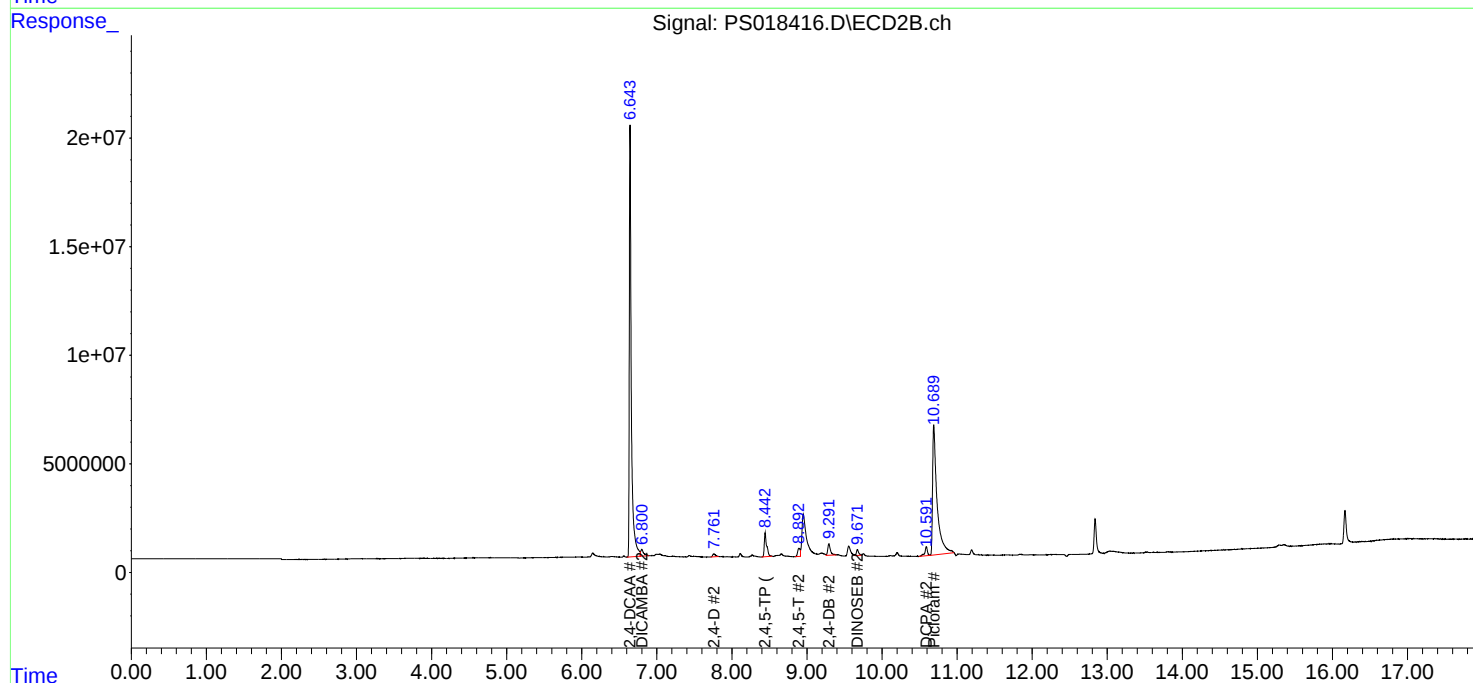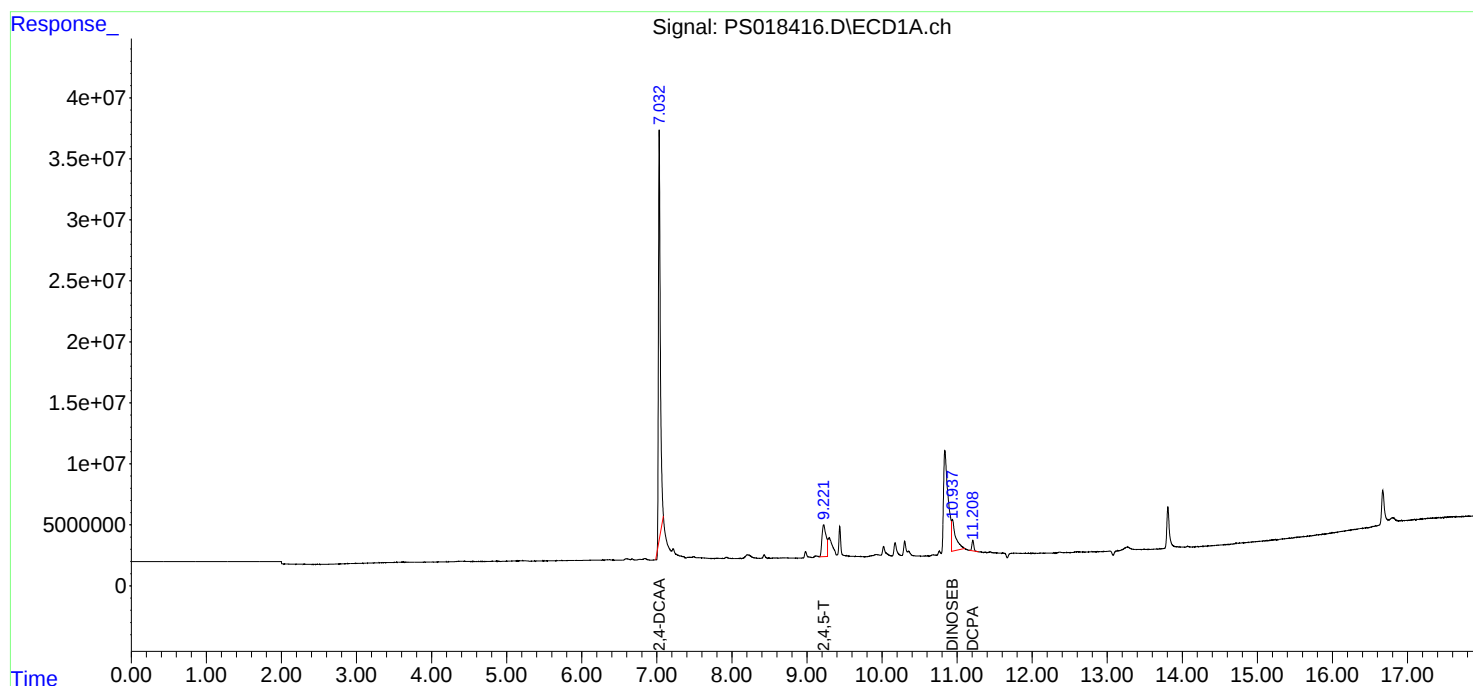


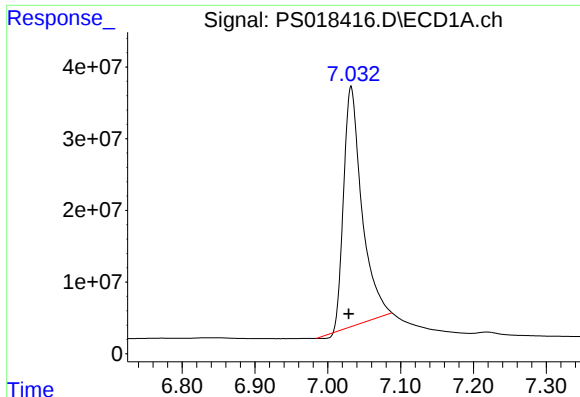

#4 2,4-DCAA


R.T.: 7.032 min
Delta R.T.: 0.003 min
Response: 582231088
Conc: 349.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

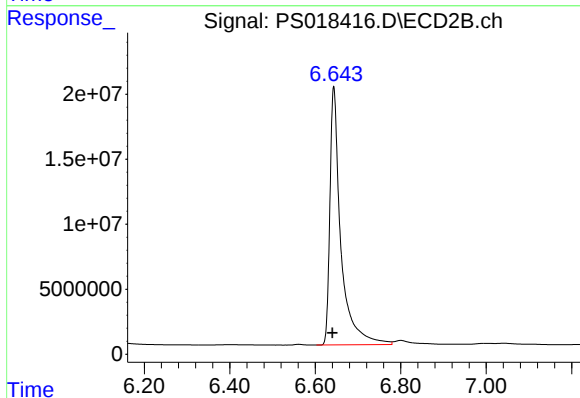


#4 2,4-DCAA

R.T.: 6.643 min
Delta R.T.: 0.003 min
Response: 354894608
Conc: 532.60 ng/ml

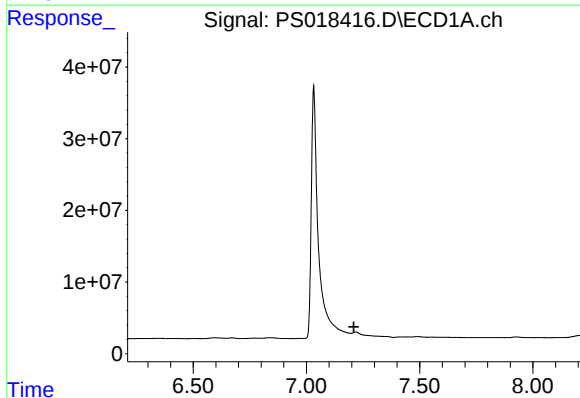


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.

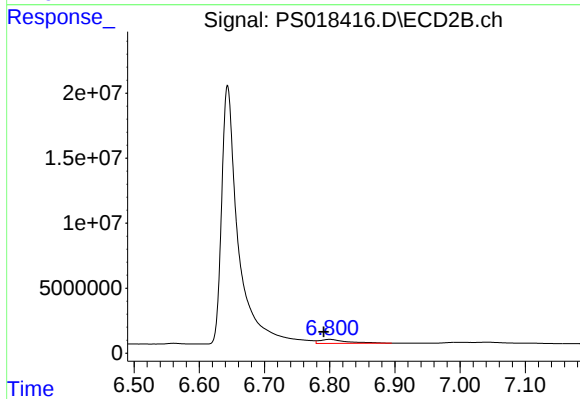

#5 DICAMBA


R.T.: 6.800 min
Delta R.T.: 0.009 min
Response: 9061595
Conc: 3.23 ng/ml

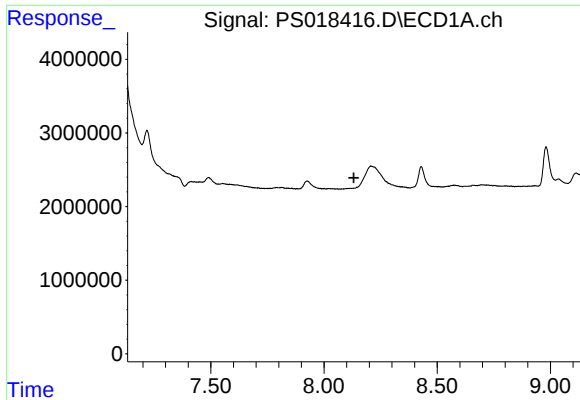

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

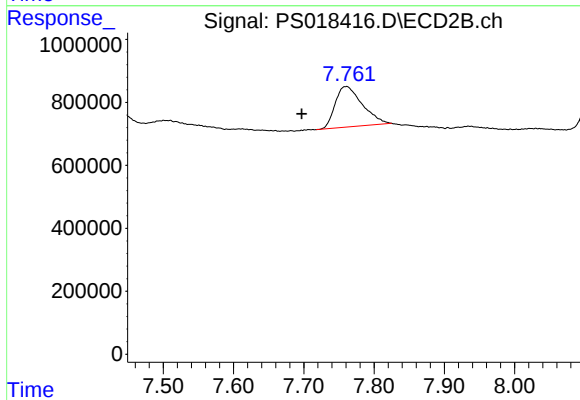


#9 2,4-D

R.T.: 7.761 min
Delta R.T.: 0.063 min
Response: 3440759
Conc: 3.68 ng/ml

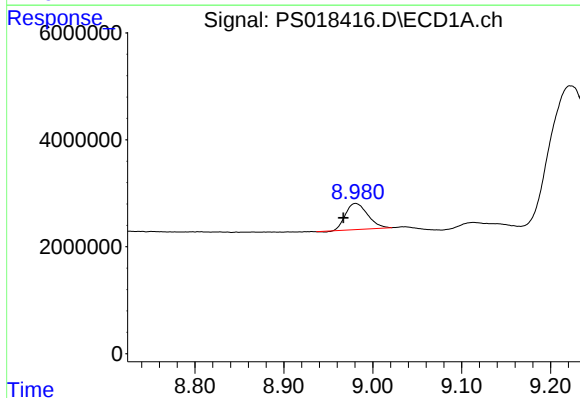


#11 2,4,5-TP (SILVEX)

R.T.: 8.981 min
Delta R.T.: 0.014 min
Response: 8438319
Conc: N.D.

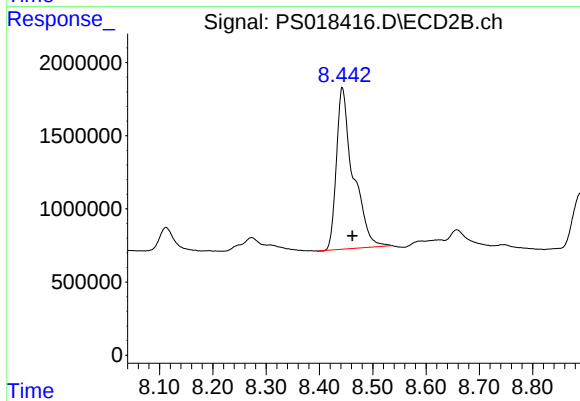

#11 2,4,5-TP (SILVEX)


R.T.: 8.443 min
Delta R.T.: -0.019 min
Response: 24035624
Conc: 5.82 ng/ml

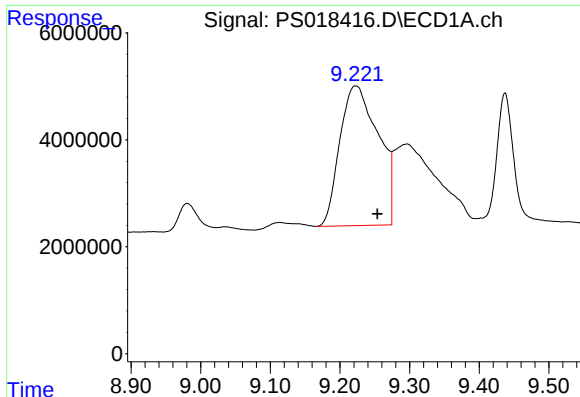

#12 2,4,5-T


R.T.: 9.222 min
Delta R.T.: -0.031 min
Response: 100445677
Conc: 9.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

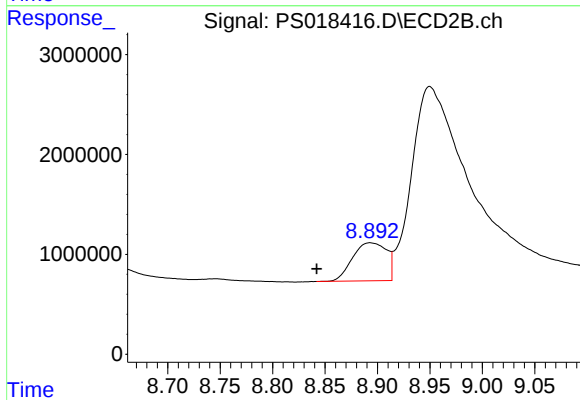


#12 2,4,5-T

R.T.: 8.893 min
Delta R.T.: 0.051 min
Response: 8608837
Conc: 2.19 ng/ml

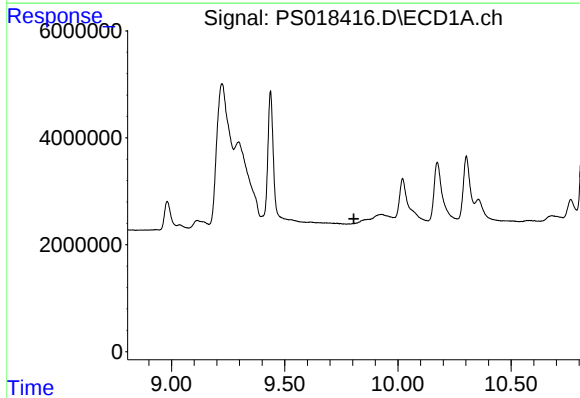


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.806 min
Response: 0
Conc: N.D.

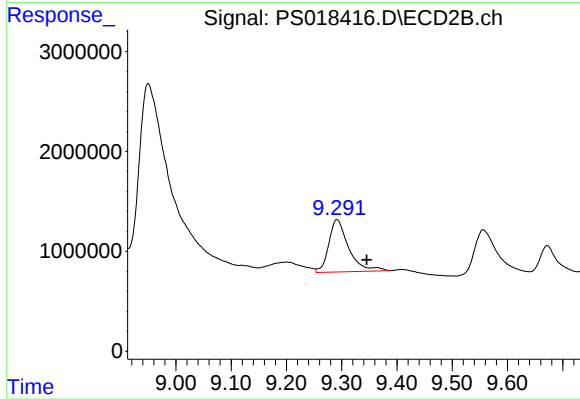

#13 2,4-DB


R.T.: 9.291 min
Delta R.T.: -0.054 min
Response: 13058199
Conc: 24.17 ng/ml

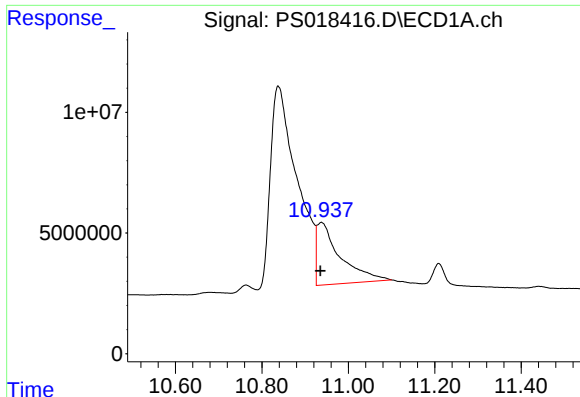

#14 DINOSEB


R.T.: 10.938 min
Delta R.T.: 0.002 min
Response: 98233688
Conc: 12.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

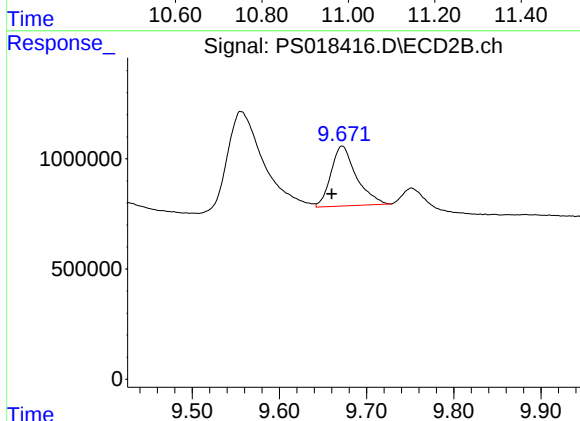


#14 DINOSEB

R.T.: 9.672 min
Delta R.T.: 0.012 min
Response: 5498315
Conc: 1.89 ng/ml

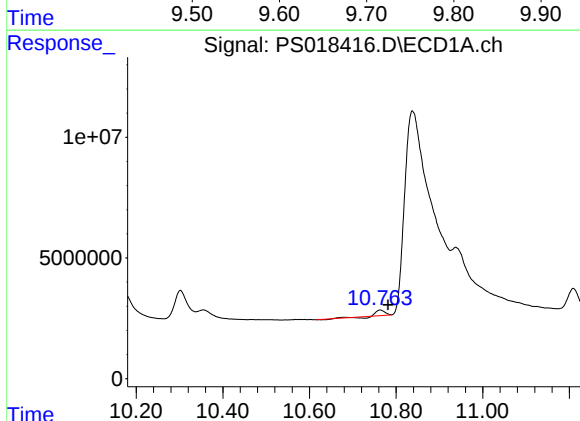


#15 Picloram

R.T.: 10.763 min
Delta R.T.: -0.018 min
Response: 2358363
Conc: N.D.

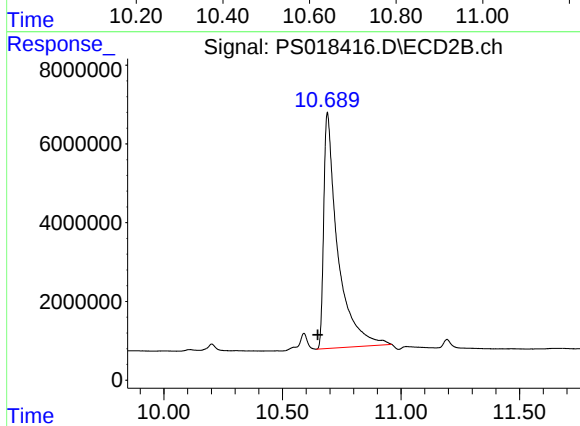

#15 Picloram


R.T.: 10.689 min
Delta R.T.: 0.040 min
Response: 246470571
Conc: 42.62 ng/ml

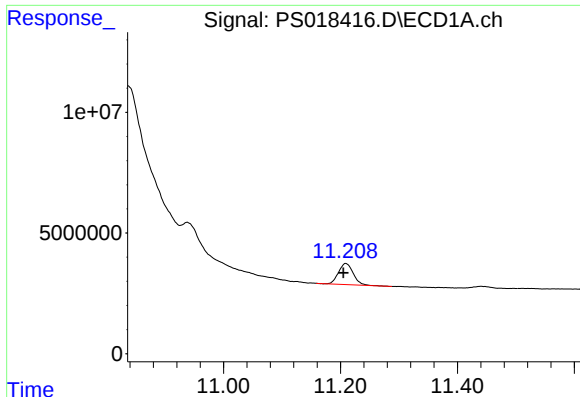

#16 DCPA

R.T.: 11.209 min
Delta R.T.: 0.004 min
Response: 15168347
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

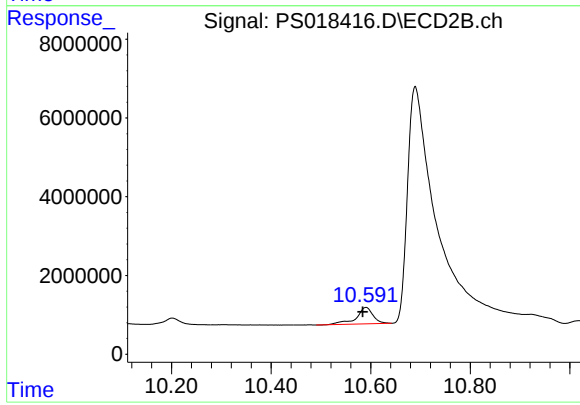

#16 DCPA

R.T.: 10.591 min
Delta R.T.: 0.006 min
Response: 9725065
Conc: 1.96 ng/ml