

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
 Data File : PS018426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 19:53
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:22:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.025	6.639	733.2E6	368.8E6	440.607	553.426 #
Target Compounds							
5) T	DICAMBA	0.000	6.795	0	1535724	N.D.	<MDL
9) T	2,4-D	8.192f	0.000	4014614	0	1.968	N.D. #
10) T	Pentachlo...	8.422	8.106	3549683	2231185	<MDL	<MDL #
11) T	2,4,5-TP ...	9.023f	8.431	9022158	11906784	<MDL	2.884 #
12) T	2,4,5-T	9.198f	0.000	11998628	0	1.193	N.D. #
13) T	2,4-DB	9.834	9.357	6977202	4597689	4.015	8.510 #
14) T	DINOSEB	10.912	9.676	42924049	13962322	5.525	4.803
15) T	Picloram	10.754	10.687	4990379	31175318	<MDL	5.391 #
16) T	DCPA	11.142f	10.517f	556392	4220657	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
Data File : PS018426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 19:53
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:22:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

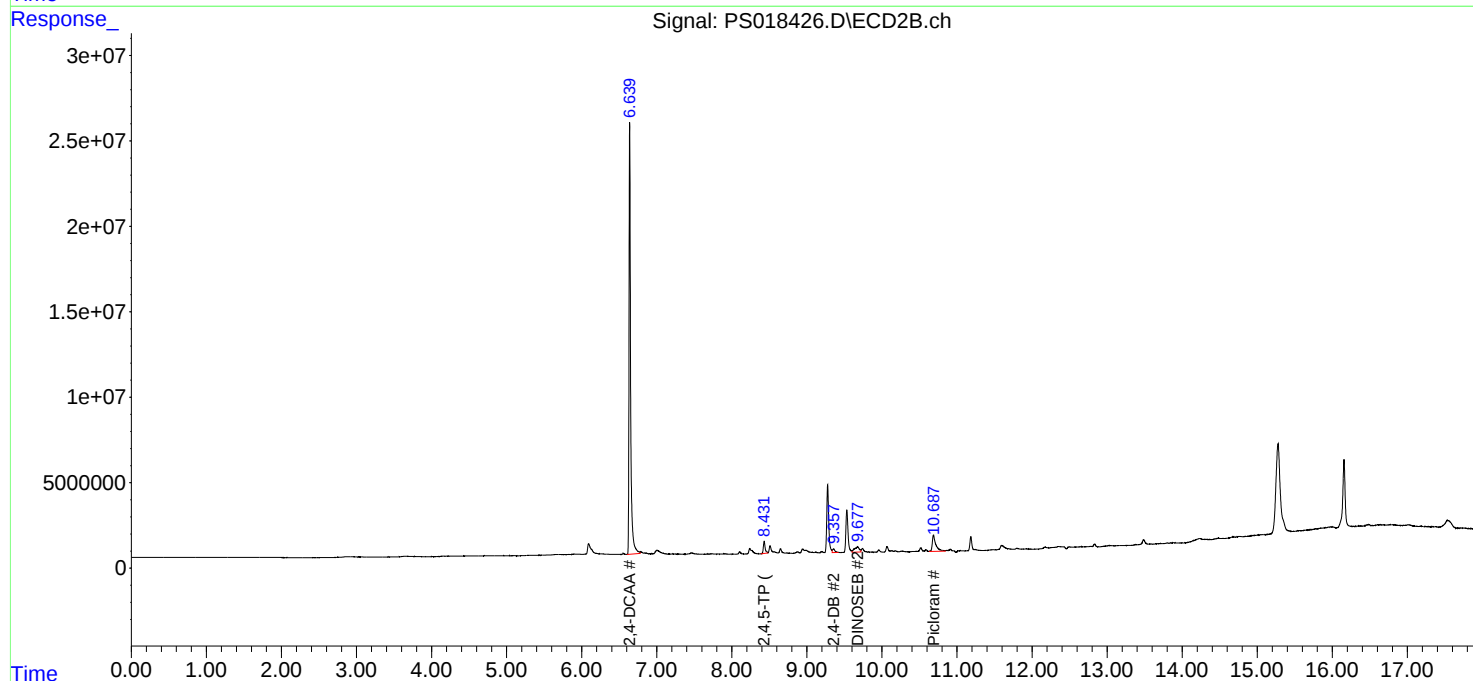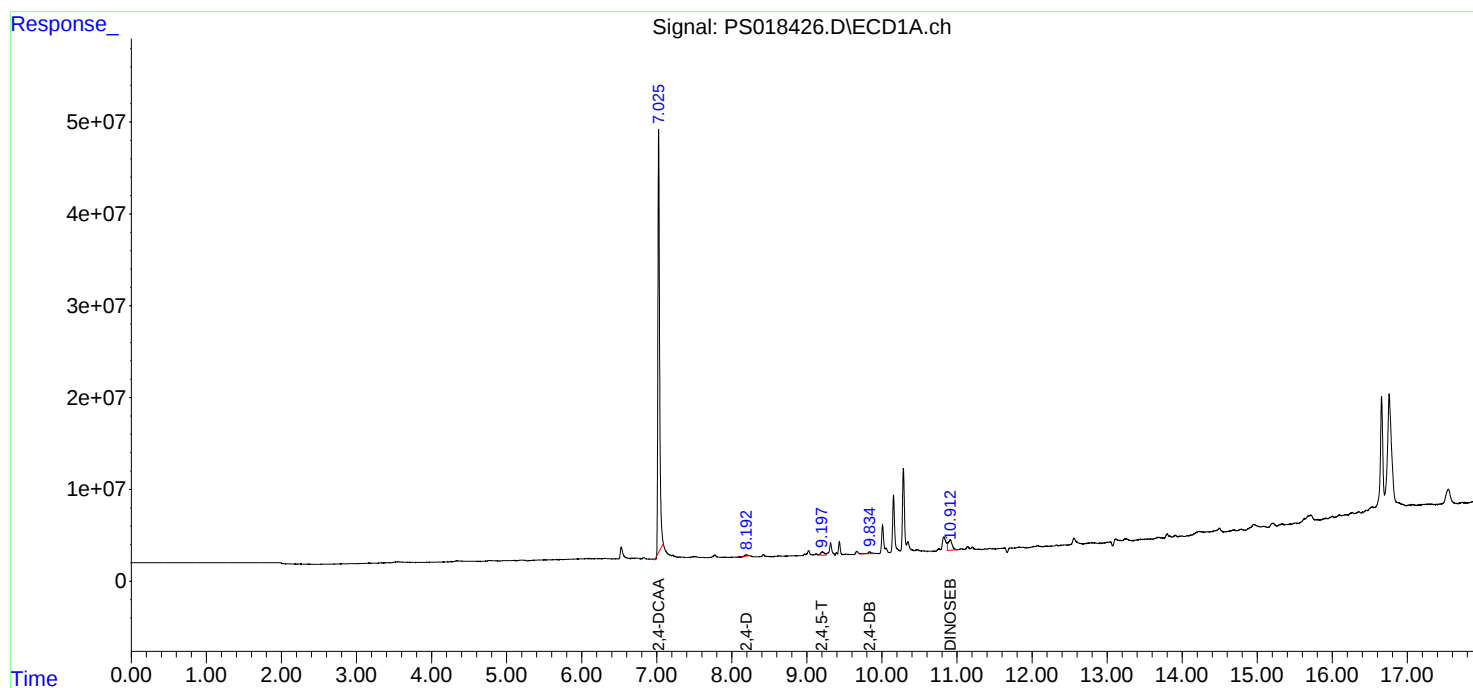


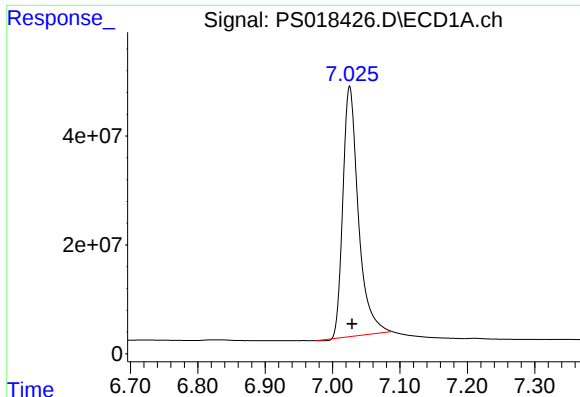

#4 2,4-DCAA


R.T.: 7.025 min
Delta R.T.: -0.003 min
Response: 733192864
Conc: 440.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

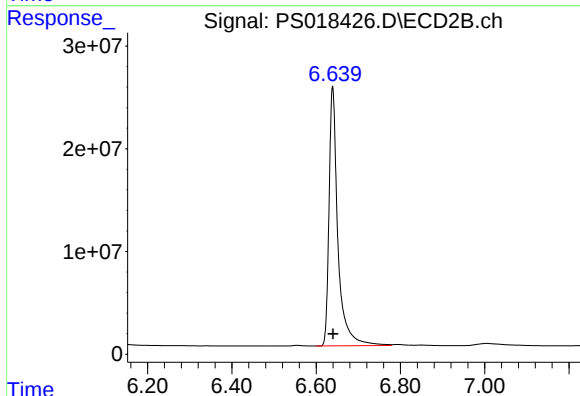


#4 2,4-DCAA

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 368771115
Conc: 553.43 ng/ml

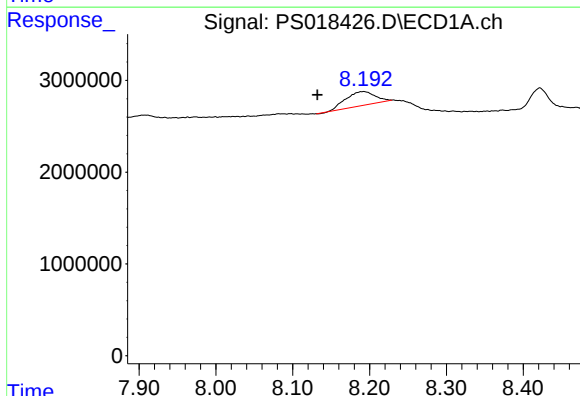


#9 2,4-D

R.T.: 8.192 min
Delta R.T.: 0.060 min
Response: 4014614
Conc: 1.97 ng/ml

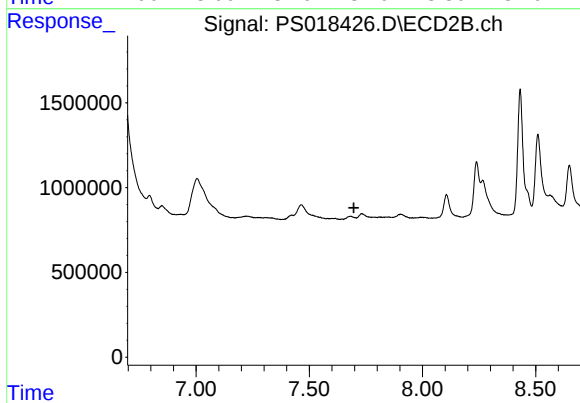

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.697 min
Response: 0
Conc: N.D.

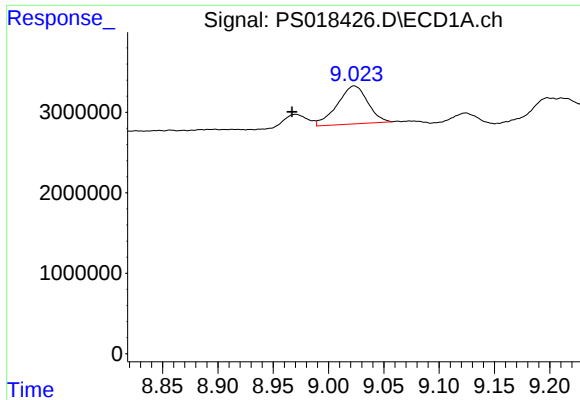

#11 2,4,5-TP (SILVEX)


R.T.: 9.023 min
Delta R.T.: 0.056 min
Response: 9022158
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

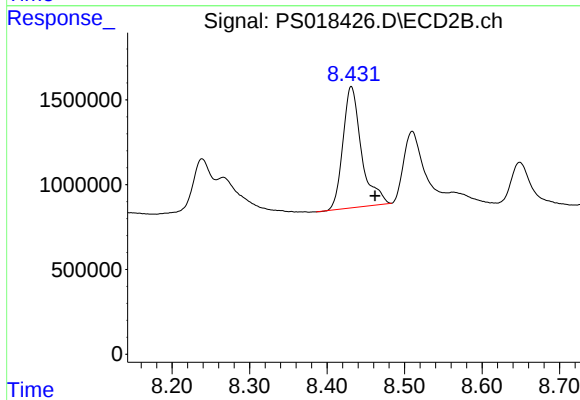


#11 2,4,5-TP (SILVEX)

R.T.: 8.431 min
Delta R.T.: -0.031 min
Response: 11906784
Conc: 2.88 ng/ml

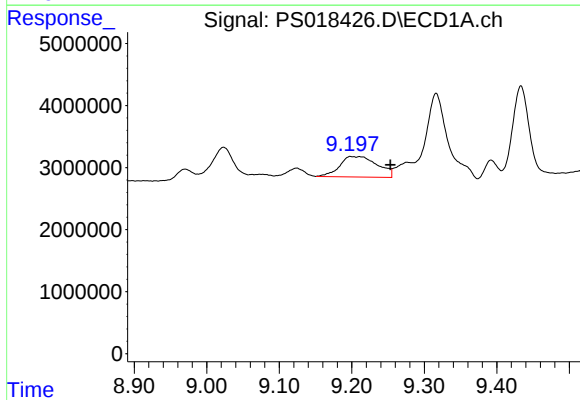


#12 2,4,5-T

R.T.: 9.198 min
Delta R.T.: -0.055 min
Response: 11998628
Conc: 1.19 ng/ml

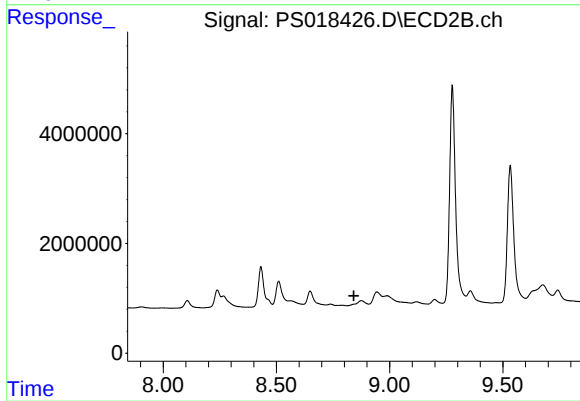

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.842 min
Response: 0
Conc: N.D.

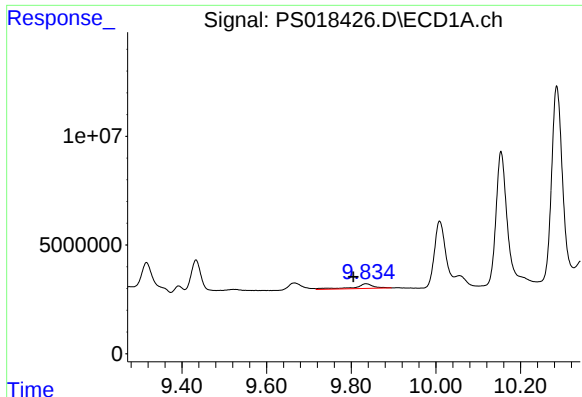

#13 2,4-DB


R.T.: 9.834 min
Delta R.T.: 0.029 min
Response: 6977202
Conc: 4.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

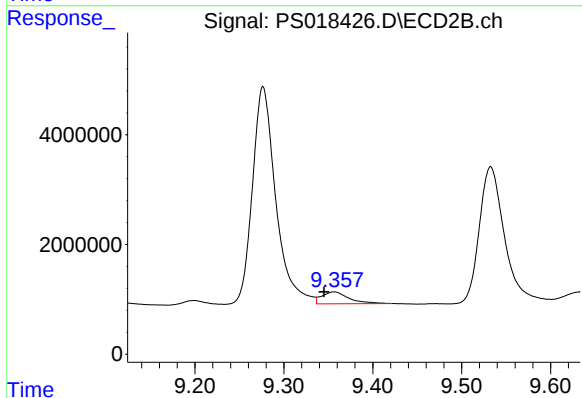


#13 2,4-DB

R.T.: 9.357 min
Delta R.T.: 0.011 min
Response: 4597689
Conc: 8.51 ng/ml

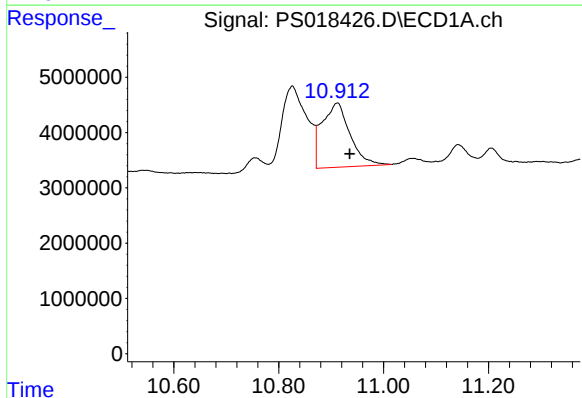


#14 DINOSEB

R.T.: 10.912 min
Delta R.T.: -0.024 min
Response: 42924049
Conc: 5.52 ng/ml

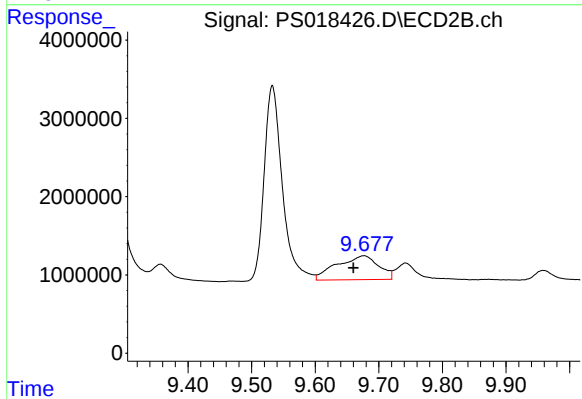

#14 DINOSEB


R.T.: 9.676 min
Delta R.T.: 0.017 min
Response: 13962322
Conc: 4.80 ng/ml

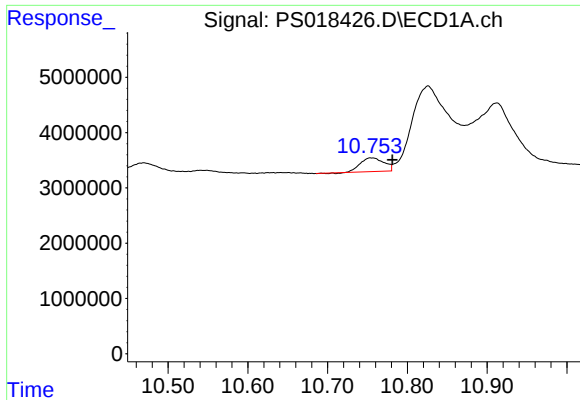

#15 Picloram

R.T.: 10.754 min
Delta R.T.: -0.027 min
Response: 4990379
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

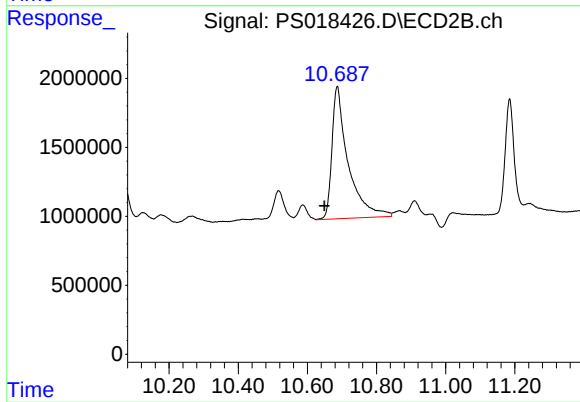

#15 Picloram

R.T.: 10.687 min
Delta R.T.: 0.038 min
Response: 31175318
Conc: 5.39 ng/ml