

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
 Data File : PS018420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 17:31
 Operator : AJ\MA
 Sample : PB142887TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB142887TB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/25/2022
 Supervised By : Ankita Jodhani 02/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:20:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.021	6.633	672.4E6	362.3E6	404.059	543.760m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022422\
Data File : PS018420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 17:31
Operator : AJ\MA
Sample : PB142887TB
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB142887TB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/25/2022
Supervised By : Ankita Jodhani 02/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:20:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

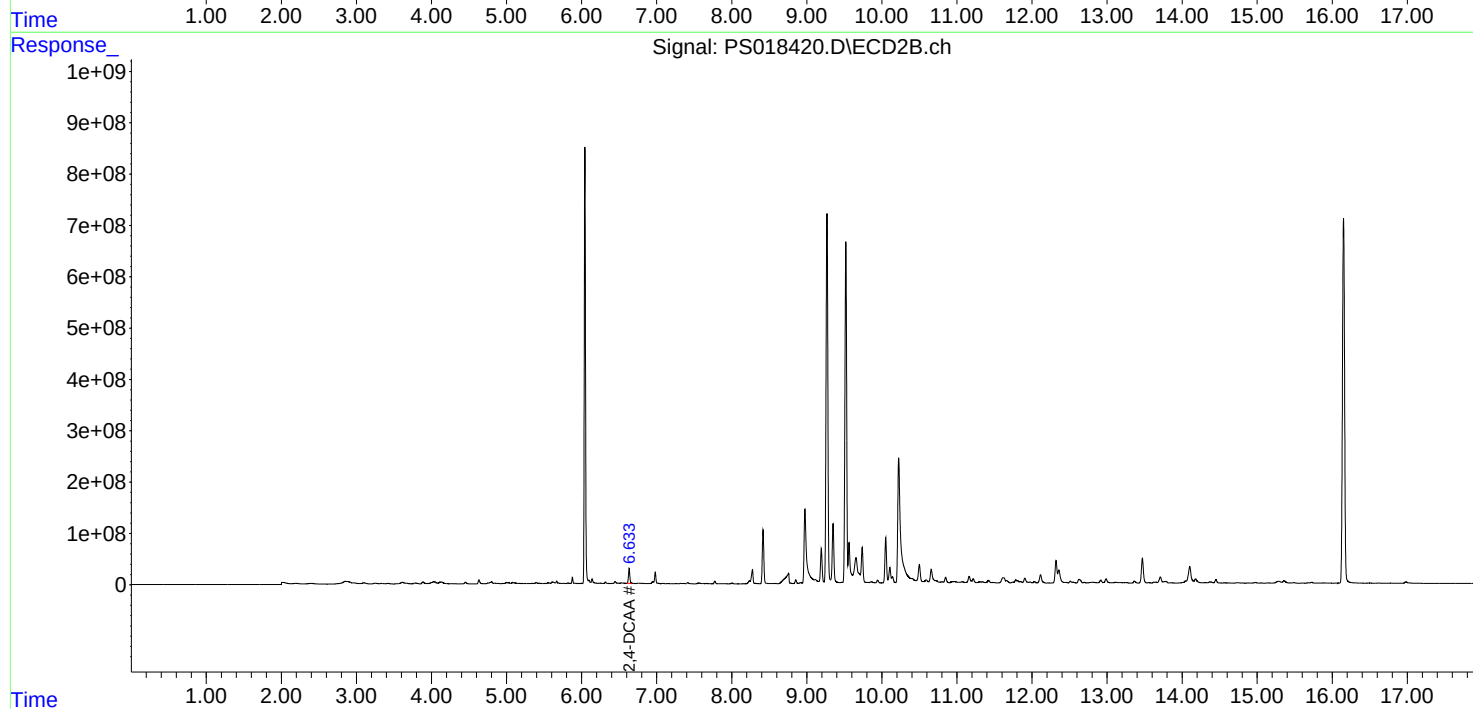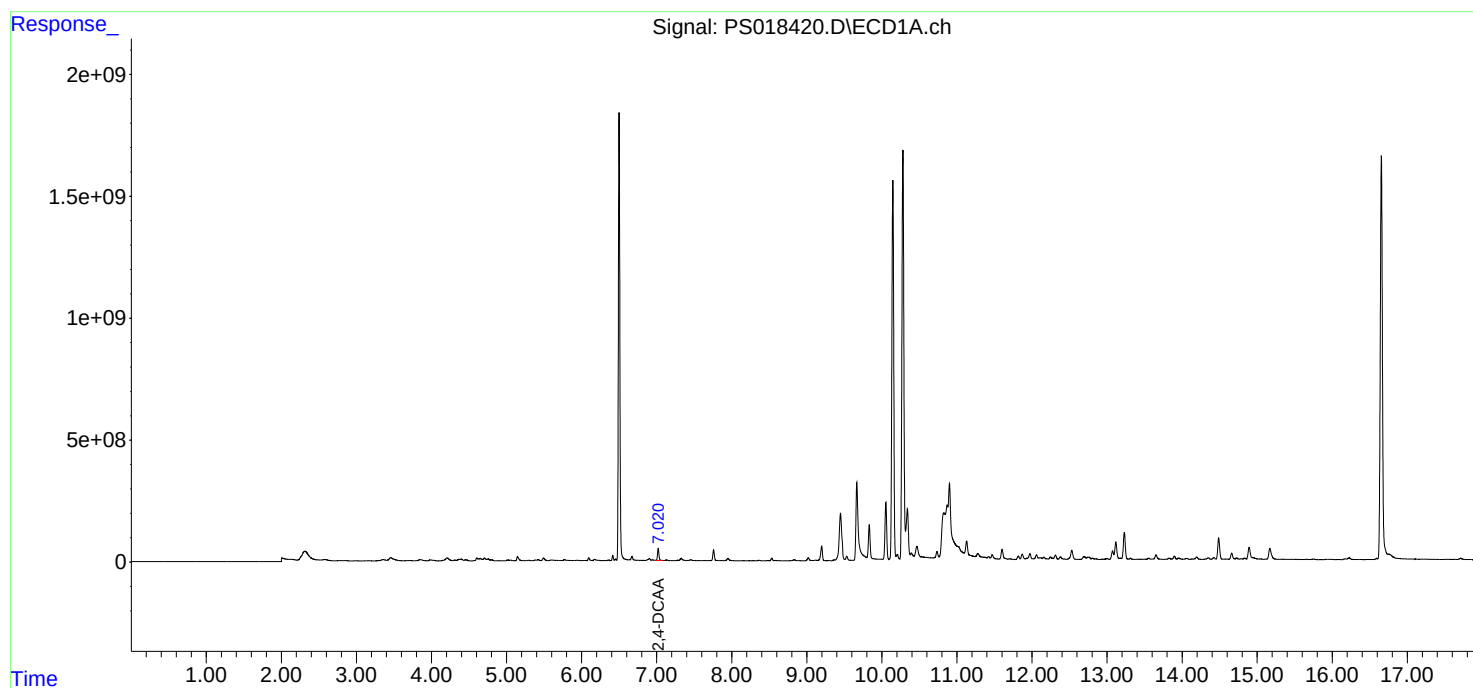

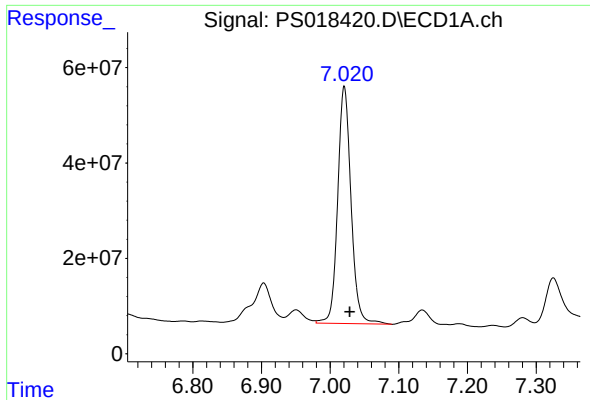

#4 2,4-DCAA

R.T.: 7.021 min
Delta R.T.: -0.008 min
Response: 672375136
Conc: 404.06 ng/ml

Instrument :

ECD_S

ClientSampleId :


PB142887TB

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 02/25/2022

Supervised By :Ankita Jodhani 02/25/2022

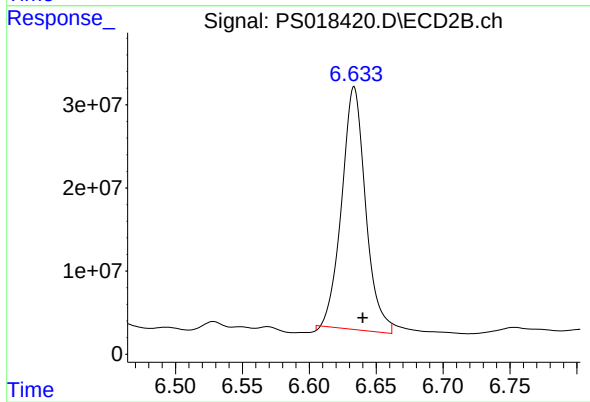

#4 2,4-DCAA

R.T.: 6.633 min
Delta R.T.: -0.007 min
Response: 362330021
Conc: 543.76 ng/ml m