

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033023\
 Data File : PS022551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2023 08:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 21:06:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.301	0.000	1585706	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.435	0.000	2269548	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.691	0.000	2160509	0	<MDL	N.D. #
3) T	4-Nitroph...	6.092f	0.000	146659	0	<MDL	N.D. #
5) T	DICAMBA	6.404	6.943f	463142	2468690	<MDL	<MDL #
6) T	MCP	0.000	6.943f	0	2468690	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.555f	0	2476251	N.D.	<MDL
10) T	Pentachlo...	7.442	0.000	786725	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.949	8.593	1605118	4109197	<MDL	<MDL #
12) T	2,4,5-T	8.249	0.000	1085994	0	<MDL	N.D. #
13) T	2,4-DB	8.673f	9.424	941271	2550212	<MDL	1.519 #
14) T	DINOSEB	9.713f	0.000	2892795	0	<MDL	N.D. #
15) T	Picloram	0.000	10.700	0	11398742	N.D.	<MDL
16) T	DCPA	0.000	10.700	0	11398742	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033023\
Data File : PS022551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2023 08:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 21:06:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

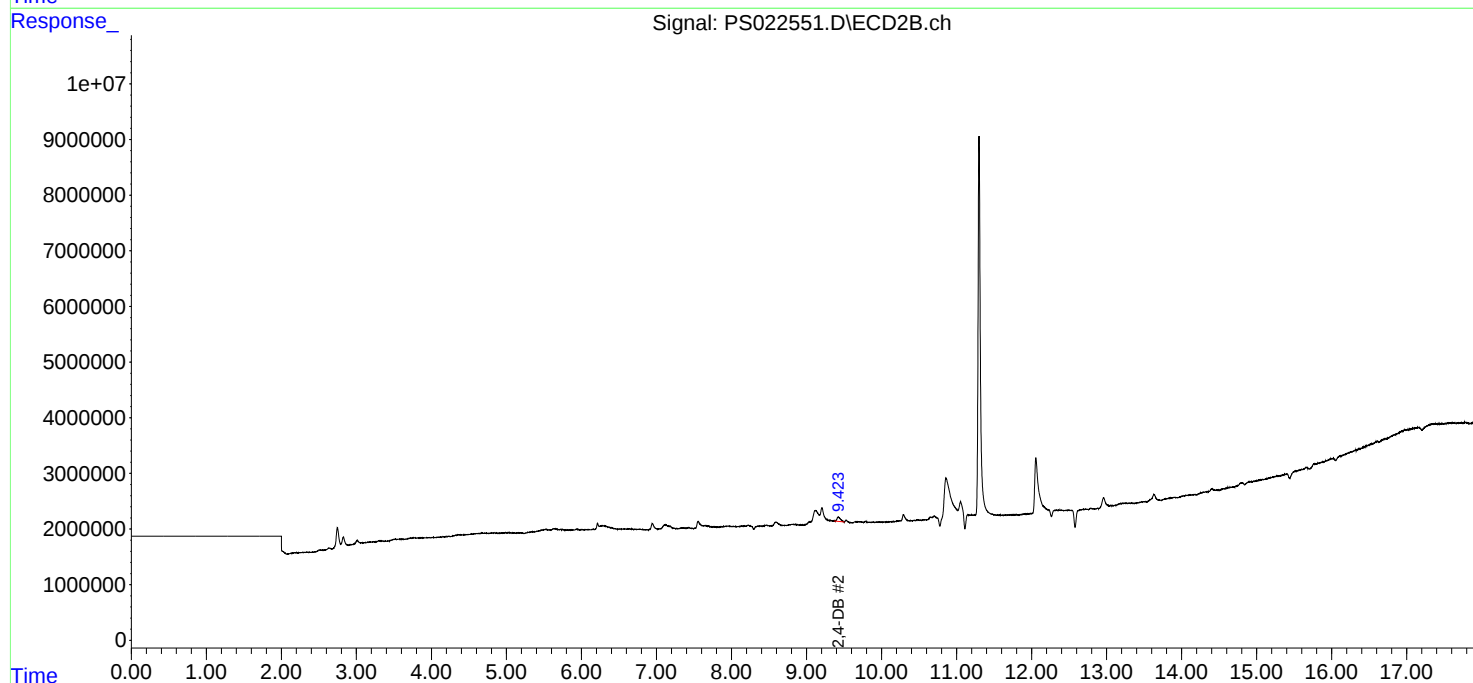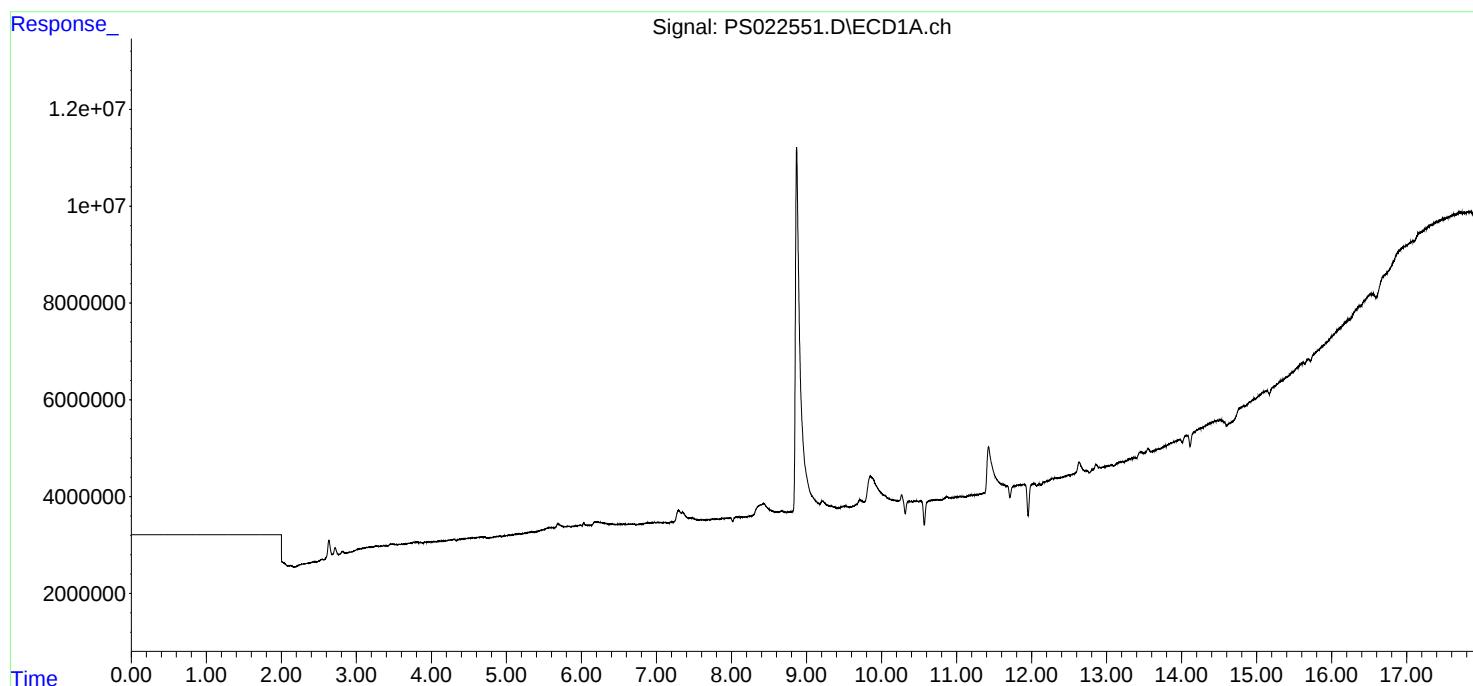


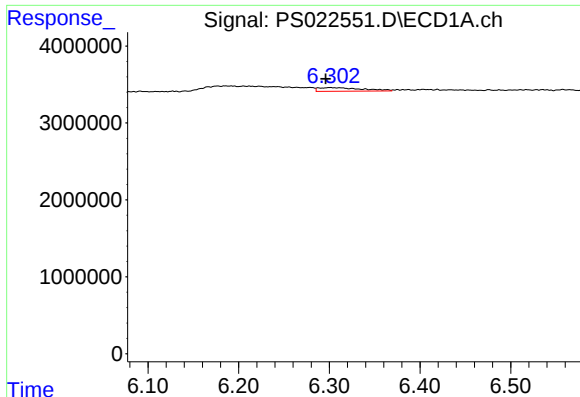

#4 2,4-DCAA


R.T.: 6.301 min
Delta R.T.: 0.005 min
Response: 1585706
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

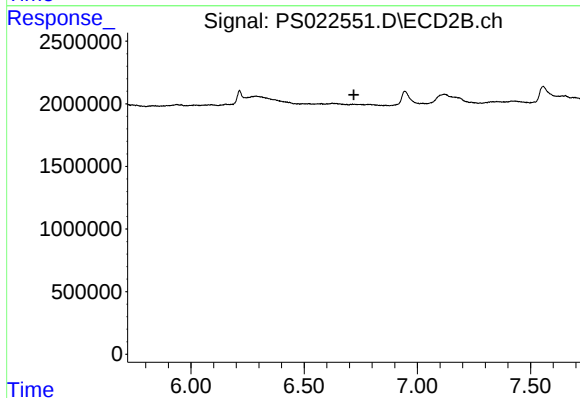


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.719 min
Response: 0
Conc: N.D.

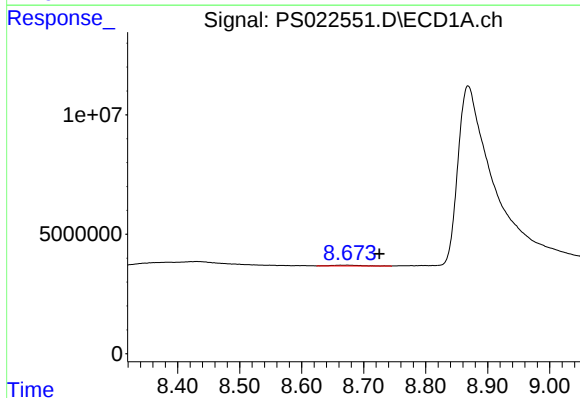

#13 2,4-DB

R.T.: 8.673 min
Delta R.T.: -0.052 min
Response: 941271
Conc: N.D.

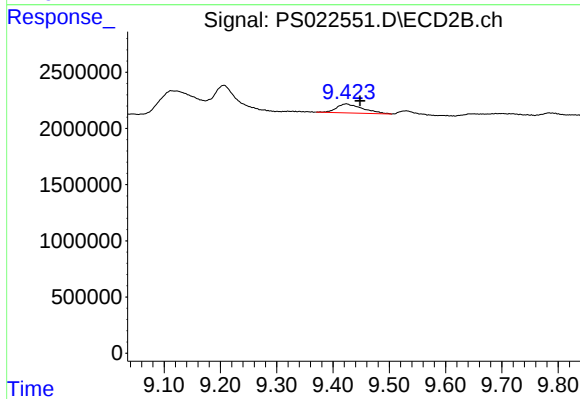

#13 2,4-DB

R.T.: 9.424 min
Delta R.T.: -0.025 min
Response: 2550212
Conc: 1.52 ng/ml