

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 08:00
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 00:59:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	0.000	8.963	0	154054	N.D. <MDL
3) T	4-Nitroph...	10.882	9.939	2935706	1328923	13.550 5.853 #
6) T	MCP	0.000	11.254	0	422430	N.D. <MDL
9) T	2,4-D	0.000	12.689	0	145498	N.D. <MDL
10) T	Pentachlo...	0.000	13.164	0	745406	N.D. <MDL
11) T	2,4,5-TP ...	0.000	13.802	0	330674	N.D. <MDL
13) T	2,4-DB	0.000	14.973	0	10839097	N.D. 36.501
14) T	DINOSEB	0.000	15.394	0	6285672	N.D. 3.276
15) T	Picloram	16.726	16.682	120.6E6	4061108	35.493 1.281 #
16) T	DCPA	0.000	16.634	0	3754546	N.D. 1.111



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 08:00
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 00:59:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

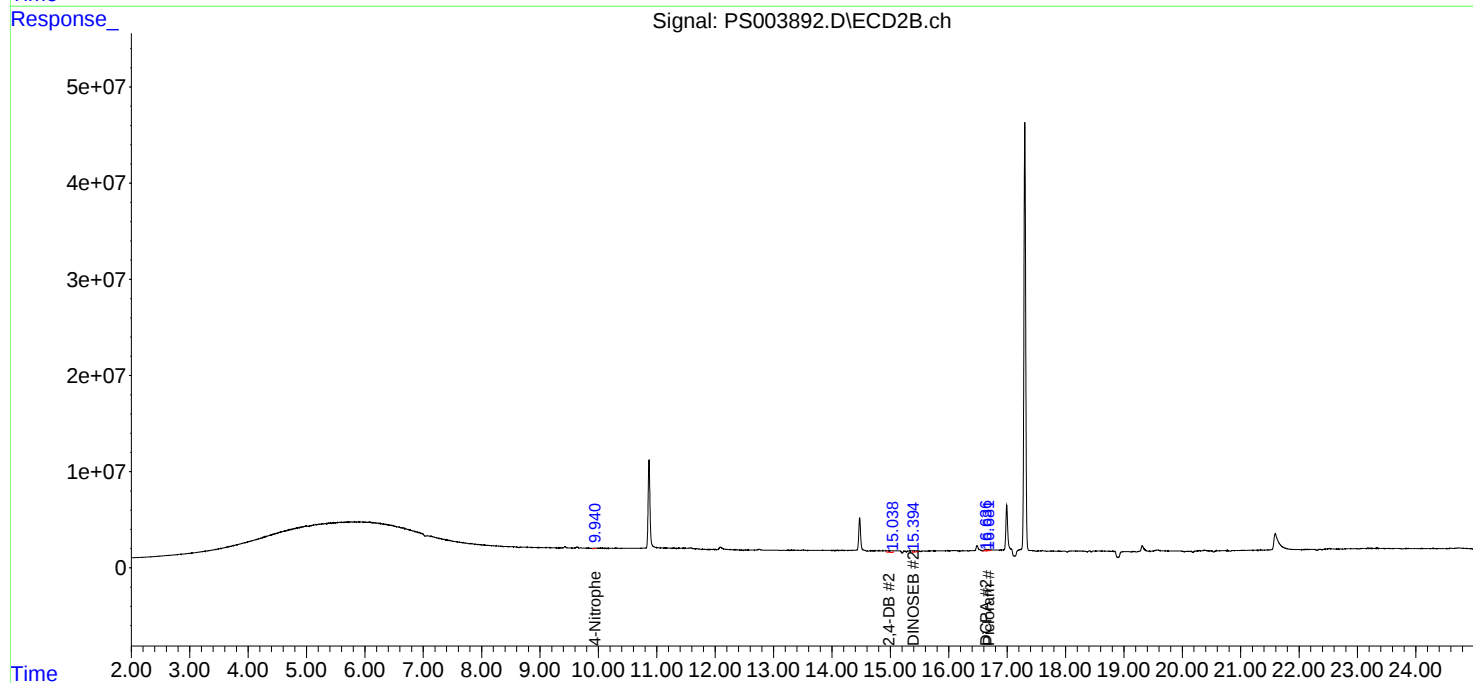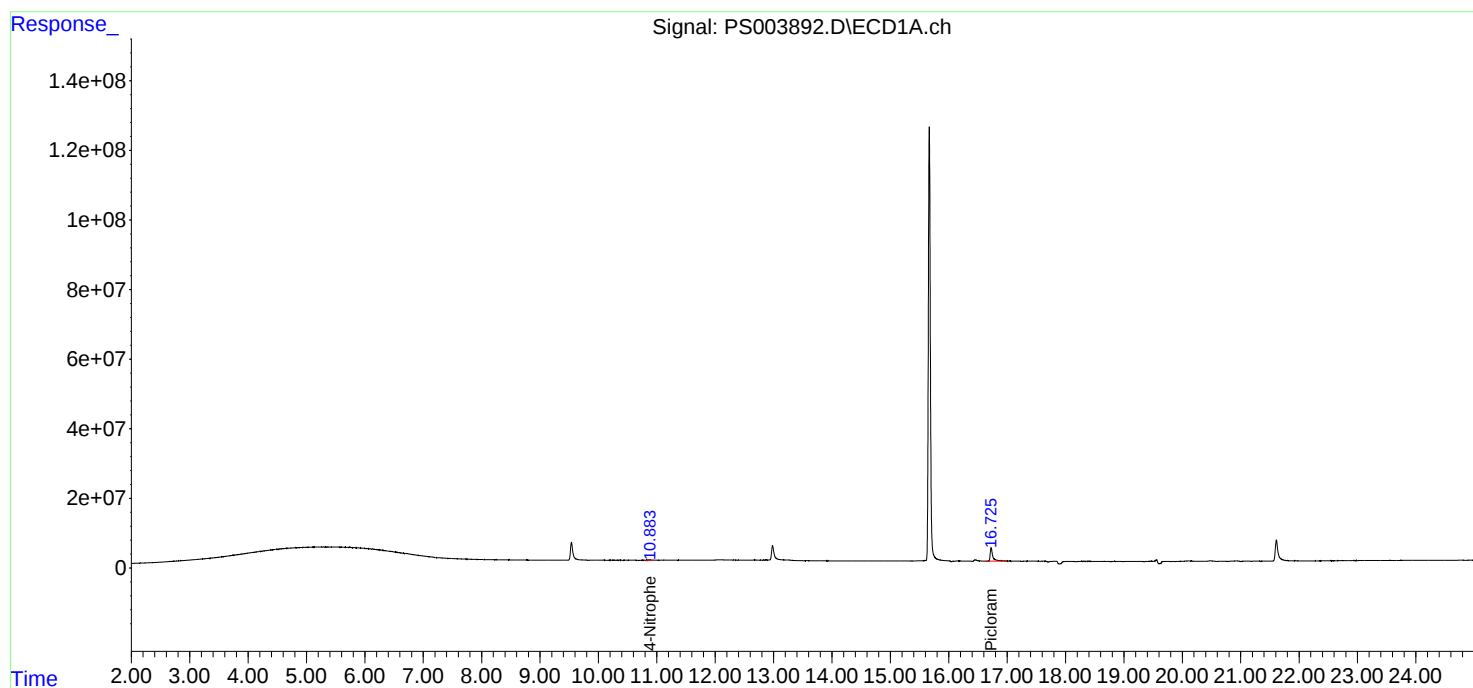


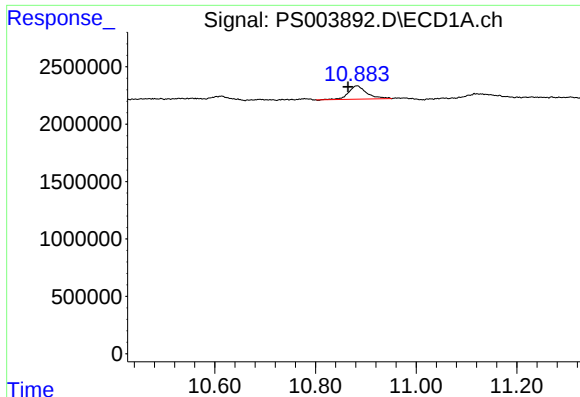

#3 4-Nitrophenol


R.T.: 10.882 min
Delta R.T.: 0.018 min
Response: 2935706
Conc: 13.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

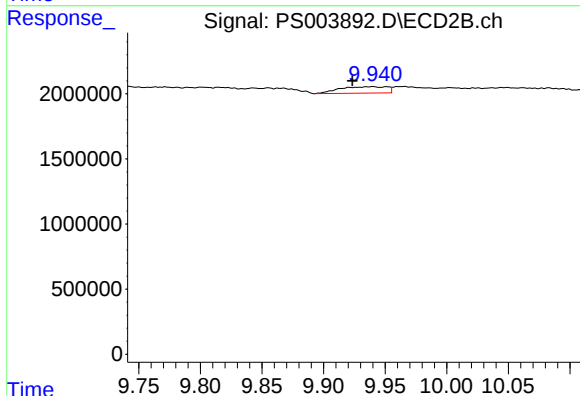


#3 4-Nitrophenol

R.T.: 9.939 min
Delta R.T.: 0.015 min
Response: 1328923
Conc: 5.85 ng/ml

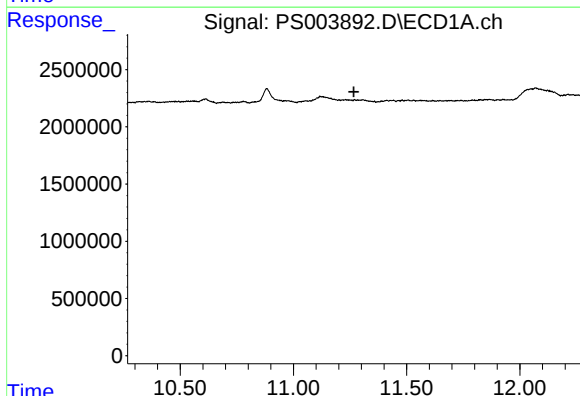


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.267 min
Response: 0
Conc: N.D.

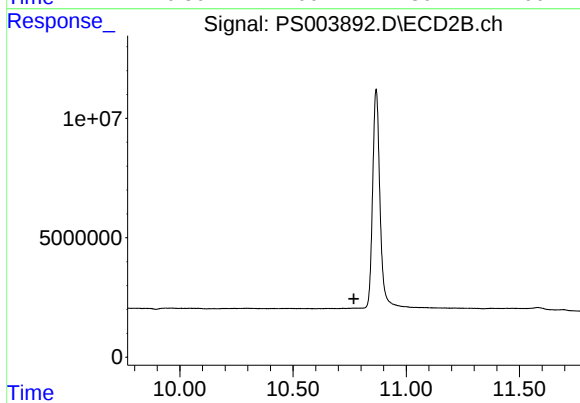

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 10.769 min
Response: 0
Conc: N.D.

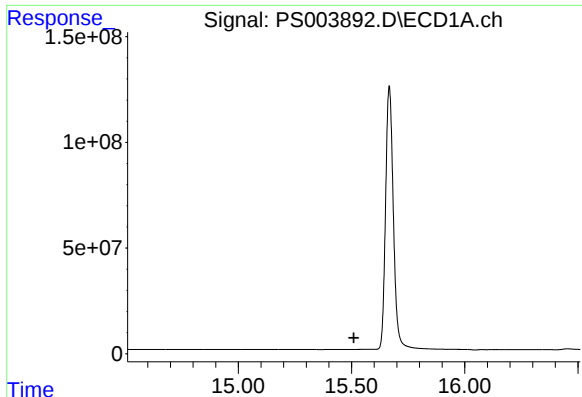

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

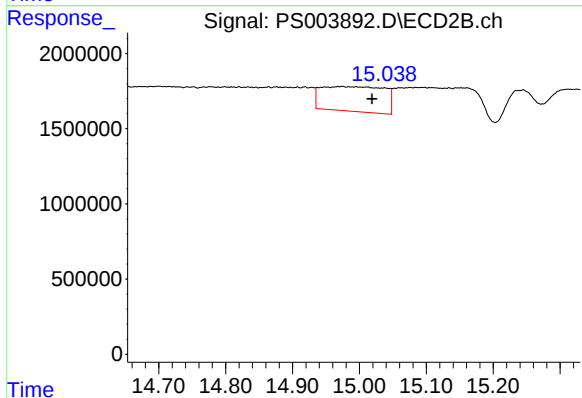


#13 2,4-DB

R.T.: 14.973 min
Delta R.T.: -0.046 min
Response: 10839097
Conc: 36.50 ng/ml

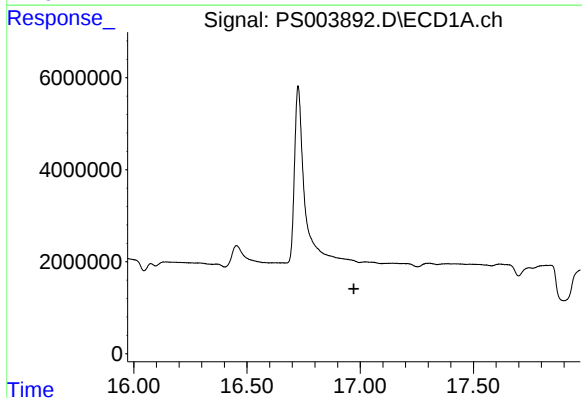


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

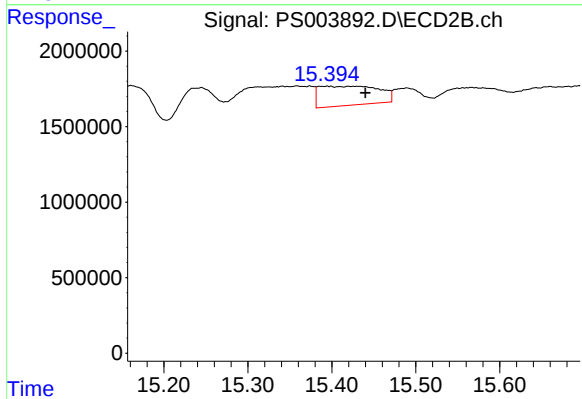

#14 DINOSEB


R.T.: 15.394 min
Delta R.T.: -0.046 min
Response: 6285672
Conc: 3.28 ng/ml

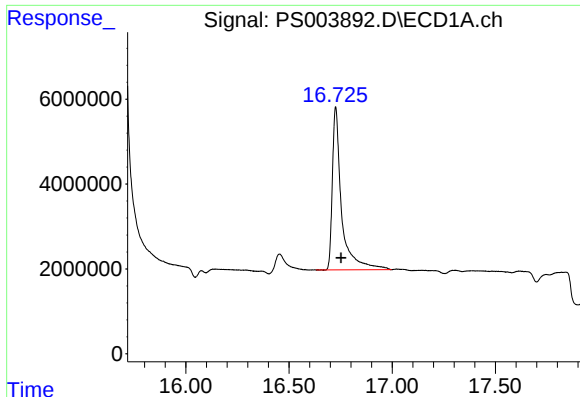

#15 Picloram


R.T.: 16.726 min
Delta R.T.: -0.026 min
Response: 120570189
Conc: 35.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

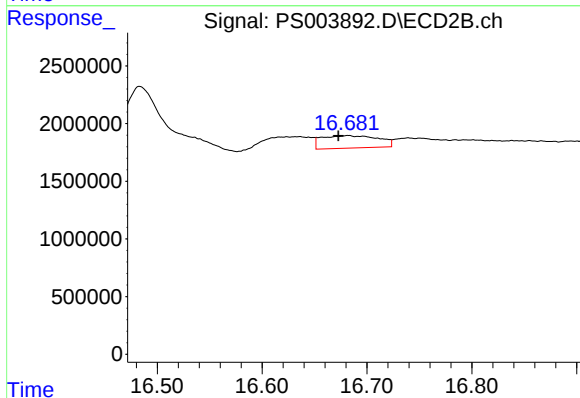


#15 Picloram

R.T.: 16.682 min
Delta R.T.: 0.009 min
Response: 4061108
Conc: 1.28 ng/ml

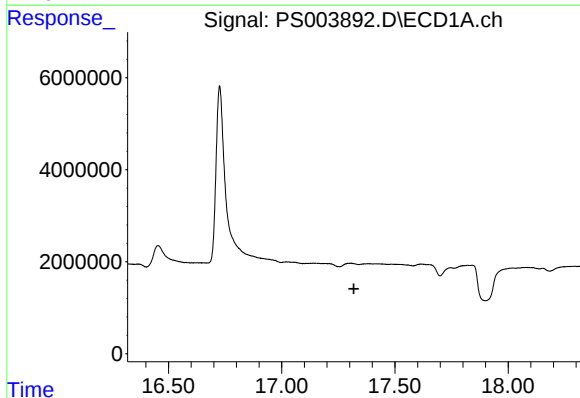

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

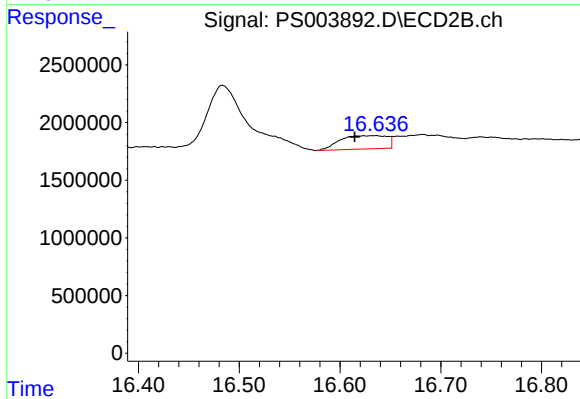

#16 DCPA

R.T.: 16.634 min
Delta R.T.: 0.020 min
Response: 3754546
Conc: 1.11 ng/ml