

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 08:31
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:00:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.292	10.790	197.9E6	192.8E6	453.732	392.870
Target Compounds							
3) T	4-Nitroph...	0.000	9.938	0	143395	N.D.	<MDL
6) T	MCP	0.000	11.271	0	148930	N.D.	<MDL
7) T	MCPA	0.000	11.677	0	342367	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.208	0	2272949	N.D.	4.882
9) T	2,4-D	0.000	12.624	0	488945	N.D.	<MDL
10) T	Pentachlo...	0.000	13.201	0	1009013	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.867	0	274121	N.D.	<MDL
12) T	2,4,5-T	0.000	14.352	0	85917	N.D.	<MDL
13) T	2,4-DB	0.000	15.019	0	650926	N.D.	2.192
14) T	DINOSEB	0.000	15.468	0	504835	N.D.	<MDL
15) T	Picloram	0.000	16.635	0	1663492	N.D.	<MDL
16) T	DCPA	0.000	16.635	0	1663492	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 08:31
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:00:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

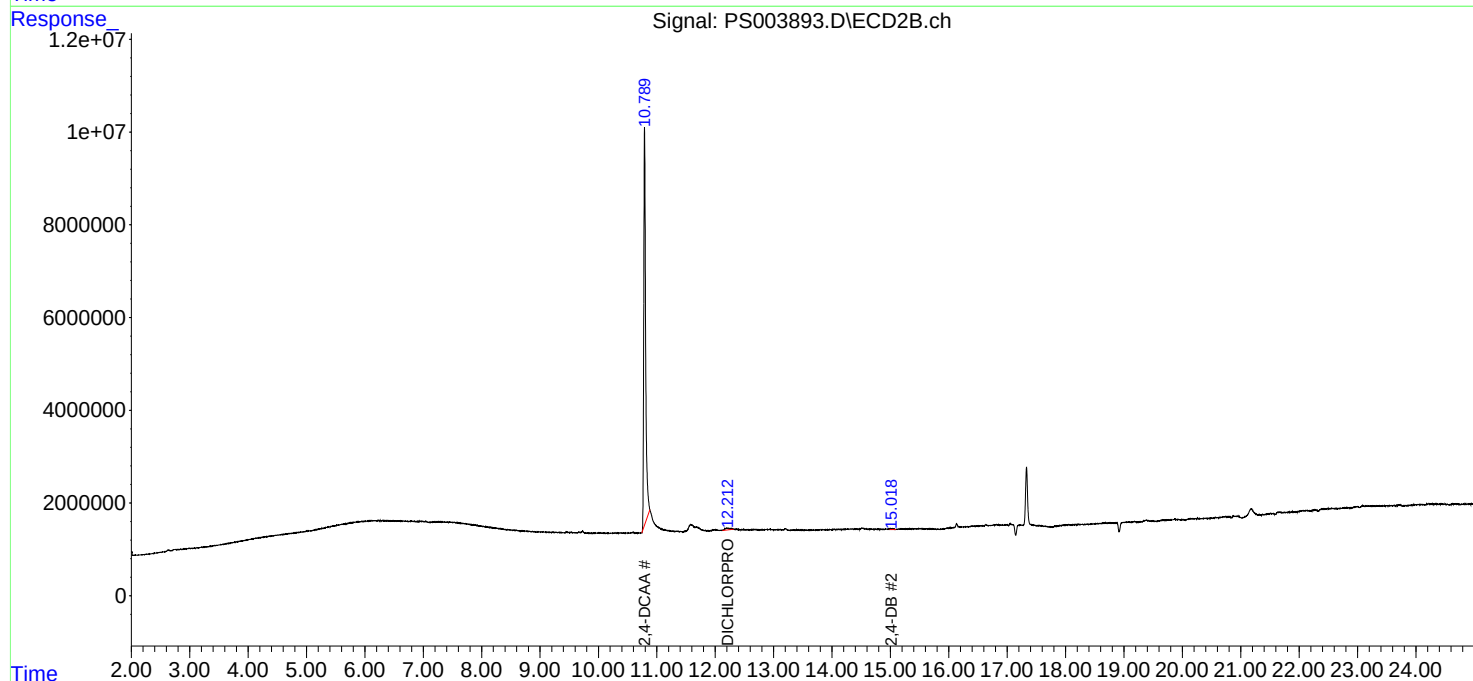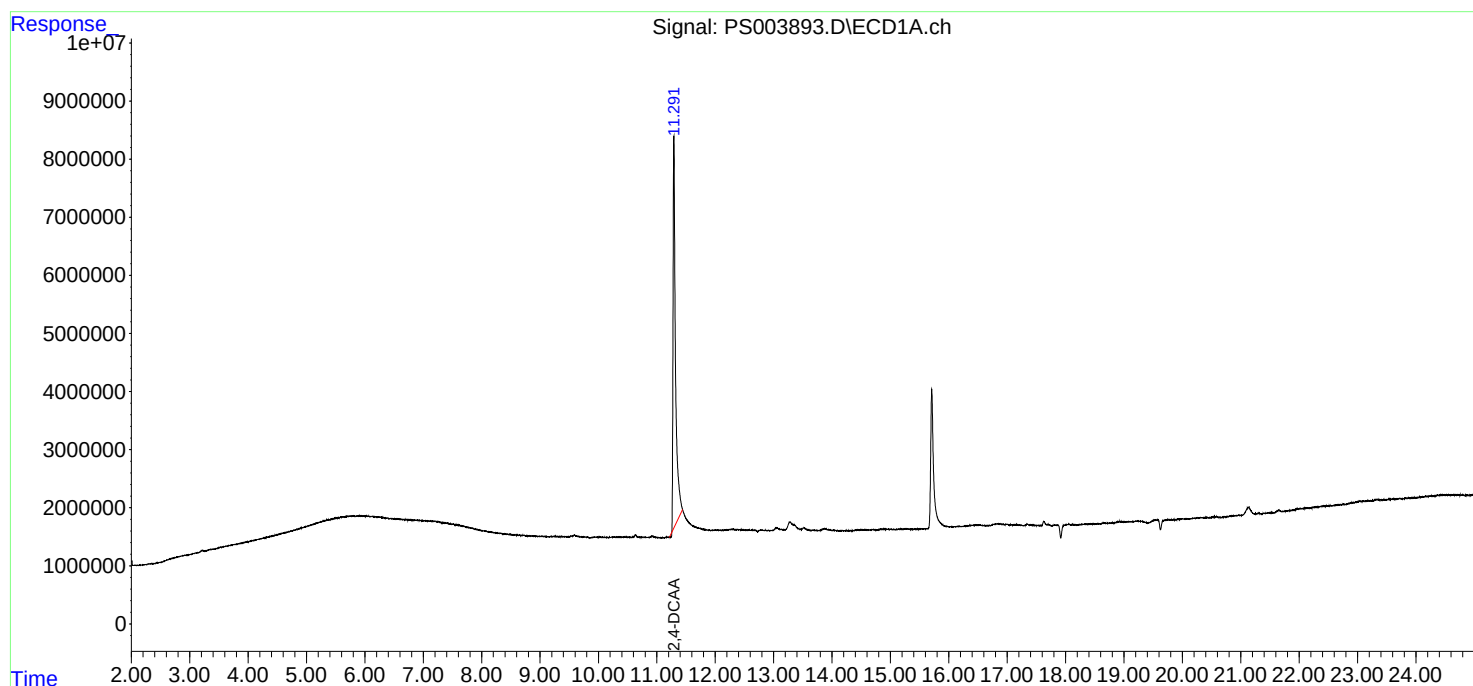


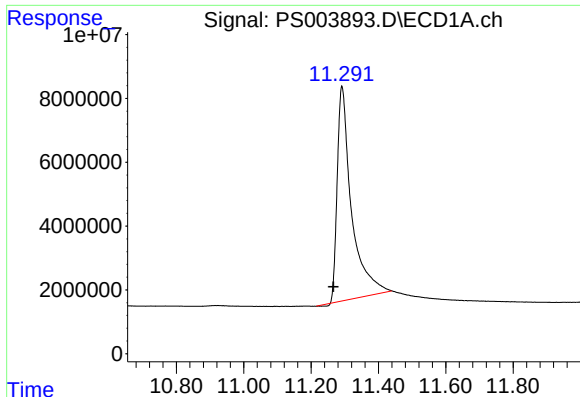

#4 2,4-DCAA


R.T.: 11.292 min
Delta R.T.: 0.025 min
Response: 197923694
Conc: 453.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

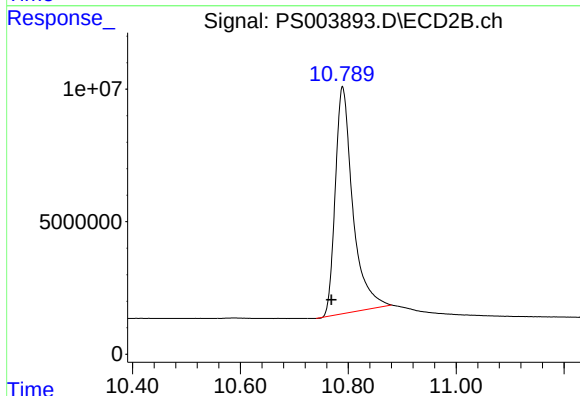


#4 2,4-DCAA

R.T.: 10.790 min
Delta R.T.: 0.021 min
Response: 192764705
Conc: 392.87 ng/ml

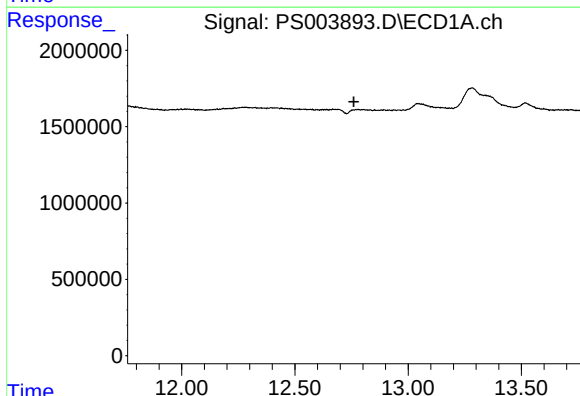


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

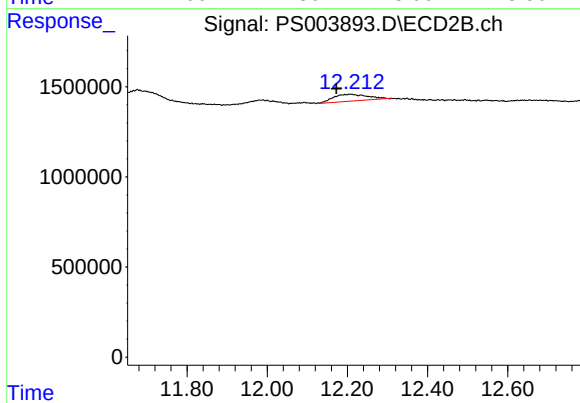

#8 DICHLORPROP


R.T.: 12.208 min
Delta R.T.: 0.035 min
Response: 2272949
Conc: 4.88 ng/ml

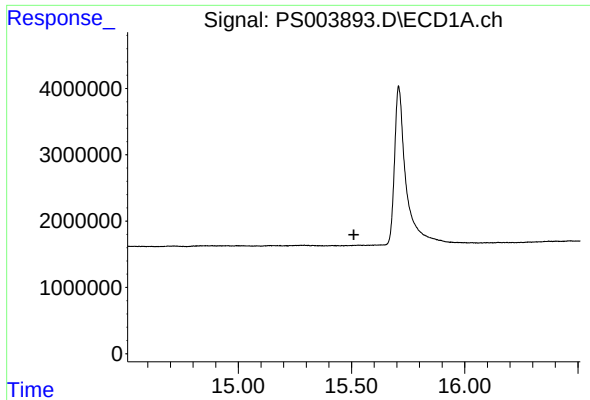

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

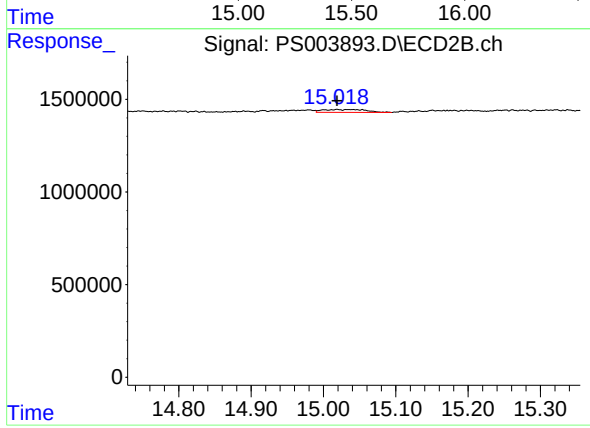

#13 2,4-DB

R.T.: 15.019 min
Delta R.T.: 0.000 min
Response: 650926
Conc: 2.19 ng/ml