

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 09:46
 Operator : EI\SJ
 Sample : MDL-Herb-S-BL-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-Herb-S-BL-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:00:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.766	223.7E6	221.5E6	512.833	451.362
Target Compounds							
3) T	4-Nitroph...	0.000	9.928	0	322612	N.D.	1.421
6) T	MCPP	0.000	11.289	0	23771	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.231	0	567482	N.D.	1.219
9) T	2,4-D	0.000	12.643	0	61125	N.D.	<MDL
10) T	Pentachlo...	0.000	13.179	0	370933	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.756	0	311936	N.D.	<MDL
12) T	2,4,5-T	0.000	14.381	0	115076	N.D.	<MDL
13) T	2,4-DB	0.000	15.000	0	143935	N.D.	<MDL
14) T	DINOSEB	0.000	15.440	0	530226	N.D.	<MDL
15) T	Picloram	0.000	16.681	0	376863	N.D.	<MDL
16) T	DCPA	0.000	16.617	0	1005568	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 09:46
Operator : EI\SJ
Sample : MDL-Herb-S-BL-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-Herb-S-BL-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:00:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

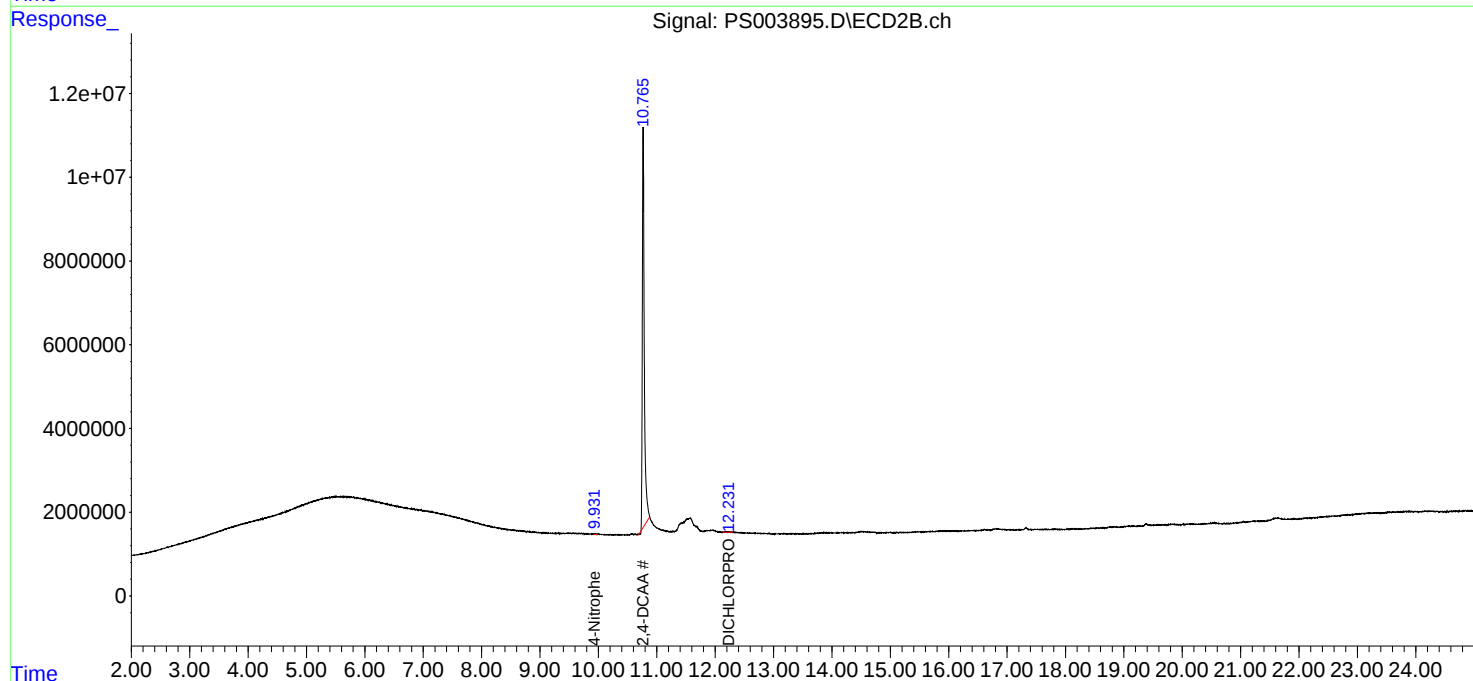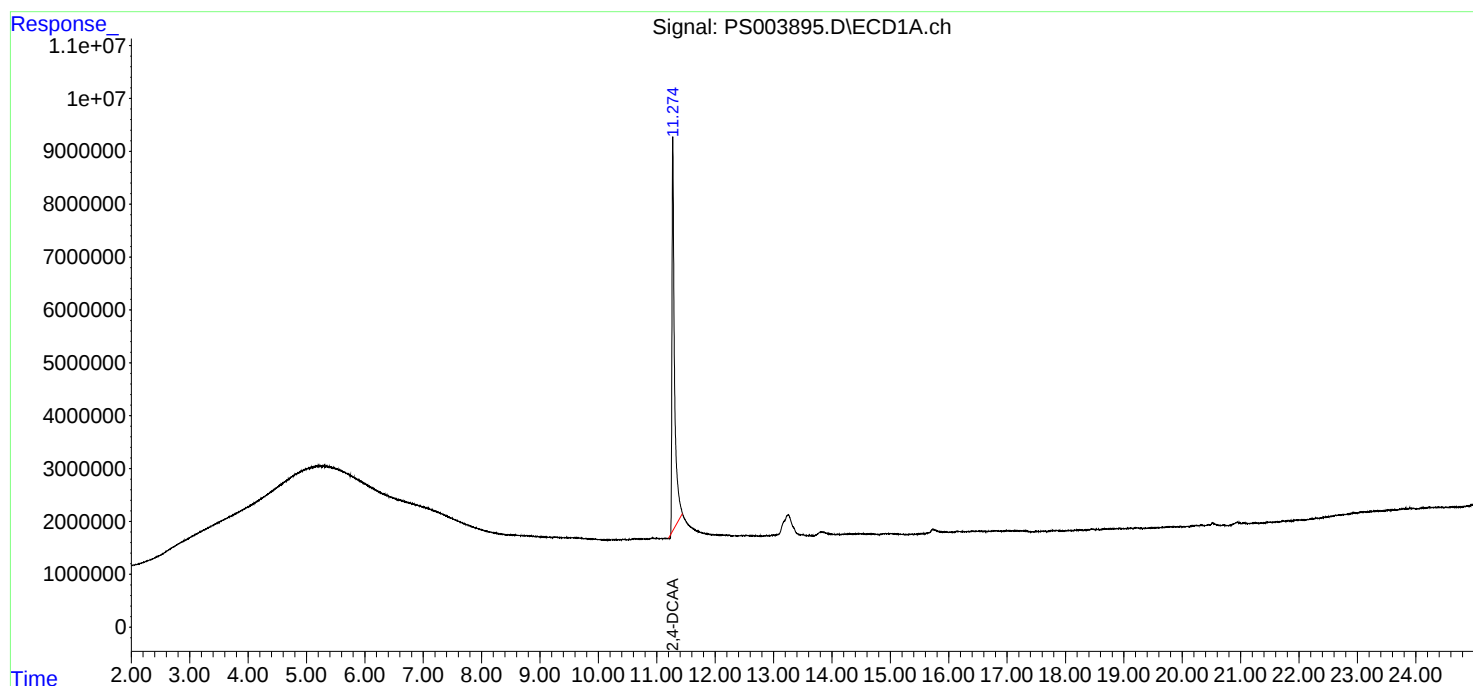


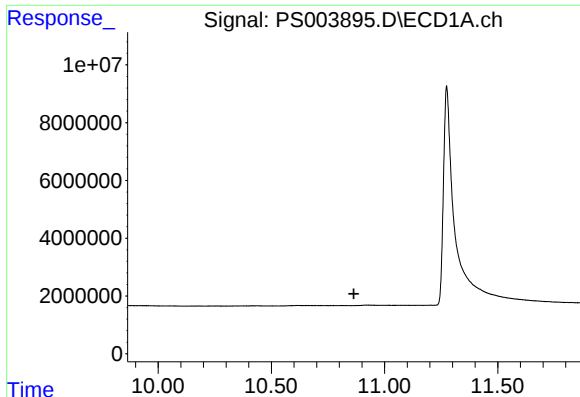

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MDL-Herb-S-BL-06

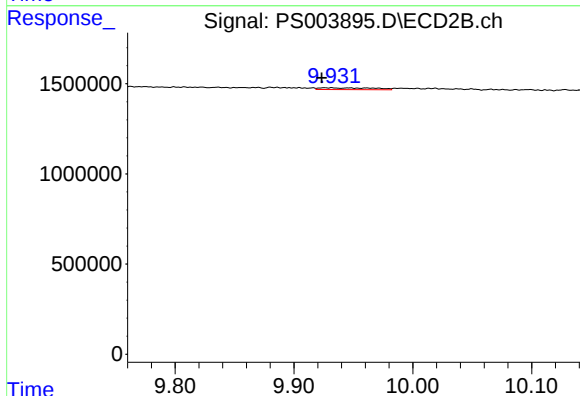


#3 4-Nitrophenol

R.T.: 9.928 min
Delta R.T.: 0.004 min
Response: 322612
Conc: 1.42 ng/ml

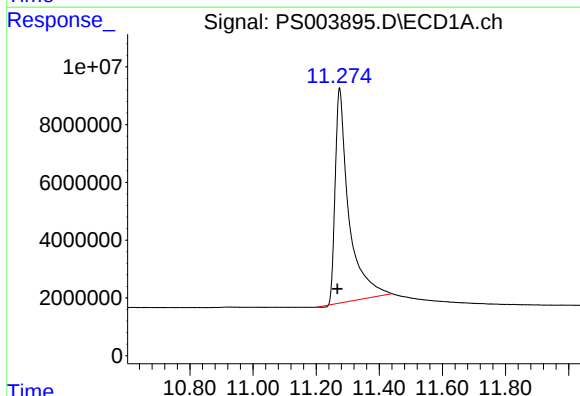


#4 2,4-DCAA

R.T.: 11.274 min
Delta R.T.: 0.008 min
Response: 223703942
Conc: 512.83 ng/ml

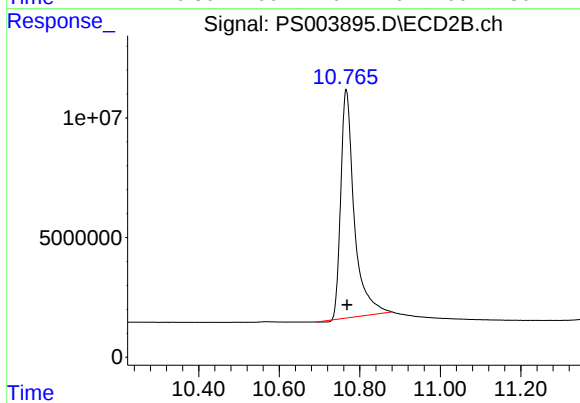

#4 2,4-DCAA


R.T.: 10.766 min
Delta R.T.: -0.002 min
Response: 221464697
Conc: 451.36 ng/ml

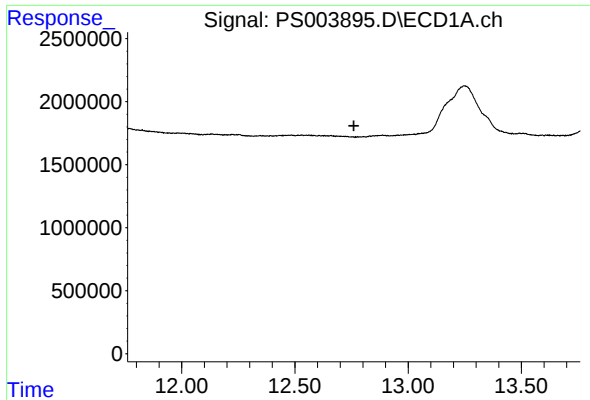

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MDL-Herb-S-BL-06

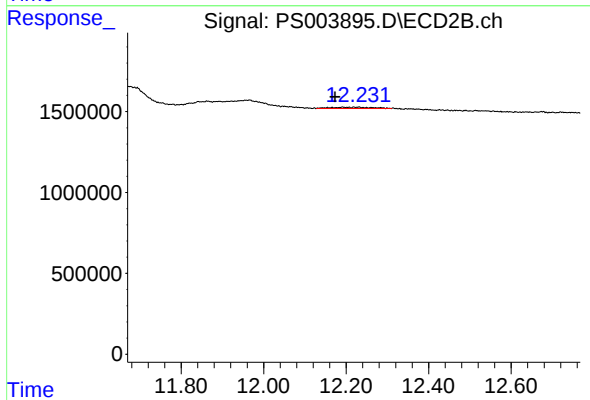

#8 DICHLORPROP

R.T.: 12.231 min
Delta R.T.: 0.058 min
Response: 567482
Conc: 1.22 ng/ml