

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 17:52
 Operator : EI\SJ
 Sample : K1692-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-032919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:04:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.768	225.2E6	216.5E6	516.309	441.233
Target Compounds							
1) T	Dalapon	2.787	2.282	21882988	29623607	29.352	40.601 #
2) T	3,5-DICHL...	0.000	8.934	0	5347760	N.D.	8.384
3) T	4-Nitroph...	0.000	9.941	0	19951651	N.D.	87.879
7) T	MCPA	12.182	11.673	77592348	780726	36.777	<MDL #
9) T	2,4-D	0.000	12.624	0	1153695	N.D.	2.169
10) T	Pentachlo...	0.000	13.169	0	453337	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.780	0	2446066	N.D.	<MDL
12) T	2,4,5-T	0.000	14.413	0	5182061	N.D.	2.384
14) T	DINOSEB	0.000	15.495	0	3390302	N.D.	1.767
15) T	Picloram	16.756	16.708	1407905	11035637	<MDL	3.480 #
16) T	DCPA	0.000	16.622	0	3207897	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 17:52
Operator : EI\SJ
Sample : K1692-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:04:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

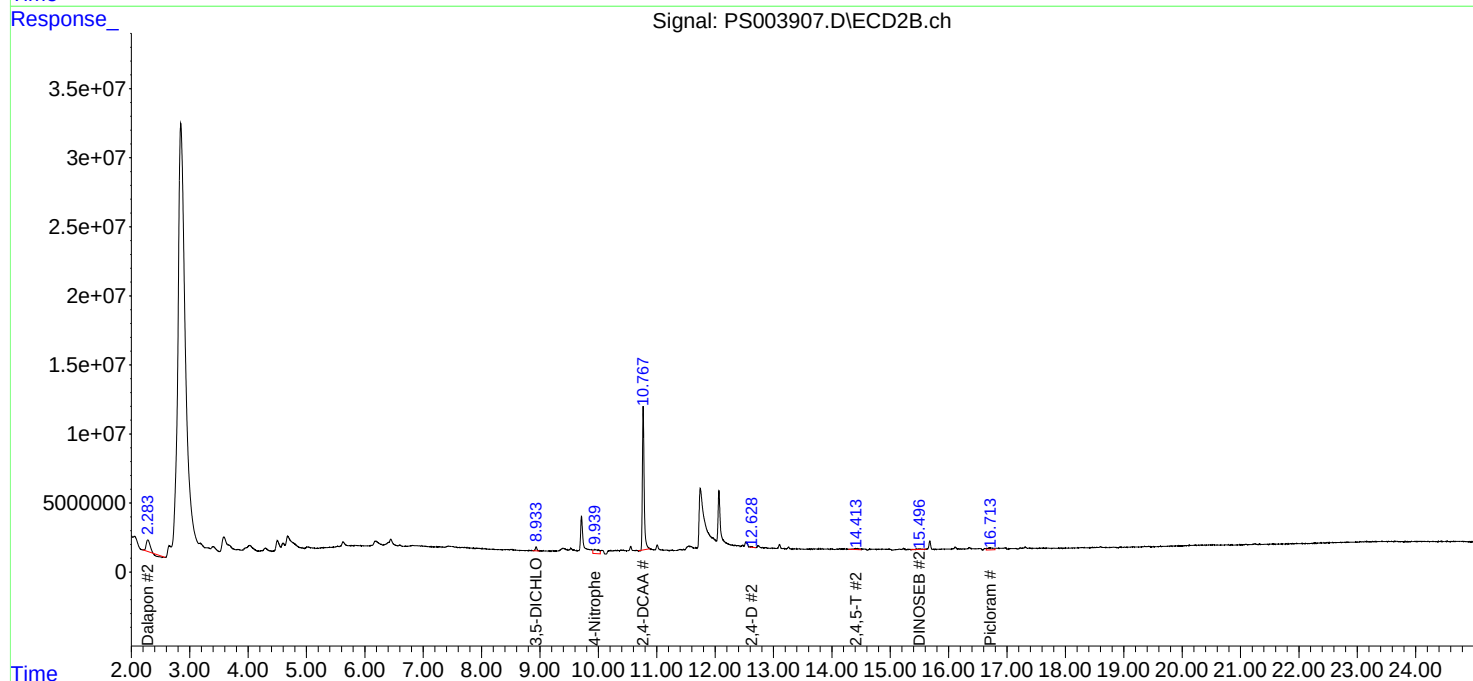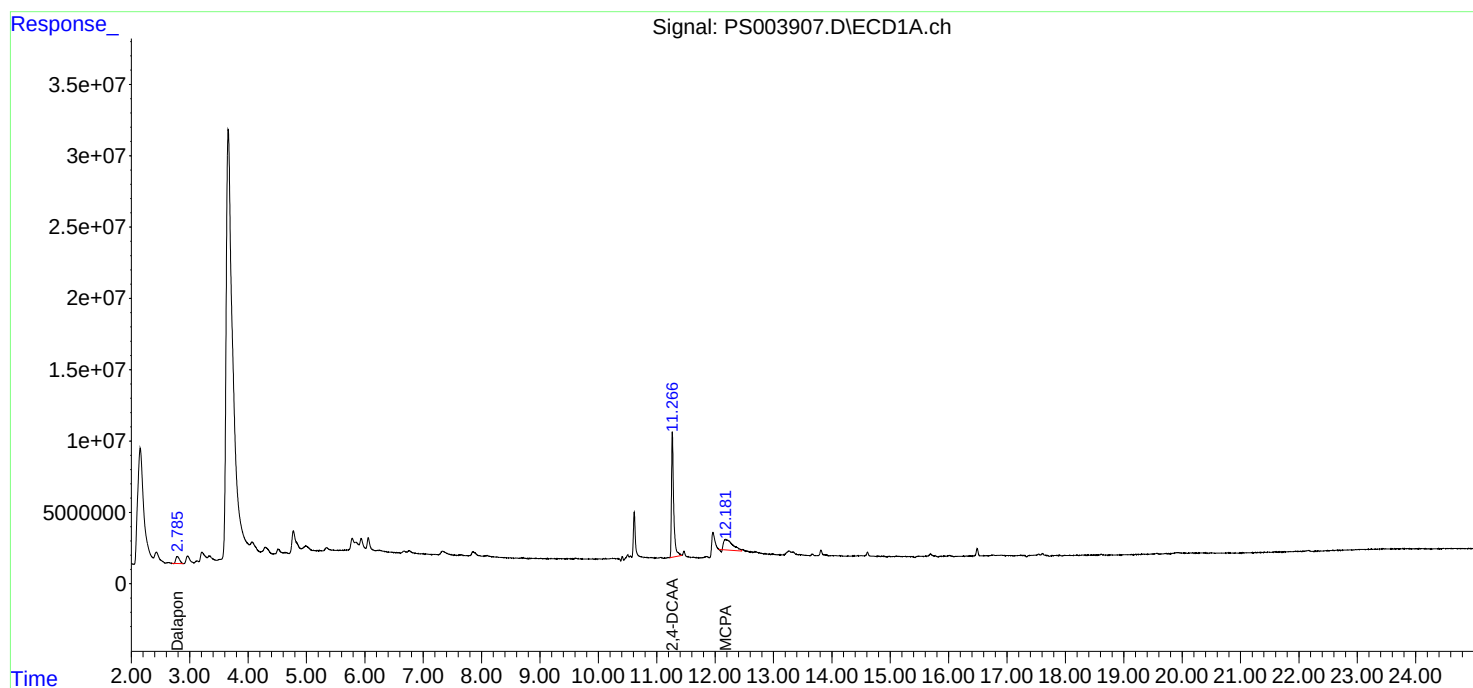


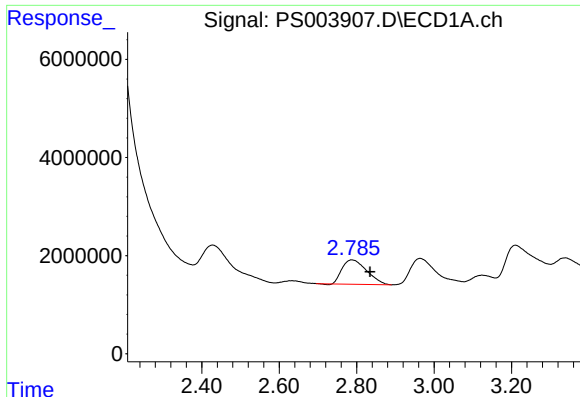

#1 Dalapon


R.T.: 2.787 min
Delta R.T.: -0.048 min
Response: 21882988
Conc: 29.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

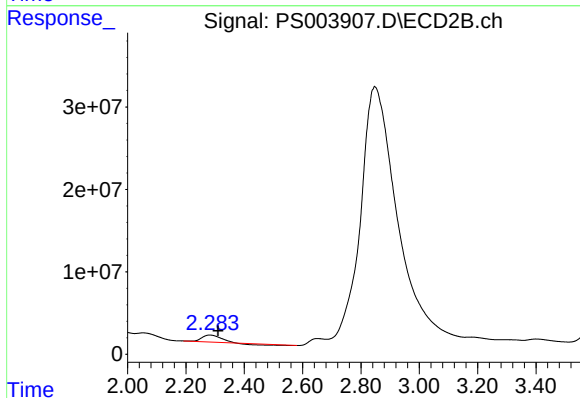


#1 Dalapon

R.T.: 2.282 min
Delta R.T.: -0.029 min
Response: 29623607
Conc: 40.60 ng/ml

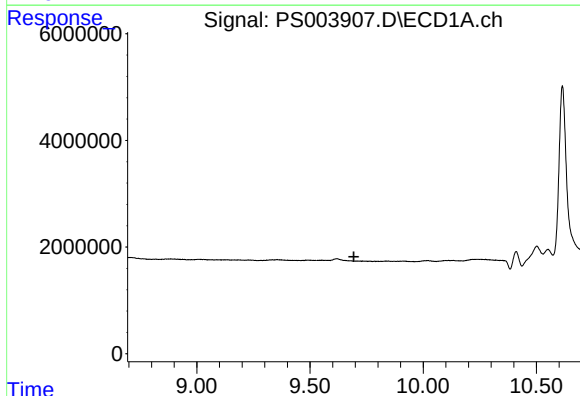


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

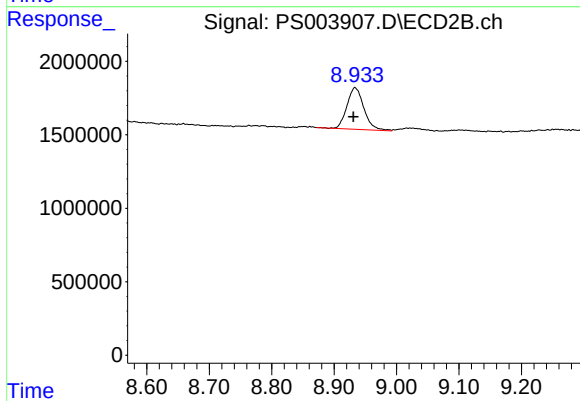

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.934 min
Delta R.T.: 0.003 min
Response: 5347760
Conc: 8.38 ng/ml

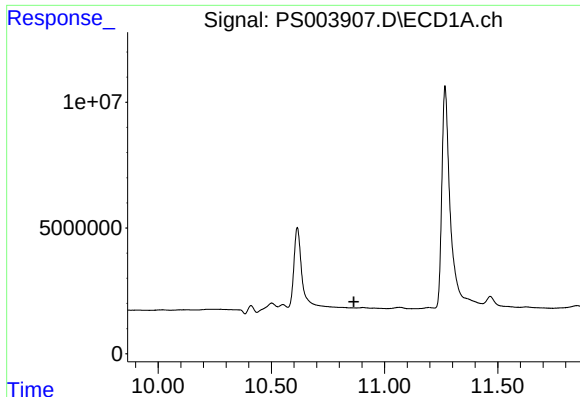

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

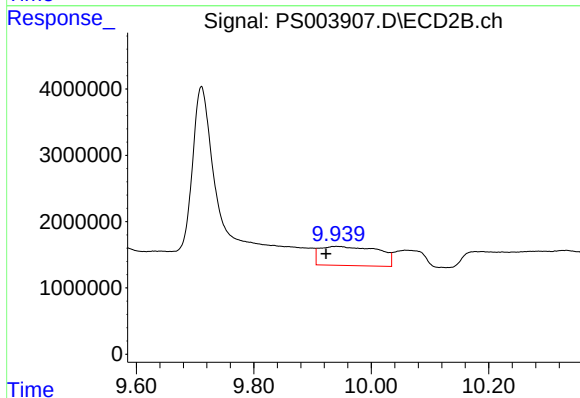


#3 4-Nitrophenol

R.T.: 9.941 min
Delta R.T.: 0.018 min
Response: 19951651
Conc: 87.88 ng/ml

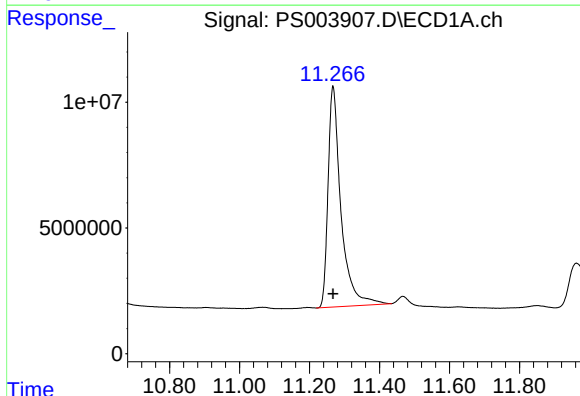


#4 2,4-DCAA

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 225220403
Conc: 516.31 ng/ml

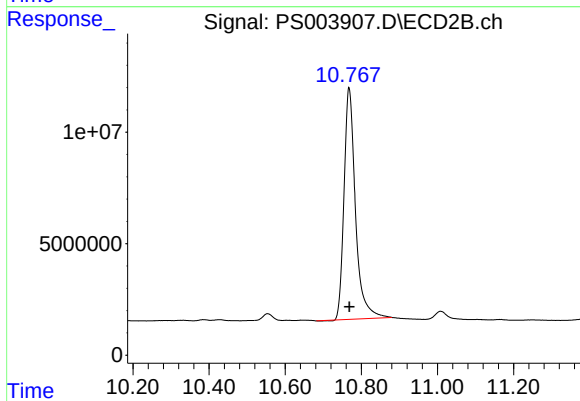

#4 2,4-DCAA


R.T.: 10.768 min
Delta R.T.: 0.000 min
Response: 216494527
Conc: 441.23 ng/ml

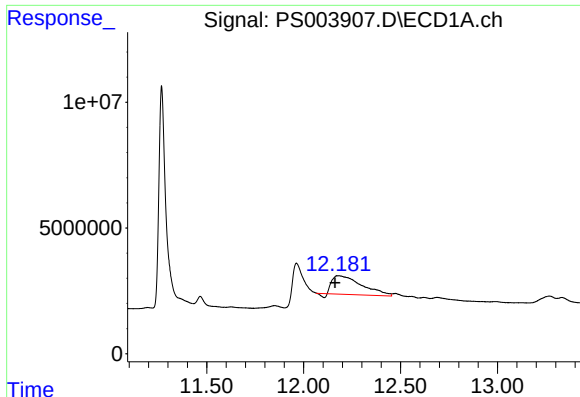

#7 MCPA


R.T.: 12.182 min
Delta R.T.: 0.020 min
Response: 77592348
Conc: 36.78 ug/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

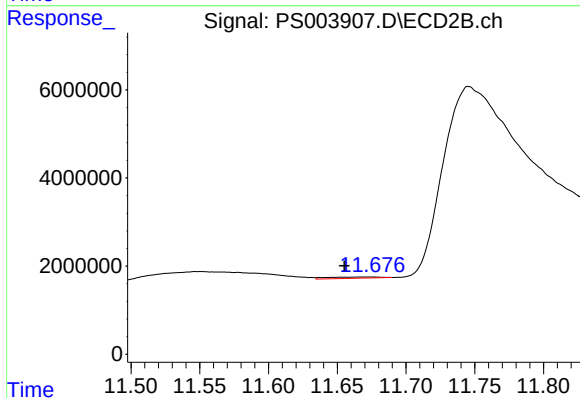


#7 MCPA

R.T.: 11.673 min
Delta R.T.: 0.018 min
Response: 780726
Conc: N.D.

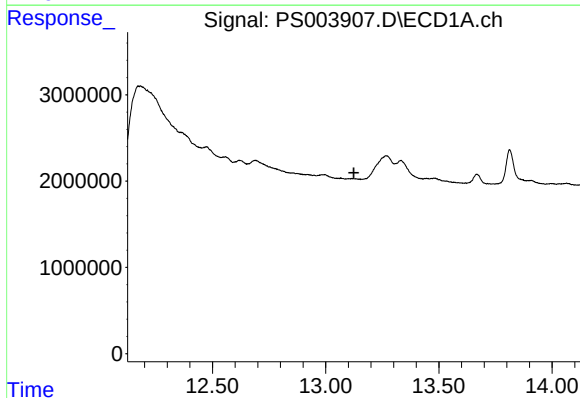


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

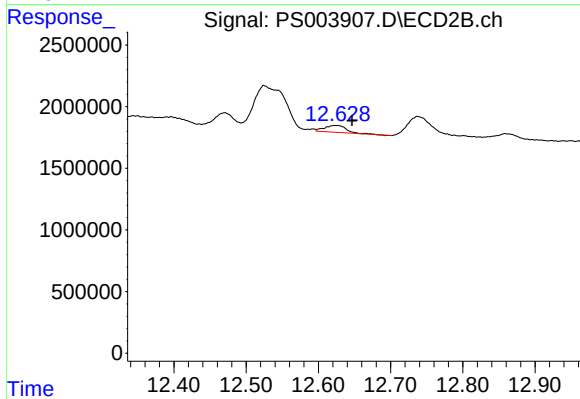

#9 2,4-D


R.T.: 12.624 min
Delta R.T.: -0.022 min
Response: 1153695
Conc: 2.17 ng/ml

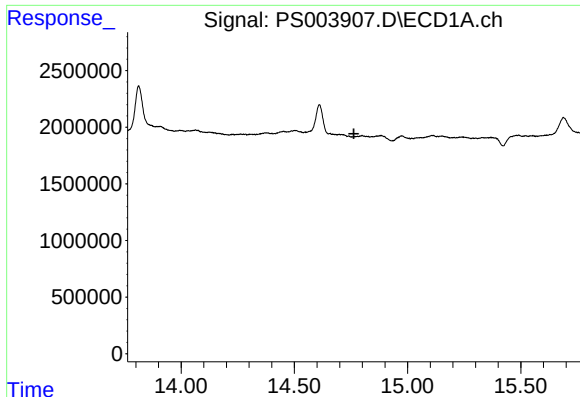

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

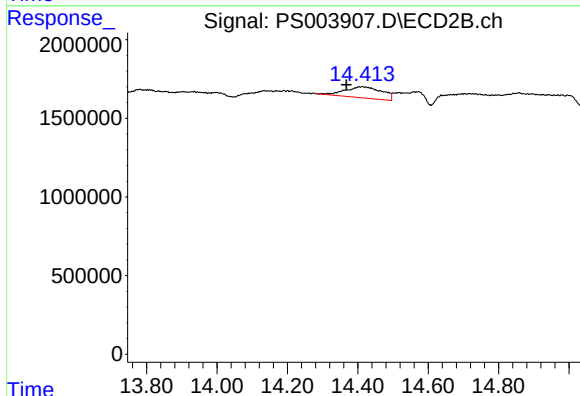


#12 2,4,5-T

R.T.: 14.413 min
Delta R.T.: 0.046 min
Response: 5182061
Conc: 2.38 ng/ml

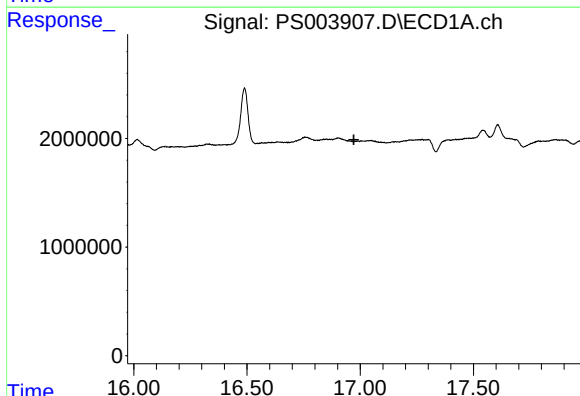


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

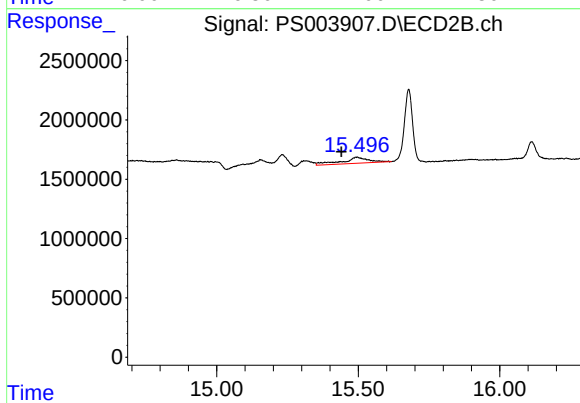

#14 DINOSEB


R.T.: 15.495 min
Delta R.T.: 0.055 min
Response: 3390302
Conc: 1.77 ng/ml

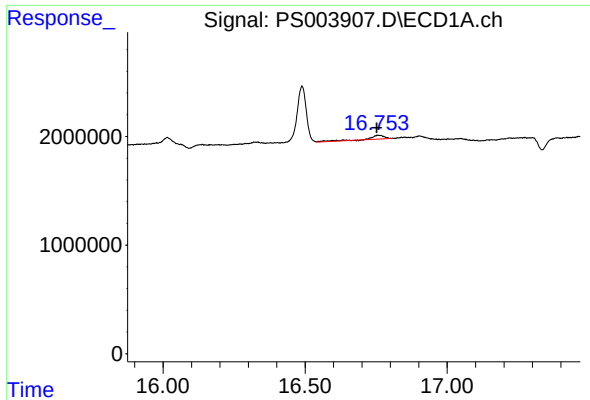

#15 Picloram

R.T.: 16.756 min
Delta R.T.: 0.005 min
Response: 1407905
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-032919

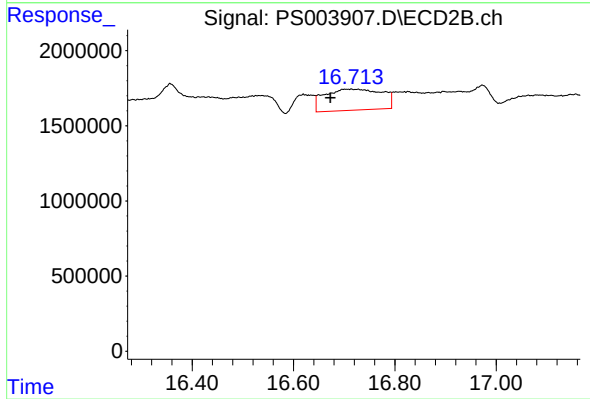

#15 Picloram

R.T.: 16.708 min
Delta R.T.: 0.035 min
Response: 11035637
Conc: 3.48 ng/ml