

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 18:24
 Operator : EI\SJ
 Sample : PB118476BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118476BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:04:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.298	10.800	316.3E6	290.7E6	724.995	592.420
Target Compounds							
1) T	Dalapon	2.817	2.312	47948711	111.4E6	64.315	152.666 #
2) T	3,5-DICHL...	0.000	8.903	0	378162	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.976	0	19975348	N.D.	87.984
5) T	DICAMBA	11.499	11.043	610837	6702106	<MDL	3.604 #
6) T	MCPD	11.981	11.281	3955182	835389	2.843	<MDL #
7) T	MCPA	12.108	11.652	25394184	9703665	12.036	5.441 #
8) T	DICHLORPROP	0.000	12.118	0	41514859	N.D.	89.177
9) T	2,4-D	0.000	12.658	0	4802652	N.D.	9.029
10) T	Pentachlo...	0.000	13.202	0	549146	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.808	0	2227037	N.D.	<MDL
12) T	2,4,5-T	0.000	14.300	0	775755	N.D.	<MDL
13) T	2,4-DB	15.567	15.044	20545375	676624	68.143	2.279 #
14) T	DINOSEB	0.000	15.410	0	499939	N.D.	<MDL
15) T	Picloram	0.000	16.693	0	10902731	N.D.	3.438
16) T	DCPA	0.000	16.574	0	11233889	N.D.	3.324



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 18:24
Operator : EI\SJ
Sample : PB118476BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118476BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:04:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

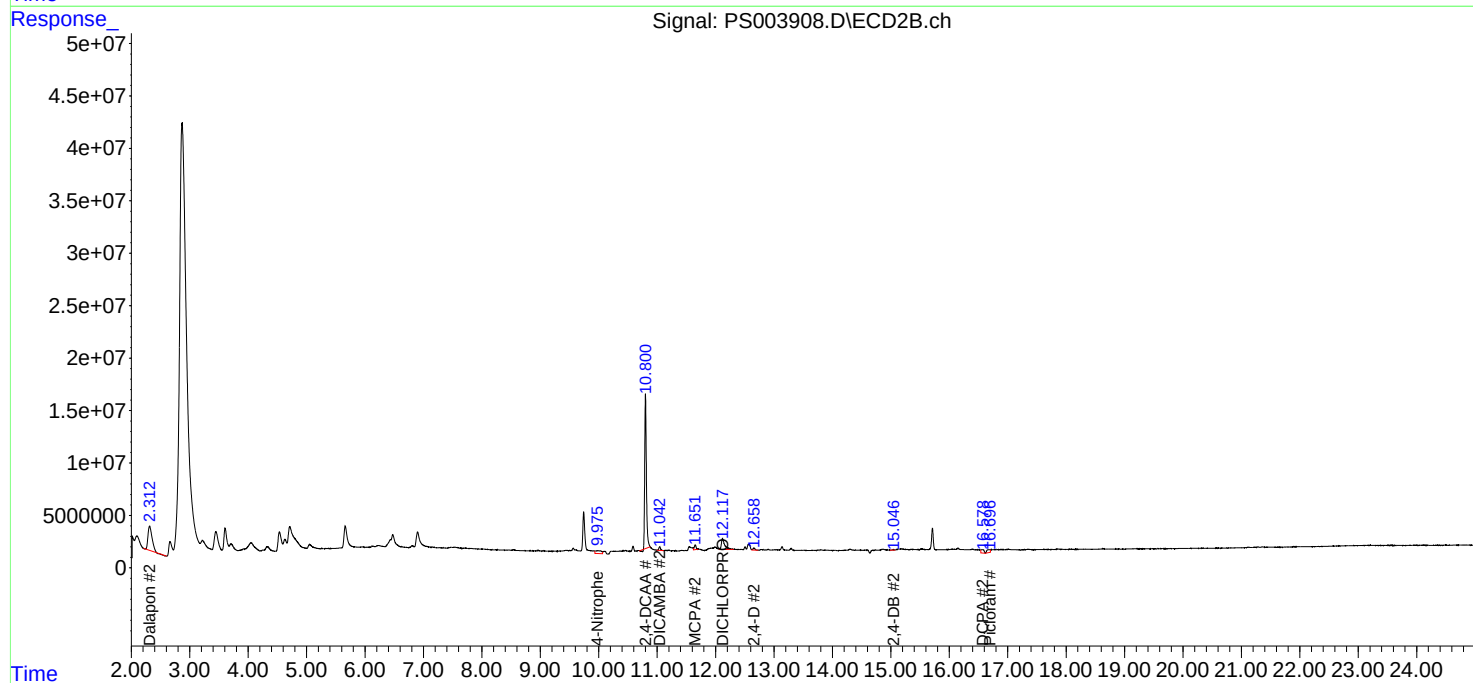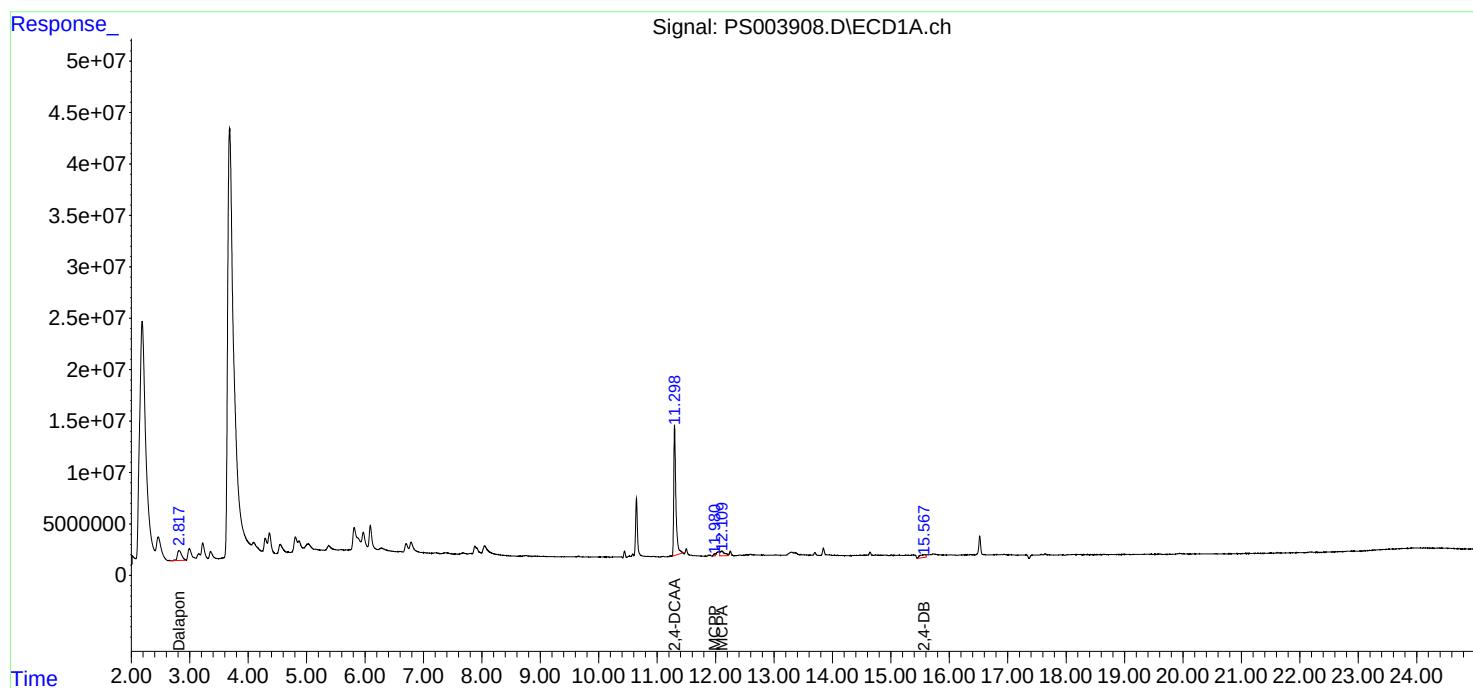


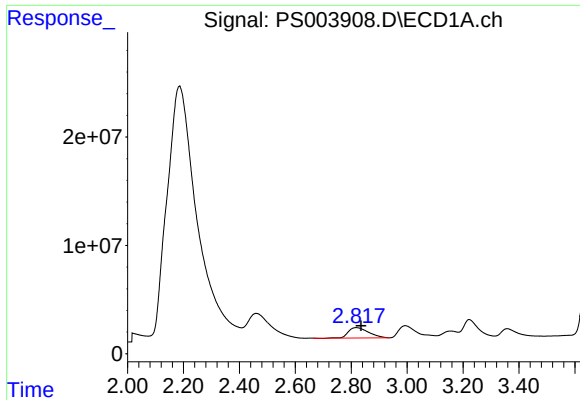

#1 Dalapon


R.T.: 2.817 min
Delta R.T.: -0.018 min
Response: 47948711
Conc: 64.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118476BL

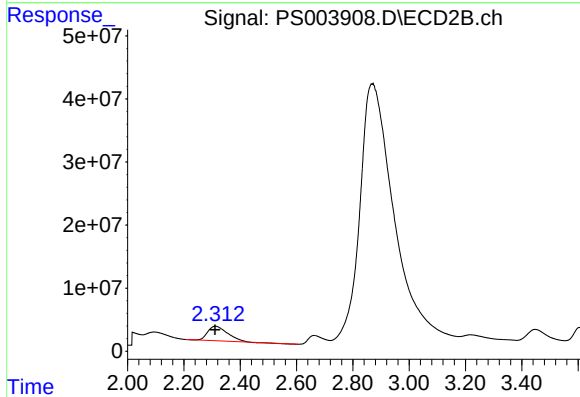


#1 Dalapon

R.T.: 2.312 min
Delta R.T.: 0.002 min
Response: 111389707
Conc: 152.67 ng/ml

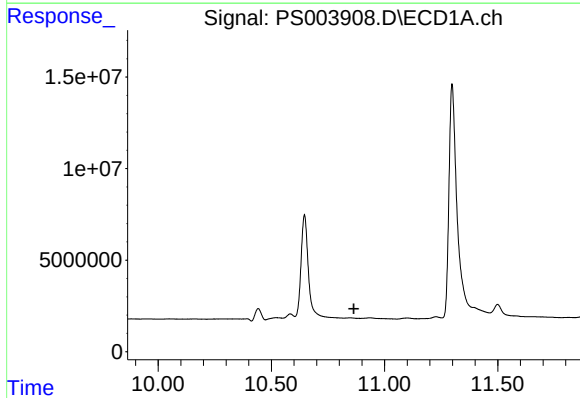


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.865 min
Response: 0
Conc: N.D.

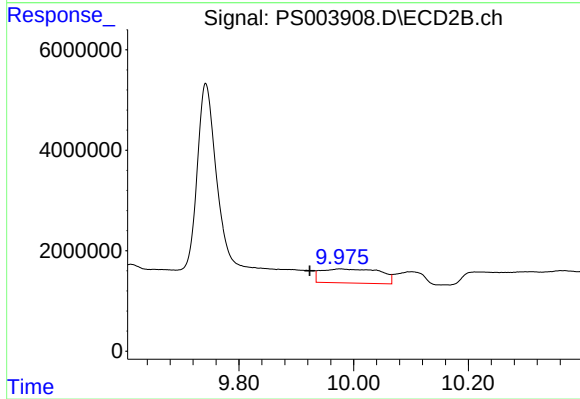

#3 4-Nitrophenol


R.T.: 9.976 min
Delta R.T.: 0.052 min
Response: 19975348
Conc: 87.98 ng/ml

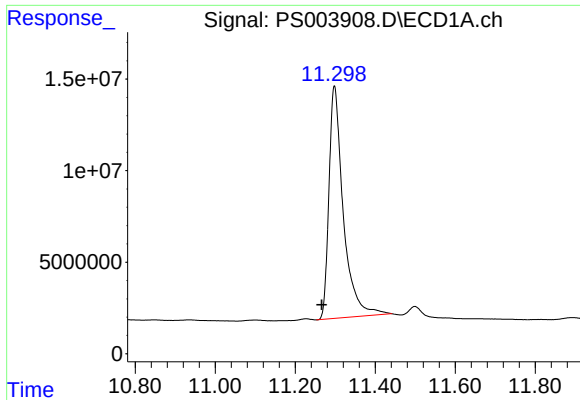

#4 2,4-DCAA


R.T.: 11.298 min
Delta R.T.: 0.031 min
Response: 316251871
Conc: 725.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118476BL

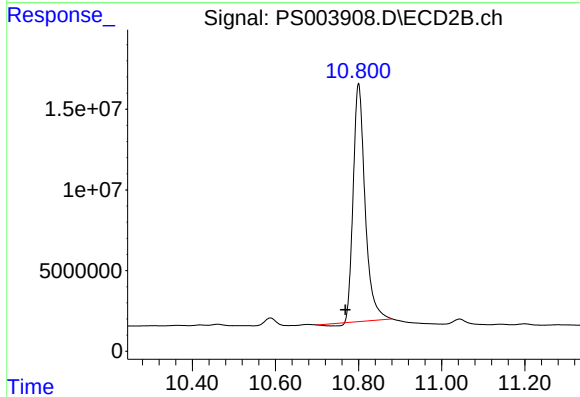


#4 2,4-DCAA

R.T.: 10.800 min
Delta R.T.: 0.031 min
Response: 290675710
Conc: 592.42 ng/ml

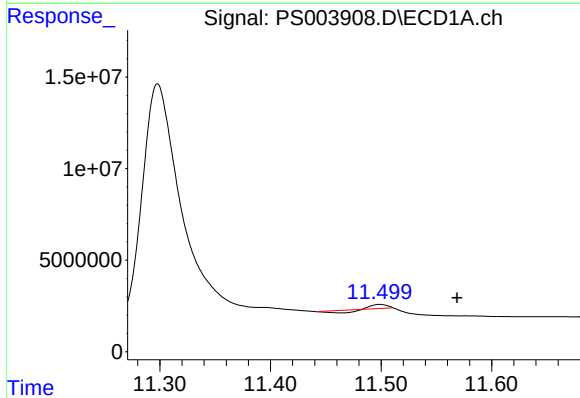


#5 DICAMBA

R.T.: 11.499 min
Delta R.T.: -0.070 min
Response: 610837
Conc: N.D.

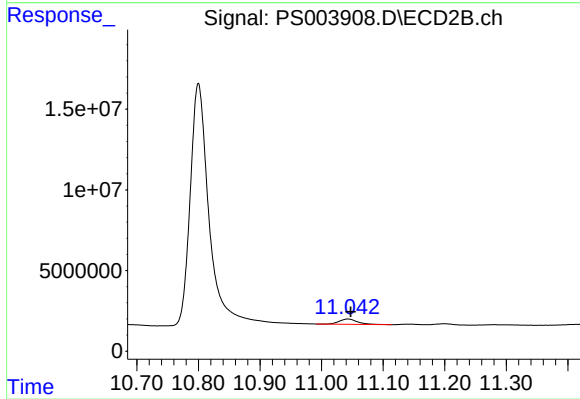

#5 DICAMBA


R.T.: 11.043 min
Delta R.T.: -0.005 min
Response: 6702106
Conc: 3.60 ng/ml

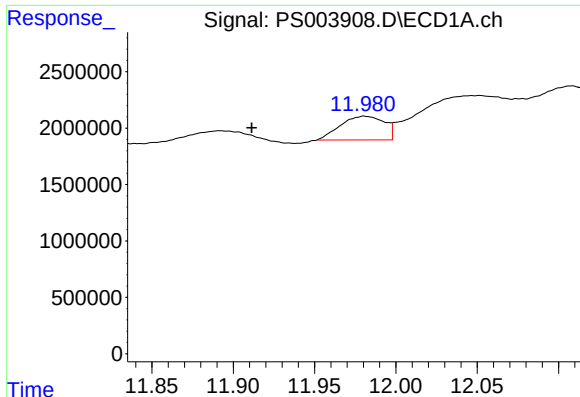

#6 MCP


R.T.: 11.981 min
Delta R.T.: 0.070 min
Response: 3955182
Conc: 2.84 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB118476BL

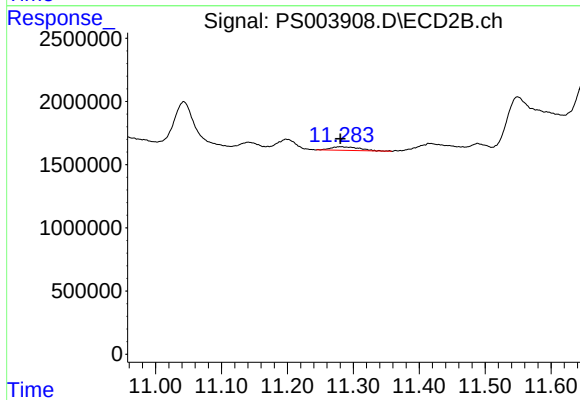


#6 MCP

R.T.: 11.281 min
Delta R.T.: 0.000 min
Response: 835389
Conc: N.D.

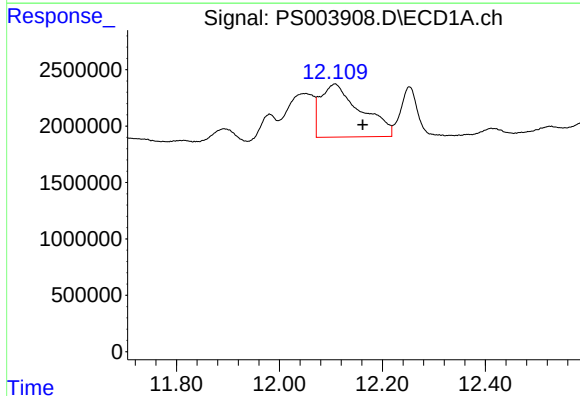


#7 MCP

R.T.: 12.108 min
Delta R.T.: -0.054 min
Response: 25394184
Conc: 12.04 ug/ml

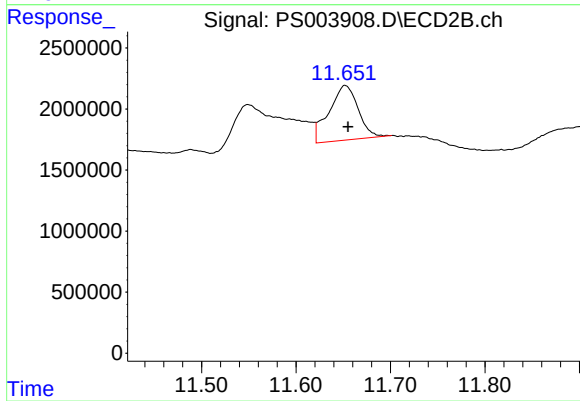

#7 MCP


R.T.: 11.652 min
Delta R.T.: -0.003 min
Response: 9703665
Conc: 5.44 ug/ml

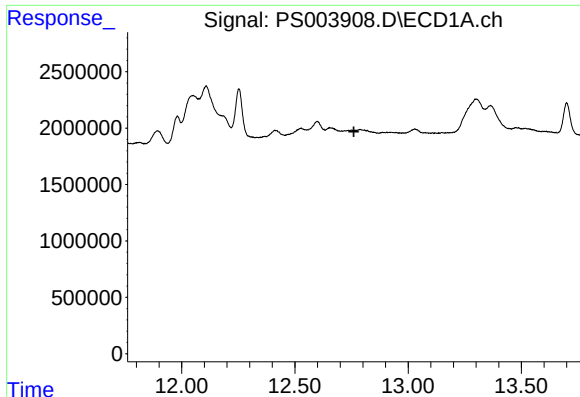

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118476BL

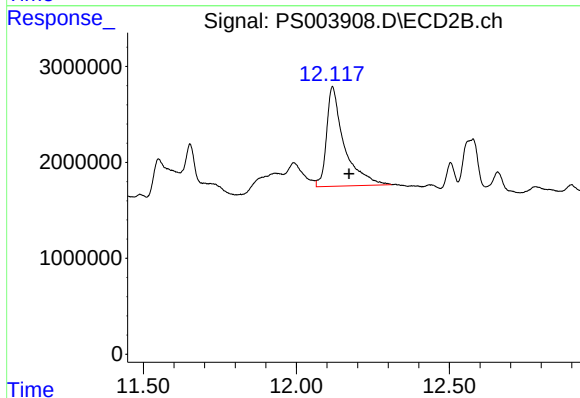


#8 DICHLORPROP

R.T.: 12.118 min
Delta R.T.: -0.055 min
Response: 41514859
Conc: 89.18 ng/ml

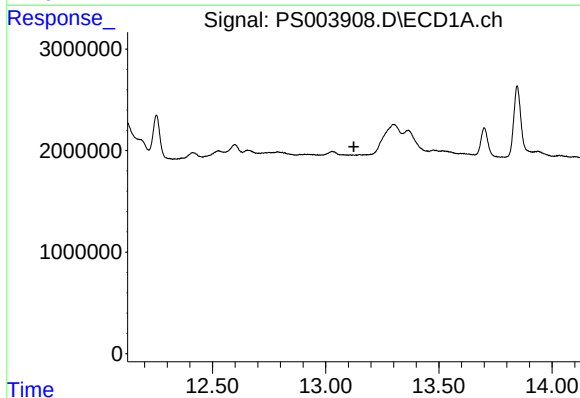


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

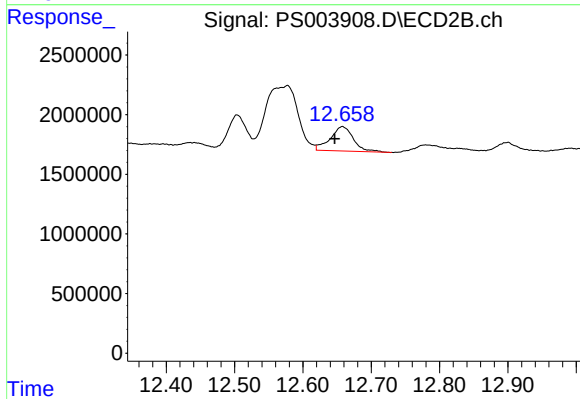

#9 2,4-D


R.T.: 12.658 min
Delta R.T.: 0.011 min
Response: 4802652
Conc: 9.03 ng/ml

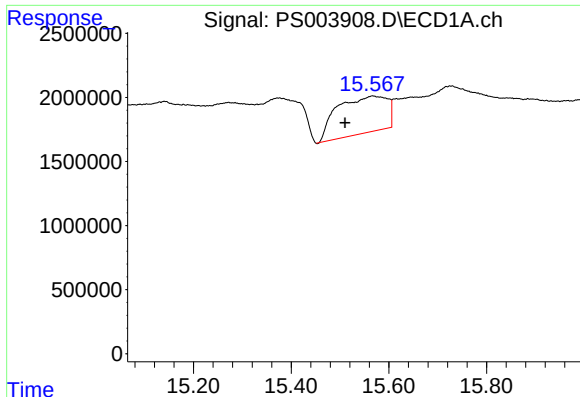

#13 2,4-DB


R.T.: 15.567 min
Delta R.T.: 0.057 min
Response: 20545375
Conc: 68.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118476BL

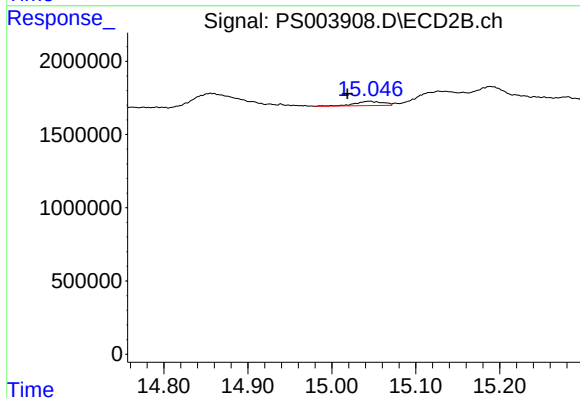


#13 2,4-DB

R.T.: 15.044 min
Delta R.T.: 0.026 min
Response: 676624
Conc: 2.28 ng/ml

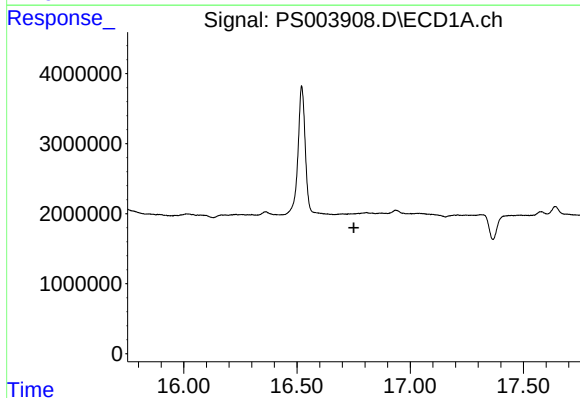


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

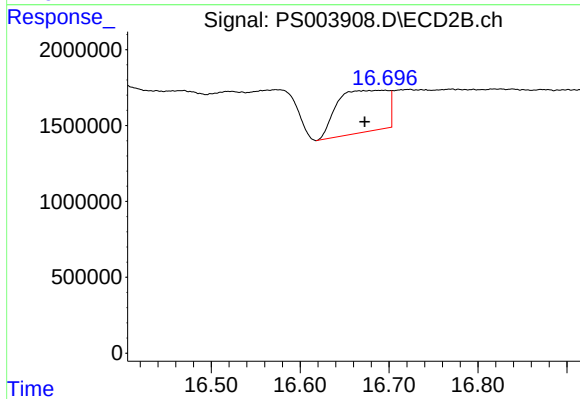

#15 Picloram


R.T.: 16.693 min
Delta R.T.: 0.021 min
Response: 10902731
Conc: 3.44 ng/ml

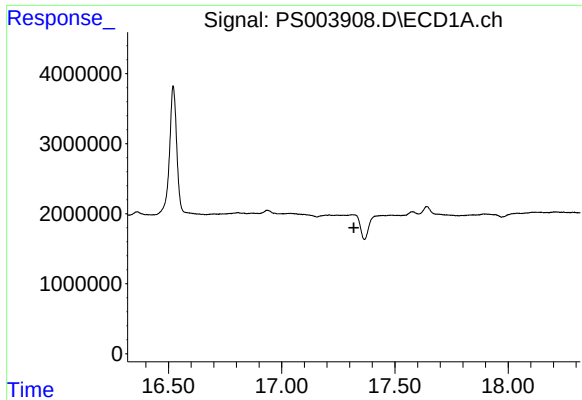

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118476BL

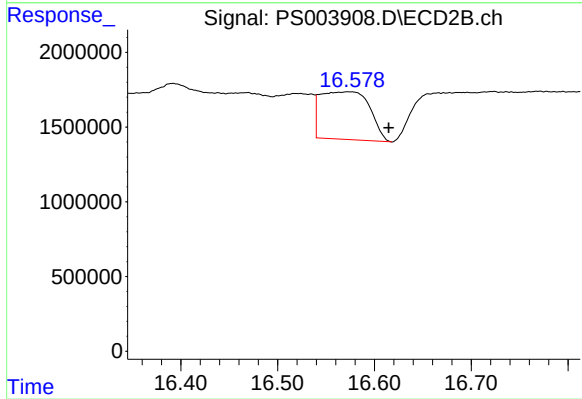

#16 DCPA

R.T.: 16.574 min
Delta R.T.: -0.041 min
Response: 11233889
Conc: 3.32 ng/ml