

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 21:00
 Operator : EI\SJ
 Sample : K2179-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-4S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:06:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.783	218.0E6	199.5E6	499.652	406.498
Target Compounds							
1) T	Dalapon	2.804	2.295	23317396	30571136	31.276	41.900 #
2) T	3,5-DICHL...	0.000	8.949	0	5691737	N.D.	8.923
3) T	4-Nitroph...	0.000	9.959	0	15764276	N.D.	69.436
5) T	DICAMBA	0.000	11.024	0	7997358	N.D.	4.300
6) T	MCPD	0.000	11.259	0	364496	N.D.	<MDL
7) T	MCPA	12.188	0.000	138.0E6	0	65.416	N.D. #
9) T	2,4-D	0.000	12.639	0	1633015	N.D.	3.070
10) T	Pentachlo...	0.000	13.190	0	1301782	N.D.	<MDL
12) T	2,4,5-T	0.000	14.325	0	187613	N.D.	<MDL
13) T	2,4-DB	0.000	15.011	0	983199	N.D.	3.311
14) T	DINOSEB	0.000	15.458	0	860269	N.D.	<MDL
15) T	Picloram	0.000	16.634	0	3648232	N.D.	1.150
16) T	DCPA	0.000	16.634	0	3648232	N.D.	1.079



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 21:00
Operator : EI\SJ
Sample : K2179-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-4S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:06:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

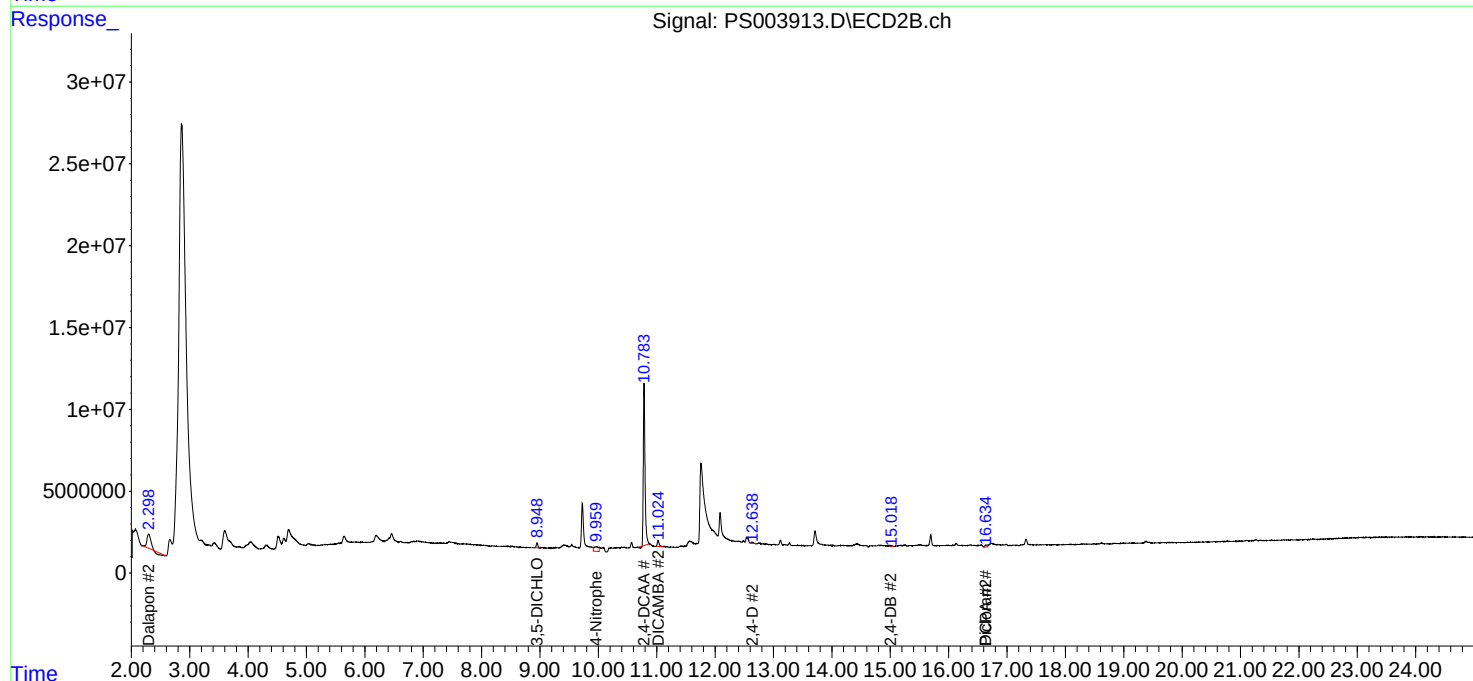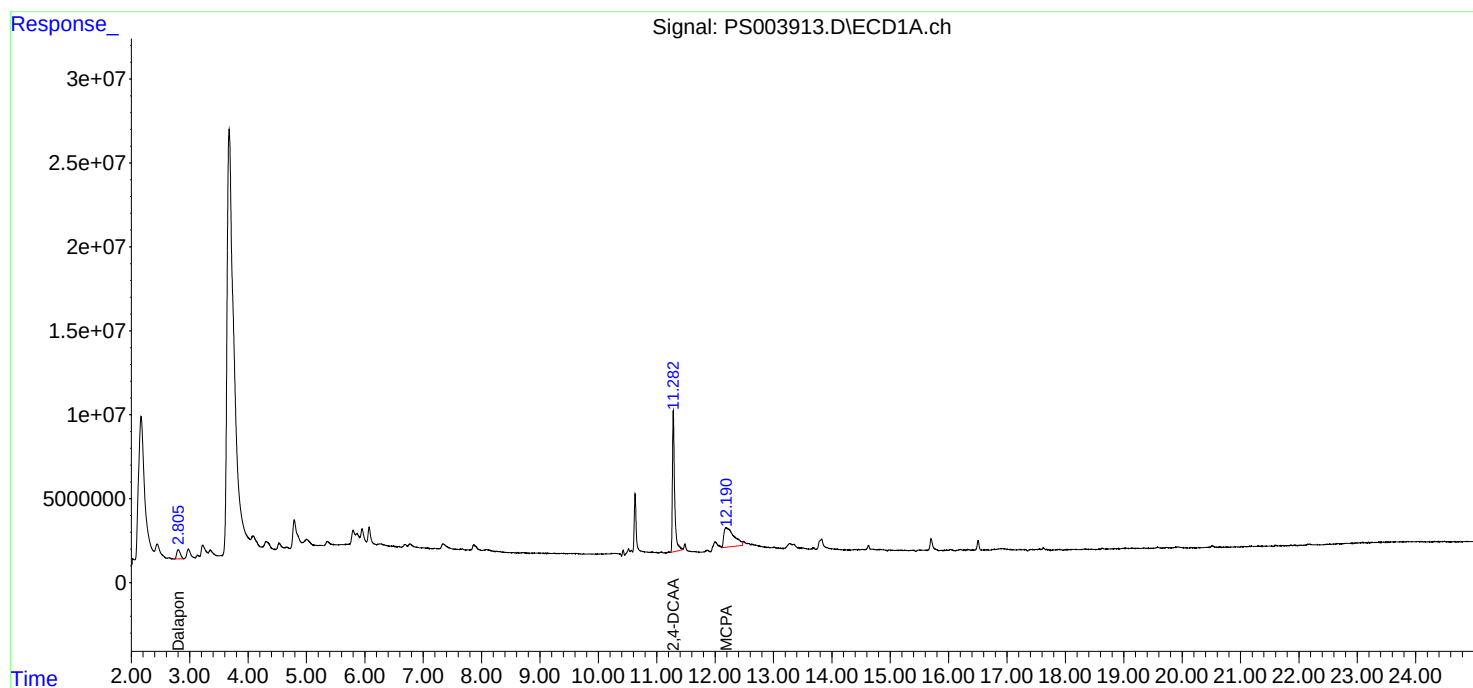


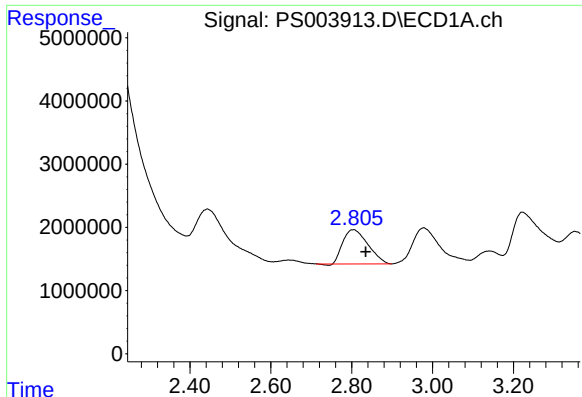

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.031 min
Response: 23317396
Conc: 31.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4S

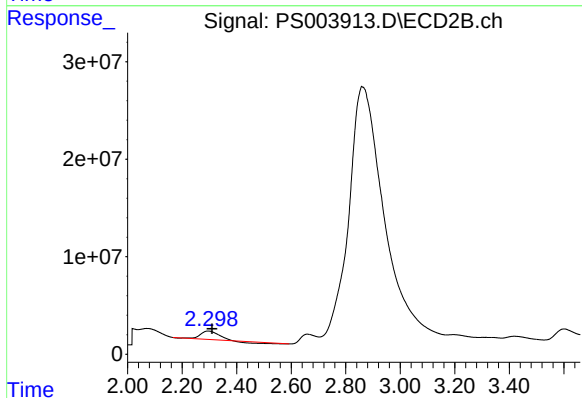


#1 Dalapon

R.T.: 2.295 min
Delta R.T.: -0.015 min
Response: 30571136
Conc: 41.90 ng/ml

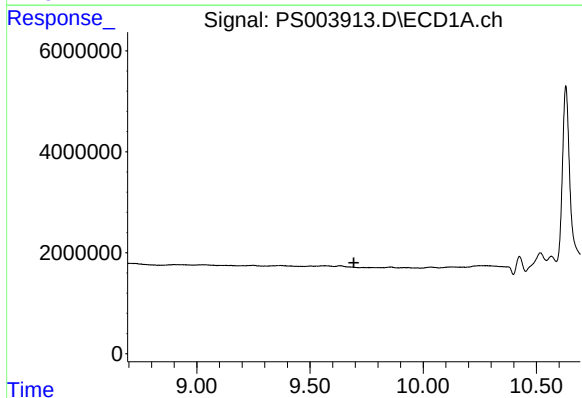


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

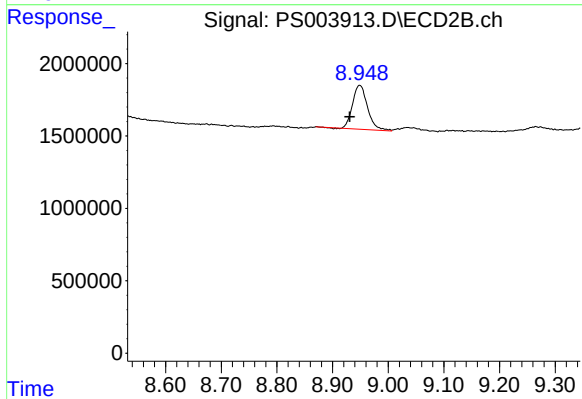

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: 0.018 min
Response: 5691737
Conc: 8.92 ng/ml

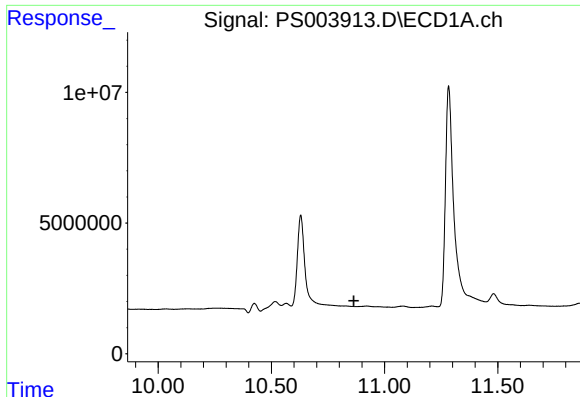

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4S

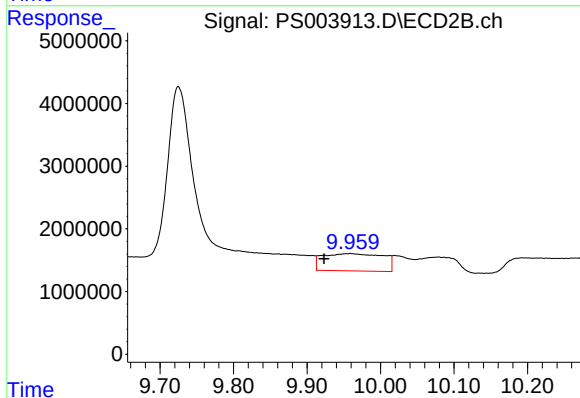


#3 4-Nitrophenol

R.T.: 9.959 min
Delta R.T.: 0.035 min
Response: 15764276
Conc: 69.44 ng/ml

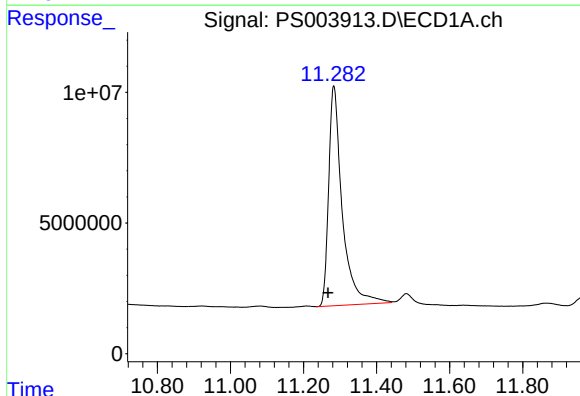


#4 2,4-DCAA

R.T.: 11.284 min
Delta R.T.: 0.017 min
Response: 217954215
Conc: 499.65 ng/ml

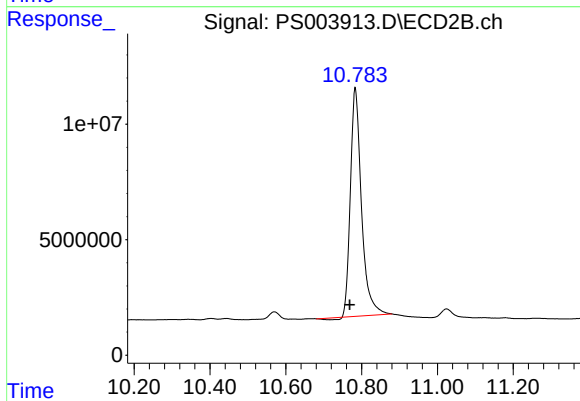

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.015 min
Response: 199451527
Conc: 406.50 ng/ml

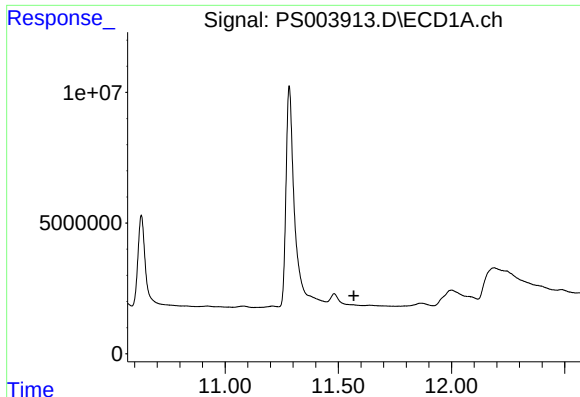

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4S

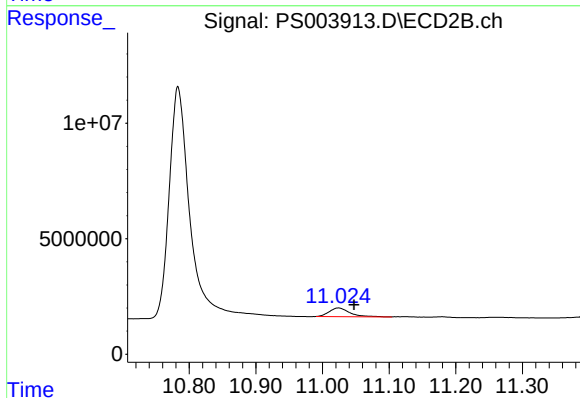


#5 DICAMBA

R.T.: 11.024 min
Delta R.T.: -0.023 min
Response: 7997358
Conc: 4.30 ng/ml

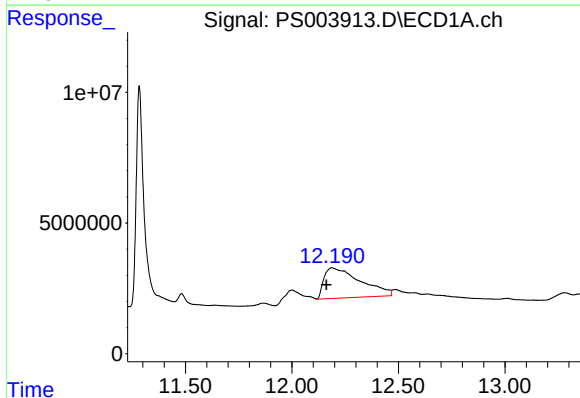


#7 MCPA

R.T.: 12.188 min
Delta R.T.: 0.026 min
Response: 138013574
Conc: 65.42 ug/ml

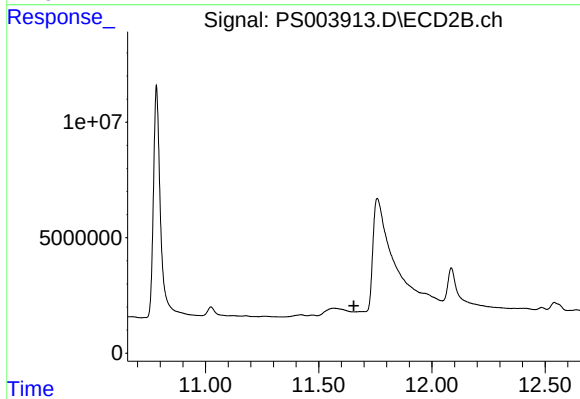

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

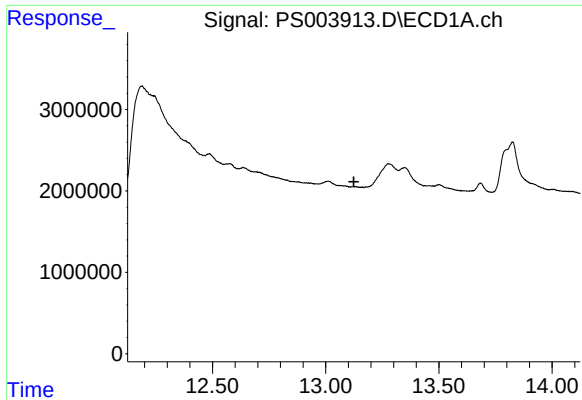

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4S

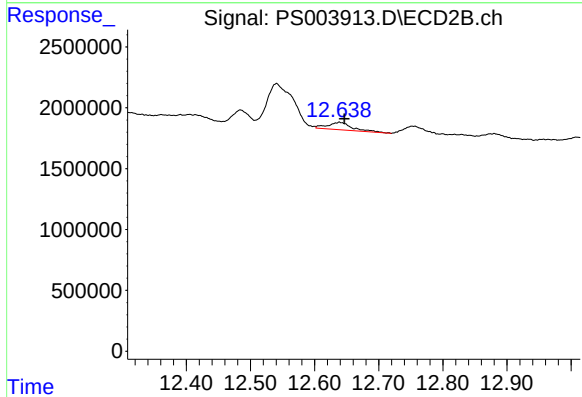


#9 2,4-D

R.T.: 12.639 min
Delta R.T.: -0.007 min
Response: 1633015
Conc: 3.07 ng/ml

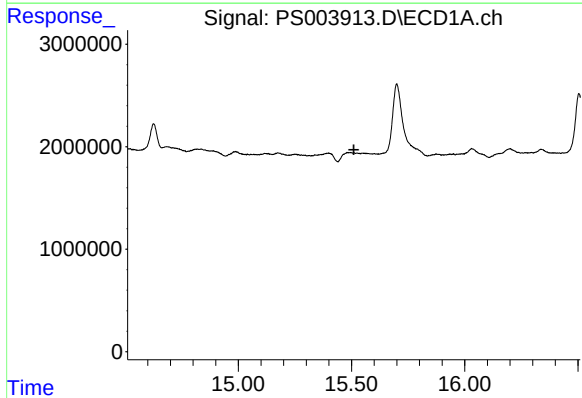


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

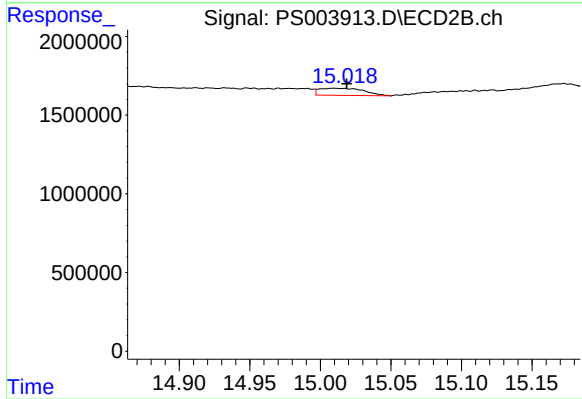

#13 2,4-DB


R.T.: 15.011 min
Delta R.T.: -0.008 min
Response: 983199
Conc: 3.31 ng/ml

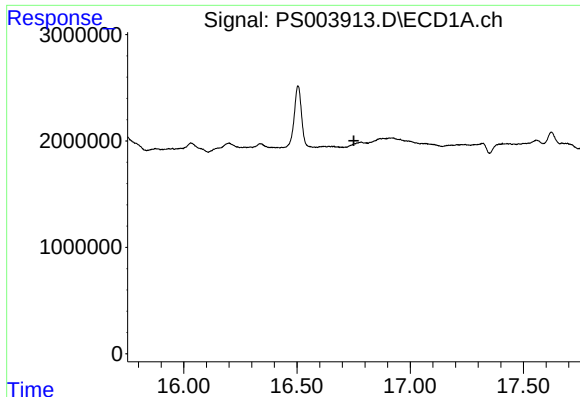

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4S

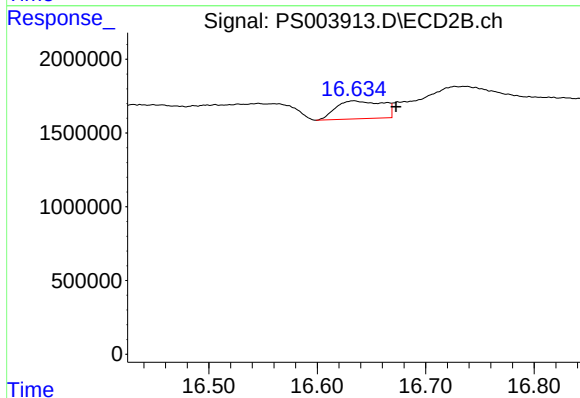


#15 Picloram

R.T.: 16.634 min
Delta R.T.: -0.039 min
Response: 3648232
Conc: 1.15 ng/ml

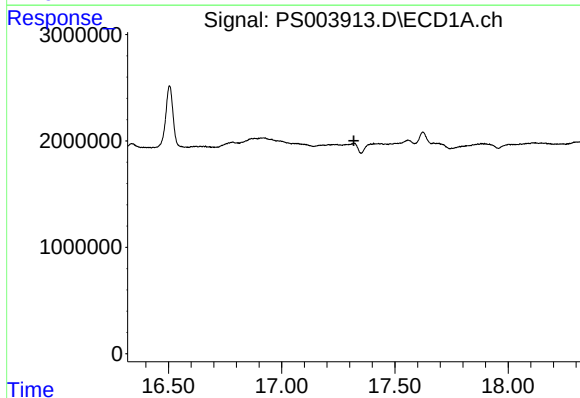

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

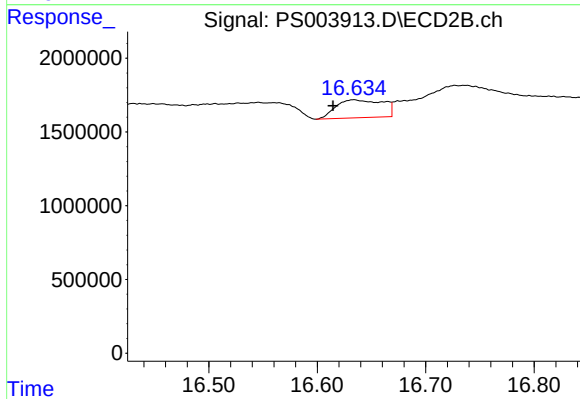

#16 DCPA

R.T.: 16.634 min
Delta R.T.: 0.019 min
Response: 3648232
Conc: 1.08 ng/ml