

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 22:03
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:06:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.286	10.784	237.9E6	227.1E6	545.407	462.797
Target Compounds							
3) T	4-Nitroph...	0.000	9.960	0	86516	N.D.	<MDL
6) T	MCP	0.000	11.304	0	107343	N.D.	<MDL
7) T	MCPA	0.000	11.670	0	892419	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.189	0	1183758	N.D.	2.543
9) T	2,4-D	0.000	12.666	0	108279	N.D.	<MDL
10) T	Pentachlo...	0.000	13.199	0	1378243	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.822	0	300648	N.D.	<MDL
12) T	2,4,5-T	0.000	14.313	0	87339	N.D.	<MDL
13) T	2,4-DB	0.000	14.985	0	305208	N.D.	1.028
14) T	DINOSEB	0.000	15.466	0	884989	N.D.	<MDL
15) T	Picloram	0.000	16.630	0	941561	N.D.	<MDL
16) T	DCPA	0.000	16.630	0	941561	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 22:03
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:06:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

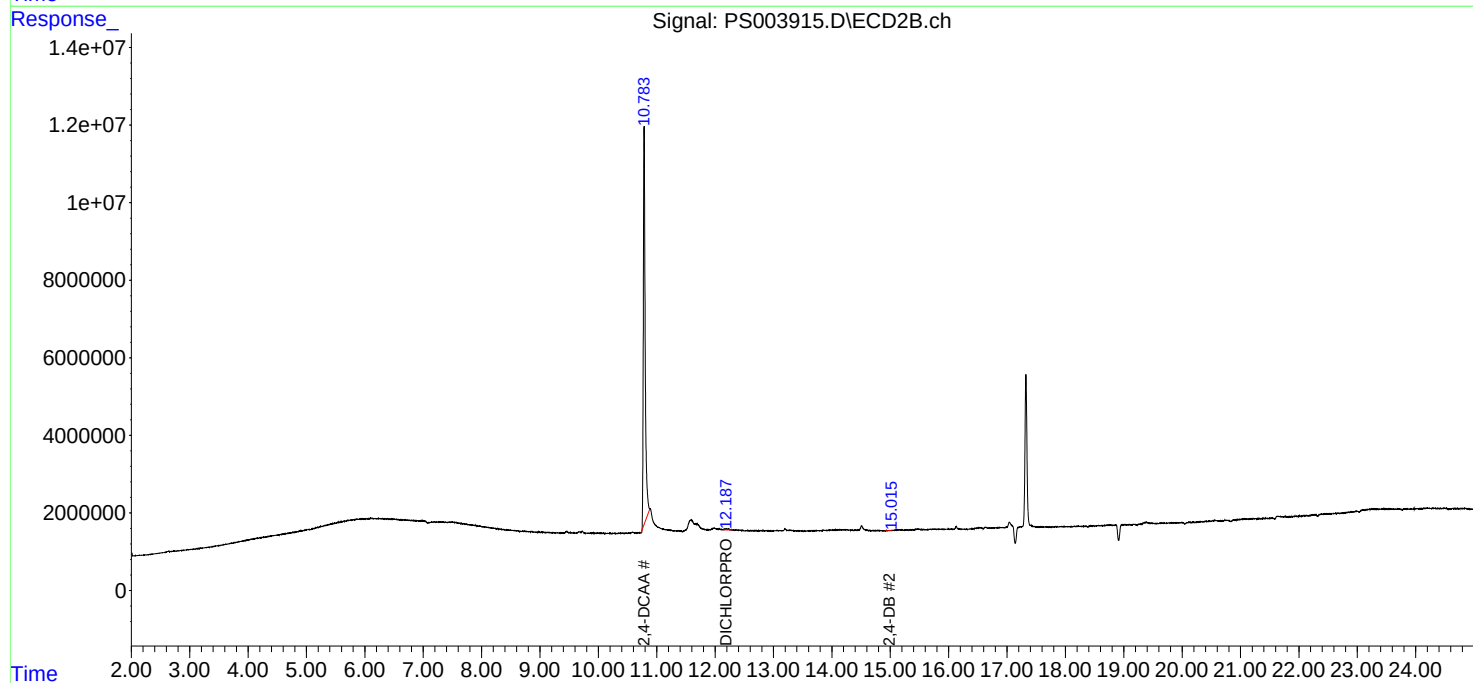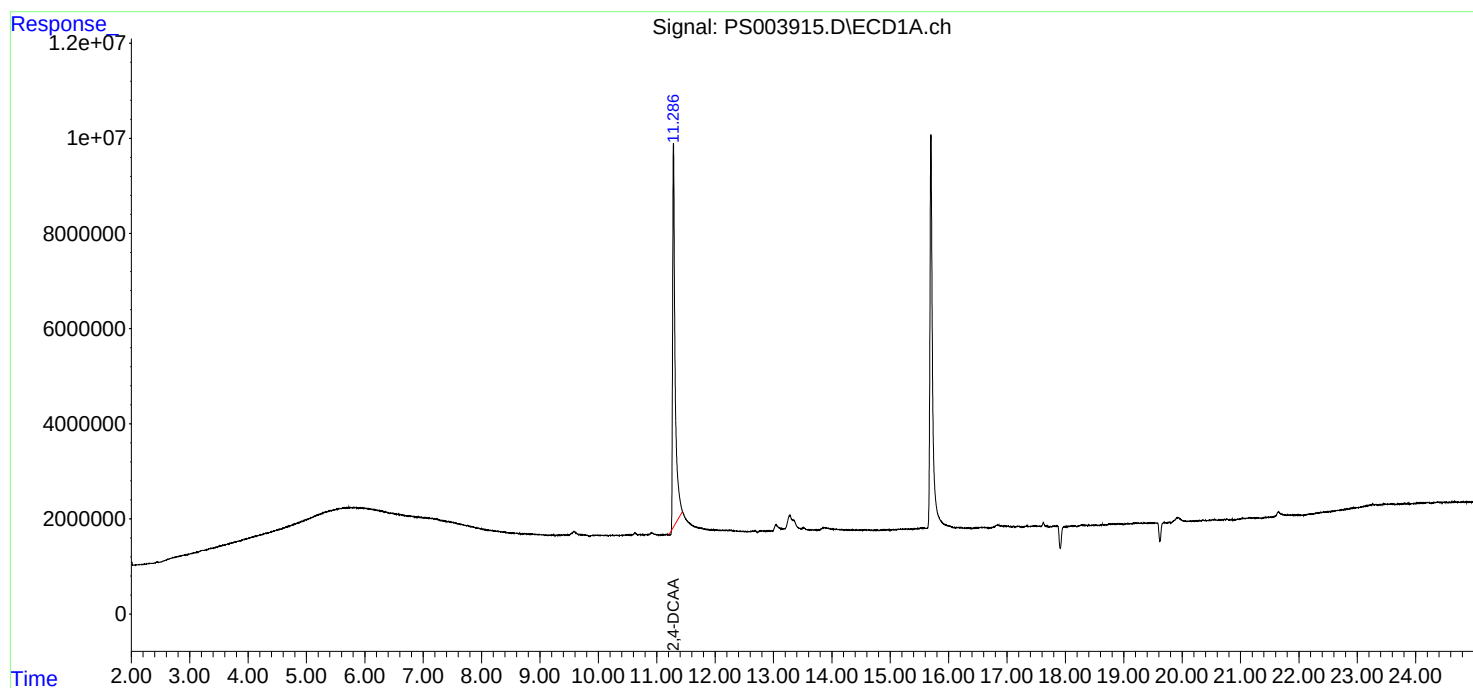


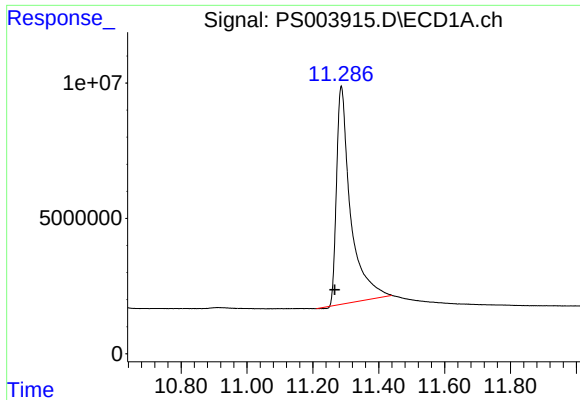

#4 2,4-DCAA


R.T.: 11.286 min
Delta R.T.: 0.020 min
Response: 237913139
Conc: 545.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

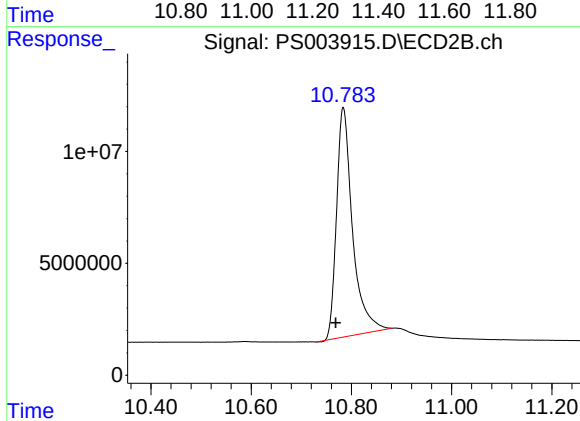


#4 2,4-DCAA

R.T.: 10.784 min
Delta R.T.: 0.015 min
Response: 227075111
Conc: 462.80 ng/ml

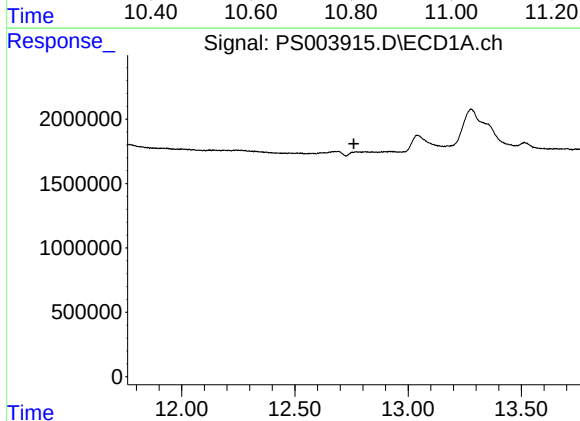


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

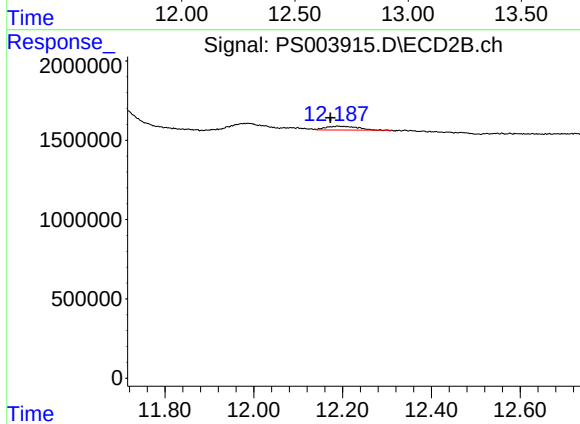

#8 DICHLORPROP


R.T.: 12.189 min
Delta R.T.: 0.016 min
Response: 1183758
Conc: 2.54 ng/ml

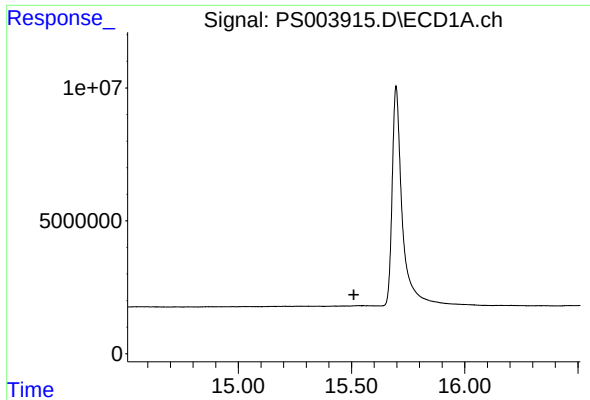

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

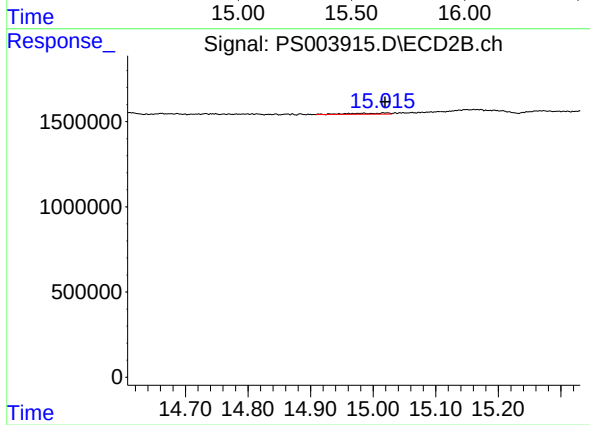

#13 2,4-DB

R.T.: 14.985 min
Delta R.T.: -0.034 min
Response: 305208
Conc: 1.03 ng/ml