

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 00:08
 Operator : EI\SJ
 Sample : K2179-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:07:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.783	260.0E6	238.4E6	595.949	485.790
Target Compounds							
1) T	Dalapon	2.804	2.298	25186841	26060945	33.784	35.718
2) T	3,5-DICHL...	0.000	8.949	0	6434781	N.D.	10.088
3) T	4-Nitroph...	0.000	9.959	0	20214398	N.D.	89.037
5) T	DICAMBA	0.000	11.025	0	7028667	N.D.	3.779
6) T	MCPD	0.000	11.268	0	560937	N.D.	<MDL
7) T	MCPA	12.190	11.666	146.6E6	666358	69.501	<MDL #
9) T	2,4-D	0.000	12.640	0	1831042	N.D.	3.442
10) T	Pentachlo...	0.000	13.119	0	7897065	N.D.	1.141
11) T	2,4,5-TP ...	0.000	13.791	0	3096875	N.D.	1.169
13) T	2,4-DB	0.000	14.980	0	3965853	N.D.	13.355
14) T	DINOSEB	0.000	15.398	0	1673775	N.D.	<MDL
15) T	Picloram	0.000	16.741	0	12364779	N.D.	3.899
16) T	DCPA	0.000	16.555	0	6915768	N.D.	2.046



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 00:08
Operator : EI\SJ
Sample : K2179-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-5S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:07:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

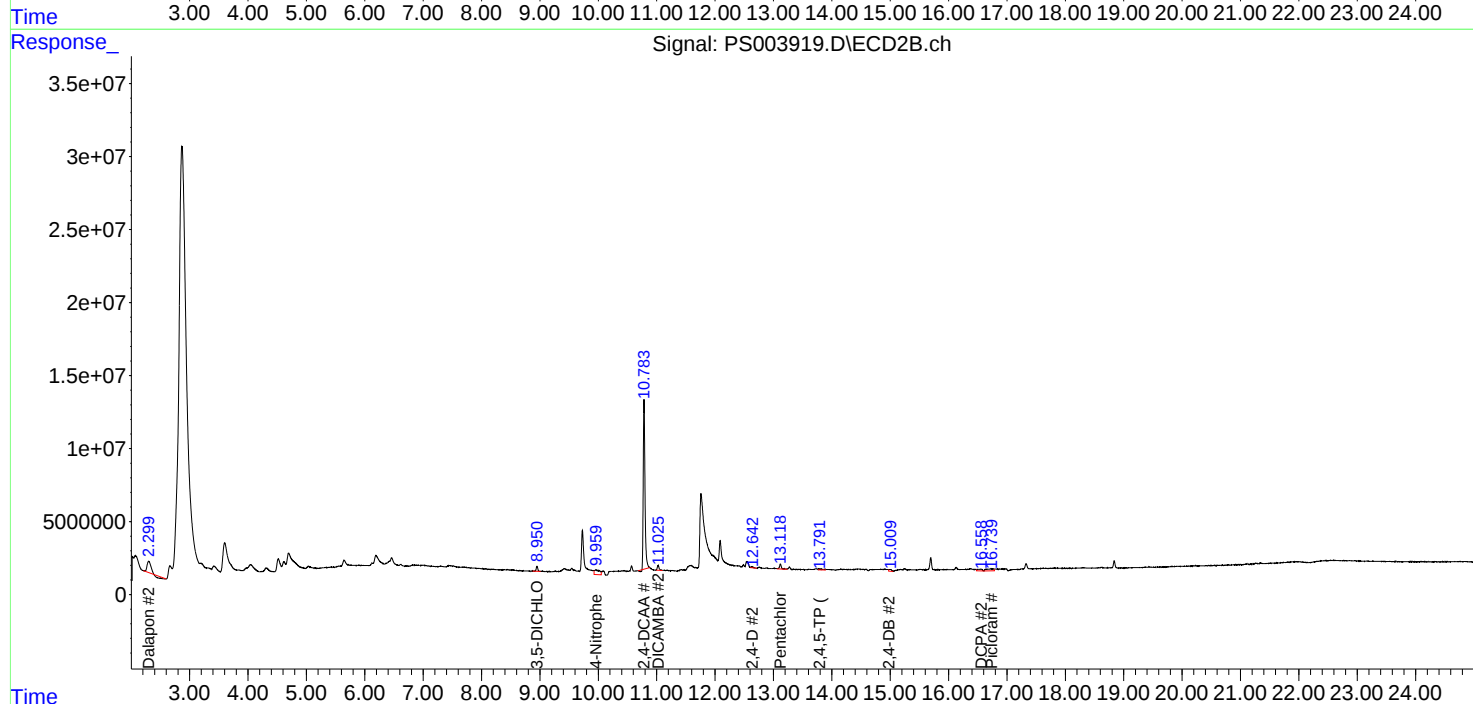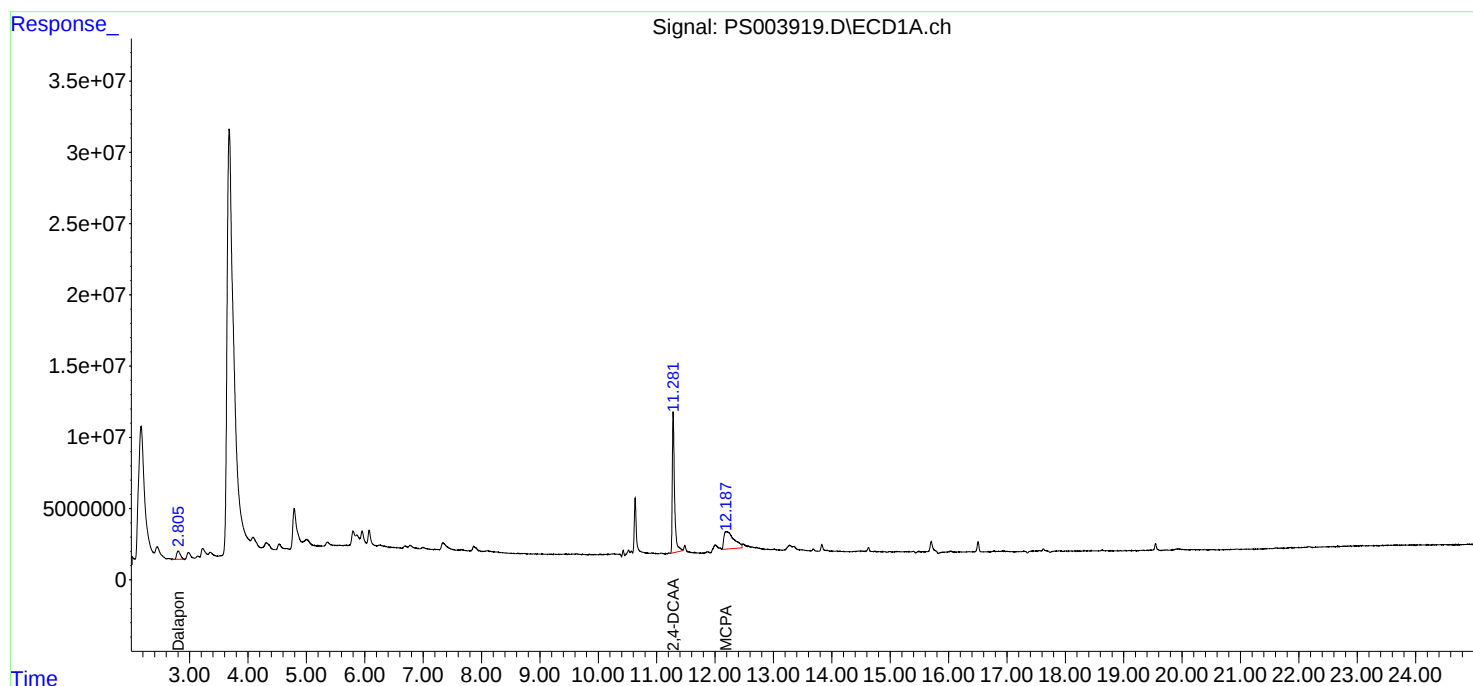


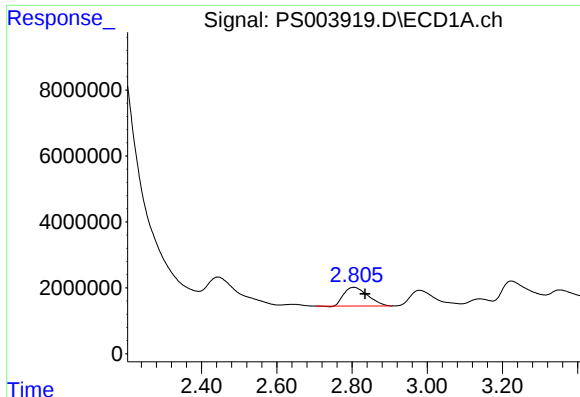

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.031 min
Response: 25186841
Conc: 33.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5S

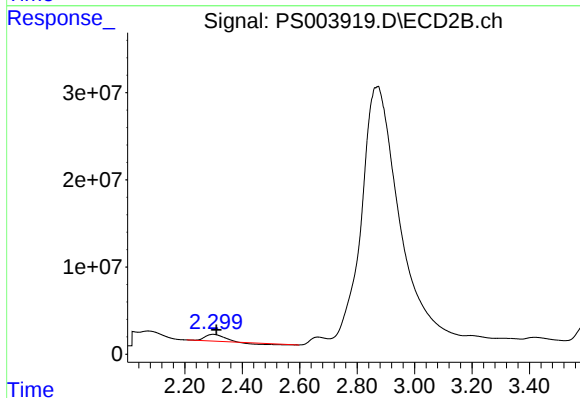


#1 Dalapon

R.T.: 2.298 min
Delta R.T.: -0.012 min
Response: 26060945
Conc: 35.72 ng/ml

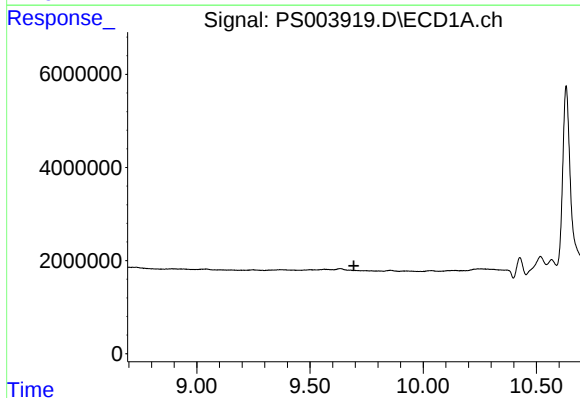


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

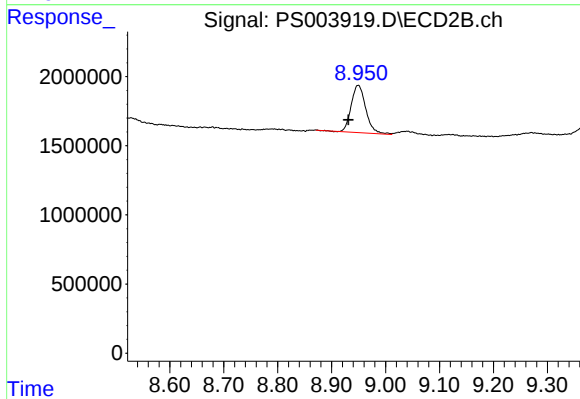

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: 0.018 min
Response: 6434781
Conc: 10.09 ng/ml

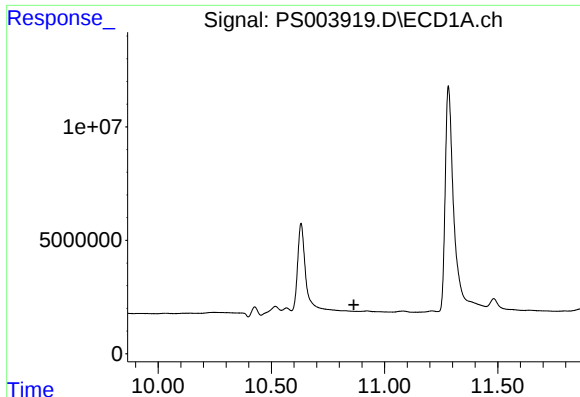

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

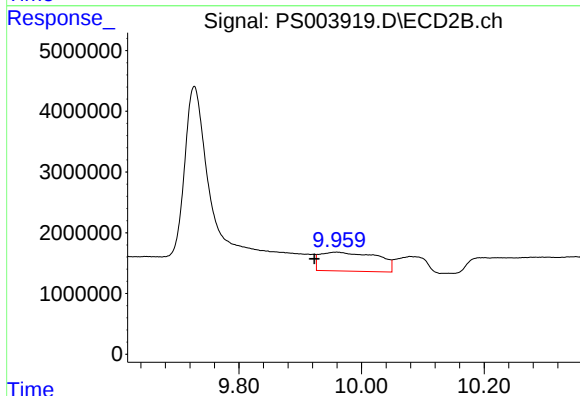


#3 4-Nitrophenol

R.T.: 9.959 min
Delta R.T.: 0.036 min
Response: 20214398
Conc: 89.04 ng/ml

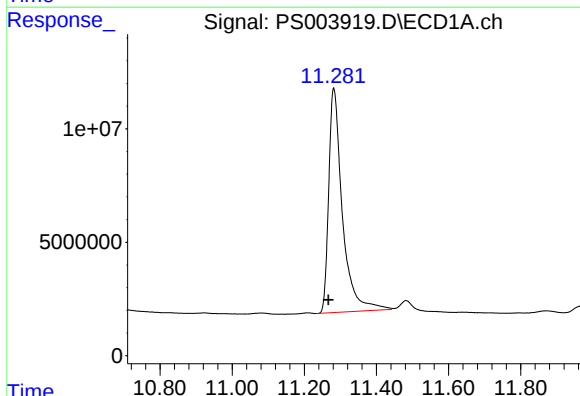


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: 0.015 min
Response: 259960312
Conc: 595.95 ng/ml

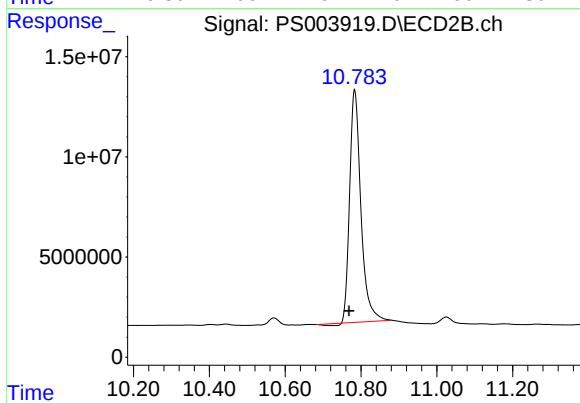

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.014 min
Response: 238357103
Conc: 485.79 ng/ml

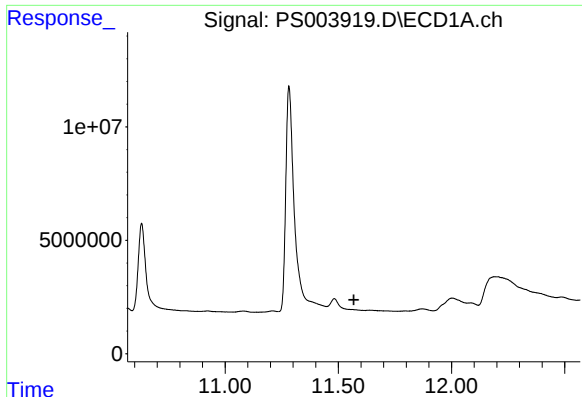

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

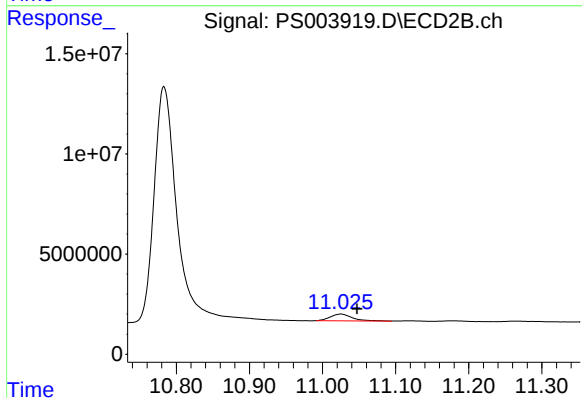


#5 DICAMBA

R.T.: 11.025 min
Delta R.T.: -0.022 min
Response: 7028667
Conc: 3.78 ng/ml

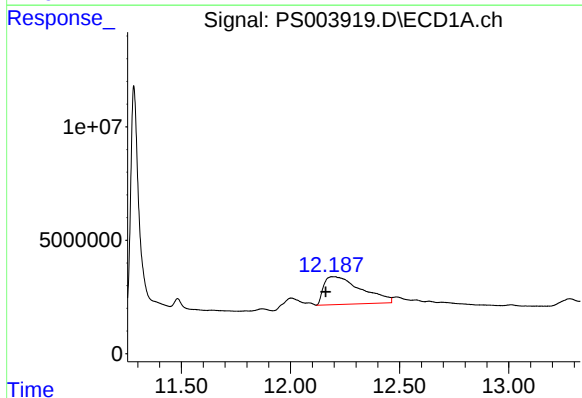


#7 MCPA

R.T.: 12.190 min
Delta R.T.: 0.028 min
Response: 146631572
Conc: 69.50 ug/ml

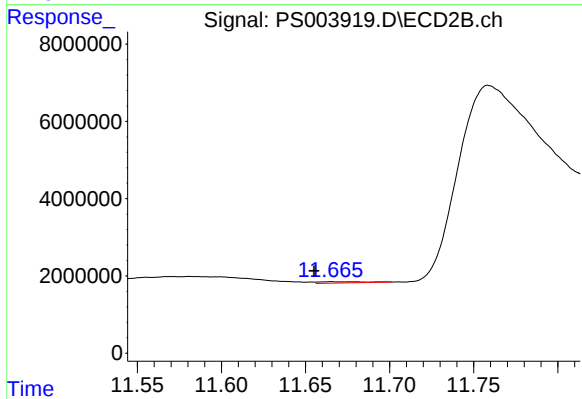

#7 MCPA


R.T.: 11.666 min
Delta R.T.: 0.010 min
Response: 666358
Conc: N.D.

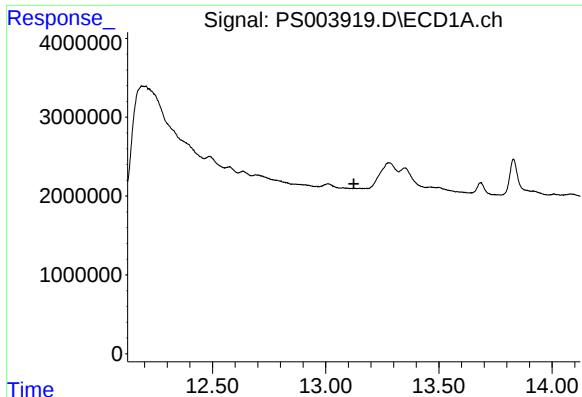

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

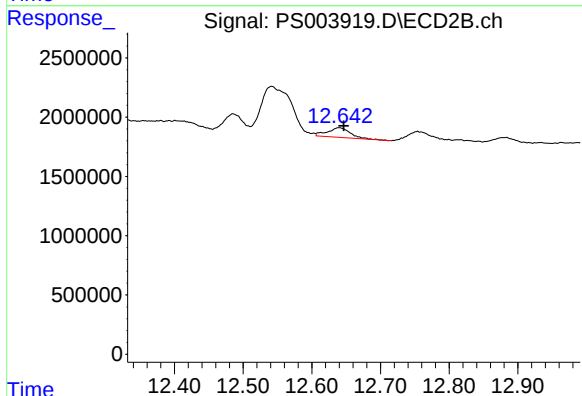


#9 2,4-D

R.T.: 12.640 min
Delta R.T.: -0.006 min
Response: 1831042
Conc: 3.44 ng/ml

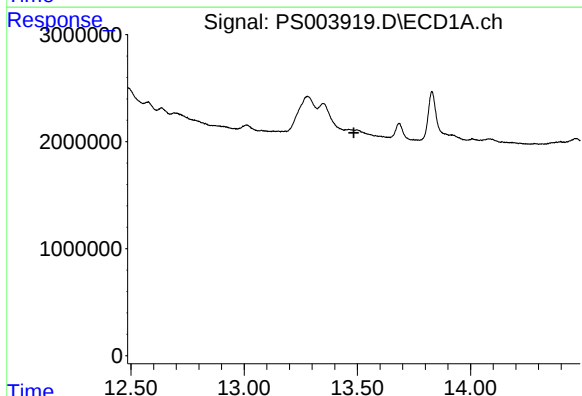


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

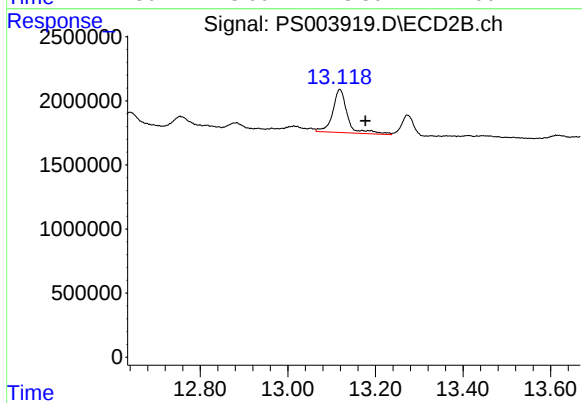

#10 Pentachlorophenol


R.T.: 13.119 min
Delta R.T.: -0.058 min
Response: 7897065
Conc: 1.14 ng/ml

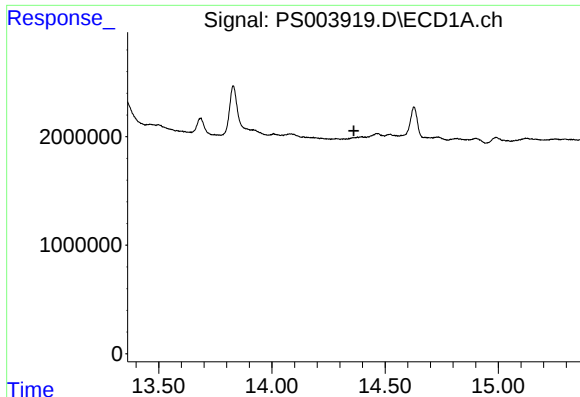

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

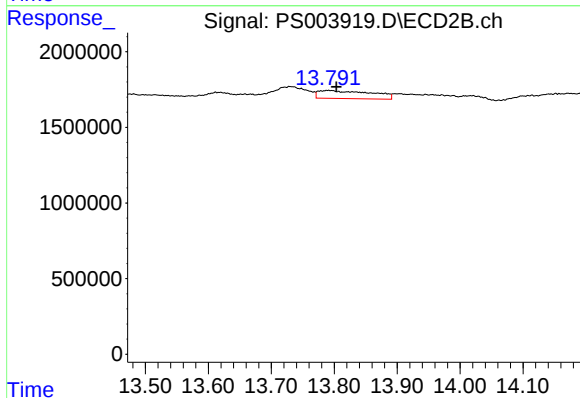


#11 2,4,5-TP (SILVEX)

R.T.: 13.791 min
Delta R.T.: -0.013 min
Response: 3096875
Conc: 1.17 ng/ml

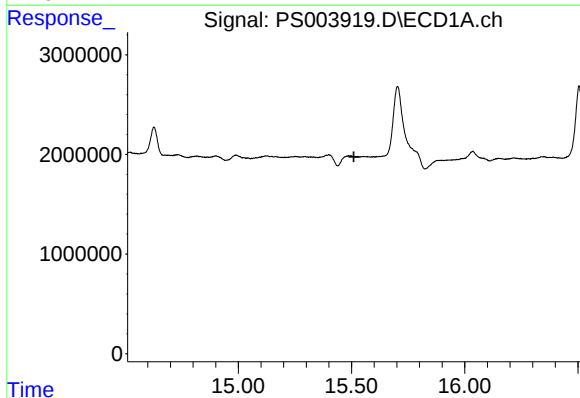


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

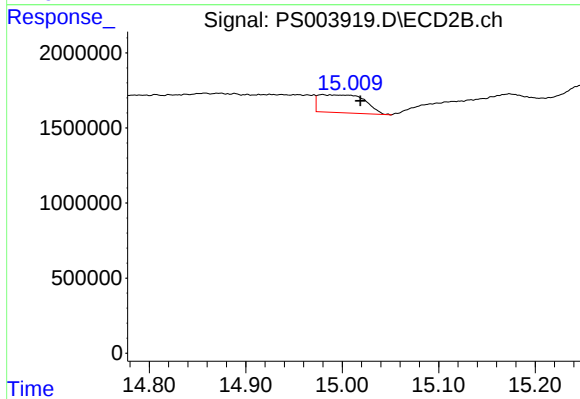

#13 2,4-DB


R.T.: 14.980 min
Delta R.T.: -0.039 min
Response: 3965853
Conc: 13.36 ng/ml

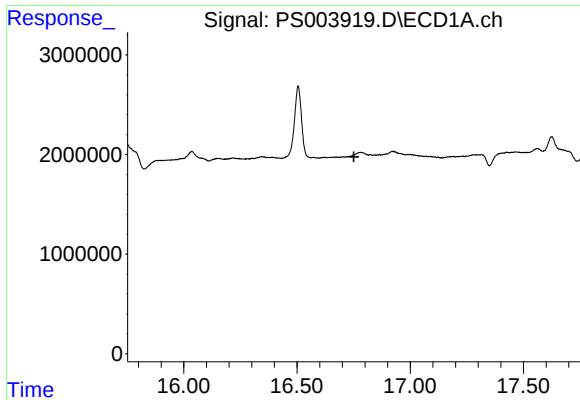

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

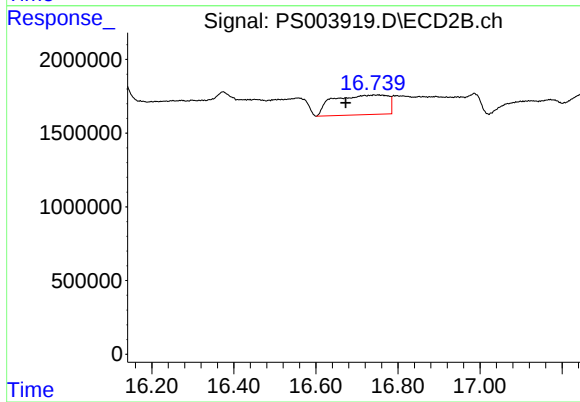


#15 Picloram

R.T.: 16.741 min
Delta R.T.: 0.069 min
Response: 12364779
Conc: 3.90 ng/ml

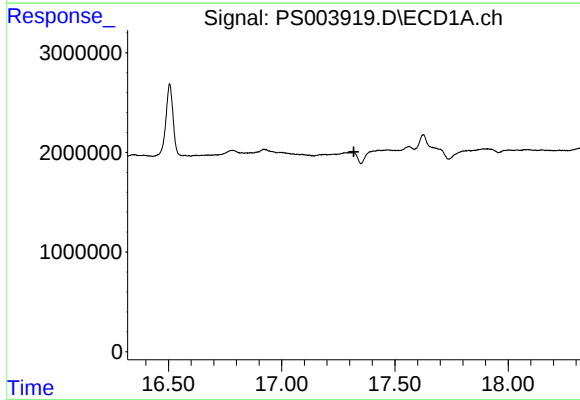

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

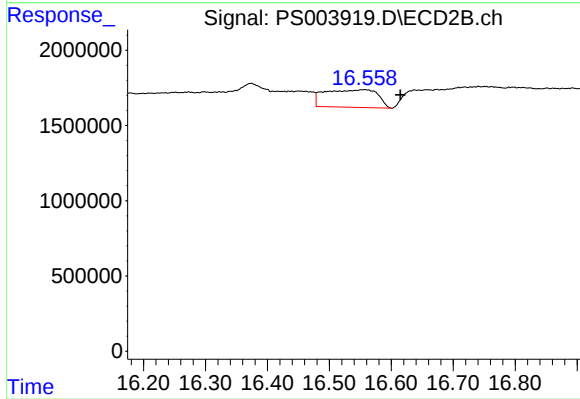

#16 DCPA

R.T.: 16.555 min
Delta R.T.: -0.059 min
Response: 6915768
Conc: 2.05 ng/ml