

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 00:39
 Operator : EI\SJ
 Sample : K2180-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:38:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.769	266.2E6	254.0E6	610.216	517.710
Target Compounds							
1) T	Dalapon	2.788	2.283	26436579	24450424	35.460	33.511
2) T	3,5-DICHL...	0.000	8.934	0	6814813	N.D.	10.684
3) T	4-Nitroph...	0.000	9.945	0	13129013	N.D.	57.828
5) T	DICAMBA	0.000	11.009	0	2743309	N.D.	1.475
7) T	MCPA	12.202	11.665	142.0E6	292772	67.315	<MDL #
9) T	2,4-D	0.000	12.626	0	2046556	N.D.	3.848
11) T	2,4,5-TP ...	0.000	13.777	0	2070831	N.D.	<MDL
12) T	2,4,5-T	0.000	14.310	0	98025	N.D.	<MDL
13) T	2,4-DB	0.000	14.964	0	3842418	N.D.	12.940
14) T	DINOSEB	0.000	15.434	0	421647	N.D.	<MDL
15) T	Picloram	0.000	16.623	0	4092890	N.D.	1.291
16) T	DCPA	0.000	16.623	0	4092890	N.D.	1.211



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 00:39
Operator : EI\SJ
Sample : K2180-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:38:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

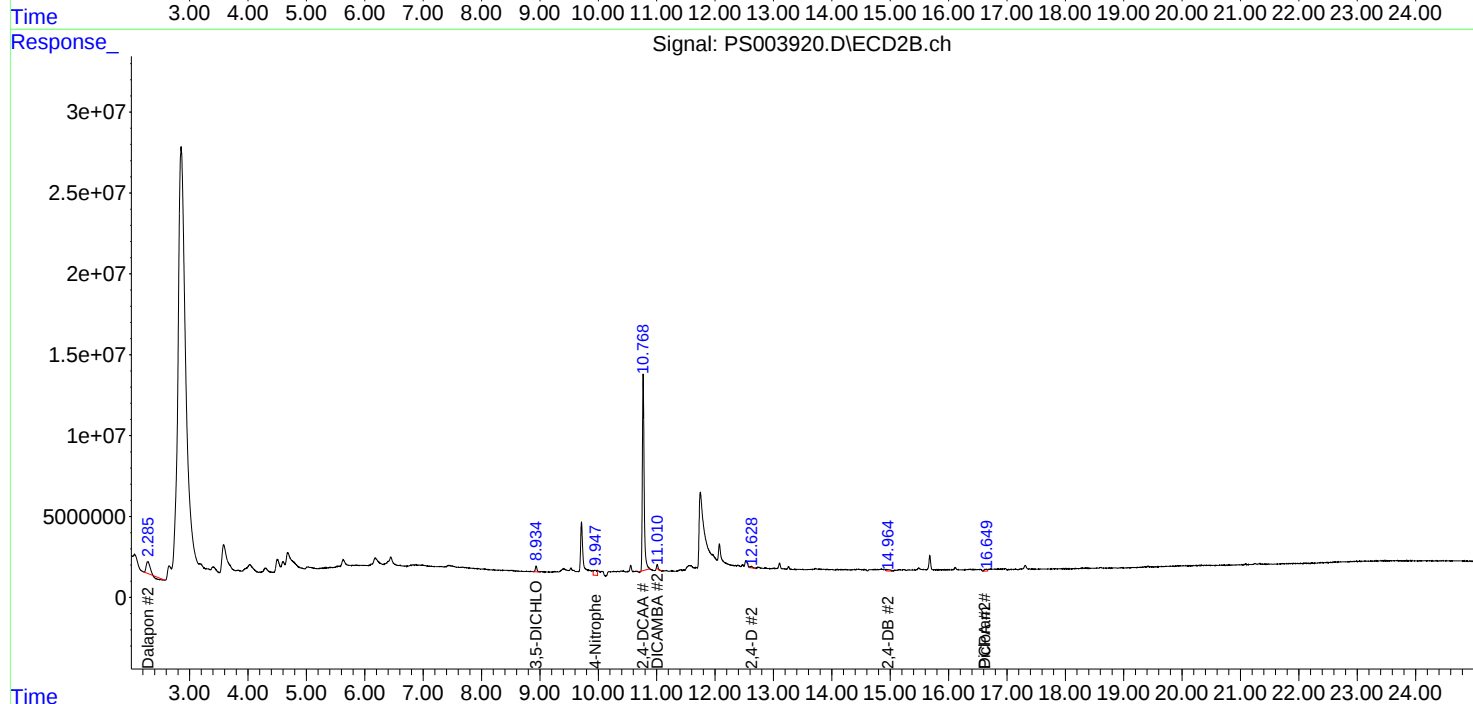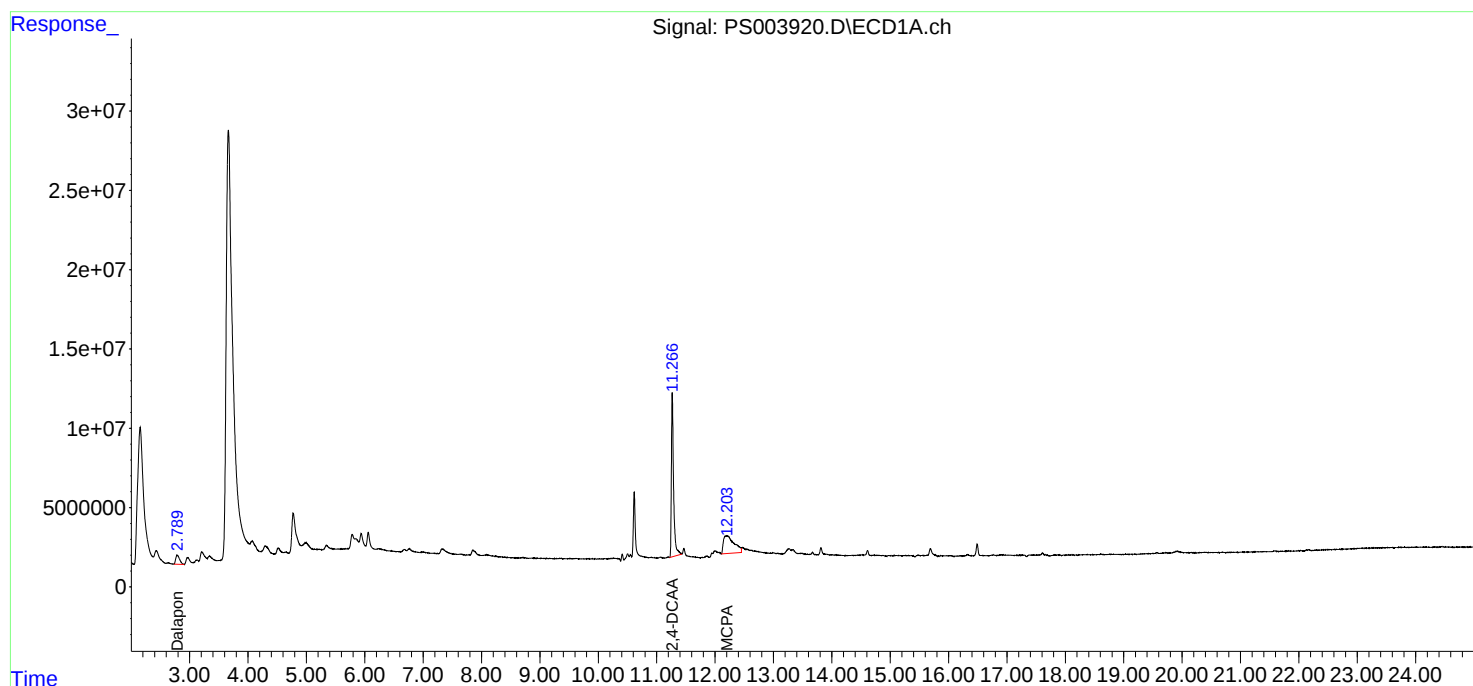


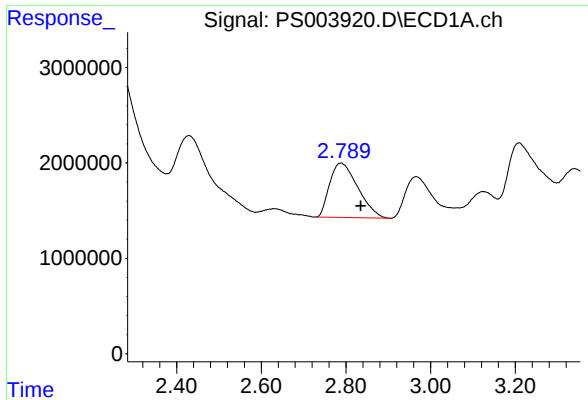

#1 Dalapon


R.T.: 2.788 min
Delta R.T.: -0.047 min
Response: 26436579
Conc: 35.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

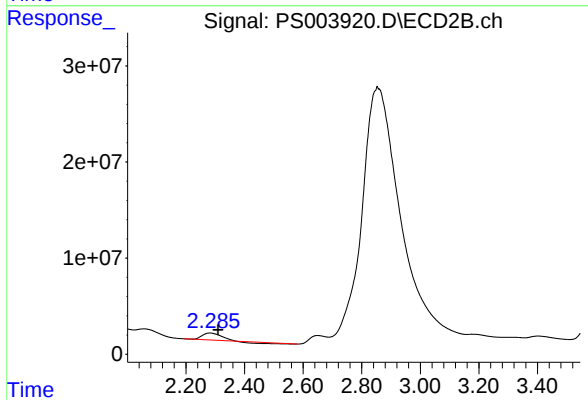


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.027 min
Response: 24450424
Conc: 33.51 ng/ml

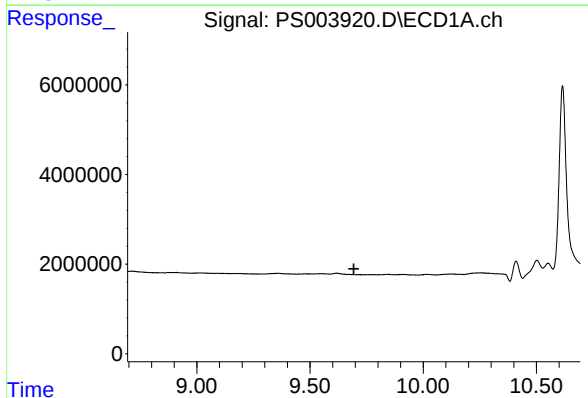


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

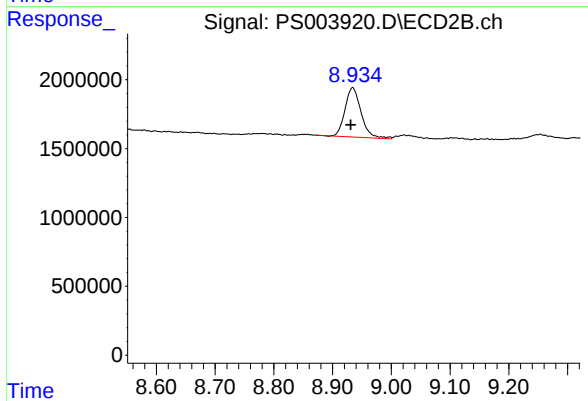

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.934 min
Delta R.T.: 0.003 min
Response: 6814813
Conc: 10.68 ng/ml

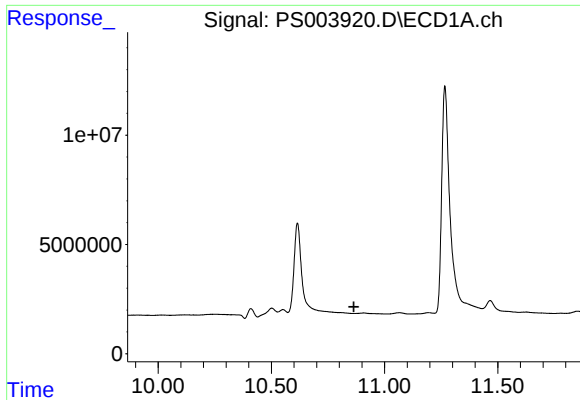

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

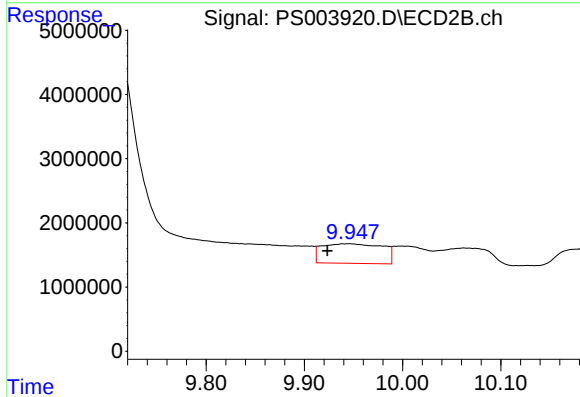


#3 4-Nitrophenol

R.T.: 9.945 min
Delta R.T.: 0.021 min
Response: 13129013
Conc: 57.83 ng/ml

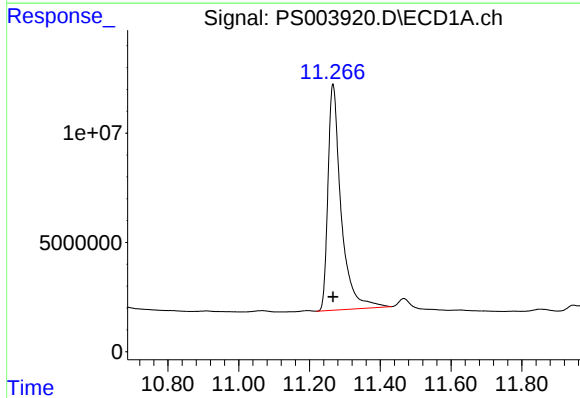


#4 2,4-DCAA

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 266183906
Conc: 610.22 ng/ml

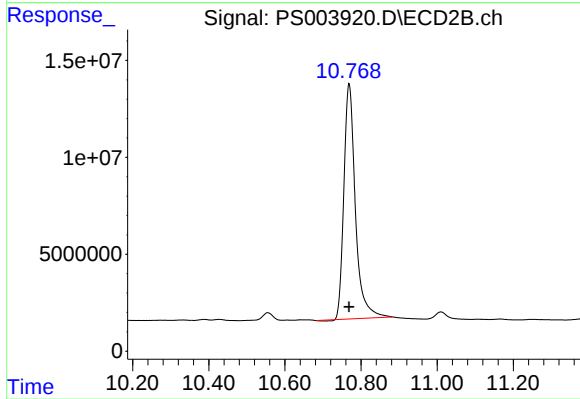

#4 2,4-DCAA


R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 254018734
Conc: 517.71 ng/ml

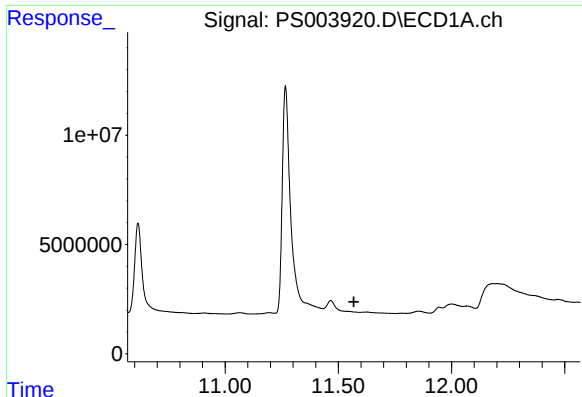

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

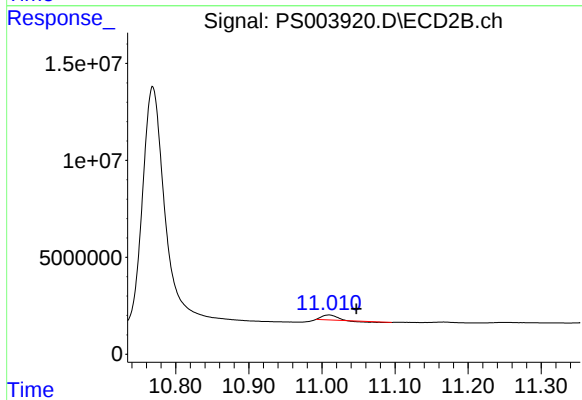


#5 DICAMBA

R.T.: 11.009 min
Delta R.T.: -0.038 min
Response: 2743309
Conc: 1.48 ng/ml

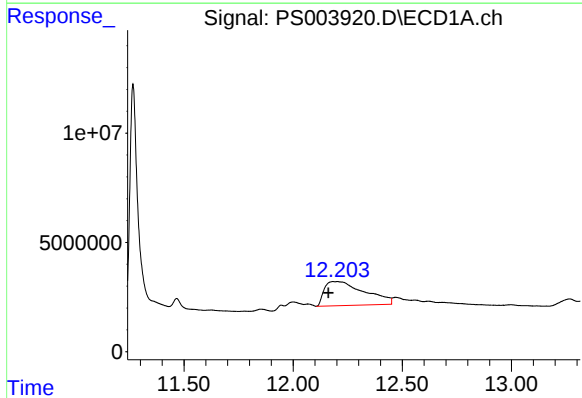


#7 MCPA

R.T.: 12.202 min
Delta R.T.: 0.040 min
Response: 142019691
Conc: 67.31 ug/ml

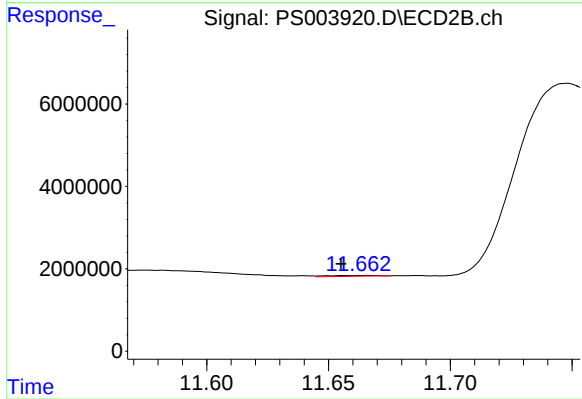

#7 MCPA


R.T.: 11.665 min
Delta R.T.: 0.010 min
Response: 292772
Conc: N.D.

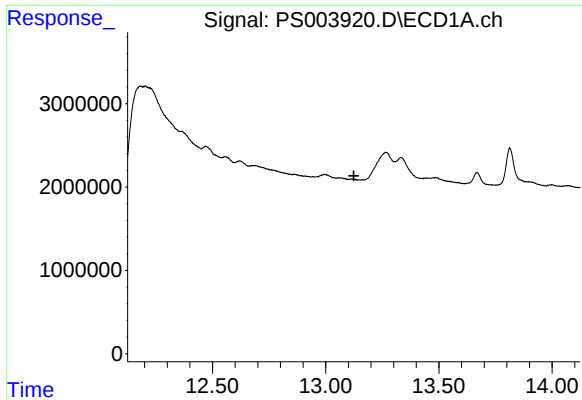

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

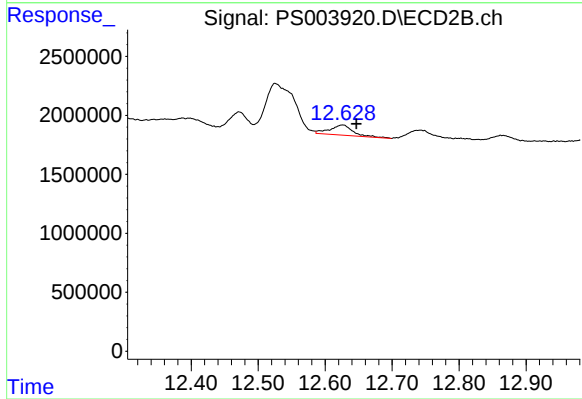


#9 2,4-D

R.T.: 12.626 min
Delta R.T.: -0.021 min
Response: 2046556
Conc: 3.85 ng/ml

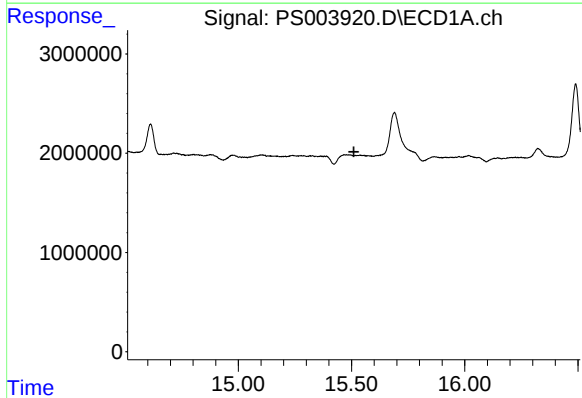


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

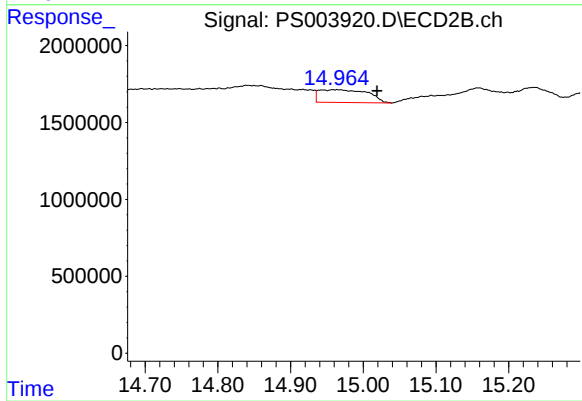

#13 2,4-DB


R.T.: 14.964 min
Delta R.T.: -0.055 min
Response: 3842418
Conc: 12.94 ng/ml

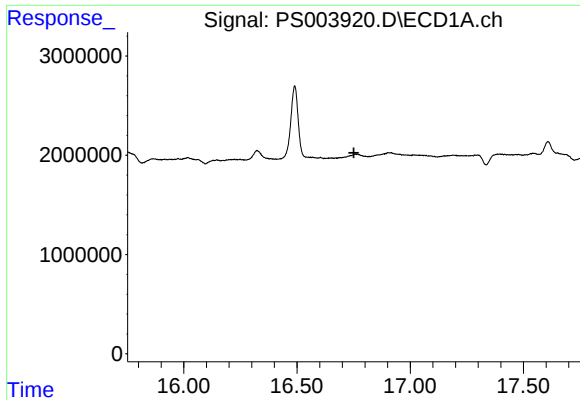

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

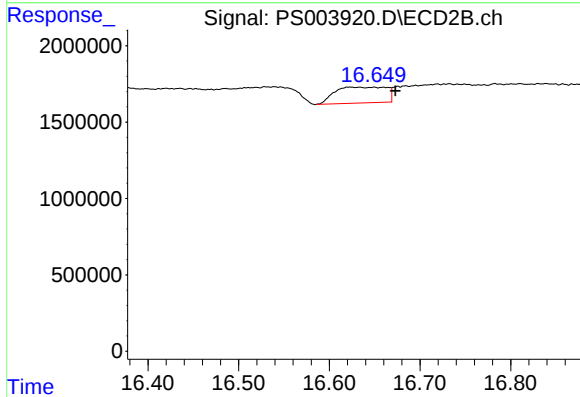


#15 Picloram

R.T.: 16.623 min
Delta R.T.: -0.050 min
Response: 4092890
Conc: 1.29 ng/ml

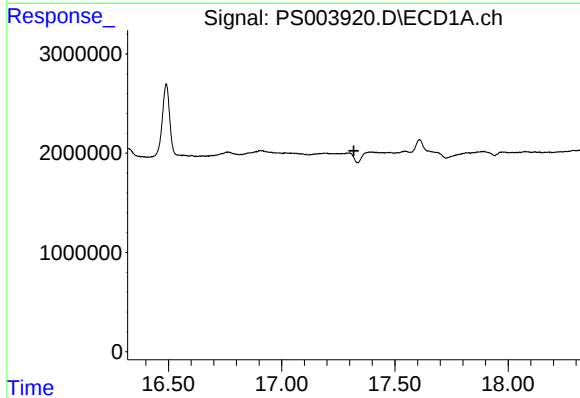

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

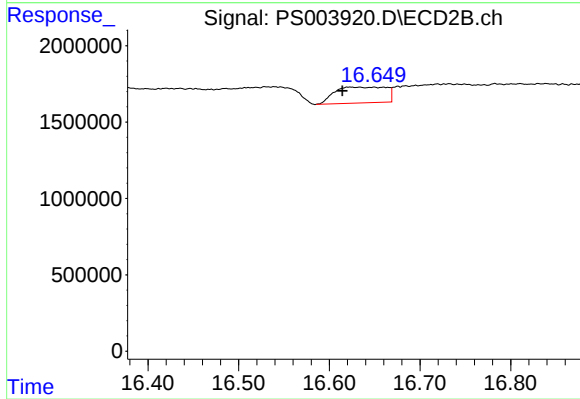

#16 DCPA

R.T.: 16.623 min
Delta R.T.: 0.008 min
Response: 4092890
Conc: 1.21 ng/ml