

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 01:11
 Operator : EI\SJ
 Sample : K2180-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:38:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.272	10.772	207.0E6	194.8E6	474.497	397.042
Target Compounds							
1) T	Dalapon	2.790	2.282	44626112	36800720	59.858	50.438
2) T	3,5-DICHL...	0.000	8.936	0	5287747	N.D.	8.290
3) T	4-Nitroph...	0.000	9.945	0	18686833	N.D.	82.308
5) T	DICAMBA	0.000	11.012	0	3395578	N.D.	1.826
6) T	MCPD	0.000	11.251	0	35130	N.D.	<MDL
7) T	MCPA	0.000	11.667	0	1304776	N.D.	<MDL
9) T	2,4-D	0.000	12.626	0	1321761	N.D.	2.485
11) T	2,4,5-TP ...	0.000	13.779	0	1166063	N.D.	<MDL
12) T	2,4,5-T	0.000	14.360	0	664317	N.D.	<MDL
14) T	DINOSEB	0.000	15.500	0	1820439	N.D.	<MDL
15) T	Picloram	0.000	16.640	0	2580838	N.D.	<MDL
16) T	DCPA	0.000	16.640	0	2580838	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 01:11
Operator : EI\SJ
Sample : K2180-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

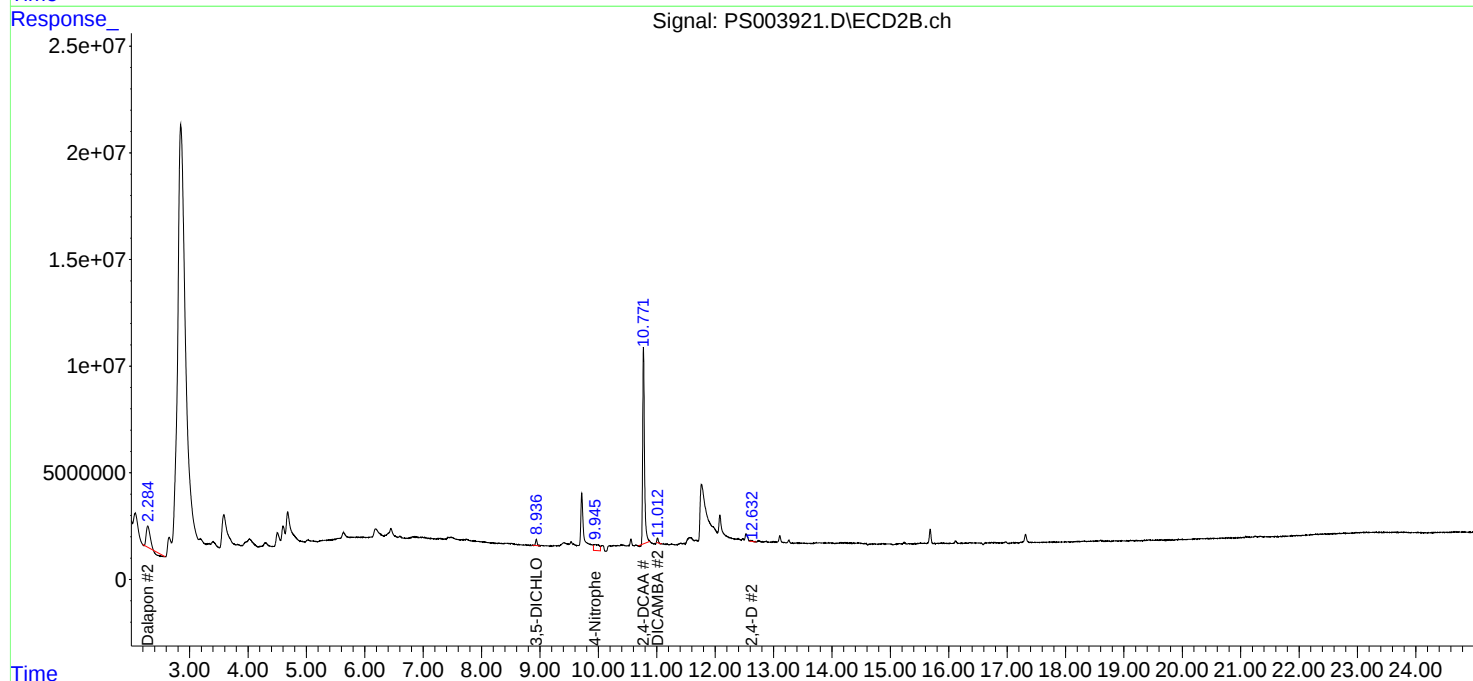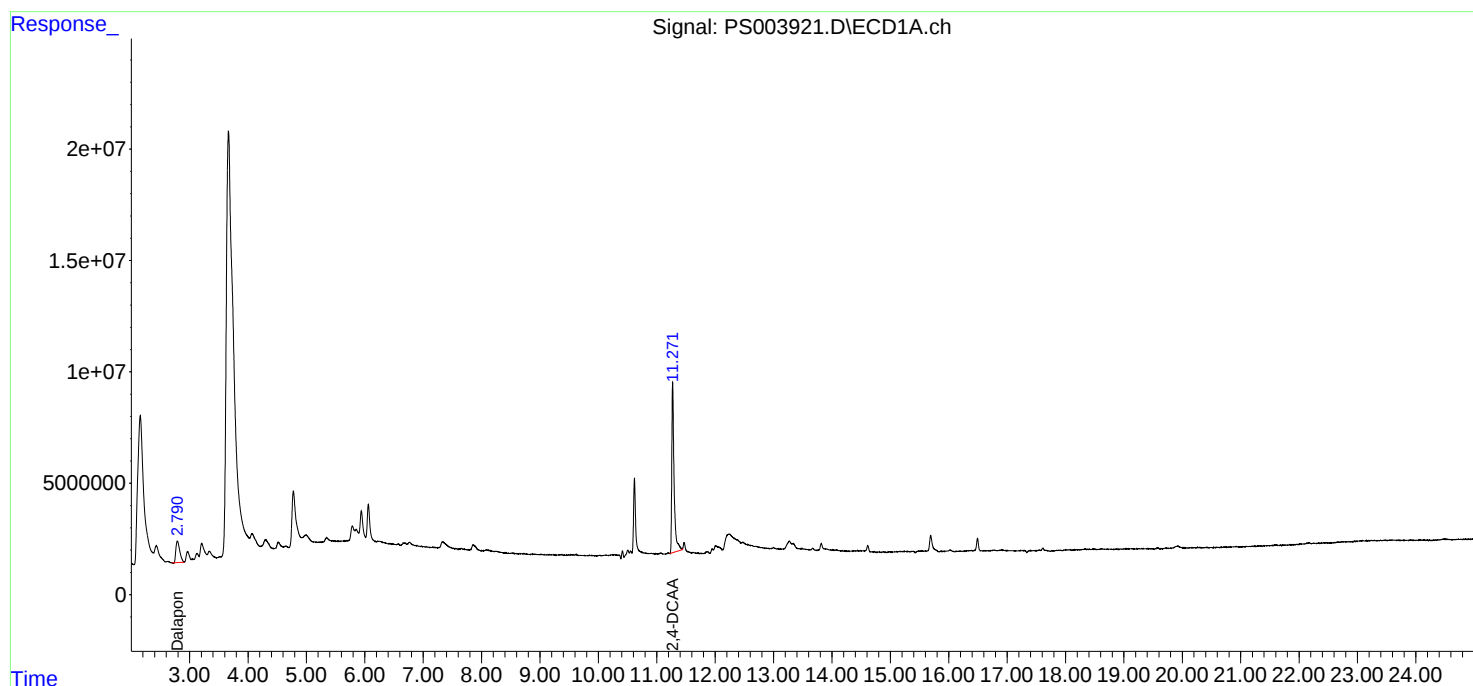


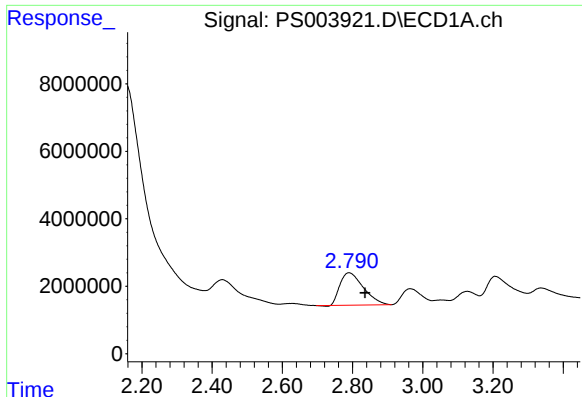

#1 Dalapon


R.T.: 2.790 min
Delta R.T.: -0.045 min
Response: 44626112
Conc: 59.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6S

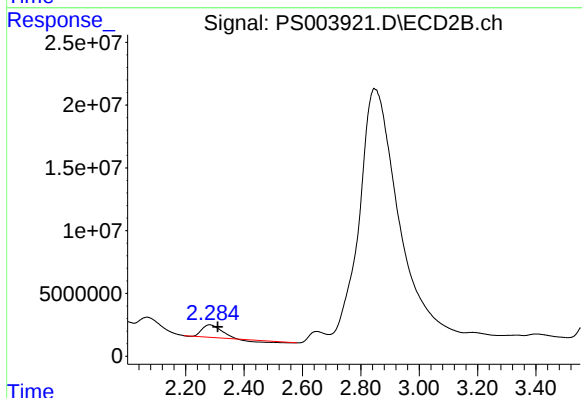


#1 Dalapon

R.T.: 2.282 min
Delta R.T.: -0.029 min
Response: 36800720
Conc: 50.44 ng/ml

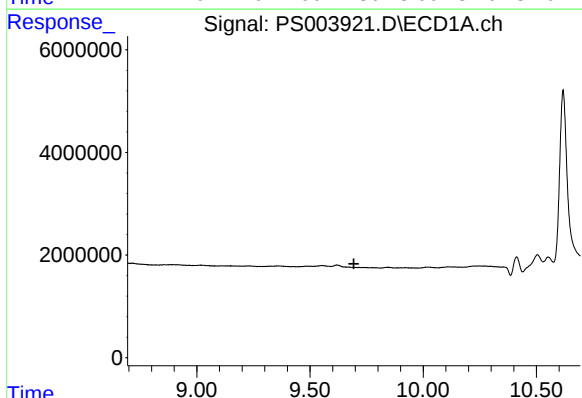


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

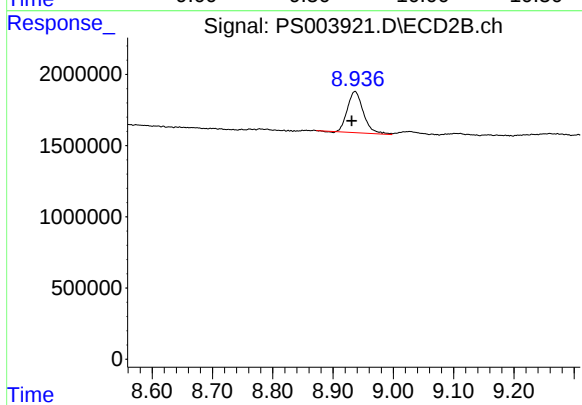

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.936 min
Delta R.T.: 0.005 min
Response: 5287747
Conc: 8.29 ng/ml

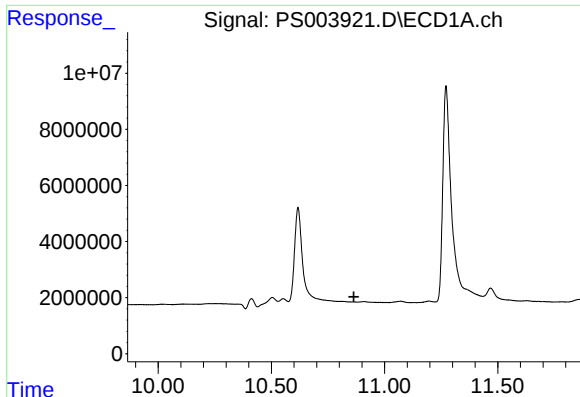

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

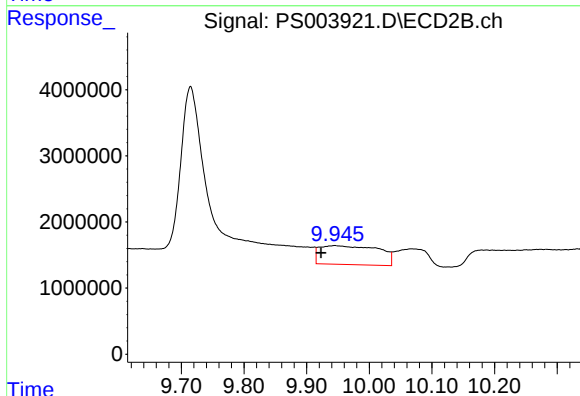


#3 4-Nitrophenol

R.T.: 9.945 min
Delta R.T.: 0.022 min
Response: 18686833
Conc: 82.31 ng/ml

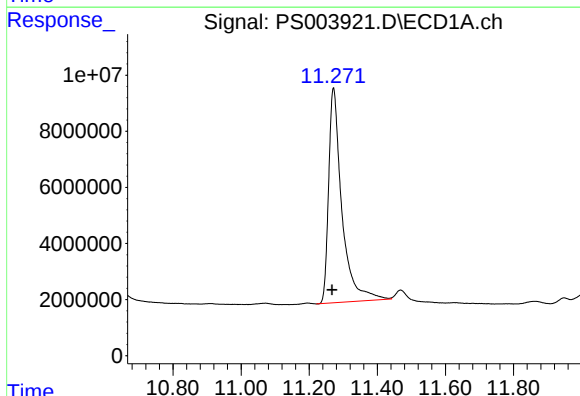


#4 2,4-DCAA

R.T.: 11.272 min
Delta R.T.: 0.005 min
Response: 206981561
Conc: 474.50 ng/ml

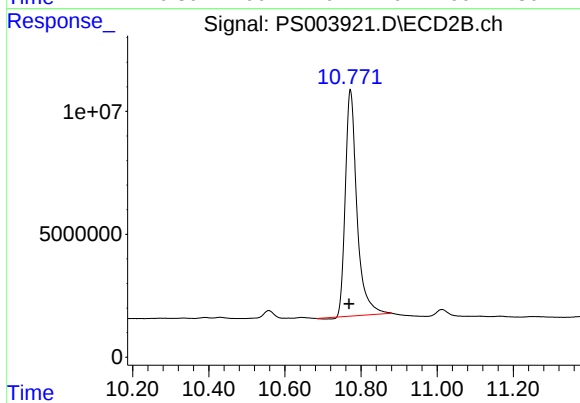

#4 2,4-DCAA


R.T.: 10.772 min
Delta R.T.: 0.003 min
Response: 194811887
Conc: 397.04 ng/ml

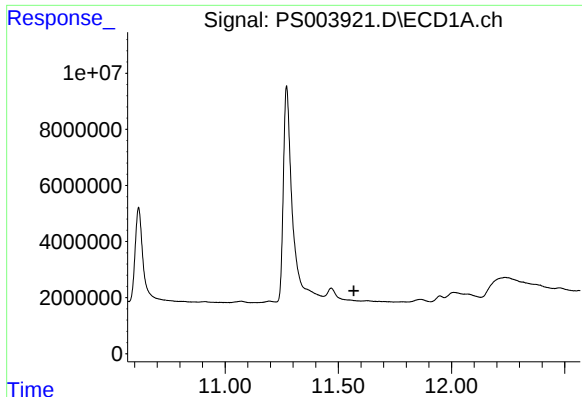

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

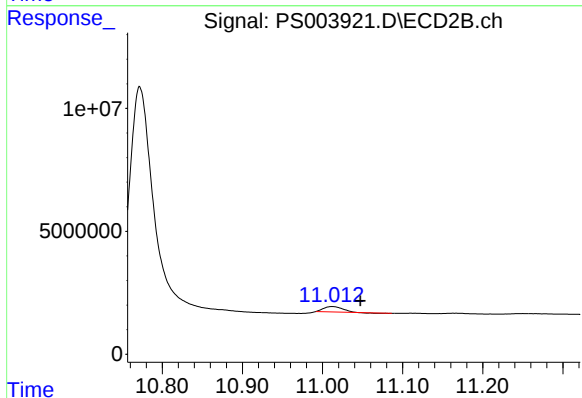


#5 DICAMBA

R.T.: 11.012 min
Delta R.T.: -0.035 min
Response: 3395578
Conc: 1.83 ng/ml

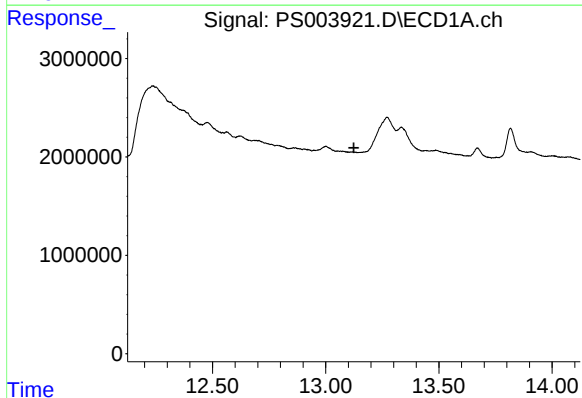

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

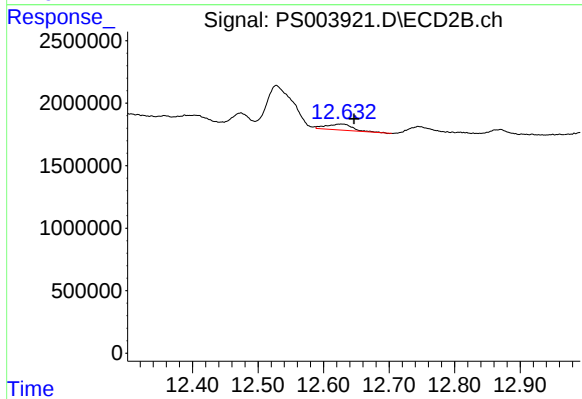

#9 2,4-D

R.T.: 12.626 min
Delta R.T.: -0.020 min
Response: 1321761
Conc: 2.48 ng/ml