

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 01:42
 Operator : EI\SJ
 Sample : K2180-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:39:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.265	10.766	266.9E6	254.6E6	611.815	518.838
Target Compounds							
1) T	Dalapon	2.785	2.279	25140034	36567869	33.721	50.118 #
2) T	3,5-DICHL...	0.000	8.932	0	6512729	N.D.	10.210
3) T	4-Nitroph...	0.000	9.941	0	20643024	N.D.	90.925
5) T	DICAMBA	0.000	11.007	0	1871113	N.D.	1.006
7) T	MCPA	12.211	11.677	116.3E6	1055069	55.121	<MDL #
9) T	2,4-D	0.000	12.624	0	1896387	N.D.	3.565
10) T	Pentachlo...	0.000	13.163	0	428306	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.772	0	1180383	N.D.	<MDL
12) T	2,4,5-T	0.000	14.350	0	793357	N.D.	<MDL
13) T	2,4-DB	0.000	14.962	0	4060499	N.D.	13.674
14) T	DINOSEB	0.000	15.489	0	3670256	N.D.	1.913
15) T	Picloram	0.000	16.628	0	5731905	N.D.	1.807
16) T	DCPA	0.000	16.628	0	5731905	N.D.	1.696



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 01:42
Operator : EI\SJ
Sample : K2180-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:39:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

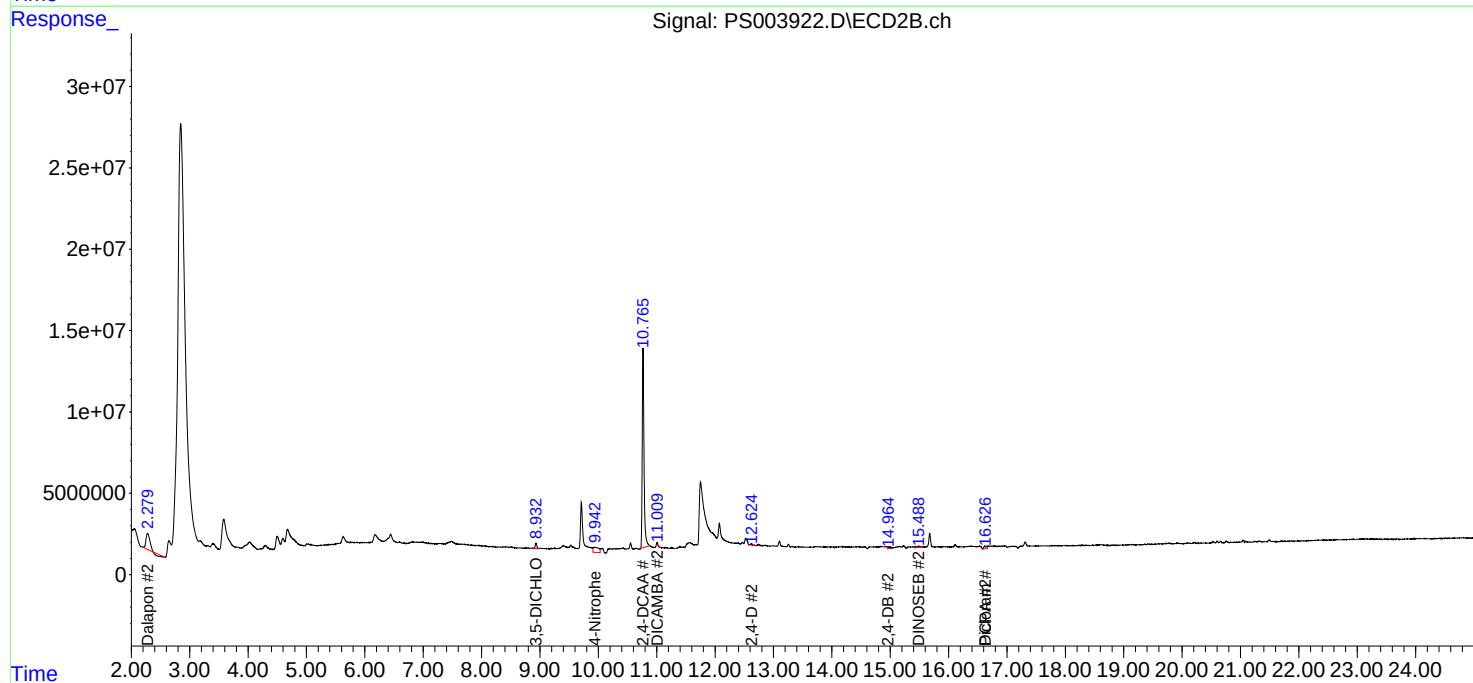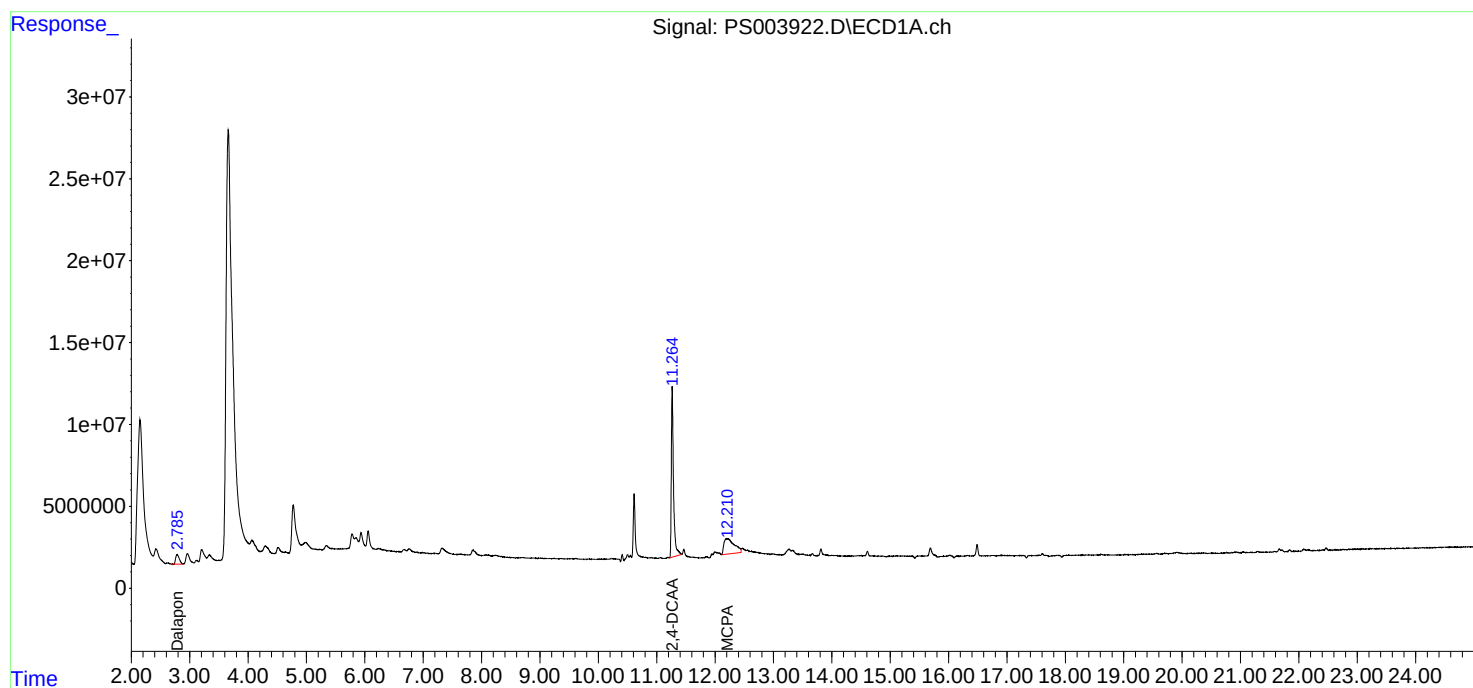


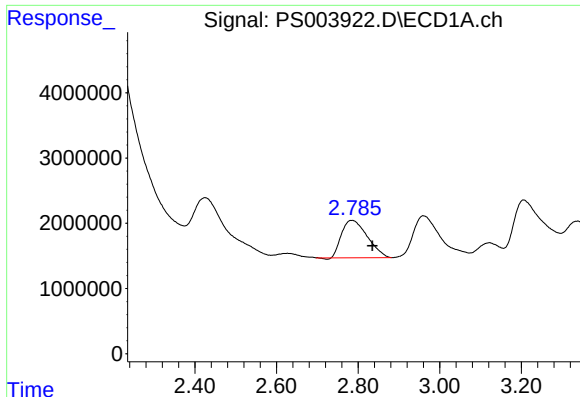

#1 Dalapon


R.T.: 2.785 min
Delta R.T.: -0.050 min
Response: 25140034
Conc: 33.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6D

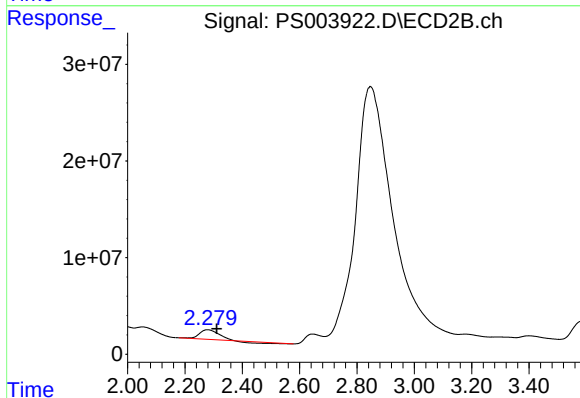


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.031 min
Response: 36567869
Conc: 50.12 ng/ml

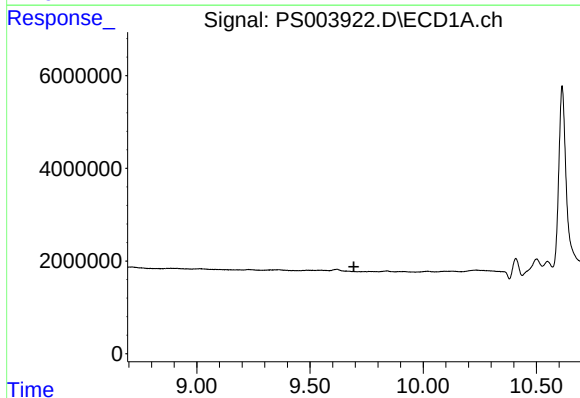


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

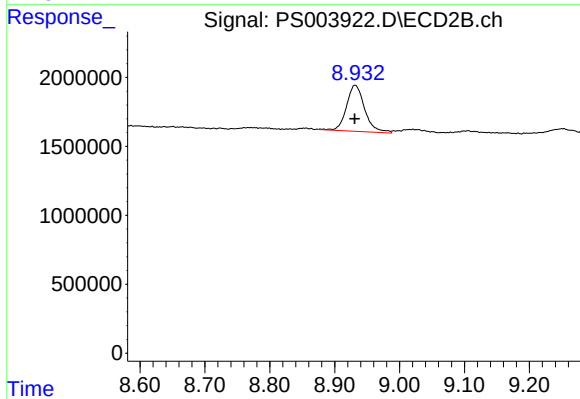

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.932 min
Delta R.T.: 0.000 min
Response: 6512729
Conc: 10.21 ng/ml

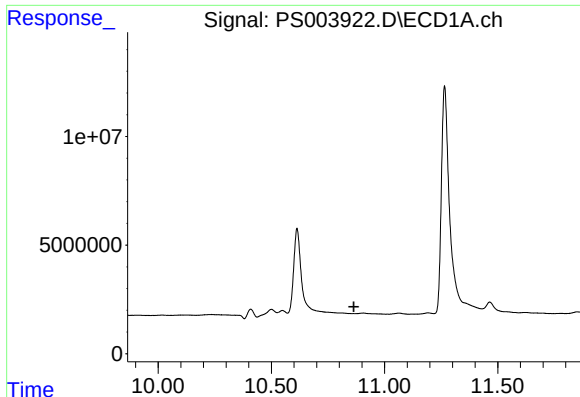

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6D

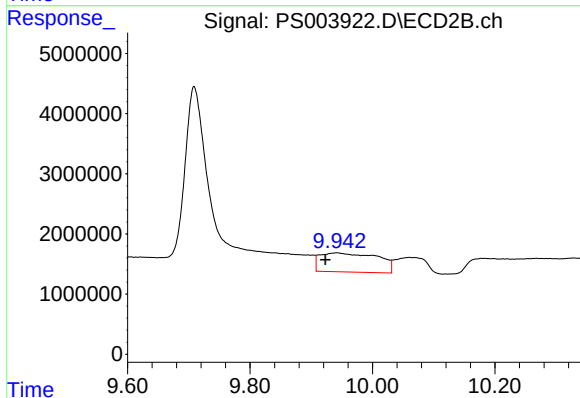


#3 4-Nitrophenol

R.T.: 9.941 min
Delta R.T.: 0.018 min
Response: 20643024
Conc: 90.92 ng/ml

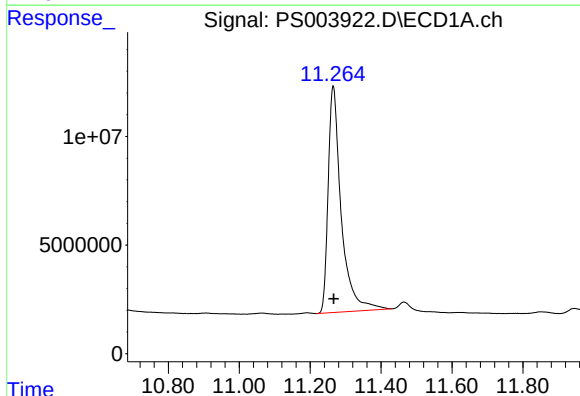


#4 2,4-DCAA

R.T.: 11.265 min
Delta R.T.: -0.002 min
Response: 266881376
Conc: 611.82 ng/ml

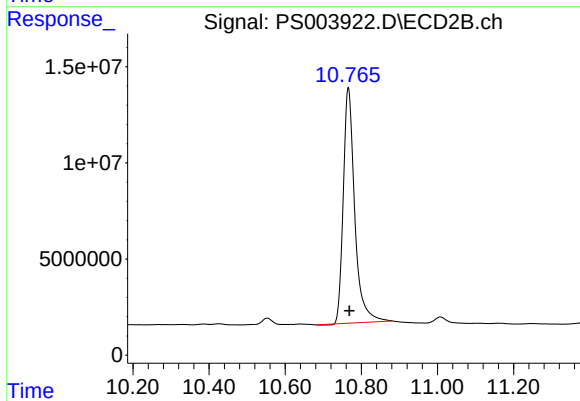

#4 2,4-DCAA


R.T.: 10.766 min
Delta R.T.: -0.003 min
Response: 254572412
Conc: 518.84 ng/ml

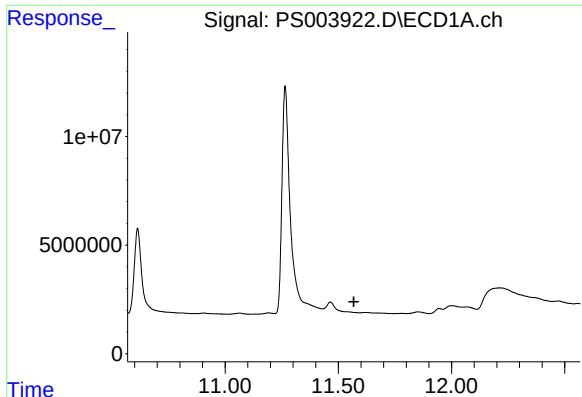

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6D

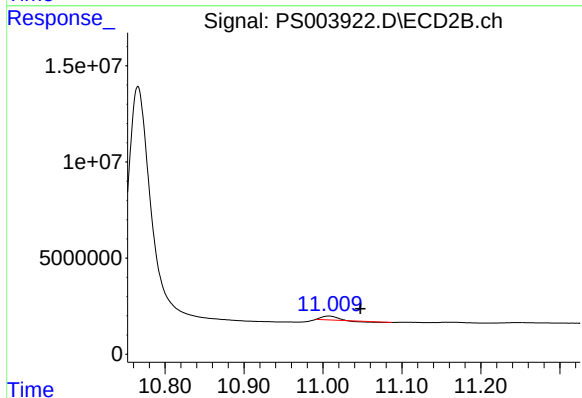


#5 DICAMBA

R.T.: 11.007 min
Delta R.T.: -0.040 min
Response: 1871113
Conc: 1.01 ng/ml

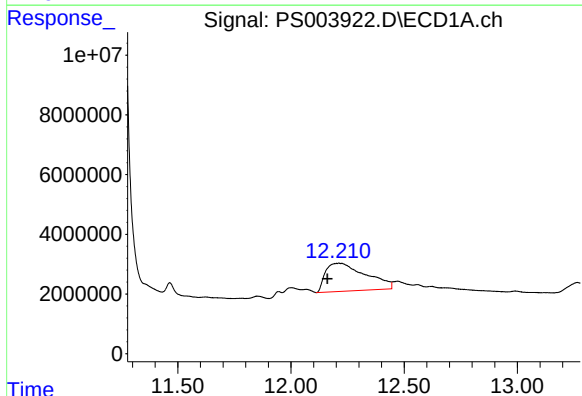


#7 MCPA

R.T.: 12.211 min
Delta R.T.: 0.050 min
Response: 116293096
Conc: 55.12 ug/ml

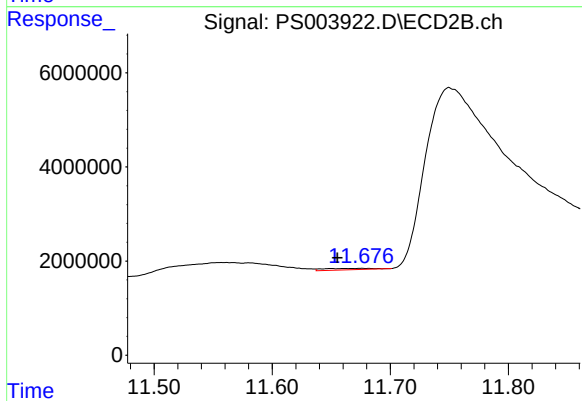

#7 MCPA


R.T.: 11.677 min
Delta R.T.: 0.022 min
Response: 1055069
Conc: N.D.

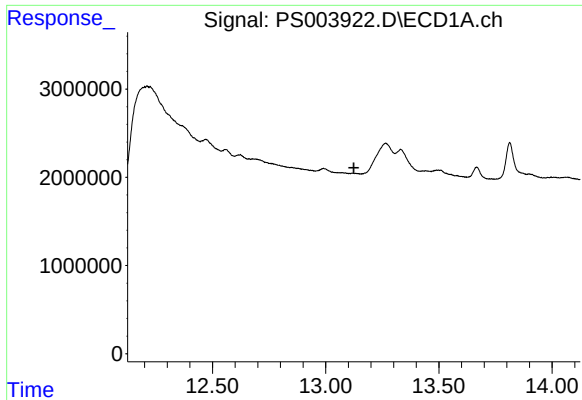

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6D

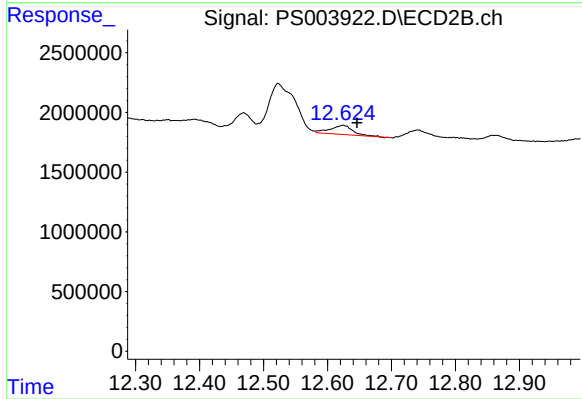


#9 2,4-D

R.T.: 12.624 min
Delta R.T.: -0.022 min
Response: 1896387
Conc: 3.57 ng/ml

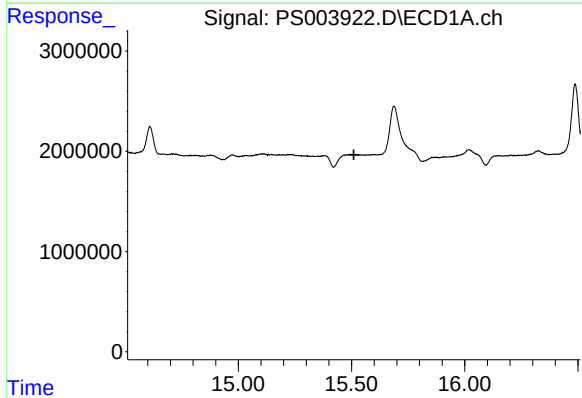


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

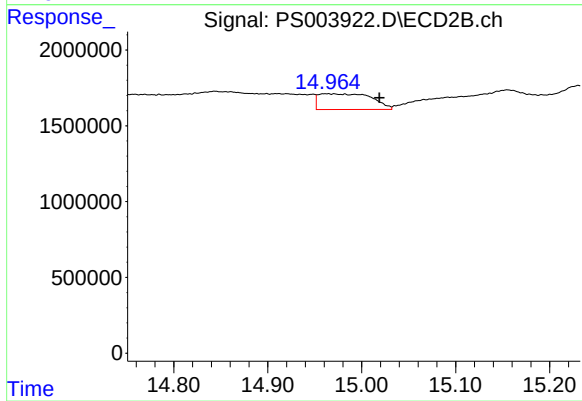

#13 2,4-DB


R.T.: 14.962 min
Delta R.T.: -0.057 min
Response: 4060499
Conc: 13.67 ng/ml

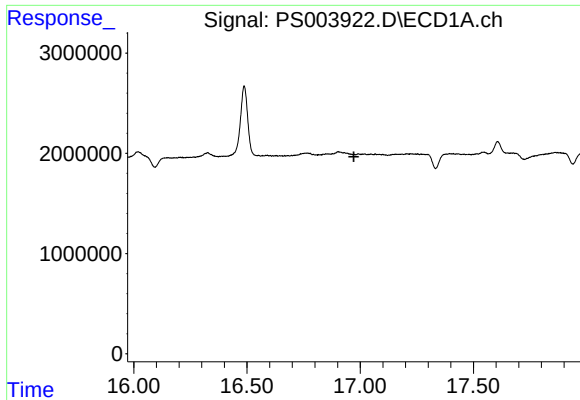

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6D

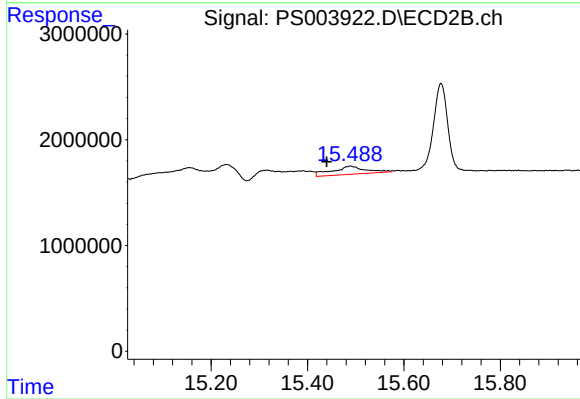


#14 DINOSEB

R.T.: 15.489 min
Delta R.T.: 0.049 min
Response: 3670256
Conc: 1.91 ng/ml

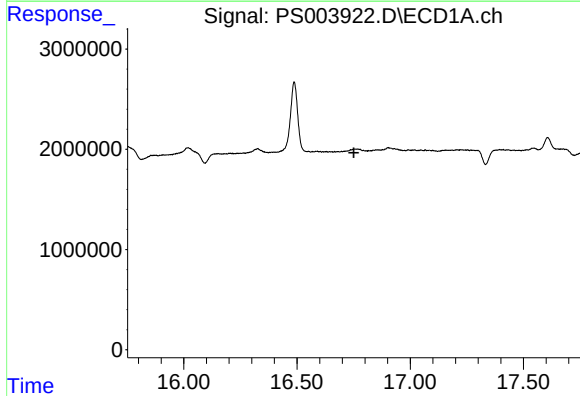


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

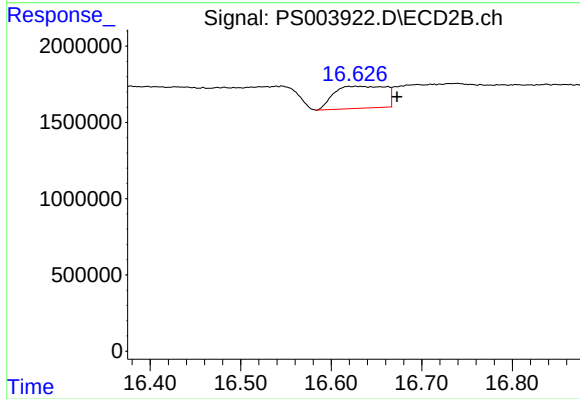

#15 Picloram


R.T.: 16.628 min
Delta R.T.: -0.044 min
Response: 5731905
Conc: 1.81 ng/ml

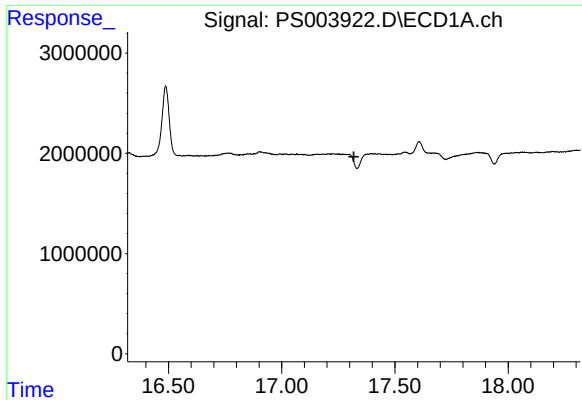

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6D

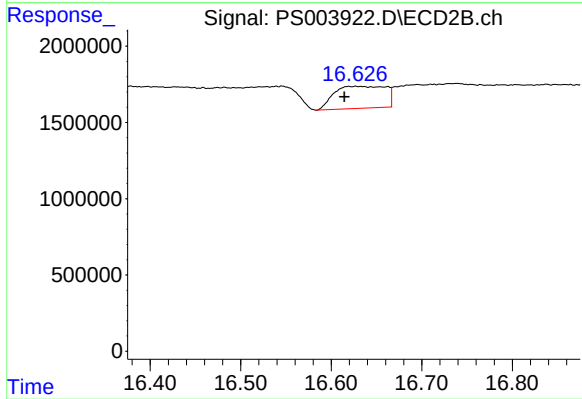

#16 DCPA

R.T.: 16.628 min
Delta R.T.: 0.014 min
Response: 5731905
Conc: 1.70 ng/ml