

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 02:13
 Operator : EI\SJ
 Sample : K2180-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:39:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.767	226.3E6	215.0E6	518.716	438.095
Target Compounds							
1) T	Dalapon	2.788	2.281	28594321	32973438	38.354	45.192
2) T	3,5-DICHL...	0.000	8.932	0	6121803	N.D.	9.597
3) T	4-Nitroph...	0.000	9.943	0	19218567	N.D.	84.650
5) T	DICAMBA	0.000	11.008	0	2861128	N.D.	1.538
6) T	MCPD	0.000	11.245	0	216740	N.D.	<MDL
7) T	MCPA	12.179	11.649	35638231	966246	16.892	<MDL #
9) T	2,4-D	0.000	12.625	0	1467008	N.D.	2.758
10) T	Pentachlo...	0.000	13.170	0	169980	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.771	0	1714994	N.D.	<MDL
12) T	2,4,5-T	0.000	14.365	0	620344	N.D.	<MDL
13) T	2,4-DB	0.000	14.988	0	3403308	N.D.	11.461
14) T	DINOSEB	0.000	15.382	0	1321565	N.D.	<MDL
15) T	Picloram	0.000	16.695	0	12553145	N.D.	3.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 02:13
Operator : EI\SJ
Sample : K2180-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:39:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

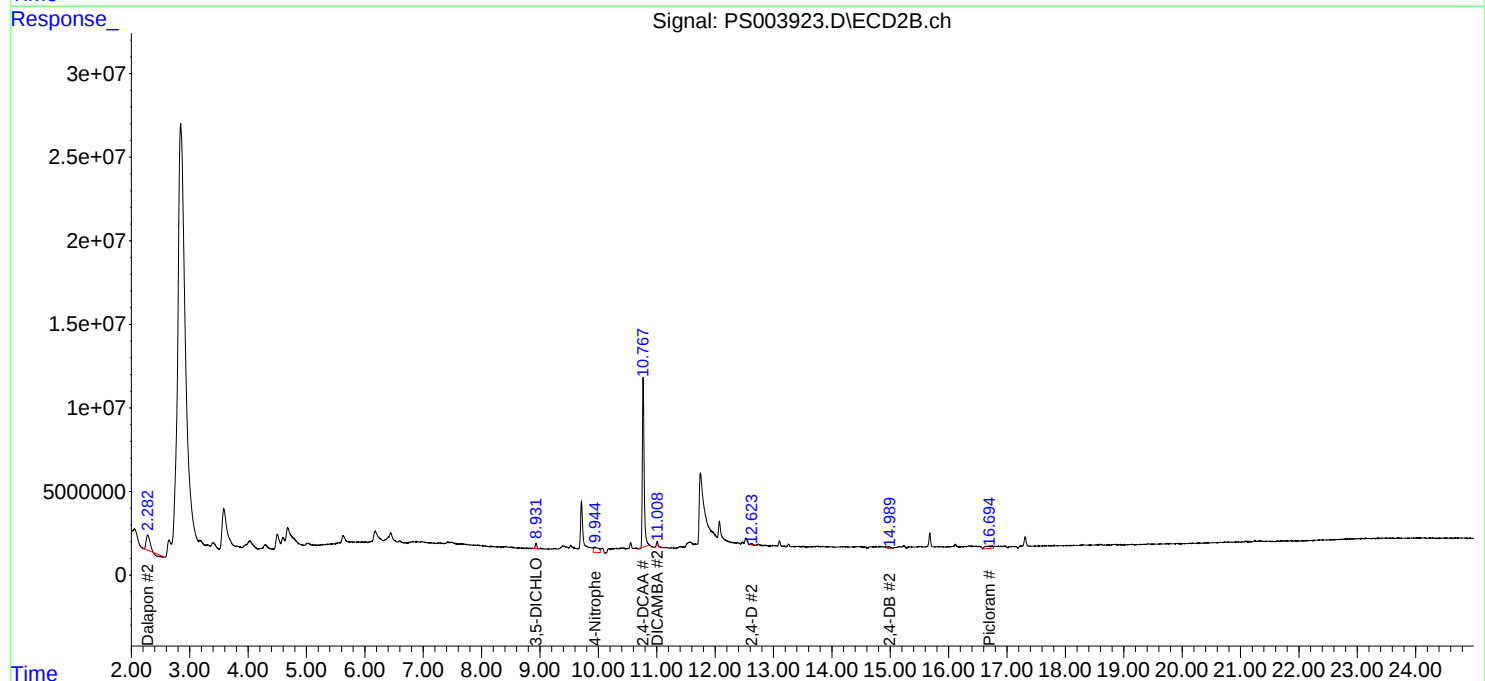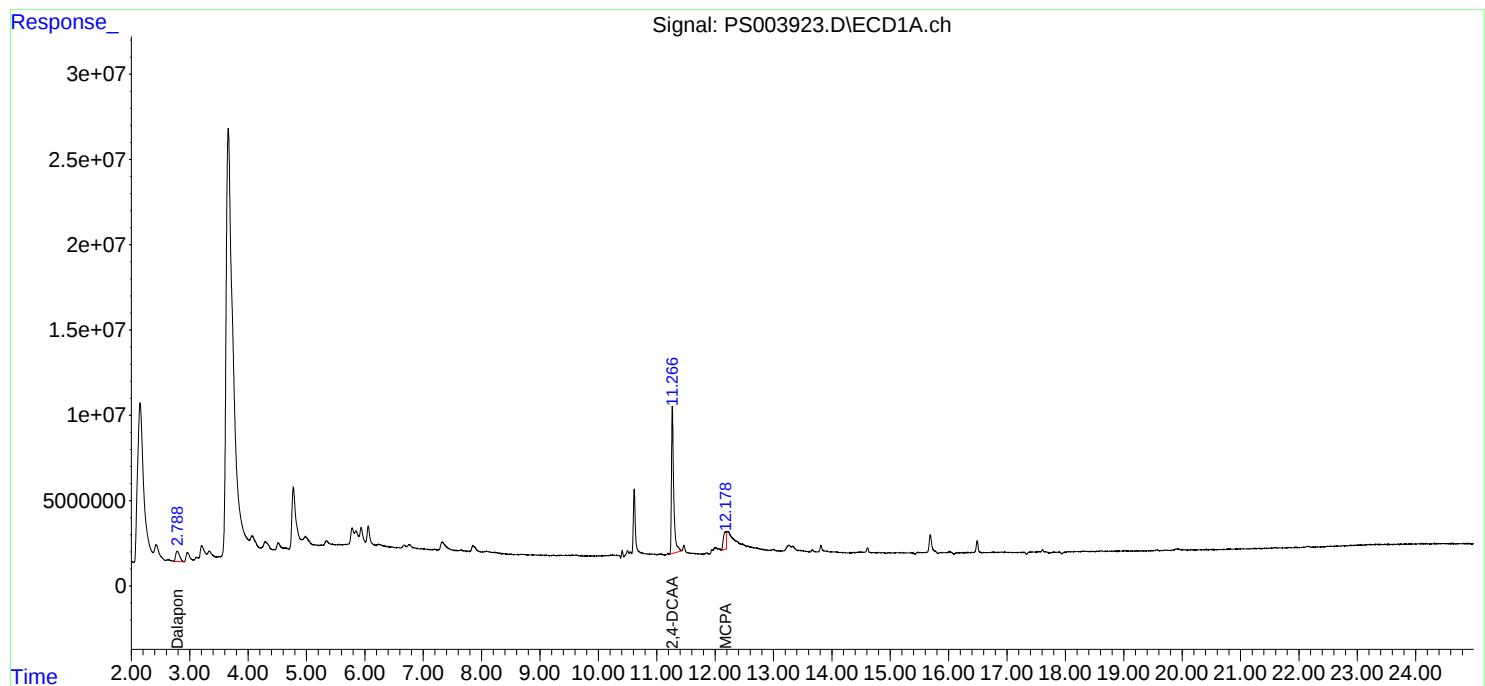


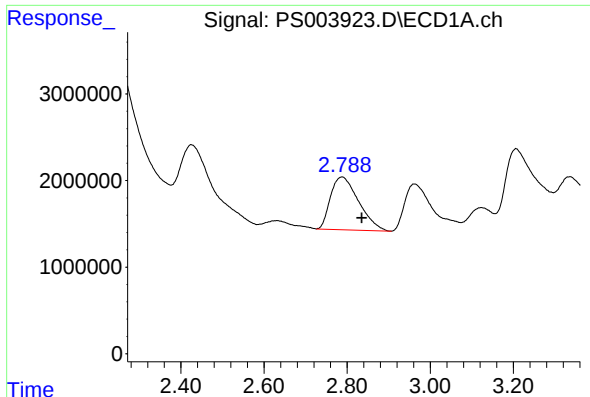

#1 Dalapon


R.T.: 2.788 min
Delta R.T.: -0.047 min
Response: 28594321
Conc: 38.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-9

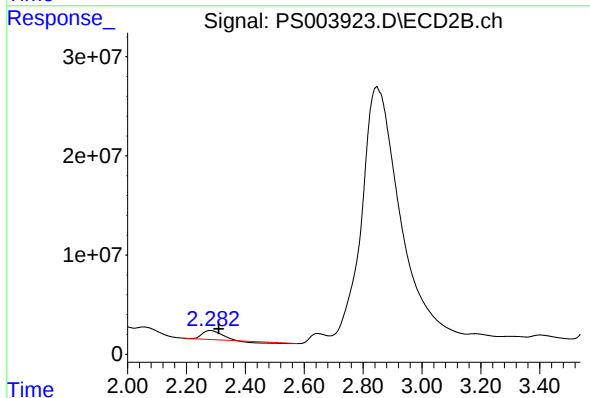


#1 Dalapon

R.T.: 2.281 min
Delta R.T.: -0.030 min
Response: 32973438
Conc: 45.19 ng/ml

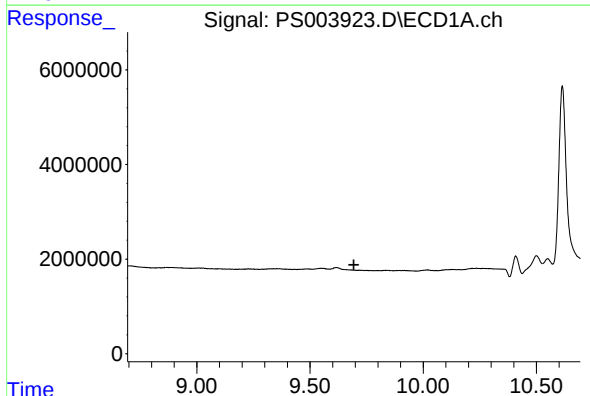


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

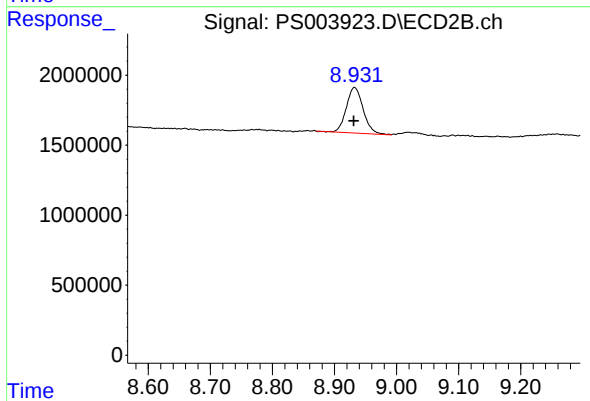

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.932 min
Delta R.T.: 0.001 min
Response: 6121803
Conc: 9.60 ng/ml

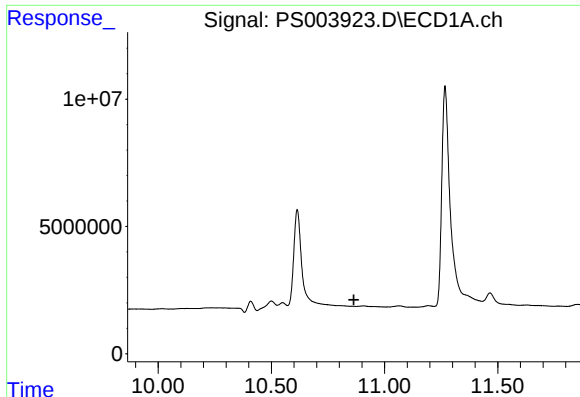

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

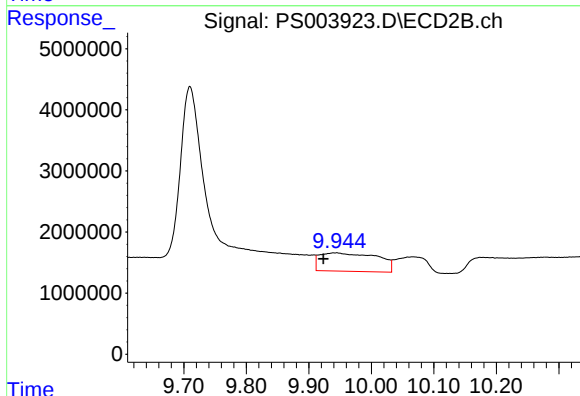


#3 4-Nitrophenol

R.T.: 9.943 min
Delta R.T.: 0.020 min
Response: 19218567
Conc: 84.65 ng/ml

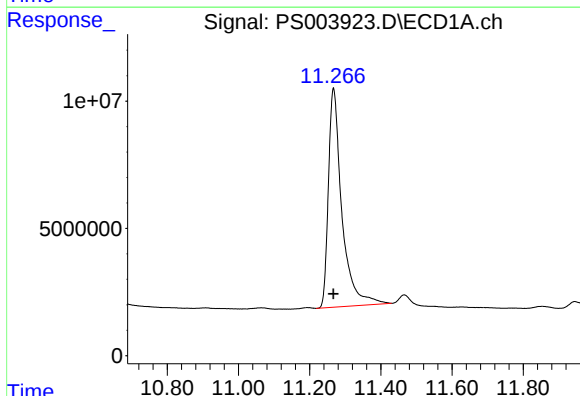


#4 2,4-DCAA

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 226270380
Conc: 518.72 ng/ml

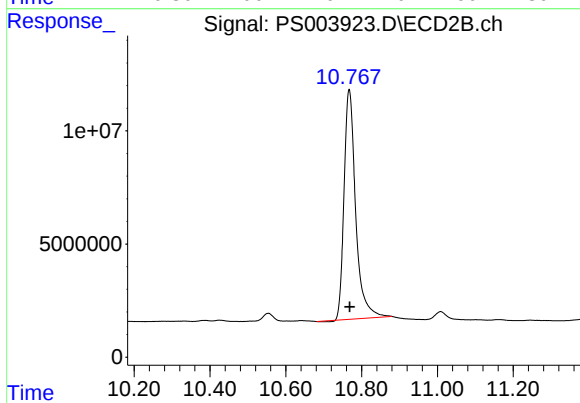

#4 2,4-DCAA


R.T.: 10.767 min
Delta R.T.: -0.002 min
Response: 214954828
Conc: 438.09 ng/ml

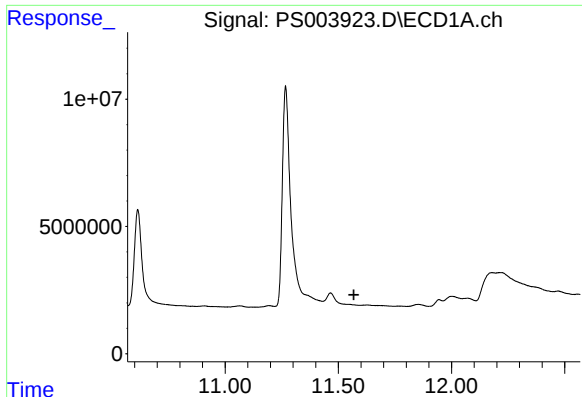

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

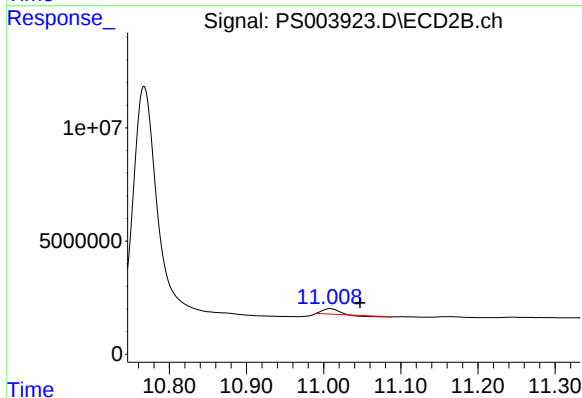


#5 DICAMBA

R.T.: 11.008 min
Delta R.T.: -0.039 min
Response: 2861128
Conc: 1.54 ng/ml

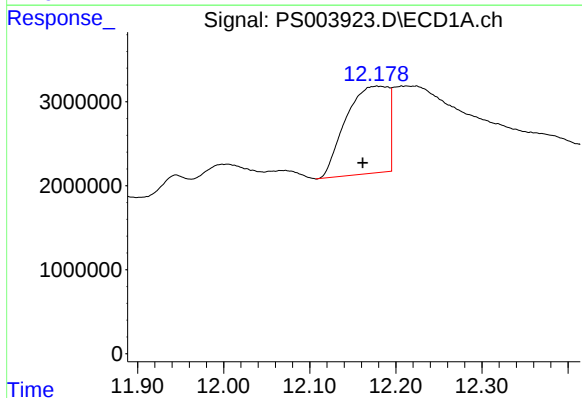


#7 MCPA

R.T.: 12.179 min
Delta R.T.: 0.017 min
Response: 35638231
Conc: 16.89 ug/ml

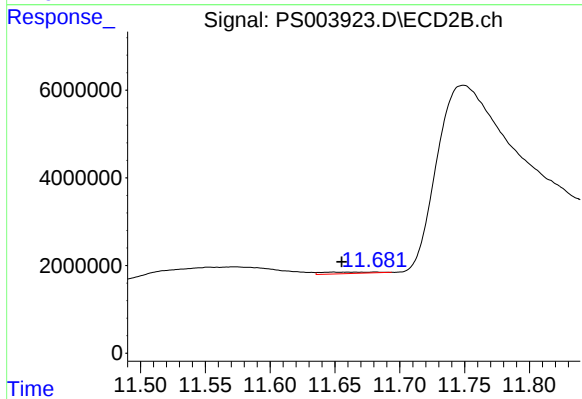

#7 MCPA


R.T.: 11.649 min
Delta R.T.: -0.006 min
Response: 966246
Conc: N.D.

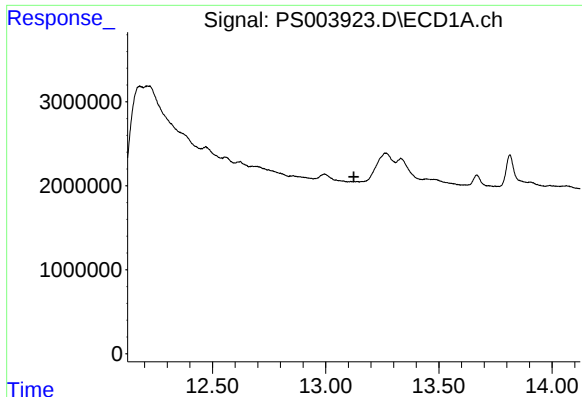

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

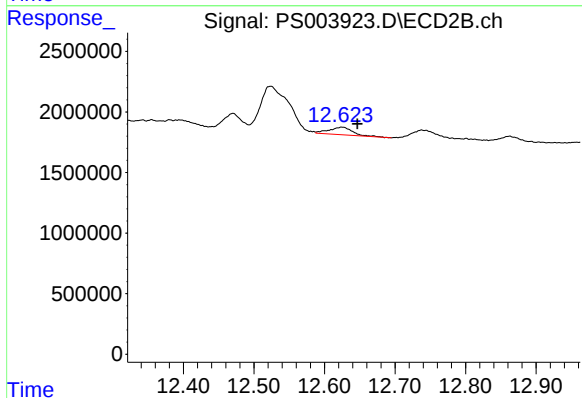


#9 2,4-D

R.T.: 12.625 min
Delta R.T.: -0.021 min
Response: 1467008
Conc: 2.76 ng/ml

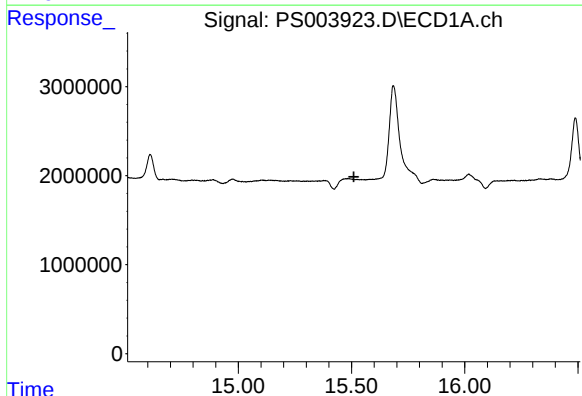


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

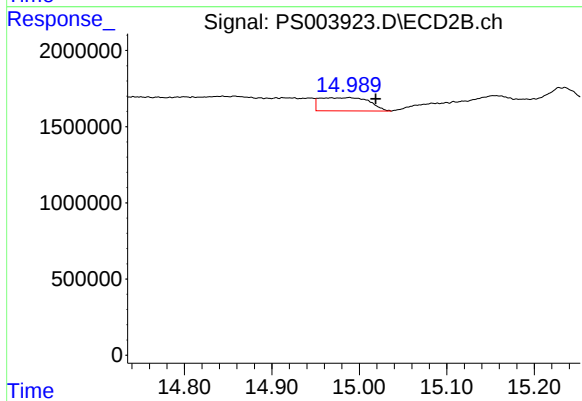

#13 2,4-DB


R.T.: 14.988 min
Delta R.T.: -0.031 min
Response: 3403308
Conc: 11.46 ng/ml

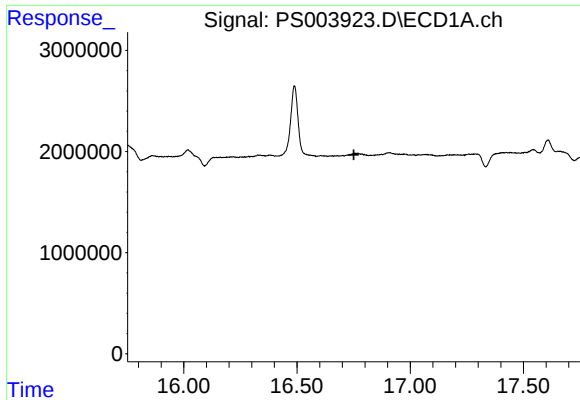

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

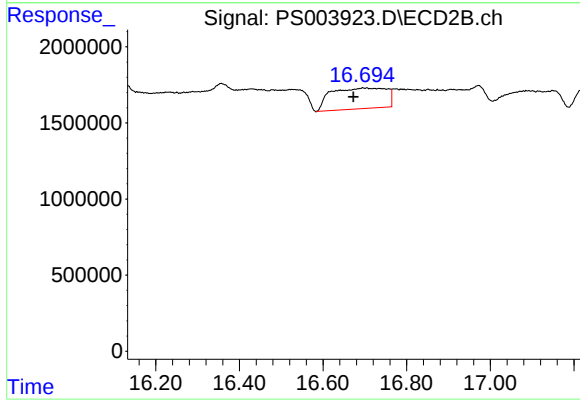

#15 Picloram

R.T.: 16.695 min
Delta R.T.: 0.023 min
Response: 12553145
Conc: 3.96 ng/ml