

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 03:47
 Operator : EI\SJ
 Sample : K2180-28
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 05:44:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.286	10.786	196.3E6	180.8E6	449.923	368.401
Target Compounds							
1) T	Dalapon	2.806	2.300	25898114	32529360	34.738	44.583 #
2) T	3,5-DICHL...	0.000	8.950	0	5291237	N.D.	8.295
3) T	4-Nitroph...	0.000	9.958	0	13978684	N.D.	61.571
5) T	DICAMBA	0.000	11.026	0	6196023	N.D.	3.332
7) T	MCPA	12.185	11.680	161.2E6	736625	76.395	<MDL #
9) T	2,4-D	0.000	12.641	0	1082287	N.D.	2.035
10) T	Pentachlo...	0.000	13.120	0	5903252	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.794	0	1899545	N.D.	<MDL
13) T	2,4-DB	0.000	14.955	0	2477838	N.D.	8.344
14) T	DINOSEB	0.000	15.401	0	1593305	N.D.	<MDL
15) T	Picloram	0.000	16.707	0	7980055	N.D.	2.516
16) T	DCPA	0.000	16.550	0	7410248	N.D.	2.192



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 03:47
Operator : EI\SJ
Sample : K2180-28
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 05:44:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

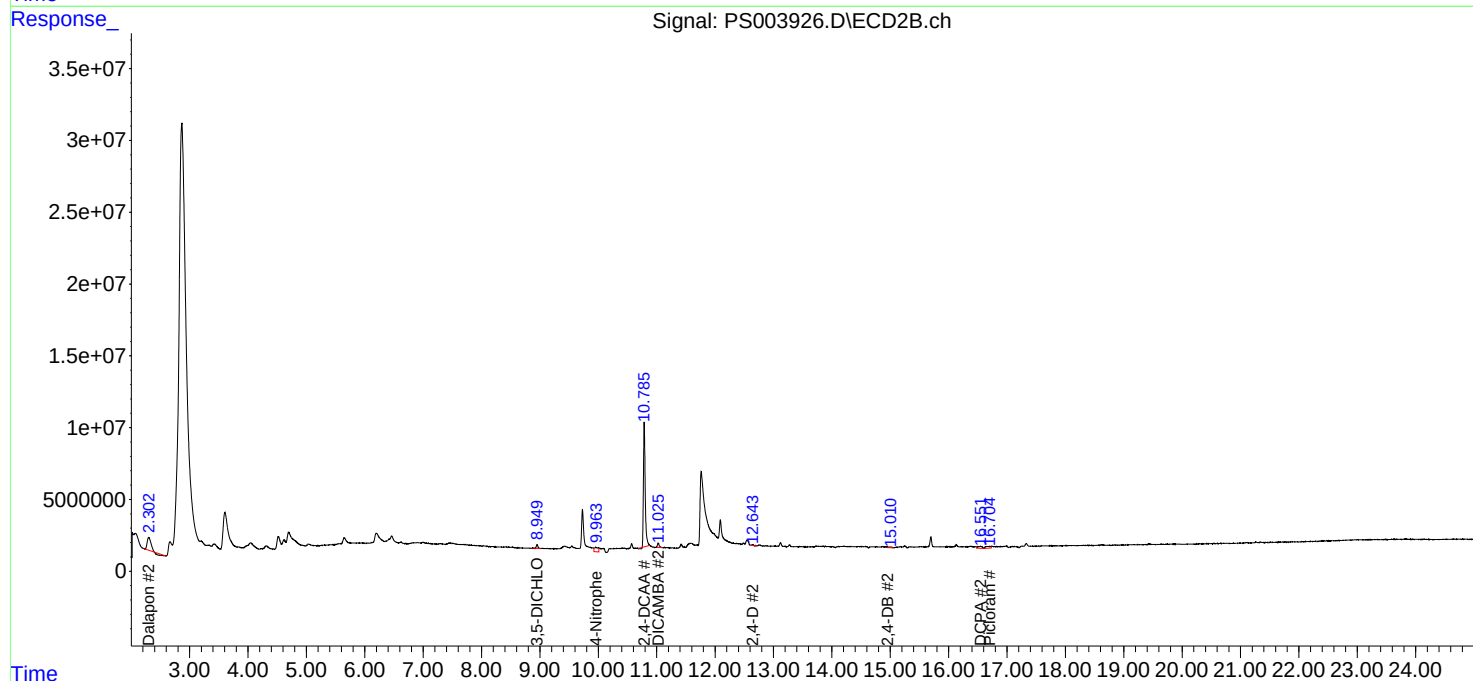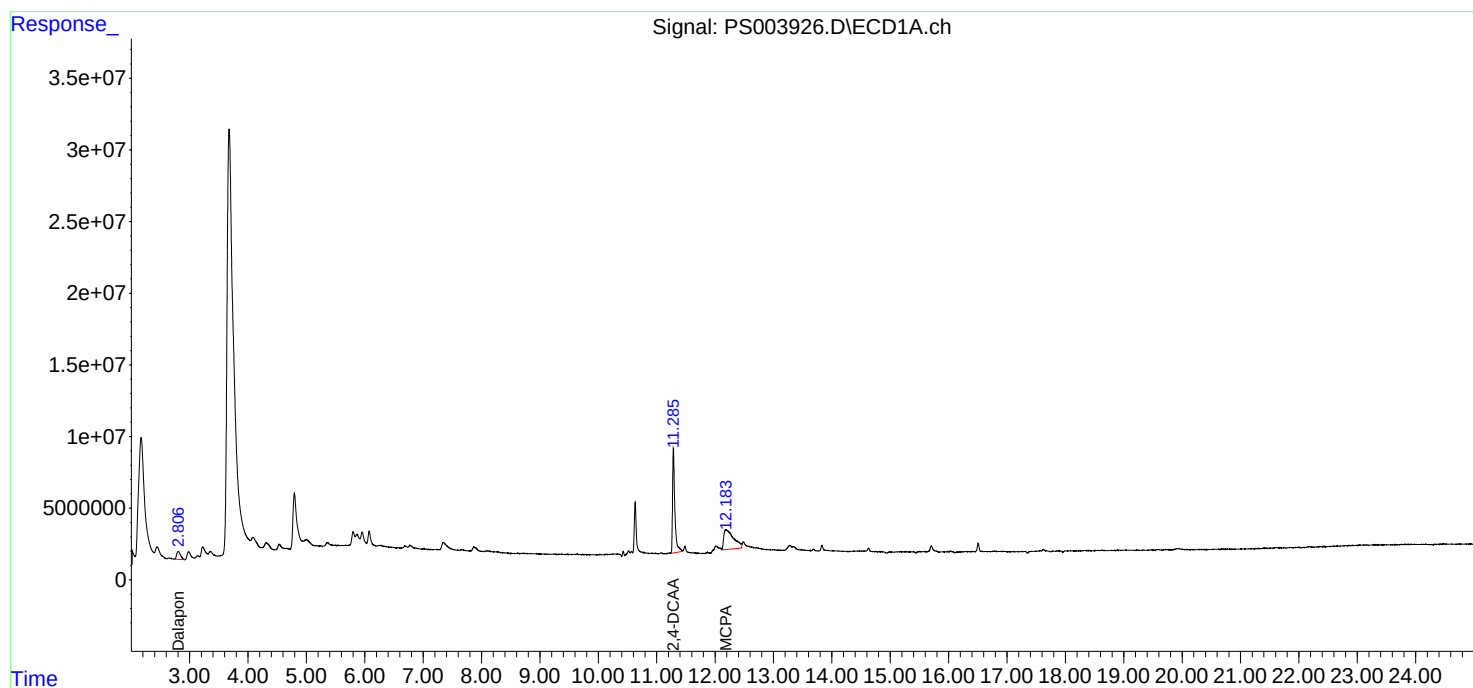


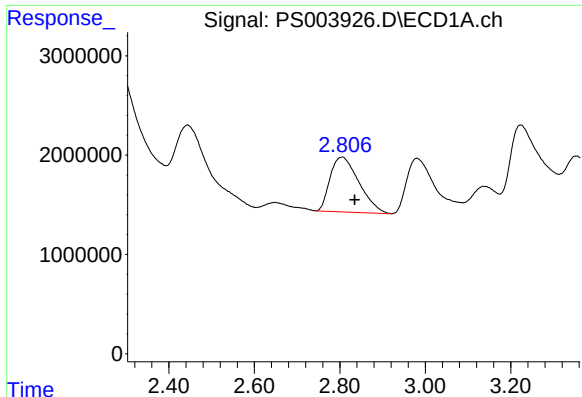

#1 Dalapon


R.T.: 2.806 min
Delta R.T.: -0.029 min
Response: 25898114
Conc: 34.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

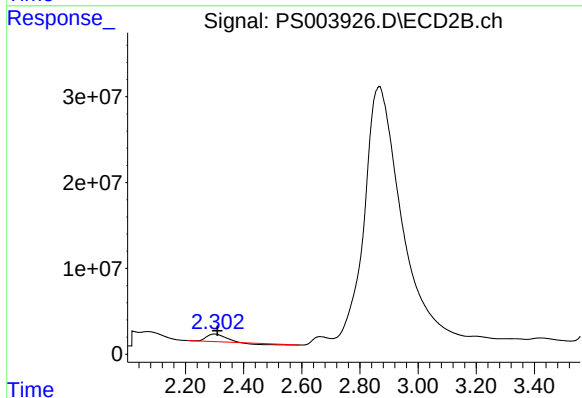


#1 Dalapon

R.T.: 2.300 min
Delta R.T.: -0.011 min
Response: 32529360
Conc: 44.58 ng/ml

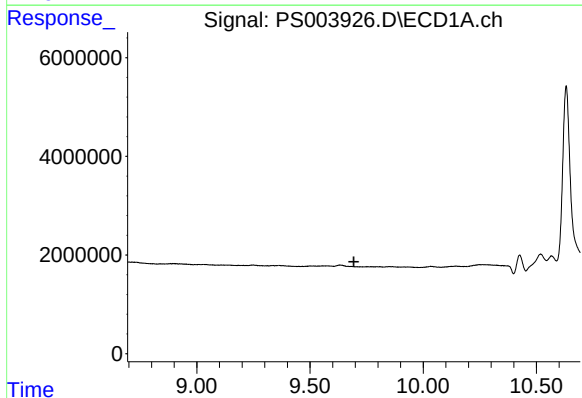


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

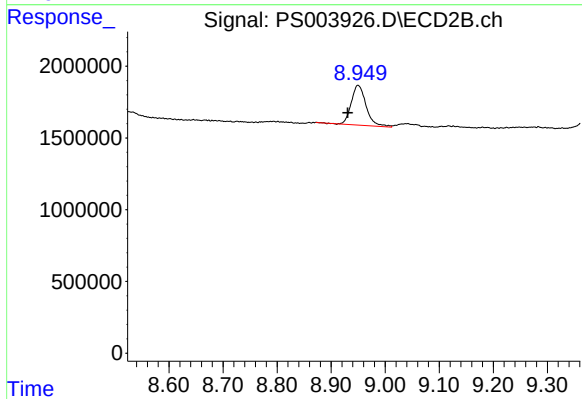

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.950 min
Delta R.T.: 0.019 min
Response: 5291237
Conc: 8.30 ng/ml

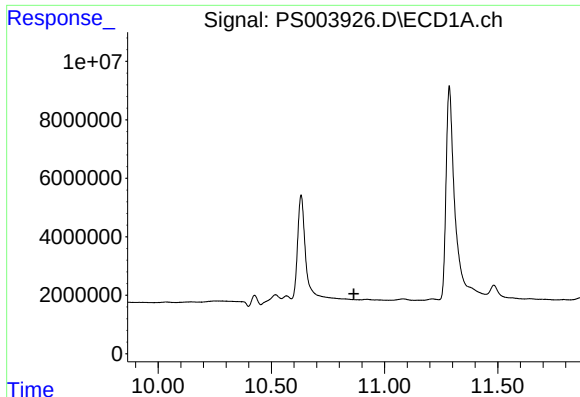

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

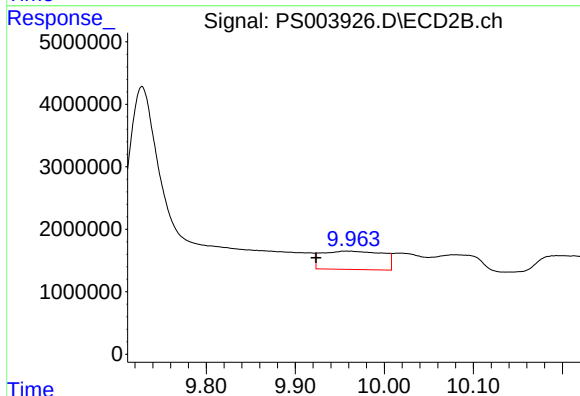


#3 4-Nitrophenol

R.T.: 9.958 min
Delta R.T.: 0.035 min
Response: 13978684
Conc: 61.57 ng/ml

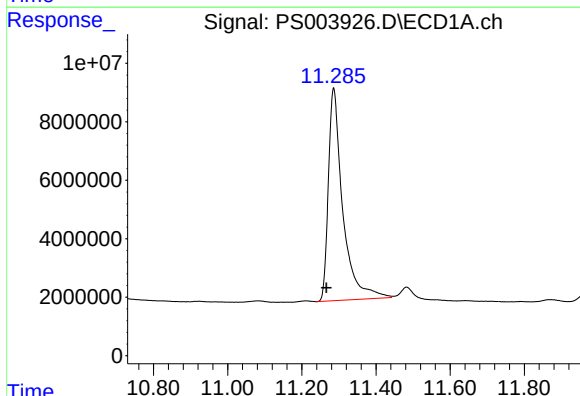


#4 2,4-DCAA

R.T.: 11.286 min
Delta R.T.: 0.019 min
Response: 196262169
Conc: 449.92 ng/ml

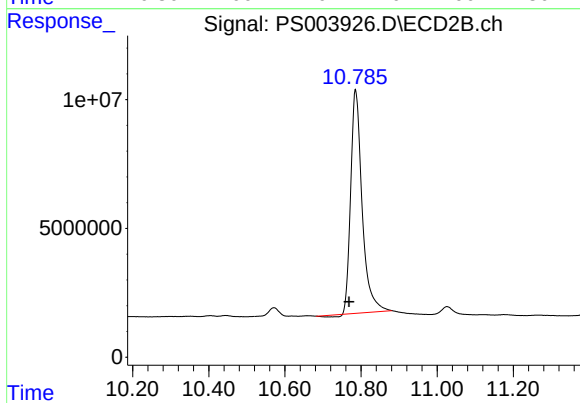

#4 2,4-DCAA


R.T.: 10.786 min
Delta R.T.: 0.017 min
Response: 180759152
Conc: 368.40 ng/ml

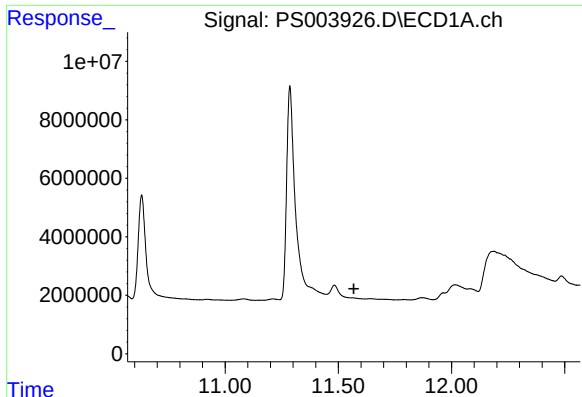

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

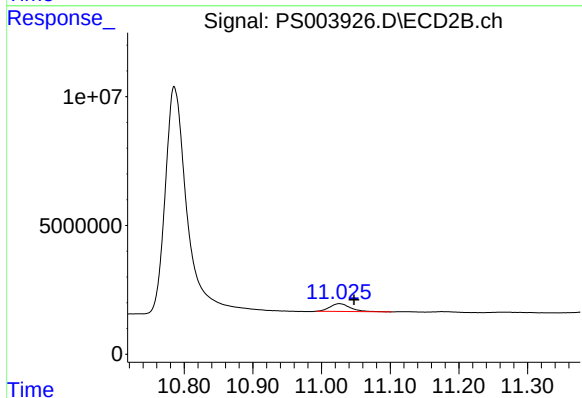


#5 DICAMBA

R.T.: 11.026 min
Delta R.T.: -0.021 min
Response: 6196023
Conc: 3.33 ng/ml

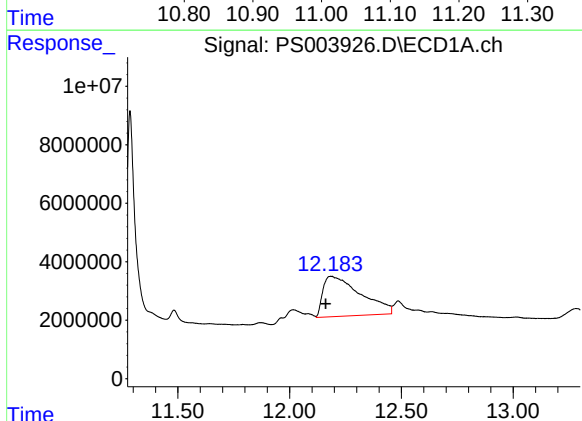


#7 MCPA

R.T.: 12.185 min
Delta R.T.: 0.023 min
Response: 161175924
Conc: 76.39 ug/ml

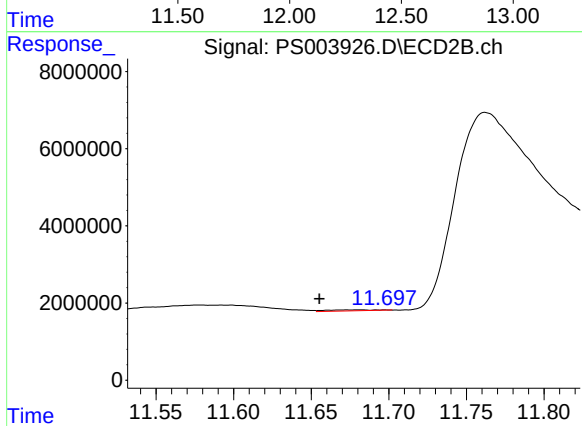

#7 MCPA


R.T.: 11.680 min
Delta R.T.: 0.025 min
Response: 736625
Conc: N.D.

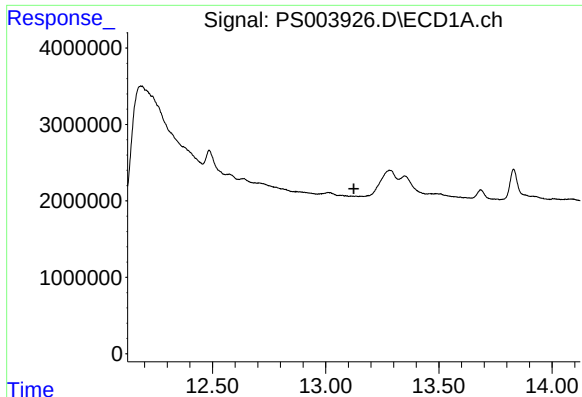

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

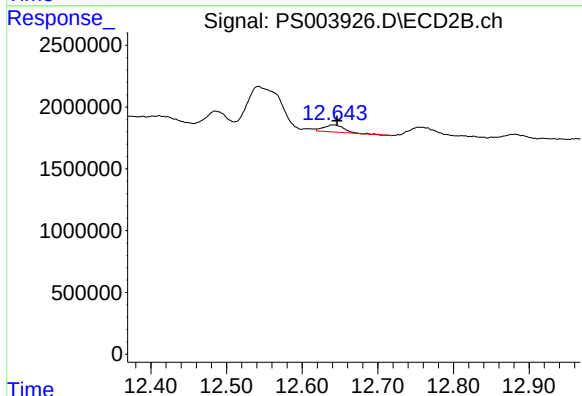


#9 2,4-D

R.T.: 12.641 min
Delta R.T.: -0.005 min
Response: 1082287
Conc: 2.03 ng/ml

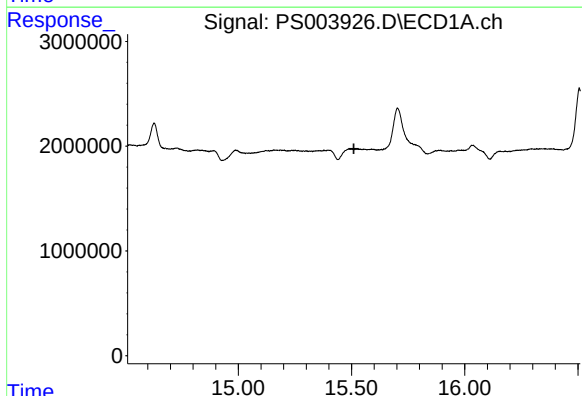


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

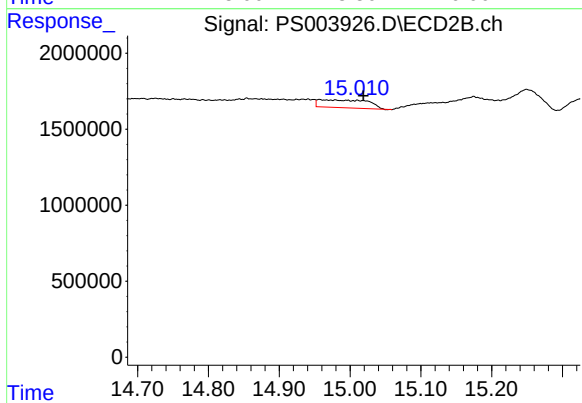

#13 2,4-DB


R.T.: 14.955 min
Delta R.T.: -0.064 min
Response: 2477838
Conc: 8.34 ng/ml

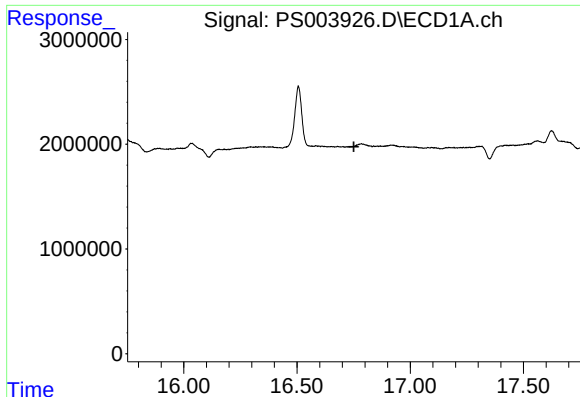

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

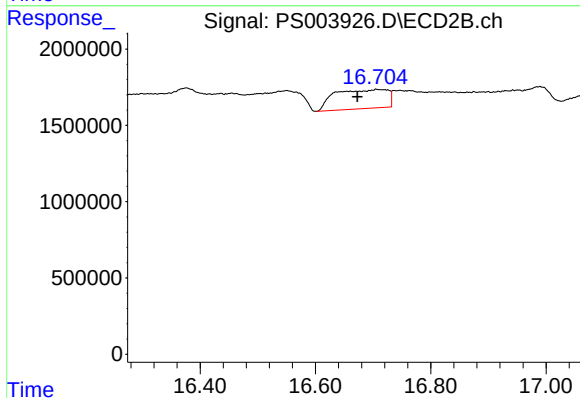


#15 Picloram

R.T.: 16.707 min
Delta R.T.: 0.034 min
Response: 7980055
Conc: 2.52 ng/ml

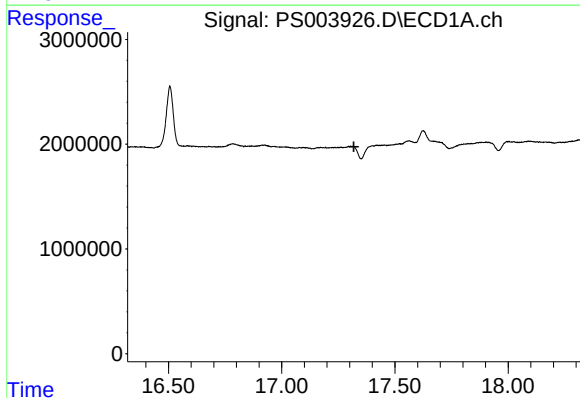

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

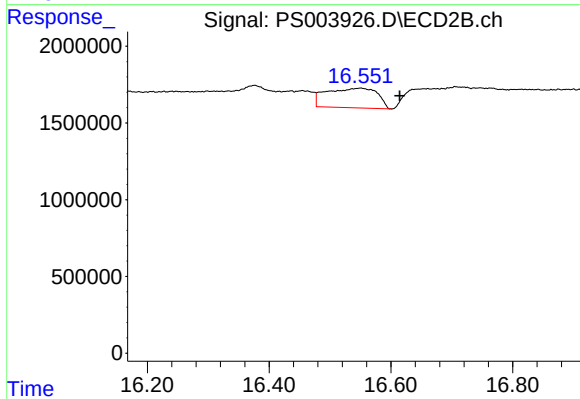

#16 DCPA

R.T.: 16.550 min
Delta R.T.: -0.064 min
Response: 7410248
Conc: 2.19 ng/ml