

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 04:19
 Operator : EI\SJ
 Sample : K2180-32
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 05:45:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.782	155.8E6	141.6E6	357.192	288.547
Target Compounds							
1) T	Dalapon	2.798	2.293	25440273	29807373	34.124	40.853
2) T	3,5-DICHL...	0.000	8.945	0	4959783	N.D.	7.776
3) T	4-Nitroph...	0.000	9.953	0	13892179	N.D.	61.190
5) T	DICAMBA	0.000	11.021	0	3308485	N.D.	1.779
7) T	MCPA	12.148	11.672	312.2E6	544225	147.999	<MDL #
9) T	2,4-D	0.000	12.637	0	975262	N.D.	1.834
10) T	Pentachlo...	0.000	13.115	0	5255049	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.823	0	4227636	N.D.	1.596
12) T	2,4,5-T	0.000	14.372	0	86286	N.D.	<MDL
13) T	2,4-DB	0.000	15.007	0	2148274	N.D.	7.234
14) T	DINOSEB	0.000	15.452	0	912148	N.D.	<MDL
15) T	Picloram	0.000	16.666	0	5203302	N.D.	1.641
16) T	DCPA	0.000	16.643	0	4098031	N.D.	1.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 04:19
Operator : EI\SJ
Sample : K2180-32
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 05:45:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

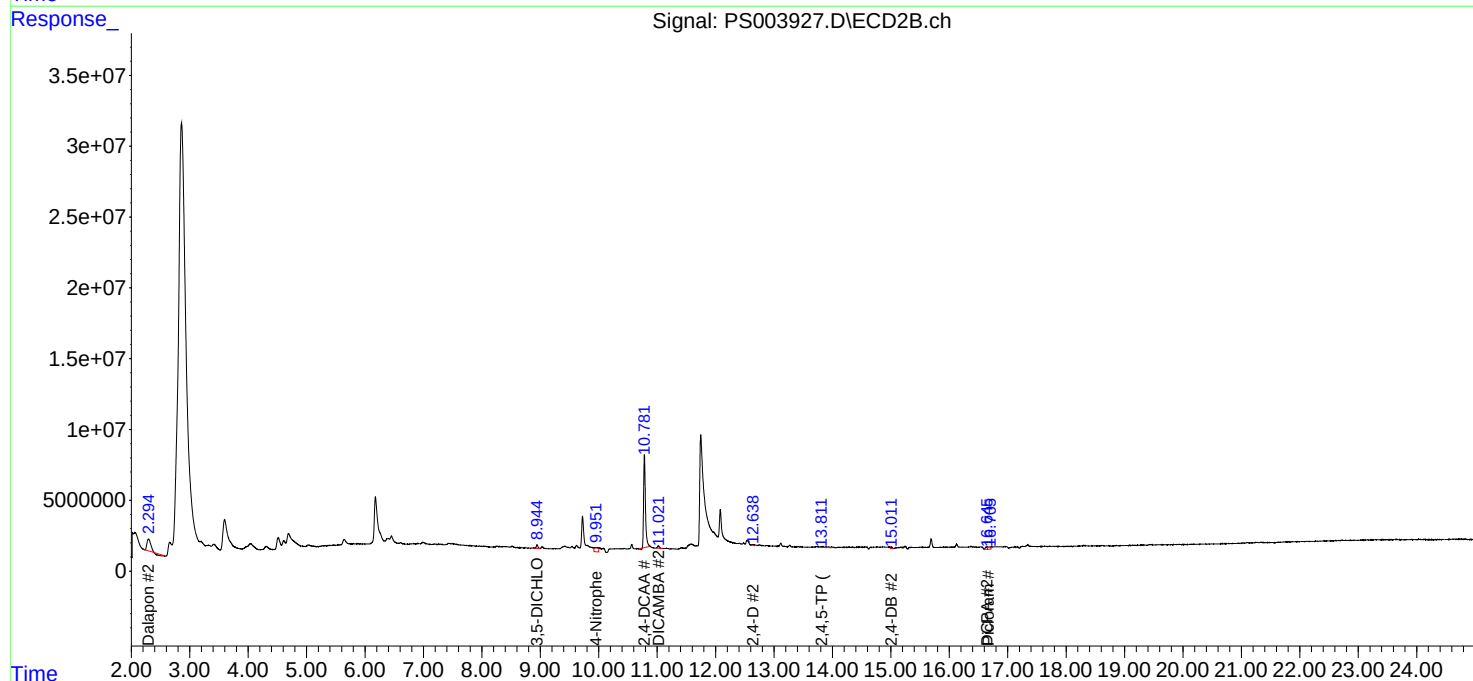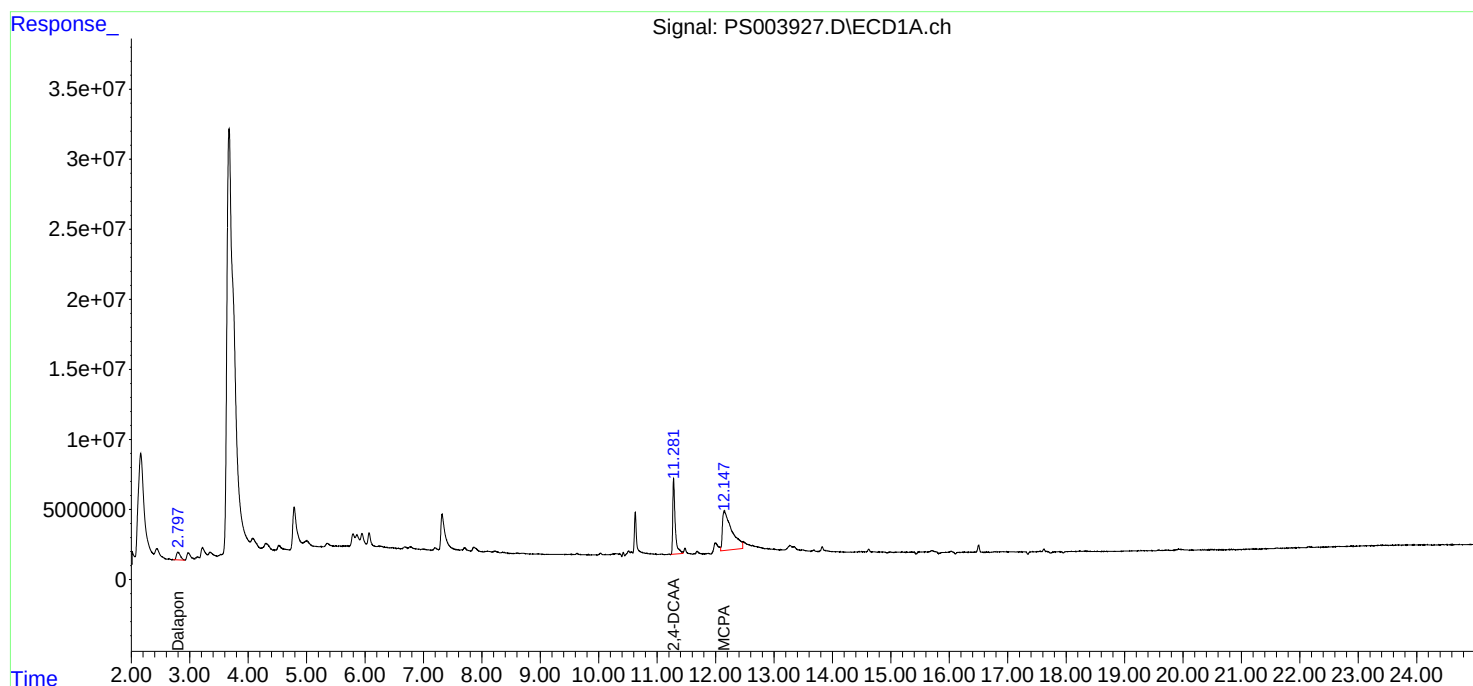


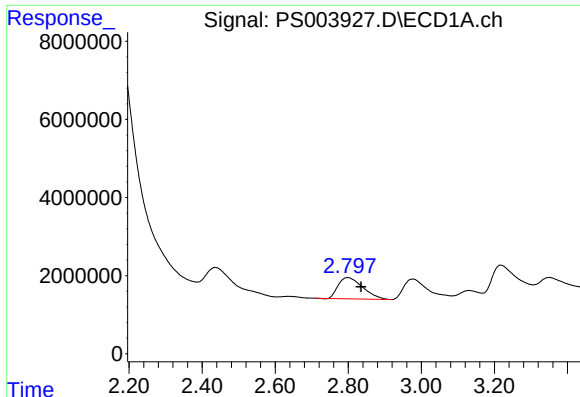

#1 Dalapon


R.T.: 2.798 min
Delta R.T.: -0.037 min
Response: 25440273
Conc: 34.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

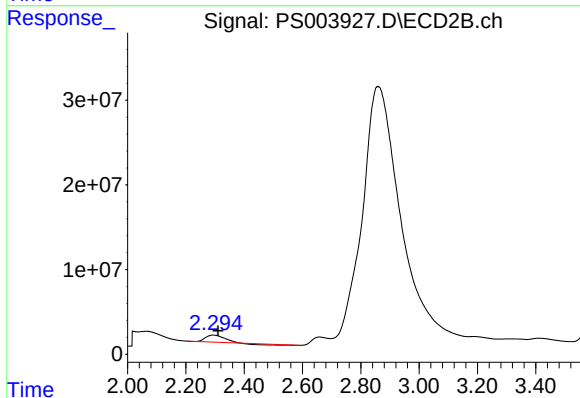


#1 Dalapon

R.T.: 2.293 min
Delta R.T.: -0.018 min
Response: 29807373
Conc: 40.85 ng/ml

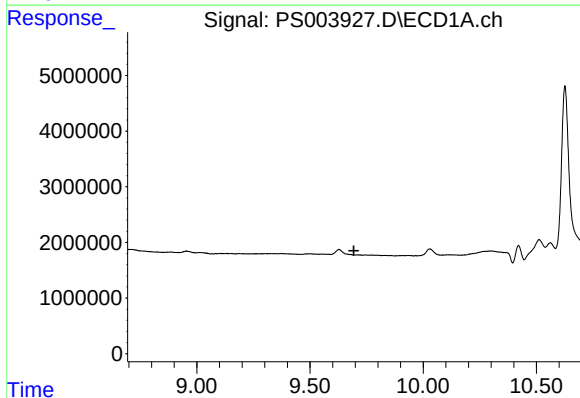


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

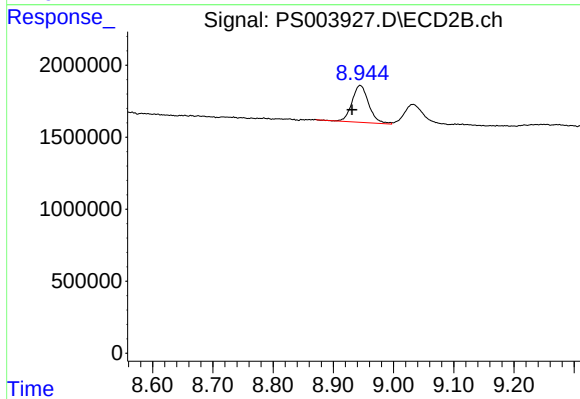

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: 0.014 min
Response: 4959783
Conc: 7.78 ng/ml

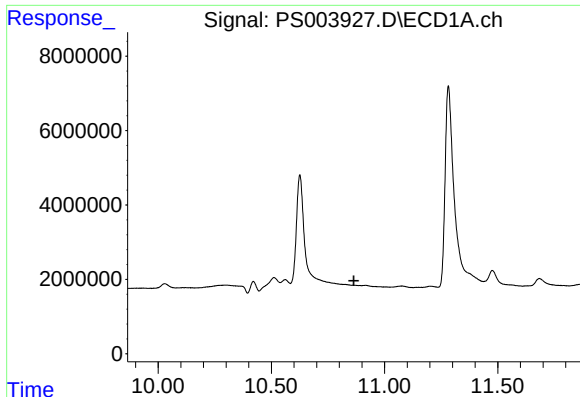

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

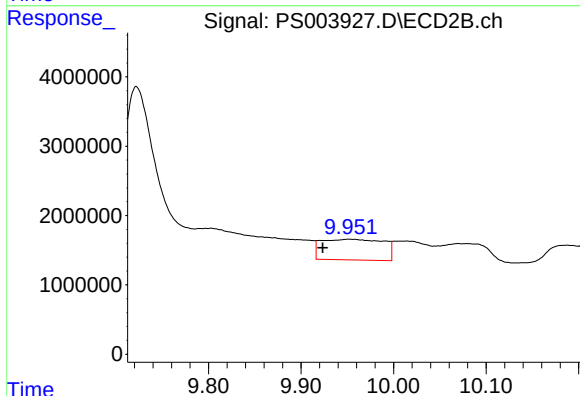


#3 4-Nitrophenol

R.T.: 9.953 min
Delta R.T.: 0.029 min
Response: 13892179
Conc: 61.19 ng/ml

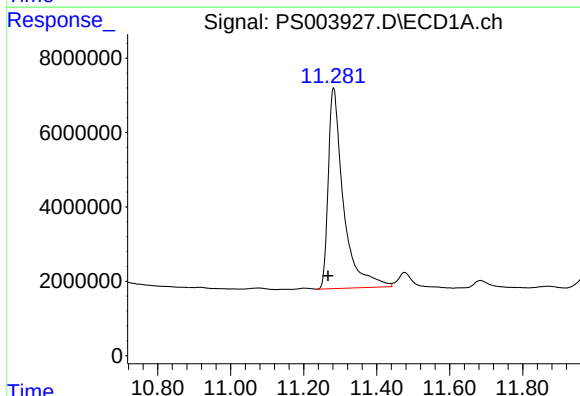


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: 0.015 min
Response: 155811425
Conc: 357.19 ng/ml

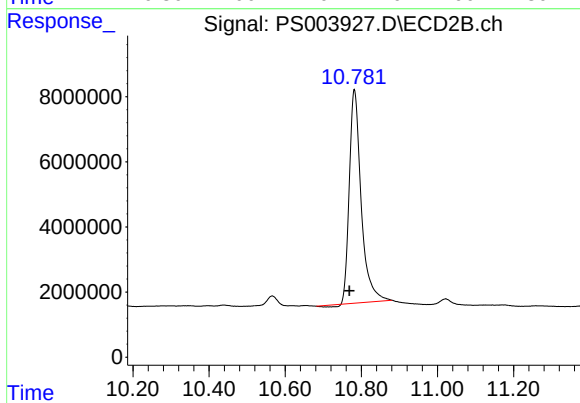

#4 2,4-DCAA


R.T.: 10.782 min
Delta R.T.: 0.013 min
Response: 141578164
Conc: 288.55 ng/ml

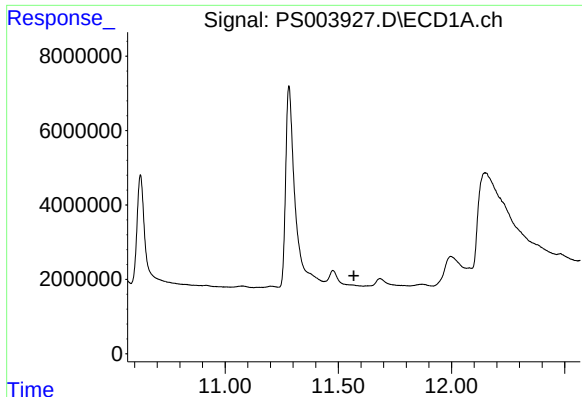

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

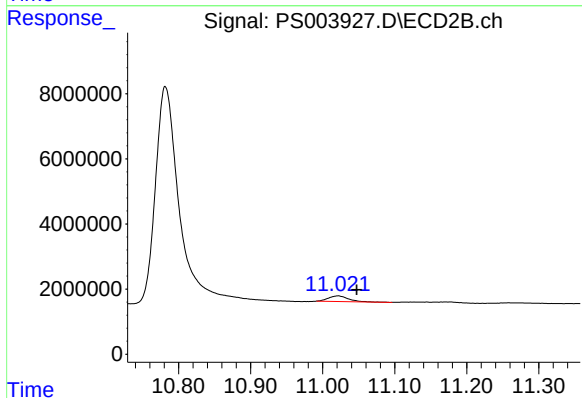


#5 DICAMBA

R.T.: 11.021 min
Delta R.T.: -0.026 min
Response: 3308485
Conc: 1.78 ng/ml

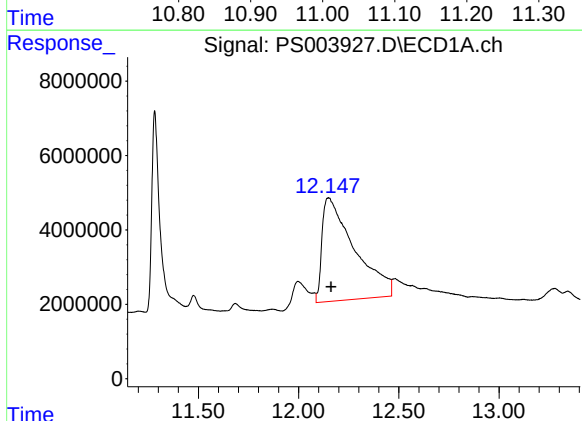


#7 MCPA

R.T.: 12.148 min
Delta R.T.: -0.013 min
Response: 312246575
Conc: 148.00 ug/ml

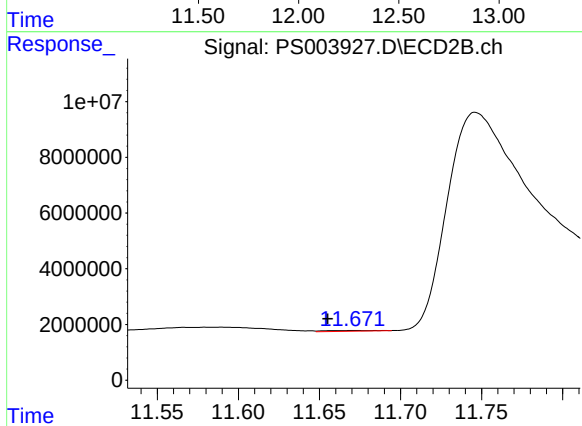

#7 MCPA


R.T.: 11.672 min
Delta R.T.: 0.016 min
Response: 544225
Conc: N.D.

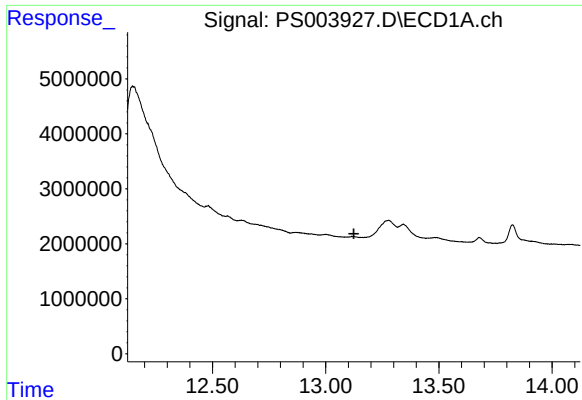

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

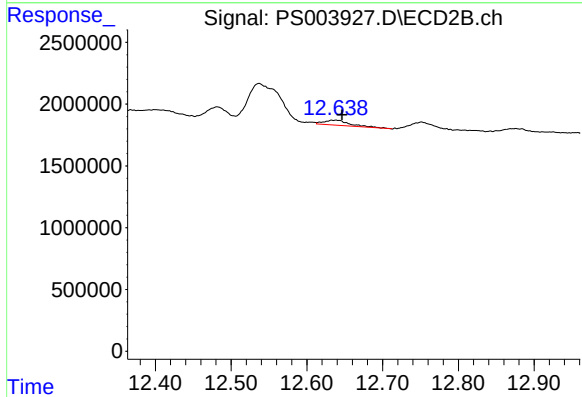


#9 2,4-D

R.T.: 12.637 min
Delta R.T.: -0.009 min
Response: 975262
Conc: 1.83 ng/ml

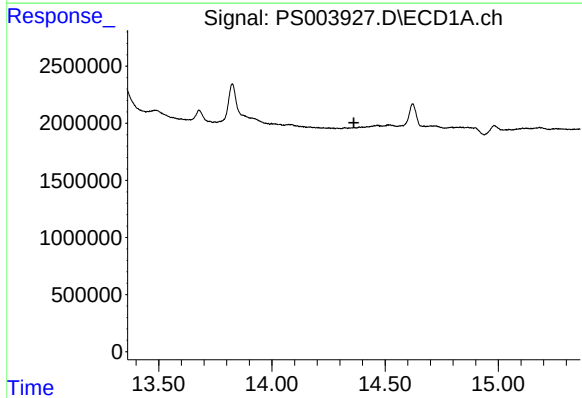


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

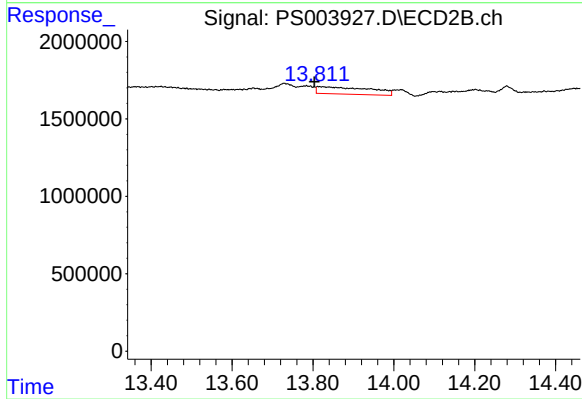

#11 2,4,5-TP (SILVEX)


R.T.: 13.823 min
Delta R.T.: 0.020 min
Response: 4227636
Conc: 1.60 ng/ml

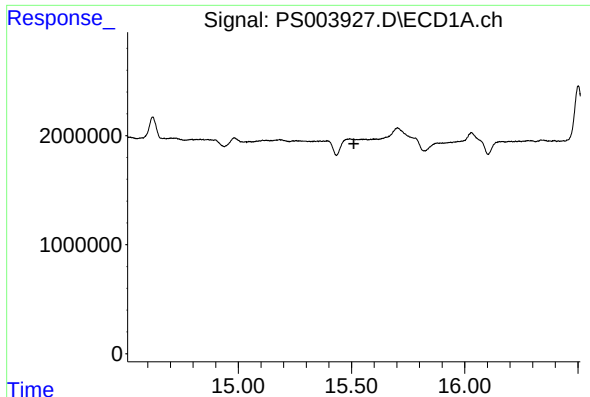

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

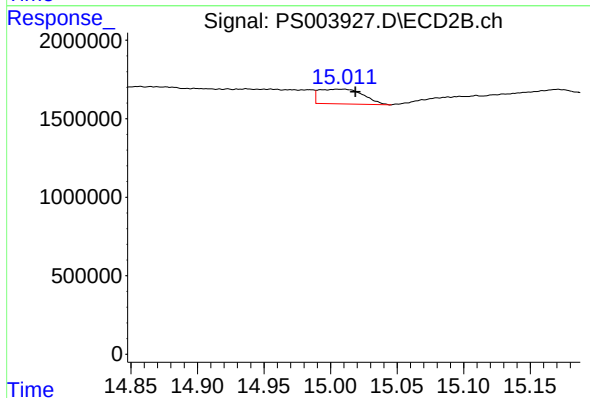


#13 2,4-DB

R.T.: 15.007 min
Delta R.T.: -0.011 min
Response: 2148274
Conc: 7.23 ng/ml

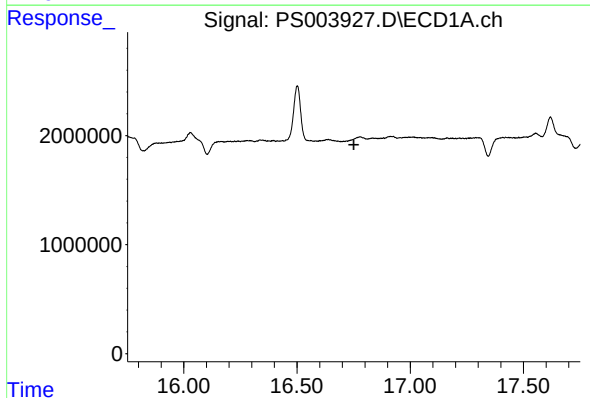


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

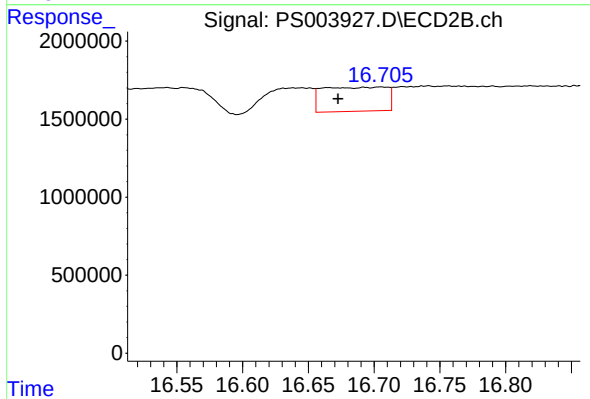

#15 Picloram


R.T.: 16.666 min
Delta R.T.: -0.007 min
Response: 5203302
Conc: 1.64 ng/ml

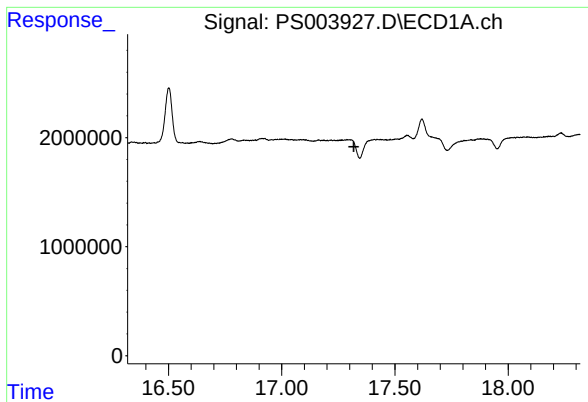

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

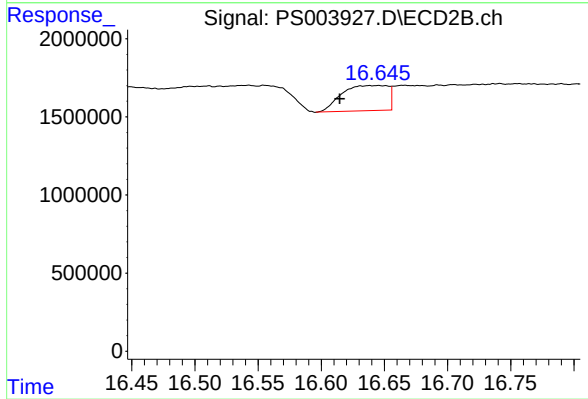

#16 DCPA

R.T.: 16.643 min
Delta R.T.: 0.029 min
Response: 4098031
Conc: 1.21 ng/ml