

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
 Data File : PS003928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 04:50
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 05:45:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.304	10.803	254.2E6	229.8E6	582.683	468.363
Target Compounds							
7) T	MCPA	0.000	11.689	0	485002	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.214	0	1395275	N.D.	2.997
9) T	2,4-D	0.000	12.677	0	436633	N.D.	<MDL
10) T	Pentachlo...	0.000	13.144	0	134598	N.D.	<MDL
12) T	2,4,5-T	0.000	14.327	0	209879	N.D.	<MDL
13) T	2,4-DB	0.000	15.075	0	1195447	N.D.	4.026
14) T	DINOSEB	0.000	15.430	0	2184672	N.D.	1.139
15) T	Picloram	0.000	16.651	0	1342998	N.D.	<MDL
16) T	DCPA	0.000	16.651	0	1342998	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040219\
Data File : PS003928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 04:50
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 05:45:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

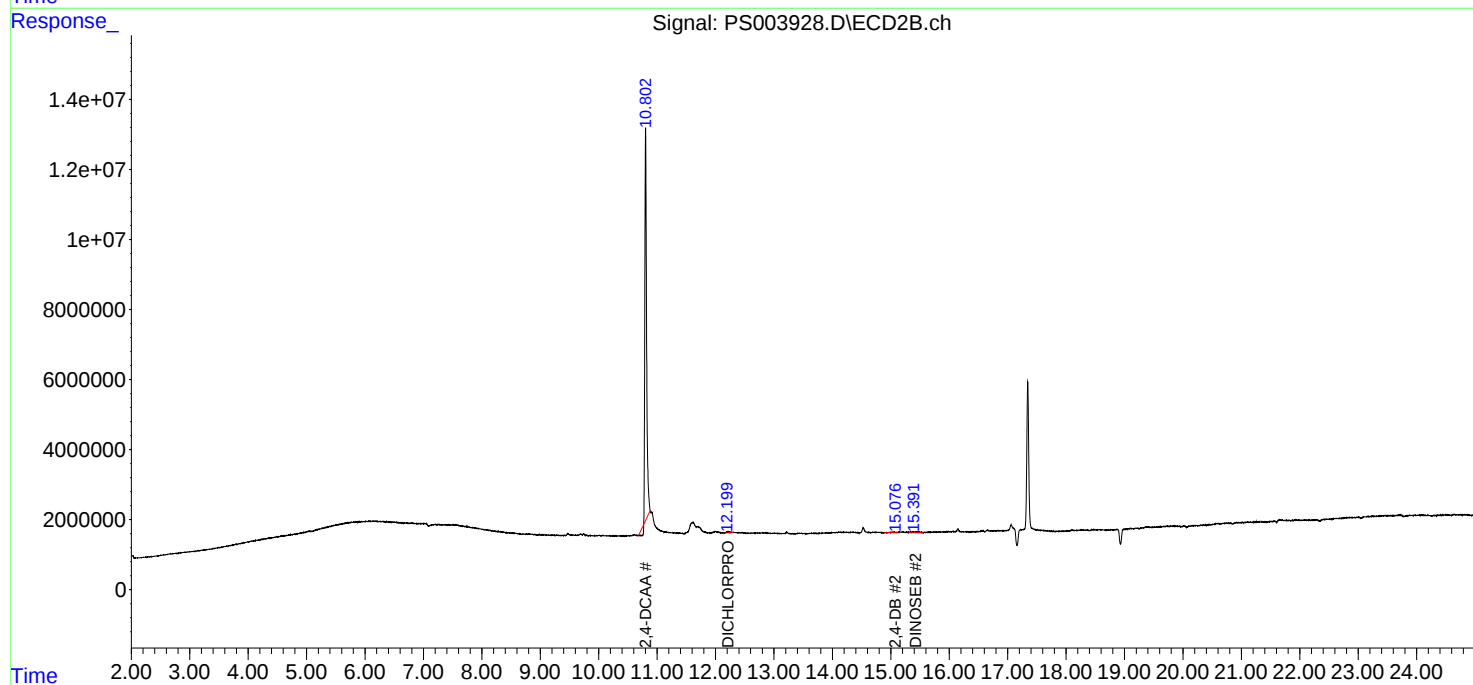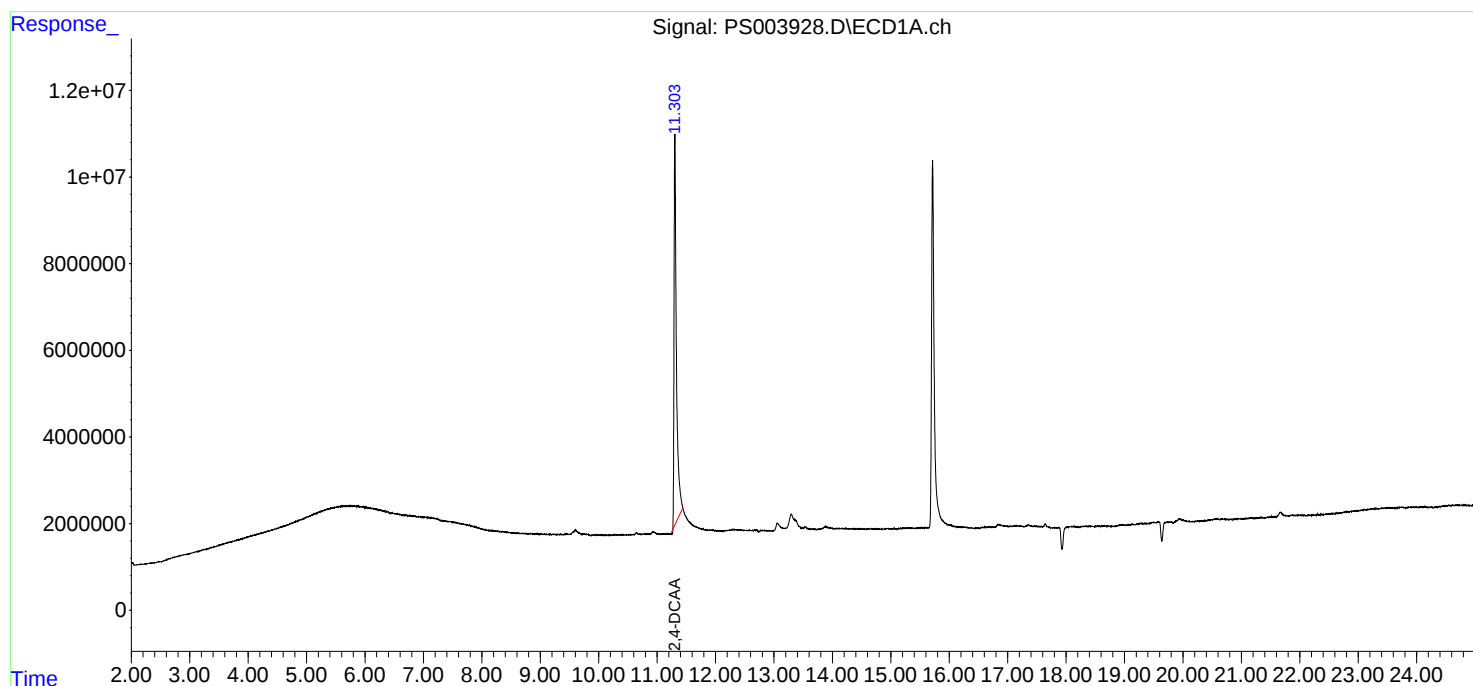


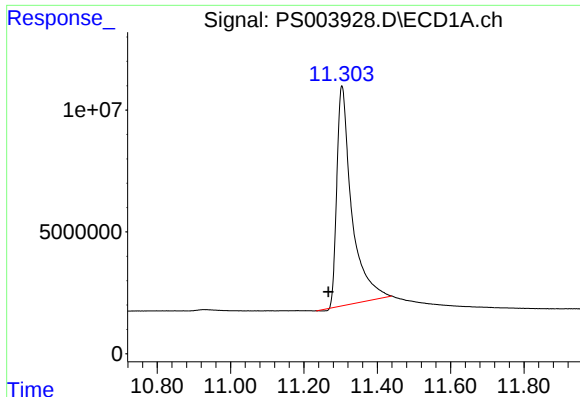

#4 2,4-DCAA


R.T.: 11.304 min
Delta R.T.: 0.037 min
Response: 254173708
Conc: 582.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

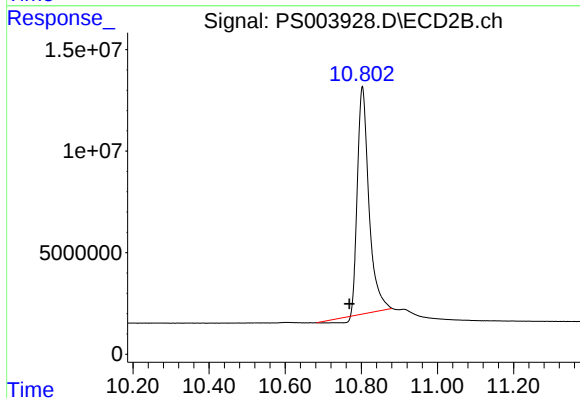


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: 0.034 min
Response: 229806207
Conc: 468.36 ng/ml

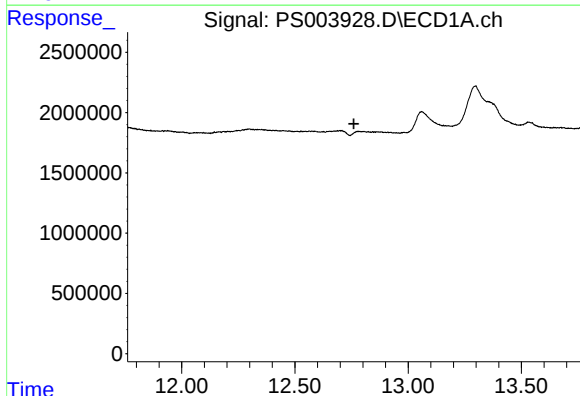


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

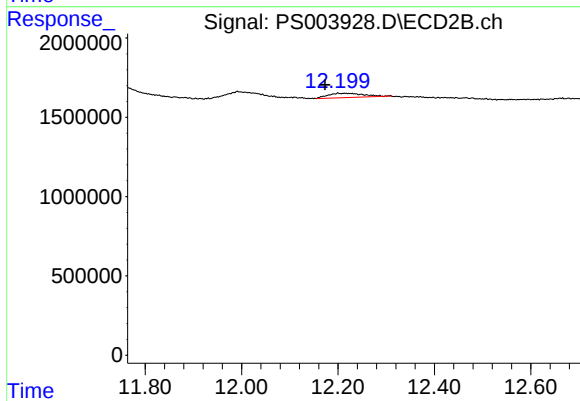

#8 DICHLORPROP


R.T.: 12.214 min
Delta R.T.: 0.041 min
Response: 1395275
Conc: 3.00 ng/ml

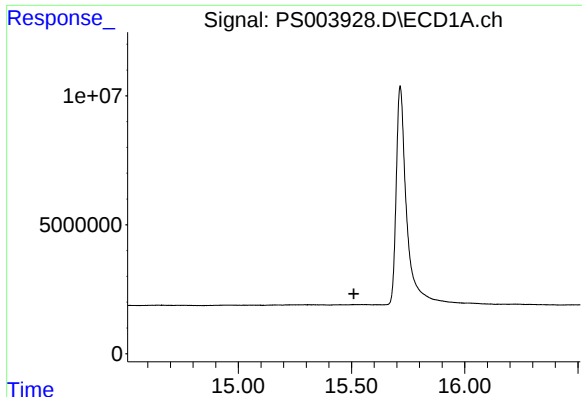

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

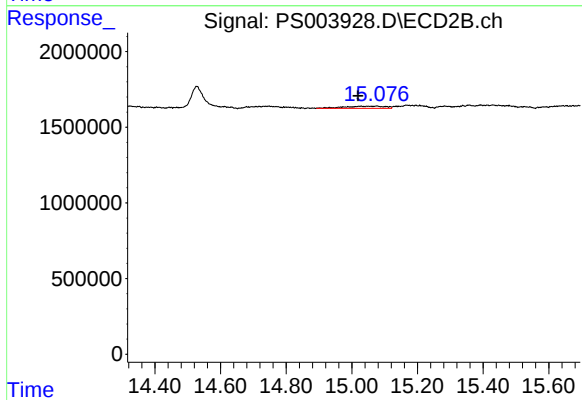


#13 2,4-DB

R.T.: 15.075 min
Delta R.T.: 0.056 min
Response: 1195447
Conc: 4.03 ng/ml

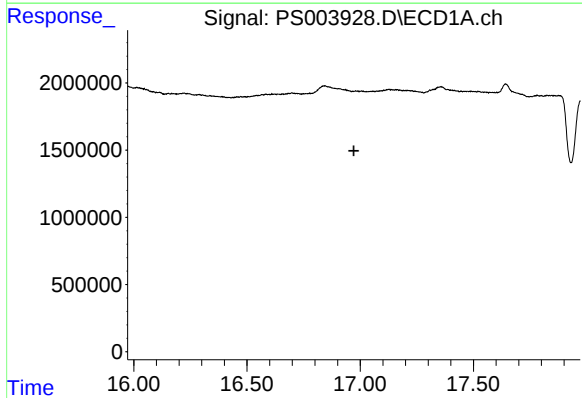

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

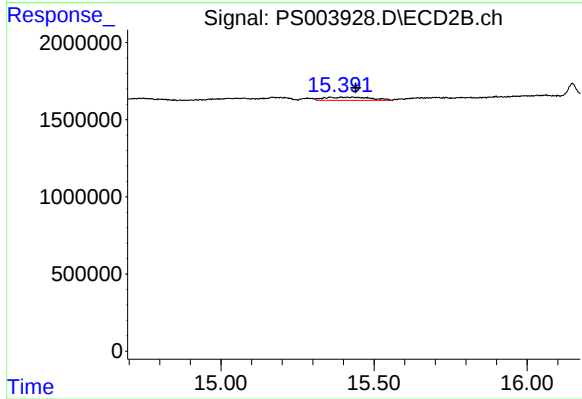

#14 DINOSEB

R.T.: 15.430 min
Delta R.T.: -0.010 min
Response: 2184672
Conc: 1.14 ng/ml