

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 08:12
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 12:00:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	10.888	9.931	4961815	6136823	22.901 27.030
7) T	MCPA	12.229	11.692	97477045	-10757	46.202 N.D. #
11) T	2,4,5-TP ...	0.000	13.836	0	2018698	N.D. <MDL
13) T	2,4-DB	0.000	14.980	0	11648340	N.D. 39.227
14) T	DINOSEB	0.000	15.422	0	22746728	N.D. 11.855
15) T	Picloram	16.729	0.000	166.2E6	0	48.926 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 08:12
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 12:00:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

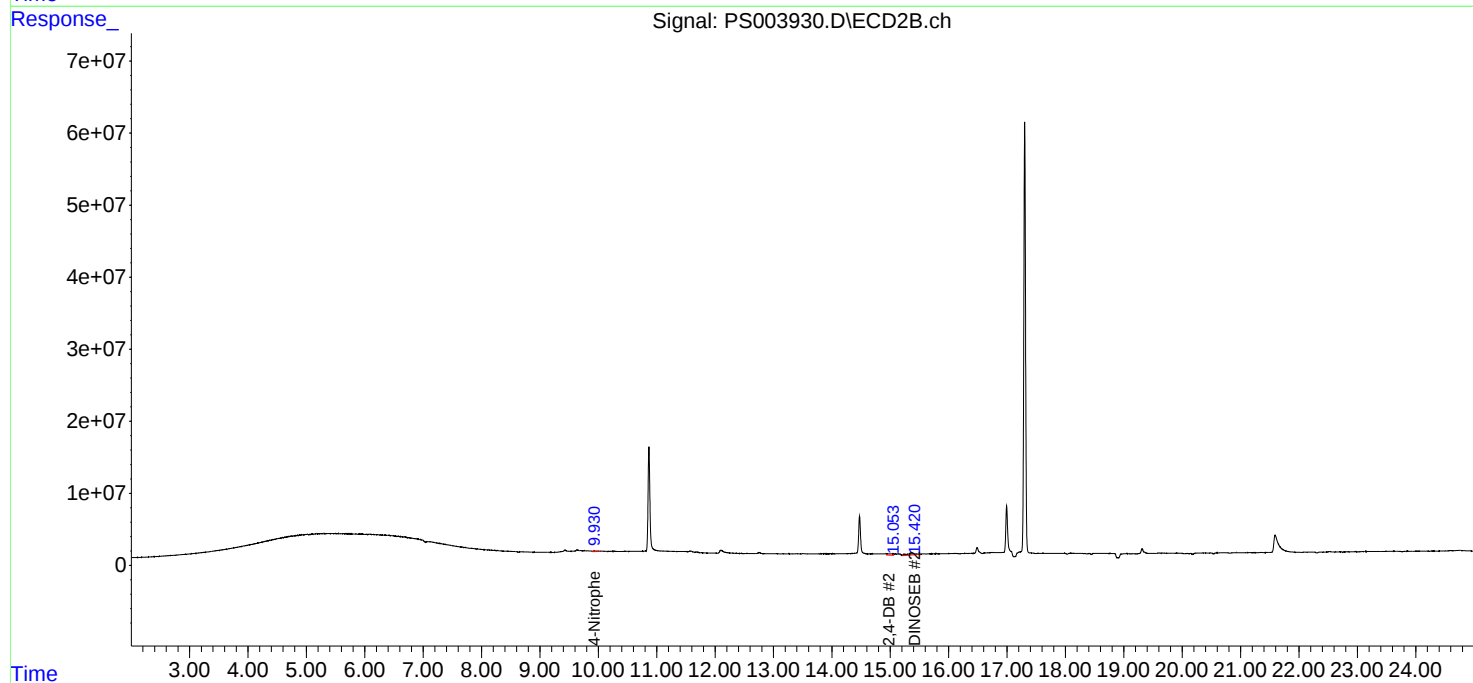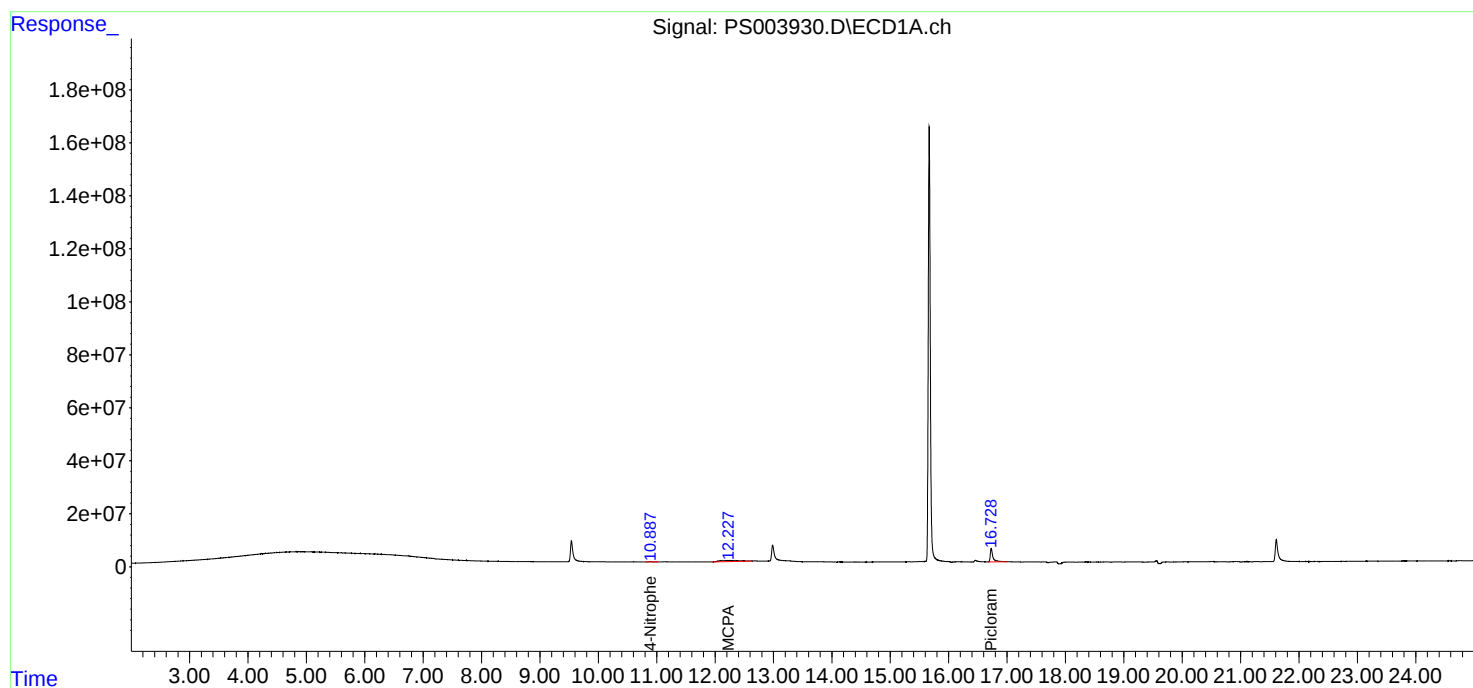


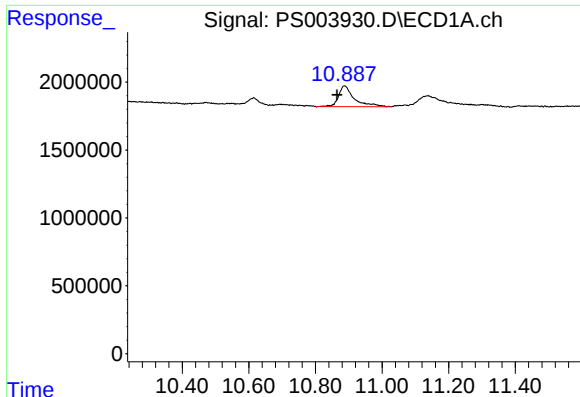

#3 4-Nitrophenol


R.T.: 10.888 min
Delta R.T.: 0.023 min
Response: 4961815
Conc: 22.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

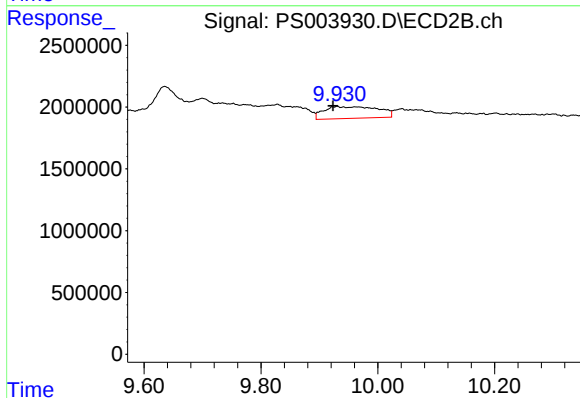


#3 4-Nitrophenol

R.T.: 9.931 min
Delta R.T.: 0.008 min
Response: 6136823
Conc: 27.03 ng/ml

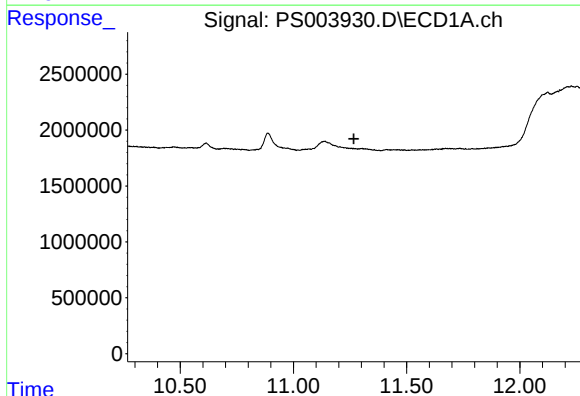


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.267 min
Response: 0
Conc: N.D.

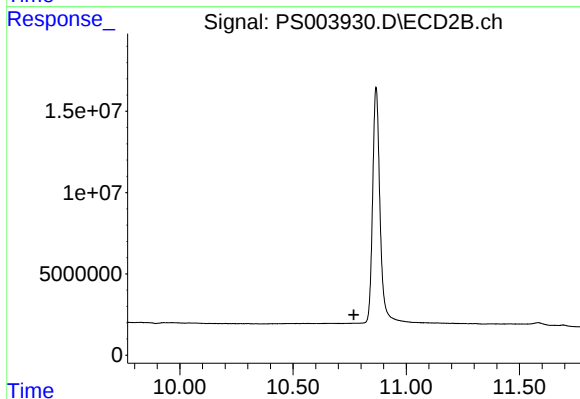

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 10.769 min
Response: 0
Conc: N.D.

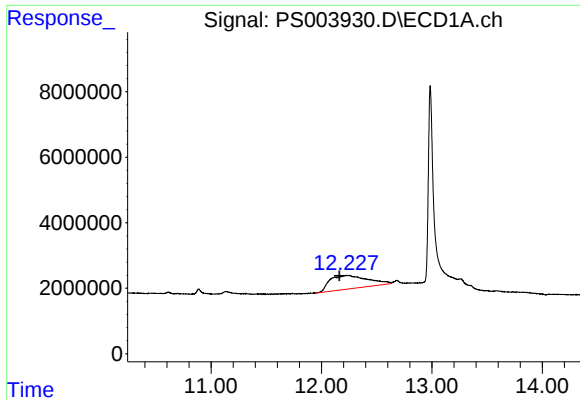

#7 MCPA


R.T.: 12.229 min
Delta R.T.: 0.067 min
Response: 97477045
Conc: 46.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

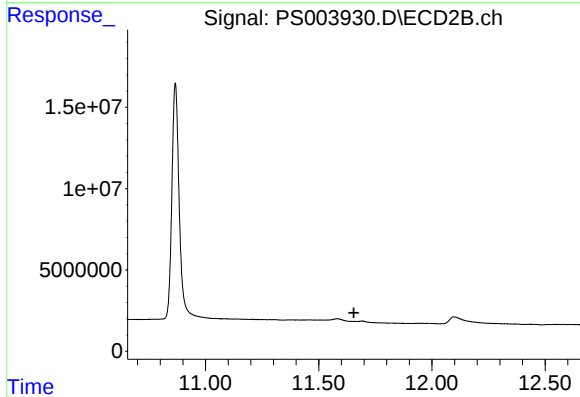


#7 MCPA

R.T.: 11.692 min
Delta R.T.: 0.036 min
Response: -10757
Conc: N.D.

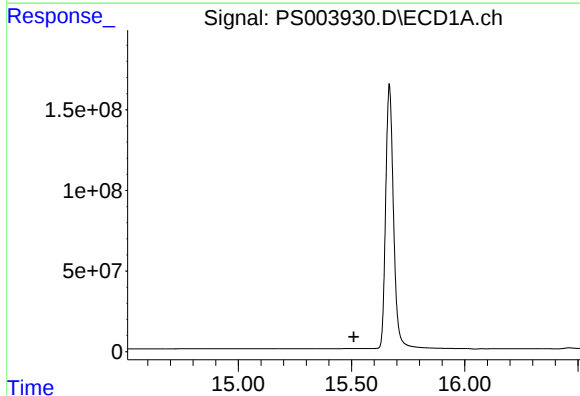


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.510 min
Response: 0
Conc: N.D.

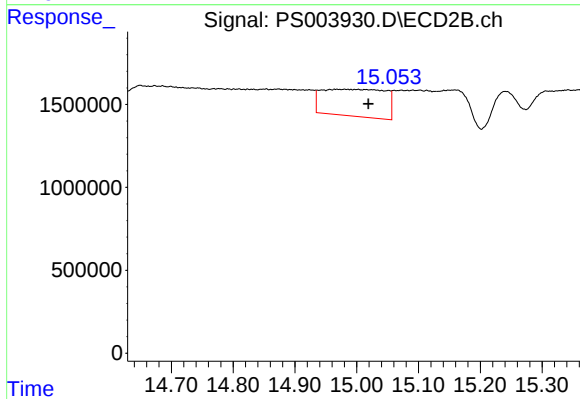

#13 2,4-DB


R.T.: 14.980 min
Delta R.T.: -0.039 min
Response: 11648340
Conc: 39.23 ng/ml

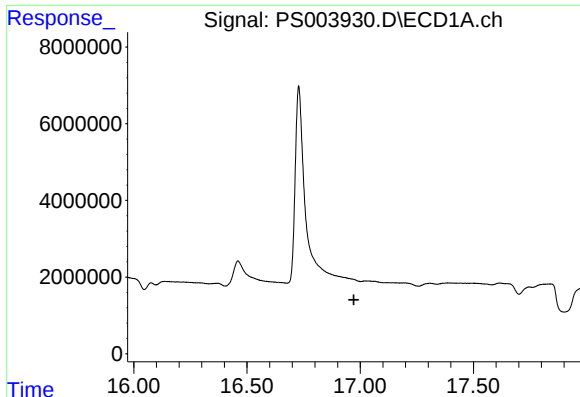

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

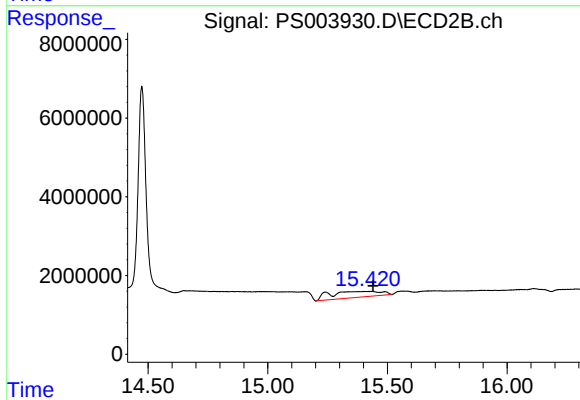


#14 DINOSEB

R.T.: 15.422 min
Delta R.T.: -0.018 min
Response: 22746728
Conc: 11.86 ng/ml

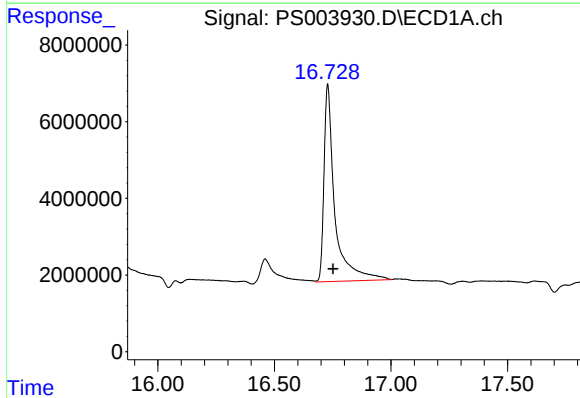

#15 Picloram

R.T.: 16.729 min
Delta R.T.: -0.023 min
Response: 166204397
Conc: 48.93 ng/ml

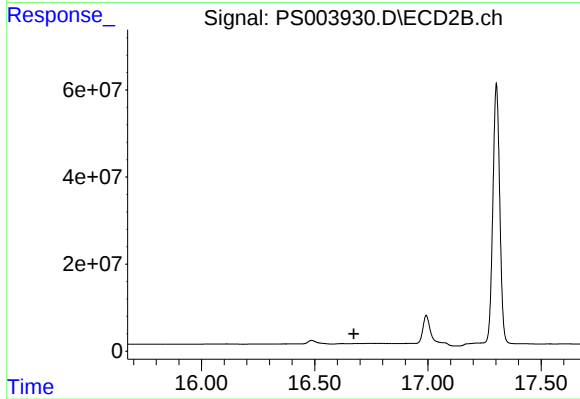

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.673 min
Response: 0
Conc: N.D.