

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 08:43
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 12:00:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.769	286.3E6	260.3E6	656.364	530.584
Target Compounds							
3) T	4-Nitroph...	0.000	9.950	0	241659	N.D.	1.064
6) T	MCP	0.000	11.264	0	1143395	N.D.	<MDL
7) T	MCPA	0.000	11.652	0	1341637	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.188	0	1849649	N.D.	3.973
9) T	2,4-D	0.000	12.633	0	469656	N.D.	<MDL
10) T	Pentachlo...	0.000	13.186	0	1846658	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.829	0	1517560	N.D.	<MDL
13) T	2,4-DB	0.000	15.032	0	1502639	N.D.	5.060
14) T	DINOSEB	0.000	15.453	0	354256	N.D.	<MDL
15) T	Picloram	0.000	16.618	0	1216021	N.D.	<MDL
16) T	DCPA	0.000	16.618	0	1216021	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 08:43
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 12:00:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

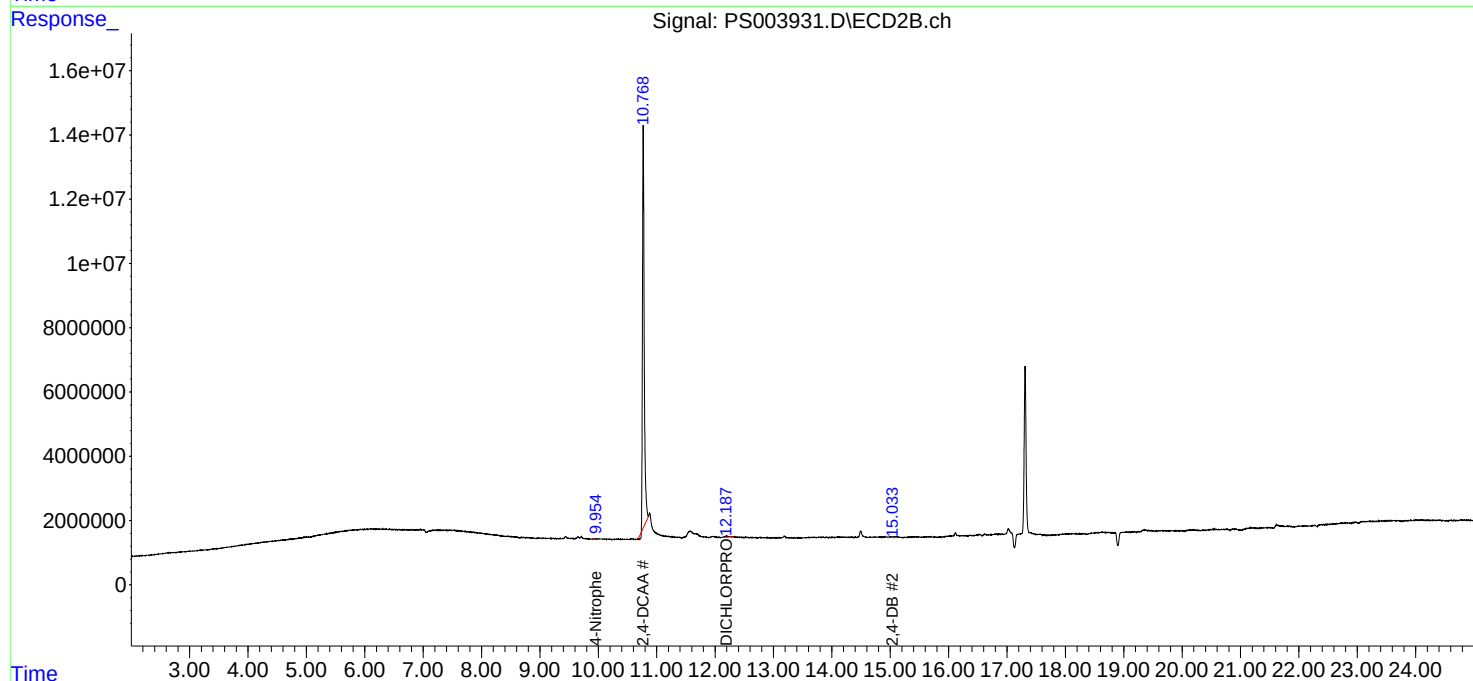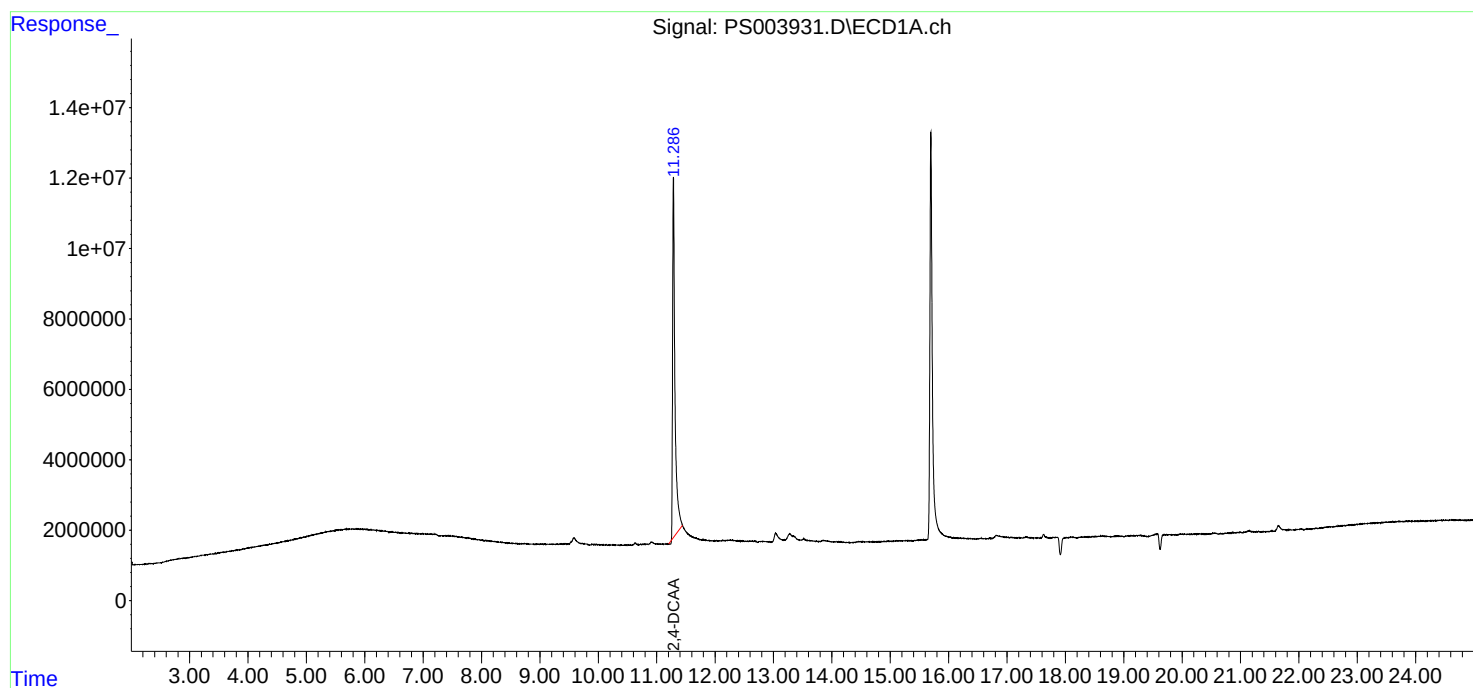


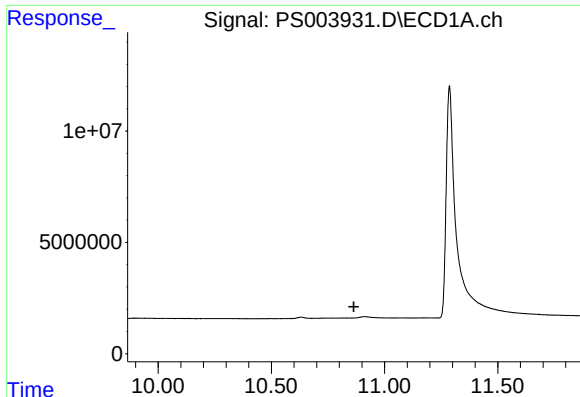

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

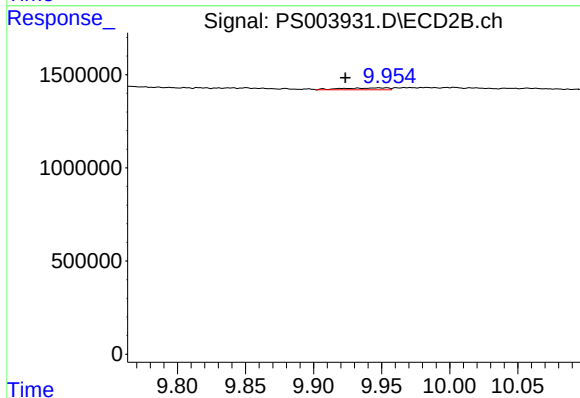


#3 4-Nitrophenol

R.T.: 9.950 min
Delta R.T.: 0.026 min
Response: 241659
Conc: 1.06 ng/ml

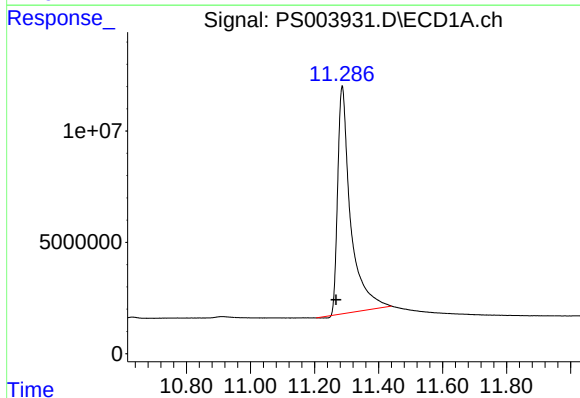


#4 2,4-DCAA

R.T.: 11.287 min
Delta R.T.: 0.020 min
Response: 286314124
Conc: 656.36 ng/ml

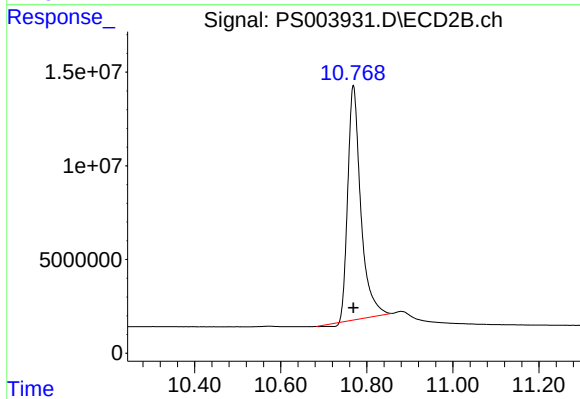

#4 2,4-DCAA


R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 260335484
Conc: 530.58 ng/ml

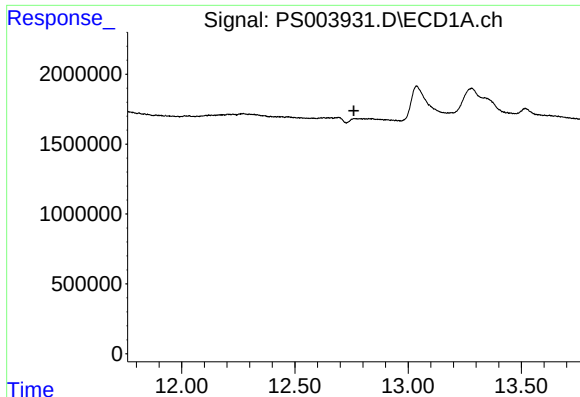

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

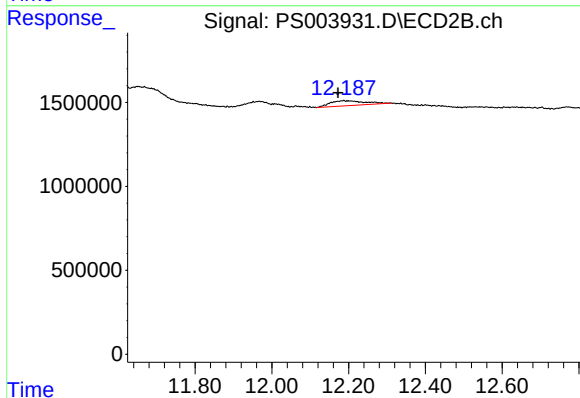


#8 DICHLORPROP

R.T.: 12.188 min
Delta R.T.: 0.015 min
Response: 1849649
Conc: 3.97 ng/ml

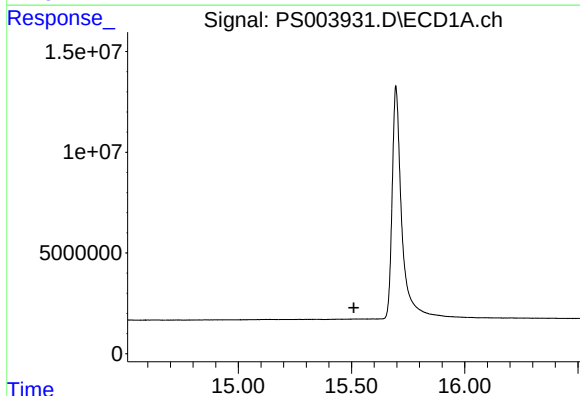

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

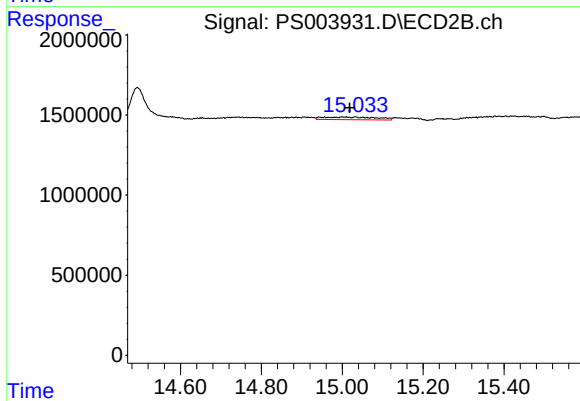

#13 2,4-DB

R.T.: 15.032 min
Delta R.T.: 0.013 min
Response: 1502639
Conc: 5.06 ng/ml