

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 11:34
 Operator : EI\SJ
 Sample : K2056-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CS-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 13:16:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.265	10.765	226.0E6	219.3E6	518.071	446.915
Target Compounds							
1) T	Dalapon	2.783	2.280	38774373	98143834	52.009	134.512 #
2) T	3,5-DICHL...	0.000	8.930	0	4296070	N.D.	6.735
3) T	4-Nitroph...	0.000	9.938	0	20521966	N.D.	90.391
9) T	2,4-D	0.000	12.622	0	2315793	N.D.	4.354
10) T	Pentachlo...	13.486	13.173	10749830	8776578	1.395	1.268
11) T	2,4,5-TP ...	0.000	13.803	0	3531884	N.D.	1.334
12) T	2,4,5-T	0.000	14.313	0	347382	N.D.	<MDL
15) T	Picloram	16.757	16.709	5599241	13576029	1.648	4.281 #
16) T	DCPA	0.000	16.622	0	3918244	N.D.	1.159



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 11:34
Operator : EI\SJ
Sample : K2056-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CS-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 13:16:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

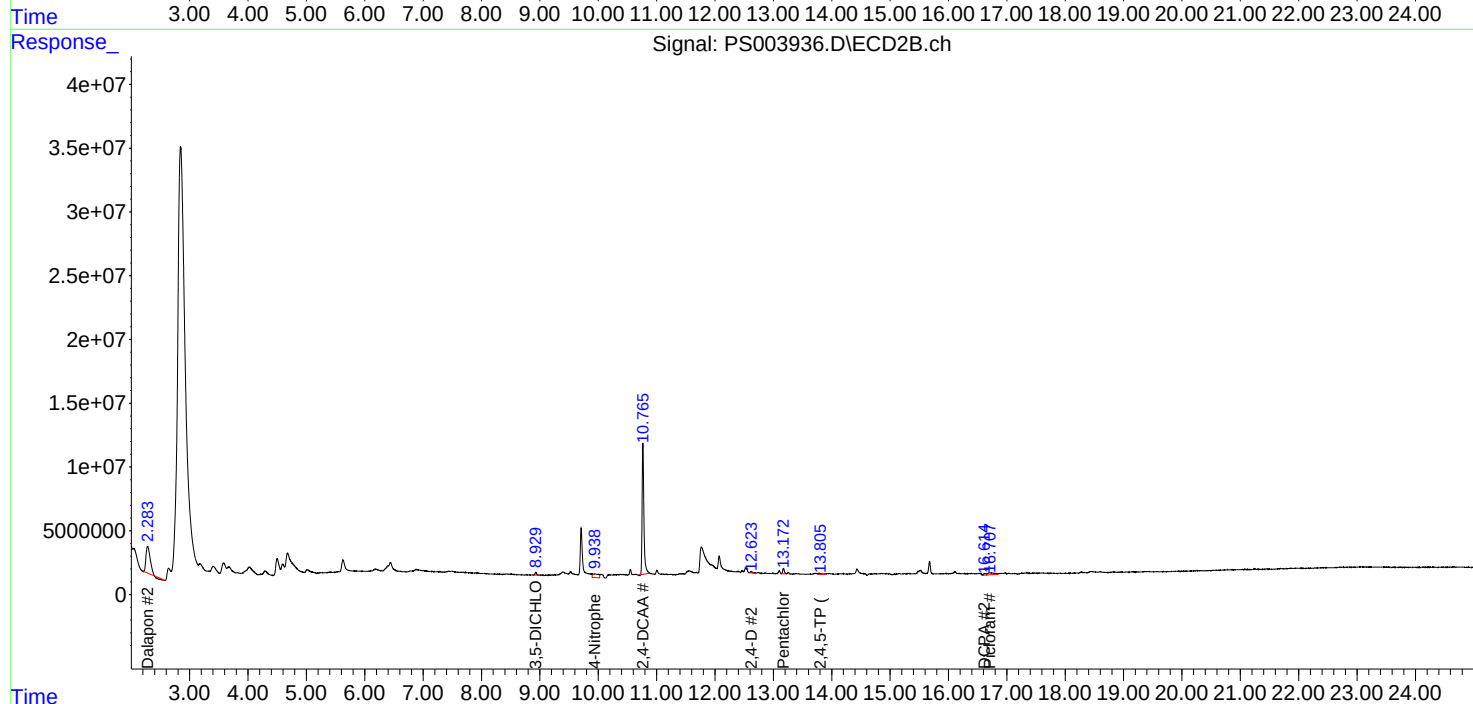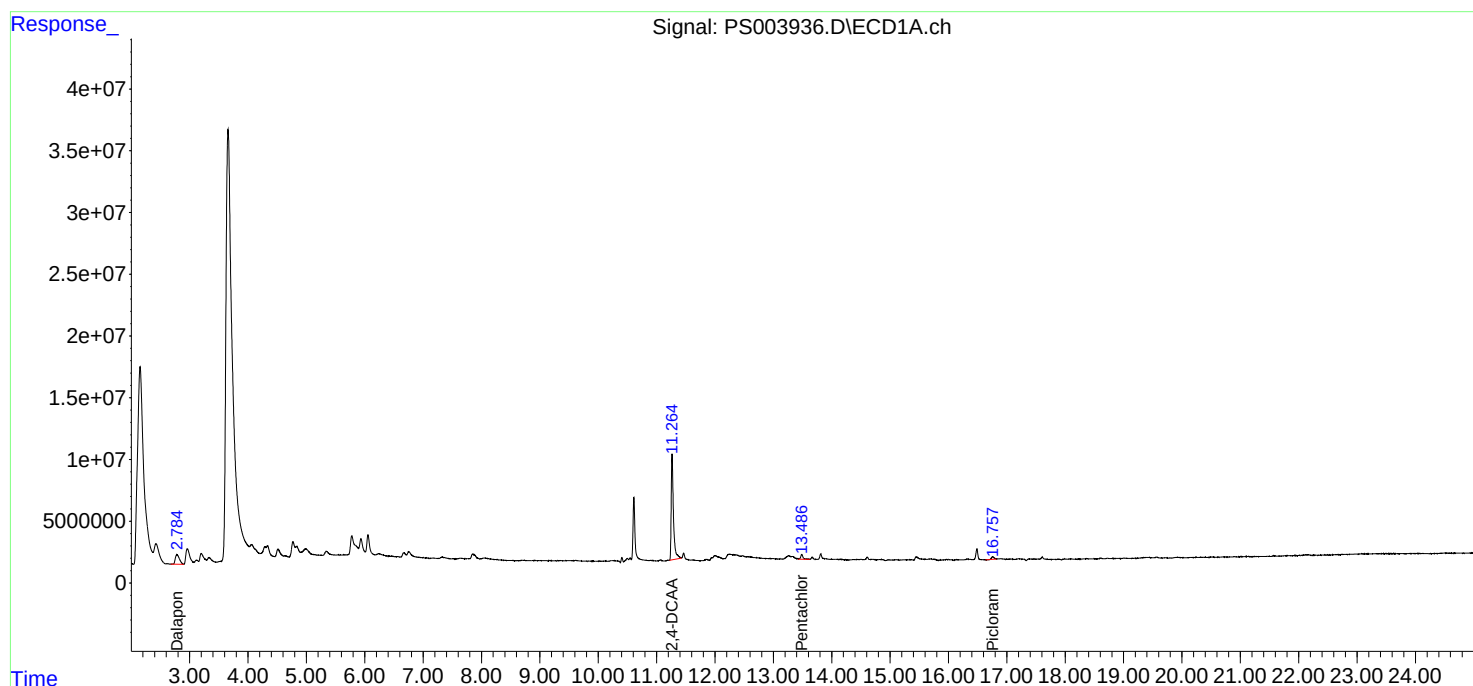


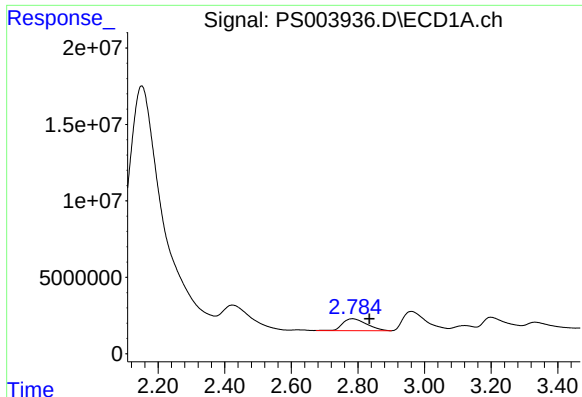

#1 Dalapon


R.T.: 2.783 min
Delta R.T.: -0.052 min
Response: 38774373
Conc: 52.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
CS-7

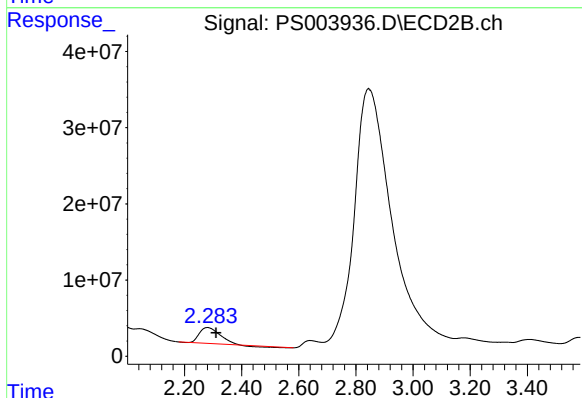


#1 Dalapon

R.T.: 2.280 min
Delta R.T.: -0.030 min
Response: 98143834
Conc: 134.51 ng/ml

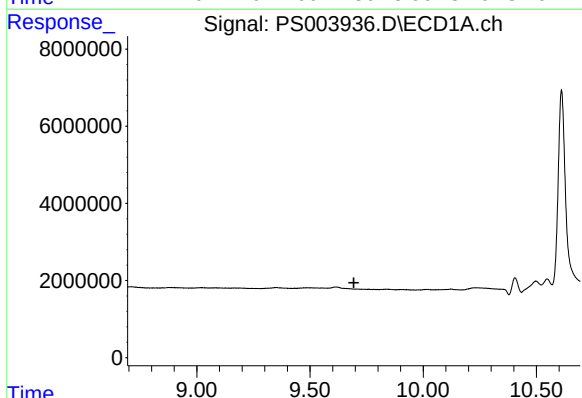


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

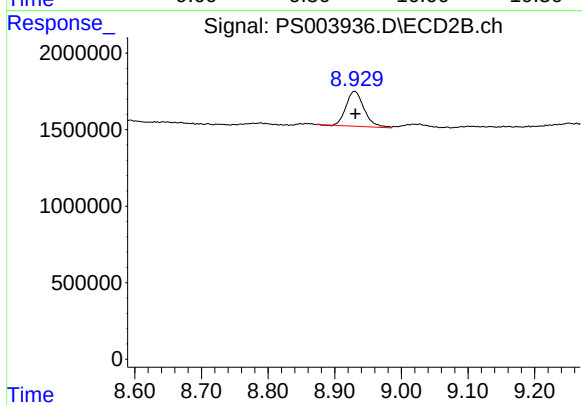

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.930 min
Delta R.T.: -0.001 min
Response: 4296070
Conc: 6.74 ng/ml

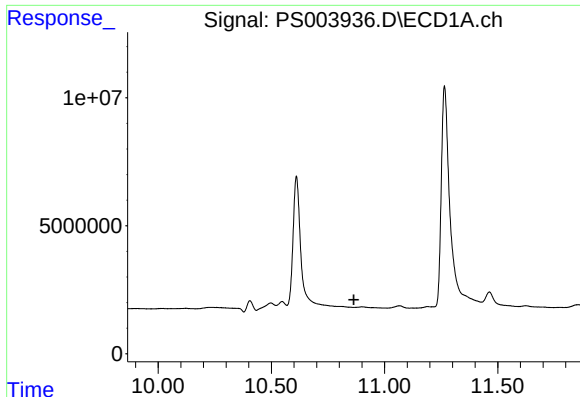

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-7

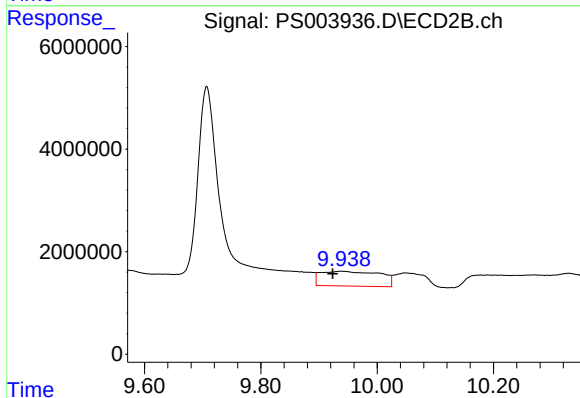


#3 4-Nitrophenol

R.T.: 9.938 min
Delta R.T.: 0.014 min
Response: 20521966
Conc: 90.39 ng/ml

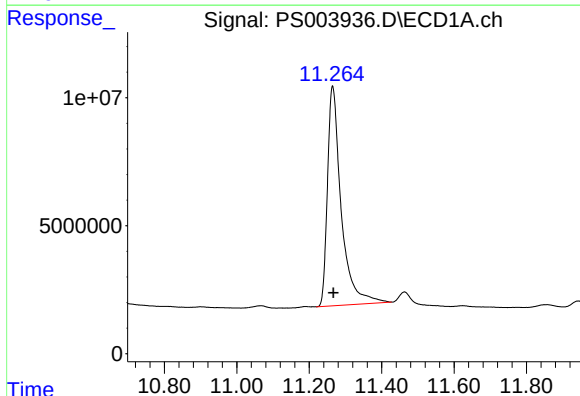


#4 2,4-DCAA

R.T.: 11.265 min
Delta R.T.: -0.002 min
Response: 225988951
Conc: 518.07 ng/ml

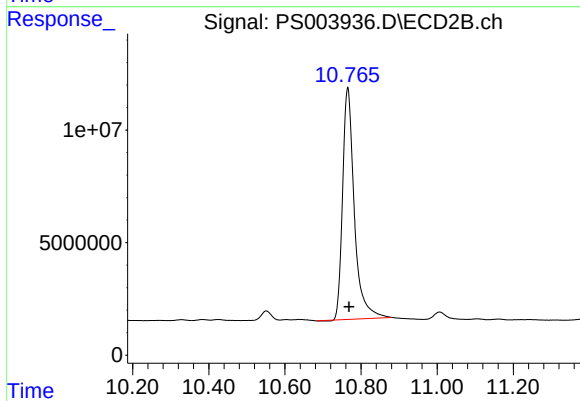

#4 2,4-DCAA


R.T.: 10.765 min
Delta R.T.: -0.004 min
Response: 219282622
Conc: 446.92 ng/ml

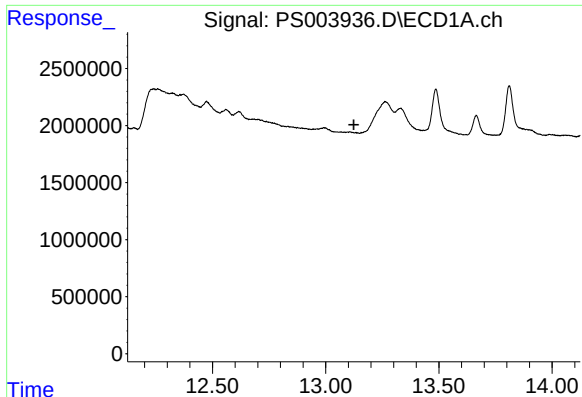

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-7

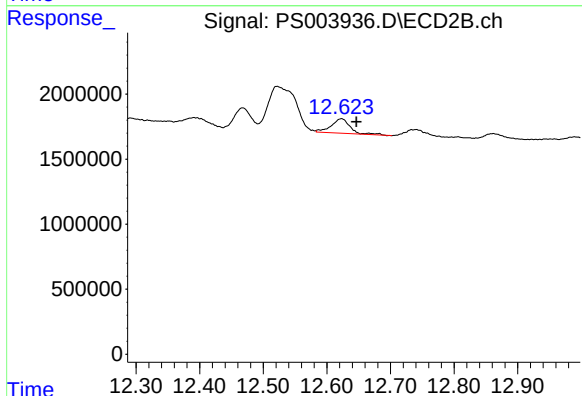


#9 2,4-D

R.T.: 12.622 min
Delta R.T.: -0.024 min
Response: 2315793
Conc: 4.35 ng/ml

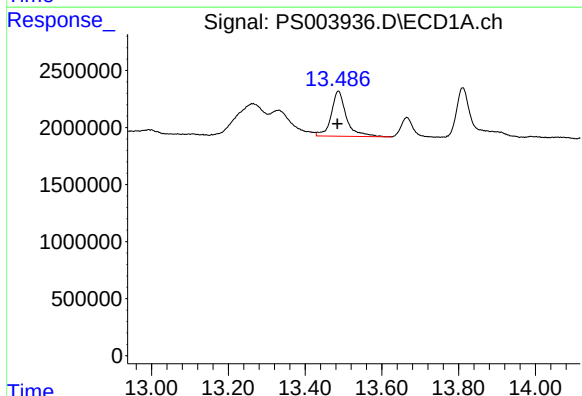


#10 Pentachlorophenol

R.T.: 13.486 min
Delta R.T.: 0.002 min
Response: 10749830
Conc: 1.40 ng/ml

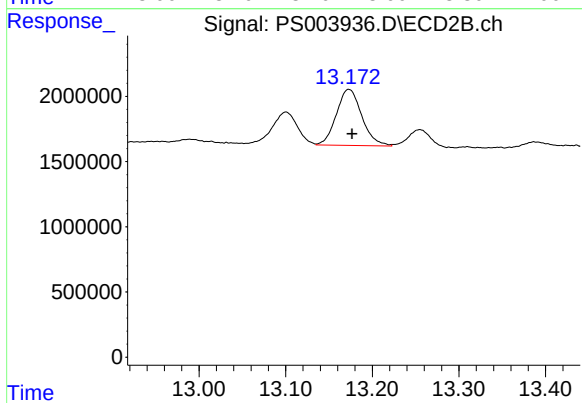

#10 Pentachlorophenol


R.T.: 13.173 min
Delta R.T.: -0.004 min
Response: 8776578
Conc: 1.27 ng/ml

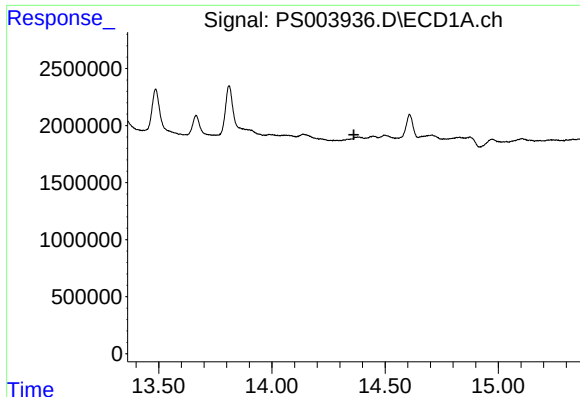

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-7

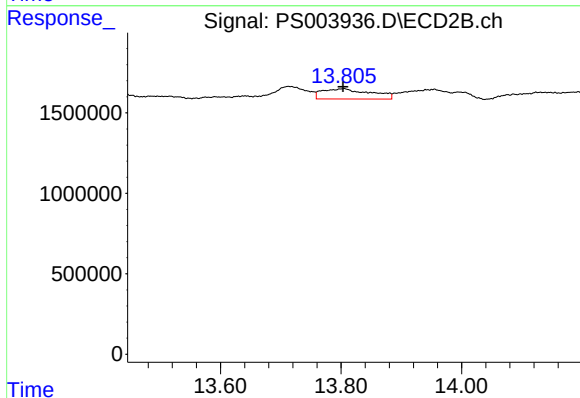


#11 2,4,5-TP (SILVEX)

R.T.: 13.803 min
Delta R.T.: 0.000 min
Response: 3531884
Conc: 1.33 ng/ml

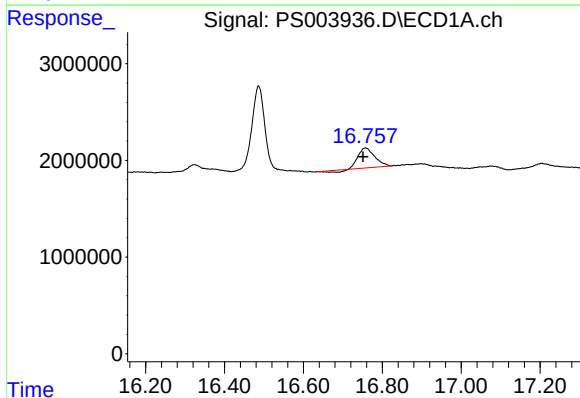


#15 Picloram

R.T.: 16.757 min
Delta R.T.: 0.006 min
Response: 5599241
Conc: 1.65 ng/ml

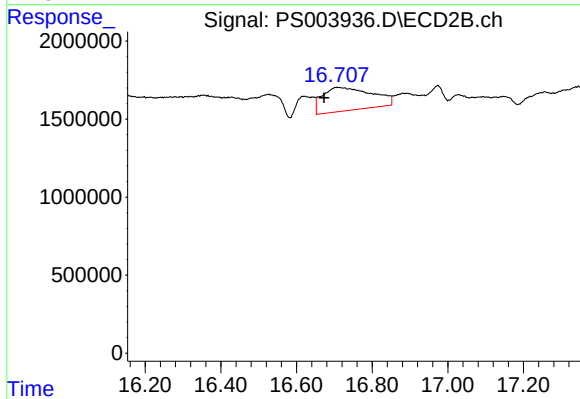

#15 Picloram


R.T.: 16.709 min
Delta R.T.: 0.037 min
Response: 13576029
Conc: 4.28 ng/ml

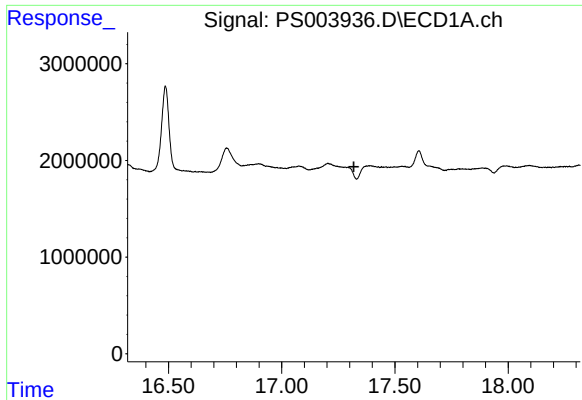

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-7

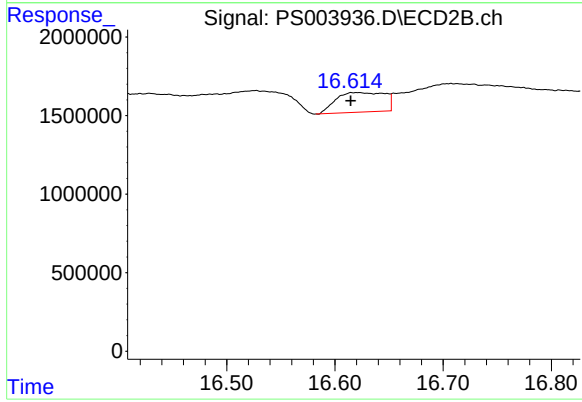

#16 DCPA

R.T.: 16.622 min
Delta R.T.: 0.007 min
Response: 3918244
Conc: 1.16 ng/ml