

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 14:10
 Operator : EI\SJ
 Sample : K2056-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CS-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 15:14:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.783	244.4E6	225.3E6	560.308	459.202
Target Compounds							
1) T	Dalapon	2.801	2.299	41748191	108.7E6	55.998	149.036 #
2) T	3,5-DICHL...	0.000	8.948	0	5603182	N.D.	8.784
3) T	4-Nitroph...	0.000	9.956	0	15765781	N.D.	69.442
5) T	DICAMBA	0.000	11.024	0	5654065	N.D.	3.040
6) T	MCPD	0.000	11.262	0	79207	N.D.	<MDL
7) T	MCPA	12.222	11.679	127.9E6	185535	60.604	<MDL #
9) T	2,4-D	0.000	12.641	0	3273999	N.D.	6.155
10) T	Pentachlo...	0.000	13.189	0	3108507	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.792	0	2583969	N.D.	<MDL
12) T	2,4,5-T	0.000	14.321	0	152888	N.D.	<MDL
13) T	2,4-DB	0.000	14.975	0	3365701	N.D.	11.334
14) T	DINOSEB	0.000	15.415	0	292934	N.D.	<MDL
15) T	Picloram	16.772	16.641	5137723	2771240	1.512	<MDL #
16) T	DCPA	0.000	16.641	0	2771240	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 14:10
Operator : EI\SJ
Sample : K2056-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CS-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 15:14:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

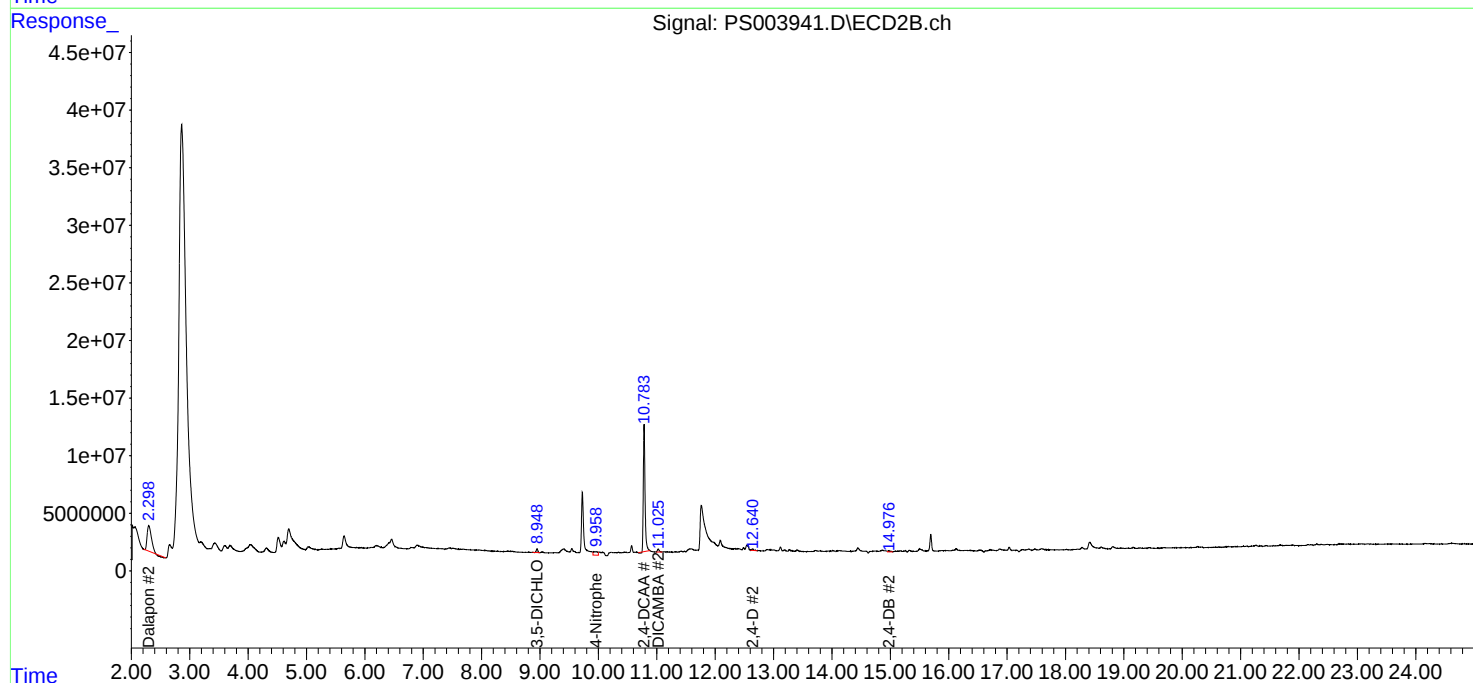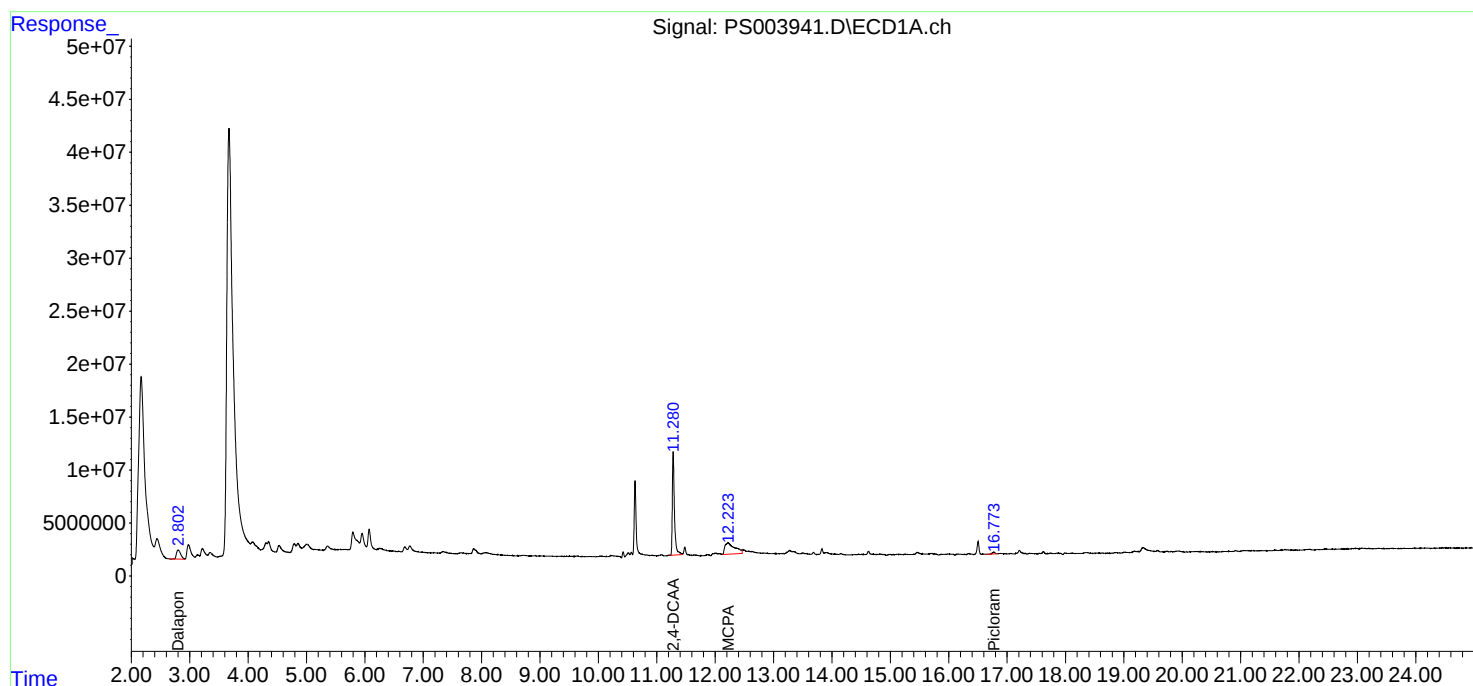


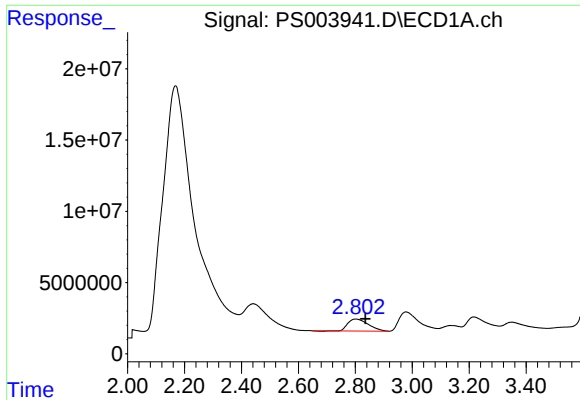

#1 Dalapon


R.T.: 2.801 min
Delta R.T.: -0.034 min
Response: 41748191
Conc: 56.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
CS-10

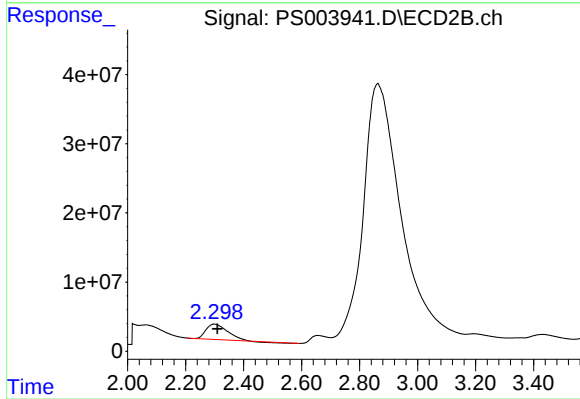


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.012 min
Response: 108740712
Conc: 149.04 ng/ml

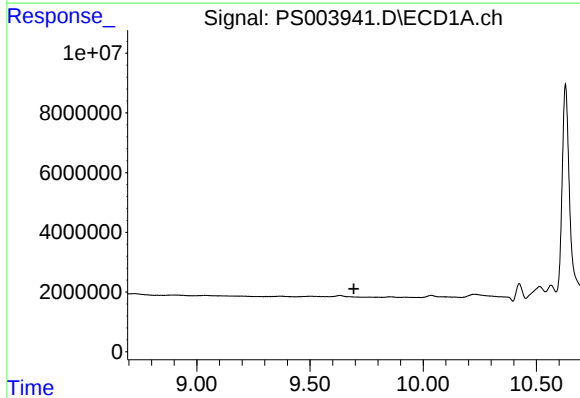


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

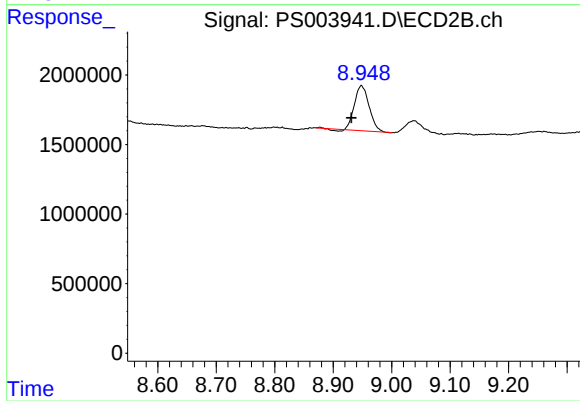

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.948 min
Delta R.T.: 0.017 min
Response: 5603182
Conc: 8.78 ng/ml

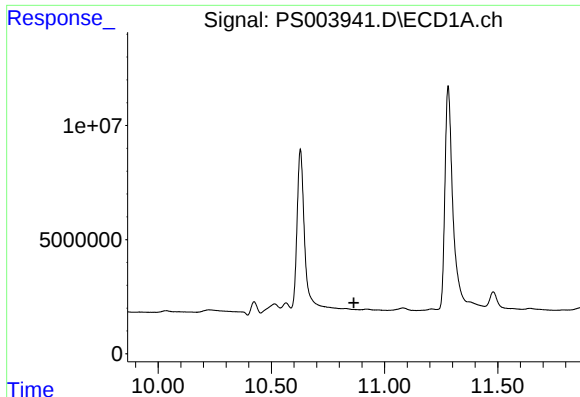

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-10

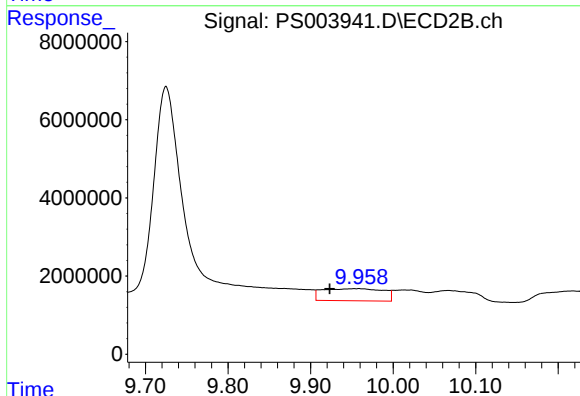


#3 4-Nitrophenol

R.T.: 9.956 min
Delta R.T.: 0.033 min
Response: 15765781
Conc: 69.44 ng/ml

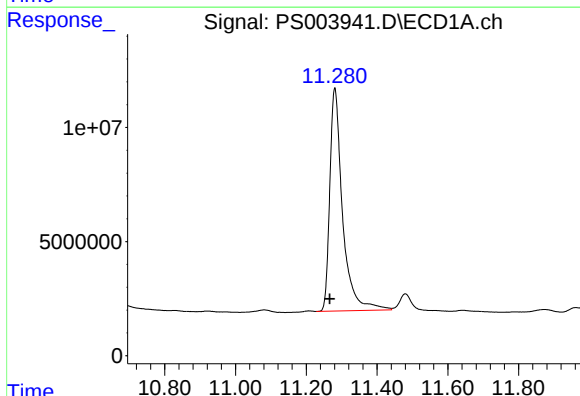


#4 2,4-DCAA

R.T.: 11.281 min
Delta R.T.: 0.014 min
Response: 244413120
Conc: 560.31 ng/ml

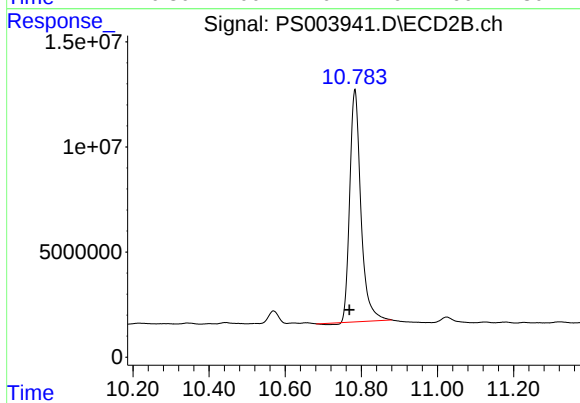

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.014 min
Response: 225311375
Conc: 459.20 ng/ml

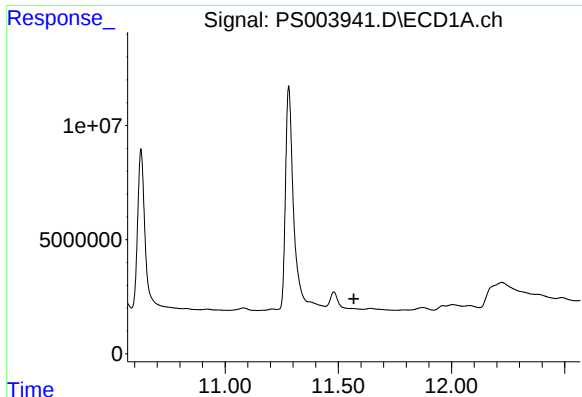

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-10

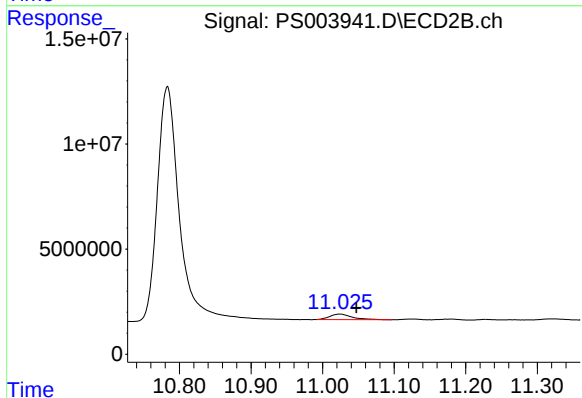


#5 DICAMBA

R.T.: 11.024 min
Delta R.T.: -0.023 min
Response: 5654065
Conc: 3.04 ng/ml

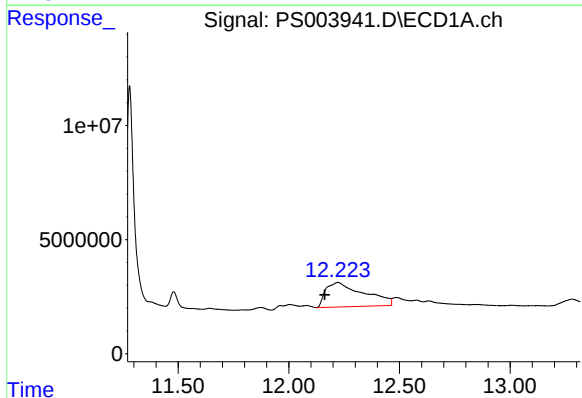


#7 MCPA

R.T.: 12.222 min
Delta R.T.: 0.061 min
Response: 127860764
Conc: 60.60 ug/ml

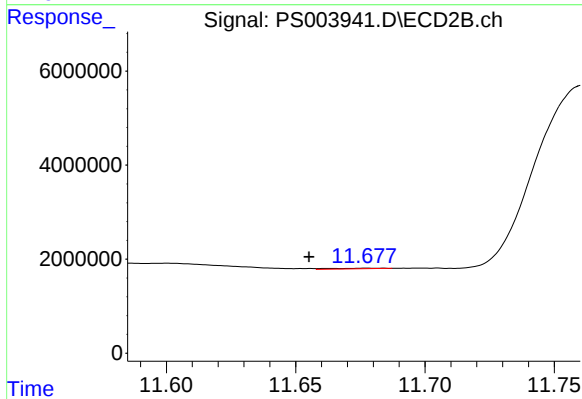

#7 MCPA


R.T.: 11.679 min
Delta R.T.: 0.023 min
Response: 185535
Conc: N.D.

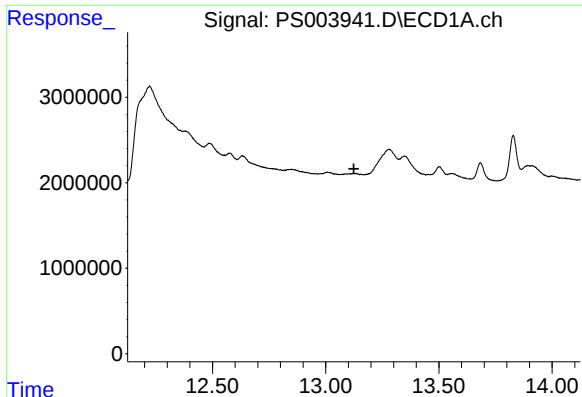

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CS-10

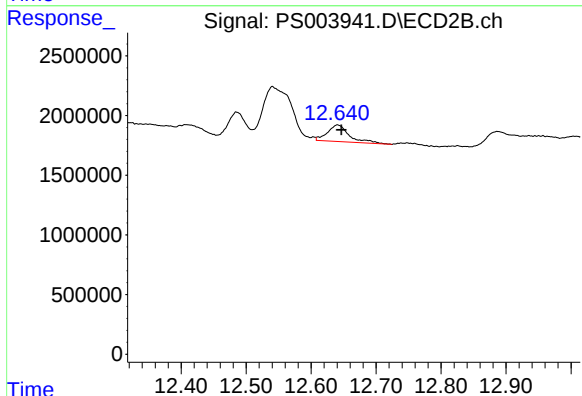


#9 2,4-D

R.T.: 12.641 min
Delta R.T.: -0.005 min
Response: 3273999
Conc: 6.16 ng/ml

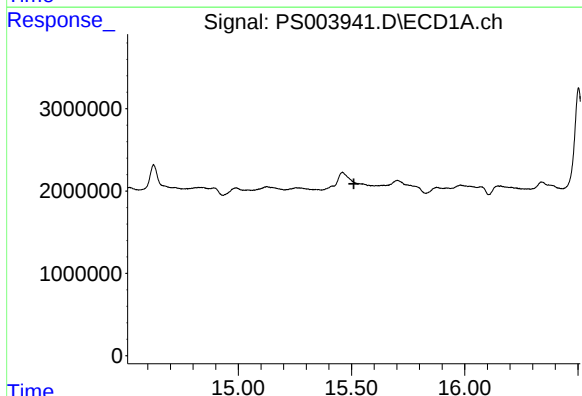


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

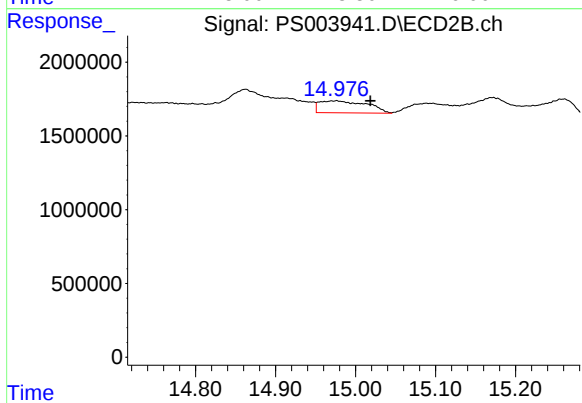

#13 2,4-DB


R.T.: 14.975 min
Delta R.T.: -0.044 min
Response: 3365701
Conc: 11.33 ng/ml

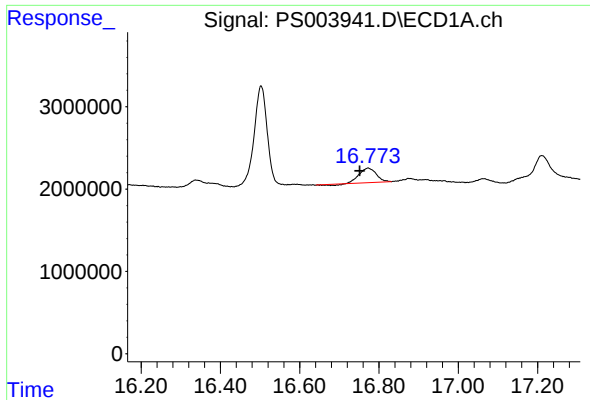

#15 Picloram

R.T.: 16.772 min
Delta R.T.: 0.021 min
Response: 5137723
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
CS-10

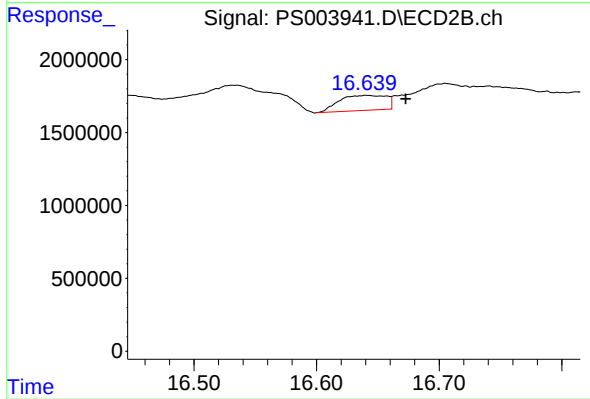

#15 Picloram

R.T.: 16.641 min
Delta R.T.: -0.032 min
Response: 2771240
Conc: N.D.