

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 17:10
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 18:46:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.774	188.0E6	181.0E6	431.013	368.976
Target Compounds							
2) T	3,5-DICHL...	0.000	8.955	0	50197	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.948	0	376648	N.D.	1.659
6) T	MCP	0.000	11.282	0	106452	N.D.	<MDL
7) T	MCPA	0.000	11.660	0	1948748	N.D.	1.093
8) T	DICHLORPROP	0.000	12.185	0	222248	N.D.	<MDL
9) T	2,4-D	0.000	12.613	0	706110	N.D.	1.328
10) T	Pentachlo...	0.000	13.186	0	1740644	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.796	0	308239	N.D.	<MDL
12) T	2,4,5-T	0.000	14.351	0	44836	N.D.	<MDL
13) T	2,4-DB	0.000	15.012	0	201627	N.D.	<MDL
14) T	DINOSEB	0.000	15.450	0	517334	N.D.	<MDL
15) T	Picloram	0.000	16.655	0	87585	N.D.	<MDL
16) T	DCPA	0.000	16.617	0	455253	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 17:10
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 18:46:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

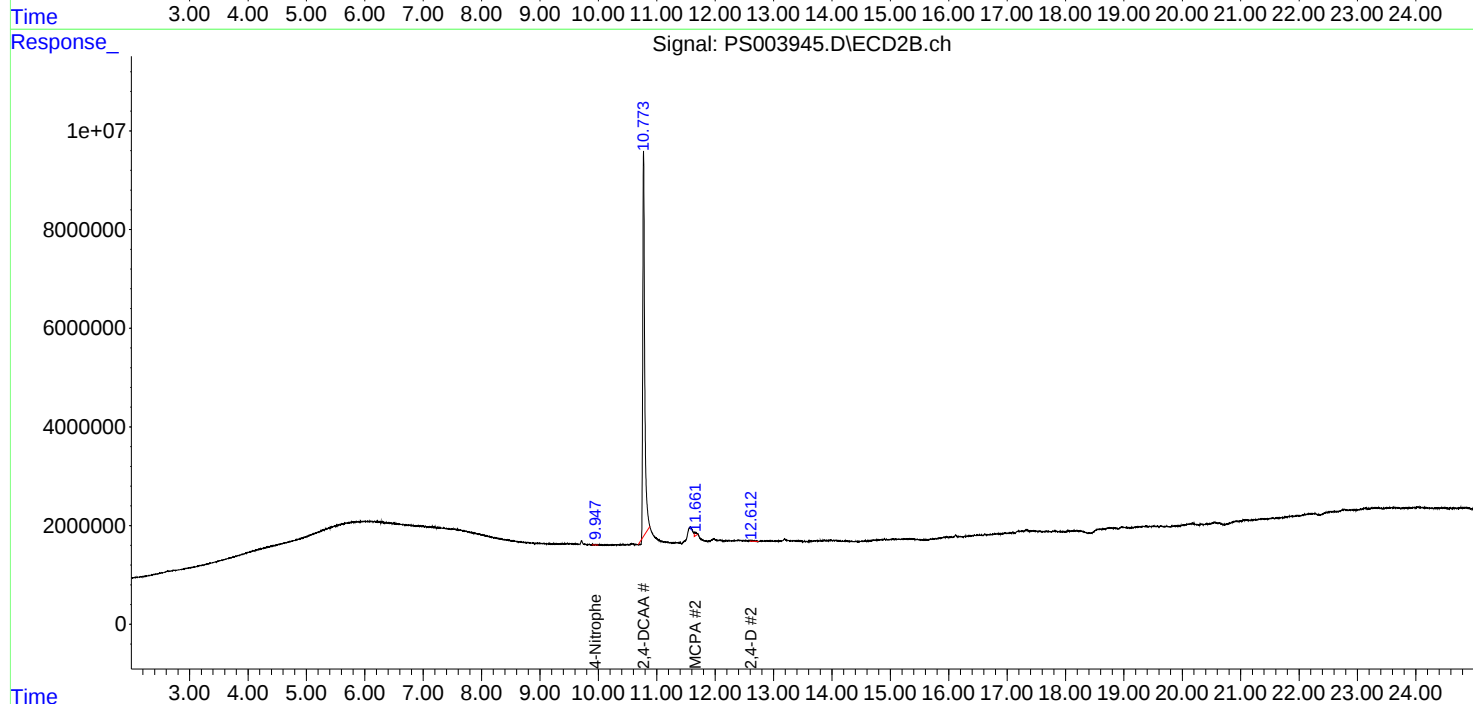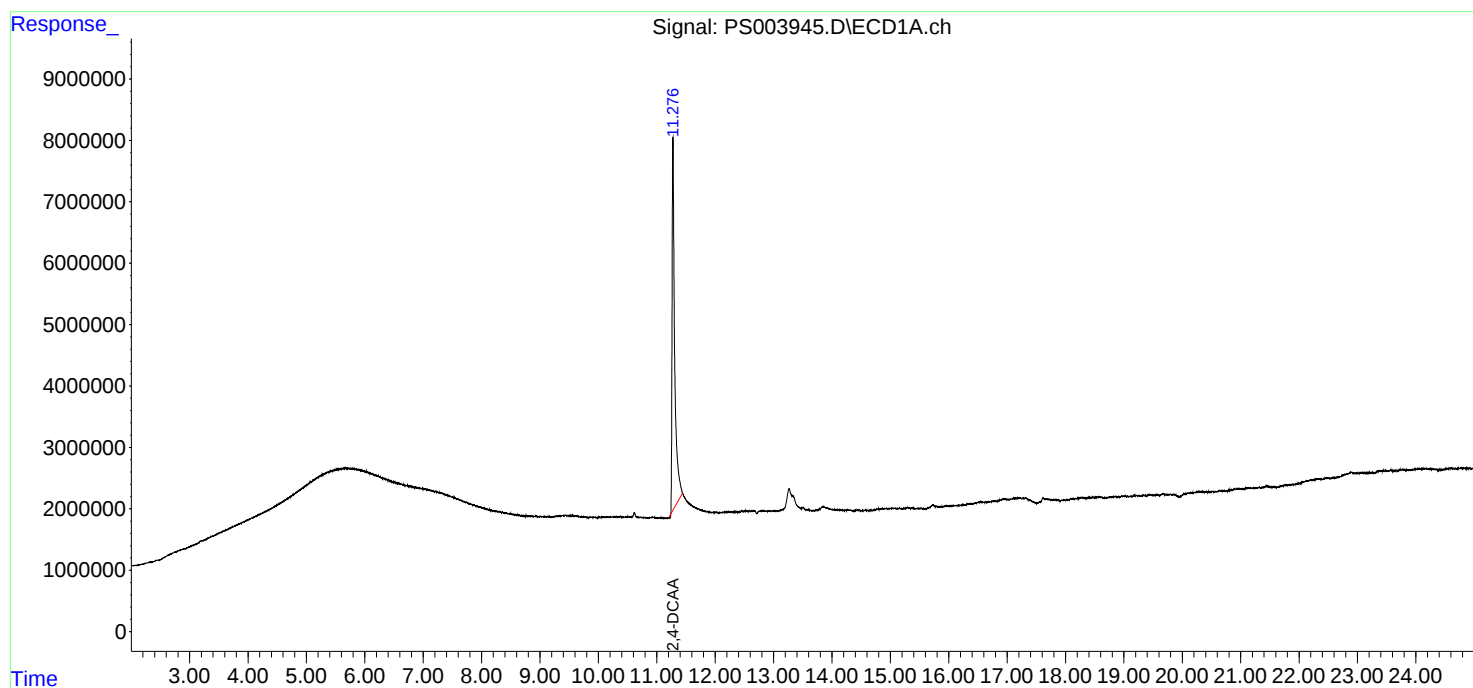


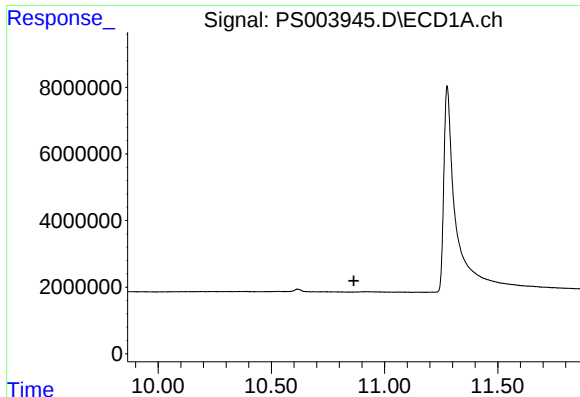

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

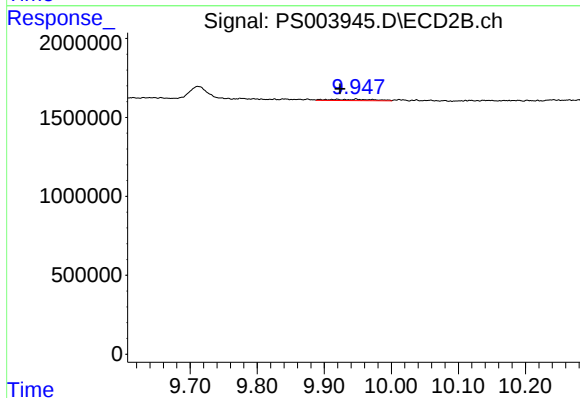


#3 4-Nitrophenol

R.T.: 9.948 min
Delta R.T.: 0.024 min
Response: 376648
Conc: 1.66 ng/ml

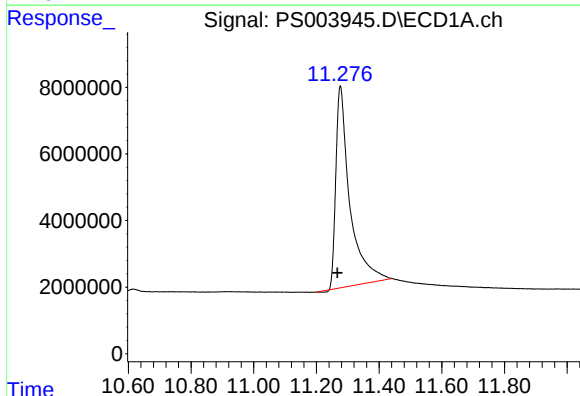


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: 0.010 min
Response: 188013293
Conc: 431.01 ng/ml

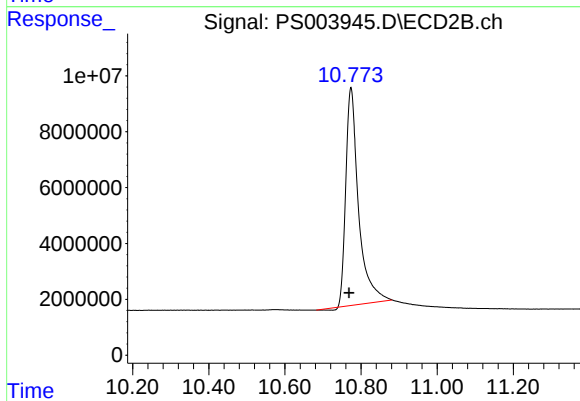

#4 2,4-DCAA


R.T.: 10.774 min
Delta R.T.: 0.005 min
Response: 181041126
Conc: 368.98 ng/ml

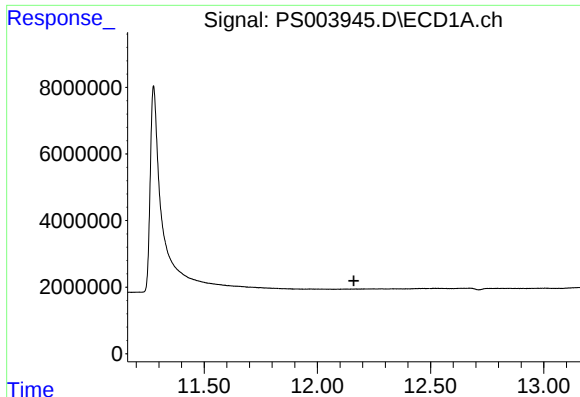

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

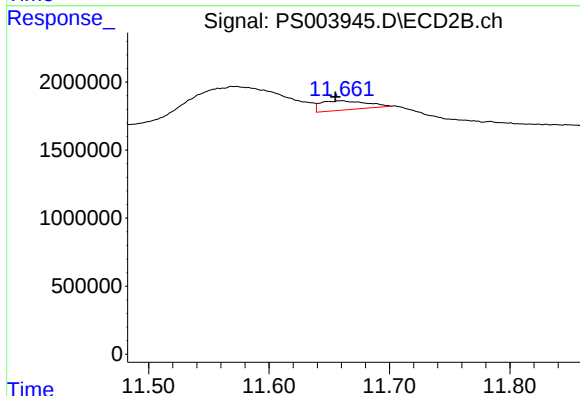


#7 MCPA

R.T.: 11.660 min
Delta R.T.: 0.005 min
Response: 1948748
Conc: 1.09 ug/ml

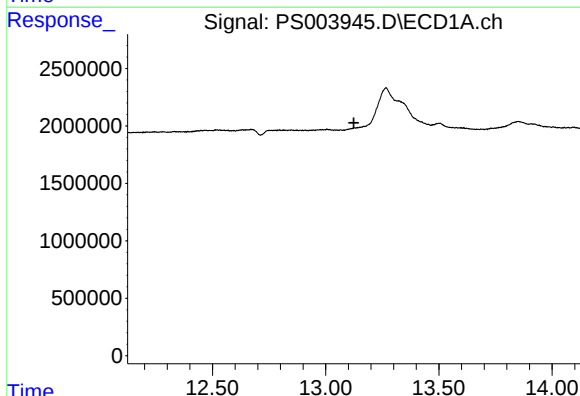

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

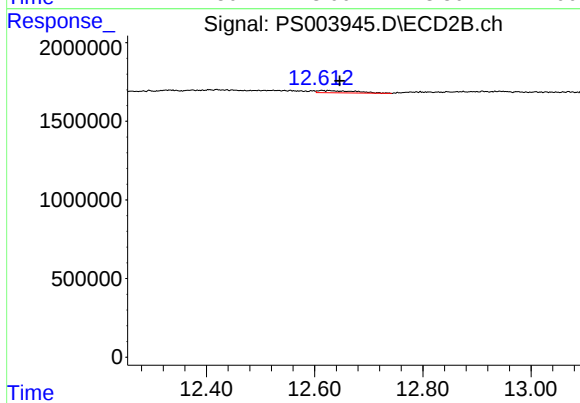

#9 2,4-D

R.T.: 12.613 min
Delta R.T.: -0.033 min
Response: 706110
Conc: 1.33 ng/ml