

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 03:54
 Operator : EI\SJ
 Sample : K2182-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S8A(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:51:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.780	294.7E6	269.4E6	675.595	548.985
Target Compounds							
1) T	Dalapon	2.801	2.298	46096990	106.2E6	61.831	145.560 #
2) T	3,5-DICHL...	0.000	8.946	0	6405749	N.D.	10.043
3) T	4-Nitroph...	0.000	9.946	0	16020566	N.D.	70.564
5) T	DICAMBA	0.000	11.021	0	6422395	N.D.	3.453
7) T	MCPA	12.148	11.688	189.6E6	586362	89.846	<MDL #
9) T	2,4-D	0.000	12.640	0	3242107	N.D.	6.095
10) T	Pentachlo...	0.000	13.184	0	756327	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.791	0	2720200	N.D.	1.027
12) T	2,4,5-T	0.000	14.366	0	687570	N.D.	<MDL
13) T	2,4-DB	0.000	15.007	0	1539007	N.D.	5.183
14) T	DINOSEB	0.000	15.397	0	784577	N.D.	<MDL
15) T	Picloram	16.763	16.669	9589281	1308716	2.823	<MDL #
16) T	DCPA	0.000	16.643	0	3789959	N.D.	1.121



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 03:54
Operator : EI\SJ
Sample : K2182-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:51:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

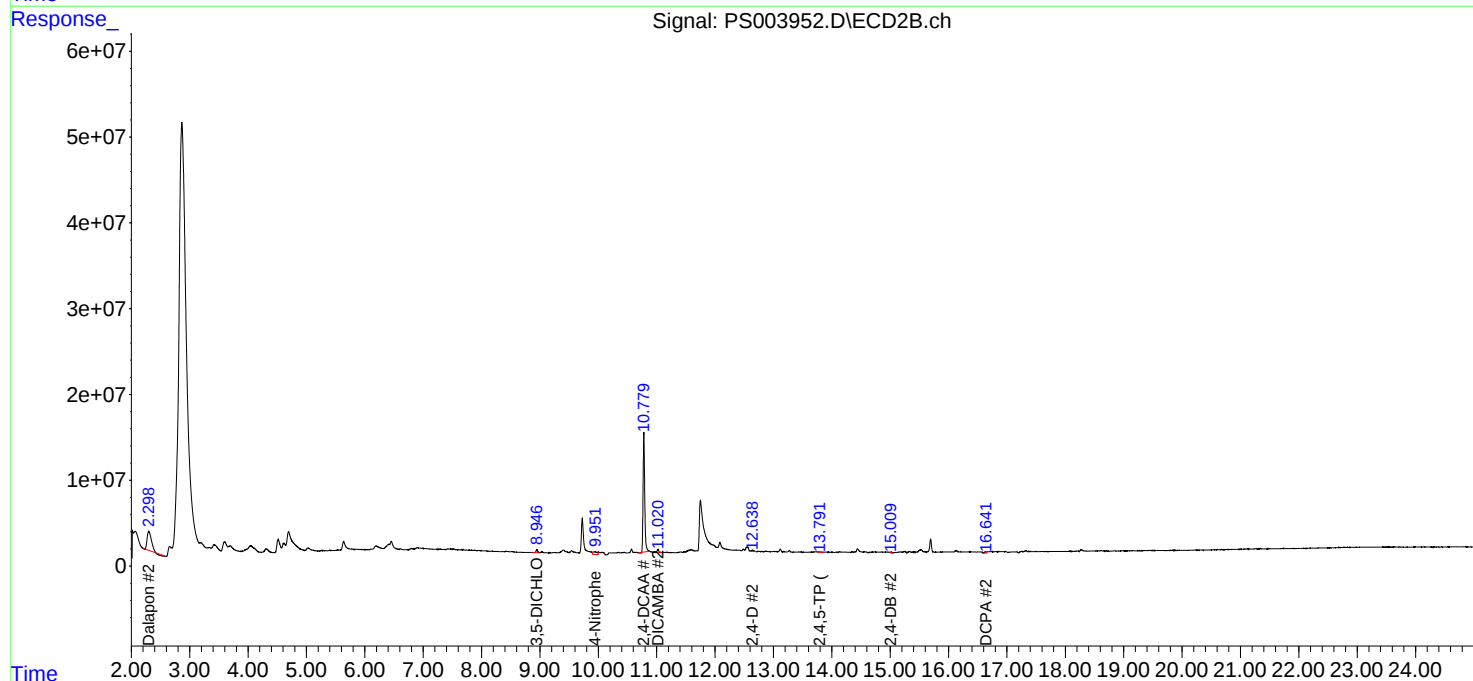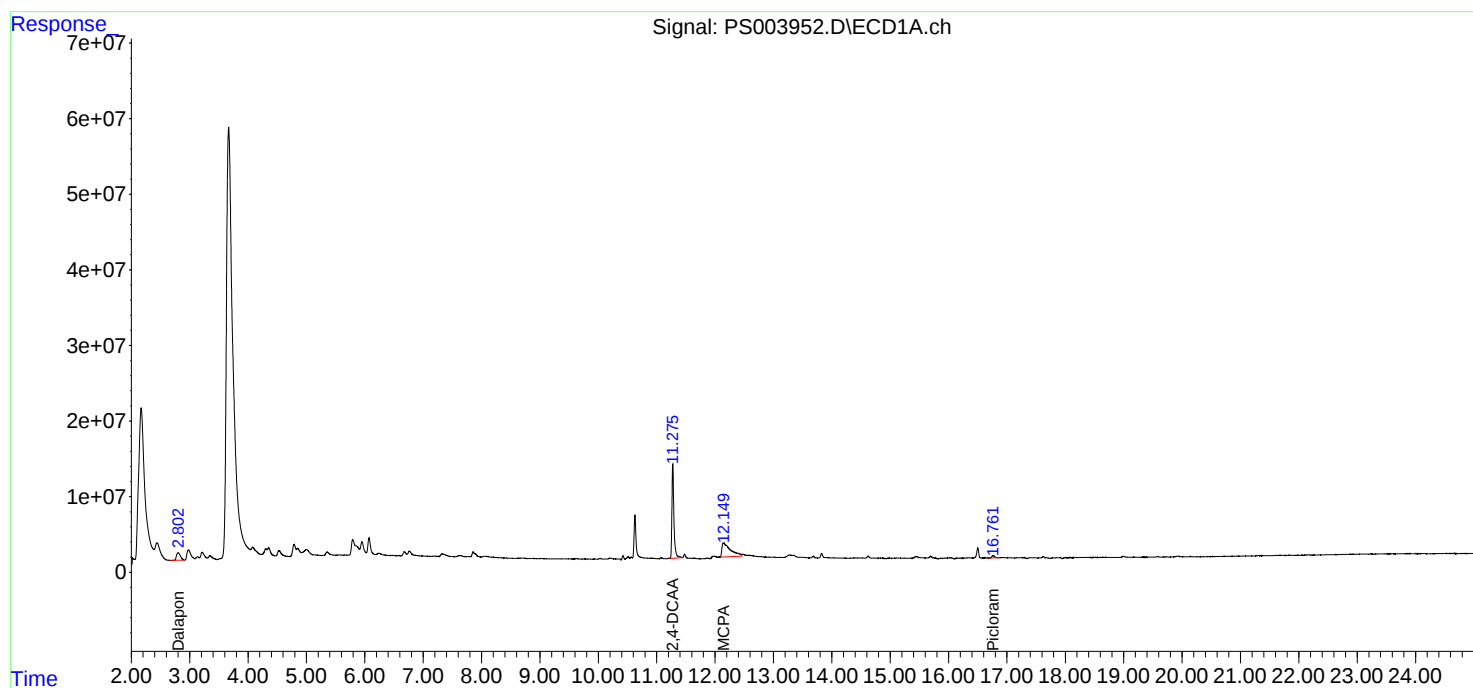


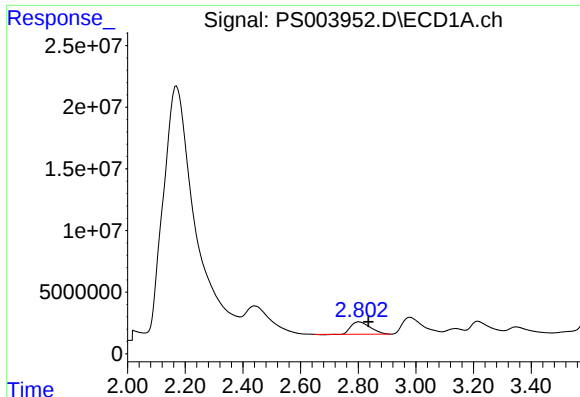

#1 Dalapon


R.T.: 2.801 min
Delta R.T.: -0.034 min
Response: 46096990
Conc: 61.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

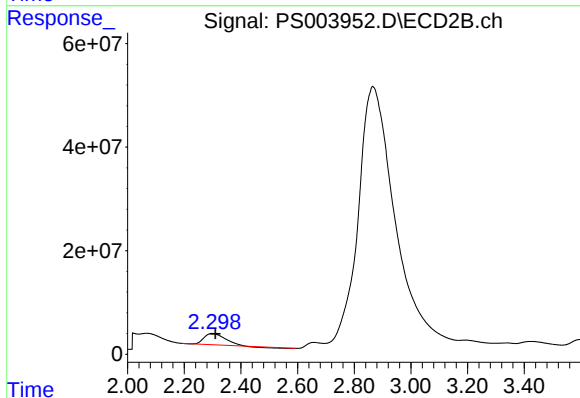


#1 Dalapon

R.T.: 2.298 min
Delta R.T.: -0.012 min
Response: 106204787
Conc: 145.56 ng/ml

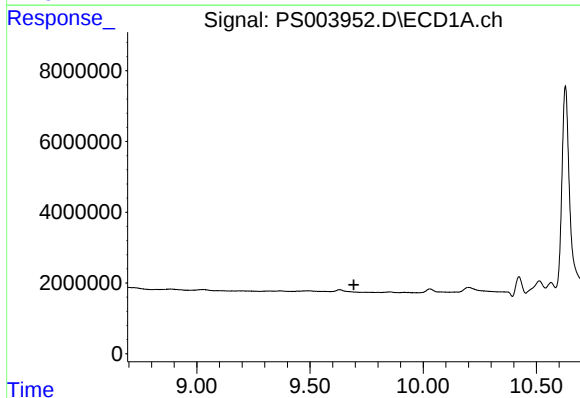


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

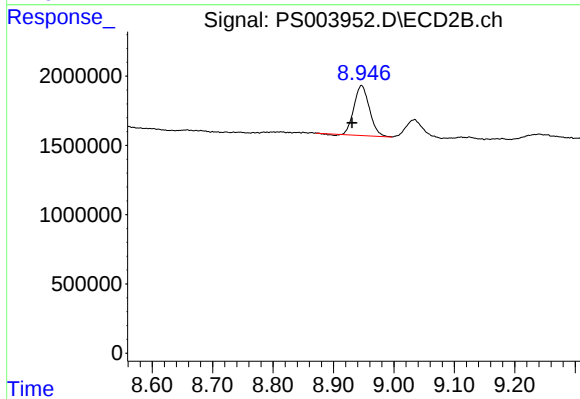

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.946 min
Delta R.T.: 0.015 min
Response: 6405749
Conc: 10.04 ng/ml

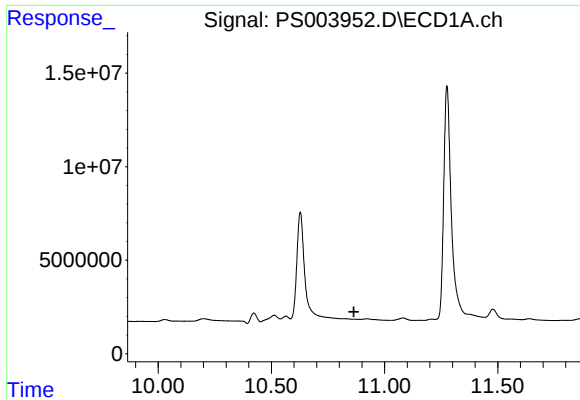

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

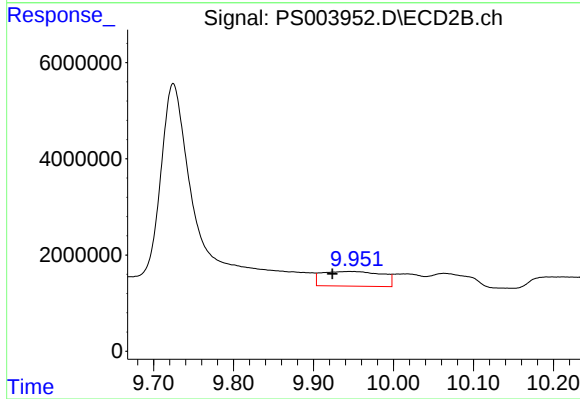


#3 4-Nitrophenol

R.T.: 9.946 min
Delta R.T.: 0.023 min
Response: 16020566
Conc: 70.56 ng/ml

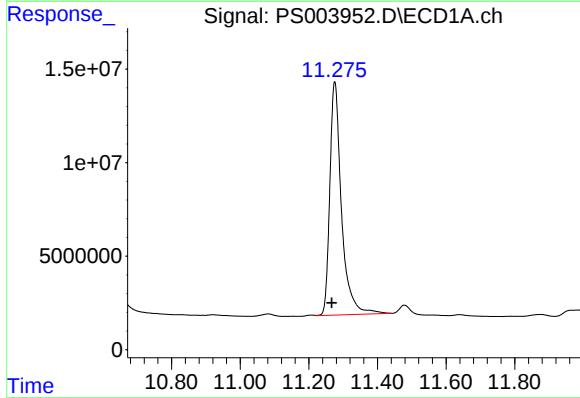


#4 2,4-DCAA

R.T.: 11.275 min
Delta R.T.: 0.009 min
Response: 294703082
Conc: 675.60 ng/ml

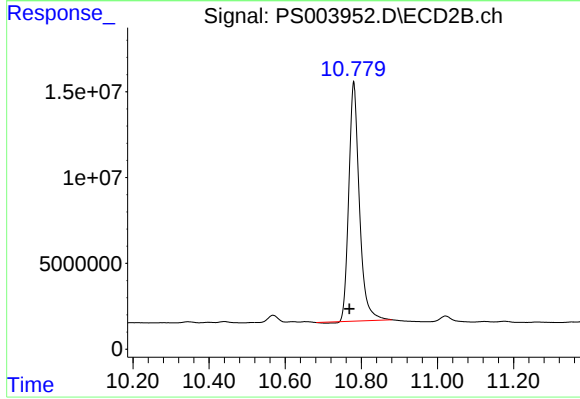

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.011 min
Response: 269364313
Conc: 548.99 ng/ml

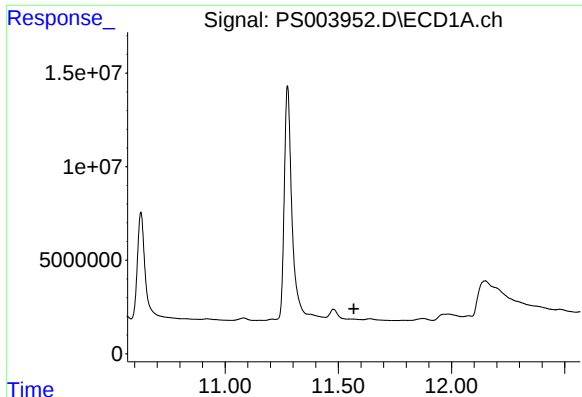

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

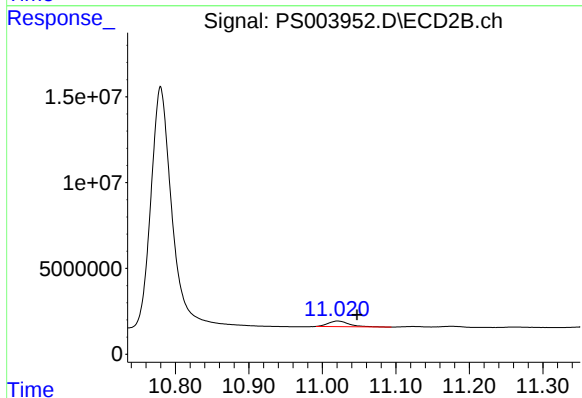


#5 DICAMBA

R.T.: 11.021 min
Delta R.T.: -0.026 min
Response: 6422395
Conc: 3.45 ng/ml

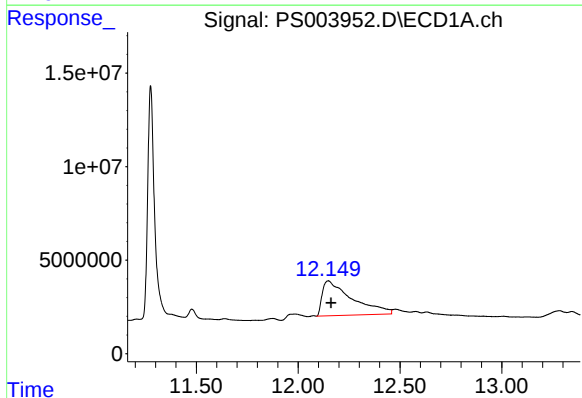


#7 MCPA

R.T.: 12.148 min
Delta R.T.: -0.014 min
Response: 189555690
Conc: 89.85 ug/ml

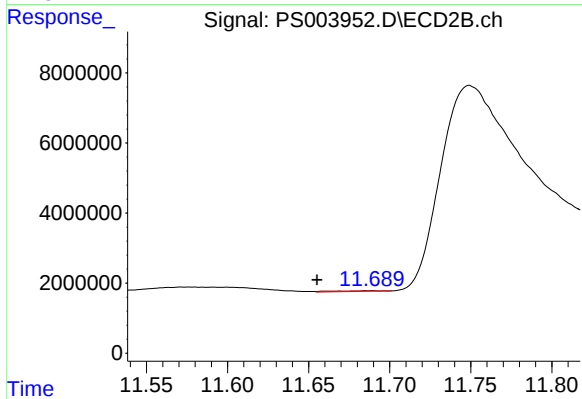

#7 MCPA


R.T.: 11.688 min
Delta R.T.: 0.032 min
Response: 586362
Conc: N.D.

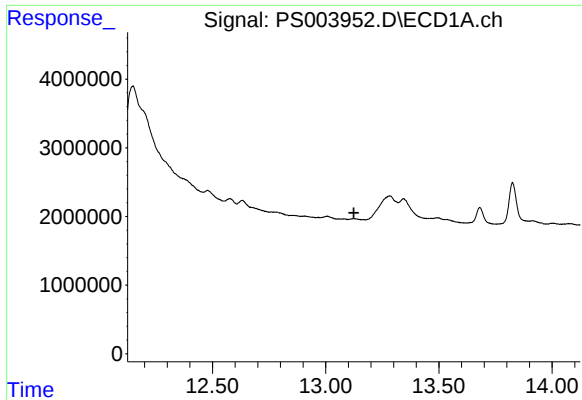

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

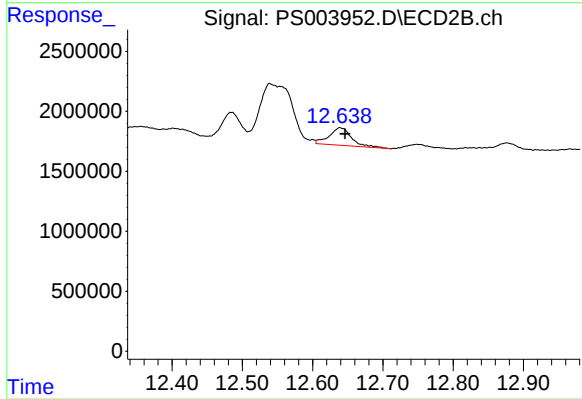


#9 2,4-D

R.T.: 12.640 min
Delta R.T.: -0.007 min
Response: 3242107
Conc: 6.10 ng/ml

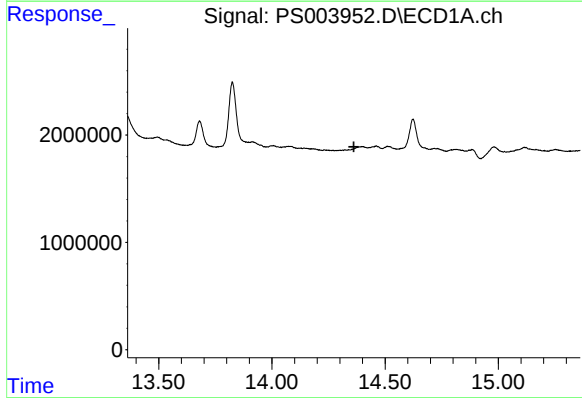


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

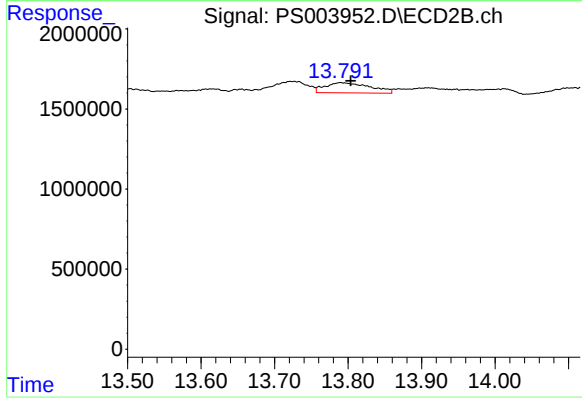

#11 2,4,5-TP (SILVEX)


R.T.: 13.791 min
Delta R.T.: -0.013 min
Response: 2720200
Conc: 1.03 ng/ml

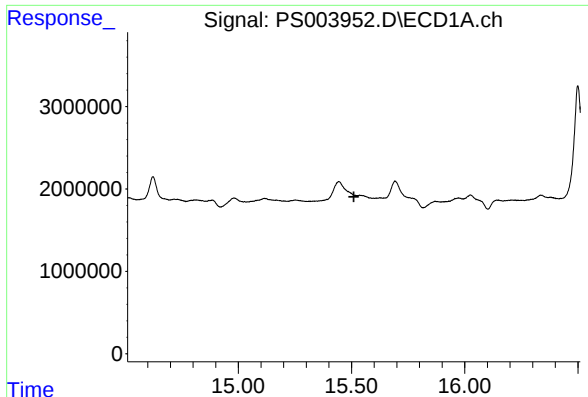

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

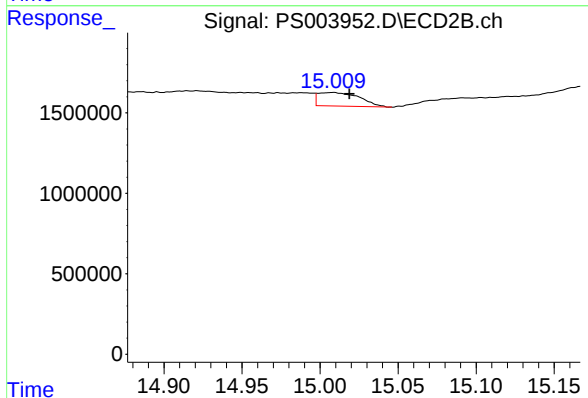


#13 2,4-DB

R.T.: 15.007 min
Delta R.T.: -0.012 min
Response: 1539007
Conc: 5.18 ng/ml

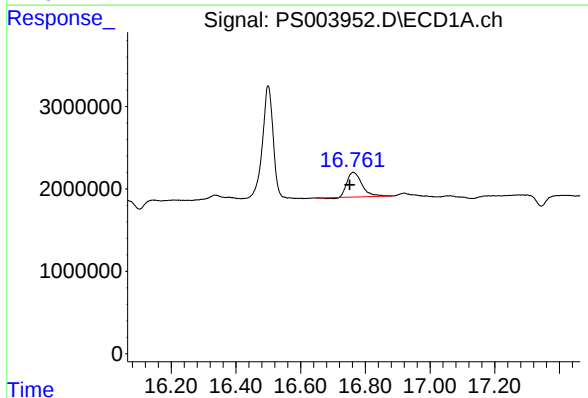


#15 Picloram

R.T.: 16.763 min
Delta R.T.: 0.011 min
Response: 9589281
Conc: 2.82 ng/ml

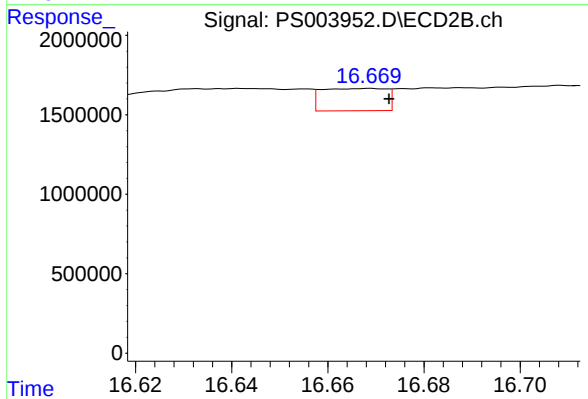

#15 Picloram


R.T.: 16.669 min
Delta R.T.: -0.003 min
Response: 1308716
Conc: N.D.

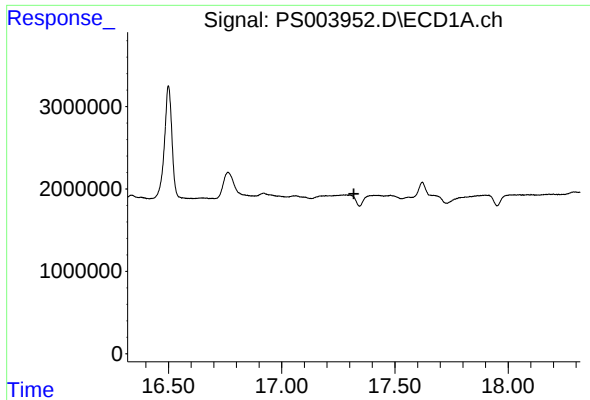

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A(2-10)COMP

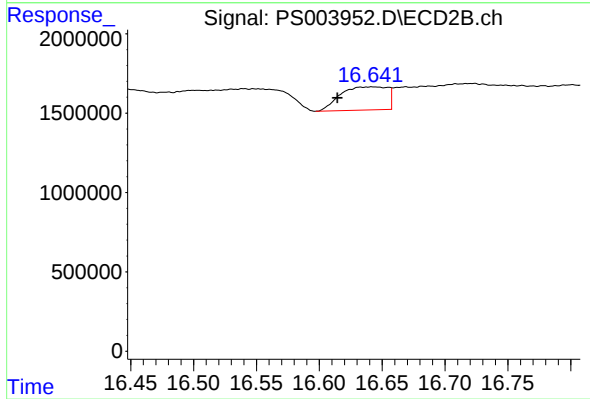

#16 DCPA

R.T.: 16.643 min
Delta R.T.: 0.028 min
Response: 3789959
Conc: 1.12 ng/ml