

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 04:25
 Operator : EI\SJ
 Sample : K2182-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S8A-S8B(12-16)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:51:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.300	10.803	353.3E6	316.3E6	809.933	644.626
Target Compounds							
1) T	Dalapon	2.825	2.322	51172925	99459119	68.639	136.315 #
2) T	3,5-DICHL...	0.000	8.971	0	5952850	N.D.	9.333
3) T	4-Nitroph...	0.000	9.970	0	15433129	N.D.	67.977
5) T	DICAMBA	0.000	11.045	0	6143599	N.D.	3.303
6) T	MCPD	0.000	11.285	0	524888	N.D.	<MDL
7) T	MCPA	12.101	11.617	3307087	4115109	1.568	2.308 #
8) T	DICHLORPROP	0.000	12.110	0	30065490	N.D.	64.583
9) T	2,4-D	0.000	12.663	0	3171976	N.D.	5.963
10) T	Pentachlo...	0.000	13.210	0	1431486	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.815	0	3588539	N.D.	1.355
13) T	2,4-DB	0.000	15.036	0	1003240	N.D.	3.378
15) T	Picloram	16.791	16.660	13259044	2575659	3.903	<MDL #
16) T	DCPA	0.000	16.578	0	6874246	N.D.	2.034



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 04:25
Operator : EI\SJ
Sample : K2182-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:51:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

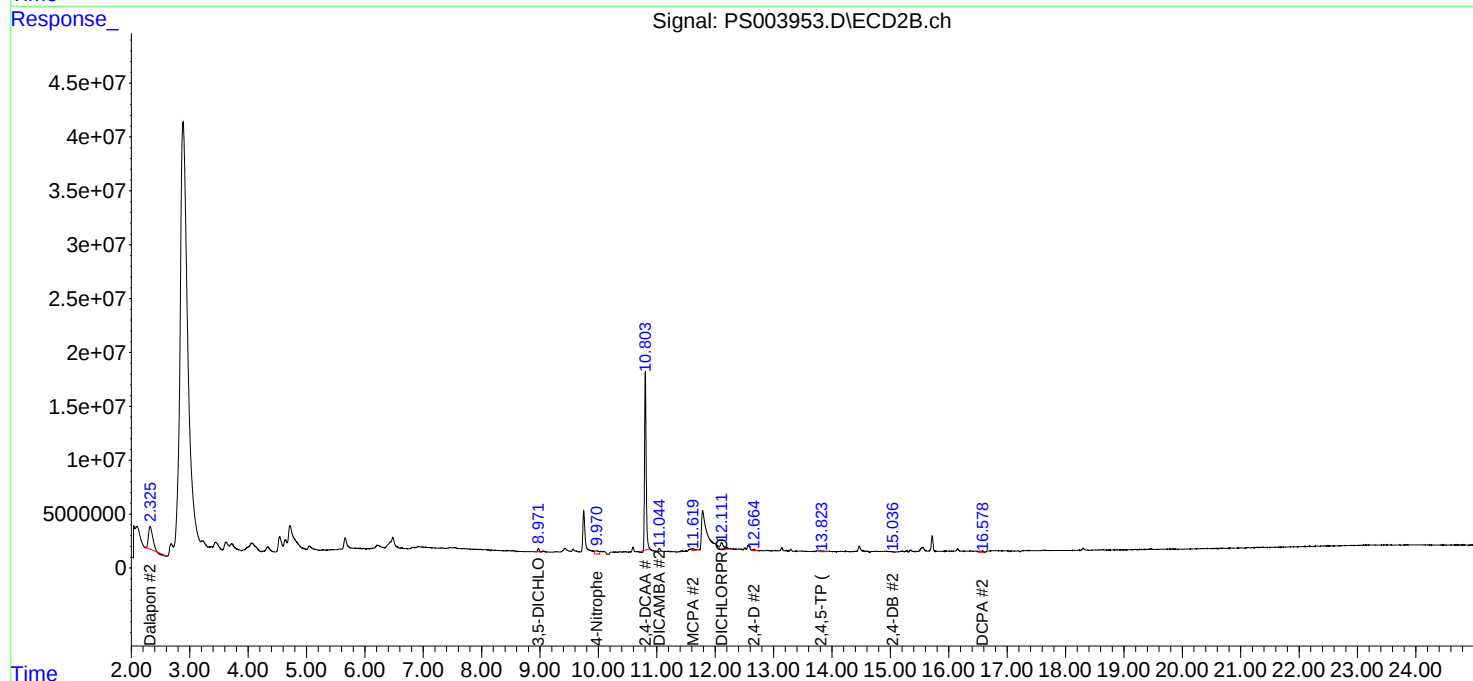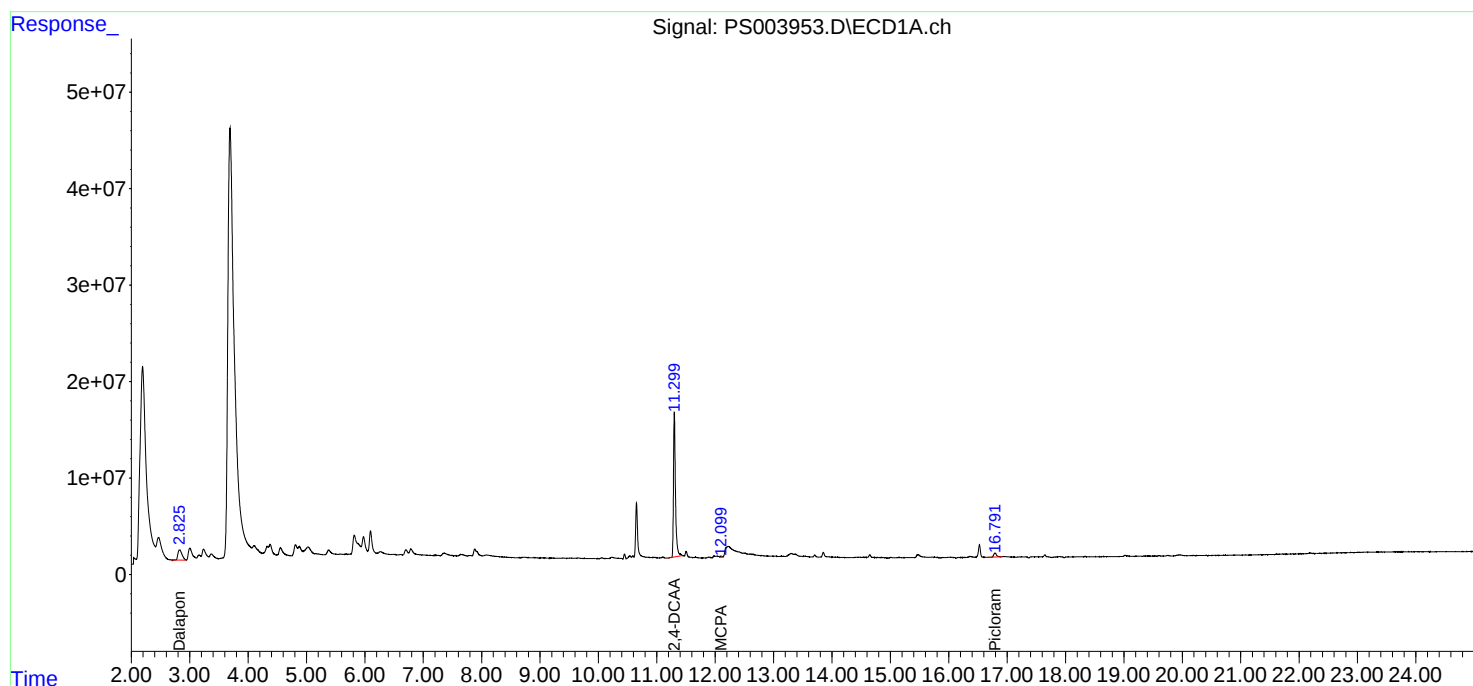


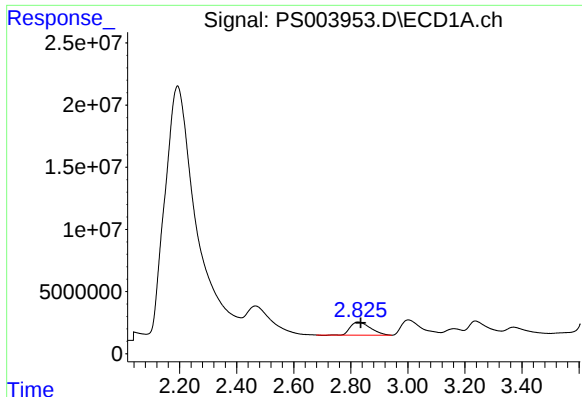

#1 Dalapon


R.T.: 2.825 min
Delta R.T.: -0.010 min
Response: 51172925
Conc: 68.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

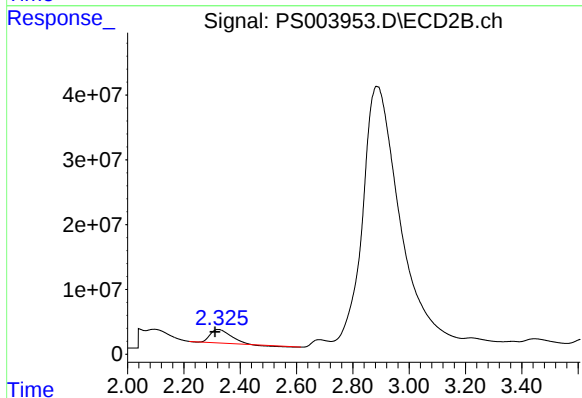


#1 Dalapon

R.T.: 2.322 min
Delta R.T.: 0.012 min
Response: 99459119
Conc: 136.31 ng/ml

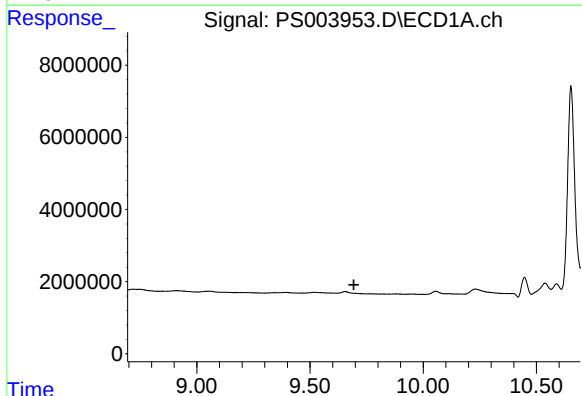


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

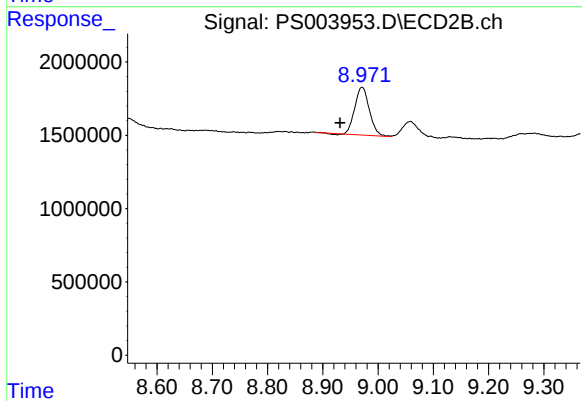

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.971 min
Delta R.T.: 0.040 min
Response: 5952850
Conc: 9.33 ng/ml

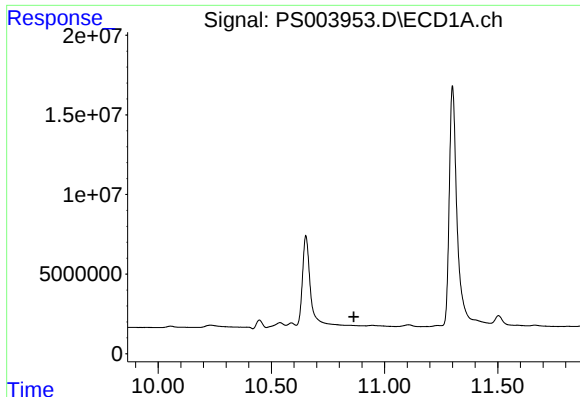

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

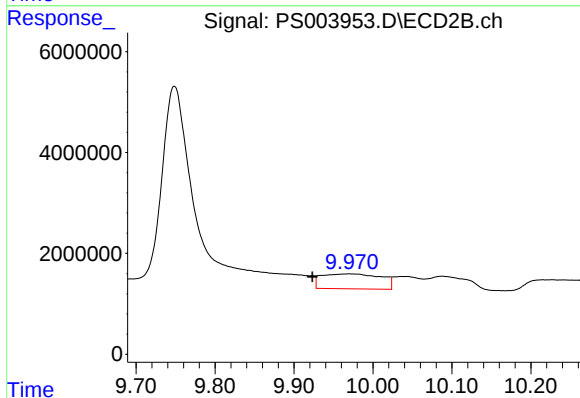


#3 4-Nitrophenol

R.T.: 9.970 min
Delta R.T.: 0.047 min
Response: 15433129
Conc: 67.98 ng/ml

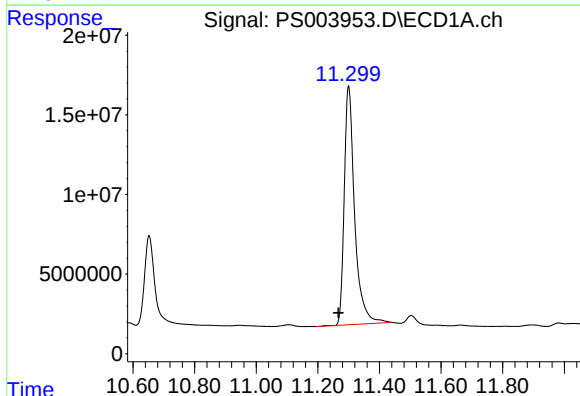


#4 2,4-DCAA

R.T.: 11.300 min
Delta R.T.: 0.034 min
Response: 353302998
Conc: 809.93 ng/ml

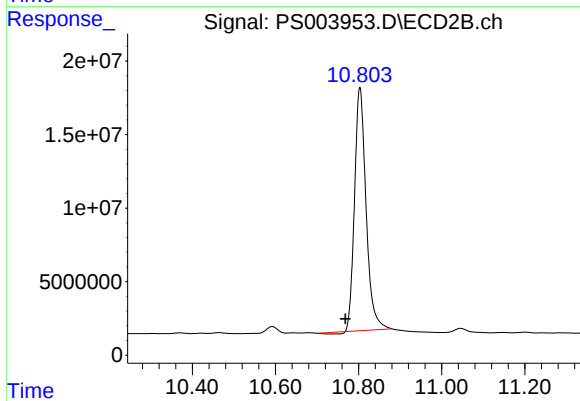

#4 2,4-DCAA


R.T.: 10.803 min
Delta R.T.: 0.034 min
Response: 316291119
Conc: 644.63 ng/ml

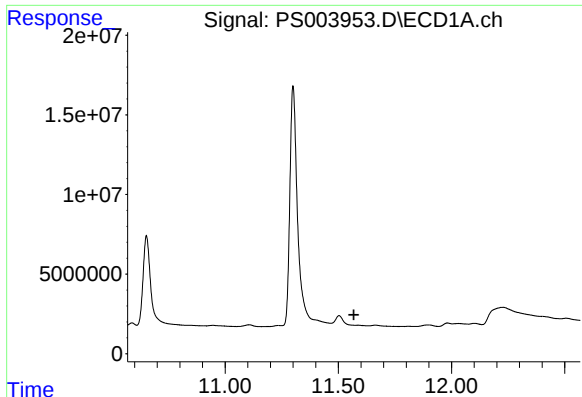

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

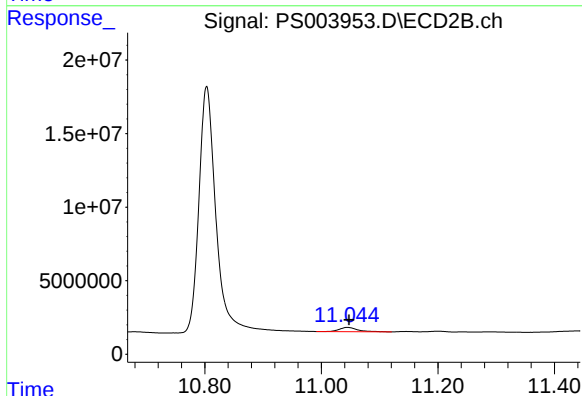


#5 DICAMBA

R.T.: 11.045 min
Delta R.T.: -0.002 min
Response: 6143599
Conc: 3.30 ng/ml

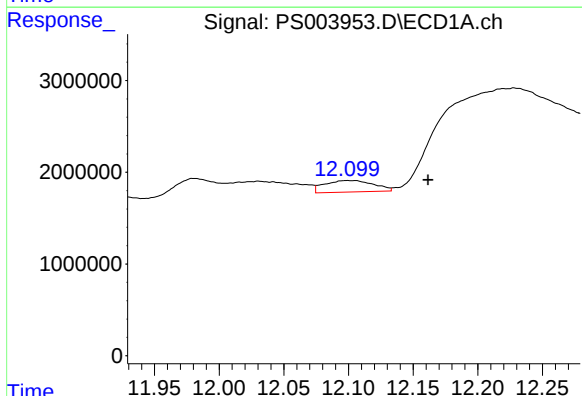


#7 MCPA

R.T.: 12.101 min
Delta R.T.: -0.061 min
Response: 3307087
Conc: 1.57 ug/ml

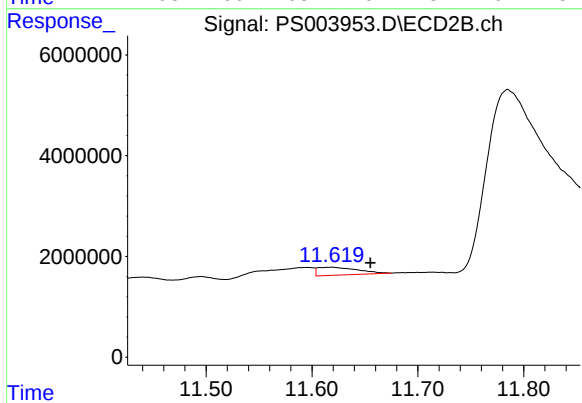

#7 MCPA


R.T.: 11.617 min
Delta R.T.: -0.038 min
Response: 4115109
Conc: 2.31 ug/ml

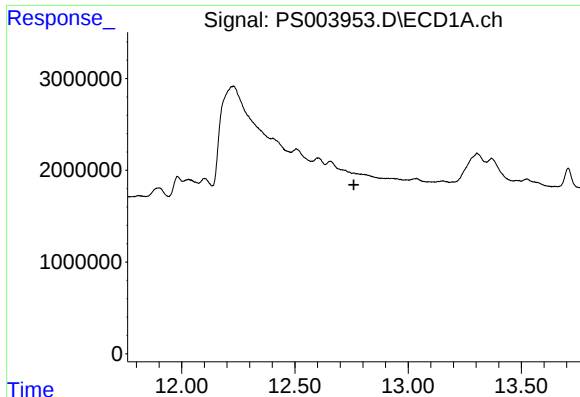

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

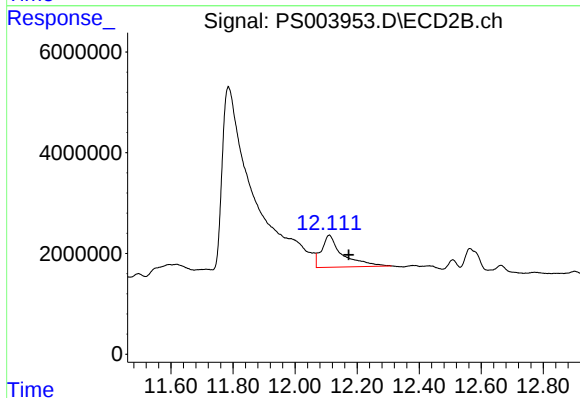


#8 DICHLORPROP

R.T.: 12.110 min
Delta R.T.: -0.063 min
Response: 30065490
Conc: 64.58 ng/ml

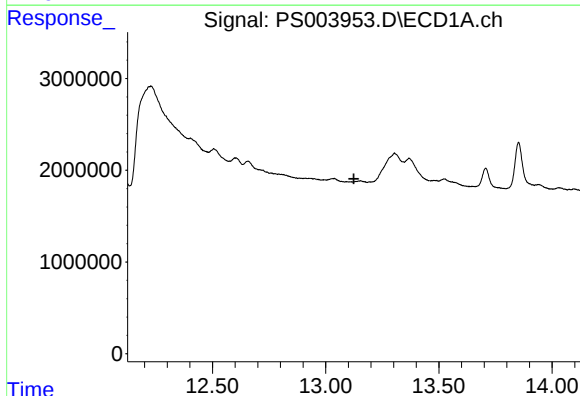


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

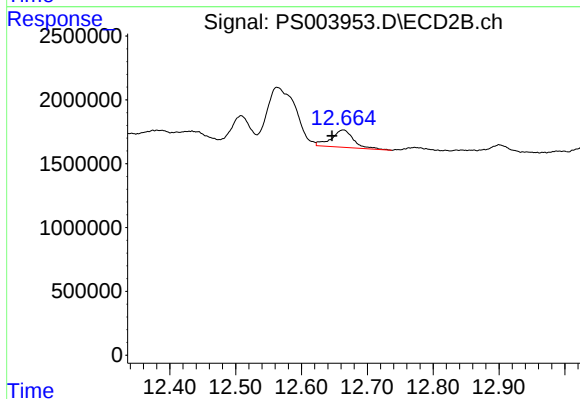

#9 2,4-D


R.T.: 12.663 min
Delta R.T.: 0.017 min
Response: 3171976
Conc: 5.96 ng/ml

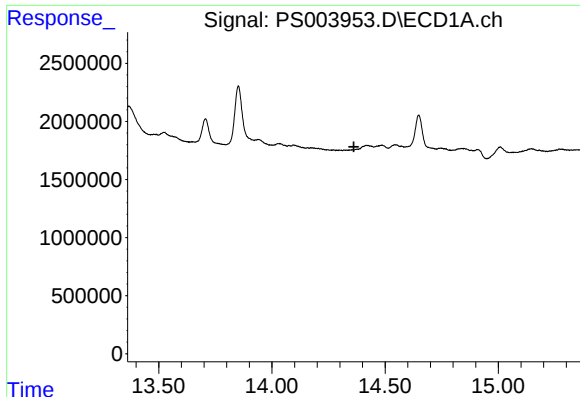

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

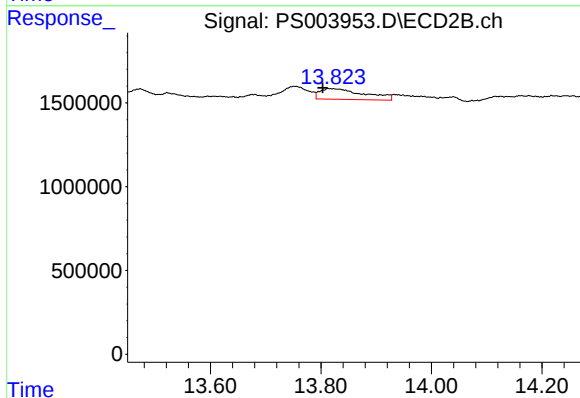


#11 2,4,5-TP (SILVEX)

R.T.: 13.815 min
Delta R.T.: 0.012 min
Response: 3588539
Conc: 1.35 ng/ml

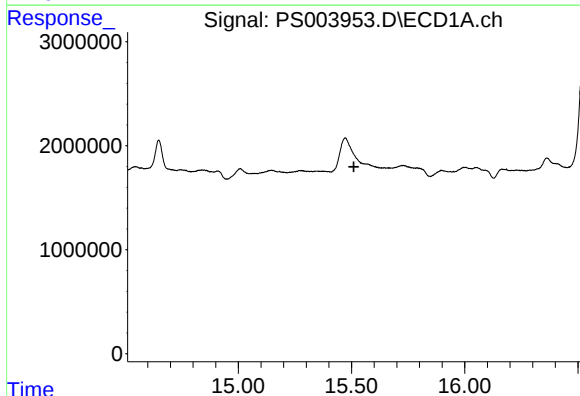


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

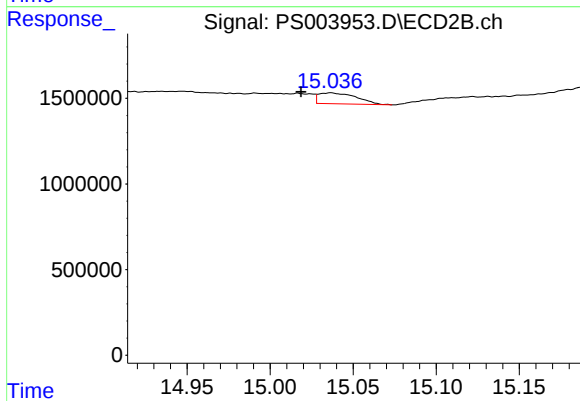

#13 2,4-DB


R.T.: 15.036 min
Delta R.T.: 0.017 min
Response: 1003240
Conc: 3.38 ng/ml

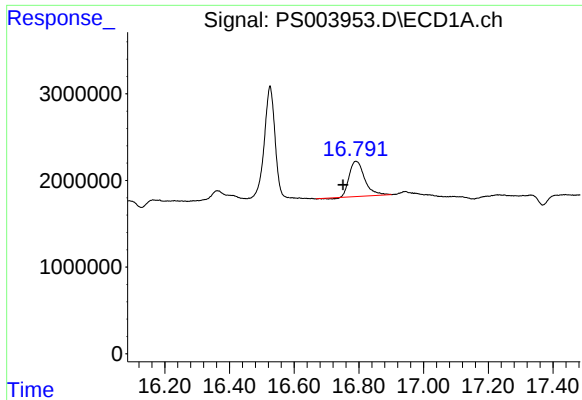

#15 Picloram


R.T.: 16.791 min
Delta R.T.: 0.040 min
Response: 13259044
Conc: 3.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

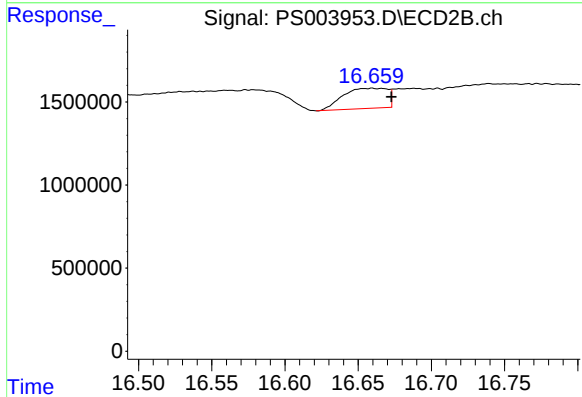


#15 Picloram

R.T.: 16.660 min
Delta R.T.: -0.013 min
Response: 2575659
Conc: N.D.

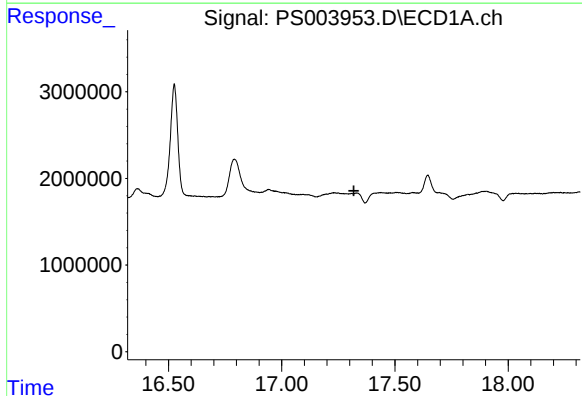

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

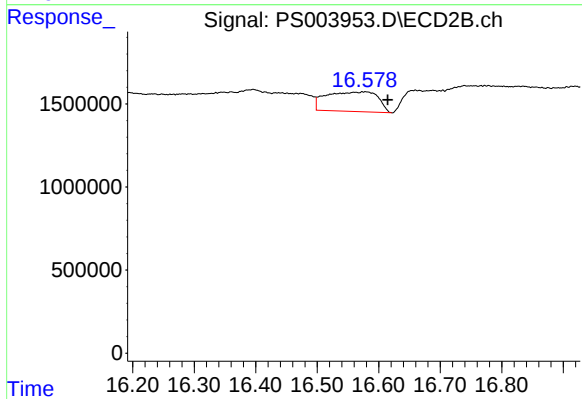

#16 DCPA

R.T.: 16.578 min
Delta R.T.: -0.037 min
Response: 6874246
Conc: 2.03 ng/ml